



Cardiac Rhythm Heart Failure

Product Performance Report

Important Patient Management Information for Physicians

2015

First Edition – Issue 72

CRHF Product Performance Report

2015

First Edition

Issue 72

| | |
|--|-----|
| Introduction | 5 |
| Method for Estimating CRT, ICD, and IPG Device Performance | 10 |
| CRT-D | 15 |
| CRT-P | 59 |
| ICD | 64 |
| IPG | 131 |
| Method for Estimating Lead Performance | 217 |
| Left-Heart | 222 |
| Defibrillation | 231 |
| Pacing | 249 |
| Epi/Myocardial | 283 |
| VDD Single Pass | 286 |
| ICD and CRT-D Charge Time Performance | 288 |
| Advisories | 301 |
| Performance Notes | 312 |

Cutoff date for this edition is 31 January 2015 for Lead Study data and 9 February for all other data.

This report is available online at [www.medtronic.com/CRDM ProductPerformance](http://www.medtronic.com/CRDM/ProductPerformance)

Our Commitment to Quality

Medtronic was founded in 1949 and has grown to become a global leader in medical technology. Seeing what a difference medical technology could make in the lives of patients inspired our founder to develop the Medtronic Mission, which remains unchanged today.

The third tenet of the mission is all about quality:

“To strive without reserve for the greatest possible reliability and quality in our products, to be the unsurpassed standard of comparison, and to be recognized as a company of dedication, honesty, integrity, and service.”

Regardless of function, all CRHF employees play a role in product quality. Whether designing new therapies, sourcing components, manufacturing products, hiring talented people, assigning financial resources to project teams, or serving in one of the hundreds of other roles, every employee has an influence on product quality.

Product performance information is received from many sources through various channels. Medtronic monitors information from many sources from Research and Development through Manufacturing and Field Performance Vigilance.

When a device is returned to Medtronic, laboratory technicians and engineers assess overall device function. Analysis of returned product is performed according to written procedures. These procedures determine the minimum analysis required. The analysis required varies depending on the type of device, age of the device, the associated information received with the device, actual experience with models of similar design, and other factors. Additional analysis is performed as necessary to investigate a performance concern from a customer, or to collect specific reliability data.

When a malfunction is identified, failure analysis is performed to provide the detailed information necessary to investigate possible causes and actions. Medtronic CRHF maintains in-house expertise and performs its failure analysis using facilities it owns and supports. This capability permits detailed failure analysis.

Analysis results are compared to original manufacturing records and design intent. Clinical observations are added to laboratory findings to help determine root cause. Each event is then compared to other events. If a pattern is detected, actions are taken to identify a common root cause, assess patient risk and an appropriate course of action.

Medtronic instituted the industry’s first product performance reports in 1983 by publishing data on our chronic lead studies. Pacemakers and other devices followed as our performance reporting has constantly evolved based on customer needs and feedback. One thing has been a constant. It is our sincere commitment to communicate clearly, offering timely and appropriate product performance data and reliability information. This has always been and will continue to be our goal.



Tim Samsel
Vice President, Quality and Regulatory Medtronic
Cardiac Rhythm Heart Failure Medtronic, Inc.

Contact Information

We invite our customers to use these telephone numbers to call with suggestions, inquiries, or specific problems related to our products.

US Technical Services Department

Phone: 1 (800) 723-4636 (Tachy)

1 (800) 505-4636 (Brady)

Fax: 1 (800) 824-2362

www.medtronic.com/corporate/contact.jsp

For questions related to this CRHF Product Performance Report, please call US Technical Services at the number above, or write to:

Tim Smith
Medtronic, Inc.
8200 Coral Sea Street NE MVN61 Mounds
View, MN 55112 USA
Email: tim.smith@medtronic.com

International Technical Centers

Europe (Heerlen NL) +31-45-566-8844

Japan (Tokyo) +81-3-6430-7026

For questions related to returning explanted product or returning product that shows signs of malfunction, please contact:

Outside the United States:
Your Medtronic representative or international technical center at the number above.

Within the United States:
Your Medtronic representative or
CRHF Returned Product Analysis Laboratory
Phone: 1 (800) 328-2518, ext. 44800
Email: crdm.returnedproduct@medtronic.com

Editorial Staff

Independent Physician Quality Panel

Steven J. Compton, MD, Anchorage, AK
John P. DiMarco, MD, PhD, Charlottesville, VA
Kevin Hackett, MD, Columbus, OH
R. Hardwin Mead, MD, Palo Alto, CA
N.A. Mark Estes, MD, Boston, MA
Andrew Krahn, MD, Vancouver, BC
David Cannon, MD, Los Angeles, CA

Editor

Tim Samsel, Vice President, CRHF Quality and Regulatory

Trademarks of Medtronic, Inc.

| | | |
|---------------------|---------------------|-----------------|
| Adapta® | InSync Maximo® | Spectraflex |
| Advisa® | InSync II | Sprint® |
| Advisa DR MRI® | Protect™ | Sprint Fidelis |
| Attain® | InSync III Protect™ | Sprint Quattro® |
| Attain Ability® | Intrinsic™ | Sprint Quattro |
| Attain StarFix® | Kappa® | Secure® |
| Attain Prevail® | Legend® | Sprint Quattro |
| Brava™ | Marquis® | Secure S® |
| CapSure® | Maximo® | SureFix® |
| CapSure Sense® | Medtronic | Syngra® |
| CapSureFix® | CareAlert® | Target Tip® |
| CapSureFix Novus™ | Medtronic CareLink® | Tenax |
| Capture | Micro Jewel | Transvene |
| Management® | Micro Minix | Versa® |
| Cardia™ | MVP® | Virtuoso® |
| CareLink® | Onyx | Viva™ |
| Concerto® | Patient Alert | |
| Consulta® | Performa™ | |
| Egida™ | Preva | |
| EnRhythm® | Prodigy | |
| EnRhythm MRI™ | Protecta® | |
| Ensura MRI™ | Quick Look™ | |
| EnTrust® | Relia™ | |
| EnTrust MRI | Revo MRI® | |
| GEM® | Secura® | |
| InSync® | SelectSecure® | |
| InSync Marquis™ | Sensia® | |
| InSync II Marquis™ | Sensing Assurance | |
| InSync III Marquis™ | Sigma | |

Introduction

All product performance reports are not created equal. For 32 years, Medtronic has monitored performance via both returned product analysis and multicenter clinical studies.

This Product Performance Report (PPR) presents device survival estimates, advisory summaries, performance notes, and other information pertinent to assessing the performance of Medtronic implantable pulse generators (IPGs), implantable cardioverter defibrillators (ICDs), cardiac resynchronization therapy (CRT) devices, and implantable pacing and defibrillation leads.

This Product Performance Report has been prepared in accordance with International Standard ISO 5841- 2:2000(E).

The survival estimates provided in this report are considered to be representative of worldwide performance.

Survival Estimates

Medtronic, like other companies, monitors CRT, ICD, and IPG device performance using returned product analysis. We also monitor CRT, ICD, and IPG device performance using an active multicenter clinical study.

Returned product analysis is a passive approach to assessing product performance. This approach provides a suitable measure of product performance only when a significant number of explanted products are returned to the manufacturer. Returned product analysis provides a measure of hardware performance, but not necessarily the total clinical performance (e.g., the incidence of complications such as infection, erosion, muscle stimulation, etc. are not estimated).

The survival estimates provided in this report for CRT, ICD, and IPG devices are based on returned product analysis. This approach is suitable because a significant number of explanted generators are returned for analysis.

Lead performance is monitored differently. In contrast to CRT, ICD, and IPG devices, a very small percentage of leads are returned to the manufacturer due to the difficulty of explanting them. For leads, an active clinical study provides more accurate survival estimates compared to estimates based solely on returned product analysis.

Survival estimates for leads are based on clinical observations recorded via Medtronic's PAN Registry. This multicenter clinical study is designed to record clinical observations representative of the total clinical experience. Therefore, the lead survival estimates include both lead hardware failure and lead-related medical complications, and do not differentiate a lead hardware failure from other clinical events such as exit block, perforation, dislodgement, or concurrent pulse generator failure.

The actuarial life table method is applied to the data collected for CRT, ICD, and IPG devices and leads to provide the survival estimates included in this report. A general introduction to understanding this method of survival analysis is given later in this introduction.

ICD Charge Times

Since May 2000, Medtronic has provided important information on charge time performance of ICDs. The information provided in this report shows how ICD charge time can vary during the time a device is implanted. The information is presented in graphical format showing charge time as a function of implant time. The data for charge times are collected from devices enrolled in the PAN registry.

Introduction continued

Advisory Summaries

This Product Performance Report includes summaries of all advisories applicable to the performance of the products included in the report. An advisory is added to the report when any product affected by the advisory remains in service and at risk of experiencing the behavior described in the advisory. The advisory will remain in the report until Medtronic estimates no product affected by the advisory remains active, or the risk of experiencing the behavior described in the advisory has passed.

For most advisories, the products subject to the advisory retain essentially the same survival probability as the products of the same model(s) not affected by the advisory. For those advisories where the survival probabilities of the affected and non-affected populations do differ significantly, Medtronic will provide separate survival data for each population. The separate survival data will remain in the report until Medtronic estimates no affected product remains in active service.

Performance Notes

This report concludes with a number of Performance Notes developed by Medtronic to provide additional product performance information relevant to follow-up practice and patient management.

How You Can Help

Medtronic urges all physicians to return explanted products and to notify Medtronic when a product is no longer in use, regardless of the reason for explant or removal from use. The procedures for returning products vary by geographic location.

Mailer kits with prepaid US postage are available for use within the United States to send CRTs, ICDs, IPGs, ICMs, and leads to Medtronic's Cardiac Rhythm and Heart Failure (CRFH) Returned Product Analysis Lab. These mailers are sized to accommodate the devices and leads from a single patient or clinical event and are designed to meet US postal regulations for mailing biohazard materials.

If the product being returned is located outside the United States, please contact your local Medtronic representative for instructions.

Medtronic also requests the return of explanted products from non-clinical sources, such as funeral homes, and will assume responsibility for storage and disposal of the product once received.

Mailer kits can be obtained by contacting the Returned Product Lab. For information on how to contact the Lab, refer to the Contact Information page of this report.

We continually strive to improve this CRFH Product Performance Report. In keeping with this philosophy, we ask for your suggestions on the content and format of this report, as well as any information you have regarding the performance of Medtronic products. For information on how to comment on this report, see the Contact Information page.

Overview of Survival Analysis

Medtronic uses the Cutler-Ederer actuarial life table method for devices and Kaplan-Meier for leads to estimate the length of time over which they will perform within performance limits established by Medtronic. This probability to perform within performance limits over time is called the survival probability.

Devices and leads are followed until an event occurs where the device or lead ceases to operate within performance limits. The length of time from implant to the event is recorded for individual devices and leads in the population sample. The population sample for CRT, ICD, and IPG devices is made up of patients whose devices are registered as implanted in the United States. For leads, the population sample is the patients enrolled in our multicenter, international prospective Product Surveillance Registry.

Introduction continued

For CRTs, IPGs and ICDs, the events can be normal battery depletion or a device malfunction. For leads, the events are complications as defined in the study protocol.

The actuarial life table method allows Medtronic to account for devices and leads removed from service for reasons unrelated to performance and for device and leads still in service. Devices and leads removed for reasons unrelated to performance or are still in service are said to be suspended. Examples of devices and leads removed from service for reasons unrelated to performance include:

- Removed to upgrade the device or lead
- No longer in service due to the death of the patient for reasons unrelated to the device or leads
- Implanted in patients who are lost to follow-up

For each suspension, the device or lead has performed within performance limits for a period of time, after which its performance is unknown.

An Example

The following example describes the survival analysis method used to establish the survival probability estimates for Medtronic CRFH devices and leads. The example is intended to provide an overview of the analysis process. The definitions of malfunctions and complications, and other details specific to calculating device and lead survival estimates, are provided in the articles Method for Estimating CRT, ICD, and IPG Device Performance and Method for Estimating Lead Performance.

Figure 1 Implant times for devices of 16 patients. Gray bars with a yellow X indicate devices removed from service due to an event. Blue bars indicate suspended devices.

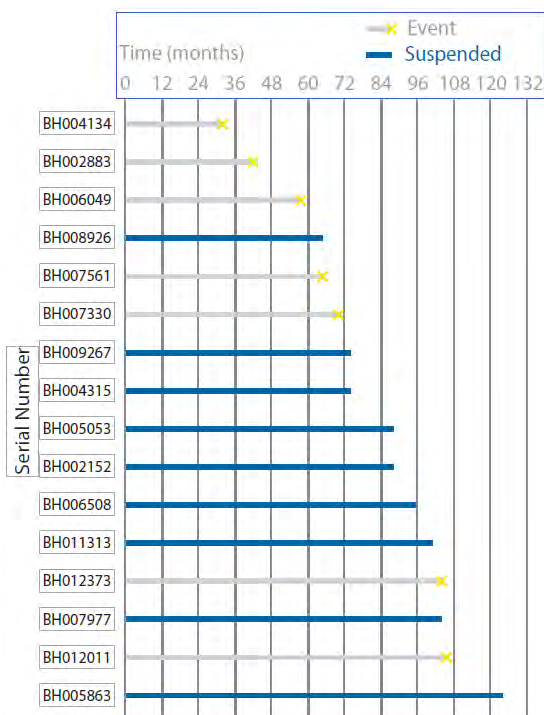


Figure 1 illustrates 16 patients who have implanted devices. The first patient's device (serial number BH004134) operated within performance limits for 32 months. At that time an event occurred. The fourth patient's device (serial number BH008926) did not have an event but is suspended, perhaps because it was still in service at the time of the analysis. This patient had 66 months of implant experience. In this example, Figure 1 shows that seven of the 16 devices suffered events, and nine are suspended.

The first step in the life table method is to divide the implant time into intervals of a specific length. This example will use 12-month intervals.

The number of devices entered, suspended, and removed due to an event are counted and summarized, as shown in Table 1. For the first two intervals, all 16 devices survived and none were removed. In the interval (24-36 months), device BH004134 was removed due to an event. Therefore the table entries show that 16 entered the interval, none were suspended, and one was removed due to an event.

For the interval from 36-48 months, only 15 devices entered the interval and one was removed for an event. The remaining intervals are examined and the data entered in columns A, B, and C in like manner. The rest of the columns are filled in using calculations on the data in columns A, B, and C.

Introduction continued

The Effective Sample Size (D) is the number of devices with full opportunity to experience a qualifying event in the interval. This is computed by subtracting one half the number suspended in the interval from the number that entered the interval. This calculation more accurately reflects the number of devices that could have experienced a qualifying event than simply using the number that entered the interval. Using the number of devices that enter an interval overestimates the sample size because the suspended devices do not complete the interval. Ignoring the suspended devices underestimates the sample size because suspended devices are not credited with their full service time. Using one half the number of suspended devices effectively splits the difference.

The next column in the table is the Proportion with Event (E). This is the proportion of devices that had an event in the interval. It is calculated by dividing the Number of Events (C) by the Effective Sample Size (D). The number can be interpreted as the estimated rate at which events occur in the time interval.

The Interval Survival Probability (F) is the estimate of probability of surviving to the end of the interval assuming the device was working at the beginning of the interval. It is calculated as 1 minus the Proportion with Event (E). This number can be interpreted as the estimated rate at which events do not occur in the time interval.

Table 1 Life Table for Figure 1

| | A | B | C | D | E | F | G |
|--------------------|----------------|------------------|------------------|-----------------------|-----------------------|-------------------------------|---------------------------------|
| Interval in Months | Number Entered | Number Suspended | Number of Events | Effective Sample Size | Proportion with Event | Interval Survival Probability | Cumulative Survival Probability |
| 0 | 16 | 0 | 0 | 16 | 0.000 | 1.000 | 1.000 |
| 0-12 | 16 | 0 | 0 | 16 | 0.000 | 1.000 | 1.000 |
| 12-24 | 16 | 0 | 0 | 16 | 0.000 | 1.000 | 1.000 |
| 24-36 | 16 | 0 | 1 | 16 | 0.063 | 0.938 | 0.938 |
| 36-48 | 15 | 0 | 1 | 15 | 0.067 | 0.933 | 0.875 |
| 48-60 | 14 | 0 | 1 | 14 | 0.071 | 0.929 | 0.813 |
| 60-72 | 13 | 1 | 2 | 12.5 | 0.160 | 0.840 | 0.683 |
| 72-84 | 10 | 2 | 0 | 9 | 0.000 | 1.000 | 0.683 |
| 84-96 | 8 | 3 | 0 | 6.5 | 0.000 | 1.000 | 0.683 |
| 96-108 | 5 | 2 | 2 | 4 | 0.500 | 0.500 | 0.341 |
| 108-120 | 1 | 0 | 0 | 1 | 0.000 | 1.000 | 0.341 |
| 120-132 | 1 | 1 | 0 | 0.5 | 0.000 | 1.000 | 0.341 |


Definitions:

| A | B | C | D | E | F | G |
|---|--|--|--|--|---|--|
| Number Entered | Number Suspended | Number of Events | Effective Sample Size | Proportion with Event | Interval Survival Probability | Cumulative Survival Probability |
| Number of devices active at the start of the interval | Number of devices removed from service for reasons other than an event | Number of units removed from service due to an event | Number of units with full opportunity to experience a qualifying event in the interval. Computed by subtracting one half the Number Suspended from the Number Entered. | Proportion of devices that had an event in the interval. Computed by dividing the Number of Events by the Effective Sample Size. | The probability of surviving to the end of the interval, assuming the device was working at the beginning of the interval. Computed as 1 minus the Proportion With Event. | The overall probability of surviving to the end of the interval. Computed by multiplying the Interval Survival Probability by the previous interval's Cumulative Survival Probability. |

Introduction continued

Cumulative Survival Probability (G) is the estimate of the unconditional probability of surviving to the end of the interval. It is computed by multiplying the Interval Survival Probability (F) by the previous interval's Cumulative Survival Probability. The probability of surviving to 132 months in the example is estimated for the table to be 0.341, or 34.1%. The Cumulative Survival Probabilities (G) of the life table can be plotted versus time intervals in the first column to give a survival curve. Figure 2 shows the survival curve for the data in Table 1.

Figure 2 Survival Curve for Data Given in Table 1

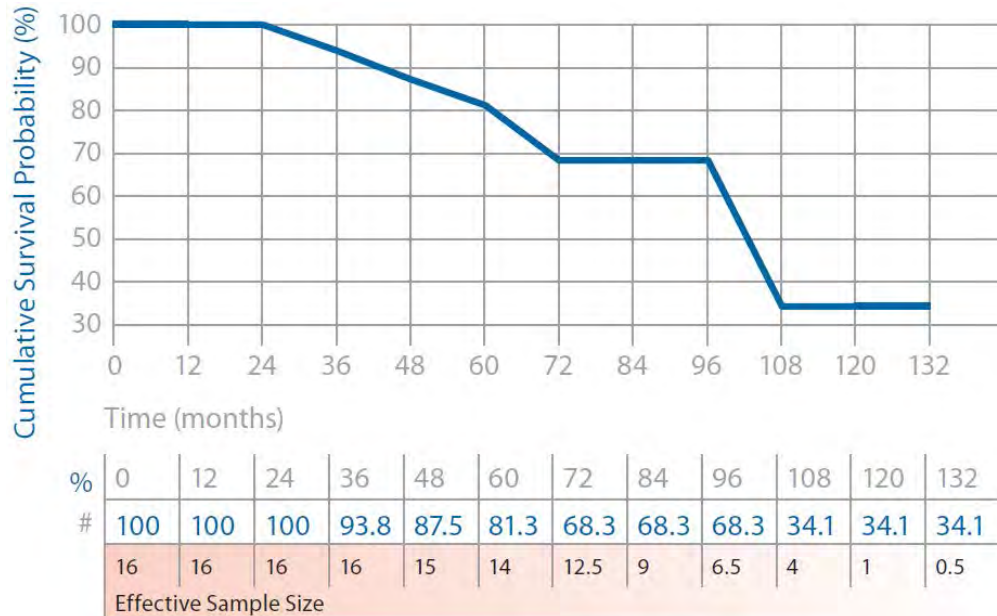

Confidence Intervals

Since survival curves are based on a sample of the device and lead population, they are only estimates of survival. The larger the effective sample size, the more confident the estimate. A confidence interval can be calculated to assess the confidence in an estimate. In the Product Performance Report, Medtronic provides a 95% confidence interval. This can be interpreted as meaning that 95% of the time, the true survival of the device will fall somewhere in the interval.

Survival Curves in the Product Performance Report

Since the survival estimate can become very imprecise with small effective sample sizes, Medtronic truncates the survival curve when the effective sample size is less than 100 for CRTs, ICDs, and IPGs, and when the number entered is less than 50 for leads. The survival charts in the Product Performance Report show the effective sample size for each year interval where Medtronic has experience. When the effective sample size reaches 100 for CRTs, ICDs, and IPGs or when the number entered reaches 50 for leads, the next data point is added to the survival curve.

Although the report provides tabular data in one-year intervals, the device curves are actually computed and plotted using the Cutler-Ederer method and 1-month intervals (for CRT, ICD, and IPG devices) and leads curves are computed and plotted using Kaplan-Meier, which uses individual survival times.

A number of references are available for additional information on survival analysis using the Cutler-Ederer life table method¹ and for the Kaplan-Meier method.²

¹ Lee, Elisa T. (2003) *Statistical Methods for Survival Data Analysis – 3rd Edition* (Wiley Series in Probability and Statistics).

² Klein, John P., Moeschberger, Melvin L. *Survival Analysis Techniques for Censored and Truncated Data*, New York: Springer-Verlag New York, Inc., 1997.

Method for Estimating CRT, ICD, and IPG Device Performance

The performance of CRT, ICD, and IPG devices is expressed in terms of device survival estimates, where “survival” refers to the function of the device, not the survival of the patient. These survival estimates are intended to illustrate the probability that a device will survive for a given number of years without malfunction or battery depletion.

The survival estimates are determined from the analysis of Medtronic Cardiac Rhythm and Heart Failure (CRHF’s) United States device registration data and US returned product analysis data. These data are presented graphically and numerically.

Because this analysis is based on returned product analysis, the performance data does not reflect any device-related medical complications such as erosion, infection, muscle stimulation, or muscle inhibition.

Categorization of Depleted and Malfunctioning Devices for Survival Analysis

For survival estimation, every device returned to Medtronic CRHF and analyzed in the CRHF Returned Product Analysis laboratory is assigned to one of three categories. The device 1) is functioning normally, 2) has reached normal battery depletion, or 3) has malfunctioned. This categorization is combined with data from our device registry for the total number of implants and the implant durations to create the survival curves presented on the following pages.

Definition of Malfunction

Medtronic CRHF considers a device as having malfunctioned whenever the analysis shows that any parameter was outside the performance limits established by Medtronic while implanted and in service. To be considered a malfunction or battery depletion, the device must have been returned to Medtronic and analyzed.

Devices damaged after explant, damaged due to failure to heed warnings or contraindications in the labeling, or damaged due to interaction with other implanted devices (including leads) are not considered device malfunctions.

A device subject to a safety advisory is not considered to have malfunctioned unless it has been returned to Medtronic CRHF and found, through analysis, to actually have performed outside the performance limits established by Medtronic.

Not all malfunctions expose the patient to a loss of therapy. Some malfunctions included in the following survival estimates may not have been detected at all by the physician or the patient. These malfunctions, however, are included in the survival estimates and provide important feedback to our product development organization.

To provide insight into the nature of malfunctions, each malfunction is categorized as Malfunction with Compromised Therapy Function or Malfunction without Compromised Therapy Function.

For this report, Normal Battery Depletion, Malfunction with Compromised Therapy Function, and Malfunction without Compromised Therapy Function are defined as follows:

Normal Battery Depletion – The condition when:

- (a) a device is returned with no associated complaint and the device has reached its elective replacement indicator(s) with implant time that meets or exceeds the nominal (50 percentile) predicted longevity at default (labeled) settings, or
- (b) a device is returned and the device has reached its elective replacement indicator(s) with implant time exceeding 80% of the expected longevity calculated using the available device setting information.

Method for Estimating CRT, ICD, and IPG Device Performance

continued

Medtronic CRHF establishes expected longevity by statistically characterizing the power consumed by the device and the power available from the device battery. This characterization is applied to a number of parameter configurations to derive a statistical mean longevity value and standard deviation for each parameter configuration. The statistical mean value minus three standard deviations is used as the expected longevity for determining if a battery depleted normally. The actual longevity achieved for any device while implanted will depend on the actual programmed parameters and patient factors, and may differ significantly from these estimates.

Malfunction with Compromised Therapy Function

The condition when a device is found to have malfunctioned in a manner that compromised pacing or defibrillation therapy (including complete loss or partial degradation), while implanted and in service, as confirmed by returned product analysis.

Examples: Sudden loss of battery voltage; accelerated current drain such that low battery was not detected before loss of therapy; sudden malfunction during defibrillation therapy resulting in aborted delivery of therapy, intermittent malfunction where therapy is compromised while in the malfunction state.

Malfunction without Compromised Therapy Function

The condition when a device is found to have malfunctioned in a manner that did not compromise pacing or defibrillation therapy, while implanted and in service, as confirmed by returned product analysis.

Examples: Error affecting diagnostic functions, telemetry function, data storage; malfunction of a component that causes battery to lose power quickly enough to cause premature battery depletion, but slowly enough that the condition is detected through normal follow-up before therapy is lost; mechanical problems with connector header that do not affect therapy.

Expanded Malfunction Detail

The malfunctions are further divided into categories that identify the subject area of the malfunction. The malfunctions are divided into the following subject areas:

Electrical Component – Findings linked to electrical components such as integrated circuits, resistors, capacitors, diodes, etc.

Electrical Interconnect – Findings linked to the connections between electrical components such as wires, solder joints, wire bonds, etc.

Battery – Findings linked to the battery and its components

Software/Firmware – Findings linked to software or firmware function

Possible Early Battery Depletion – Findings where the actual reported implant time is less than 80% of the expected longevity calculated using the available device setting information with no device malfunction observed. There may not be sufficient device setting information to determine conclusively if battery depletion was normal or premature in the absence of a specific root cause finding. However, returned devices meeting the above criteria are conservatively classified as Possible Early Battery Depletion malfunctions.

Other – Findings related to other components such as insulators, grommets, setscrews, and packaging, and findings where analysis is inconclusive.

Method for Estimating CRT, ICD, and IPG Device Performance

continued

Returned Product Analysis Process

Analysis of returned product is performed according to written procedures. These procedures determine the minimum analysis required. The analysis required varies depending on the type of device, age of the device, the associated information received with the device, actual experience with models of similar design, and other factors. Additional analysis is performed as necessary to investigate a performance concern from a customer, or to collect specific reliability data.

When a device is returned with a performance concern from a customer, the general analysis process includes a preliminary analysis of the device in its as-received condition, followed by an automated functional test using test equipment equivalent to the equipment used in manufacturing.

When a malfunction is identified, failure analysis is performed to provide the detailed information necessary to investigate possible causes and actions. Medtronic CRHF maintains in-house expertise and performs its failure analysis using facilities it owns and supports. This capability permits detailed failure analysis.

Statistical Methods for Survival Analysis

Of the several different statistical methods available for survival analysis, the Standard Actuarial Method, with suspensions assumed distributed evenly within the intervals (Cutler-Ederer Method), is used to determine survival estimates for CRT, IPG and ICD devices. Implant times are calculated from the implant date to the earlier of the explant date or the cutoff date of the report. From this data an estimate of the probability of device survival is calculated at each monthly interval.

On the following pages, each graph includes a survival curve where events include malfunctions and normal battery depletions. This survival curve is a good representation of the probability a device will survive a period of time without malfunction and without battery depletion. For example, if a device survival probability is 95% after 5 years of service, then the device has a 5% chance of being removed due to battery depletion or malfunction in the first 5 years following implant.

In addition, a second curve is included to show survival excluding normal battery depletion. This curve is a good representation of the probability for a device to survive without malfunction. This curve includes only malfunctions as events and excludes normal battery depletion.

Since the survival estimate can become very imprecise with small effective sample sizes, Medtronic truncates the survival curve when the effective sample size is less than 100 for CRT, ICD, and IPG devices. The survival charts in the Product Performance Report show the effective sample size for each year interval where we have experience. When the effective sample size reaches 100, the next data point is added to the survival curve.

Although the report provides tabular data in one-year intervals, the curves are actually computed and plotted using one-month intervals.

The data in the tables are rounded to the nearest tenth of one percent. Occasionally, a graph may show 100% survival, but have one or more malfunctions or battery depletions. This occurs because, even with the malfunctions or battery depletions, the data rounds to 100%.

Sample Size and How the Population and Population Samples Are Defined

The population sample from which the survival estimates are derived is comprised of the devices registered as implanted in the United States as of the report cutoff date. The number of registered implants, as well as an estimate of the number that remain in active service, is listed for each model. To be included in the population, the device must have been registered with Medtronic's registration system and implanted for at least one day.

Method for Estimating CRT, ICD, and IPG Device Performance

continued

This sample based on US implants is considered to be representative of the worldwide population, and therefore the survival estimates shown in this report should be representative of the performance worldwide of these models.

A CRT, ICD, or IPG model or model family will be included in this report when it has accumulated at least 10,000 implant months and will remain in the report as long as at least 500 devices remain active.

Methods Used to Adjust for Underreporting of Malfunction and Battery Depletion

The tables on the following pages show the actual number of malfunctions and battery depletions recorded by the analysis lab for US registered devices. Since not all devices are returned to Medtronic CRHF for analysis, these numbers underestimate the true number of malfunctions and battery depletions. To more accurately estimate the all-cause device survival probabilities, the number of malfunctions and battery depletions used to plot each interval of the all-cause survival curves is adjusted (multiplied) by a factor that is based on an estimate of the magnitude of underreporting. The magnitude of underreporting is estimated by comparing data in Medtronic's Device And Registrant Tracking (DART) system with data from Returned Product Analysis.

The DART system is an important element of Medtronic's Quality System. The DART system is designed to meet or exceed the US FDA's device tracking requirements set forth by the Safe Medical Devices Act. In the United States, over 98% of Medtronic's CRT, ICD, and IPG implants become registered in the DART system.

Because pacemakers do not cure the patient's underlying health problem, when a pacemaker stops functioning (due to either normal battery replacement or malfunction) it is replaced with a new pacemaker. Therefore, the replacement recorded in the DART system is a good indication that the previous pacemaker experienced either battery depletion or malfunction. The fraction of replaced devices that are subsequently returned can be used to estimate the correction factor for the under reporting of the combination of battery depletion and malfunction.

Note that devices of patients who have expired do not factor into the calculation of the correction. It is possible some proportion of these devices experienced battery depletion or malfunction. Since these are not counted into the correction factor based on the return rate of replaced devices, a correction factor based only on the return rate of replaced devices may still underestimate the true rate of battery depletion and malfunction. However, devices that are replaced because the patient is receiving a system upgrade or are removed because the patient no longer needs it (e.g., due to heart transplant) do contribute to the calculation of the correction factor and therefore impart an opposite bias.

Also note that this method of calculating the correction factor cannot distinguish between devices that are removed due to malfunction and those due to normal battery depletion. It might seem intuitive that devices that unexpectedly malfunction should be much more likely to be returned to the manufacturer than a device with ordinary normal battery depletion. But this has not been conclusively demonstrated. Therefore, this method only provides a correction factor reflecting the combination of battery depletion and malfunction.

No adjustment for underreporting is applied to the malfunction-free survival curve because a method for estimating malfunction-only underreporting has not been developed.

Adjustments to Registered Implants to Compensate for Unreported Devices Removed from Service

Devices are at times removed from service for reasons other than device malfunction or battery depletion. Examples are devices removed from service due to non-device related patient mortality and devices removed due to changes in the patient's medical condition. Because an accurate estimate of device survival depends on an accurate estimate of the number of devices in service, it is important not to overstate the number of devices in service.

Method for Estimating CRT, ICD, and IPG Device Performance

continued

Medtronic addresses this under reporting to ensure the number of devices in service is not overstated . Regular updates obtained from the Social Security Administration about deceased persons are used to update Medtronic's DART data about patients who have died but whose deaths had not been reported to Medtronic. In addition, the patient mortality rate derived from our DART system is monitored and compared to published mortality rates for comparable patient populations. If, during calculation of the survival curves, the patient mortality indicated by the data in DART is significantly different from published rates, an adjustment is applied to correct the difference. The correction factor for under reporting devices is also applied to account for devices that were removed and not reported or returned.

Cardiac Resynchronization Therapy


7285

InSync III Protect

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 04/07/2004 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 30 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

7285, 7295, Survival Curve

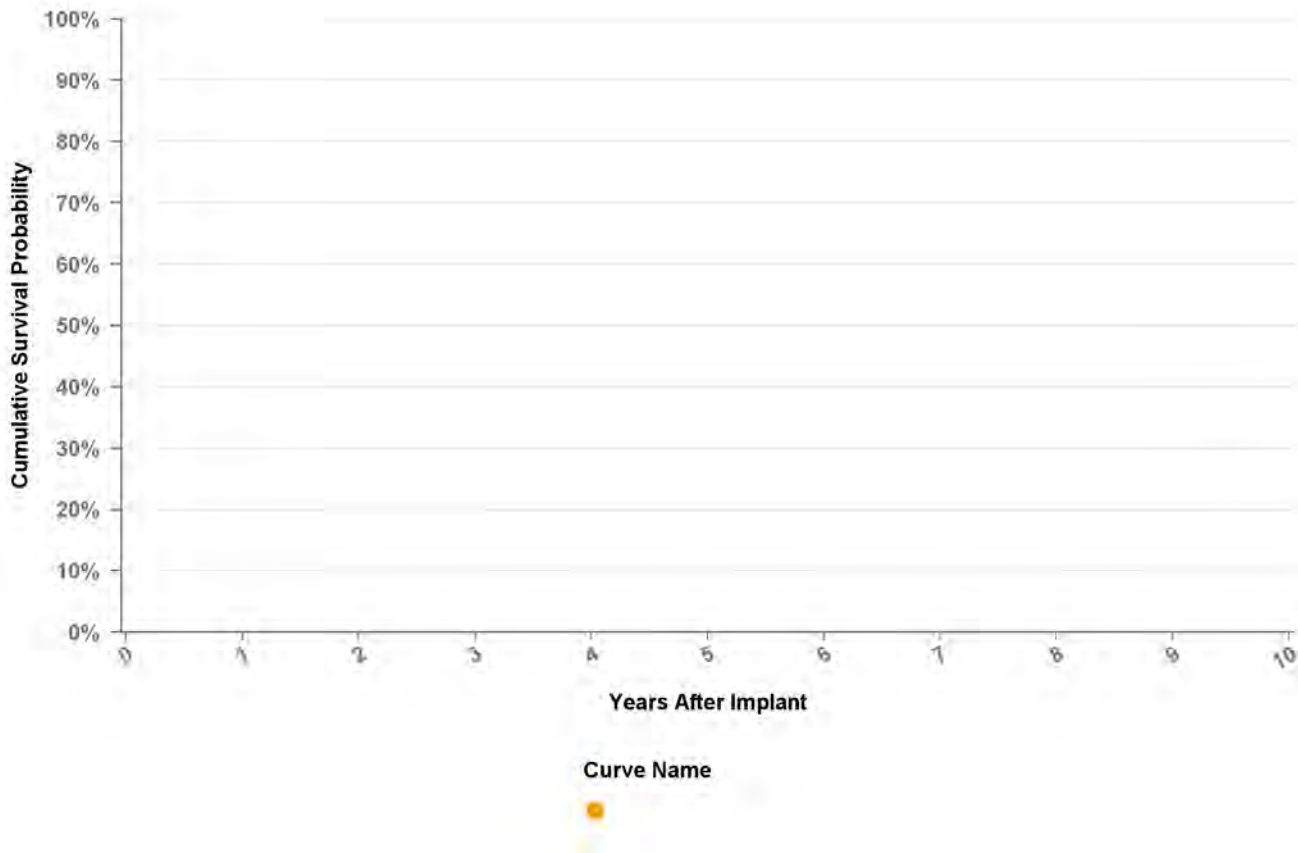

Years

Excluding NBD

Including NBD

Effective Sample Size

Cardiac Resynchronization Therapy


7295

InSync II Protect

| | |
|---------------------------------------|------------|
| US Market Release Date | 02/02/2004 |
| CE Market Approval Date | |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 30 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

7285, 7295, Survival Curve

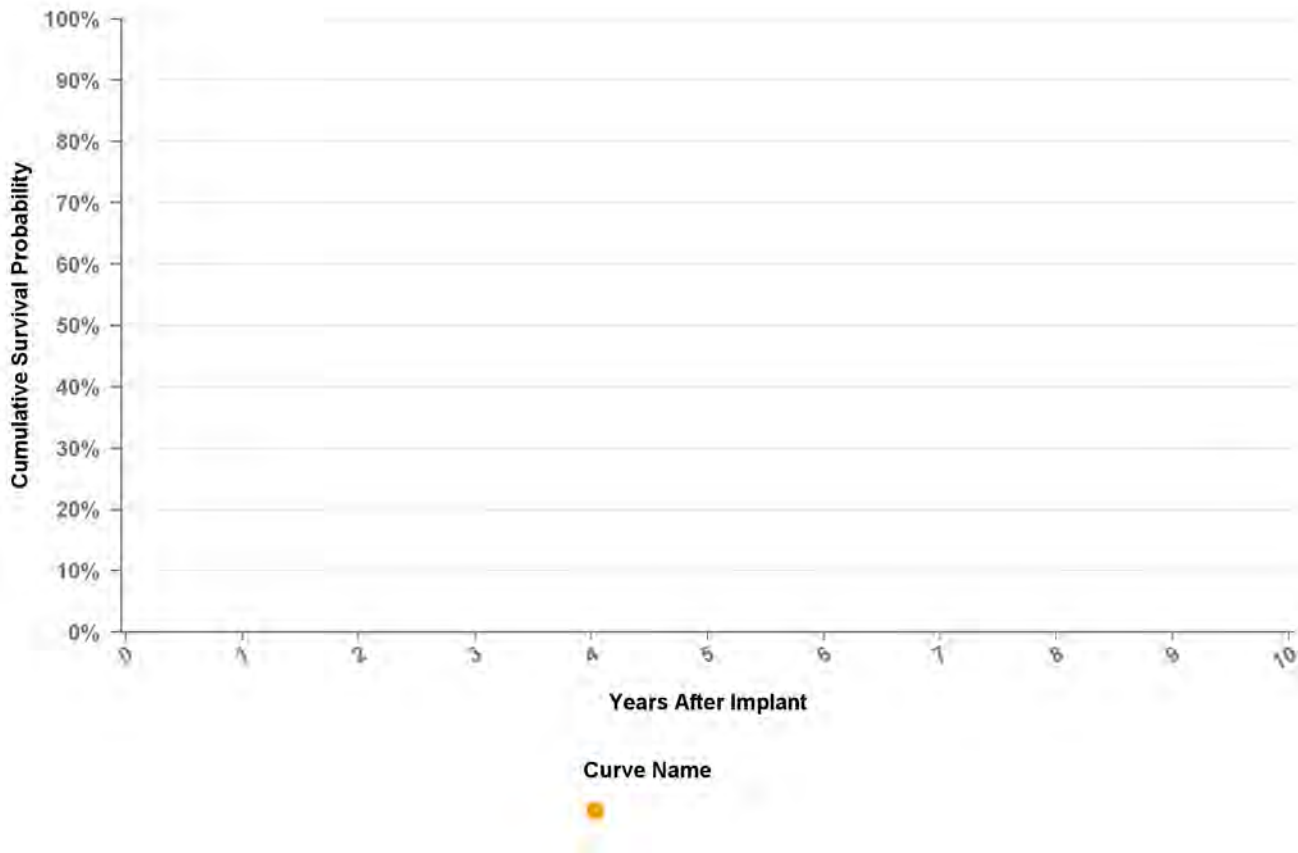

Years

Excluding NBD

Including NBD

Effective
Sample Size

Cardiac Resynchronization Therapy

7299

InSync Sentry

Total Malfunctions (US)

179

Therapy Not Compromised Malfunctions

169

Battery Malfunction 0

Electrical Component 19

Electrical Interconnect 0

Other Malfunction 1

Poss Early Battery Depltn 147

Software Malfunction 2

Therapy Compromised Malfunctions

10

Battery Malfunction 0

Electrical Component 10

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

US Market Release Date 04/08/2005

CE Market Approval Date

Registered US Implants 31,184


Estimated Active US Implants 1,974

Normal Battery Depletions (US) 9,906

NBG Code VVE-DDDR

Max Delivered Energy 35 J

7299, Survival Curve

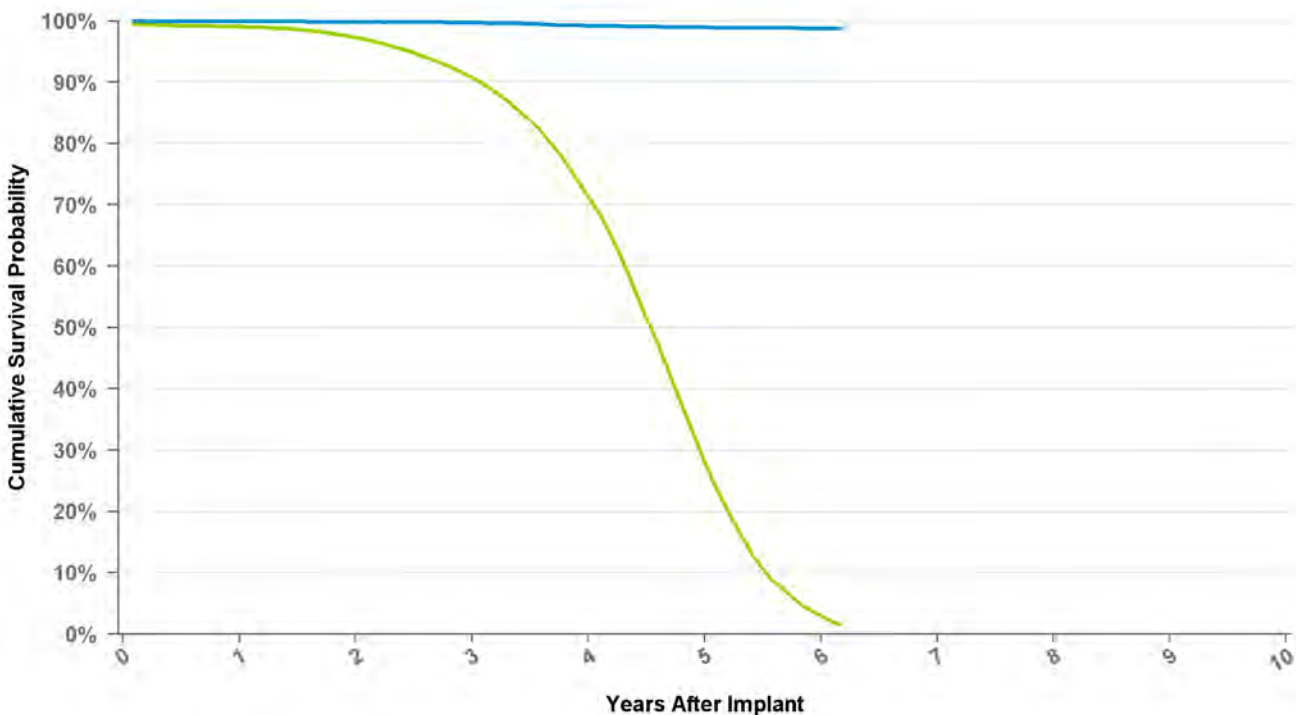

Curve Name

● Excluding Normal Battery Depletion

● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 74 mo |
|-----------------------|--------|-------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.7% | 99.2% | 99.0% | 98.8% | 98.8% |
| Including NBD | 99.1% | 97.3% | 90.7% | 71.4% | 28.1% | 3.0% | 1.5% |
| Effective Sample Size | 27077 | 23696 | 19200 | 12911 | 4472 | 318 | 146 |


Cardiac Resynchronization Therapy

7304

InSync Maximo

| | |
|---------------------------------------|------------|
| US Market Release Date | 04/08/2005 |
| CE Market Approval Date | 01/14/2005 |
| Registered US Implants | 18,985 |
| Estimated Active US Implants | 1,454 |
| Normal Battery Depletions (US) | 5,565 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|-----|
| Total Malfunctions (US) | 114 |
| Therapy Not Compromised Malfunctions | 109 |
| Battery Malfunction | 1 |
| Electrical Component | 15 |
| Electrical Interconnect | 0 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 92 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 5 |
| Battery Malfunction | 0 |
| Electrical Component | 4 |
| Electrical Interconnect | 0 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

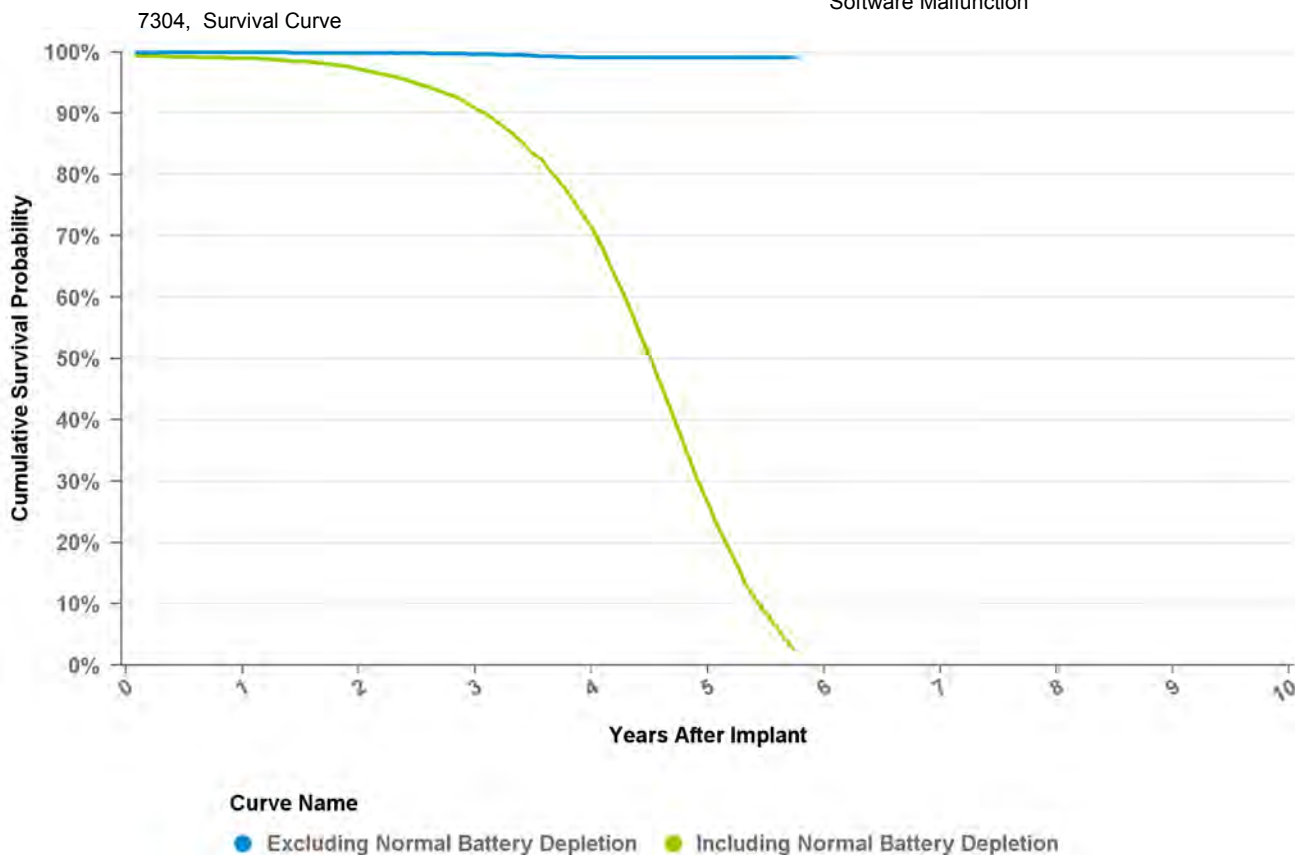


| Years | 1 | 2 | 3 | 4 | 5 | at 69 mo |
|------------------------------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.6% | 99.1% | 99.1% | 99.1% |
| Including NBD | 99.0% | 97.2% | 90.8% | 71.5% | 26.6% | 2.5% |
| Effective Sample Size | 16802 | 14690 | 11949 | 8034 | 2420 | 208 |

Cardiac Resynchronization Therapy

C154DWK Concerto CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | 05/12/2006 |
| CE Market Approval Date | |
| Registered US Implants | 81,309 |
| Estimated Active US Implants | 13,363 |
| Normal Battery Depletions (US) | 22,779 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|-------|
| Total Malfunctions (US) | 1,424 |
| Therapy Not Compromised Malfunctions | 1,377 |
| Battery Malfunction | 0 |
| Electrical Component | 717 |
| Electrical Interconnect | 2 |
| Other Malfunction | 3 |
| Poss Early Battery Depltn | 651 |
| Software Malfunction | 4 |
| Therapy Compromised Malfunctions | 47 |
| Battery Malfunction | 0 |
| Electrical Component | 45 |
| Electrical Interconnect | 2 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

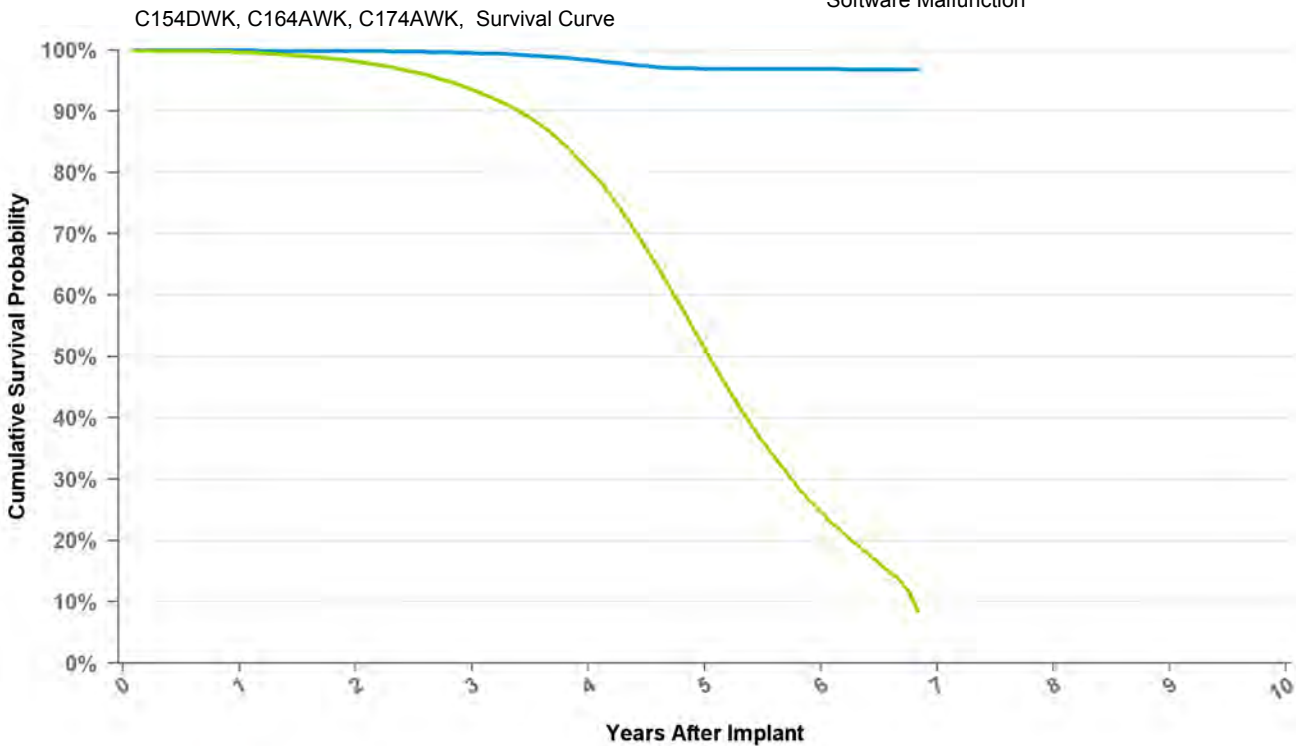

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 82 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.8% | 99.5% | 98.4% | 96.9% | 96.9% | 96.8% |
| Including NBD | 99.6% | 98.1% | 93.5% | 80.6% | 51.4% | 24.7% | 8.5% |
| Effective Sample Size | 72761 | 64326 | 54951 | 42868 | 24424 | 7191 | 317 |

Cardiac Resynchronization Therapy

C164AWK Concerto CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | 04/17/2007 |
| CE Market Approval Date | |
| Registered US Implants | 178 |
| Estimated Active US Implants | 5 |
| Normal Battery Depletions (US) | 72 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 4 |
| Therapy Not Compromised Malfunctions | 4 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 4 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

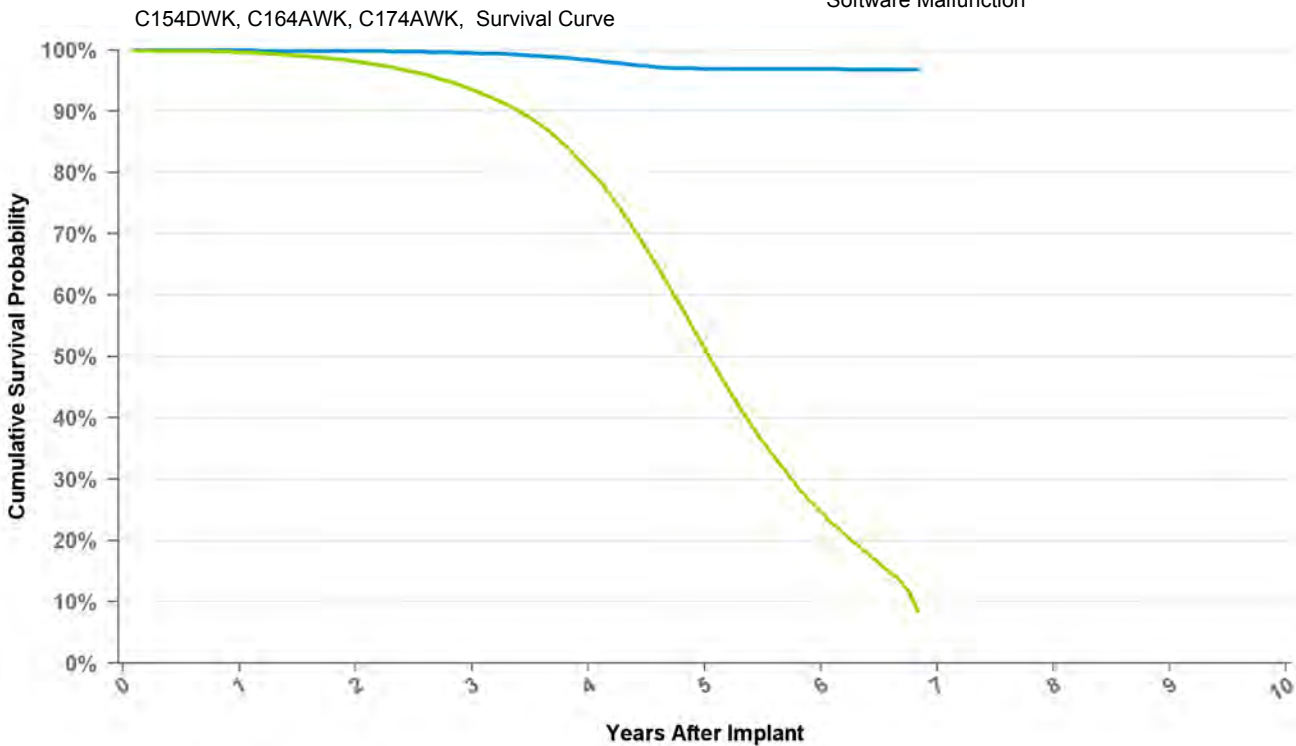

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 82 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.8% | 99.5% | 98.4% | 96.9% | 96.9% | 96.8% |
| Including NBD | 99.6% | 98.1% | 93.5% | 80.6% | 51.4% | 24.7% | 8.5% |
| Effective Sample Size | 72761 | 64326 | 54951 | 42868 | 24424 | 7191 | 317 |

Cardiac Resynchronization Therapy

C174AWK Concerto CRT-D

US Market Release Date

CE Market Approval Date 03/07/2006

Registered US Implants 5

Estimated Active US Implants 3

Normal Battery Depletions (US) 0

NBG Code DDE-DDDR

Max Delivered Energy 35 J

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

C154DWK, C164AWK, C174AWK, Survival Curve

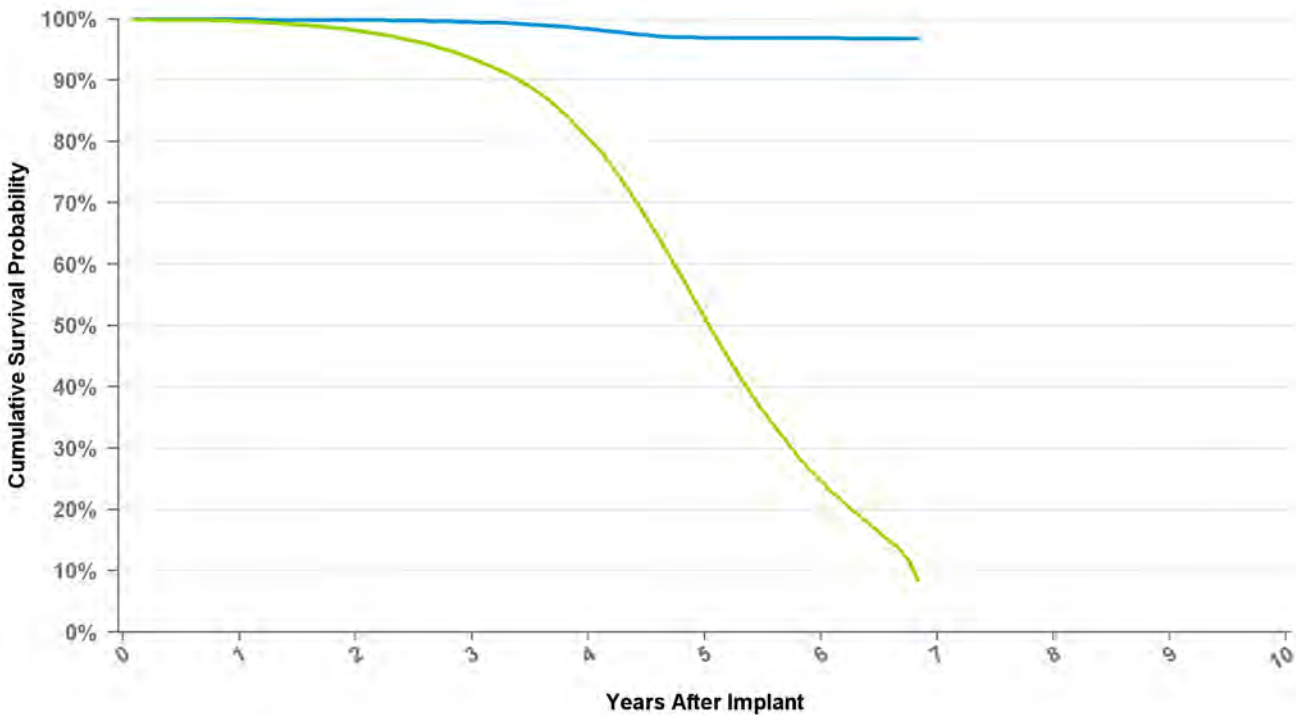

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 82 mo |
|-----------------------|--------|-------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.8% | 99.5% | 98.4% | 96.9% | 96.9% | 96.8% |
| Including NBD | 99.6% | 98.1% | 93.5% | 80.6% | 51.4% | 24.7% | 8.5% |
| Effective Sample Size | 72761 | 64326 | 54951 | 42868 | 24424 | 7191 | 317 |

Cardiac Resynchronization Therapy

D204TRM Consulta CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/09/2012 |
| CE Market Approval Date | |
| Registered US Implants | 2,080 |
| Estimated Active US Implants | 1,874 |
| Normal Battery Depletions (US) | 12 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 1 |
| Therapy Not Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

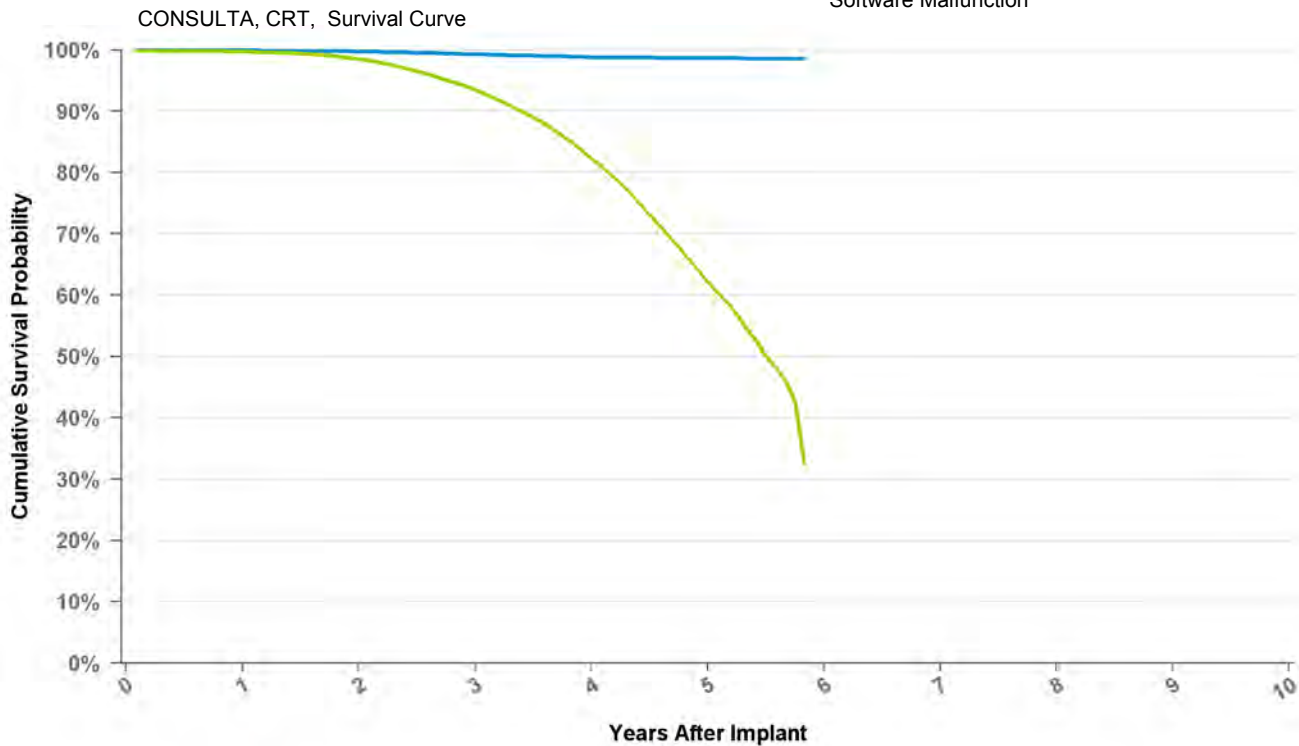

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | at 70 mo |
|------------------------------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.7% | 99.3% | 98.8% | 98.7% | 98.6% |
| Including NBD | 99.7% | 98.5% | 93.5% | 82.3% | 62.2% | 32.5% |
| Effective Sample Size | 62504 | 54612 | 43556 | 27821 | 7662 | 154 |

Cardiac Resynchronization Therapy

D214TRM Consulta CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 07/22/2010 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

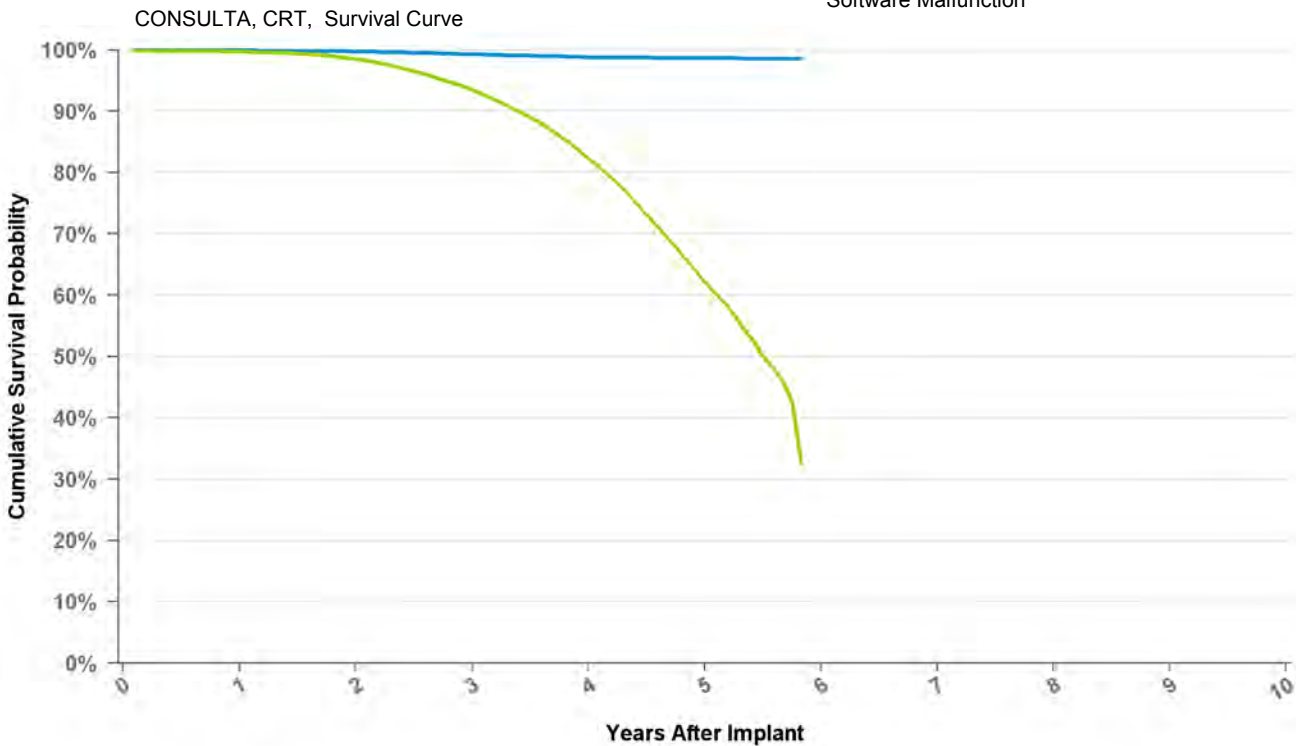

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | at 70 mo |
|------------------------------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.7% | 99.3% | 98.8% | 98.7% | 98.6% |
| Including NBD | 99.7% | 98.5% | 93.5% | 82.3% | 62.2% | 32.5% |
| Effective Sample Size | 62504 | 54612 | 43556 | 27821 | 7662 | 154 |

Cardiac Resynchronization Therapy

D224TRK Consulta CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | 09/15/2008 |
| CE Market Approval Date | |
| Registered US Implants | 65,770 |
| Estimated Active US Implants | 33,720 |
| Normal Battery Depletions (US) | 8,368 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|-----|
| Total Malfunctions (US) | 567 |
| Therapy Not Compromised Malfunctions | 546 |
| Battery Malfunction | 2 |
| Electrical Component | 43 |
| Electrical Interconnect | 1 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 493 |
| Software Malfunction | 6 |
| Therapy Compromised Malfunctions | 21 |
| Battery Malfunction | 1 |
| Electrical Component | 20 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

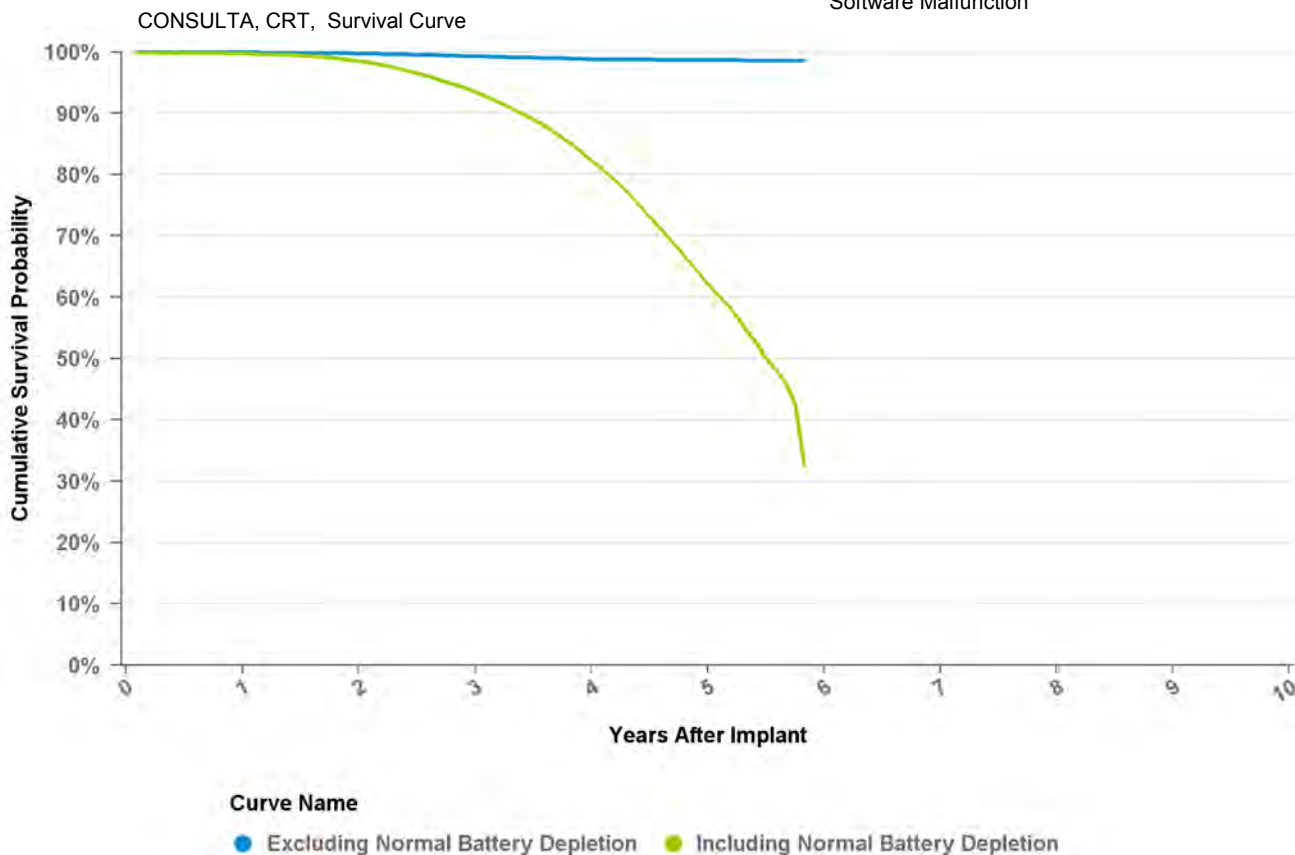


| Years | 1 | 2 | 3 | 4 | 5 | at 70 mo |
|------------------------------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.7% | 99.3% | 98.8% | 98.7% | 98.6% |
| Including NBD | 99.7% | 98.5% | 93.5% | 82.3% | 62.2% | 32.5% |
| Effective Sample Size | 62504 | 54612 | 43556 | 27821 | 7662 | 154 |

Cardiac Resynchronization Therapy

D234TRK Consulta CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 03/14/2008 |
| Registered US Implants | 1 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

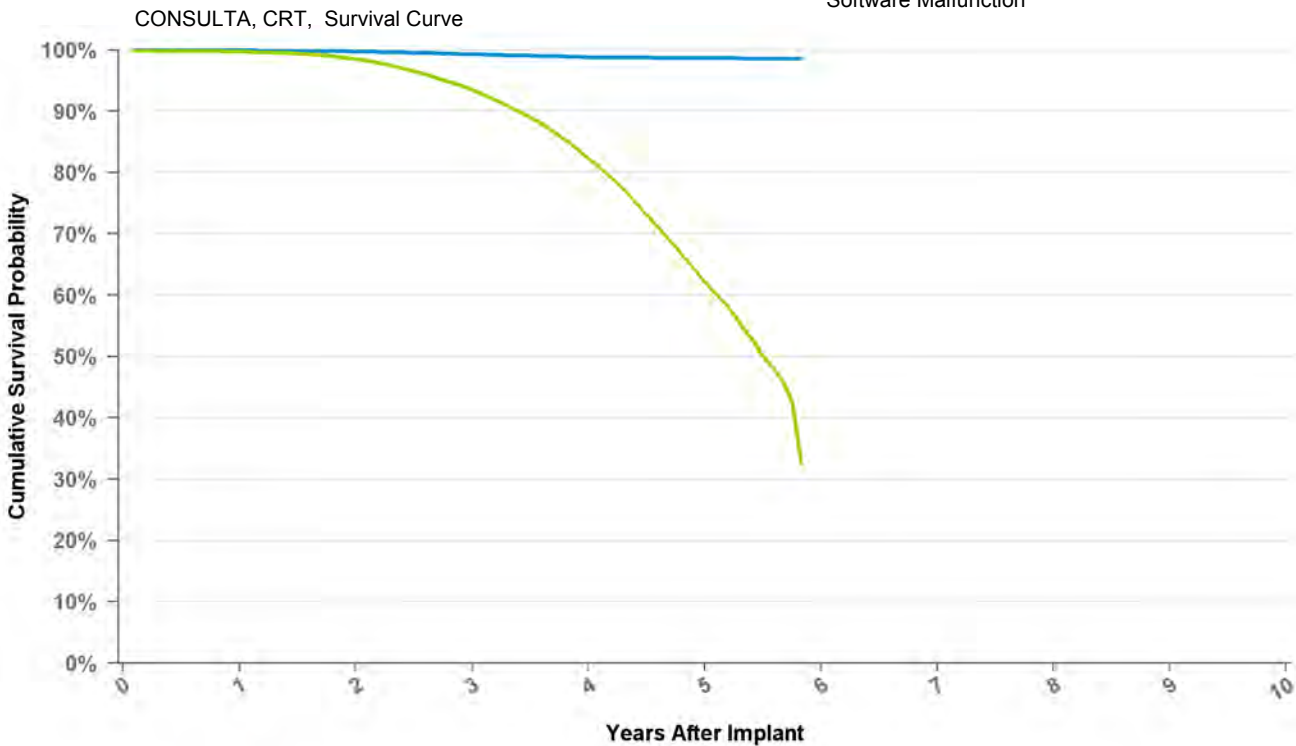

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | at 70 mo |
|------------------------------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.7% | 99.3% | 98.8% | 98.7% | 98.6% |
| Including NBD | 99.7% | 98.5% | 93.5% | 82.3% | 62.2% | 32.5% |
| Effective Sample Size | 62504 | 54612 | 43556 | 27821 | 7662 | 154 |

Cardiac Resynchronization Therapy

D264TRM Maximo II CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/09/2012 |
| CE Market Approval Date | 07/22/2010 |
| Registered US Implants | 15 |
| Estimated Active US Implants | 13 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

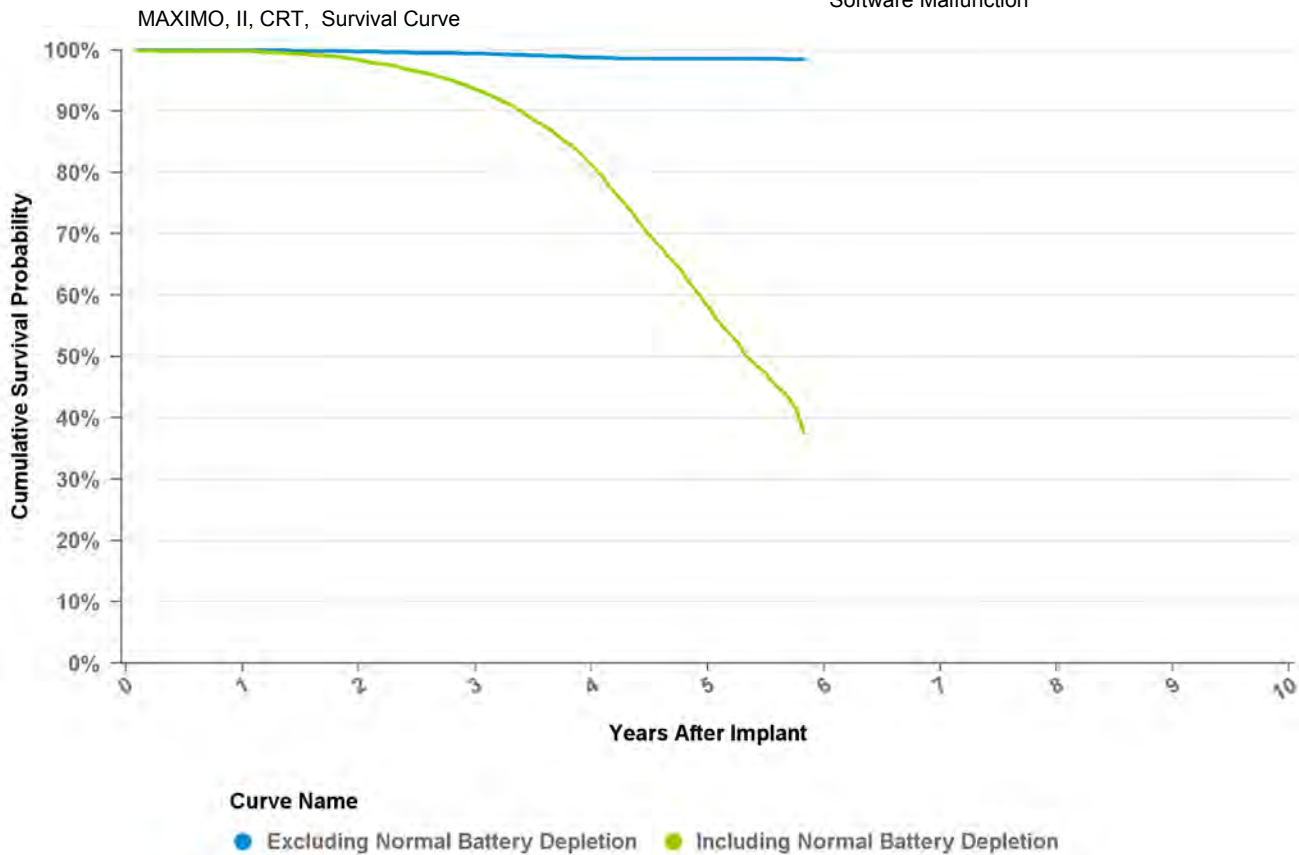


| Years | 1 | 2 | 3 | 4 | 5 | at 70 mo |
|------------------------------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.7% | 99.4% | 98.8% | 98.6% | 98.5% |
| Including NBD | 99.8% | 98.4% | 93.6% | 81.3% | 58.3% | 37.4% |
| Effective Sample Size | 14141 | 12273 | 9752 | 6100 | 1971 | 145 |

Cardiac Resynchronization Therapy

D274TRK Concerto II CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | 08/15/2009 |
| CE Market Approval Date | |
| Registered US Implants | 30,166 |
| Estimated Active US Implants | 16,579 |
| Normal Battery Depletions (US) | 3,266 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|-----|
| Total Malfunctions (US) | 175 |
| Therapy Not Compromised Malfunctions | 170 |
| Battery Malfunction | 1 |
| Electrical Component | 16 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 152 |
| Software Malfunction | 1 |
| Therapy Compromised Malfunctions | 5 |
| Battery Malfunction | 1 |
| Electrical Component | 4 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

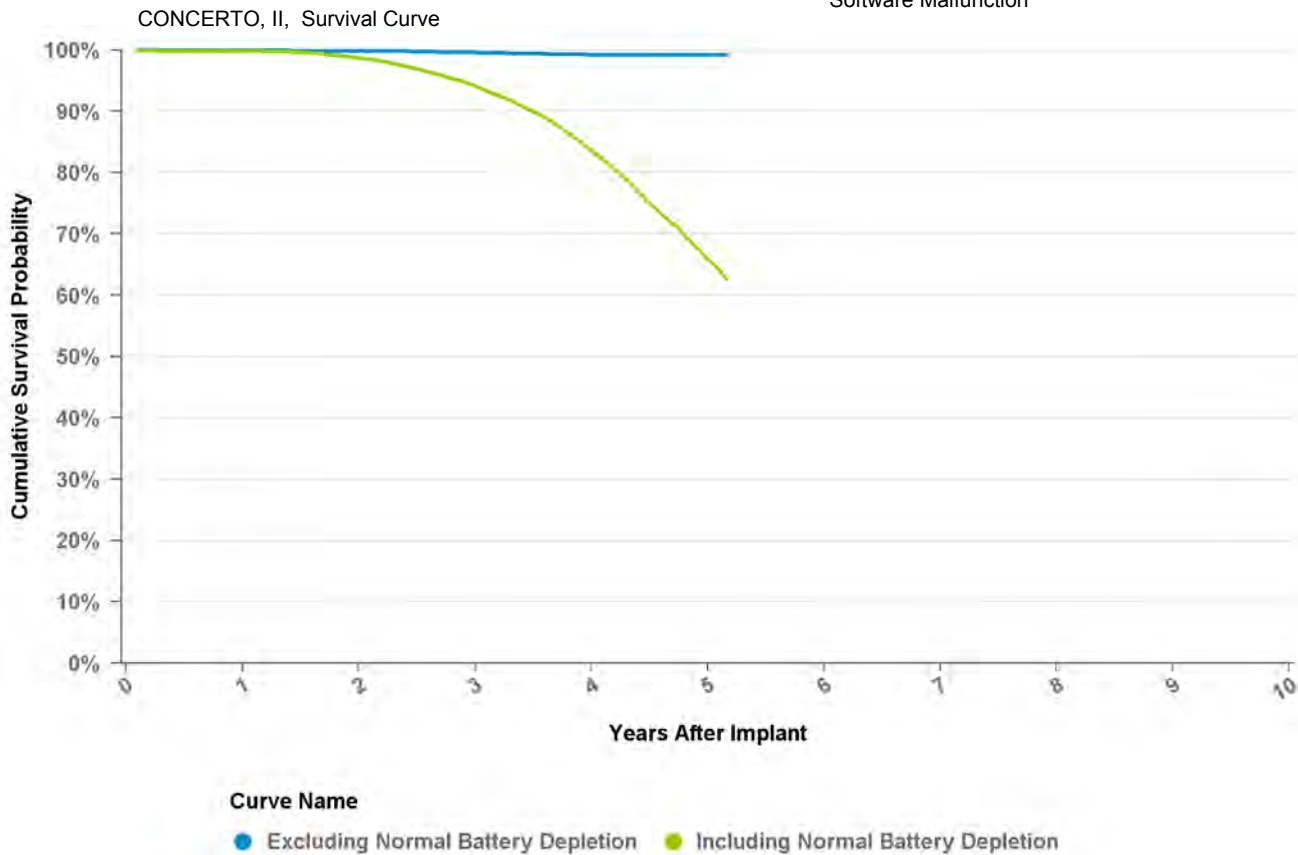


| Years | 1 | 2 | 3 | 4 | 5 | at 62 mo |
|------------------------------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.6% | 99.2% | 99.2% | 99.2% |
| Including NBD | 99.8% | 98.7% | 94.1% | 83.5% | 65.9% | 62.6% |
| Effective Sample Size | 27419 | 25273 | 22253 | 13404 | 1584 | 432 |

Cardiac Resynchronization Therapy

D284TRK Maximo II CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | 09/17/2008 |
| CE Market Approval Date | 03/14/2008 |
| Registered US Implants | 15,119 |
| Estimated Active US Implants | 7,489 |
| Normal Battery Depletions (US) | 2,136 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|-----|
| Total Malfunctions (US) | 132 |
| Therapy Not Compromised Malfunctions | 127 |
| Battery Malfunction | 0 |
| Electrical Component | 5 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 122 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 5 |
| Battery Malfunction | 0 |
| Electrical Component | 5 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

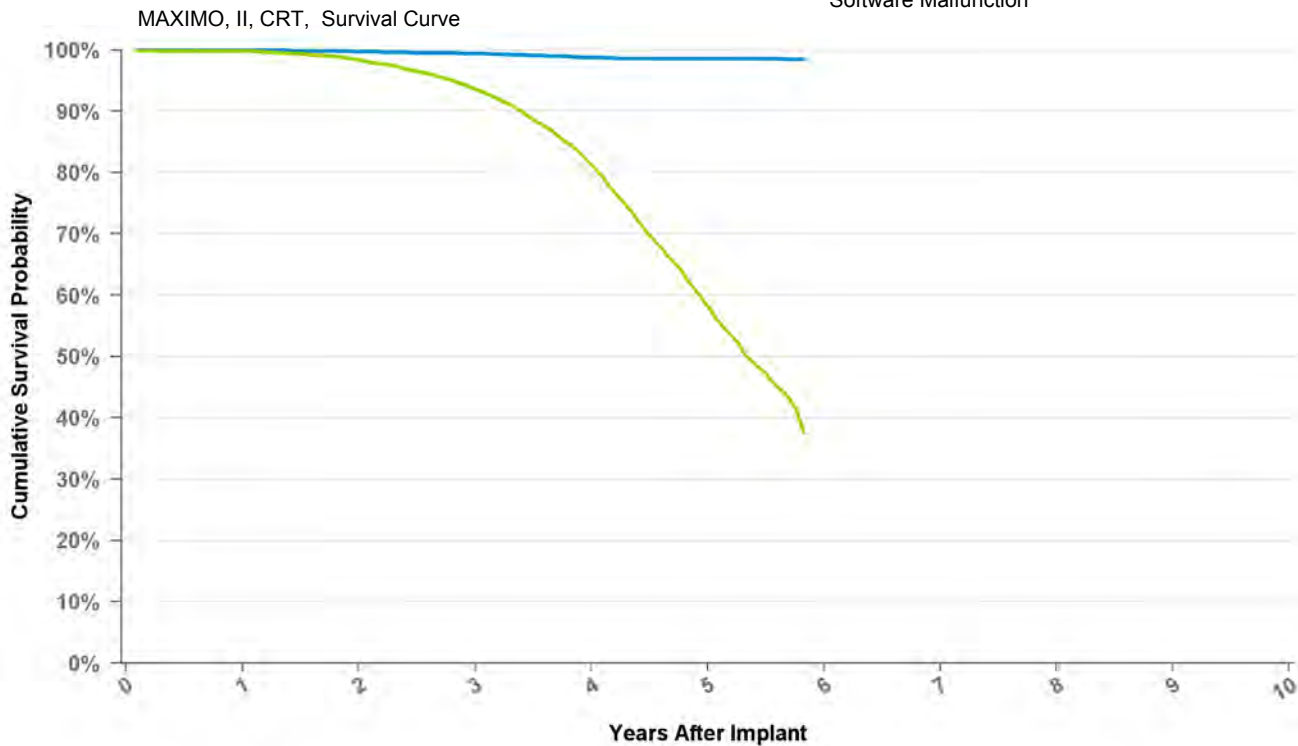

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | at 70 mo |
|------------------------------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.7% | 99.4% | 98.8% | 98.6% | 98.5% |
| Including NBD | 99.8% | 98.4% | 93.6% | 81.3% | 58.3% | 37.4% |
| Effective Sample Size | 14141 | 12273 | 9752 | 6100 | 1971 | 145 |

Cardiac Resynchronization Therapy

D294TRK Concerto II CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 08/20/2008 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

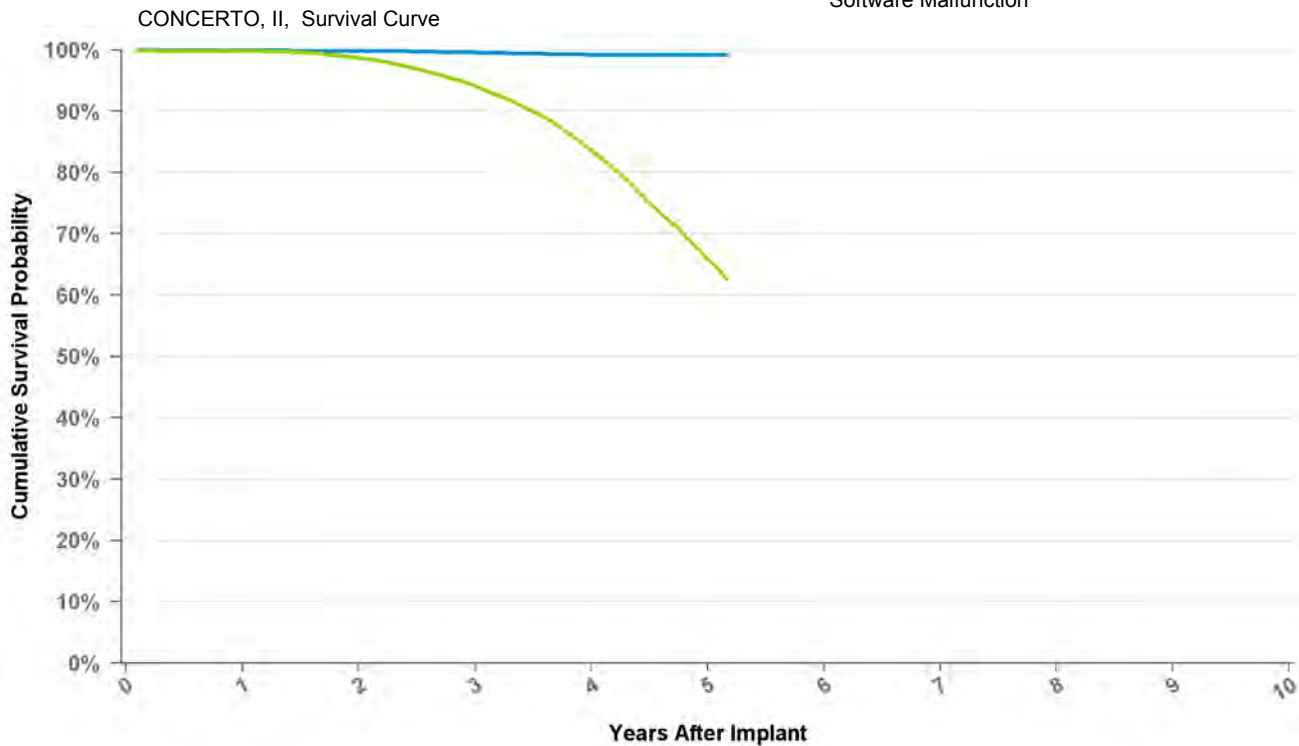

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | at 62 mo |
|------------------------------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.6% | 99.2% | 99.2% | 99.2% |
| Including NBD | 99.8% | 98.7% | 94.1% | 83.5% | 65.9% | 62.6% |
| Effective Sample Size | 27419 | 25273 | 22253 | 13404 | 1584 | 432 |

Cardiac Resynchronization Therapy

D314TRG Protecta XT CRT-D

US Market Release Date 03/25/2011

CE Market Approval Date

Registered US Implants 41,680

Estimated Active US Implants 34,909

Normal Battery Depletions (US) 737

NBG Code DDE-DDDR

Max Delivered Energy 35 J

Total Malfunctions (US) 40

Therapy Not Compromised Malfunctions 38

Battery Malfunction 0

Electrical Component 10

Electrical Interconnect 0

Other Malfunction 1

Poss Early Battery Depltn 27

Software Malfunction 0

Therapy Compromised Malfunctions 2

Battery Malfunction 0


Electrical Component 2

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

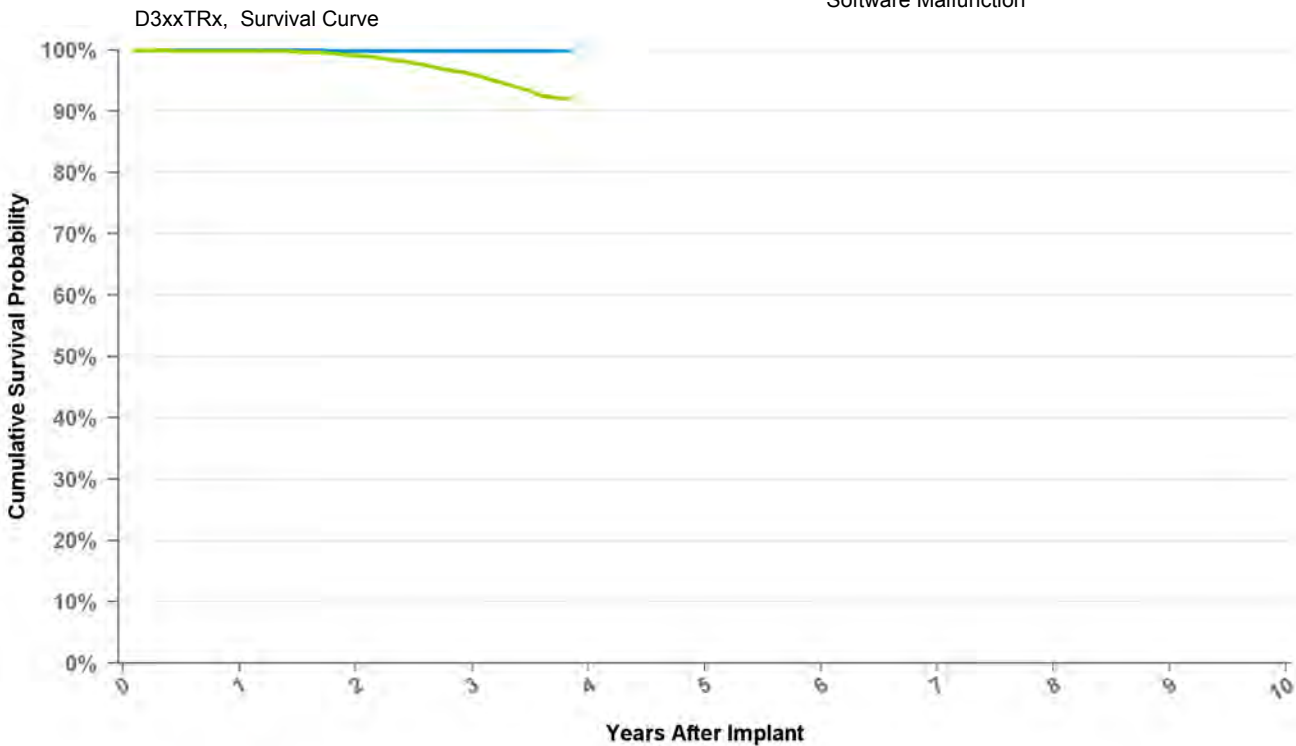

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.1% | 96.0% | 92.1% |
| Effective Sample Size | 57354 | 40614 | 12554 | 131 |

Cardiac Resynchronization Therapy

D314TRM Protecta XT CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | 11/09/2011 |
| CE Market Approval Date | |
| Registered US Implants | 12,182 |
| Estimated Active US Implants | 11,144 |
| Normal Battery Depletions (US) | 61 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 6 |
| Therapy Not Compromised Malfunctions | 5 |
| Battery Malfunction | 0 |
| Electrical Component | 4 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

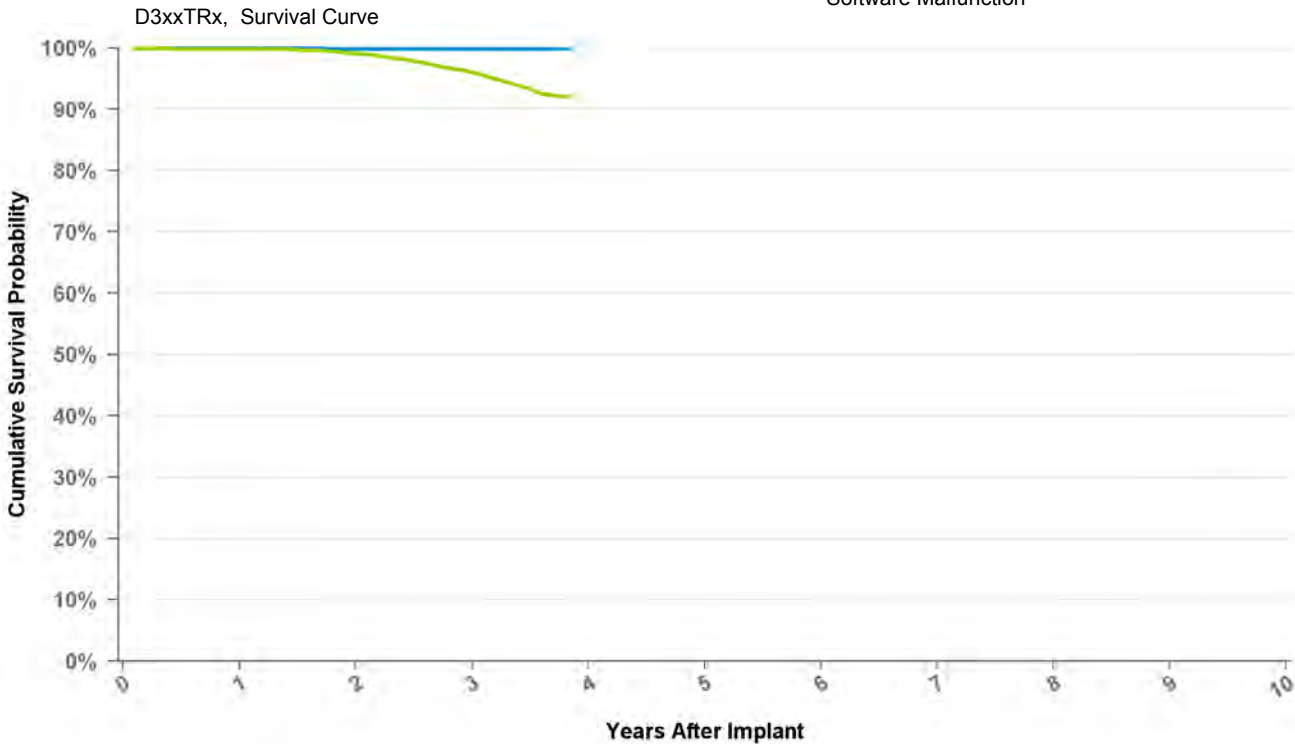

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.1% | 96.0% | 92.1% |
| Effective Sample Size | 57354 | 40614 | 12554 | 131 |

Cardiac Resynchronization Therapy

D334TRG Protecta CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | 03/25/2011 |
| CE Market Approval Date | |
| Registered US Implants | 7,820 |
| Estimated Active US Implants | 6,677 |
| Normal Battery Depletions (US) | 108 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 8 |
| Therapy Not Compromised Malfunctions | 7 |
| Battery Malfunction | 0 |
| Electrical Component | 3 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 4 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

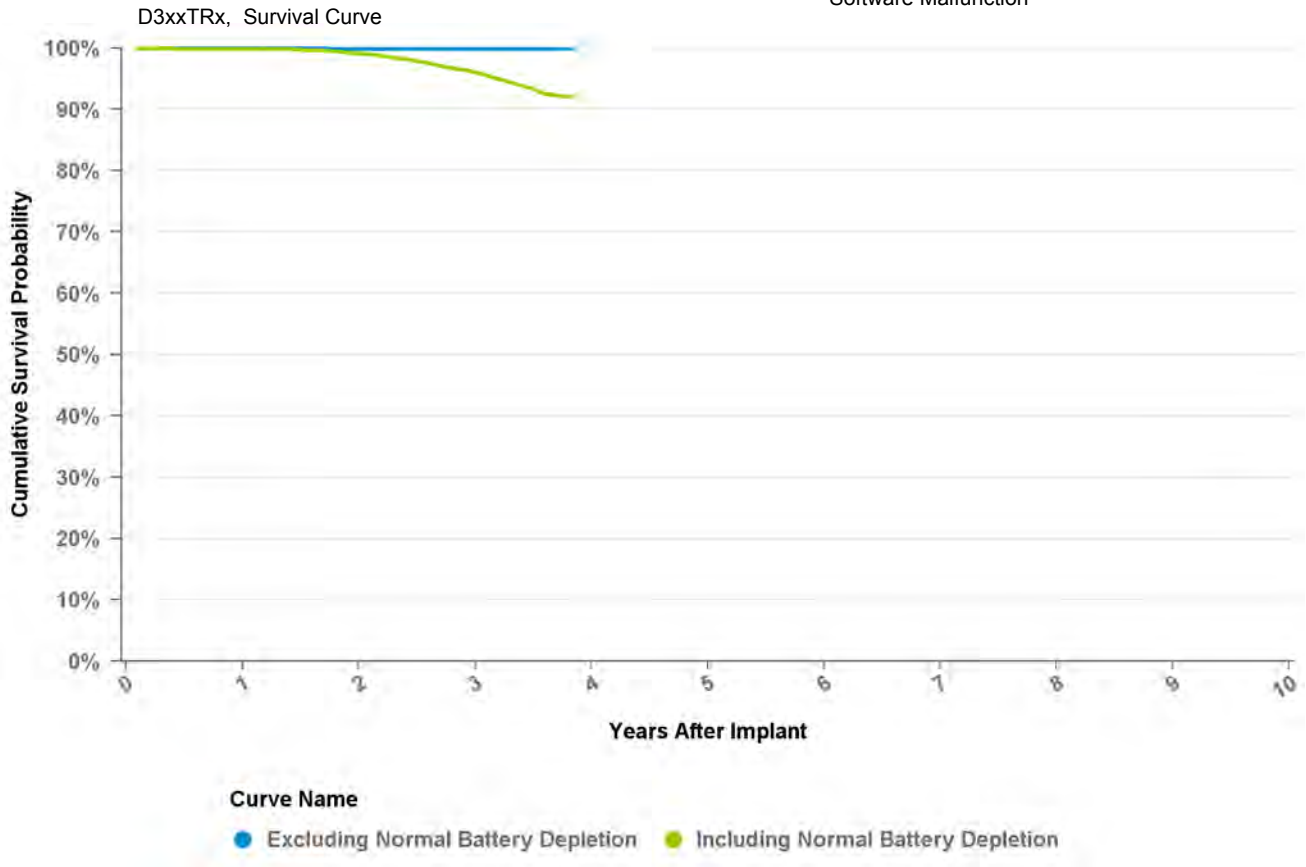

| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.1% | 96.0% | 92.1% |
| Effective Sample Size | 57354 | 40614 | 12554 | 131 |

Cardiac Resynchronization Therapy

D334TRM Protecta CRT-D

US Market Release Date 11/09/2011

CE Market Approval Date

Registered US Implants 1,729

Estimated Active US Implants 1,583

Normal Battery Depletions (US) 9

NBG Code DDE-DDDR

Max Delivered Energy 35 J

Total Malfunctions (US) 2

Therapy Not Compromised Malfunctions 2

Battery Malfunction 0

Electrical Component 1

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 1

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

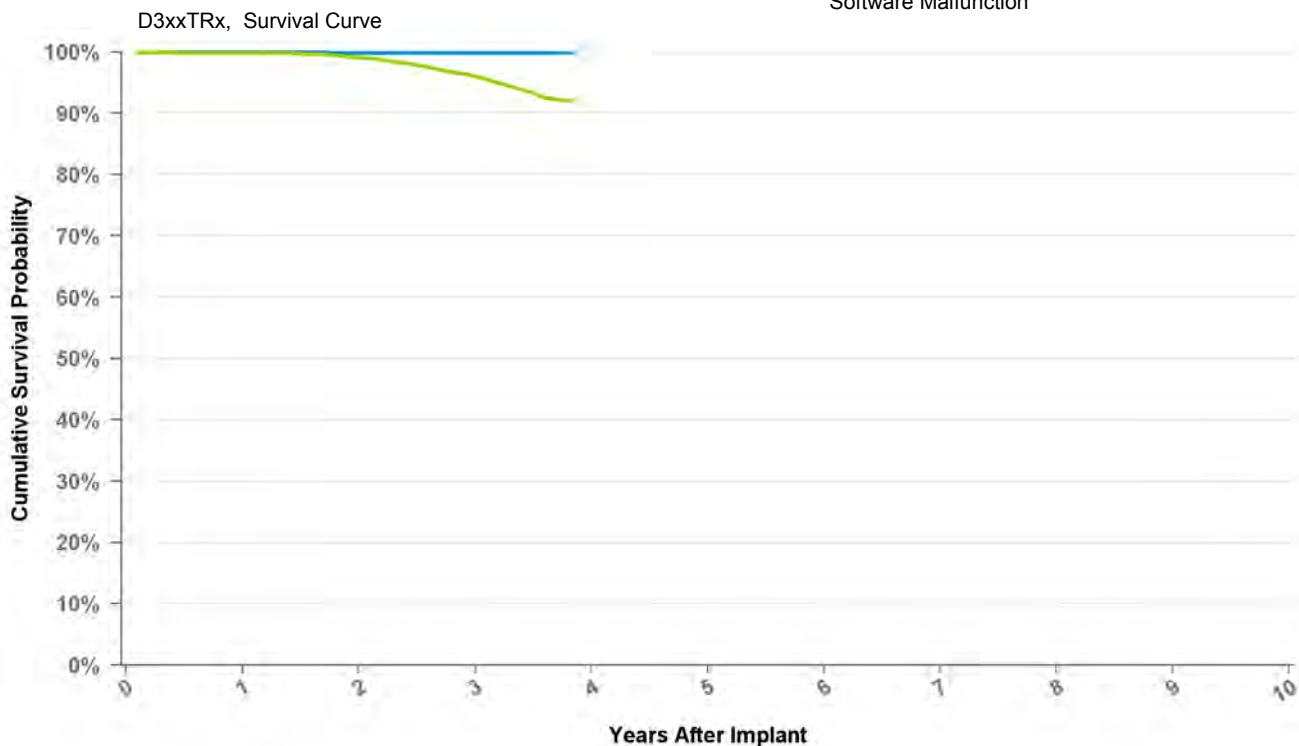

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.1% | 96.0% | 92.1% |
| Effective Sample Size | 57354 | 40614 | 12554 | 131 |

Cardiac Resynchronization Therapy

D354TRG Protecta XT CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 03/25/2010 |
| Registered US Implants | 1 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

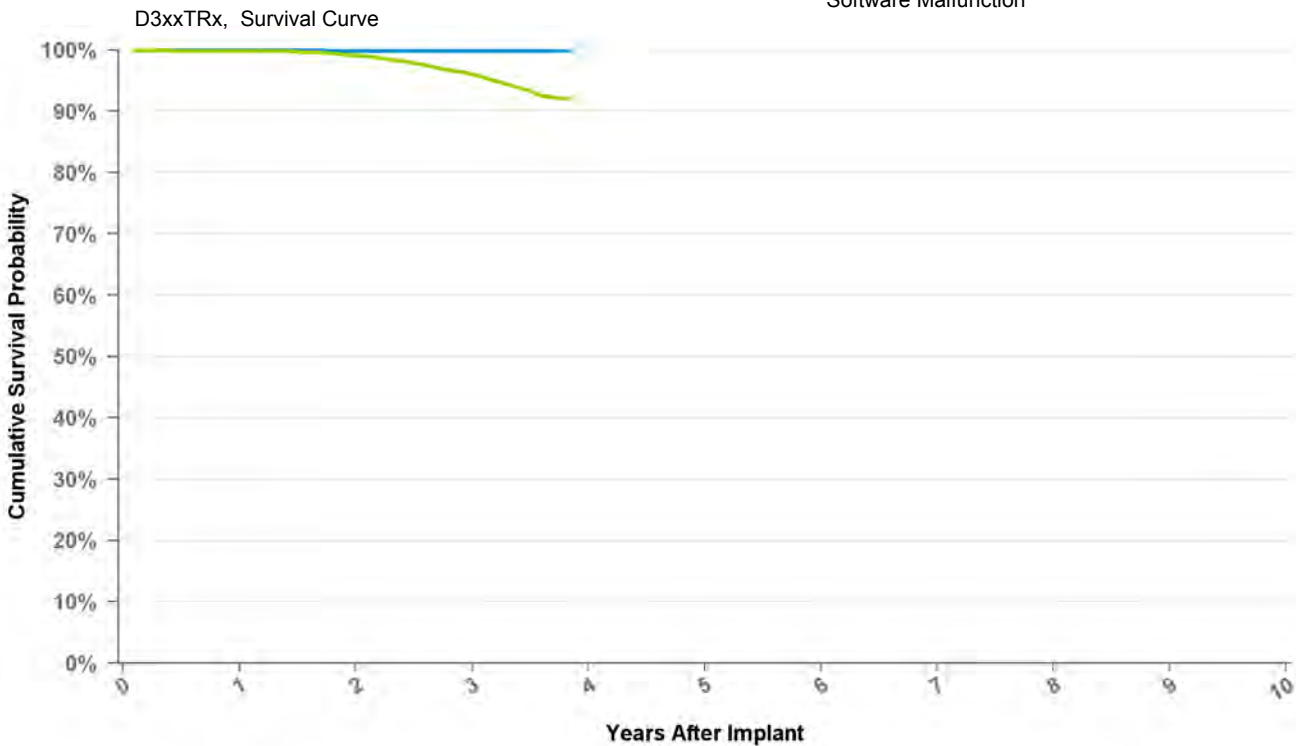

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.1% | 96.0% | 92.1% |
| Effective Sample Size | 57354 | 40614 | 12554 | 131 |

Cardiac Resynchronization Therapy

D354TRM Protecta XT CRT-D

US Market Release Date

CE Market Approval Date 07/15/2010

Registered US Implants 1

Estimated Active US Implants 1

Normal Battery Depletions (US) 0

NBG Code DDE-DDDR

Max Delivered Energy 35 J

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

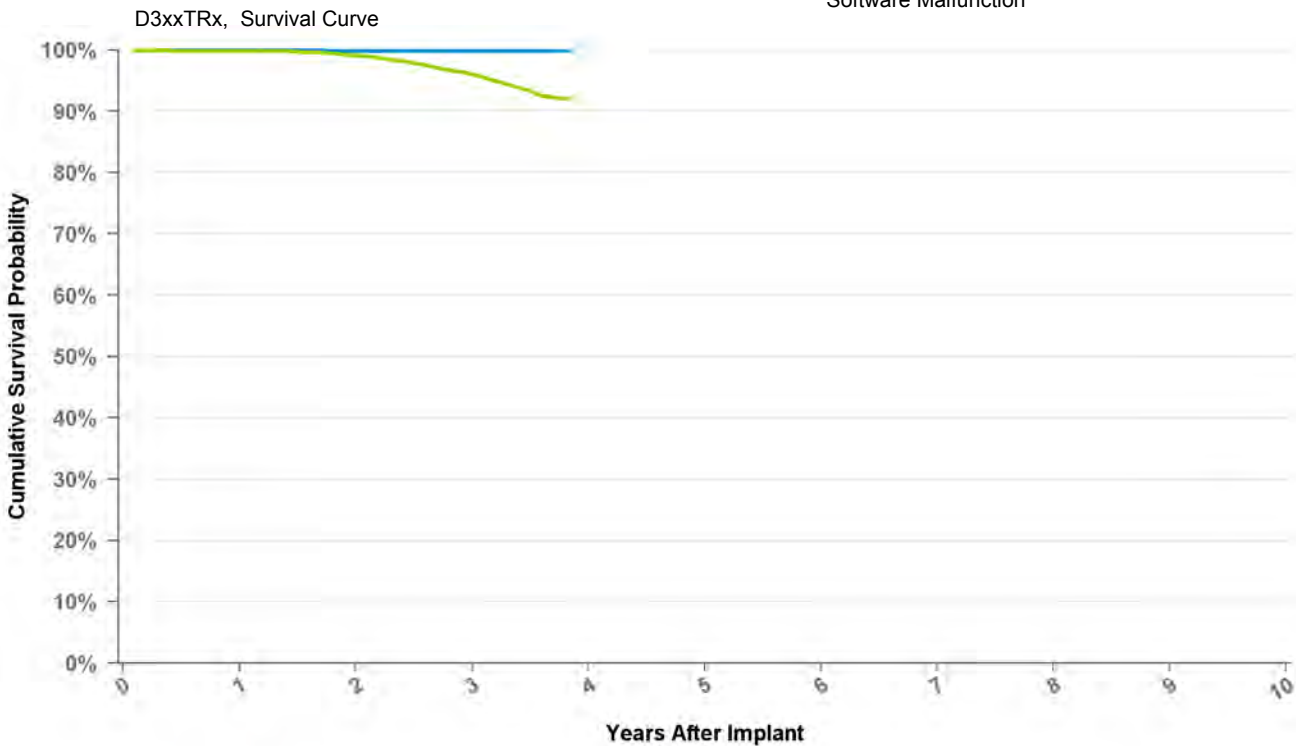

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.1% | 96.0% | 92.1% |
| Effective Sample Size | 57354 | 40614 | 12554 | 131 |

Cardiac Resynchronization Therapy

D364TRG Protecta CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 03/25/2010 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

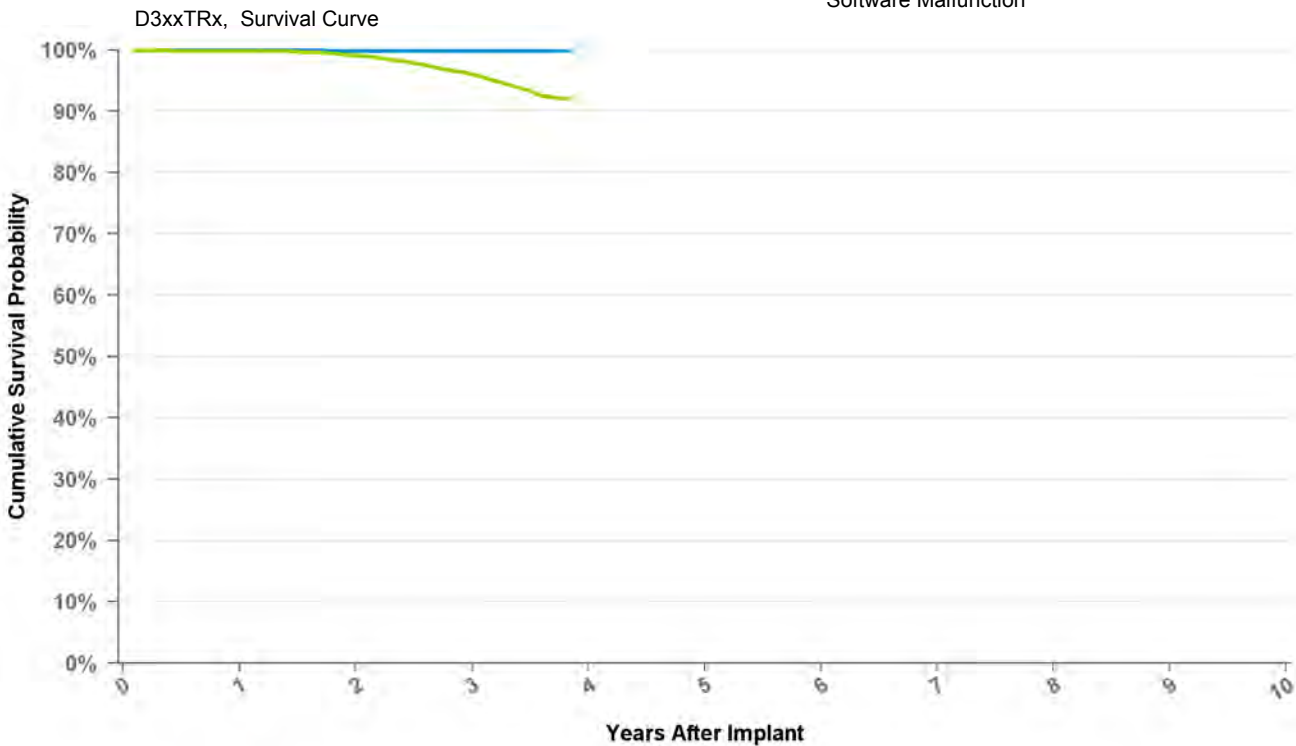

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.1% | 96.0% | 92.1% |
| Effective Sample Size | 57354 | 40614 | 12554 | 131 |

Cardiac Resynchronization Therapy

D364TRM Protecta CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 07/15/2010 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

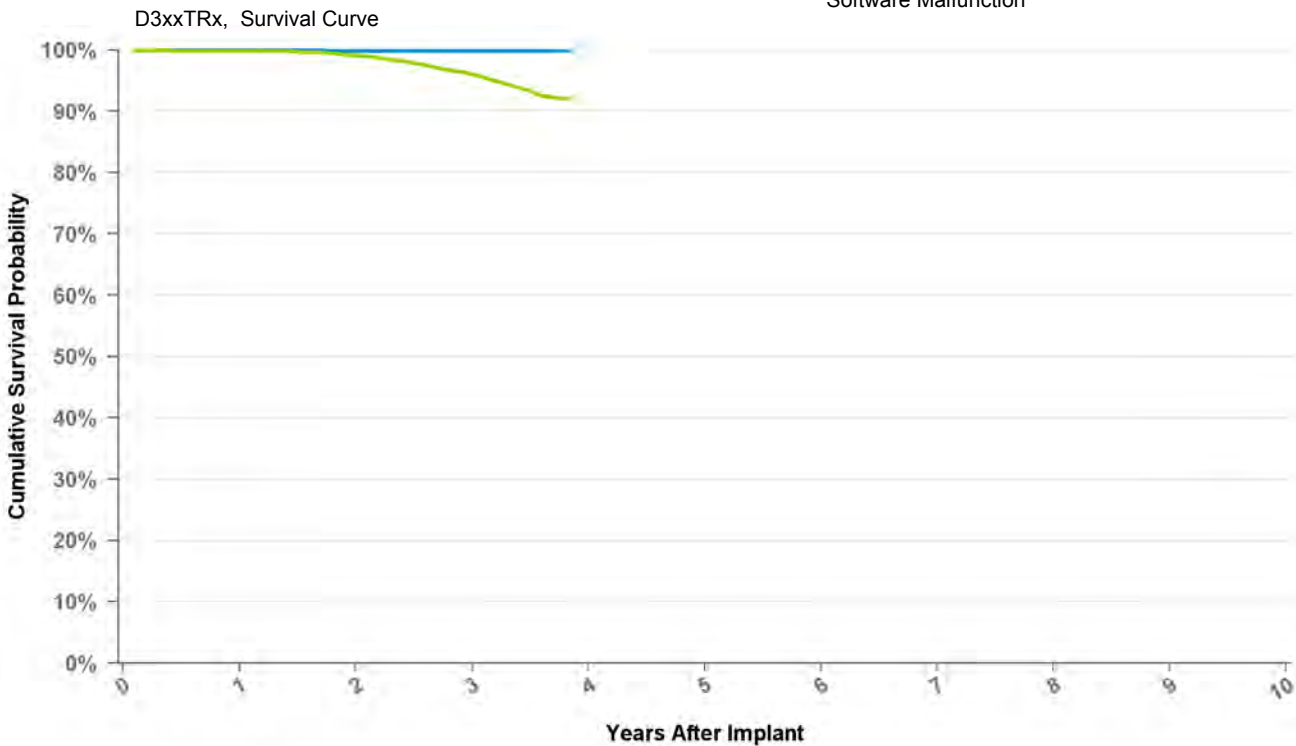

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.1% | 96.0% | 92.1% |
| Effective Sample Size | 57354 | 40614 | 12554 | 131 |

Cardiac Resynchronization Therapy

D384TRG Cardia CRT-D

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 01/12/2011 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

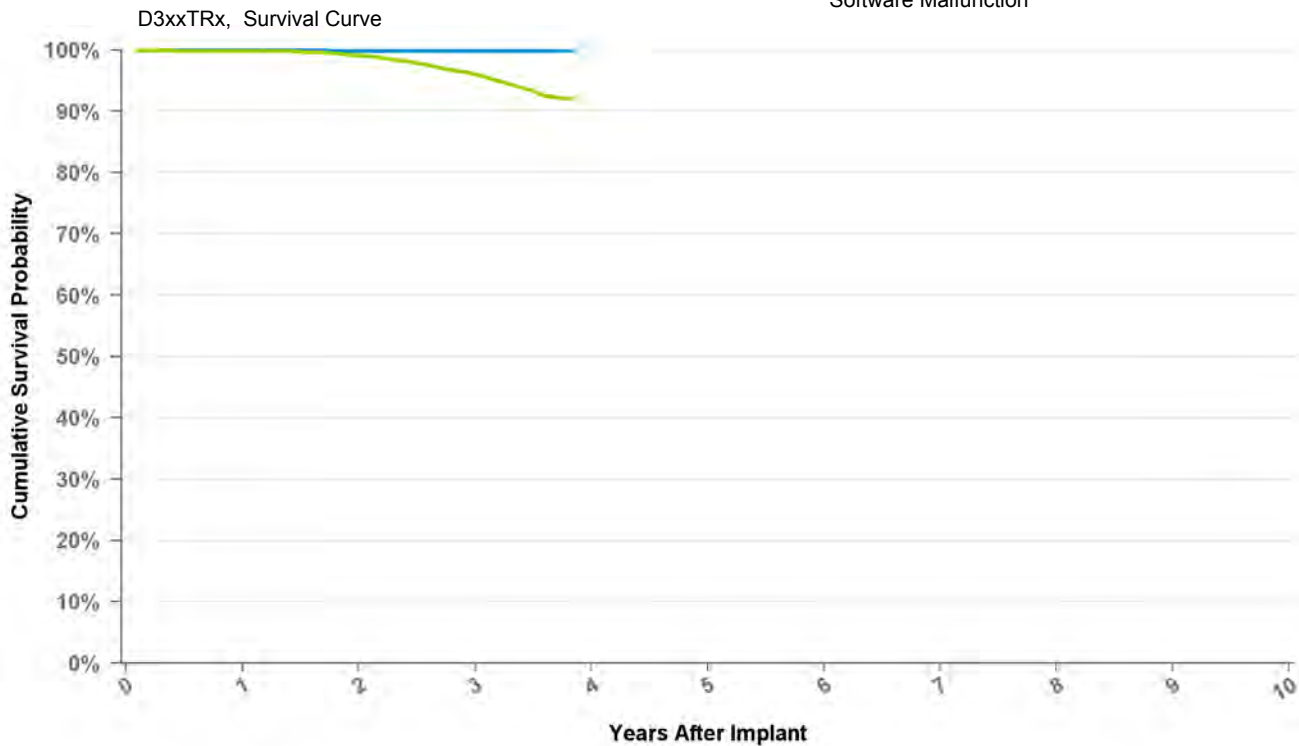

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.1% | 96.0% | 92.1% |
| Effective Sample Size | 57354 | 40614 | 12554 | 131 |

Cardiac Resynchronization Therapy

D394TRG Egida CRT-D

US Market Release Date

CE Market Approval Date 01/12/2011

Registered US Implants 0

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code VVE-DDDR

Max Delivered Energy 35 J

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

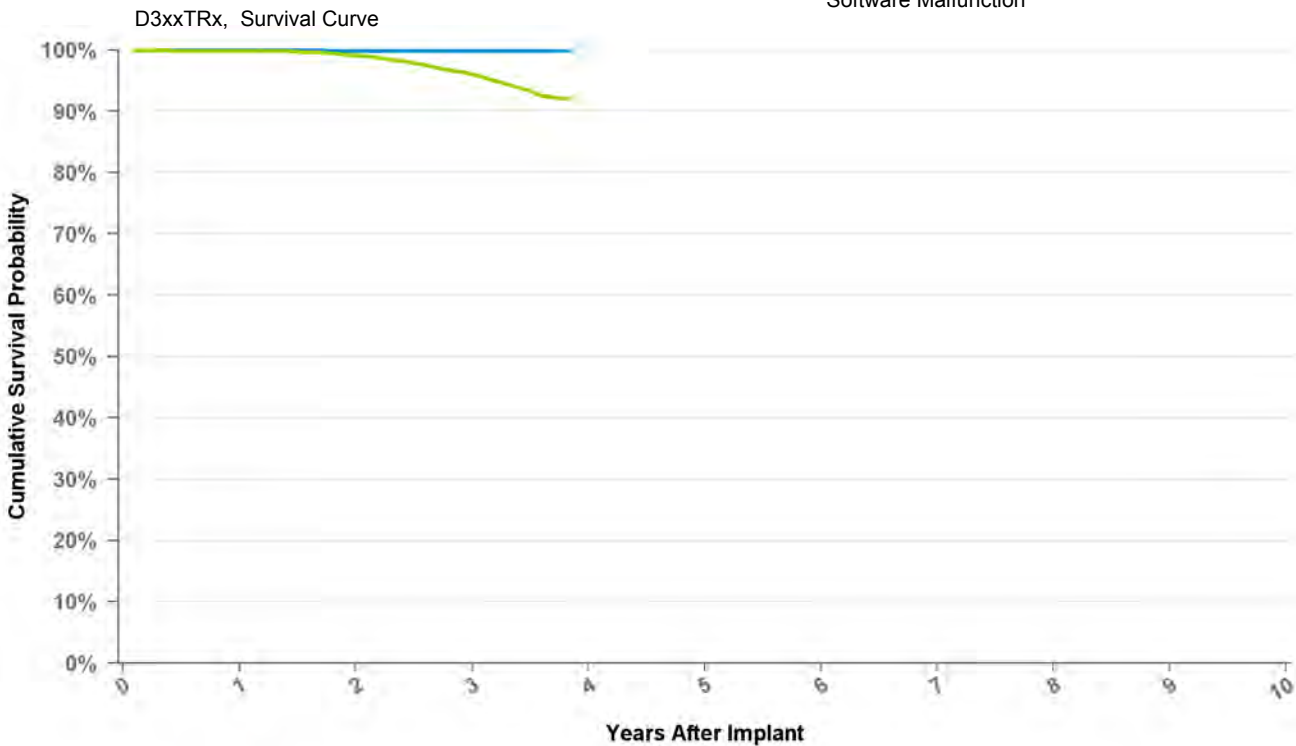

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.1% | 96.0% | 92.1% |
| Effective Sample Size | 57354 | 40614 | 12554 | 131 |

Cardiac Resynchronization Therapy

DTBA1D1 Viva XT

US Market Release Date 01/29/2013

CE Market Approval Date

Registered US Implants 22,275

Estimated Active US Implants 21,273

Normal Battery Depletions (US) 1

NBG Code DDE-DDDR

Max Delivered Energy 36 J

Total Malfunctions (US) 1

Therapy Not Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 1

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

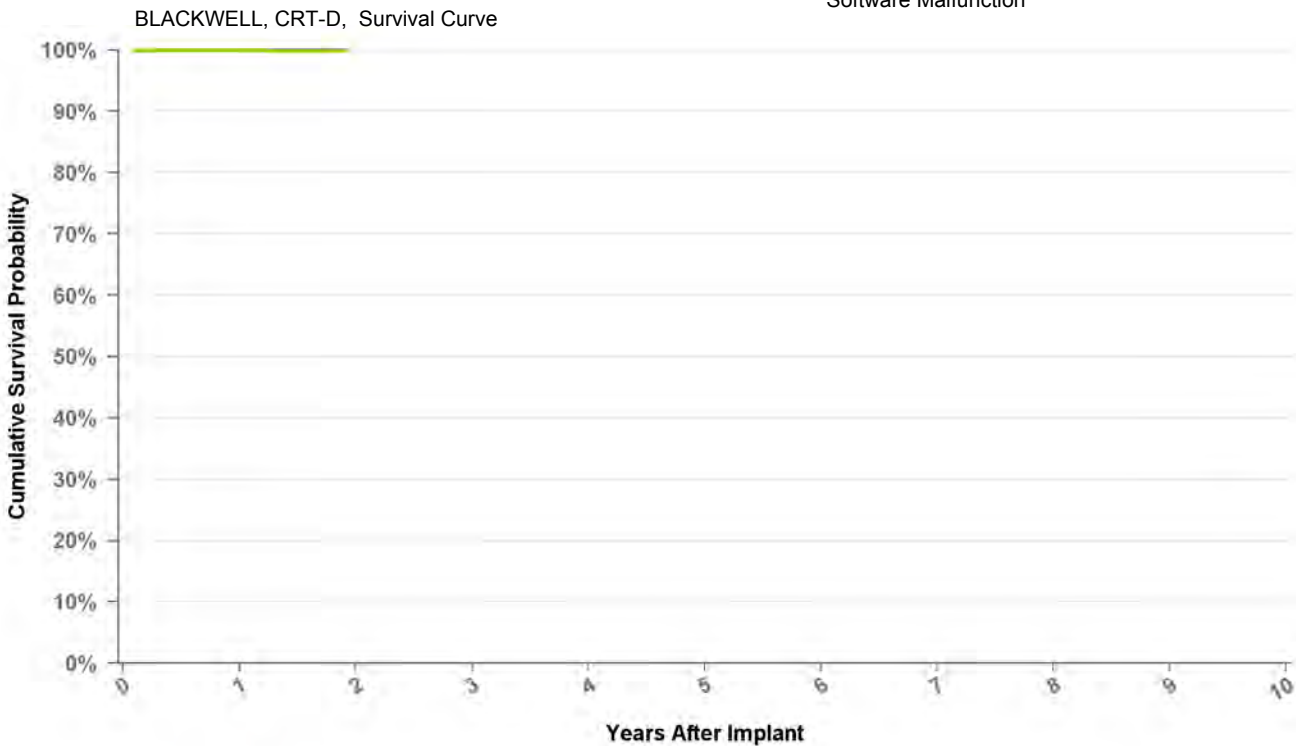

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBA1D4 Viva XT

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/29/2013 |
| CE Market Approval Date | |
| Registered US Implants | 12,125 |
| Estimated Active US Implants | 11,689 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 3 |
| Therapy Not Compromised Malfunctions | 2 |
| Battery Malfunction | 0 |
| Electrical Component | 2 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

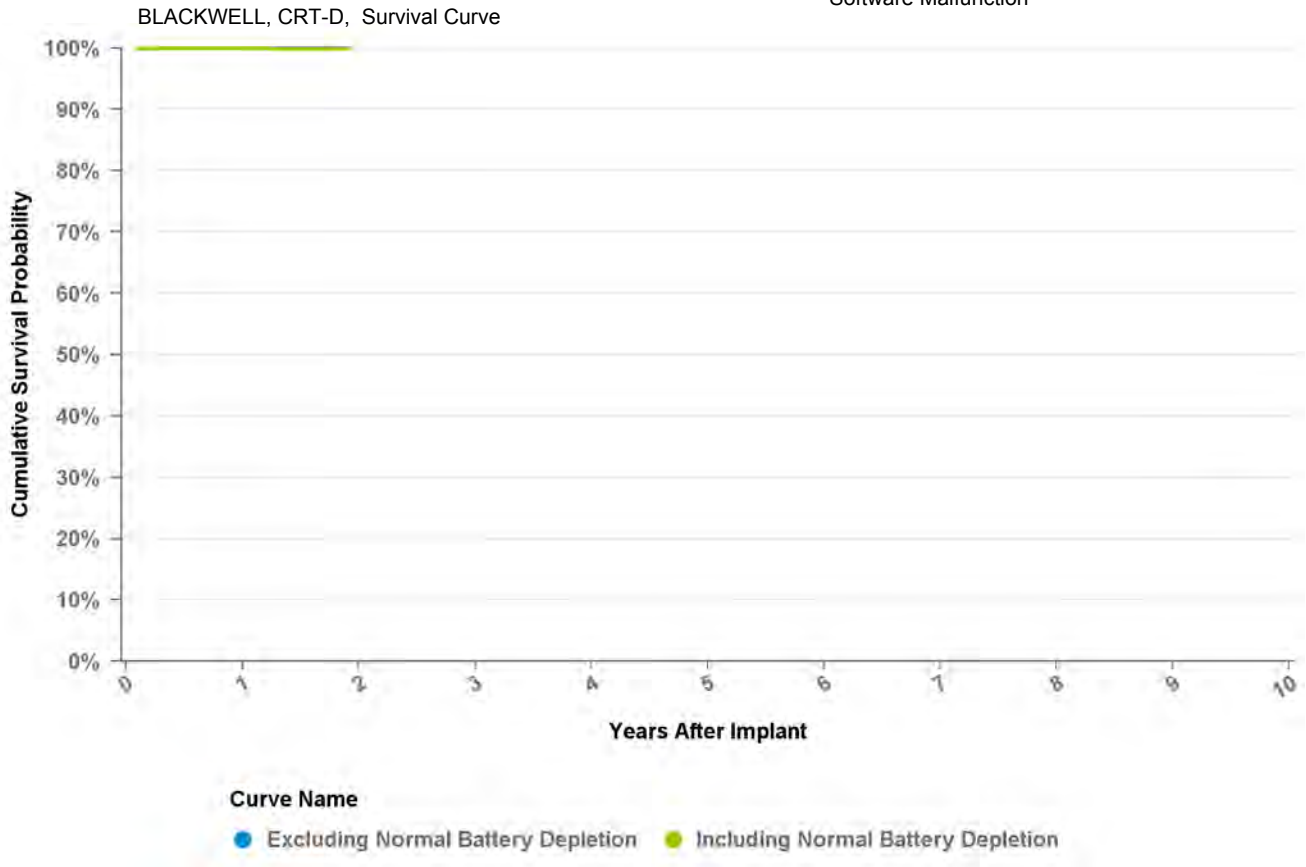


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBA1Q1 Viva Quad XT

| | |
|---------------------------------------|----------|
| US Market Release Date | |
| CE Market Approval Date | |
| Registered US Implants | 1,768 |
| Estimated Active US Implants | 1,738 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

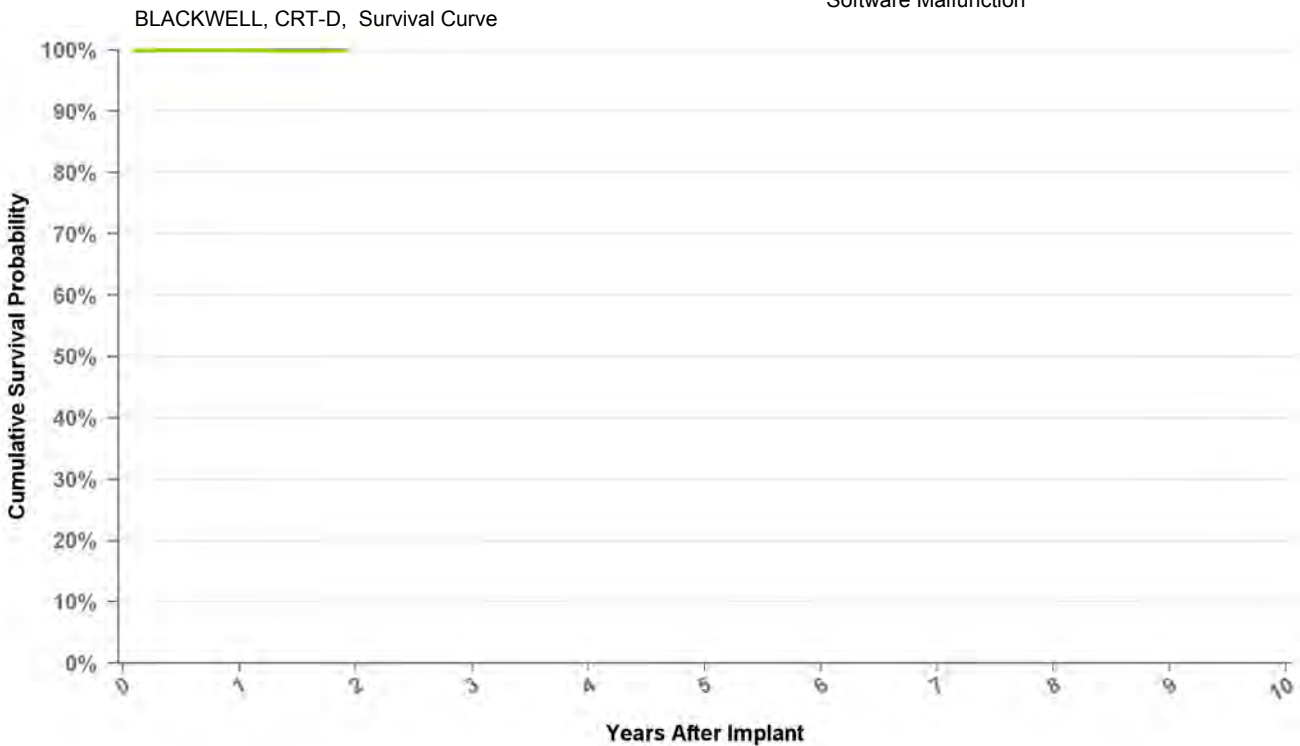

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBA1QQ Viva Quad XT

| | |
|---------------------------------------|----------|
| US Market Release Date | |
| CE Market Approval Date | |
| Registered US Implants | 4,949 |
| Estimated Active US Implants | 4,897 |
| Normal Battery Depletions (US) | 1 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

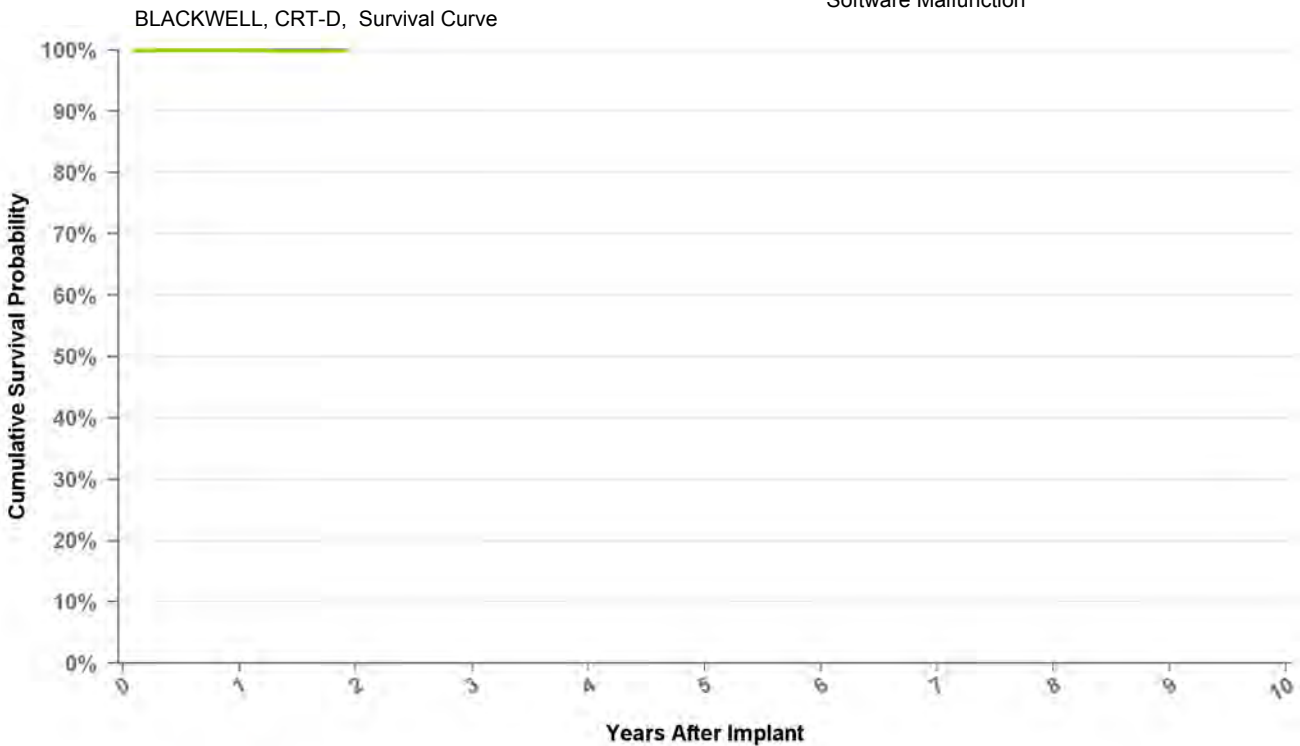

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBA2D1 Viva XT

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 08/10/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

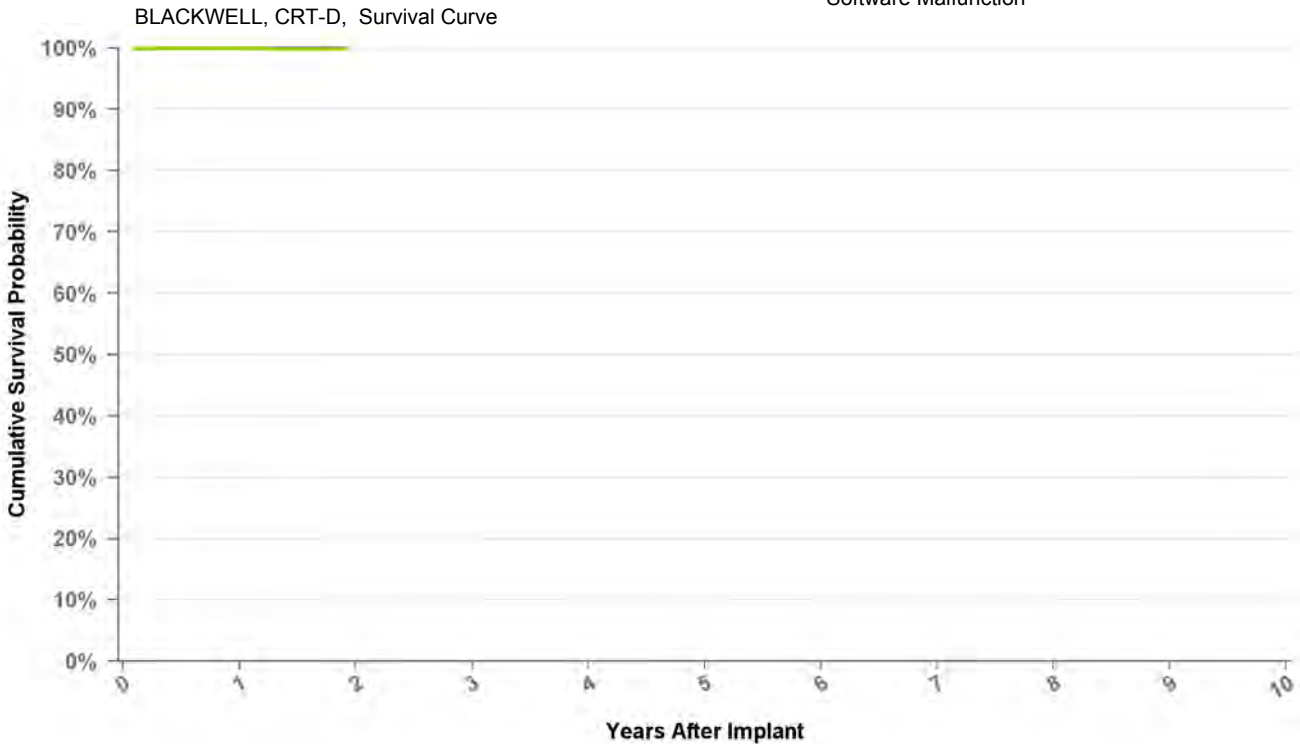

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBA2D4 Viva XT

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 08/10/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

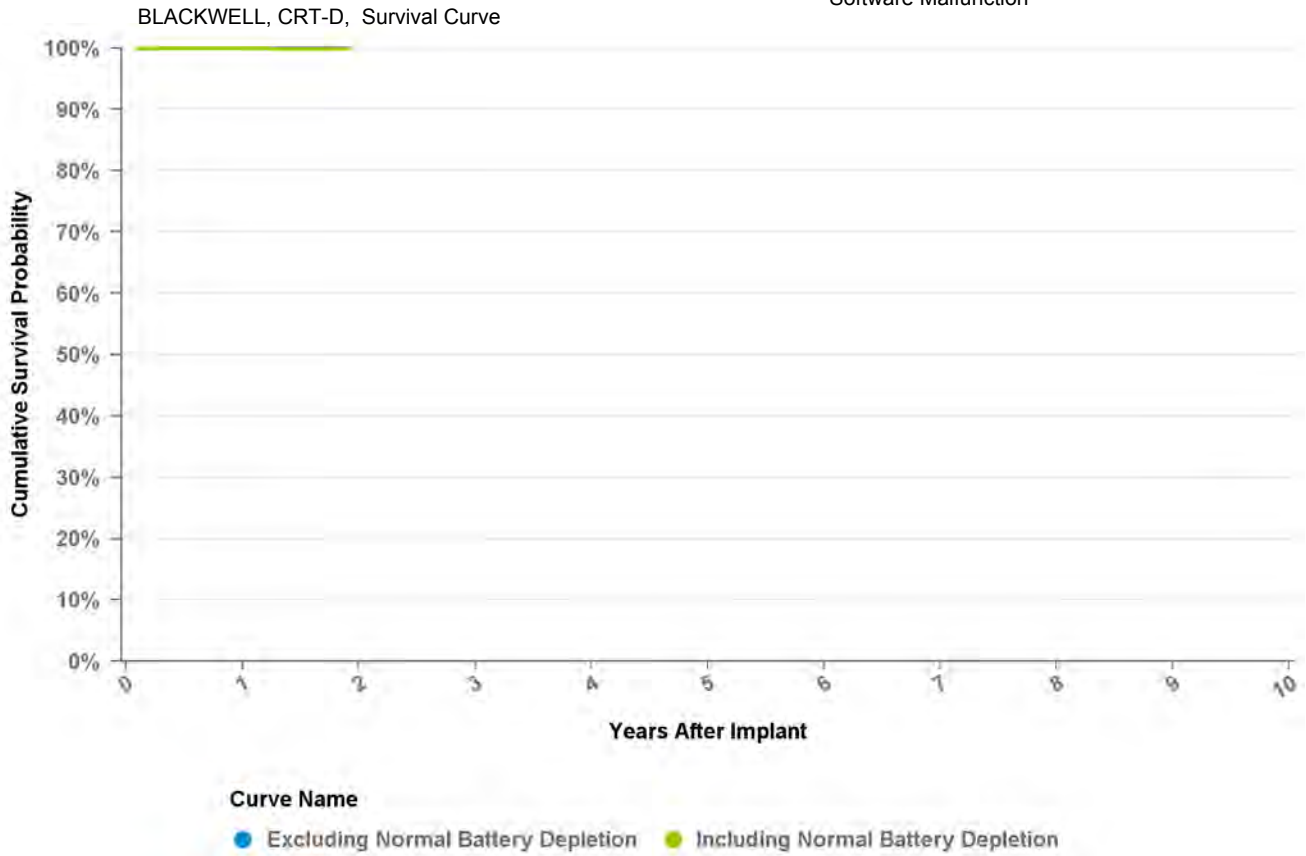


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBA2Q1 Viva Quad XT

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 09/13/2013 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

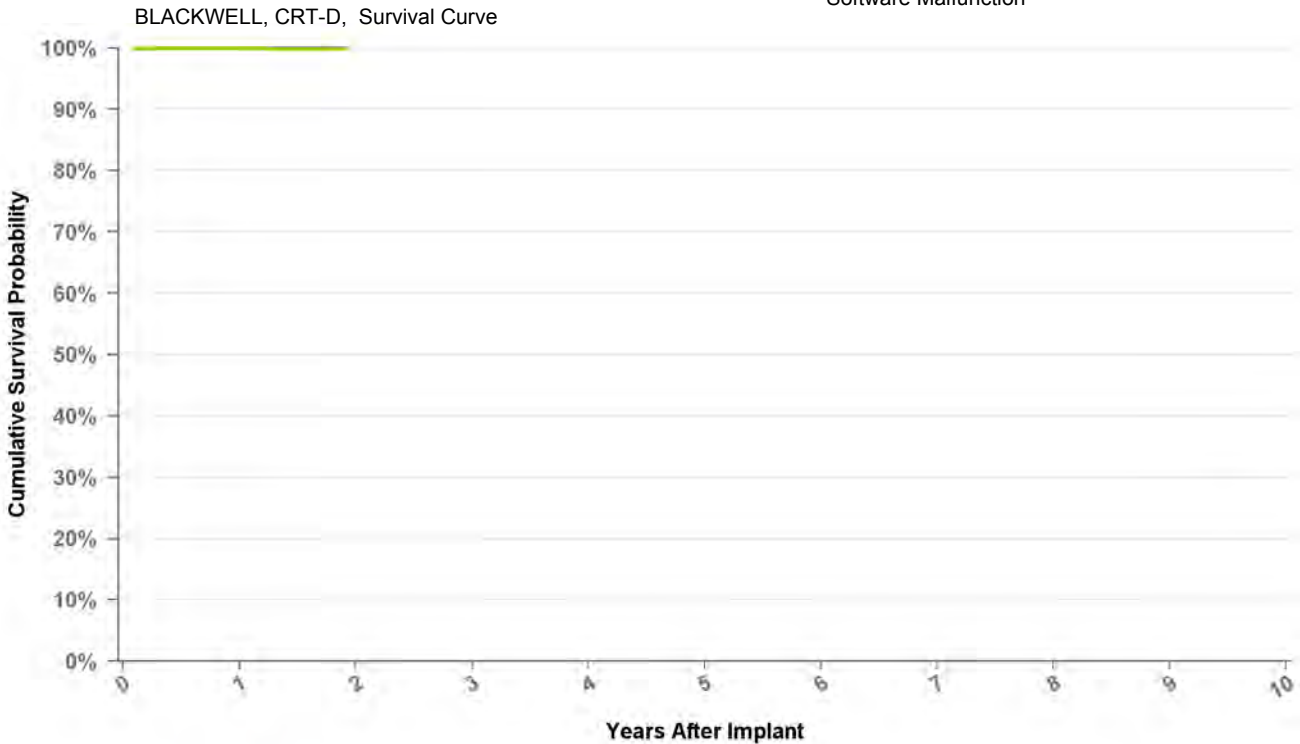

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBA2QQ Viva Quad XT

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 08/10/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

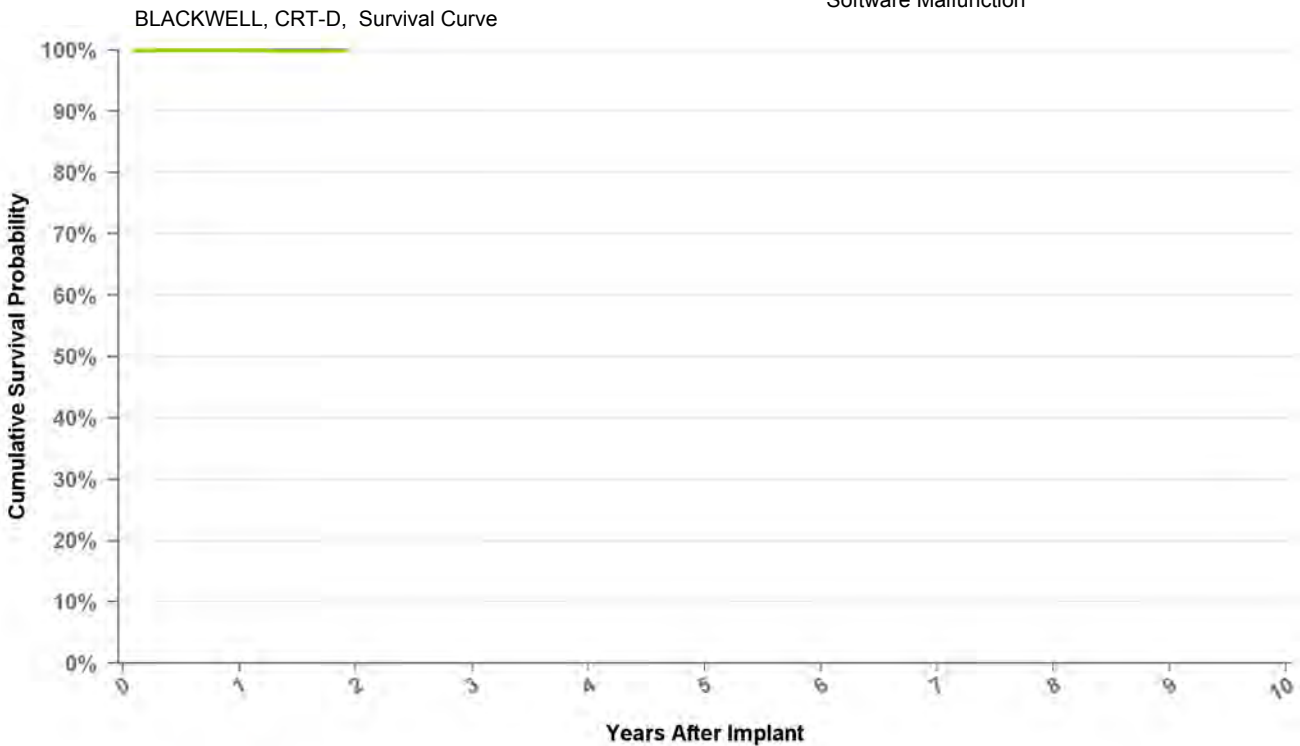

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBB1D1 Viva S

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/29/2013 |
| CE Market Approval Date | |
| Registered US Implants | 6,419 |
| Estimated Active US Implants | 6,077 |
| Normal Battery Depletions (US) | 1 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

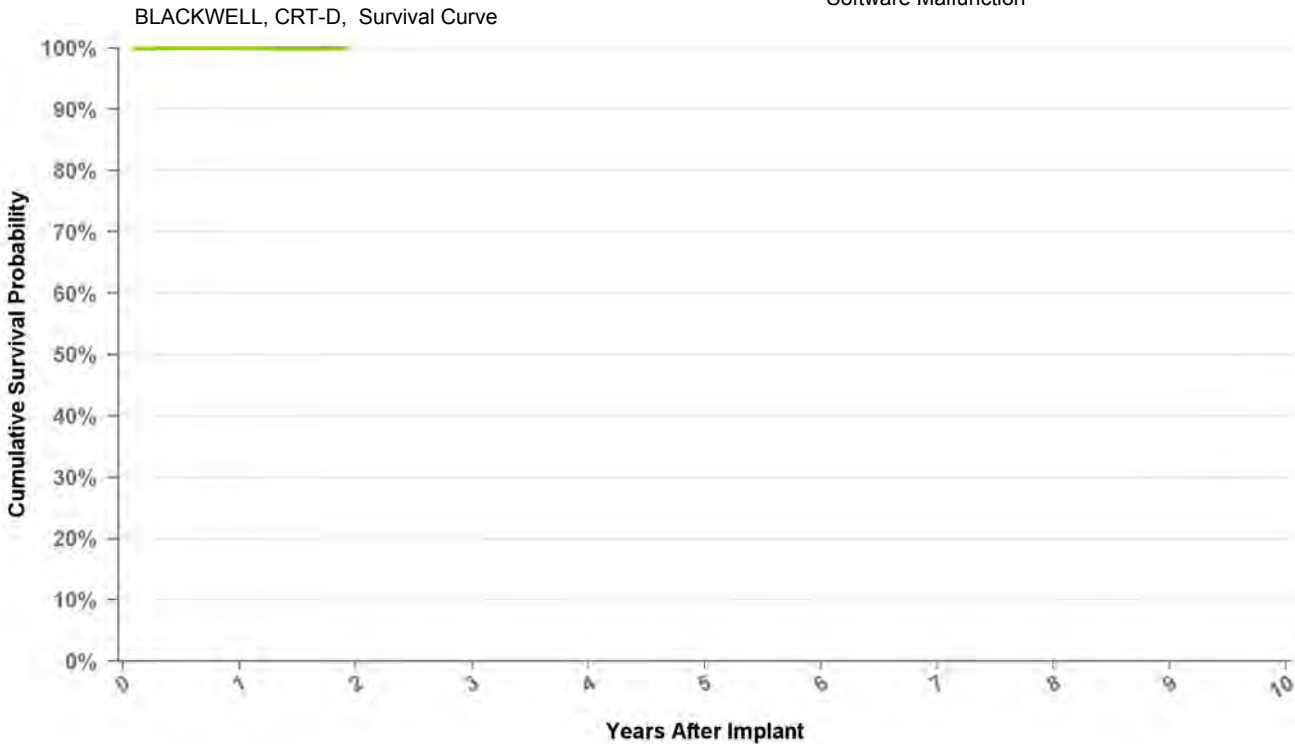

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBB1D4 Viva S

US Market Release Date 01/29/2013

CE Market Approval Date

Registered US Implants 2,820

Estimated Active US Implants 2,718

Normal Battery Depletions (US) 1

NBG Code DDE-DDDR

Max Delivered Energy 36 J

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

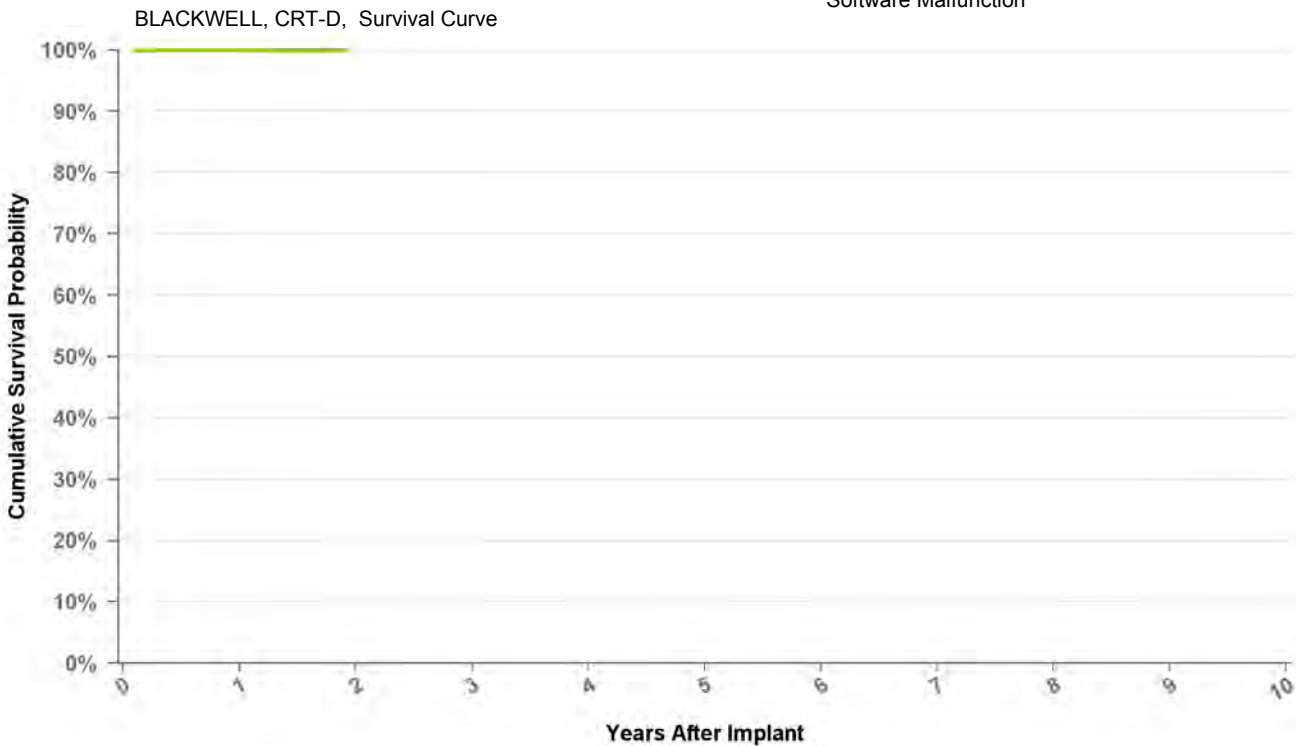

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBB1Q1 Viva Quad S

| | |
|---------------------------------------|----------|
| US Market Release Date | |
| CE Market Approval Date | |
| Registered US Implants | 254 |
| Estimated Active US Implants | 248 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

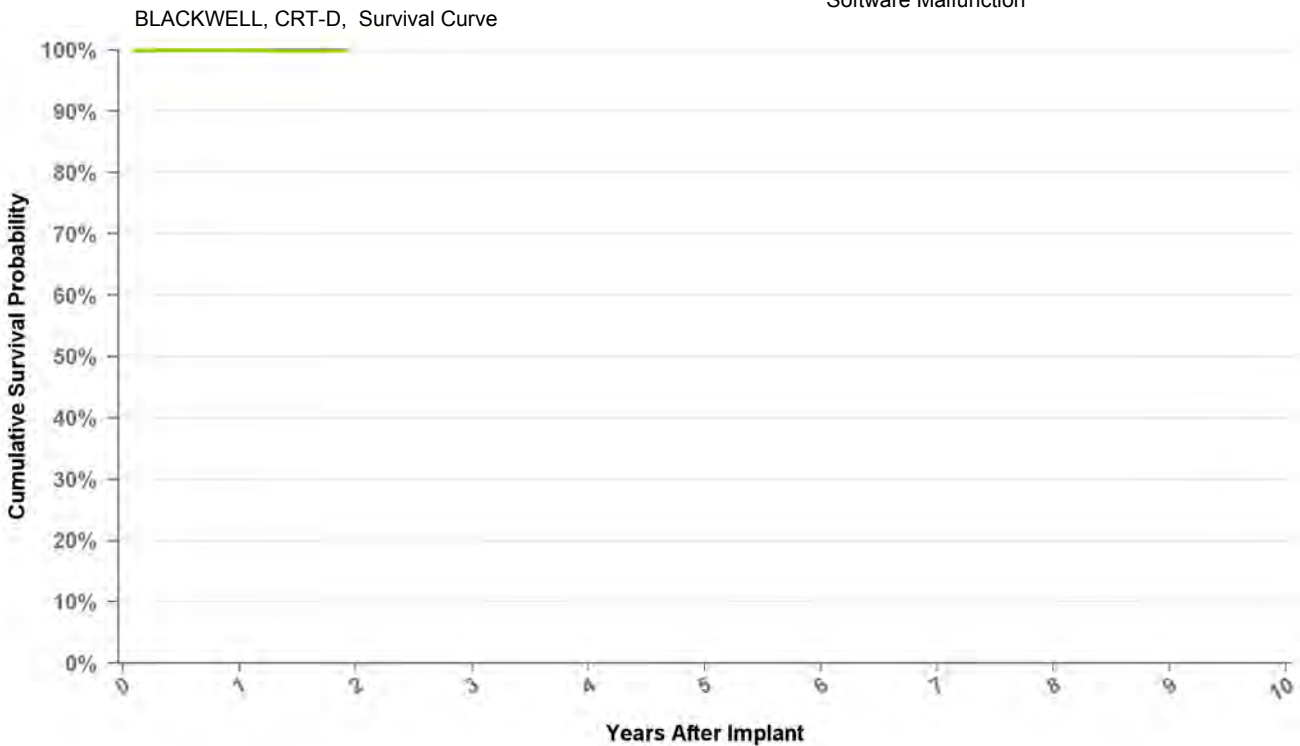

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBB1QQ Viva Quad S

| | |
|---------------------------------------|----------|
| US Market Release Date | |
| CE Market Approval Date | |
| Registered US Implants | 634 |
| Estimated Active US Implants | 625 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

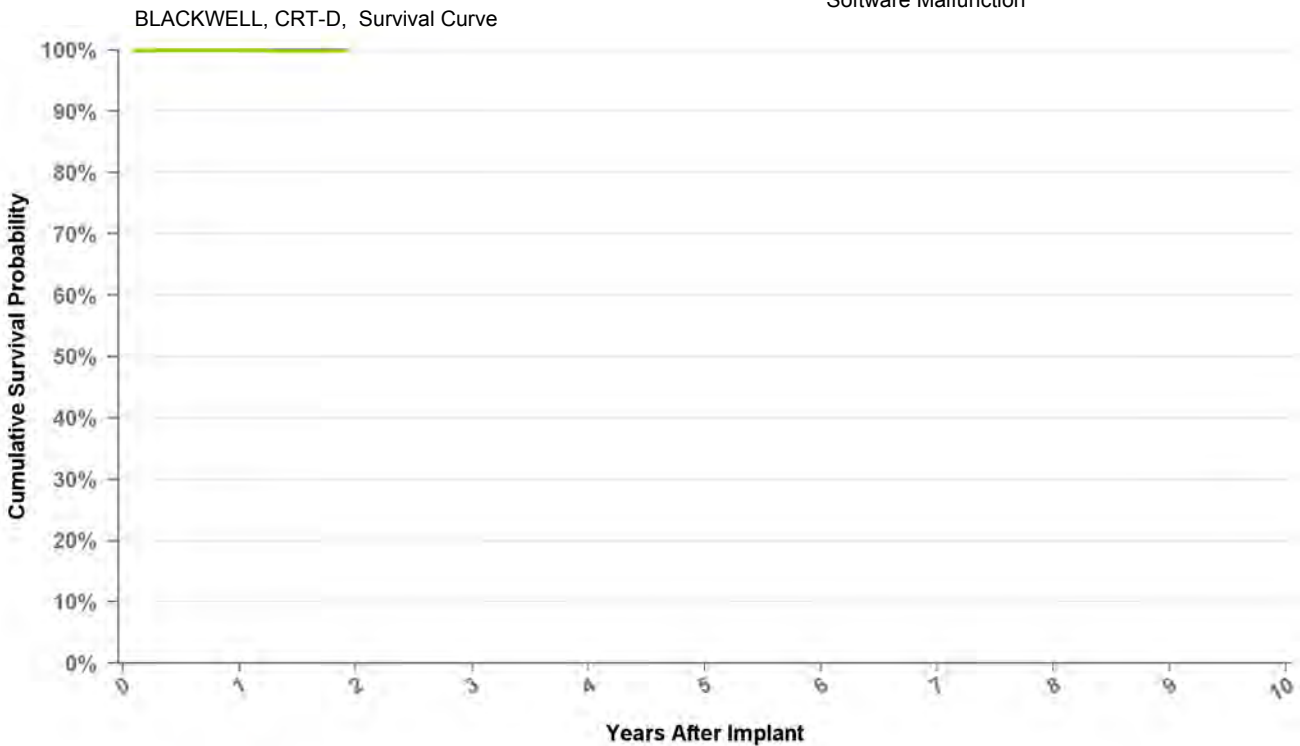

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBB2D1 Viva S

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 08/10/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

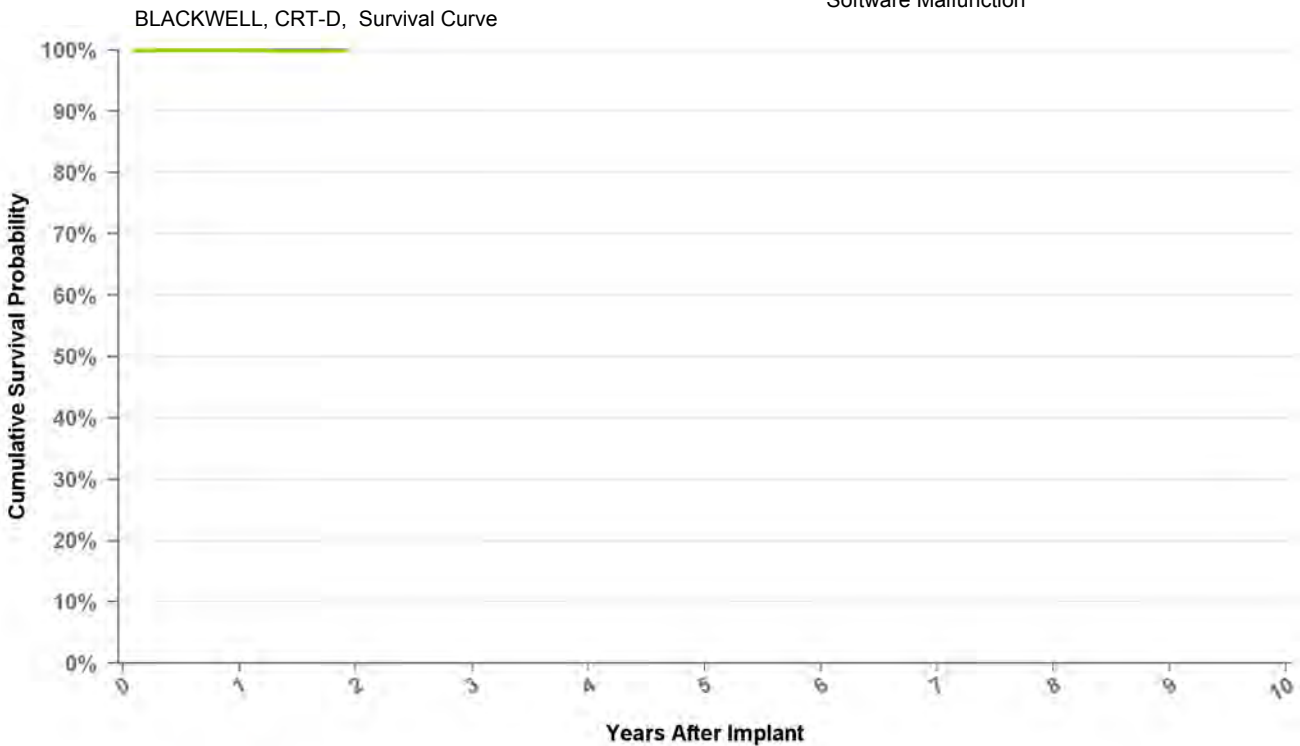

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBB2D4 Viva S

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 08/10/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

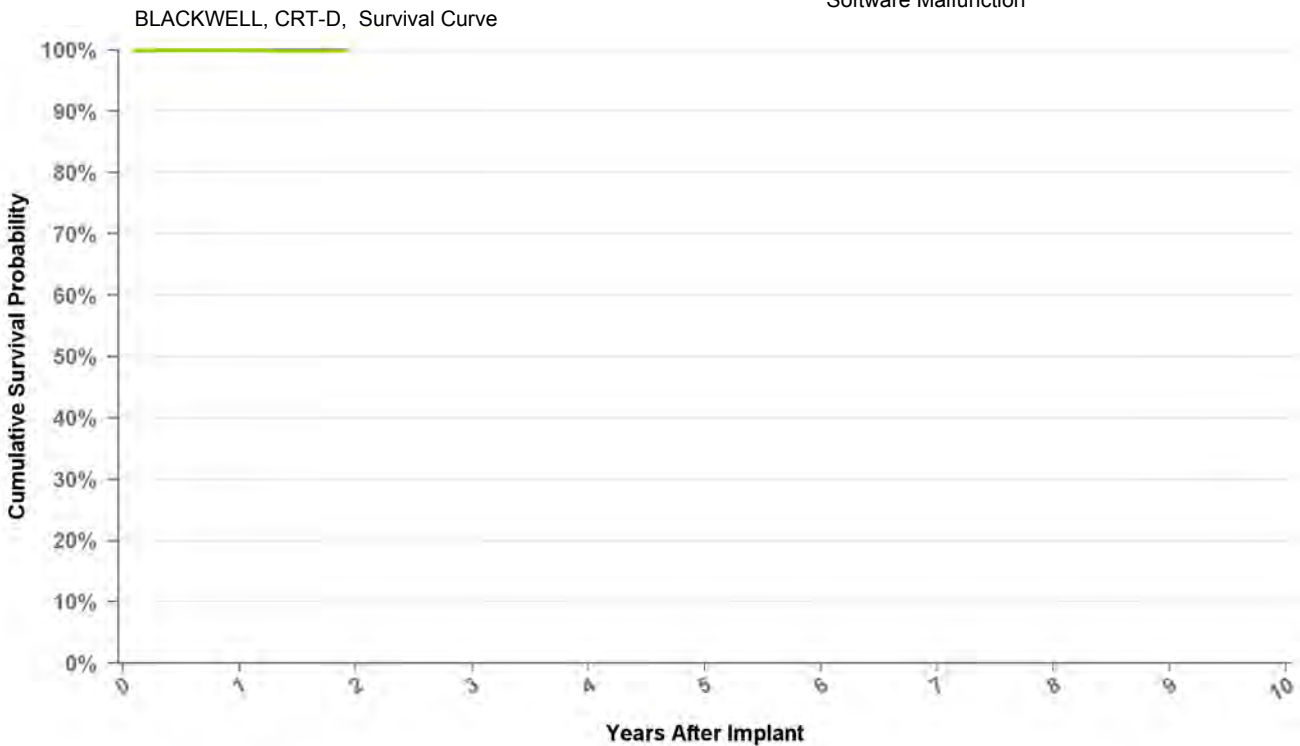

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBB2QQ Viva Quad S

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 08/10/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

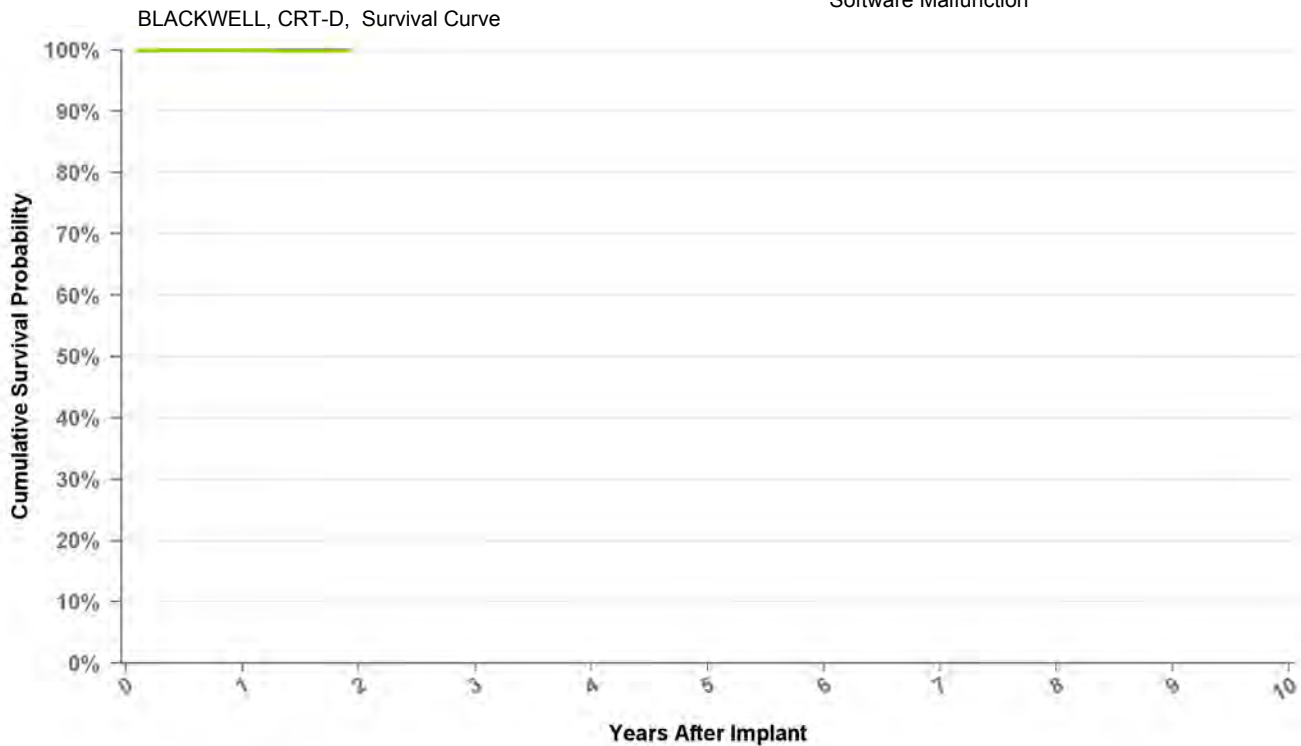

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBC2D1 Brava

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 08/10/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

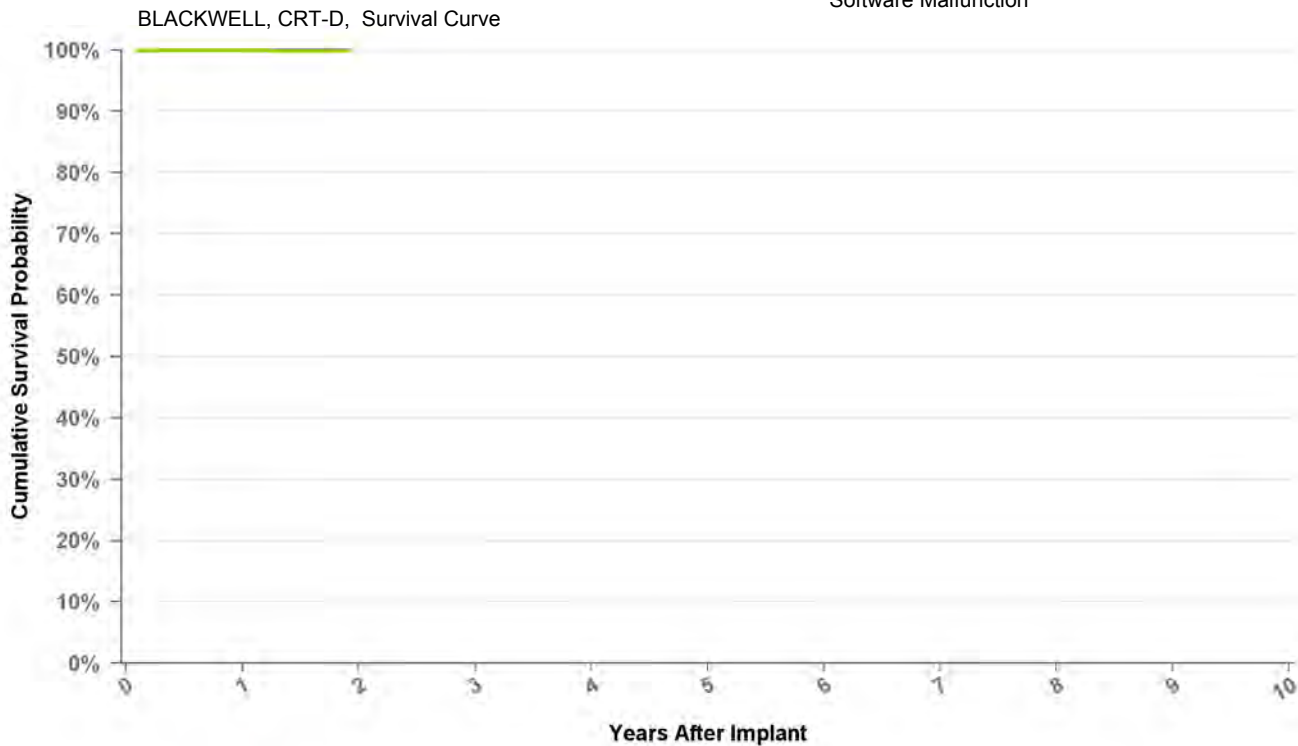

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBC2D4 Brava

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 08/10/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

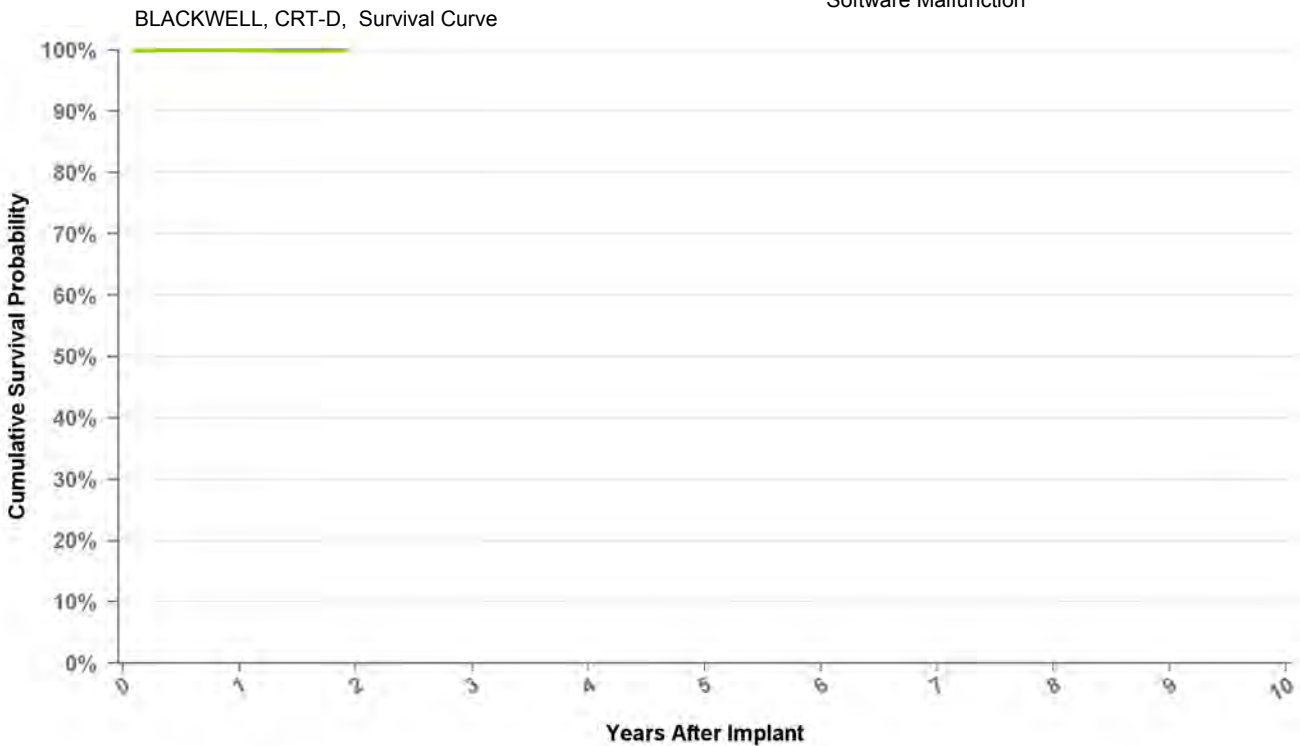

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBC2Q1 Brava Quad

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 09/13/2013 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

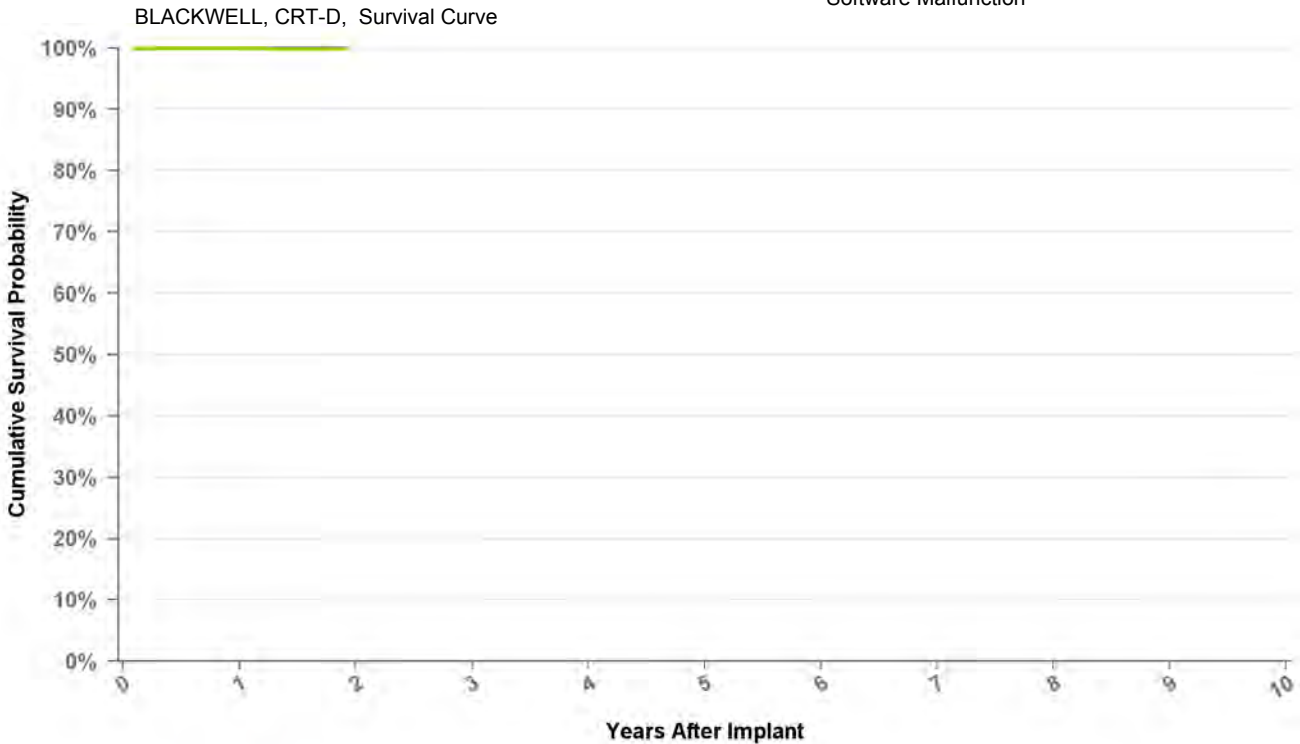

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |

Cardiac Resynchronization Therapy

DTBC2QQ Brava Quad

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 08/10/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

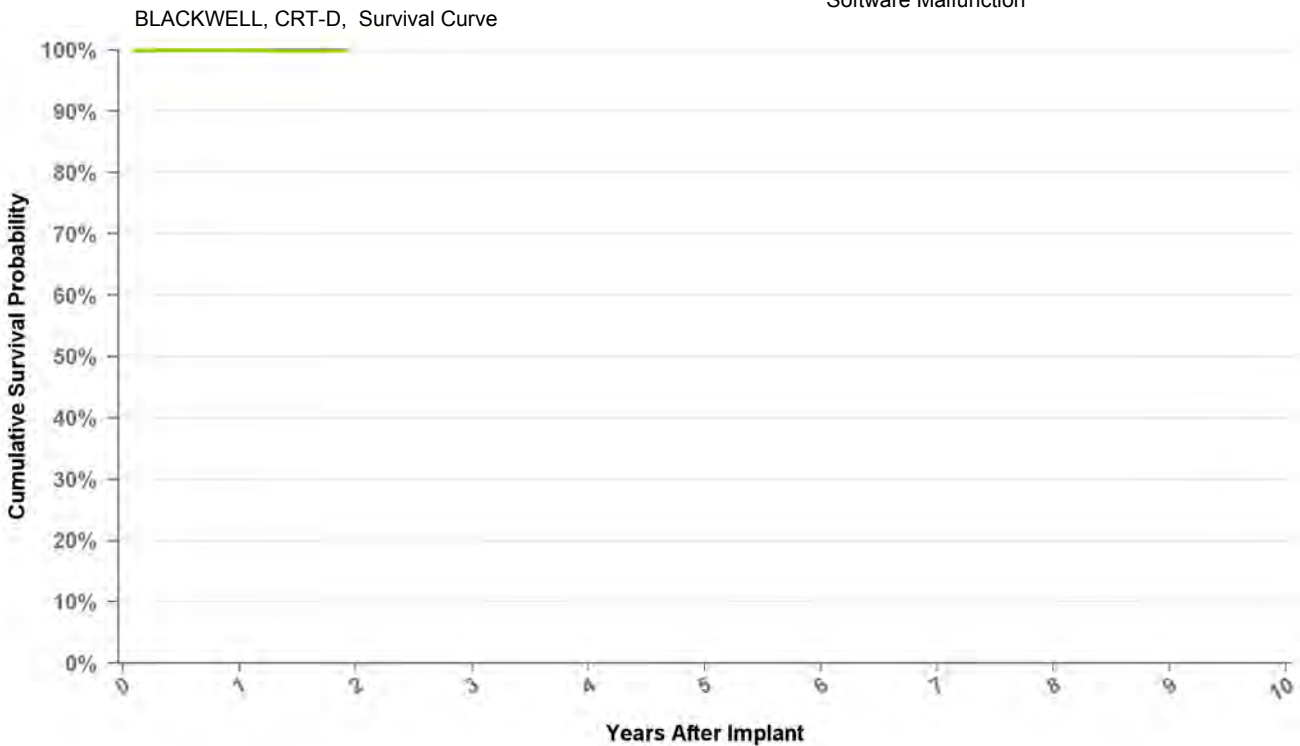

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | at 23 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% |
| Effective Sample Size | 17880 | 140 |


Cardiac Resynchronization Therapy

8040

InSync

| | |
|---------------------------------------|------------|
| US Market Release Date | 08/28/2001 |
| CE Market Approval Date | |
| Registered US Implants | 15,332 |
| Estimated Active US Implants | 1,142 |
| Normal Battery Depletions (US) | 1,501 |
| NBG Code | DDDR |
| Max Delivered Energy | N/A |

| | |
|---|----|
| Total Malfunctions (US) | 34 |
| Therapy Not Compromised Malfunctions | 24 |
| Battery Malfunction | 0 |
| Electrical Component | 4 |
| Electrical Interconnect | 16 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 3 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 10 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 10 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

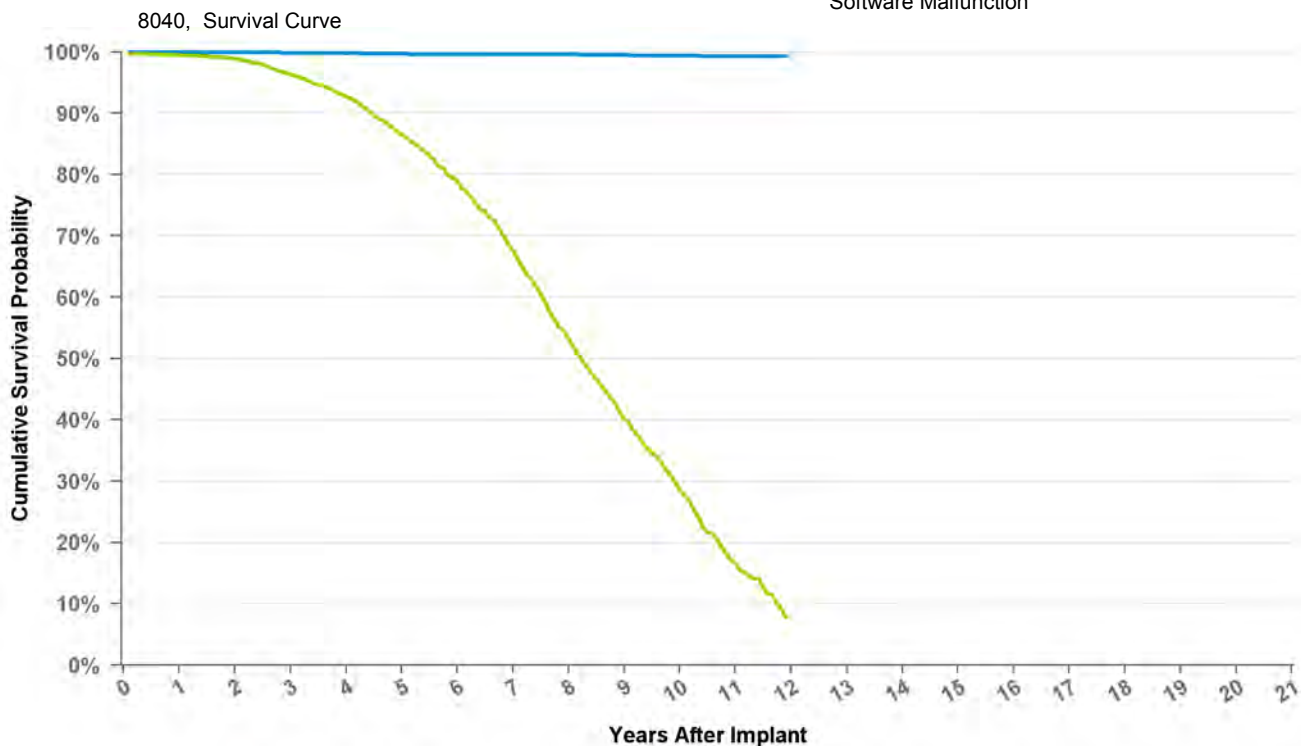

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 143 mo |
|------------------------------|--------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.8% | 99.7% | 99.6% | 99.6% | 99.6% | 99.5% | 99.4% | 99.3% | 99.3% |
| Including NBD | 99.5% | 98.9% | 96.3% | 92.7% | 86.5% | 78.9% | 67.6% | 53.3% | 40.2% | 28.6% | 16.5% | 7.7% |
| Effective Sample Size | 12231 | 10056 | 8027 | 6248 | 4848 | 3666 | 2619 | 1708 | 1082 | 644 | 305 | 101 |


Cardiac Resynchronization Therapy

8042

InSync III

| | |
|---------------------------------------|------------|
| US Market Release Date | 02/25/2003 |
| CE Market Approval Date | 02/07/2001 |
| Registered US Implants | 39,428 |
| Estimated Active US Implants | 11,744 |
| Normal Battery Depletions (US) | 3,326 |
| NBG Code | DDDR |
| Max Delivered Energy | N/A |

| | |
|---|----|
| Total Malfunctions (US) | 29 |
| Therapy Not Compromised Malfunctions | 19 |
| Battery Malfunction | 5 |
| Electrical Component | 2 |
| Electrical Interconnect | 3 |
| Other Malfunction | 7 |
| Poss Early Battery Depltn | 2 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 10 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 10 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

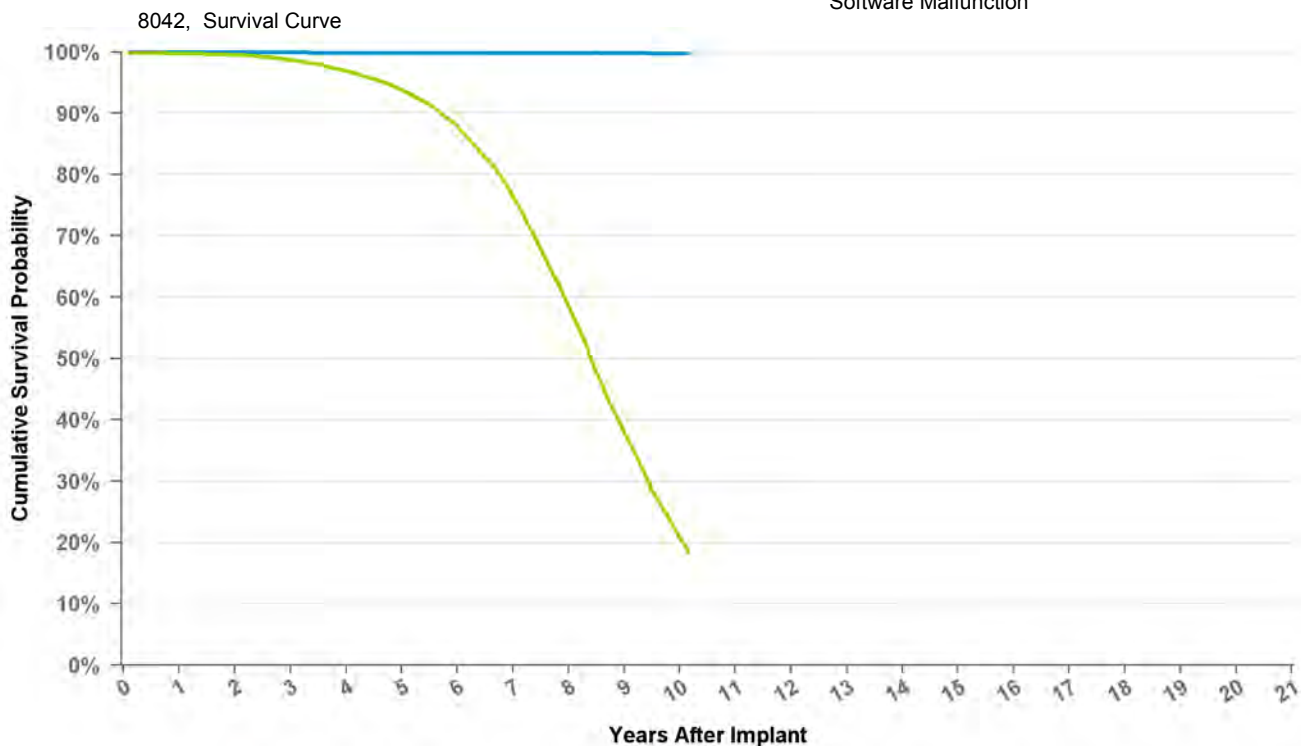

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 122 mo |
|------------------------------|--------|--------|--------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% | 99.8% | 99.7% | 99.7% |
| Including NBD | 99.7% | 99.5% | 98.7% | 96.9% | 93.8% | 87.9% | 76.4% | 58.6% | 37.9% | 20.7% | 18.3% |
| Effective Sample Size | 34468 | 30086 | 26389 | 23155 | 17013 | 11311 | 6964 | 3601 | 1355 | 231 | 125 |

Cardiac Resynchronization Therapy

C2TR01 Syncra CRT-P

| | |
|---------------------------------------|------------|
| US Market Release Date | 03/22/2011 |
| CE Market Approval Date | 05/11/2010 |
| Registered US Implants | 8,281 |
| Estimated Active US Implants | 7,087 |
| Normal Battery Depletions (US) | 6 |
| NBG Code | OOE-DDDR |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

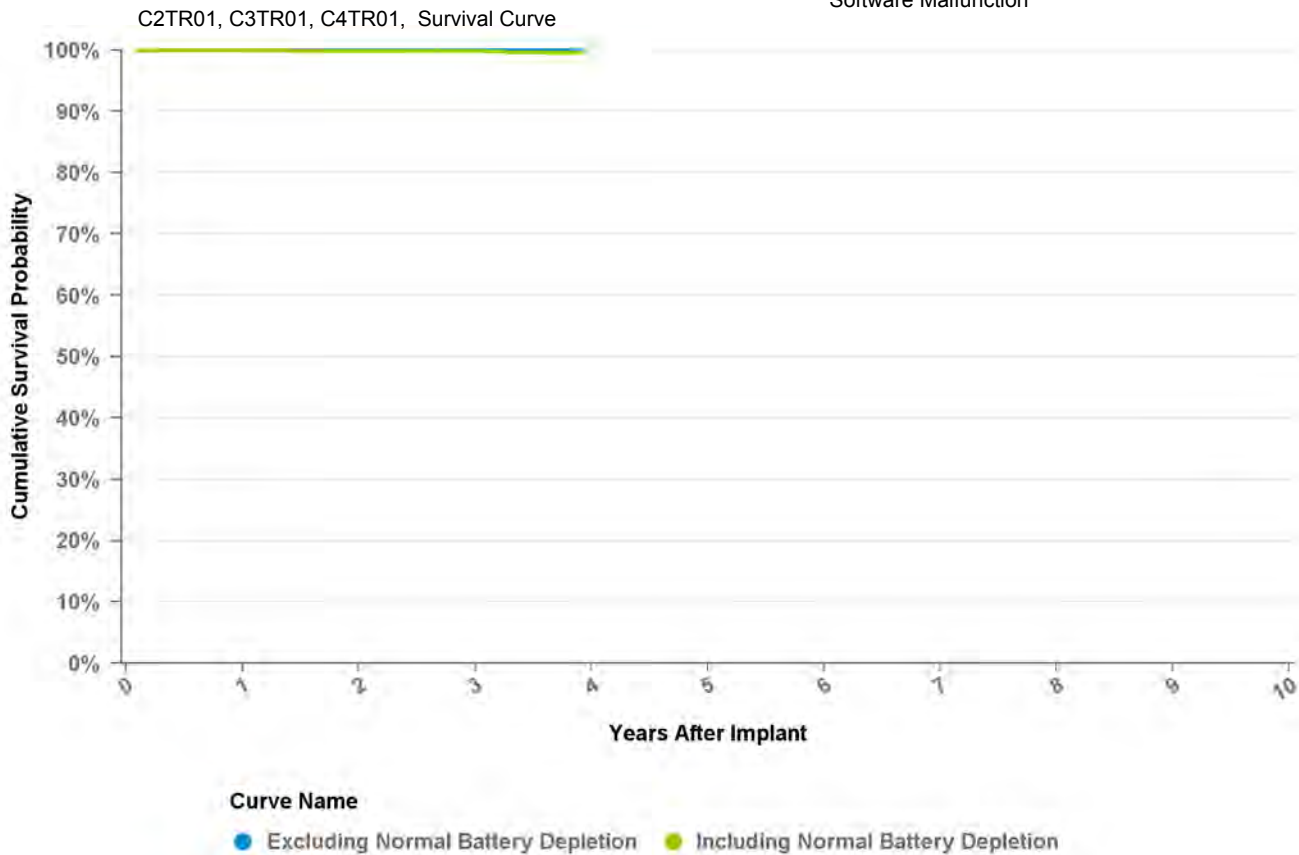


| Years | 1 | 2 | 3 | at 47 mo |
|------------------------------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% | 99.8% | 99.5% |
| Effective Sample Size | 18671 | 11417 | 5076 | 238 |

Cardiac Resynchronization Therapy

C3TR01 Consulta CRT-P

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 05/11/2010 |
| Registered US Implants | 1 |
| Estimated Active US Implants | 1 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | OAE-DDDR |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

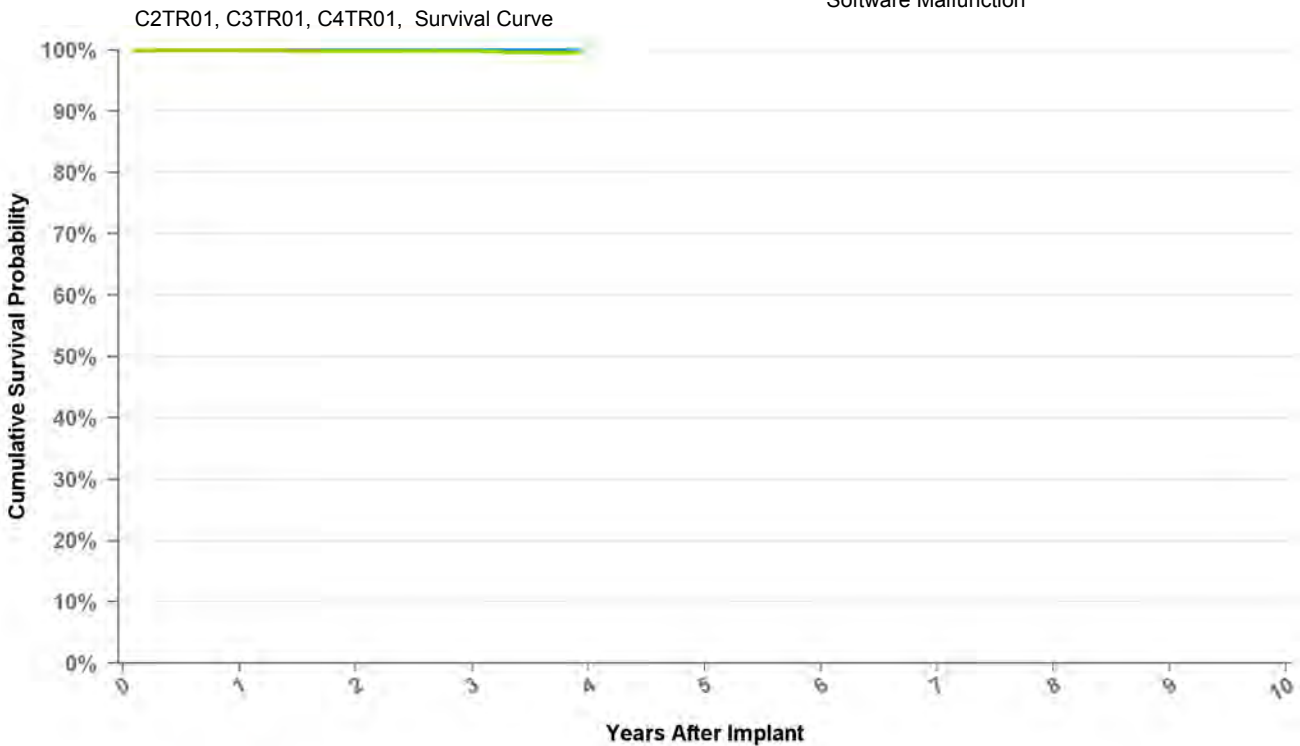

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 47 mo |
|------------------------------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% | 99.8% | 99.5% |
| Effective Sample Size | 18671 | 11417 | 5076 | 238 |

Cardiac Resynchronization Therapy

C4TR01 Consulta CRT-P

US Market Release Date 03/22/2011

CE Market Approval Date

Registered US Implants 16,845

Estimated Active US Implants 15,127

Normal Battery Depletions (US) 11

NBG Code OAE-DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

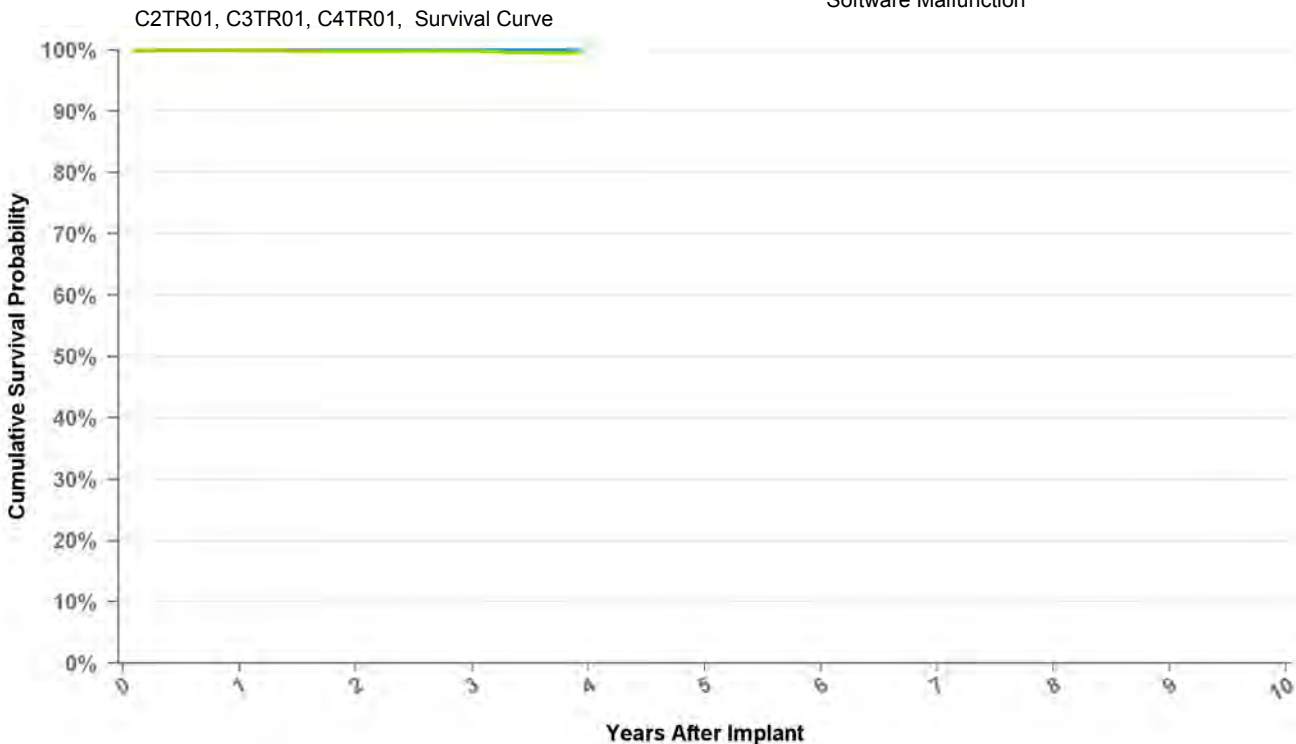

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 47 mo |
|------------------------------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% | 99.8% | 99.5% |
| Effective Sample Size | 18671 | 11417 | 5076 | 238 |


Implantable Cardioverter Defibrillator

7230B

Marquis VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 12/17/2002 |
| CE Market Approval Date | 08/21/2002 |
| Registered US Implants | 237 |
| Estimated Active US Implants | 17 |
| Normal Battery Depletions (US) | 26 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 30J |

| | |
|---|---|
| Total Malfunctions (US) | 1 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 1 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

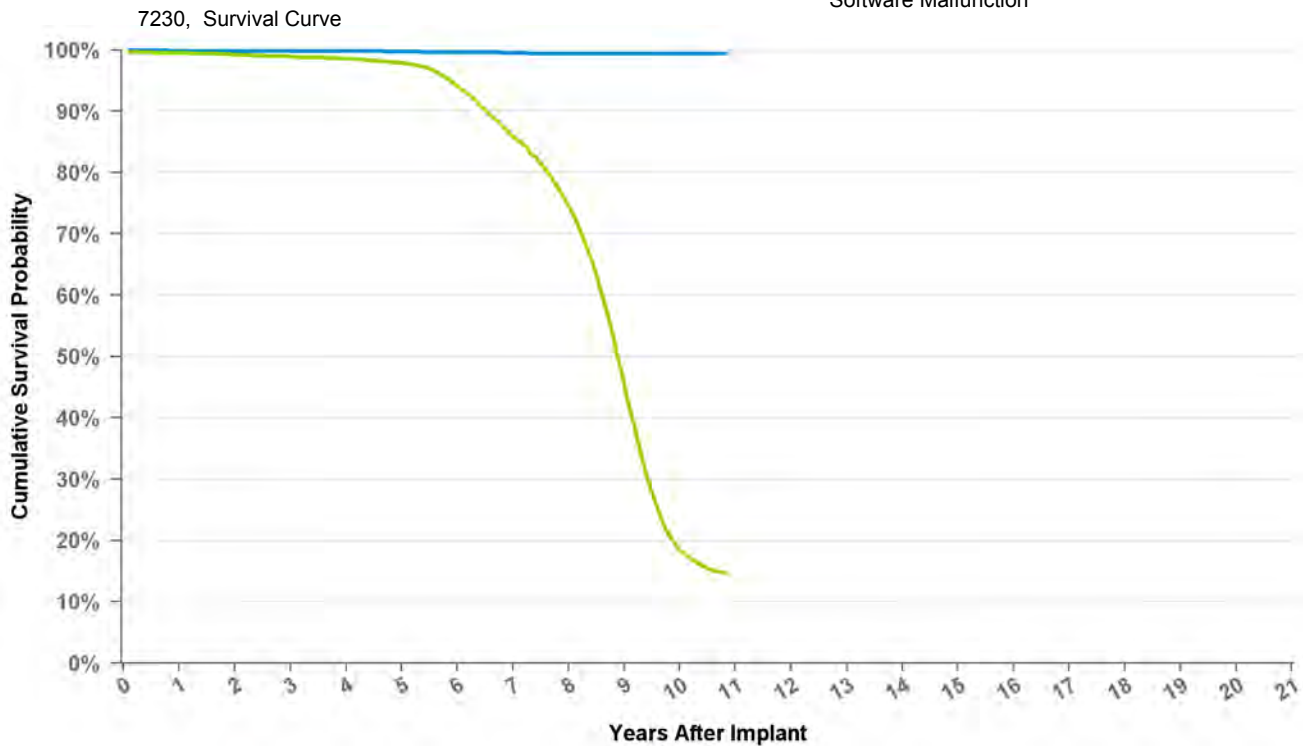

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 130 mo |
|------------------------------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 99.9% | 99.9% | 99.9% | 99.8% | 99.7% | 99.6% | 99.5% | 99.4% | 99.4% | 99.4% | 99.4% |
| Including NBD | 99.5% | 99.2% | 98.9% | 98.6% | 97.9% | 94.1% | 85.9% | 74.6% | 45.4% | 18.4% | 14.7% |
| Effective Sample Size | 17325 | 13571 | 11364 | 10210 | 9151 | 8035 | 6781 | 5477 | 3090 | 845 | 107 |


Implantable Cardioverter Defibrillator

7230Cx

Marquis VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 12/17/2002 |
| CE Market Approval Date | 04/10/2002 |
| Registered US Implants | 18,565 |
| Estimated Active US Implants | 1,735 |
| Normal Battery Depletions (US) | 3,324 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 30J |

| | |
|---|----|
| Total Malfunctions (US) | 57 |
| Therapy Not Compromised Malfunctions | 31 |
| Battery Malfunction | 1 |
| Electrical Component | 14 |
| Electrical Interconnect | 0 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 14 |
| Software Malfunction | 1 |
| Therapy Compromised Malfunctions | 26 |
| Battery Malfunction | 17 |
| Electrical Component | 9 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

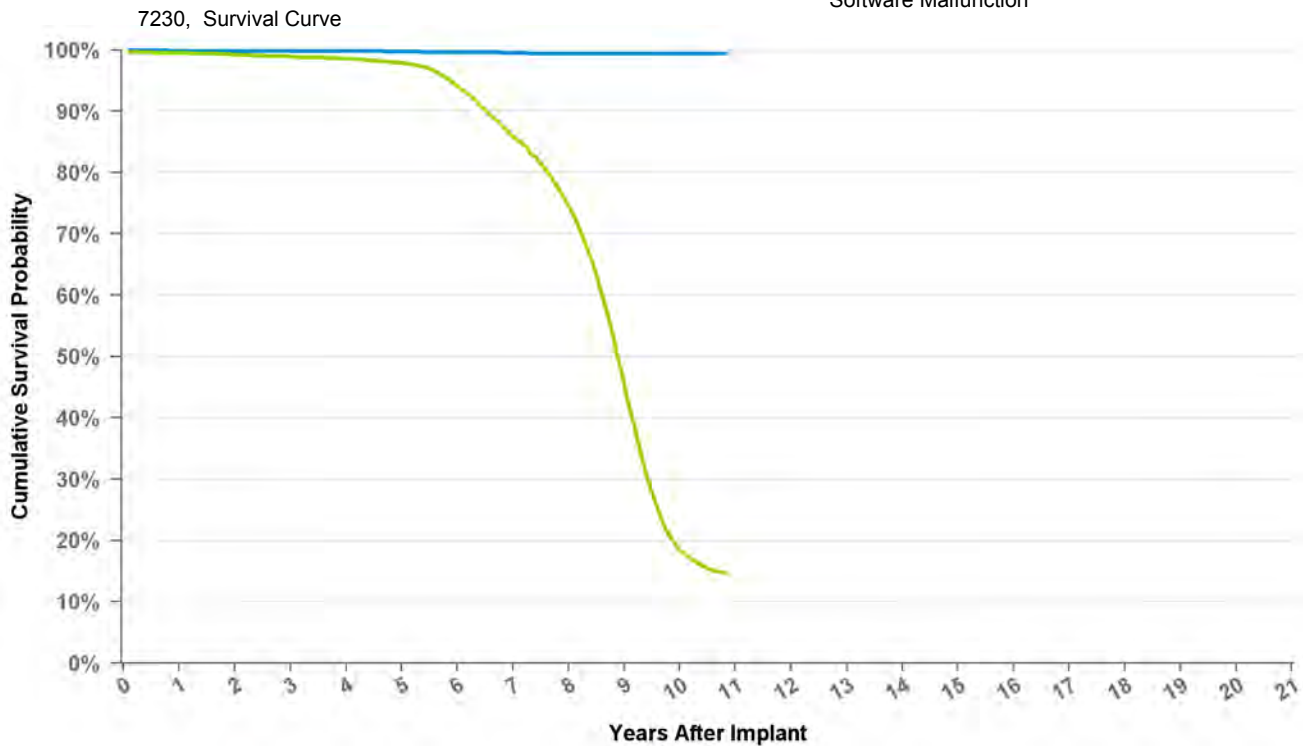

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 130 mo |
|------------------------------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 99.9% | 99.9% | 99.9% | 99.8% | 99.7% | 99.6% | 99.5% | 99.4% | 99.4% | 99.4% | 99.4% |
| Including NBD | 99.5% | 99.2% | 98.9% | 98.6% | 97.9% | 94.1% | 85.9% | 74.6% | 45.4% | 18.4% | 14.7% |
| Effective Sample Size | 17325 | 13571 | 11364 | 10210 | 9151 | 8035 | 6781 | 5477 | 3090 | 845 | 107 |


Implantable Cardioverter Defibrillator

7230E

Marquis VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 12/17/2002 |
| CE Market Approval Date | 08/21/2002 |
| Registered US Implants | 633 |
| Estimated Active US Implants | 62 |
| Normal Battery Depletions (US) | 77 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 30J |

| | |
|---|---|
| Total Malfunctions (US) | 3 |
| Therapy Not Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 2 |
| Battery Malfunction | 2 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

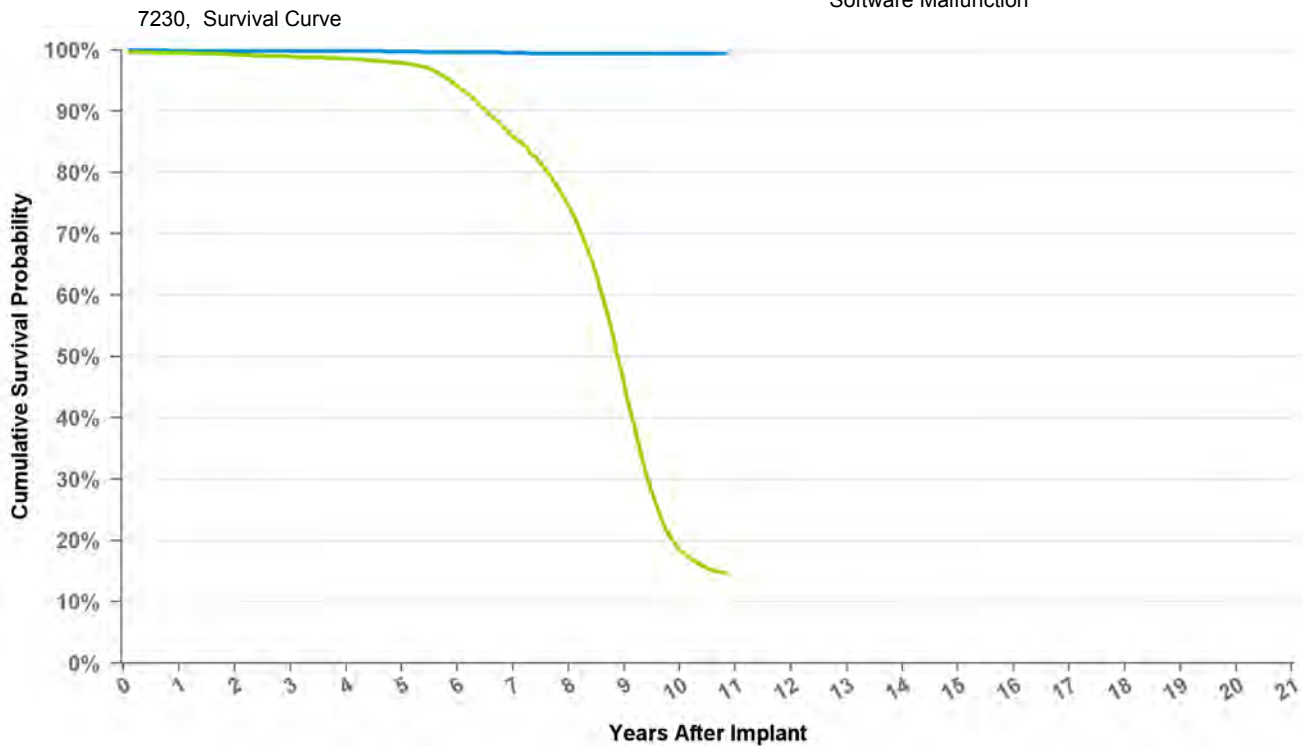

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 130 mo |
|------------------------------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 99.9% | 99.9% | 99.9% | 99.8% | 99.7% | 99.6% | 99.5% | 99.4% | 99.4% | 99.4% | 99.4% |
| Including NBD | 99.5% | 99.2% | 98.9% | 98.6% | 97.9% | 94.1% | 85.9% | 74.6% | 45.4% | 18.4% | 14.7% |
| Effective Sample Size | 17325 | 13571 | 11364 | 10210 | 9151 | 8035 | 6781 | 5477 | 3090 | 845 | 107 |


Implantable Cardioverter Defibrillator

7231Cx

GEM III VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 12/12/2000 |
| CE Market Approval Date | 12/08/2000 |
| Registered US Implants | 17,494 |
| Estimated Active US Implants | 1,474 |
| Normal Battery Depletions (US) | 3,915 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 30J |

| | |
|---|----|
| Total Malfunctions (US) | 36 |
| Therapy Not Compromised Malfunctions | 26 |
| Battery Malfunction | 1 |
| Electrical Component | 21 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 4 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 10 |
| Battery Malfunction | 1 |
| Electrical Component | 8 |
| Electrical Interconnect | 1 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

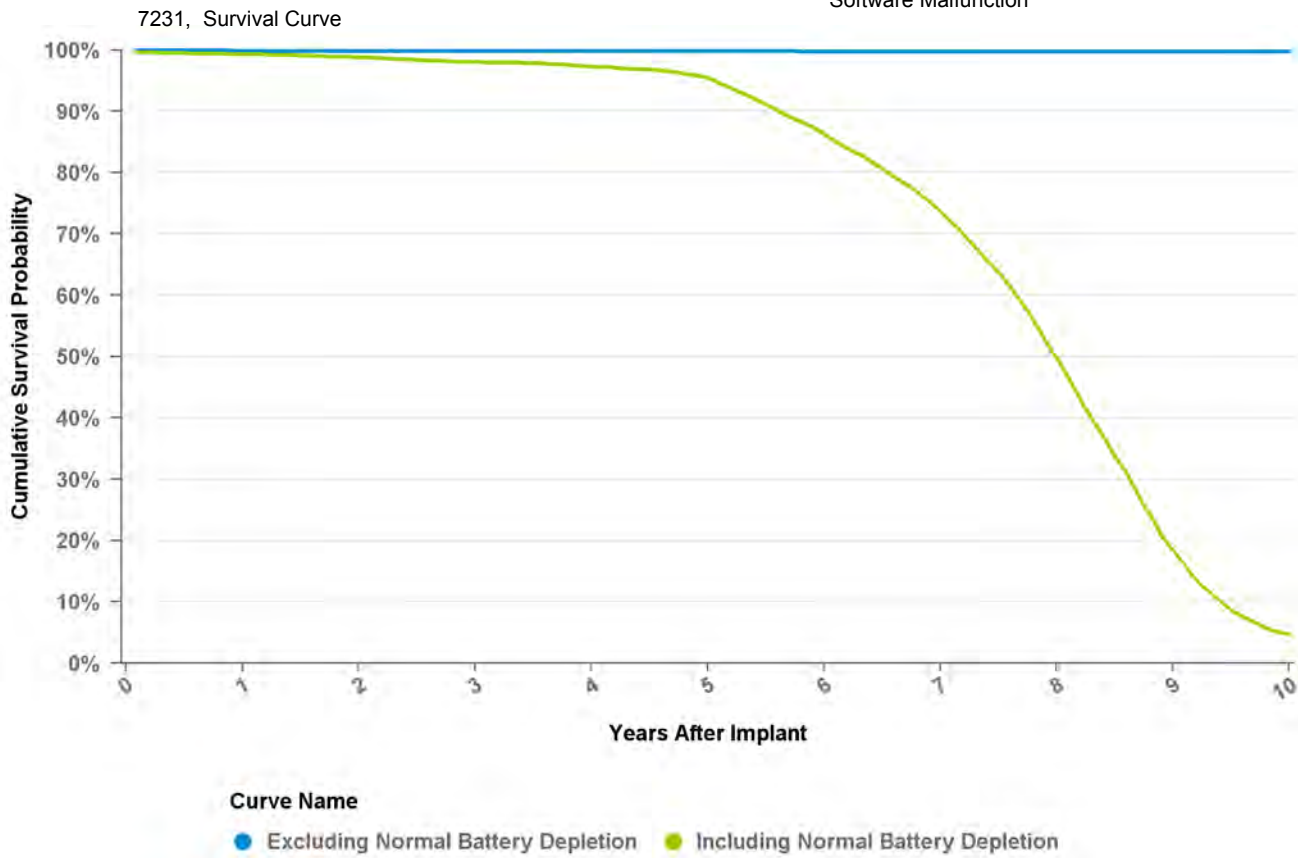

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 120 mo |
|------------------------------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 99.9% | 99.9% | 99.8% | 99.8% | 99.8% | 99.7% | 99.7% | 99.7% | 99.7% | 99.7% |
| Including NBD | 99.3% | 98.8% | 98.1% | 97.3% | 95.5% | 86.3% | 73.6% | 49.9% | 18.5% | 4.7% |
| Effective Sample Size | 15740 | 14055 | 12441 | 10949 | 9552 | 7901 | 6156 | 3750 | 1114 | 103 |


Implantable Cardioverter Defibrillator

7232B

Maximo VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 10/06/2003 |
| CE Market Approval Date | 10/22/2004 |
| Registered US Implants | 170 |
| Estimated Active US Implants | 59 |
| Normal Battery Depletions (US) | 18 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

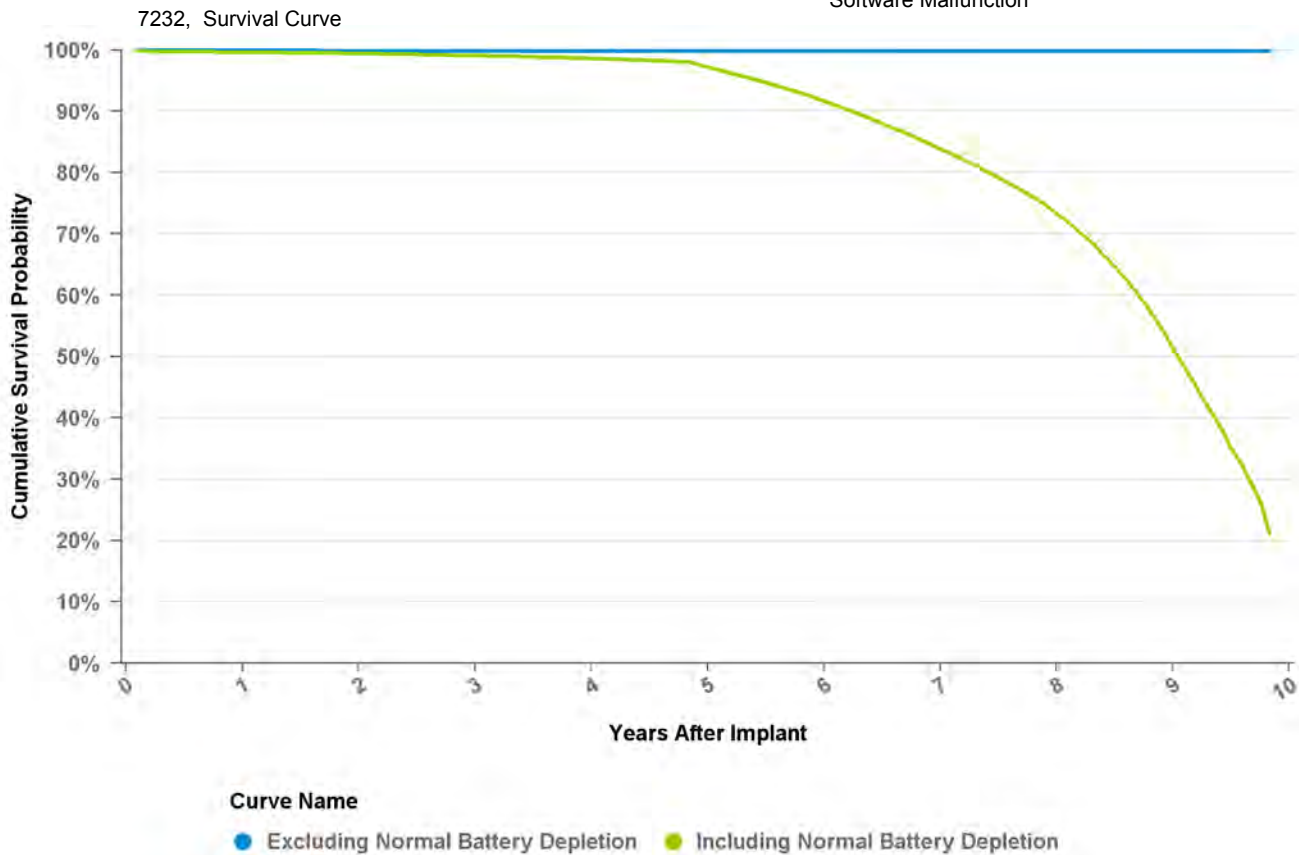

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 118 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% | 99.8% | 99.8% | 99.8% | 99.8% | 99.8% | 99.8% |
| Including NBD | 99.6% | 99.4% | 99.1% | 98.6% | 97.2% | 91.7% | 83.8% | 73.3% | 51.4% | 21.1% |
| Effective Sample Size | 40686 | 36632 | 32881 | 29216 | 25876 | 22472 | 18411 | 13726 | 6636 | 331 |


Implantable Cardioverter Defibrillator

7232Cx

Maximo VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 10/06/2003 |
| CE Market Approval Date | 10/28/2003 |
| Registered US Implants | 43,681 |
| Estimated Active US Implants | 11,144 |
| Normal Battery Depletions (US) | 7,268 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35J |

| | |
|---|----|
| Total Malfunctions (US) | 76 |
| Therapy Not Compromised Malfunctions | 61 |
| Battery Malfunction | 0 |
| Electrical Component | 28 |
| Electrical Interconnect | 0 |
| Other Malfunction | 6 |
| Poss Early Battery Depltn | 25 |
| Software Malfunction | 2 |
| Therapy Compromised Malfunctions | 15 |
| Battery Malfunction | 0 |
| Electrical Component | 12 |
| Electrical Interconnect | 1 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |

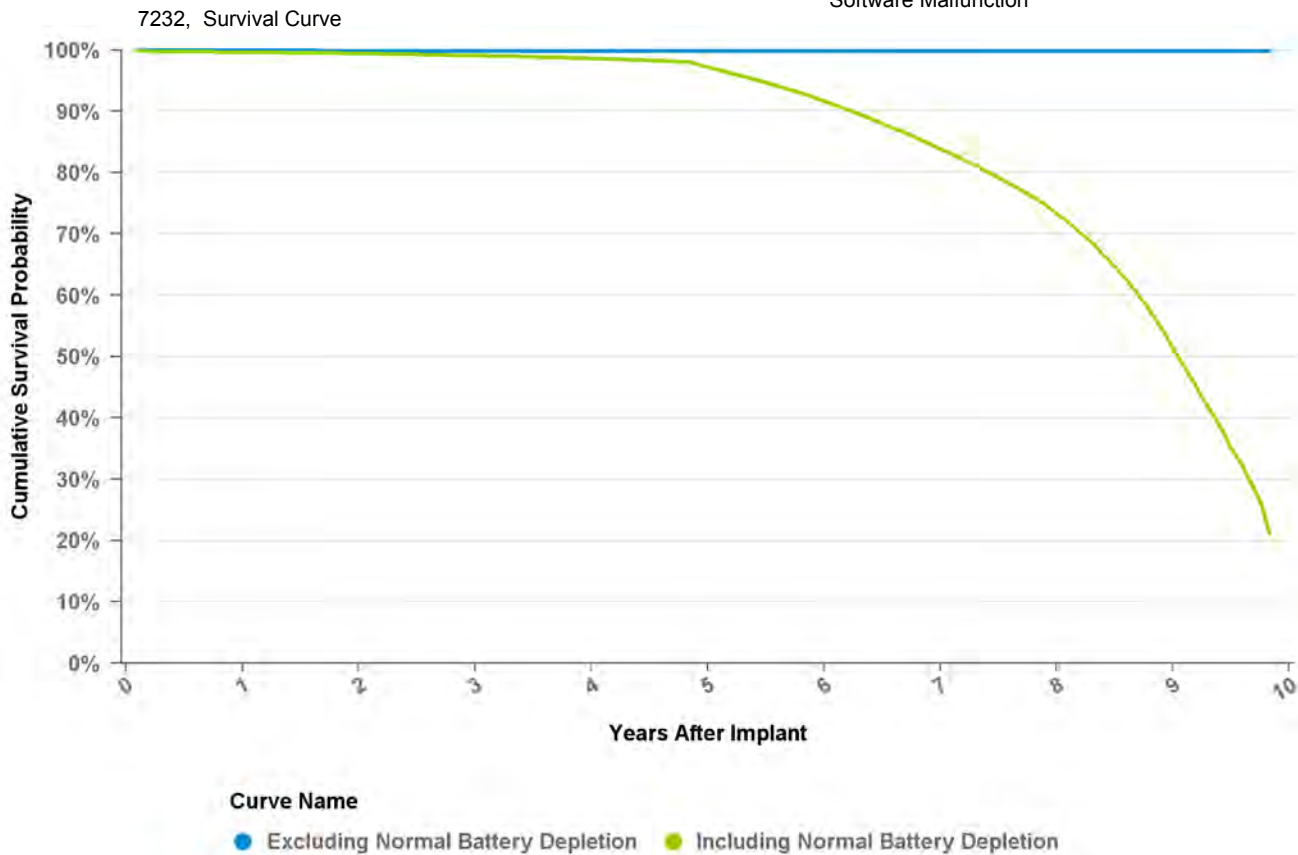

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 118 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% | 99.8% | 99.8% | 99.8% | 99.8% | 99.8% | 99.8% |
| Including NBD | 99.6% | 99.4% | 99.1% | 98.6% | 97.2% | 91.7% | 83.8% | 73.3% | 51.4% | 21.1% |
| Effective Sample Size | 40686 | 36632 | 32881 | 29216 | 25876 | 22472 | 18411 | 13726 | 6636 | 331 |


Implantable Cardioverter Defibrillator

7232E

Maximo VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 10/06/2003 |
| CE Market Approval Date | 10/22/2004 |
| Registered US Implants | 491 |
| Estimated Active US Implants | 149 |
| Normal Battery Depletions (US) | 41 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35J |

| | |
|---|---|
| Total Malfunctions (US) | 1 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

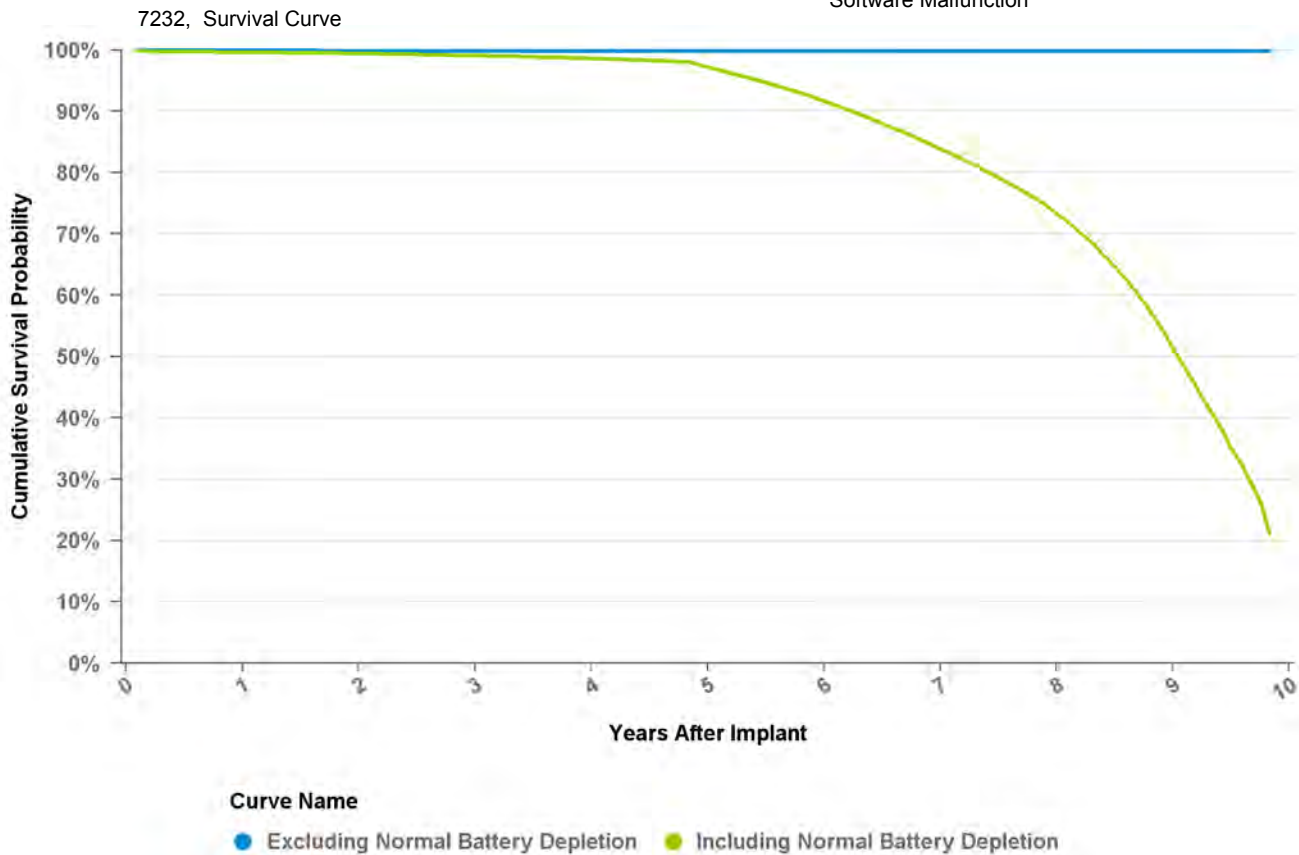

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 118 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.9% | 99.8% | 99.8% | 99.8% | 99.8% | 99.8% | 99.8% |
| Including NBD | 99.6% | 99.4% | 99.1% | 98.6% | 97.2% | 91.7% | 83.8% | 73.3% | 51.4% | 21.1% |
| Effective Sample Size | 40686 | 36632 | 32881 | 29216 | 25876 | 22472 | 18411 | 13726 | 6636 | 331 |


Implantable Cardioverter Defibrillator

7274

Marquis DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 03/01/2002 |
| CE Market Approval Date | 02/25/2002 |
| Registered US Implants | 48,387 |
| Estimated Active US Implants | 2,616 |
| Normal Battery Depletions (US) | 9,077 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 30J |

| | |
|---|-----|
| Total Malfunctions (US) | 196 |
| Therapy Not Compromised Malfunctions | 89 |
| Battery Malfunction | 6 |
| Electrical Component | 31 |
| Electrical Interconnect | 0 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 51 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 107 |
| Battery Malfunction | 80 |
| Electrical Component | 27 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

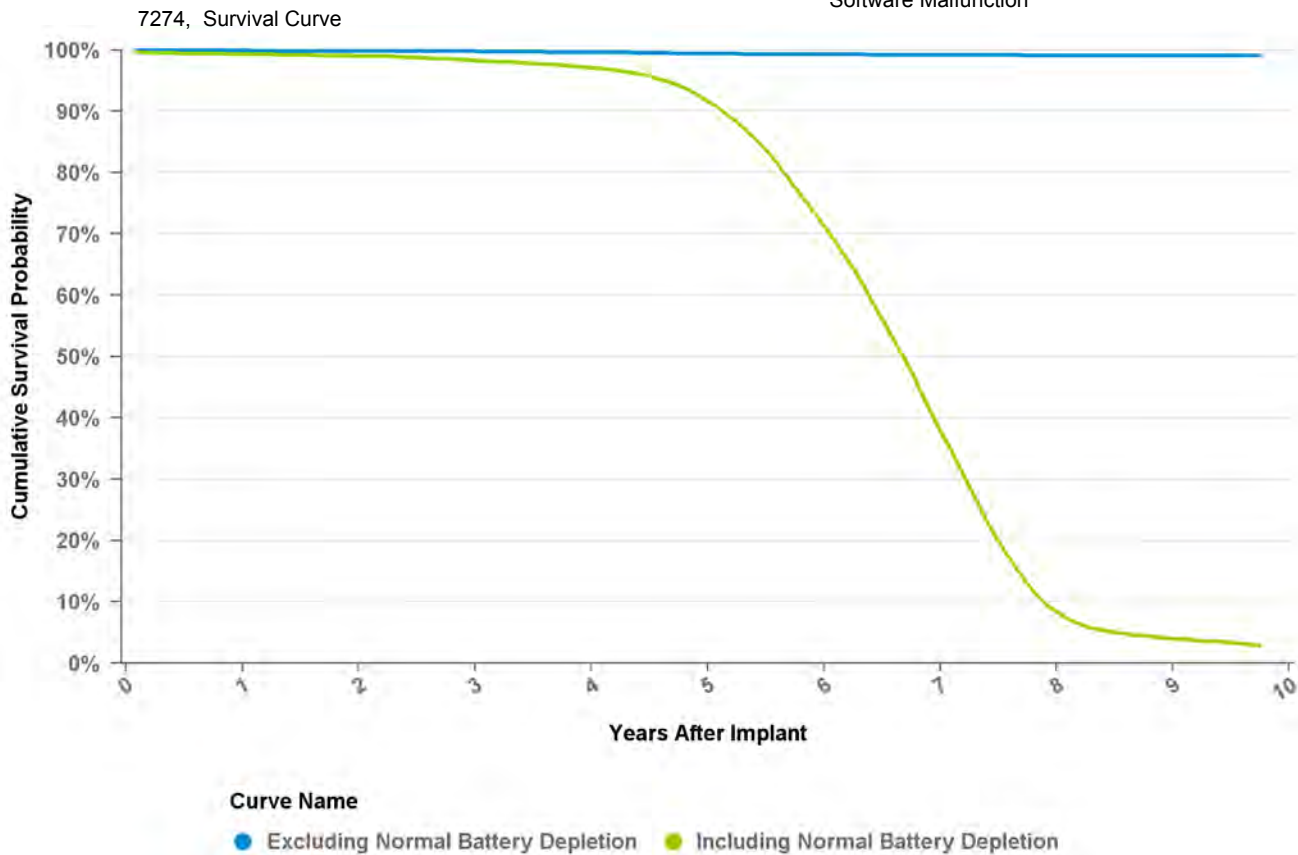

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 117 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 99.9% | 99.8% | 99.6% | 99.4% | 99.3% | 99.2% | 99.1% | 99.1% | 99.1% |
| Including NBD | 99.3% | 99.0% | 98.3% | 97.1% | 91.6% | 71.4% | 37.9% | 8.4% | 4.0% | 2.9% |
| Effective Sample Size | 42837 | 34501 | 26566 | 22609 | 18798 | 12963 | 6049 | 1015 | 298 | 104 |


Implantable Cardioverter Defibrillator

7278

Maximo DR

| | |
|---|----|
| Total Malfunctions (US) | 72 |
| Therapy Not Compromised Malfunctions | 62 |
| Battery Malfunction | 0 |
| Electrical Component | 24 |
| Electrical Interconnect | 0 |
| Other Malfunction | 4 |
| Poss Early Battery Depltn | 34 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 10 |
| Battery Malfunction | 0 |
| Electrical Component | 9 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |

| | |
|---------------------------------------|------------|
| US Market Release Date | 10/06/2003 |
| CE Market Approval Date | 10/28/2003 |
| Registered US Implants | 37,666 |
| Estimated Active US Implants | 4,094 |
| Normal Battery Depletions (US) | 10,483 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 35J |

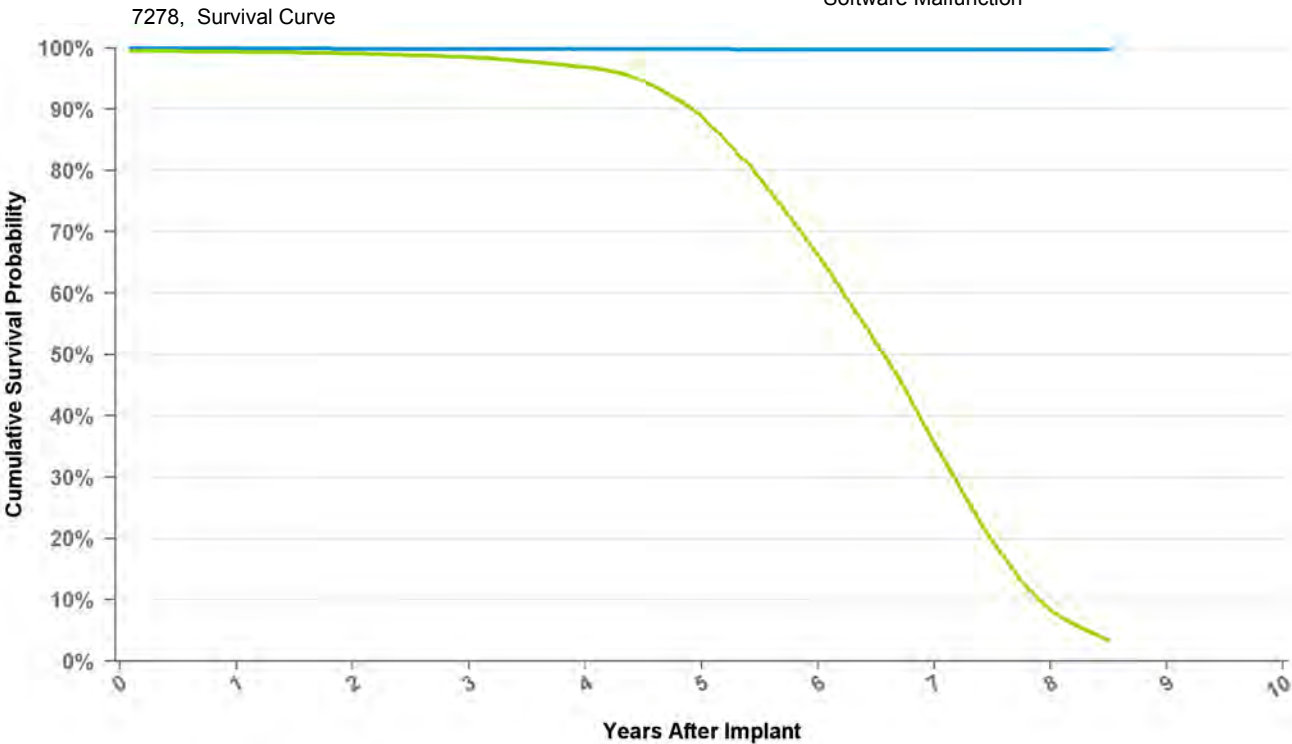

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 102 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.8% | 99.8% | 99.7% | 99.7% | 99.7% | 99.7% |
| Including NBD | 99.4% | 99.1% | 98.5% | 96.9% | 88.8% | 66.3% | 35.6% | 8.3% | 3.3% |
| Effective Sample Size | 33861 | 30308 | 27185 | 23955 | 19874 | 13308 | 6138 | 1053 | 207 |

Implantable Cardioverter Defibrillator

7288

Intrinsic

Total Malfunctions (US)

71

Therapy Not Compromised Malfunctions

64

Battery Malfunction

2

Electrical Component

27

Electrical Interconnect

0

Other Malfunction

1

Poss Early Battery Depltn

33

Software Malfunction

1

Therapy Compromised Malfunctions

7

Battery Malfunction

0

Electrical Component

5

Electrical Interconnect

0

Other Malfunction

2

Poss Early Battery Depltn

0

Software Malfunction

0

US Market Release Date 06/21/2004

CE Market Approval Date 05/04/2004

Registered US Implants 30,665


Estimated Active US Implants 2,870

Normal Battery Depletions (US) 10,029

NBG Code VVE-DDDR

Max Delivered Energy 35J

7288, Survival Curve

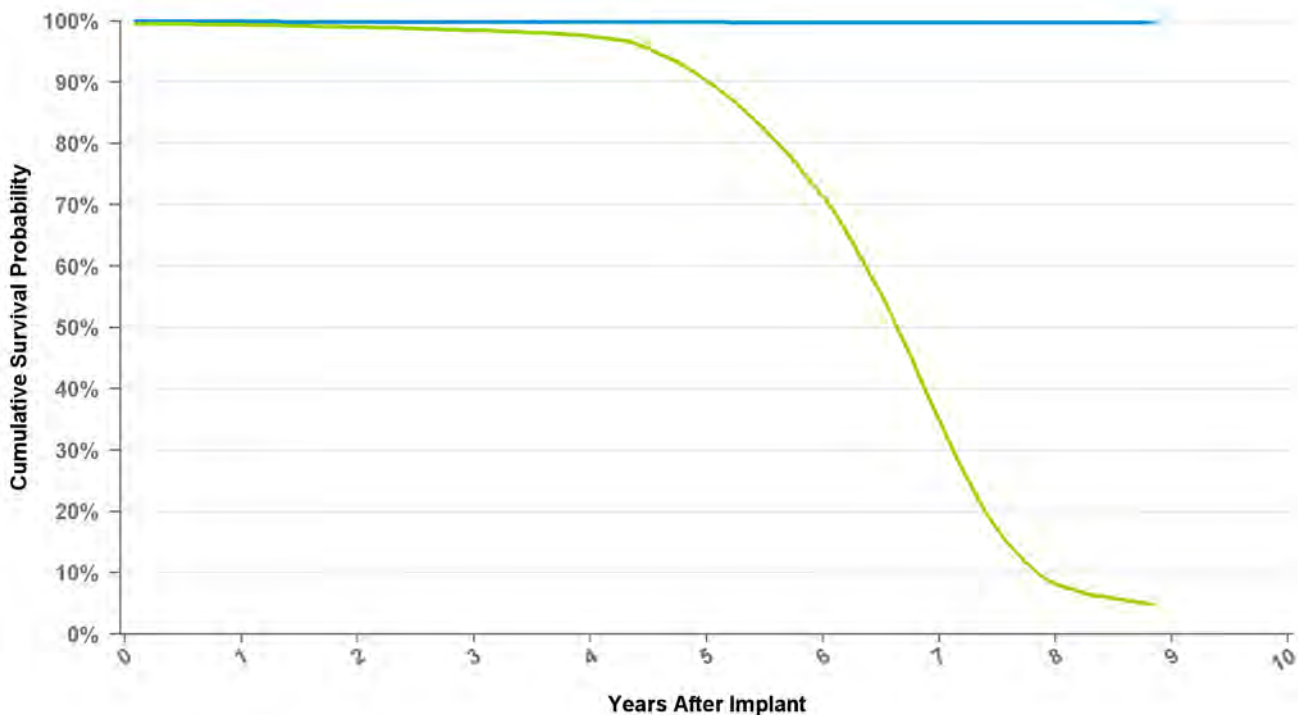

Curve Name

● Excluding Normal Battery Depletion

● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 106 mo |
|-----------------------|--------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.8% | 99.8% | 99.7% | 99.7% | 99.7% | 99.7% |
| Including NBD | 99.4% | 99.0% | 98.5% | 97.5% | 90.2% | 71.4% | 34.9% | 8.1% | 4.8% |
| Effective Sample Size | 28595 | 26260 | 23691 | 20984 | 17800 | 12924 | 5869 | 954 | 140 |

Implantable Cardioverter Defibrillator

D144DRG Entrust Escudo

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 06/05/2008 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

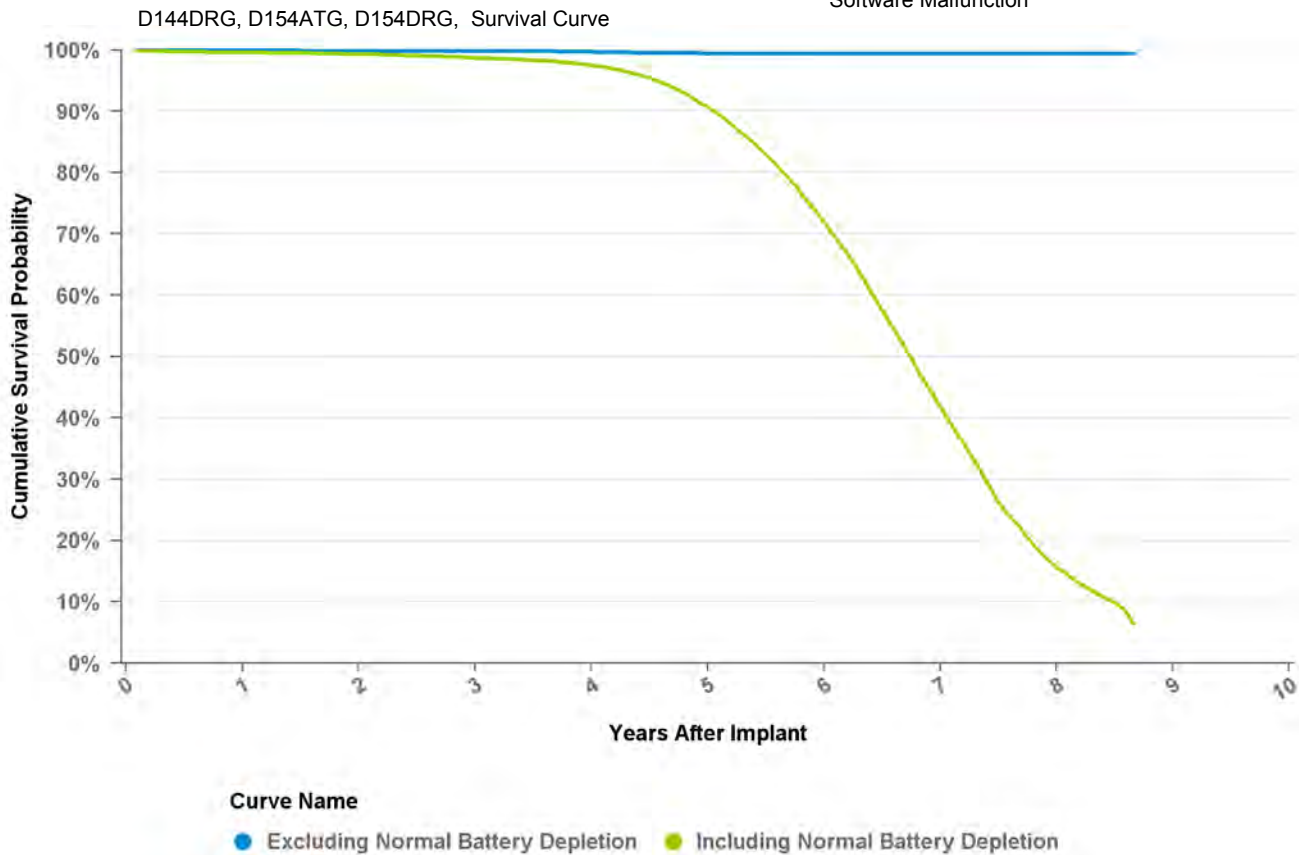

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 104 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 99.9% | 99.8% | 99.7% | 99.4% | 99.4% | 99.4% | 99.4% | 99.4% |
| Including NBD | 99.6% | 99.3% | 98.7% | 97.5% | 90.7% | 72.0% | 41.8% | 15.6% | 6.4% |
| Effective Sample Size | 26272 | 24061 | 21693 | 19252 | 16148 | 11945 | 6073 | 1727 | 107 |


Implantable Cardioverter Defibrillator

D144VRC Entrust Escudo

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 06/05/2008 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

D144VRC, D154VRC, Survival Curve

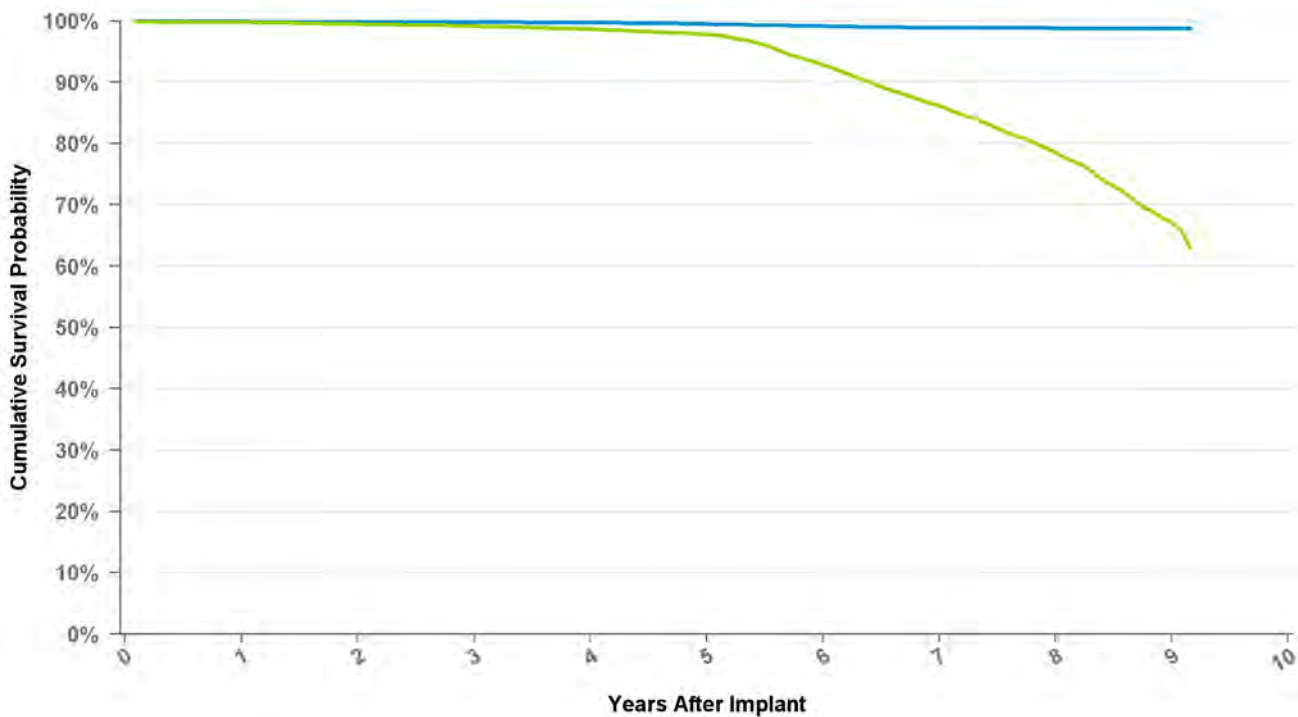

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 110 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 99.9% | 99.8% | 99.7% | 99.5% | 99.2% | 98.9% | 98.8% | 98.8% | 98.8% |
| Including NBD | 99.8% | 99.5% | 99.2% | 98.7% | 97.8% | 92.8% | 86.2% | 78.5% | 67.1% | 62.9% |
| Effective Sample Size | 13630 | 12418 | 11171 | 9950 | 8872 | 7862 | 6558 | 4915 | 777 | 270 |

Implantable Cardioverter Defibrillator

D154ATG Entrust AT

| | |
|---------------------------------------|------------|
| US Market Release Date | 06/30/2005 |
| CE Market Approval Date | 02/04/2005 |
| Registered US Implants | 28,169 |
| Estimated Active US Implants | 3,680 |
| Normal Battery Depletions (US) | 8,572 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|-----|
| Total Malfunctions (US) | 124 |
| Therapy Not Compromised Malfunctions | 110 |
| Battery Malfunction | 0 |
| Electrical Component | 30 |
| Electrical Interconnect | 1 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 75 |
| Software Malfunction | 3 |
| Therapy Compromised Malfunctions | 14 |
| Battery Malfunction | 0 |
| Electrical Component | 14 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

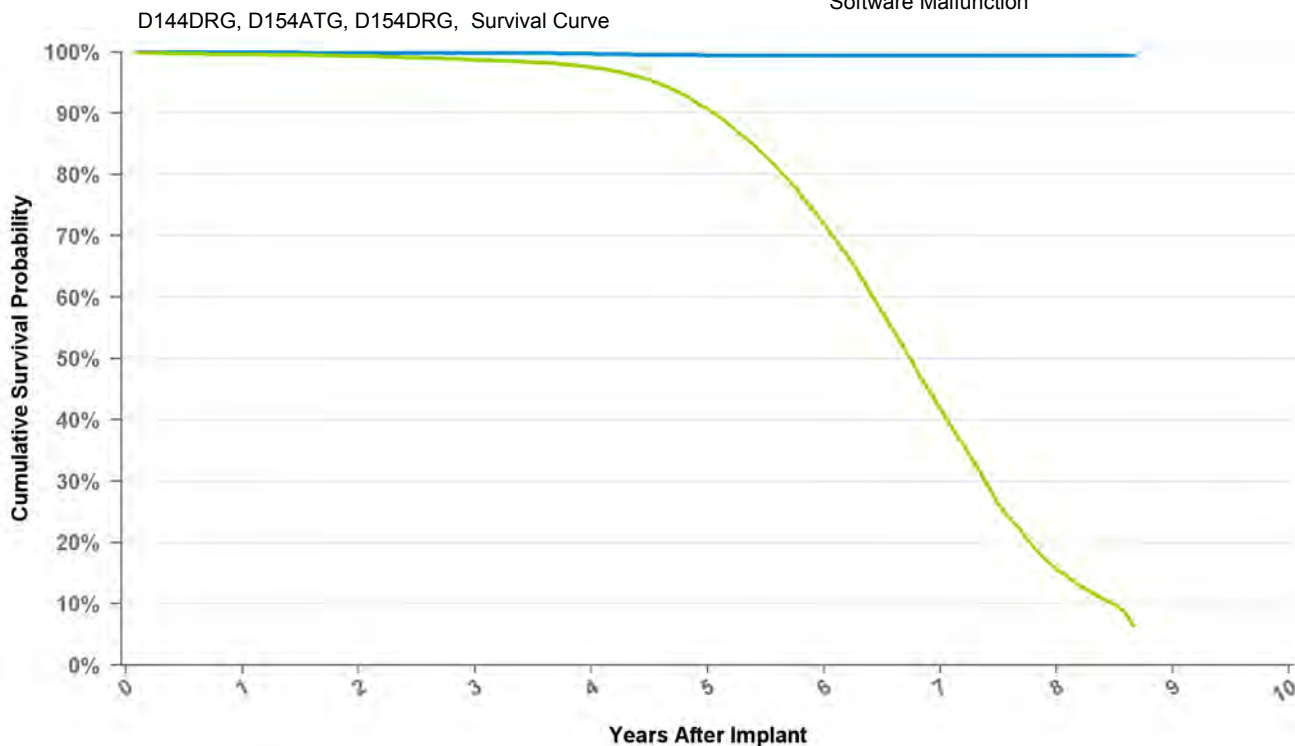

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 104 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 99.9% | 99.8% | 99.7% | 99.4% | 99.4% | 99.4% | 99.4% | 99.4% |
| Including NBD | 99.6% | 99.3% | 98.7% | 97.5% | 90.7% | 72.0% | 41.8% | 15.6% | 6.4% |
| Effective Sample Size | 26272 | 24061 | 21693 | 19252 | 16148 | 11945 | 6073 | 1727 | 107 |

Implantable Cardioverter Defibrillator

D154AWG Virtuoso DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 05/12/2006 |
| CE Market Approval Date | |
| Registered US Implants | 72,709 |
| Estimated Active US Implants | 25,470 |
| Normal Battery Depletions (US) | 13,847 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|-------|
| Total Malfunctions (US) | 1,455 |
| Therapy Not Compromised Malfunctions | 1,426 |
| Battery Malfunction | 6 |
| Electrical Component | 1,277 |
| Electrical Interconnect | 2 |
| Other Malfunction | 4 |
| Poss Early Battery Depltn | 133 |
| Software Malfunction | 4 |
| Therapy Compromised Malfunctions | 29 |
| Battery Malfunction | 0 |
| Electrical Component | 26 |
| Electrical Interconnect | 0 |
| Other Malfunction | 2 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |

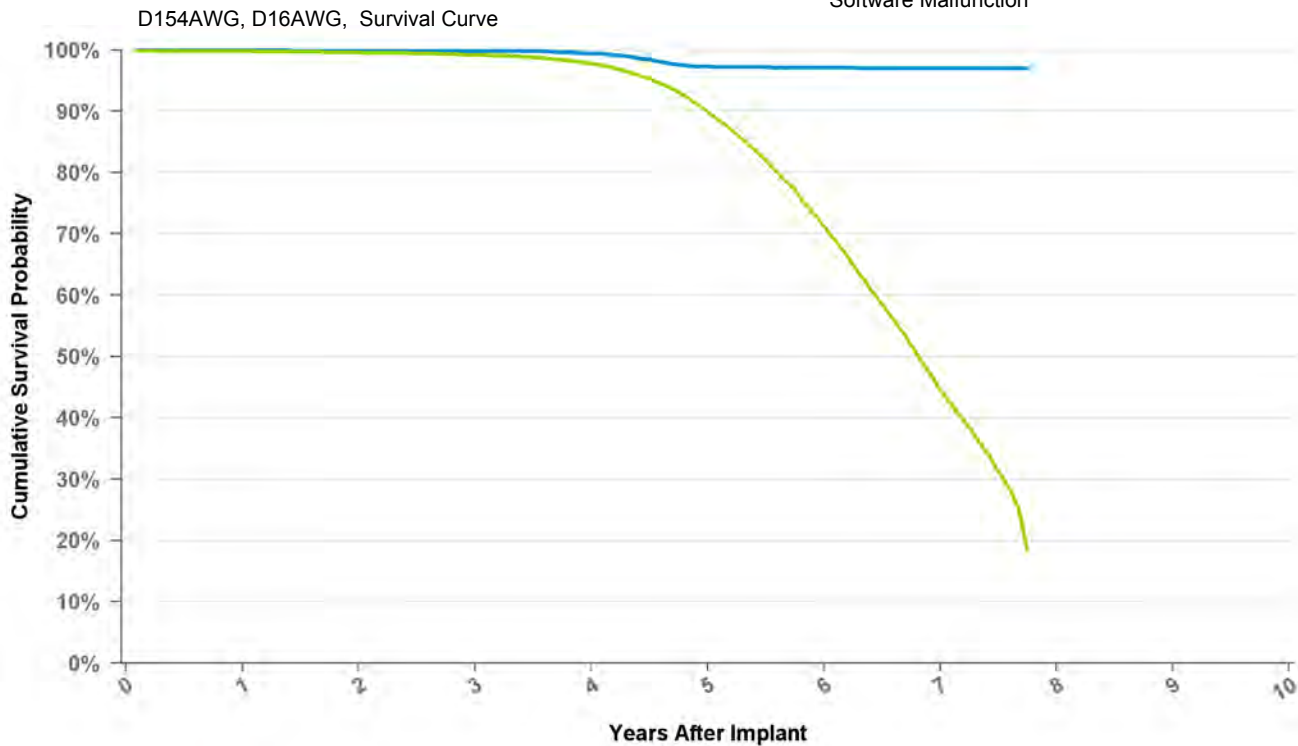

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 93 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.4% | 97.3% | 97.1% | 97.0% | 97.0% |
| Including NBD | 99.8% | 99.6% | 99.2% | 97.8% | 89.9% | 71.3% | 44.5% | 18.4% |
| Effective Sample Size | 67681 | 62397 | 57205 | 52252 | 44517 | 28257 | 9577 | 335 |

Implantable Cardioverter Defibrillator

D154DRG Entrust DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 06/14/2005 |
| CE Market Approval Date | 02/04/2005 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

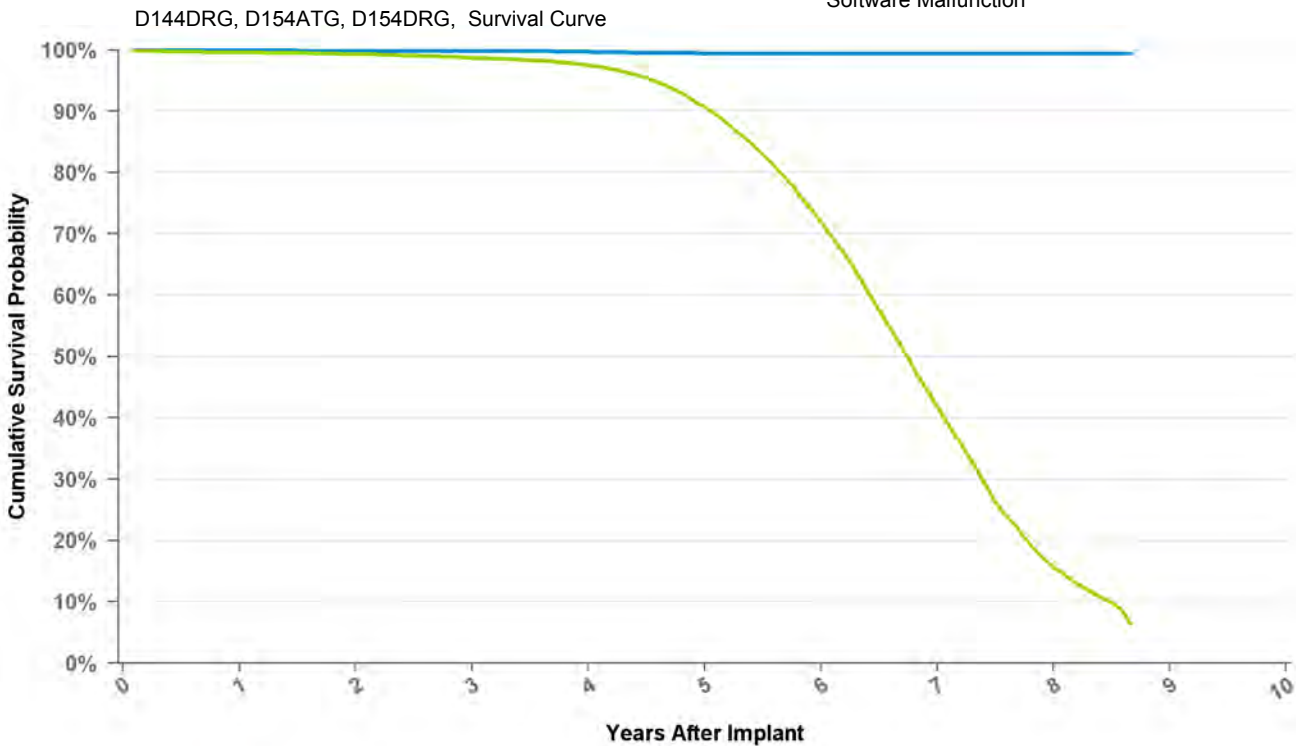

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 104 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 99.9% | 99.8% | 99.7% | 99.4% | 99.4% | 99.4% | 99.4% | 99.4% |
| Including NBD | 99.6% | 99.3% | 98.7% | 97.5% | 90.7% | 72.0% | 41.8% | 15.6% | 6.4% |
| Effective Sample Size | 26272 | 24061 | 21693 | 19252 | 16148 | 11945 | 6073 | 1727 | 107 |

Implantable Cardioverter Defibrillator

D154VRC Entrust VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 06/30/2005 |
| CE Market Approval Date | 02/04/2005 |
| Registered US Implants | 14,468 |
| Estimated Active US Implants | 5,673 |
| Normal Battery Depletions (US) | 1,326 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|-----|
| Total Malfunctions (US) | 109 |
| Therapy Not Compromised Malfunctions | 88 |
| Battery Malfunction | 10 |
| Electrical Component | 44 |
| Electrical Interconnect | 0 |
| Other Malfunction | 10 |
| Poss Early Battery Depltn | 24 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 21 |
| Battery Malfunction | 1 |
| Electrical Component | 19 |
| Electrical Interconnect | 0 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

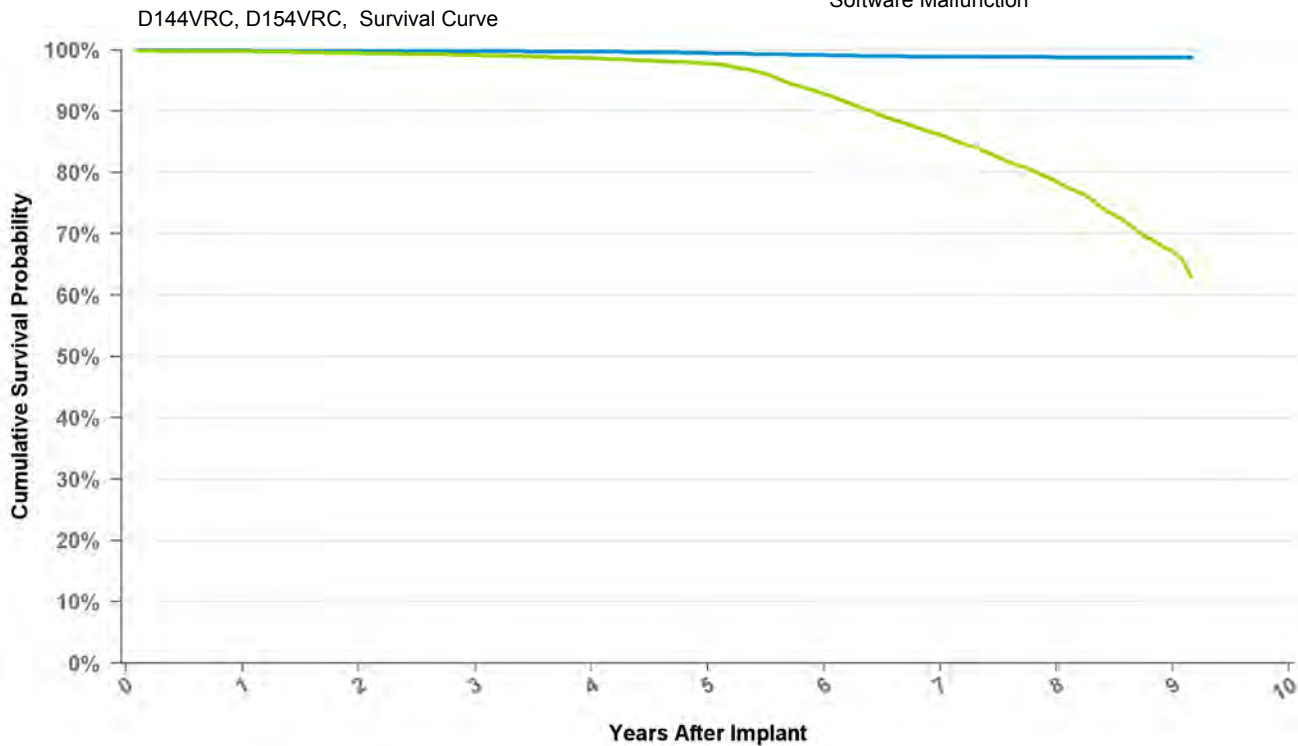

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 110 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 99.9% | 99.8% | 99.7% | 99.5% | 99.2% | 98.9% | 98.8% | 98.8% | 98.8% |
| Including NBD | 99.8% | 99.5% | 99.2% | 98.7% | 97.8% | 92.8% | 86.2% | 78.5% | 67.1% | 62.9% |
| Effective Sample Size | 13630 | 12418 | 11171 | 9950 | 8872 | 7862 | 6558 | 4915 | 777 | 270 |

Implantable Cardioverter Defibrillator

D154VWC Virtuoso VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 05/12/2006 |
| CE Market Approval Date | |
| Registered US Implants | 33,137 |
| Estimated Active US Implants | 16,372 |
| Normal Battery Depletions (US) | 2,478 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|-----|
| Total Malfunctions (US) | 662 |
| Therapy Not Compromised Malfunctions | 646 |
| Battery Malfunction | 1 |
| Electrical Component | 625 |
| Electrical Interconnect | 1 |
| Other Malfunction | 4 |
| Poss Early Battery Depltn | 15 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 16 |
| Battery Malfunction | 1 |
| Electrical Component | 15 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

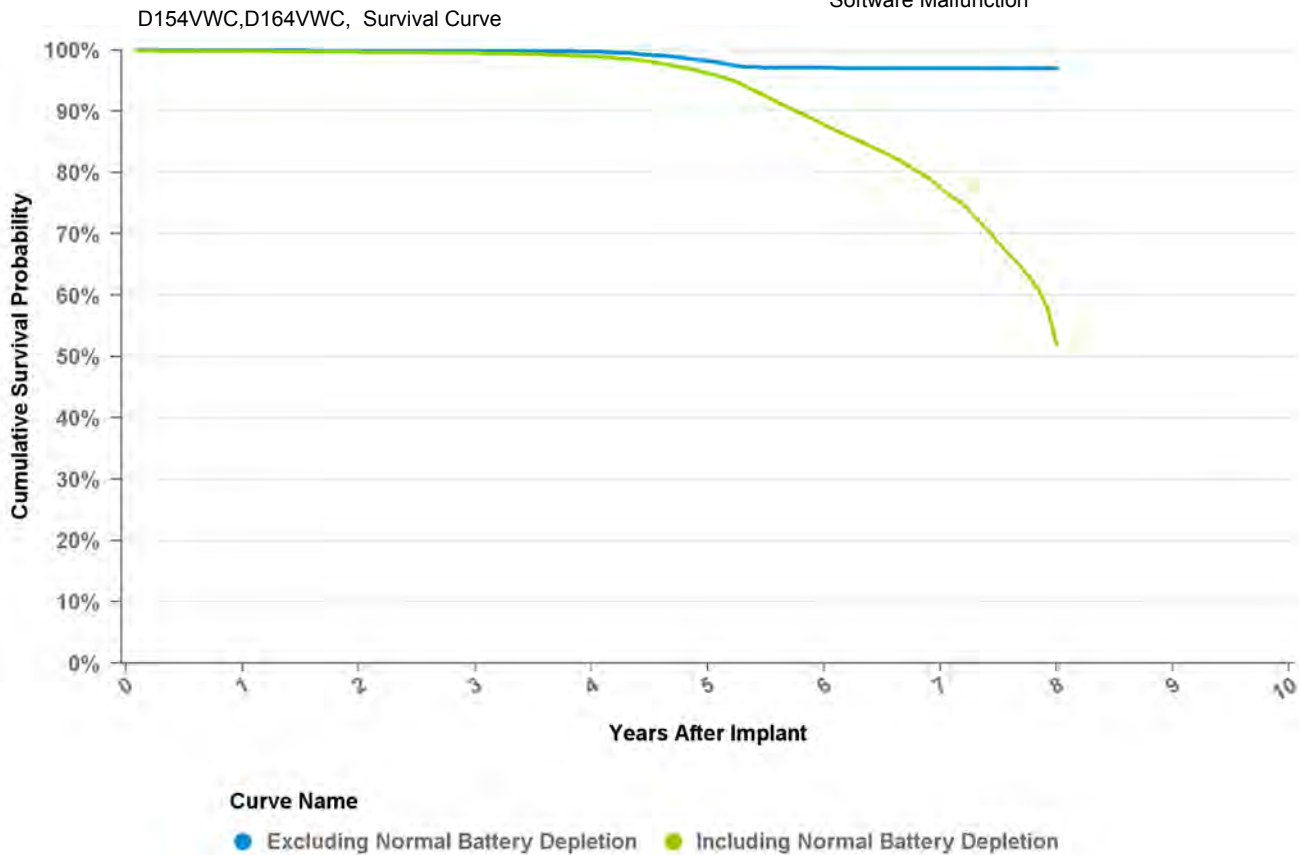


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 96 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.7% | 98.2% | 97.1% | 97.0% | 97.0% |
| Including NBD | 99.8% | 99.7% | 99.5% | 99.0% | 96.2% | 87.8% | 77.5% | 52.0% |
| Effective Sample Size | 30825 | 28284 | 25951 | 23840 | 21343 | 15843 | 7839 | 190 |

Implantable Cardioverter Defibrillator

D164AWG Virtuoso DR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 03/07/2006 |
| Registered US Implants | 10 |
| Estimated Active US Implants | 6 |
| Normal Battery Depletions (US) | 1 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

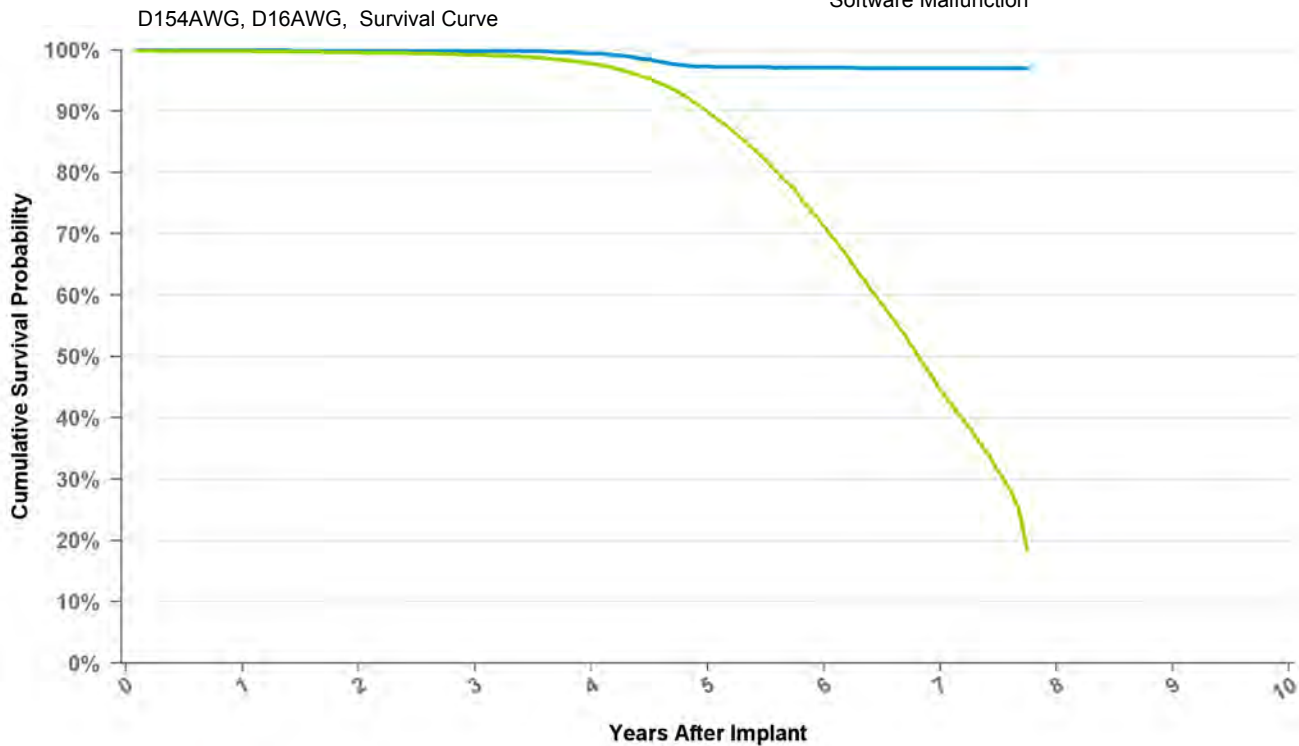

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 93 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.4% | 97.3% | 97.1% | 97.0% | 97.0% |
| Including NBD | 99.8% | 99.6% | 99.2% | 97.8% | 89.9% | 71.3% | 44.5% | 18.4% |
| Effective Sample Size | 67681 | 62397 | 57205 | 52252 | 44517 | 28257 | 9577 | 335 |

Implantable Cardioverter Defibrillator

D164VWC Virtuoso VR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 03/07/2006 |
| Registered US Implants | 6 |
| Estimated Active US Implants | 4 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 1 |
| Therapy Not Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

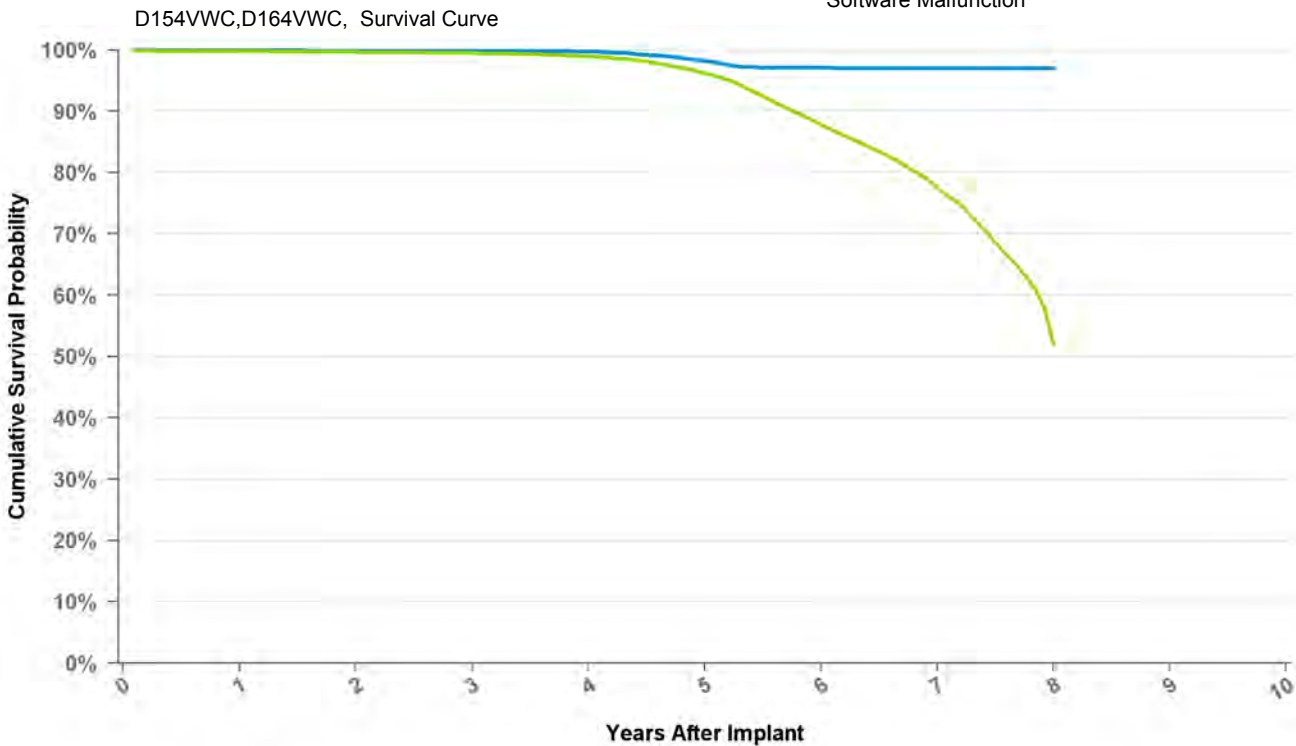

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 96 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.7% | 98.2% | 97.1% | 97.0% | 97.0% |
| Including NBD | 99.8% | 99.7% | 99.5% | 99.0% | 96.2% | 87.8% | 77.5% | 52.0% |
| Effective Sample Size | 30825 | 28284 | 25951 | 23840 | 21343 | 15843 | 7839 | 190 |

Implantable Cardioverter Defibrillator

D204DRM Secura DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/09/2012 |
| CE Market Approval Date | |
| Registered US Implants | 1,874 |
| Estimated Active US Implants | 1,746 |
| Normal Battery Depletions (US) | 1 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 3 |
| Therapy Not Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 2 |
| Battery Malfunction | 0 |
| Electrical Component | 2 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

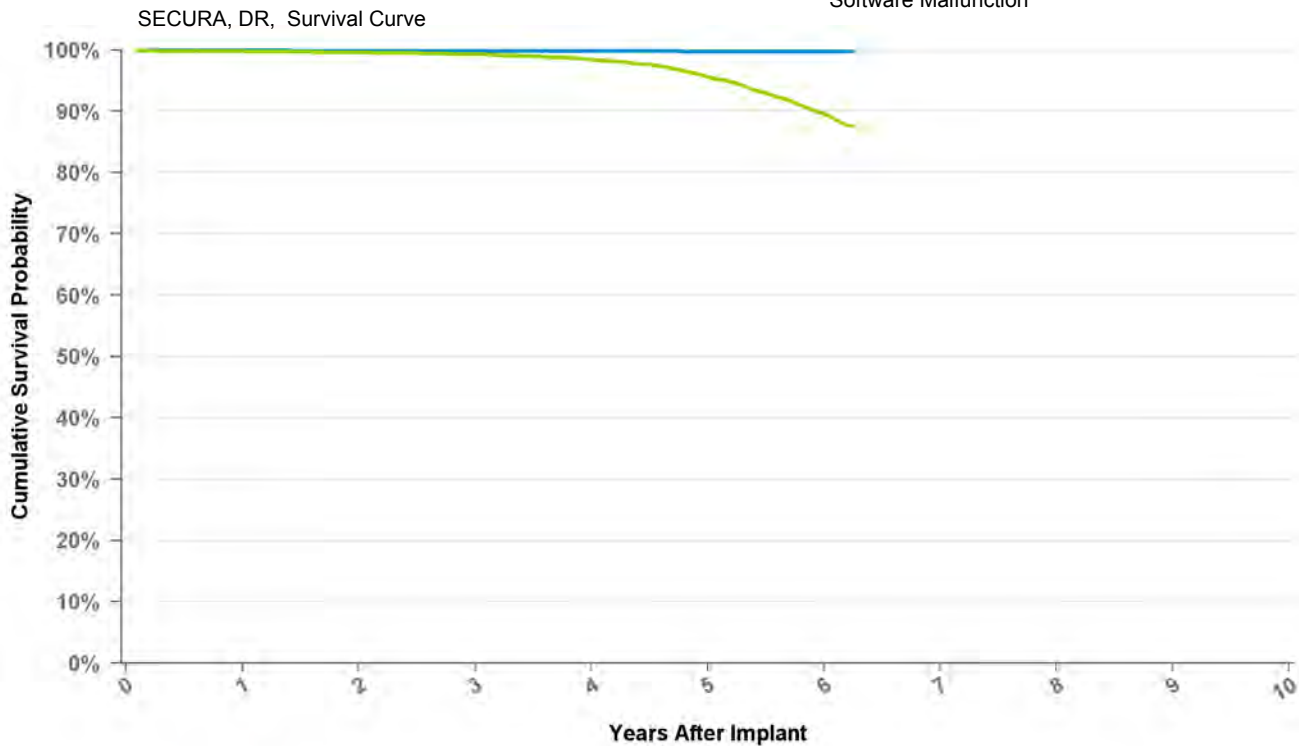

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 75 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.8% | 99.7% | 99.7% | 99.7% |
| Including NBD | 99.8% | 99.6% | 99.3% | 98.4% | 95.6% | 89.6% | 87.5% |
| Effective Sample Size | 49158 | 44354 | 38602 | 29019 | 12966 | 1990 | 436 |

Implantable Cardioverter Defibrillator

D204VRM Secura VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 05/02/2012 |
| CE Market Approval Date | |
| Registered US Implants | 1,172 |
| Estimated Active US Implants | 1,108 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

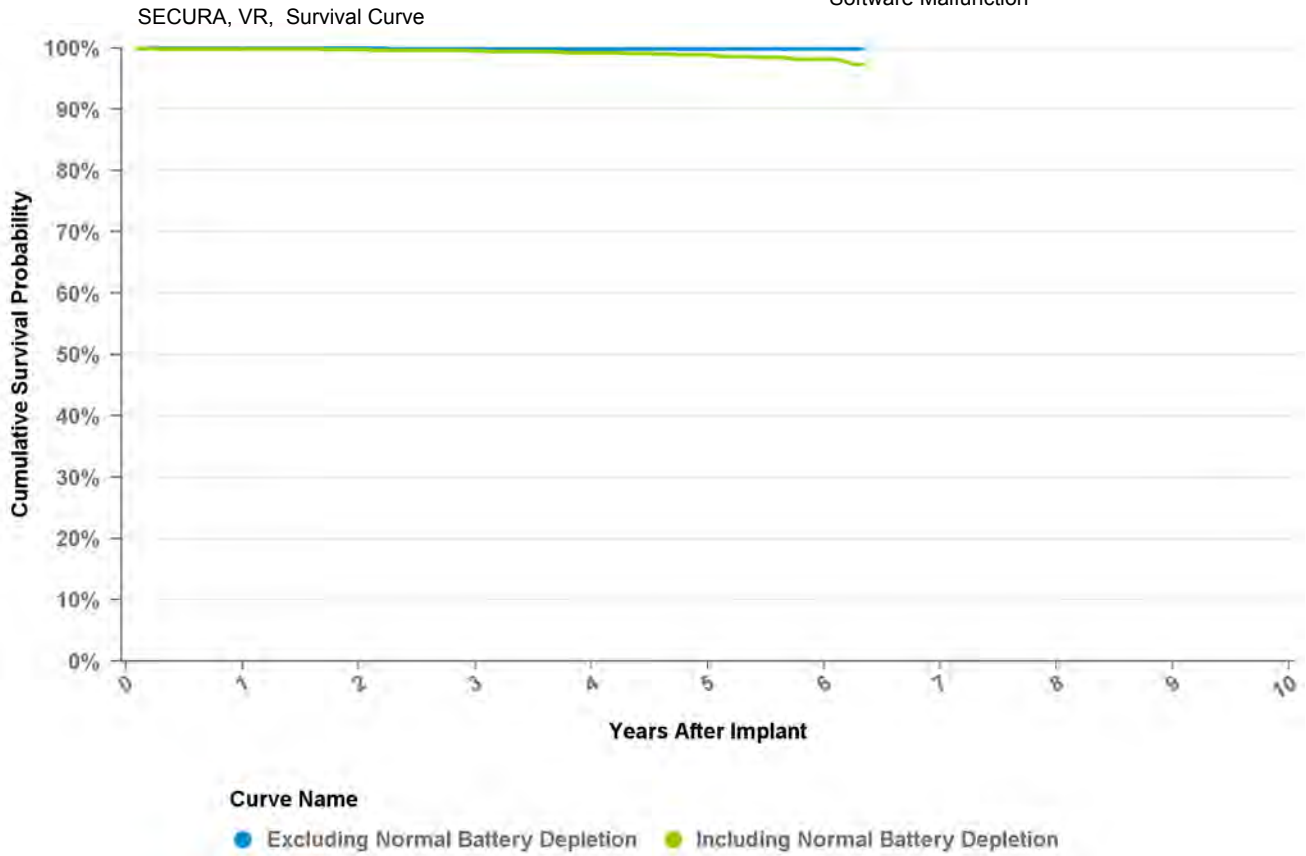


| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 76 mo |
|------------------------------|--------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.8% | 99.8% |
| Including NBD | 99.9% | 99.7% | 99.5% | 99.2% | 98.9% | 98.2% | 97.3% |
| Effective Sample Size | 20469 | 18017 | 15262 | 11344 | 5633 | 1104 | 156 |

Implantable Cardioverter Defibrillator

D214DRM Secura DR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 07/22/2010 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

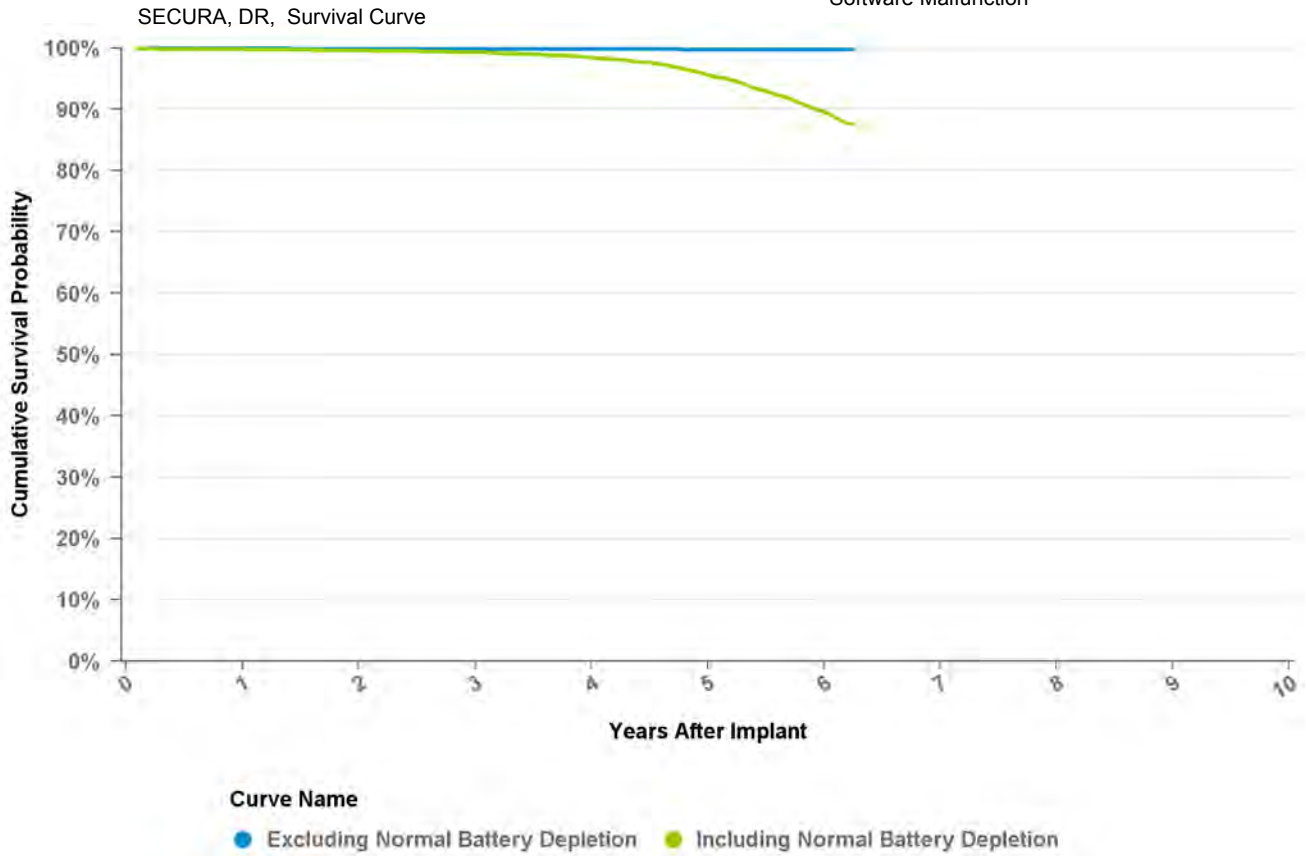


| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 75 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.8% | 99.7% | 99.7% | 99.7% |
| Including NBD | 99.8% | 99.6% | 99.3% | 98.4% | 95.6% | 89.6% | 87.5% |
| Effective Sample Size | 49158 | 44354 | 38602 | 29019 | 12966 | 1990 | 436 |

Implantable Cardioverter Defibrillator

D214VRM Secura VR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 12/17/2010 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

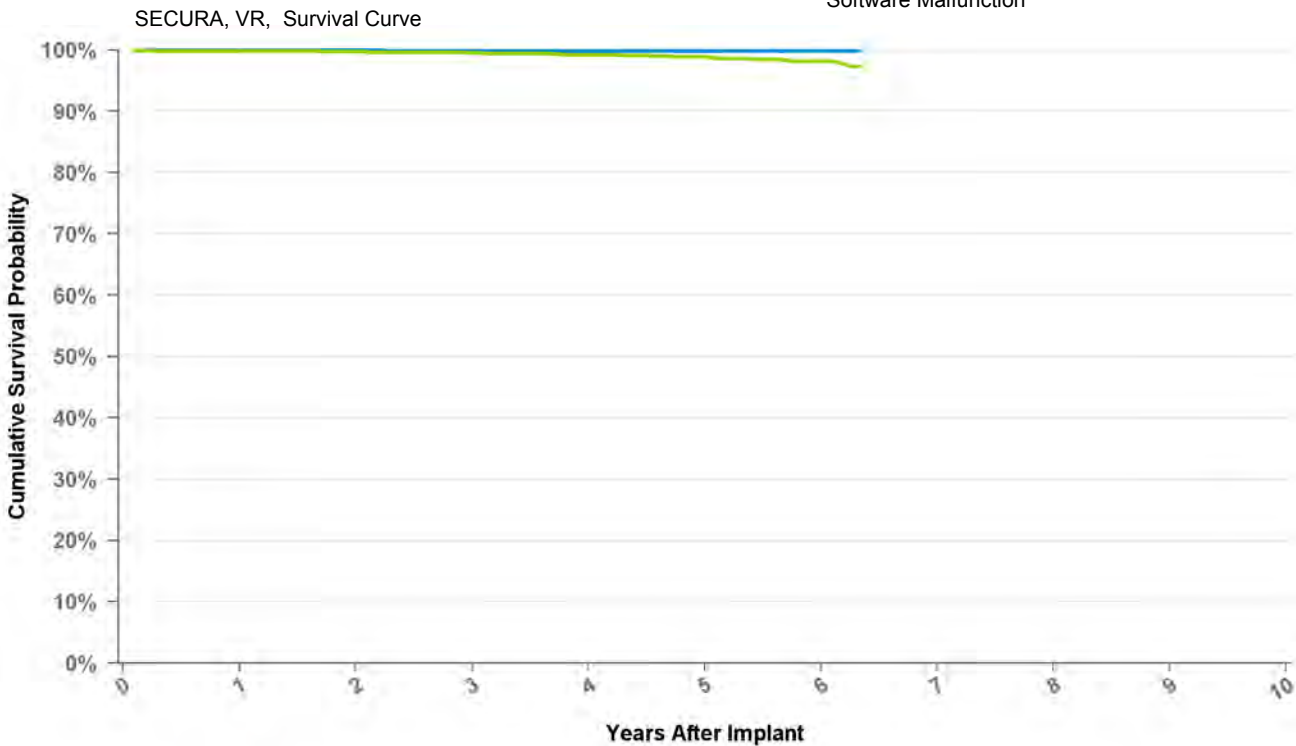

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 76 mo |
|------------------------------|--------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.8% | 99.8% |
| Including NBD | 99.9% | 99.7% | 99.5% | 99.2% | 98.9% | 98.2% | 97.3% |
| Effective Sample Size | 20469 | 18017 | 15262 | 11344 | 5633 | 1104 | 156 |

Implantable Cardioverter Defibrillator

D224DRG Secura DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 09/15/2008 |
| CE Market Approval Date | |
| Registered US Implants | 49,845 |
| Estimated Active US Implants | 37,187 |
| Normal Battery Depletions (US) | 903 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|----|
| Total Malfunctions (US) | 93 |
| Therapy Not Compromised Malfunctions | 78 |
| Battery Malfunction | 0 |
| Electrical Component | 22 |
| Electrical Interconnect | 0 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 46 |
| Software Malfunction | 9 |
| Therapy Compromised Malfunctions | 15 |
| Battery Malfunction | 1 |
| Electrical Component | 12 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 1 |

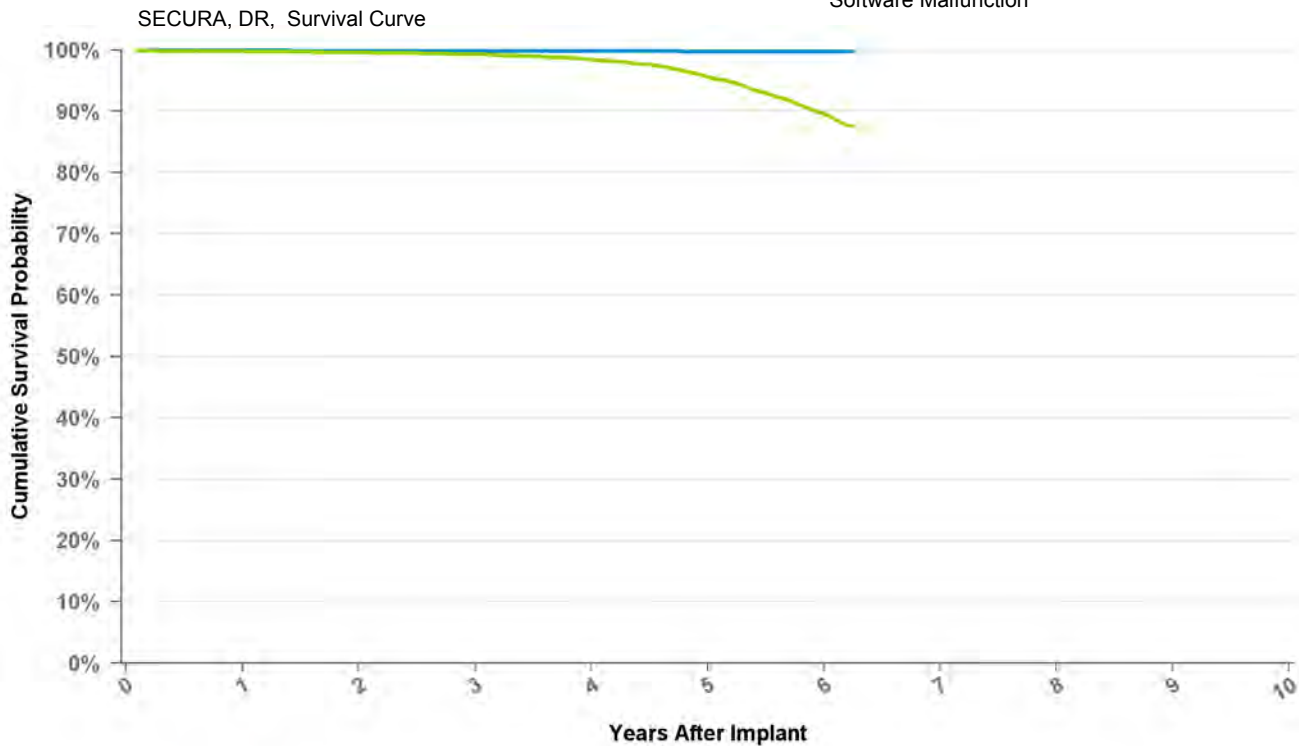

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 75 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.8% | 99.7% | 99.7% | 99.7% |
| Including NBD | 99.8% | 99.6% | 99.3% | 98.4% | 95.6% | 89.6% | 87.5% |
| Effective Sample Size | 49158 | 44354 | 38602 | 29019 | 12966 | 1990 | 436 |

Implantable Cardioverter Defibrillator

D224VRC Secura VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 09/15/2008 |
| CE Market Approval Date | |
| Registered US Implants | 19,942 |
| Estimated Active US Implants | 15,474 |
| Normal Battery Depletions (US) | 85 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|----|
| Total Malfunctions (US) | 24 |
| Therapy Not Compromised Malfunctions | 18 |
| Battery Malfunction | 4 |
| Electrical Component | 5 |
| Electrical Interconnect | 0 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 6 |
| Software Malfunction | 2 |
| Therapy Compromised Malfunctions | 6 |
| Battery Malfunction | 0 |
| Electrical Component | 5 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 1 |

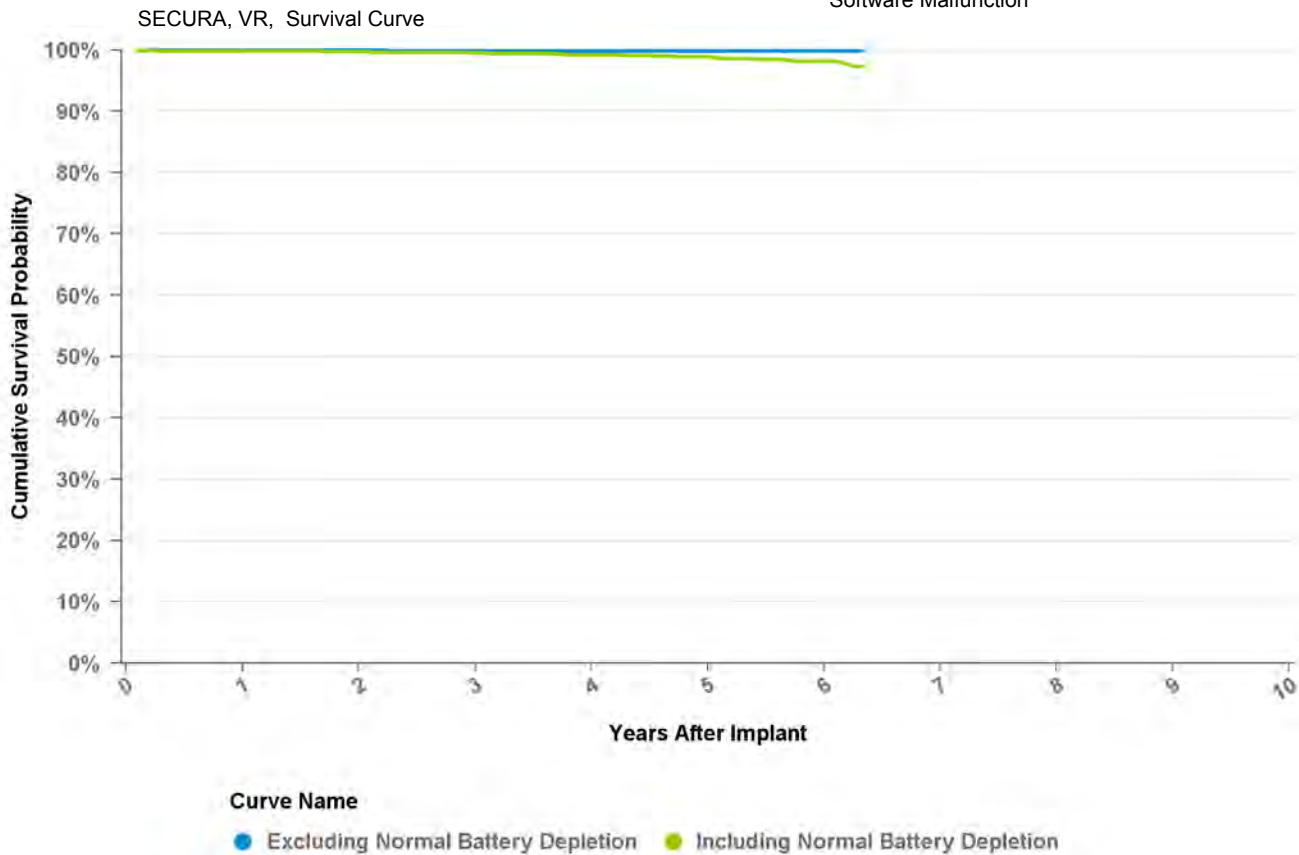


| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 76 mo |
|------------------------------|--------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.8% | 99.8% |
| Including NBD | 99.9% | 99.7% | 99.5% | 99.2% | 98.9% | 98.2% | 97.3% |
| Effective Sample Size | 20469 | 18017 | 15262 | 11344 | 5633 | 1104 | 156 |

Implantable Cardioverter Defibrillator

D234DRG Secura DR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 03/14/2008 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

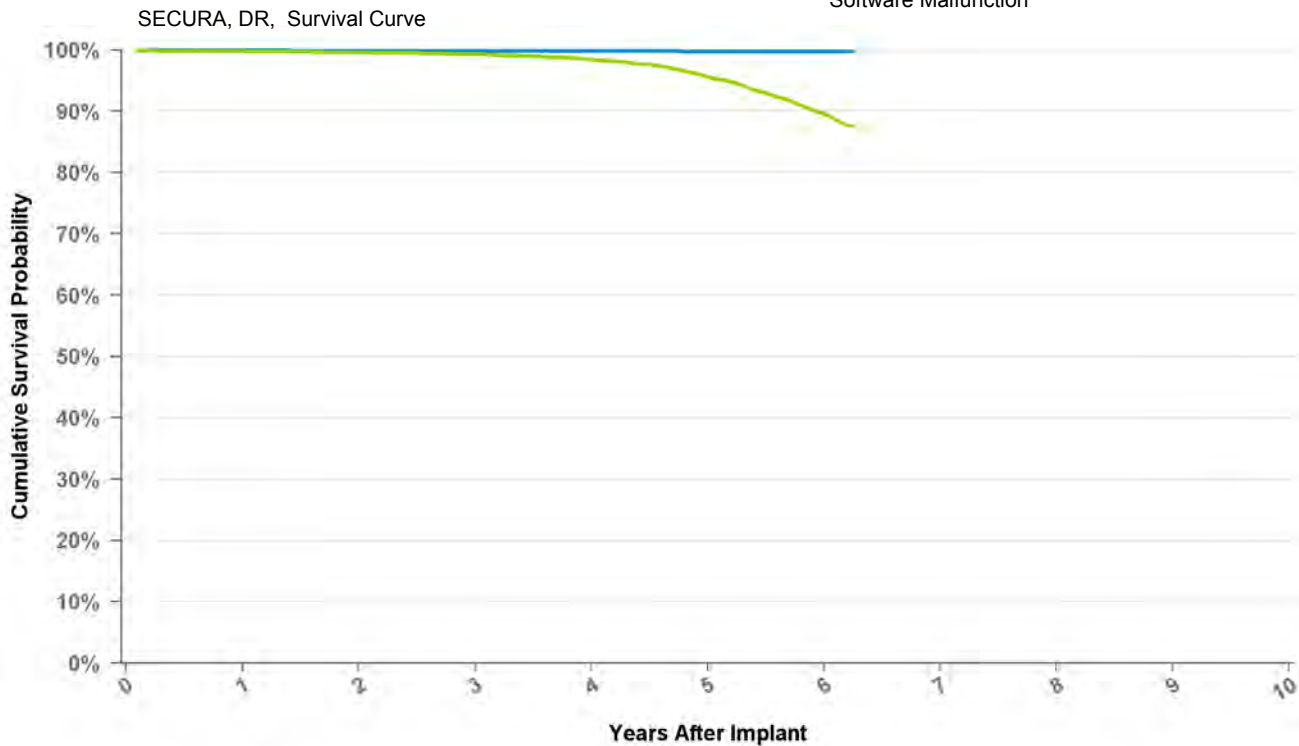

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 75 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 99.9% | 99.9% | 99.8% | 99.7% | 99.7% | 99.7% |
| Including NBD | 99.8% | 99.6% | 99.3% | 98.4% | 95.6% | 89.6% | 87.5% |
| Effective Sample Size | 49158 | 44354 | 38602 | 29019 | 12966 | 1990 | 436 |

Implantable Cardioverter Defibrillator

D234VRC Secura VR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 03/14/2008 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

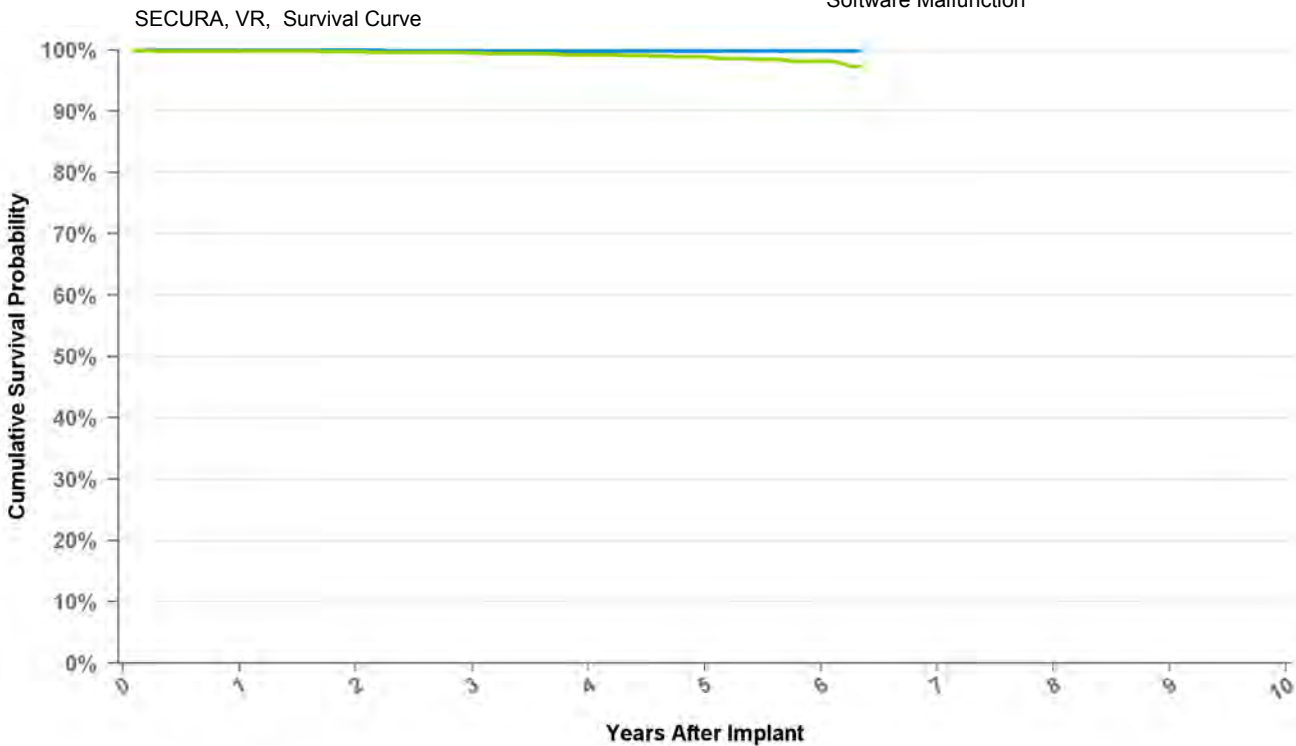

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 76 mo |
|------------------------------|--------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.8% | 99.8% |
| Including NBD | 99.9% | 99.7% | 99.5% | 99.2% | 98.9% | 98.2% | 97.3% |
| Effective Sample Size | 20469 | 18017 | 15262 | 11344 | 5633 | 1104 | 156 |

Implantable Cardioverter Defibrillator

D264DRM Maximo II DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/09/2012 |
| CE Market Approval Date | 07/22/2010 |
| Registered US Implants | 6 |
| Estimated Active US Implants | 6 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

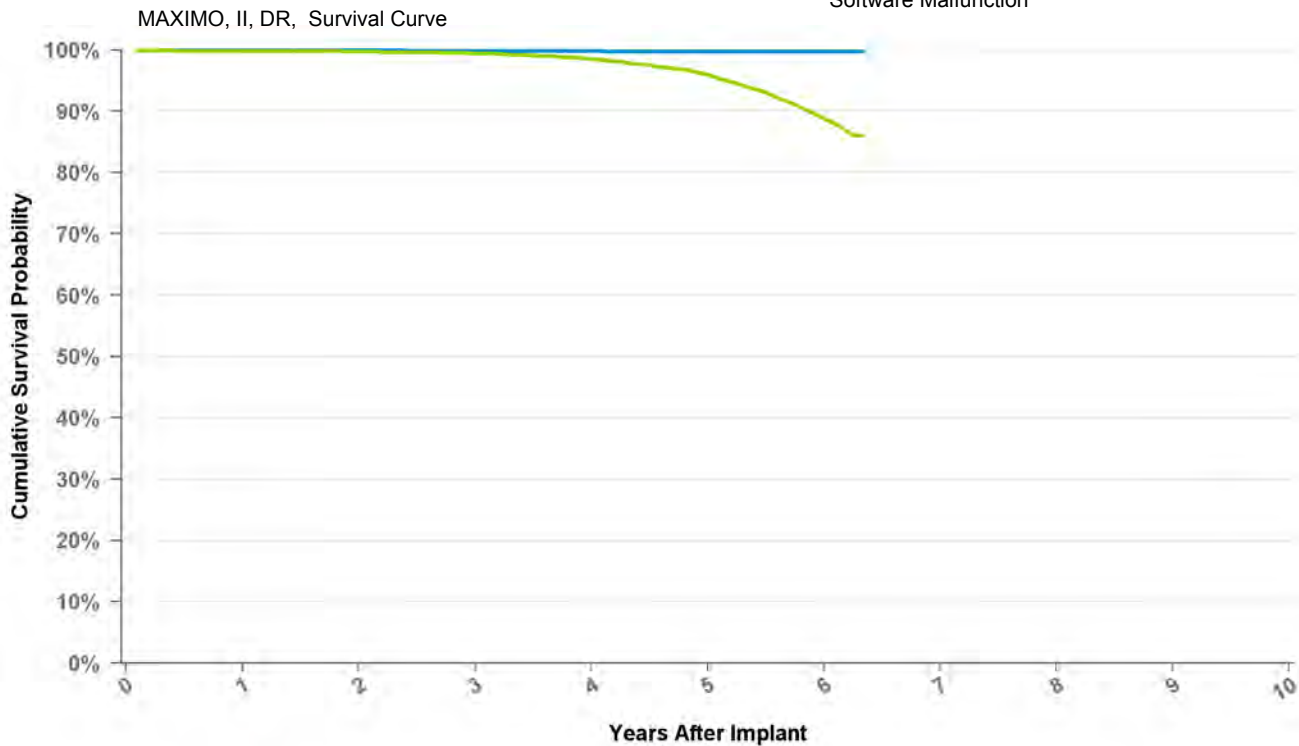

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 76 mo |
|------------------------------|--------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.8% | 99.7% | 99.7% | 99.7% |
| Including NBD | 99.9% | 99.7% | 99.4% | 98.5% | 96.0% | 88.7% | 86.0% |
| Effective Sample Size | 19345 | 17344 | 14860 | 11089 | 5963 | 1199 | 104 |

Implantable Cardioverter Defibrillator

D264VRM Maximo II VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 05/02/2012 |
| CE Market Approval Date | 12/17/2010 |
| Registered US Implants | 1 |
| Estimated Active US Implants | 1 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

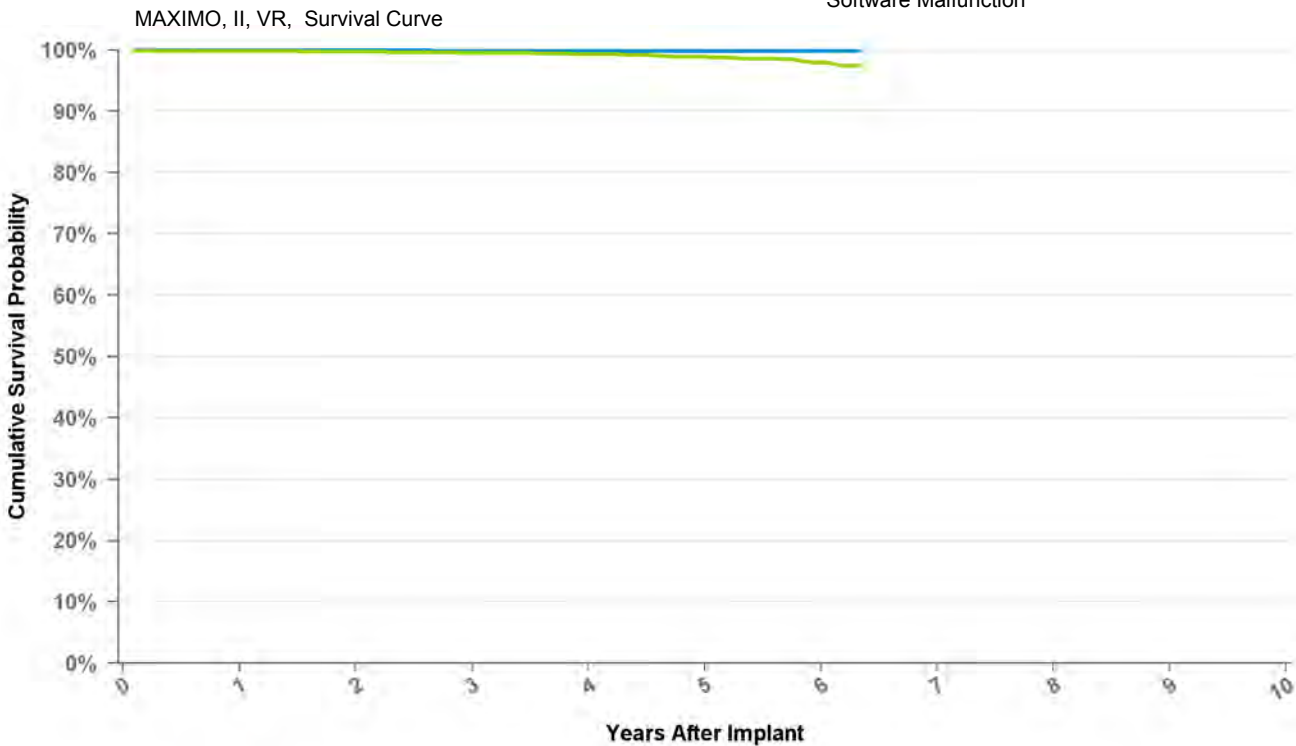

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 76 mo |
|------------------------------|--------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.8% | 99.7% | 99.5% | 99.3% | 98.9% | 98.0% | 97.4% |
| Effective Sample Size | 13177 | 11853 | 9981 | 7319 | 3965 | 793 | 108 |

Implantable Cardioverter Defibrillator

D274DRG Virtuoso II DR

US Market Release Date 08/15/2009

CE Market Approval Date

Registered US Implants 22,220

Estimated Active US Implants 17,206

Normal Battery Depletions (US) 202

NBG Code DDE-DDDR

Max Delivered Energy 35 J

Total Malfunctions (US) 16

Therapy Not Compromised Malfunctions 13

Battery Malfunction 3

Electrical Component 3

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 6

Software Malfunction 1

Therapy Compromised Malfunctions 3

Battery Malfunction 0


Electrical Component 2

Electrical Interconnect 0

Other Malfunction 1

Poss Early Battery Depltn 0

Software Malfunction 0

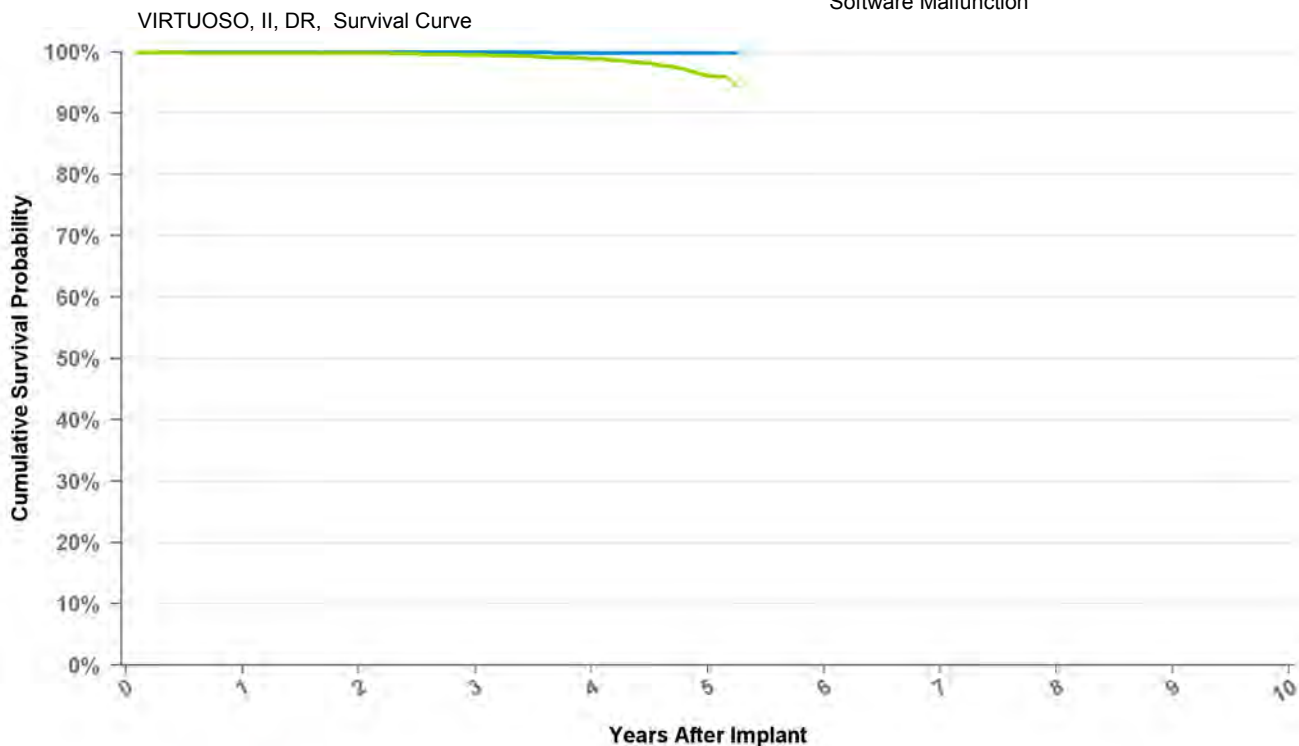

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | at 63 mo |
|------------------------------|--------|--------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.8% | 99.5% | 98.9% | 96.1% | 94.3% |
| Effective Sample Size | 20630 | 19226 | 17718 | 12087 | 2215 | 334 |

Implantable Cardioverter Defibrillator

D274VRC Virtuoso II VR

US Market Release Date 08/15/2009

CE Market Approval Date

Registered US Implants 9,113

Estimated Active US Implants 7,312

Normal Battery Depletions (US) 23

NBG Code VVE-VVIR

Max Delivered Energy 35 J

Total Malfunctions (US) 6

Therapy Not Compromised Malfunctions 6

Battery Malfunction 1

Electrical Component 2

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 2

Software Malfunction 1

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

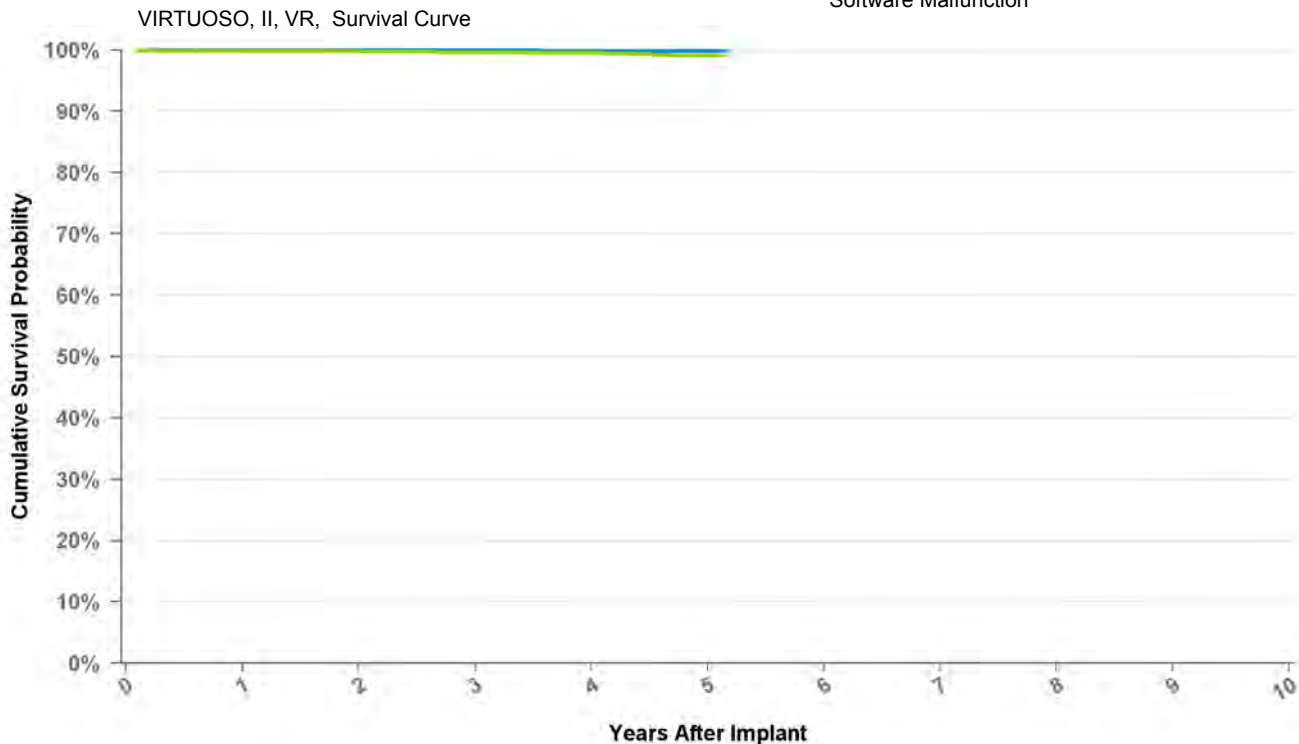

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | at 62 mo |
|------------------------------|--------|--------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.8% | 99.8% | 99.6% | 99.5% | 99.1% | 99.1% |
| Effective Sample Size | 8581 | 8008 | 7330 | 4810 | 796 | 263 |

Implantable Cardioverter Defibrillator

D284DRG Maximo II DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 09/17/2008 |
| CE Market Approval Date | 03/14/2008 |
| Registered US Implants | 20,045 |
| Estimated Active US Implants | 14,936 |
| Normal Battery Depletions (US) | 415 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|----|
| Total Malfunctions (US) | 42 |
| Therapy Not Compromised Malfunctions | 36 |
| Battery Malfunction | 0 |
| Electrical Component | 9 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 27 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 6 |
| Battery Malfunction | 0 |
| Electrical Component | 5 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |

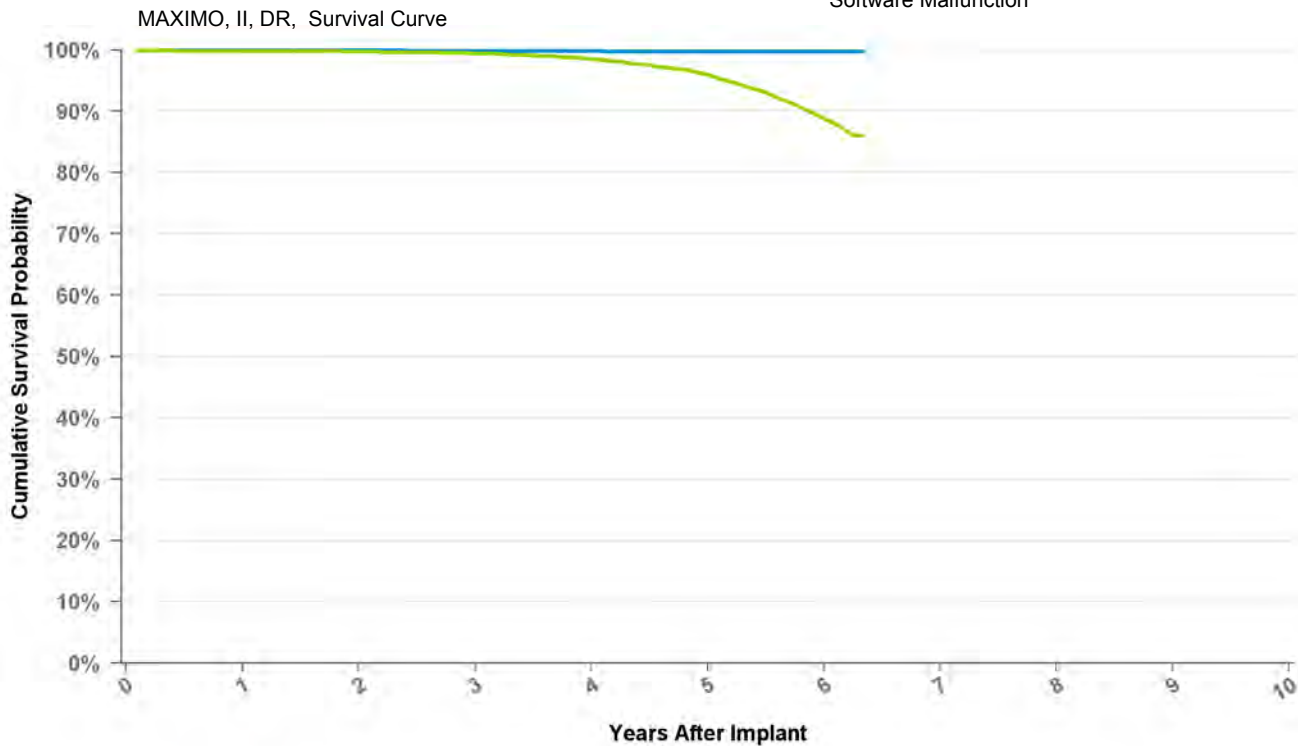

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 76 mo |
|------------------------------|--------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.8% | 99.7% | 99.7% | 99.7% |
| Including NBD | 99.9% | 99.7% | 99.4% | 98.5% | 96.0% | 88.7% | 86.0% |
| Effective Sample Size | 19345 | 17344 | 14860 | 11089 | 5963 | 1199 | 104 |

Implantable Cardioverter Defibrillator

D284VRC Maximo II VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 09/17/2008 |
| CE Market Approval Date | 03/14/2008 |
| Registered US Implants | 12,951 |
| Estimated Active US Implants | 10,210 |
| Normal Battery Depletions (US) | 61 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|----|
| Total Malfunctions (US) | 15 |
| Therapy Not Compromised Malfunctions | 11 |
| Battery Malfunction | 1 |
| Electrical Component | 4 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 3 |
| Software Malfunction | 3 |
| Therapy Compromised Malfunctions | 4 |
| Battery Malfunction | 1 |
| Electrical Component | 2 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 1 |

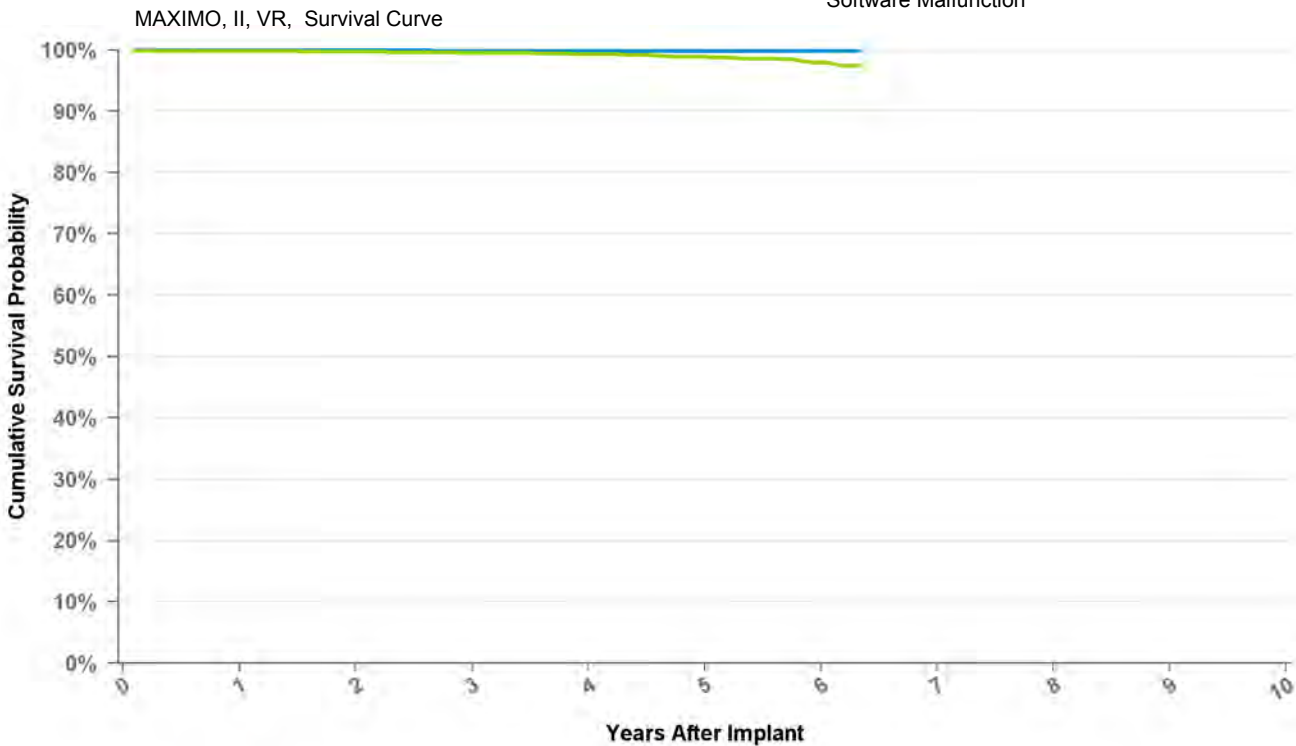

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 76 mo |
|------------------------------|--------|--------|-------|-------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.8% | 99.7% | 99.5% | 99.3% | 98.9% | 98.0% | 97.4% |
| Effective Sample Size | 13177 | 11853 | 9981 | 7319 | 3965 | 793 | 108 |

Implantable Cardioverter Defibrillator

D294DRG Virtuoso II DR

US Market Release Date

CE Market Approval Date 08/20/2008

Registered US Implants 1

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code DDE-DDDR

Max Delivered Energy 35 J

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

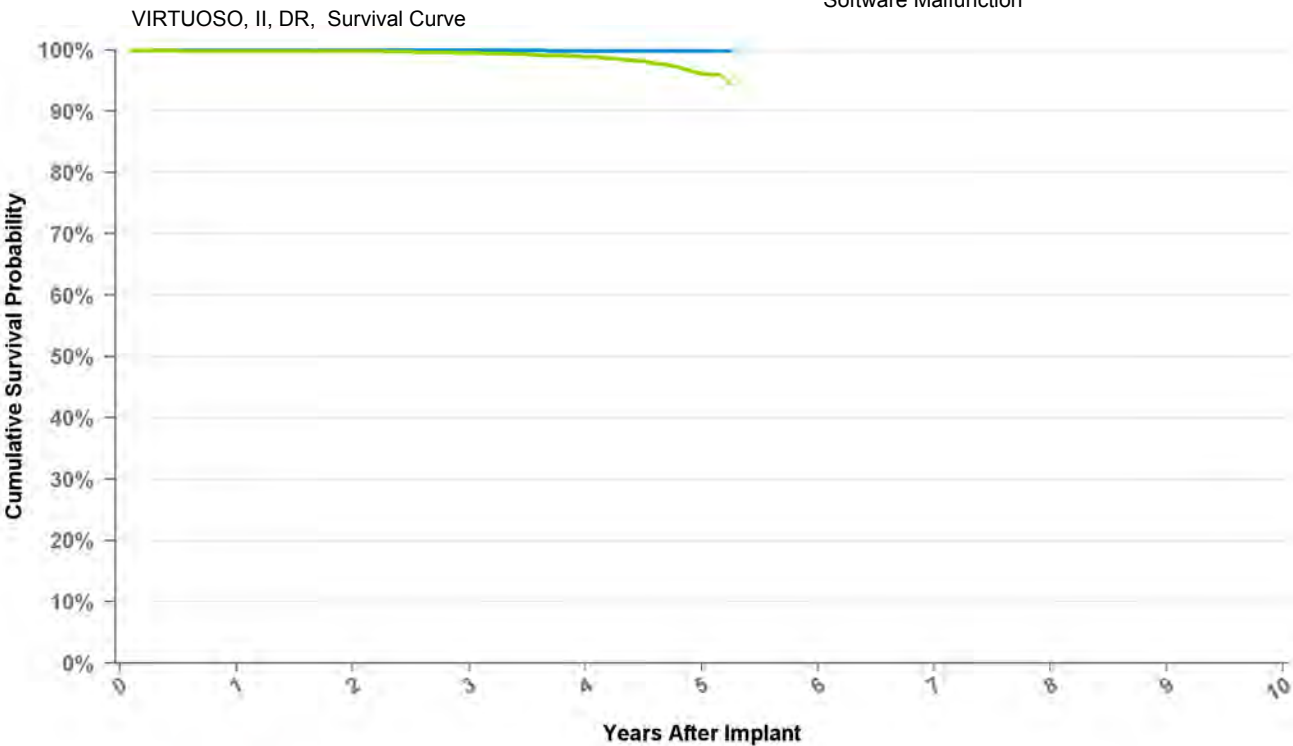

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | at 63 mo |
|------------------------------|--------|--------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.8% | 99.5% | 98.9% | 96.1% | 94.3% |
| Effective Sample Size | 20630 | 19226 | 17718 | 12087 | 2215 | 334 |

Implantable Cardioverter Defibrillator

D294VRC Virtuoso II VR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 08/20/2008 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

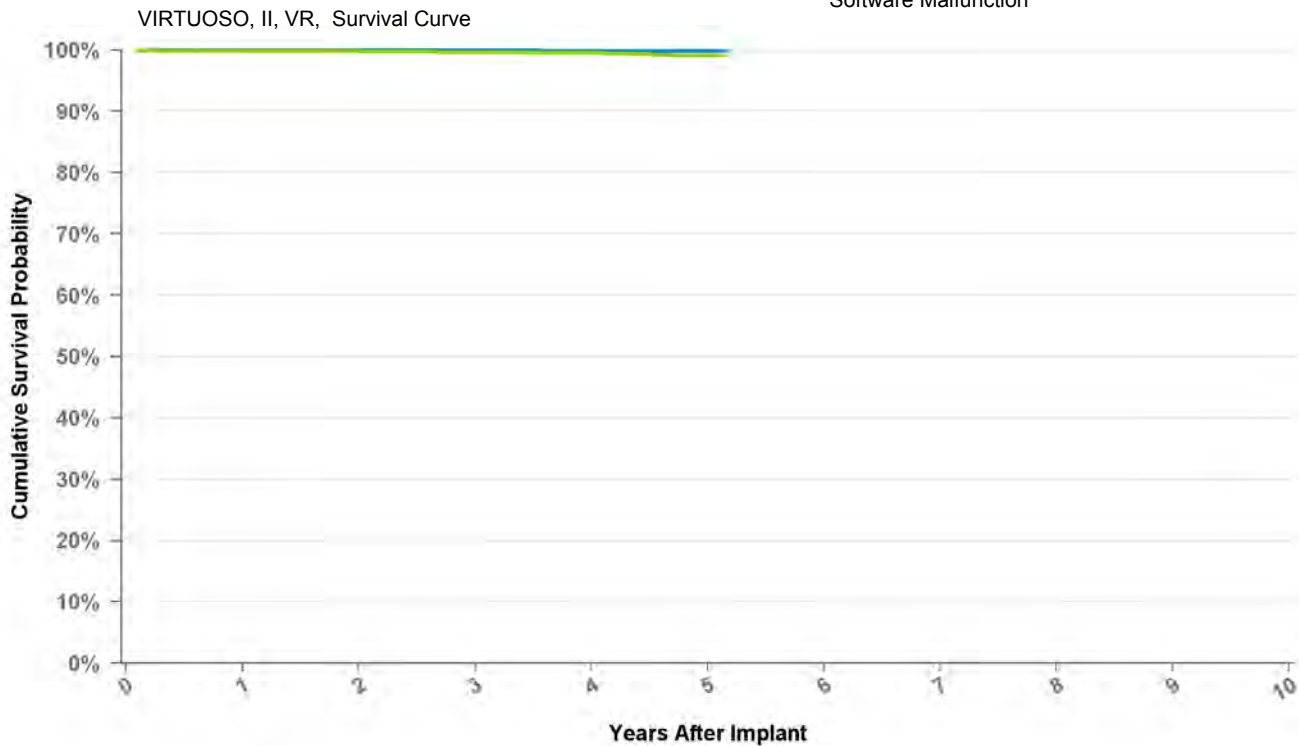

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | at 62 mo |
|------------------------------|--------|--------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.8% | 99.8% | 99.6% | 99.5% | 99.1% | 99.1% |
| Effective Sample Size | 8581 | 8008 | 7330 | 4810 | 796 | 263 |

Implantable Cardioverter Defibrillator

D314DRG Protecta XT DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 03/25/2011 |
| CE Market Approval Date | |
| Registered US Implants | 34,312 |
| Estimated Active US Implants | 30,503 |
| Normal Battery Depletions (US) | 53 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|----|
| Total Malfunctions (US) | 18 |
| Therapy Not Compromised Malfunctions | 13 |
| Battery Malfunction | 1 |
| Electrical Component | 11 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 5 |
| Battery Malfunction | 0 |
| Electrical Component | 5 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

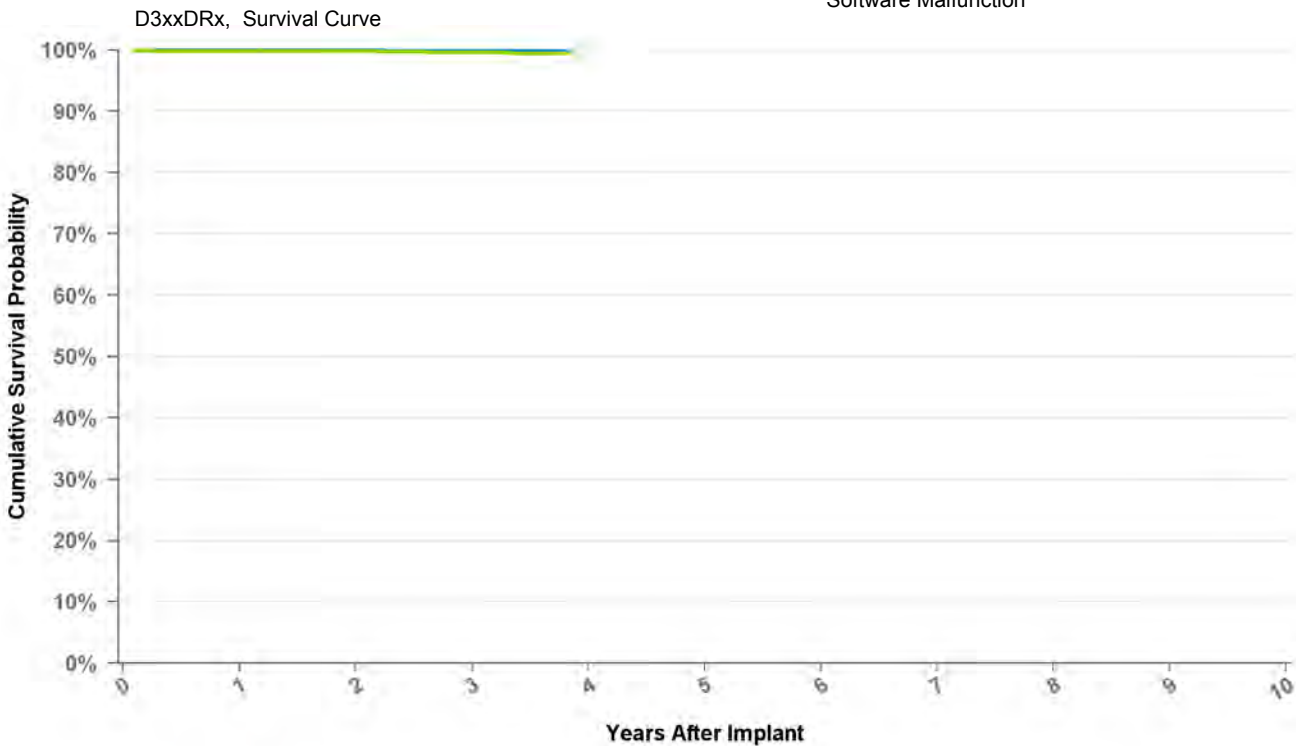

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.8% | 99.6% | 99.4% |
| Effective Sample Size | 57472 | 40632 | 13475 | 337 |

Implantable Cardioverter Defibrillator

D314DRM Protecta XT DR

US Market Release Date 11/09/2011

CE Market Approval Date

Registered US Implants 13,665

Estimated Active US Implants 12,669

Normal Battery Depletions (US) 9

NBG Code DDE-DDDR

Max Delivered Energy 35 J

Total Malfunctions (US) 4

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 3

Electrical Interconnect 0

Other Malfunction 1

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

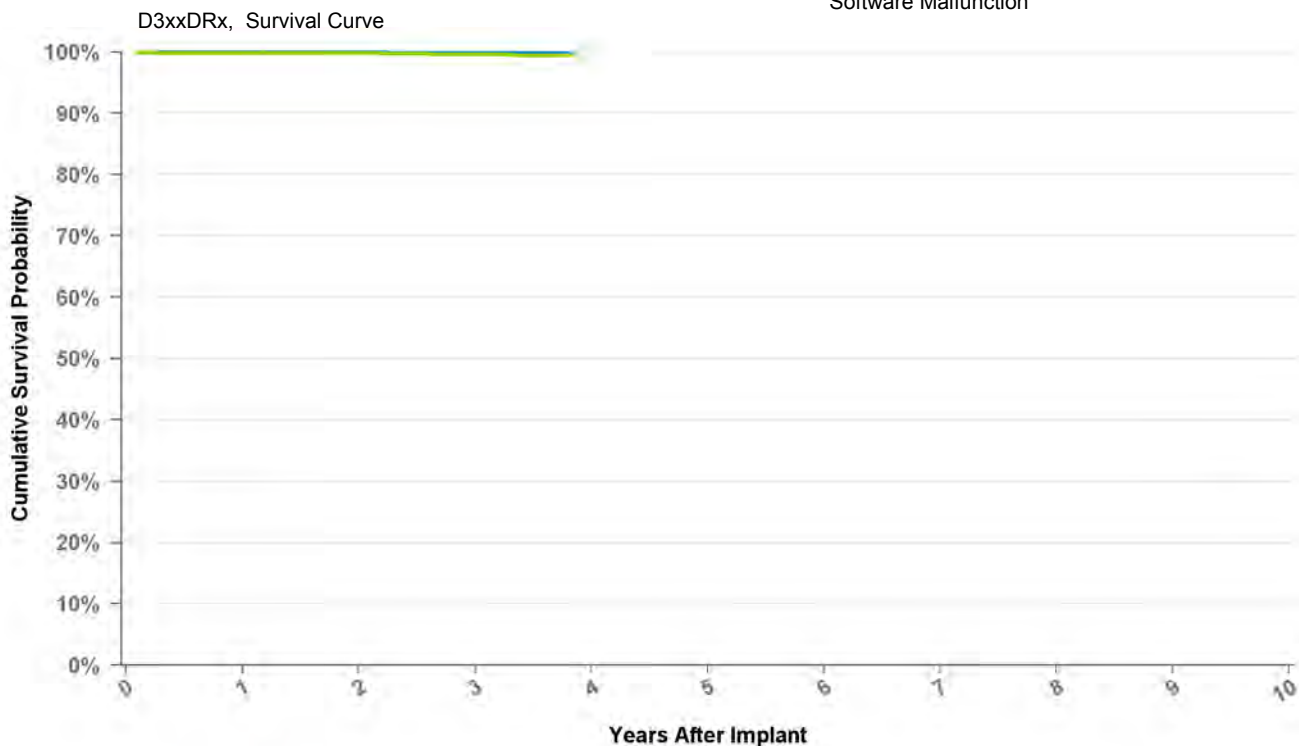

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.8% | 99.6% | 99.4% |
| Effective Sample Size | 57472 | 40632 | 13475 | 337 |

Implantable Cardioverter Defibrillator

D314VRG Protecta XT VR

US Market Release Date 03/25/2011

CE Market Approval Date

Registered US Implants 13,929

Estimated Active US Implants 12,514

Normal Battery Depletions (US) 15

NBG Code VVE-VVIR

Max Delivered Energy 35 J

Total Malfunctions (US) 6

Therapy Not Compromised Malfunctions 5

Battery Malfunction 0

Electrical Component 4

Electrical Interconnect 0

Other Malfunction 1

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 1

Battery Malfunction 0


Electrical Component 1

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

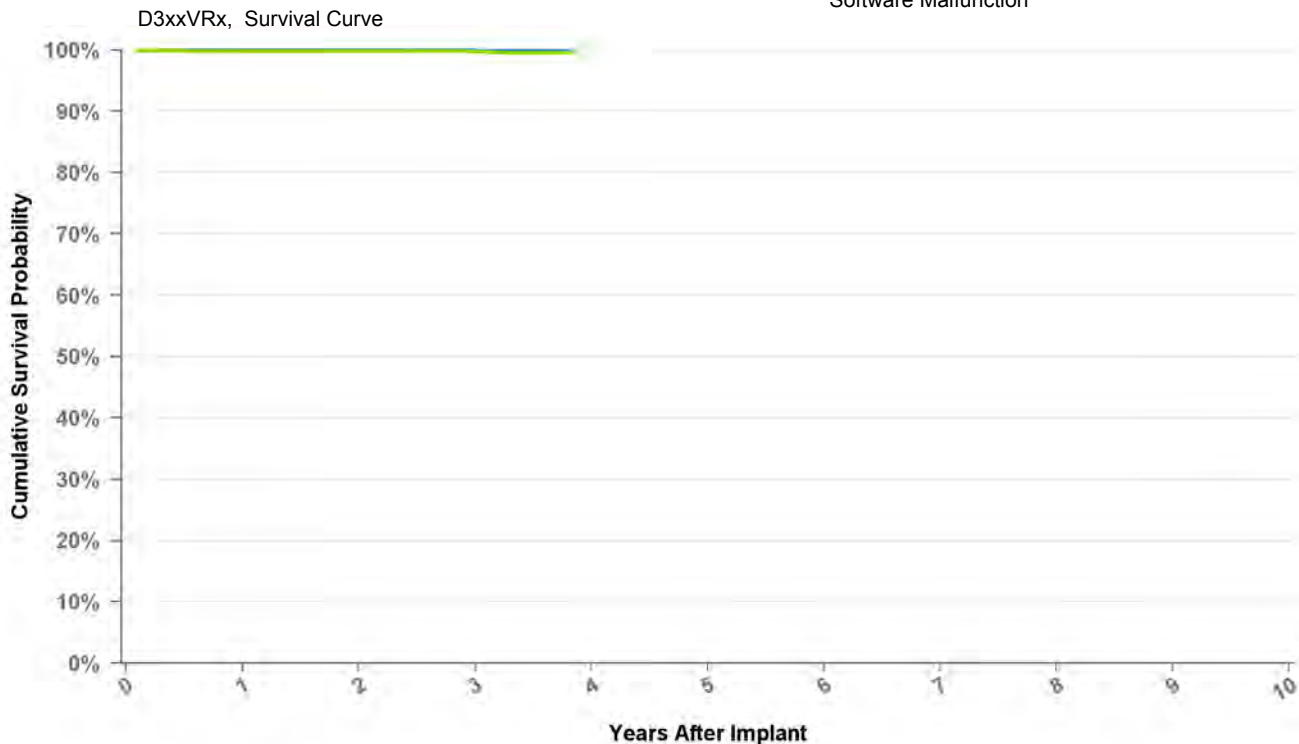

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.9% | 99.7% | 99.5% |
| Effective Sample Size | 27216 | 18397 | 5746 | 167 |

Implantable Cardioverter Defibrillator

D314VRM Protecta XT VR

US Market Release Date 05/02/2012

CE Market Approval Date

Registered US Implants 7,226

Estimated Active US Implants 6,721

Normal Battery Depletions (US) 2

NBG Code VVE-VVIR

Max Delivered Energy 35 J

Total Malfunctions (US) 1

Therapy Not Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 1

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

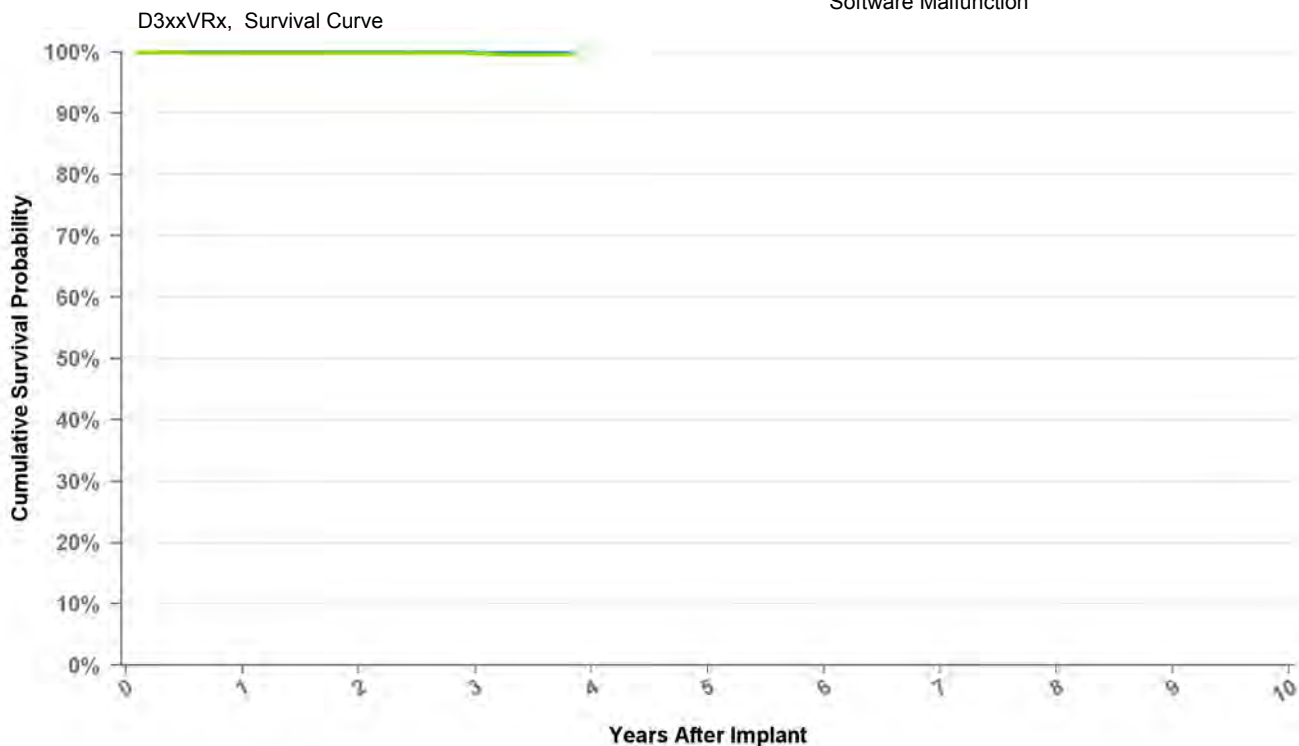

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.9% | 99.7% | 99.5% |
| Effective Sample Size | 27216 | 18397 | 5746 | 167 |

Implantable Cardioverter Defibrillator

D334DRG Protecta DR

US Market Release Date 03/25/2011

CE Market Approval Date

Registered US Implants 10,415

Estimated Active US Implants 9,348

Normal Battery Depletions (US) 20

NBG Code DDE-DDDR

Max Delivered Energy 35 J

Total Malfunctions (US) 8

Therapy Not Compromised Malfunctions 6

Battery Malfunction 0

Electrical Component 5

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 1

Software Malfunction 0

Therapy Compromised Malfunctions 2

Battery Malfunction 0


Electrical Component 2

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

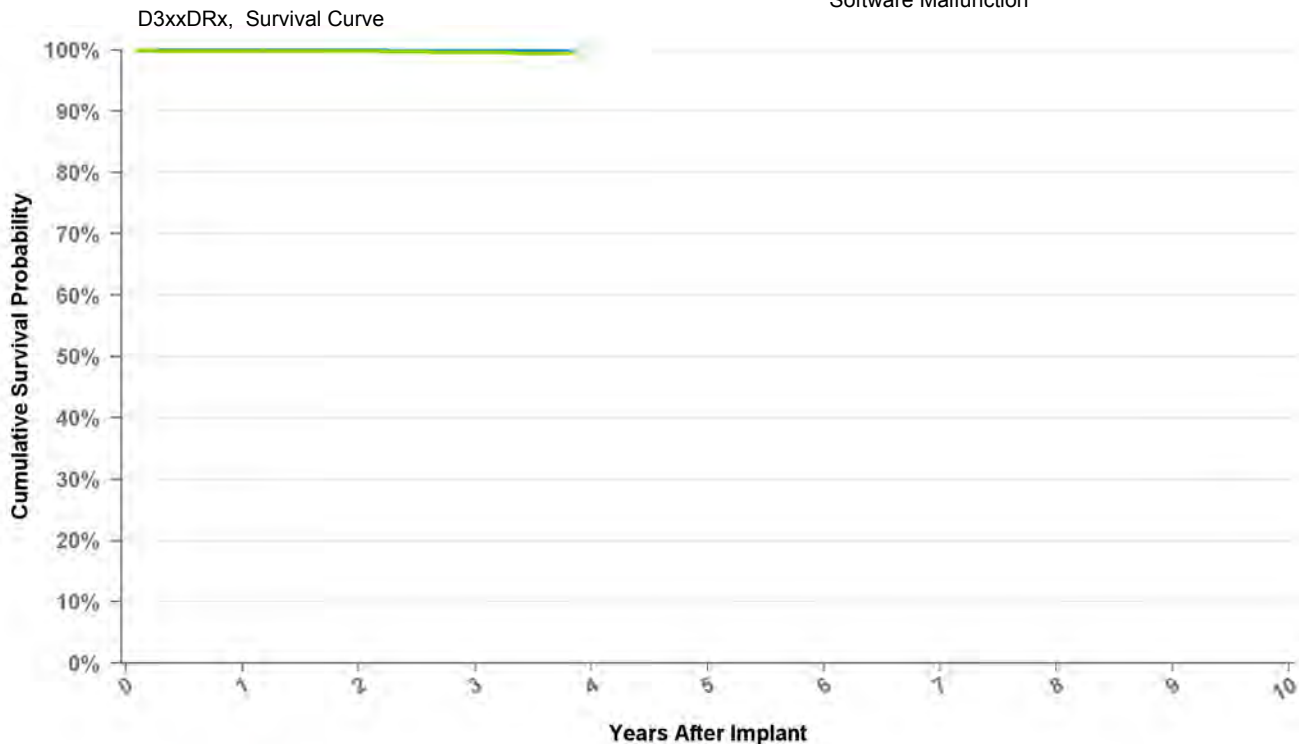

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.8% | 99.6% | 99.4% |
| Effective Sample Size | 57472 | 40632 | 13475 | 337 |

Implantable Cardioverter Defibrillator

D334DRM Protecta DR

US Market Release Date 11/09/2011

CE Market Approval Date

Registered US Implants 2,881

Estimated Active US Implants 2,698

Normal Battery Depletions (US) 4

NBG Code DDE-DDDR

Max Delivered Energy 35 J

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

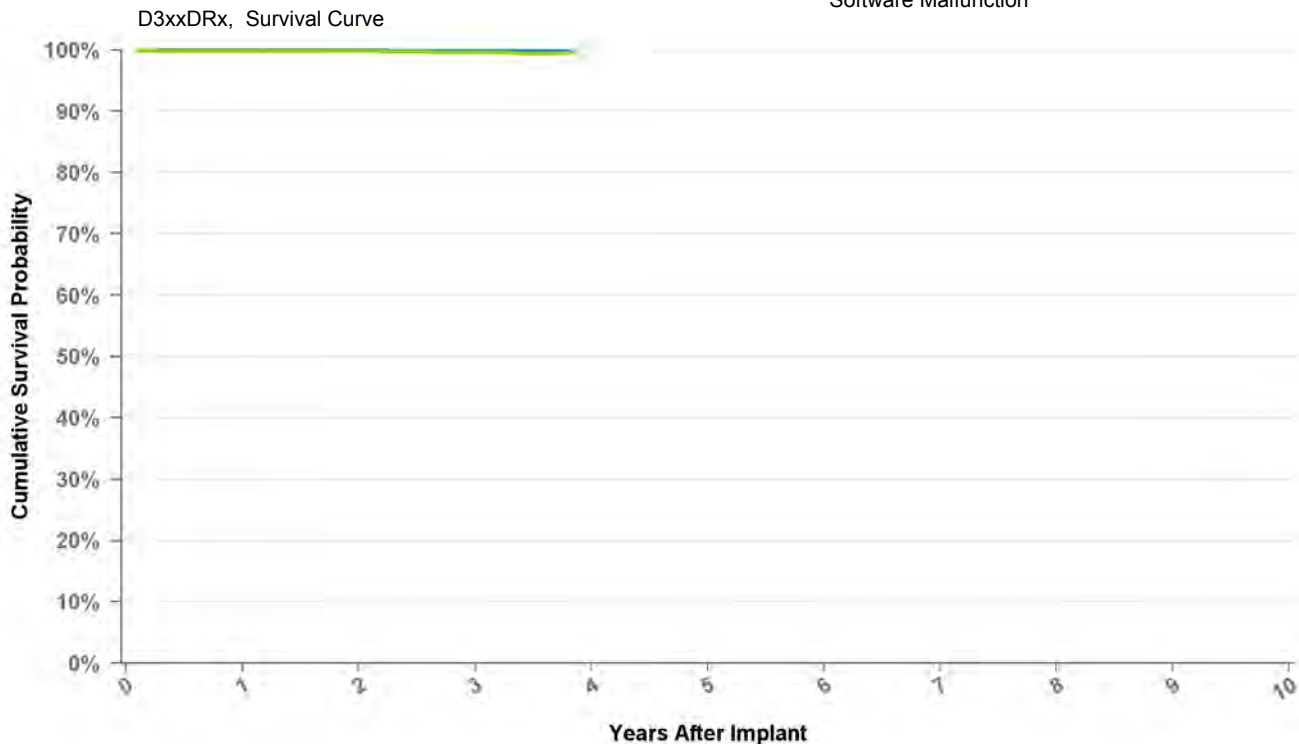

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.8% | 99.6% | 99.4% |
| Effective Sample Size | 57472 | 40632 | 13475 | 337 |

Implantable Cardioverter Defibrillator

D334VRG Protecta VR

| | |
|---------------------------------------|------------|
| US Market Release Date | 03/25/2011 |
| CE Market Approval Date | |
| Registered US Implants | 6,190 |
| Estimated Active US Implants | 5,584 |
| Normal Battery Depletions (US) | 5 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 3 |
| Therapy Not Compromised Malfunctions | 2 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

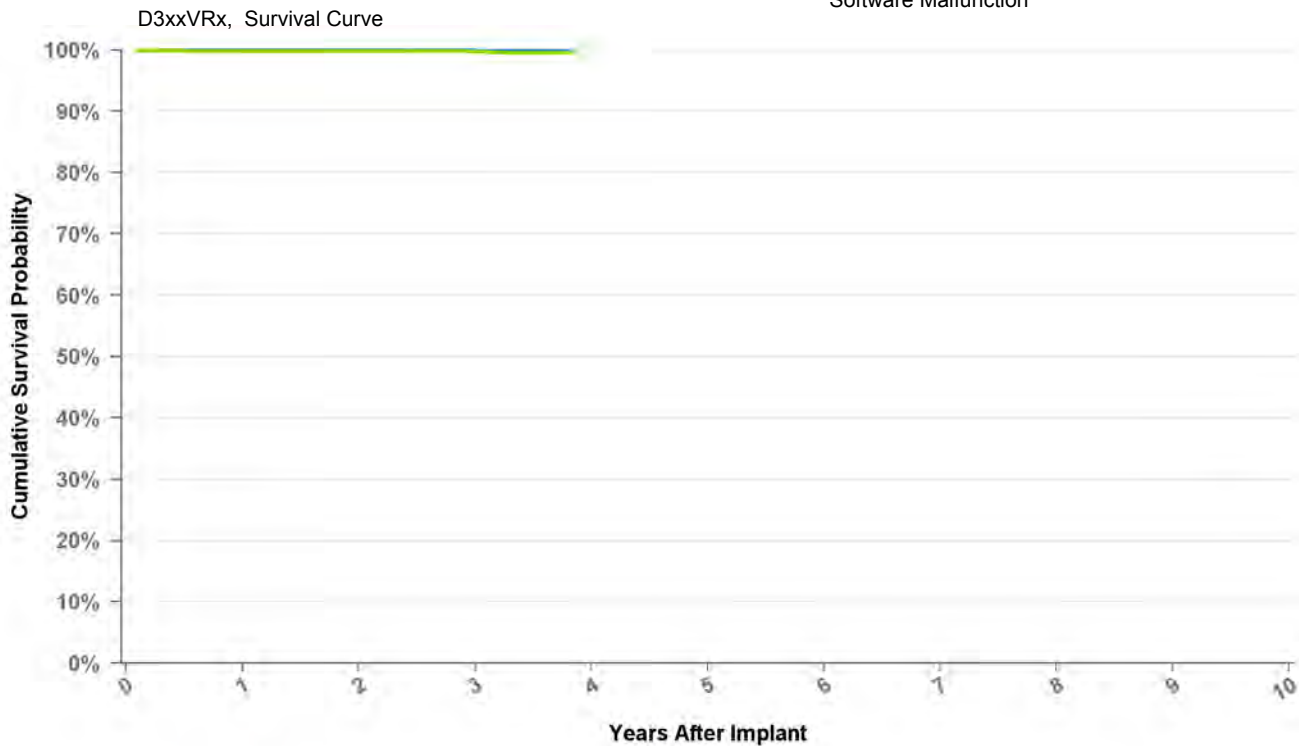

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.9% | 99.7% | 99.5% |
| Effective Sample Size | 27216 | 18397 | 5746 | 167 |

Implantable Cardioverter Defibrillator

D334VRM Protecta VR

US Market Release Date 05/02/2012

CE Market Approval Date

Registered US Implants 2,123

Estimated Active US Implants 1,990

Normal Battery Depletions (US) 0

NBG Code VVE-VVIR

Max Delivered Energy 35 J

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

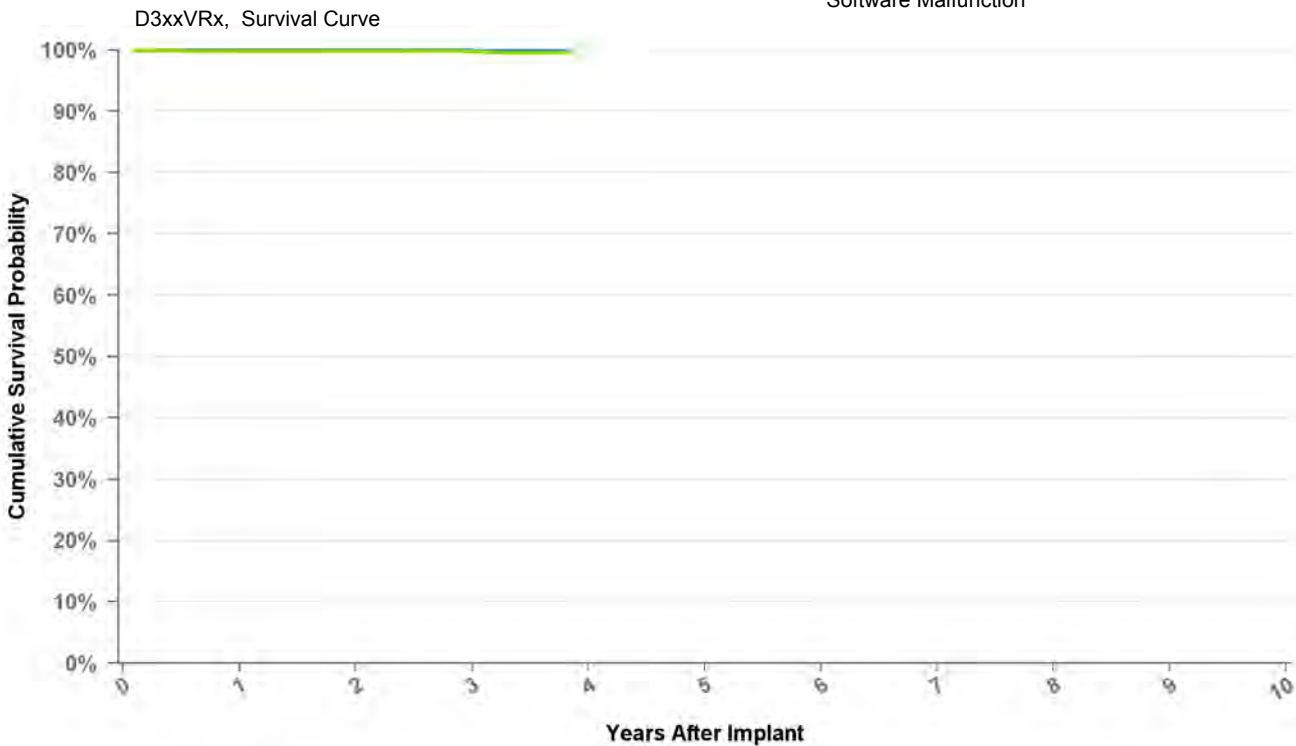

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.9% | 99.7% | 99.5% |
| Effective Sample Size | 27216 | 18397 | 5746 | 167 |

Implantable Cardioverter Defibrillator

D354DRG Protecta XT DR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 03/25/2010 |
| Registered US Implants | 2 |
| Estimated Active US Implants | 1 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

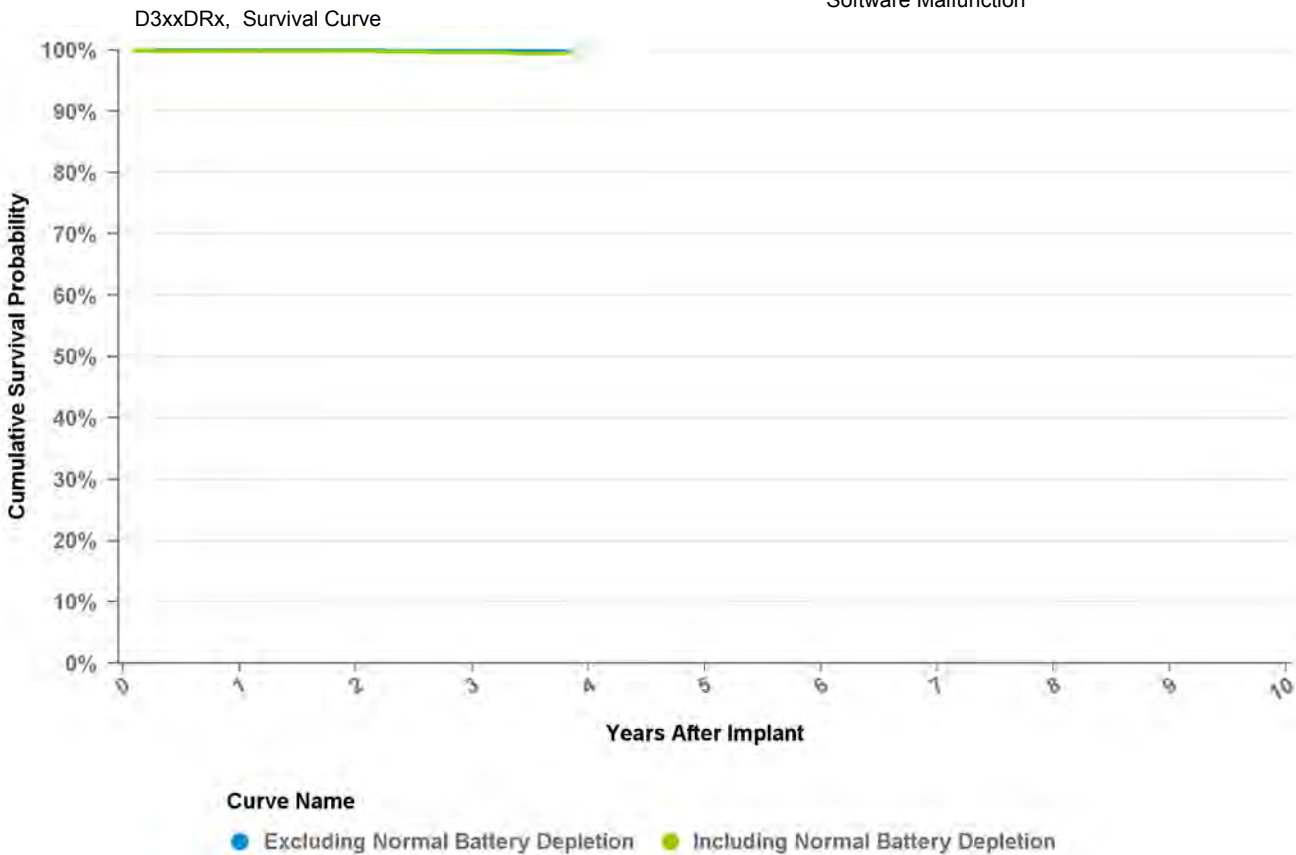


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.8% | 99.6% | 99.4% |
| Effective Sample Size | 57472 | 40632 | 13475 | 337 |

Implantable Cardioverter Defibrillator

D354DRM Protecta XT DR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 07/15/2010 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

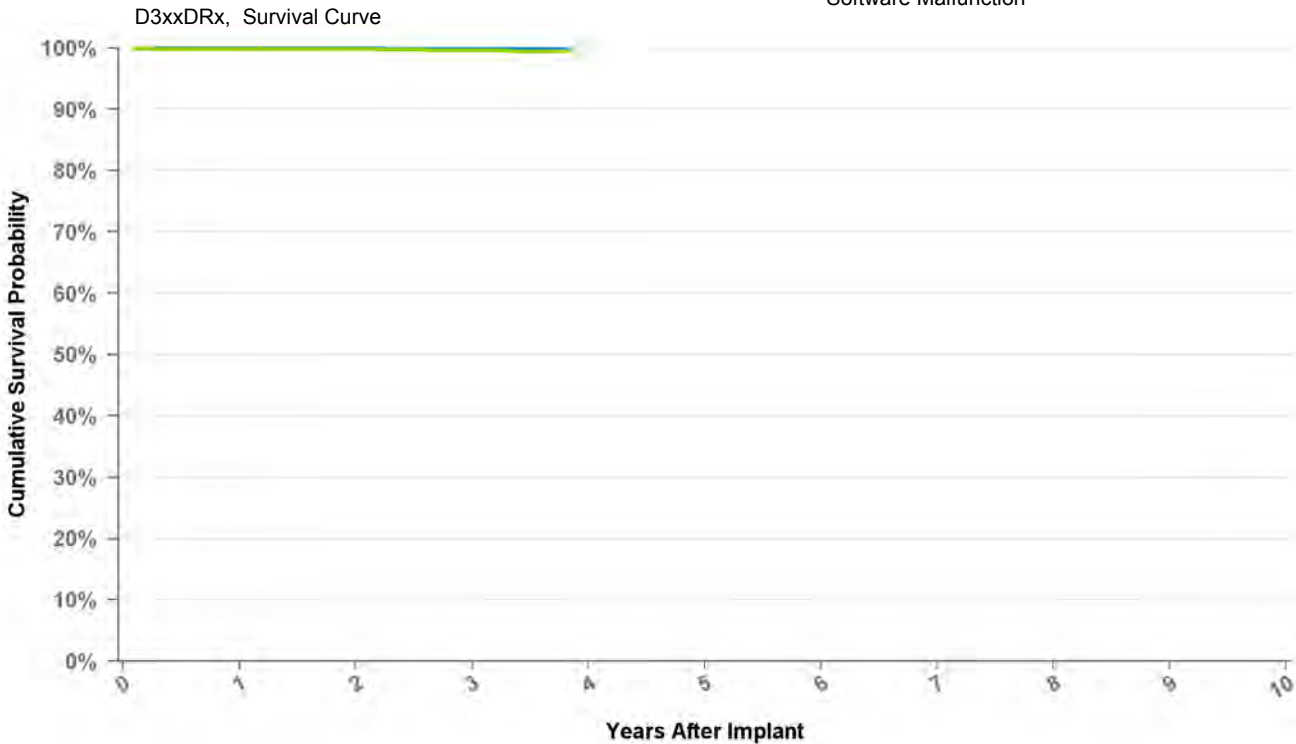

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.8% | 99.6% | 99.4% |
| Effective Sample Size | 57472 | 40632 | 13475 | 337 |

Implantable Cardioverter Defibrillator

D354VRG Protecta XT VR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 03/25/2010 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

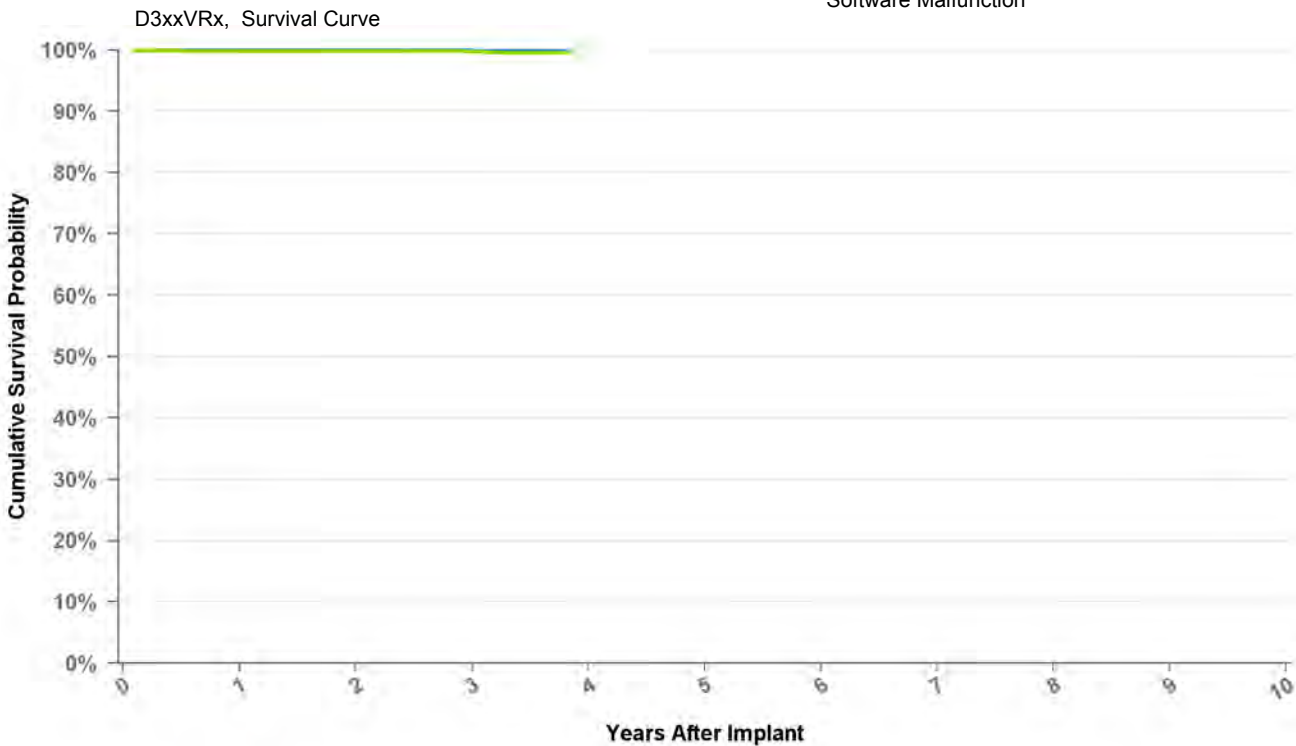

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.9% | 99.7% | 99.5% |
| Effective Sample Size | 27216 | 18397 | 5746 | 167 |

Implantable Cardioverter Defibrillator

D354VRM Protecta XT VR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 12/17/2010 |
| Registered US Implants | 1 |
| Estimated Active US Implants | 1 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

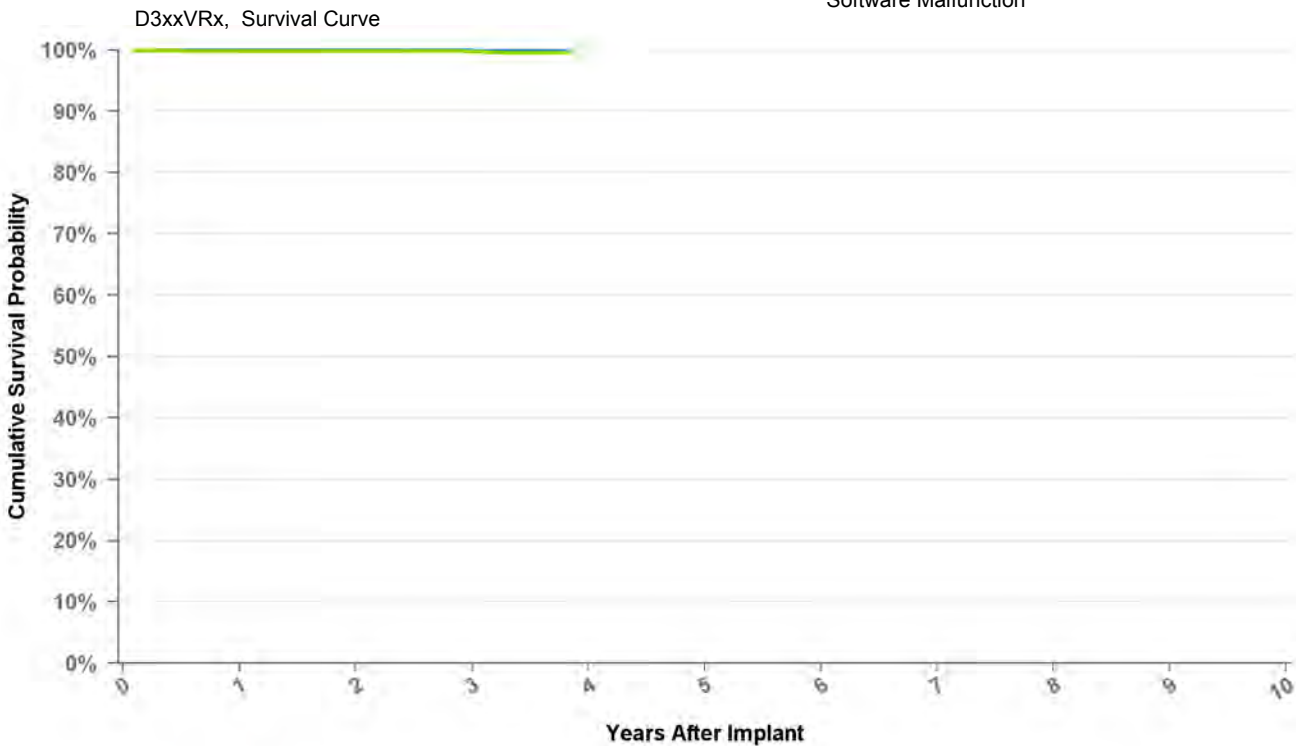

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.9% | 99.7% | 99.5% |
| Effective Sample Size | 27216 | 18397 | 5746 | 167 |

Implantable Cardioverter Defibrillator

D364DRG Protecta DR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 03/25/2010 |
| Registered US Implants | 1 |
| Estimated Active US Implants | 1 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

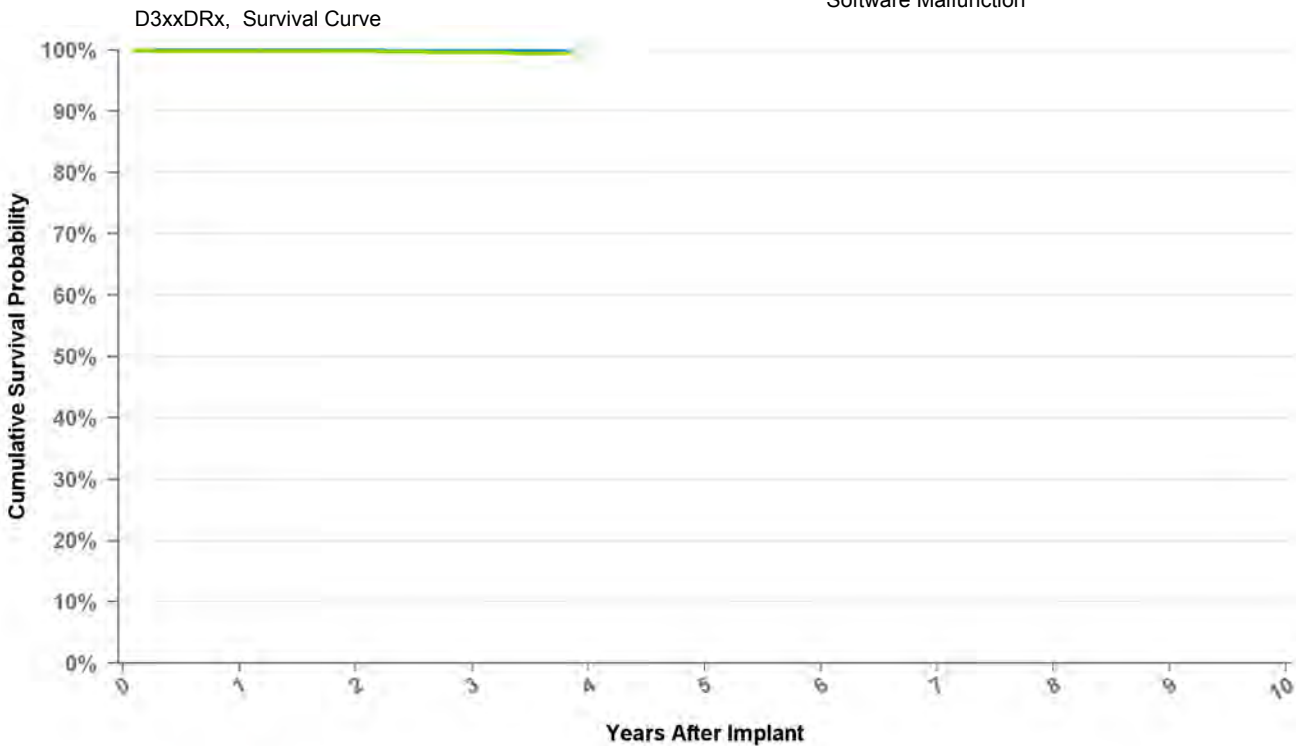

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.8% | 99.6% | 99.4% |
| Effective Sample Size | 57472 | 40632 | 13475 | 337 |

Implantable Cardioverter Defibrillator

D364DRM Protecta DR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 07/15/2010 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

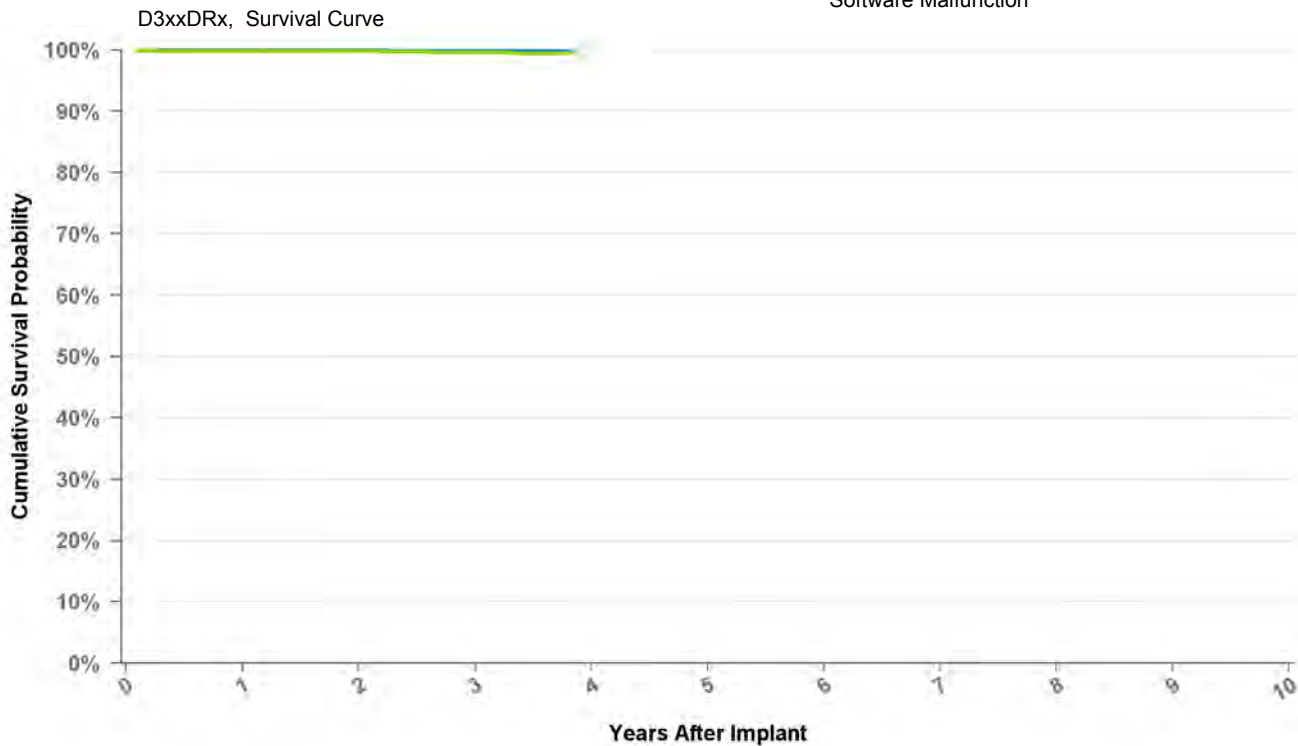

Curve Name
● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.8% | 99.6% | 99.4% |
| Effective Sample Size | 57472 | 40632 | 13475 | 337 |

Implantable Cardioverter Defibrillator

D364VRG Protecta VR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 03/25/2010 |
| Registered US Implants | 1 |
| Estimated Active US Implants | 1 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

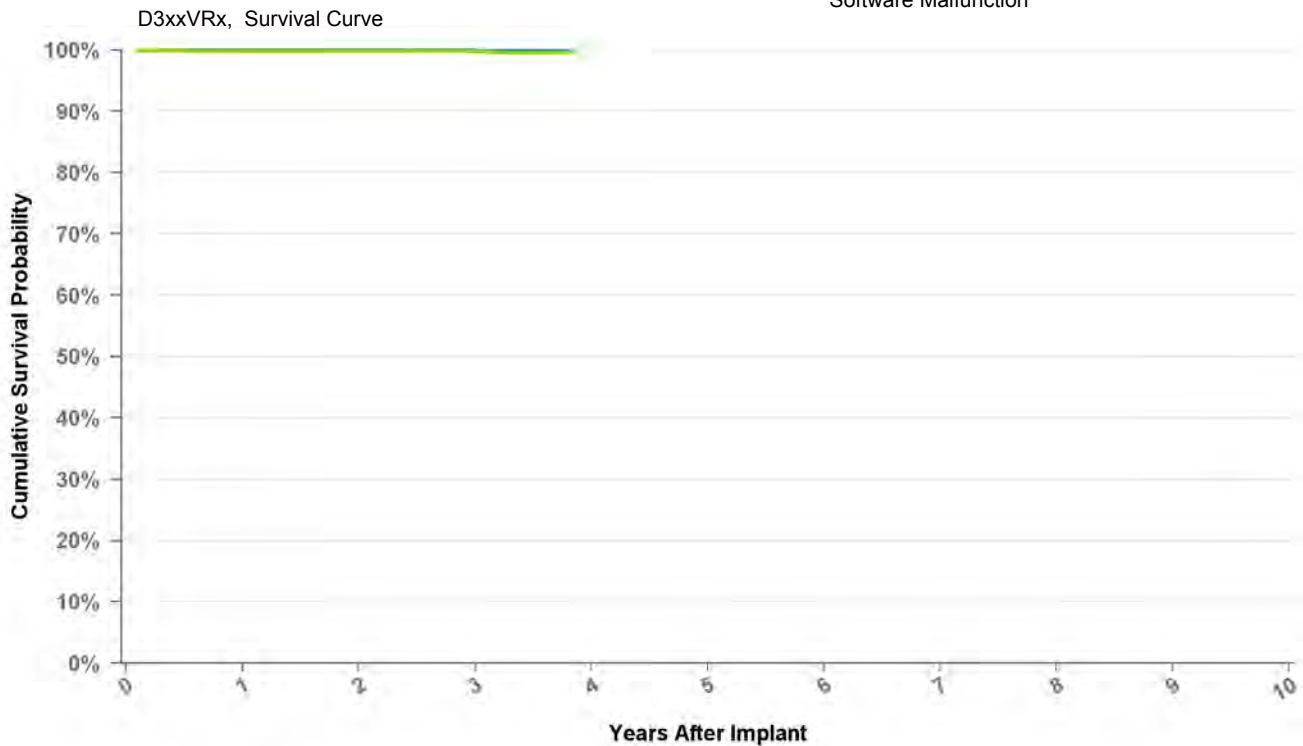

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.9% | 99.7% | 99.5% |
| Effective Sample Size | 27216 | 18397 | 5746 | 167 |

Implantable Cardioverter Defibrillator

D364VRM Protecta VR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 12/17/2010 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

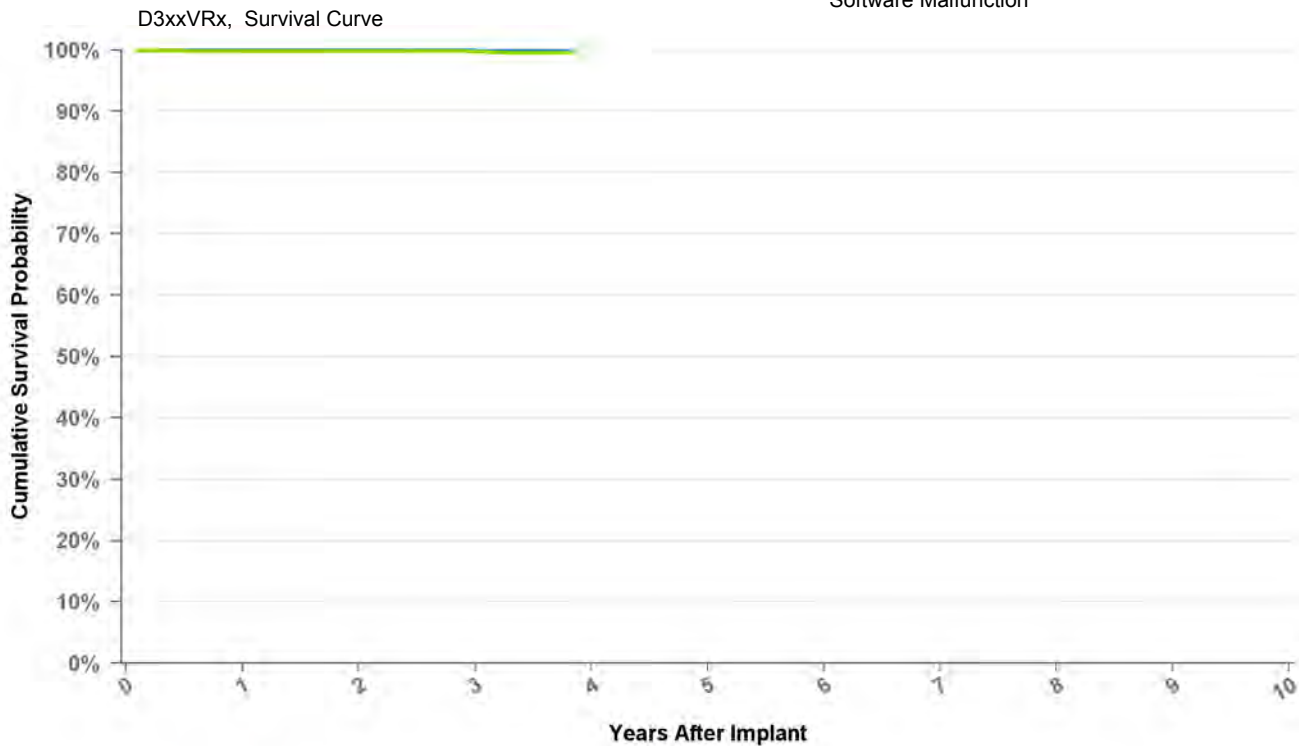

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.9% | 99.7% | 99.5% |
| Effective Sample Size | 27216 | 18397 | 5746 | 167 |

Implantable Cardioverter Defibrillator

D384DRG Cardia DR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 01/12/2011 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

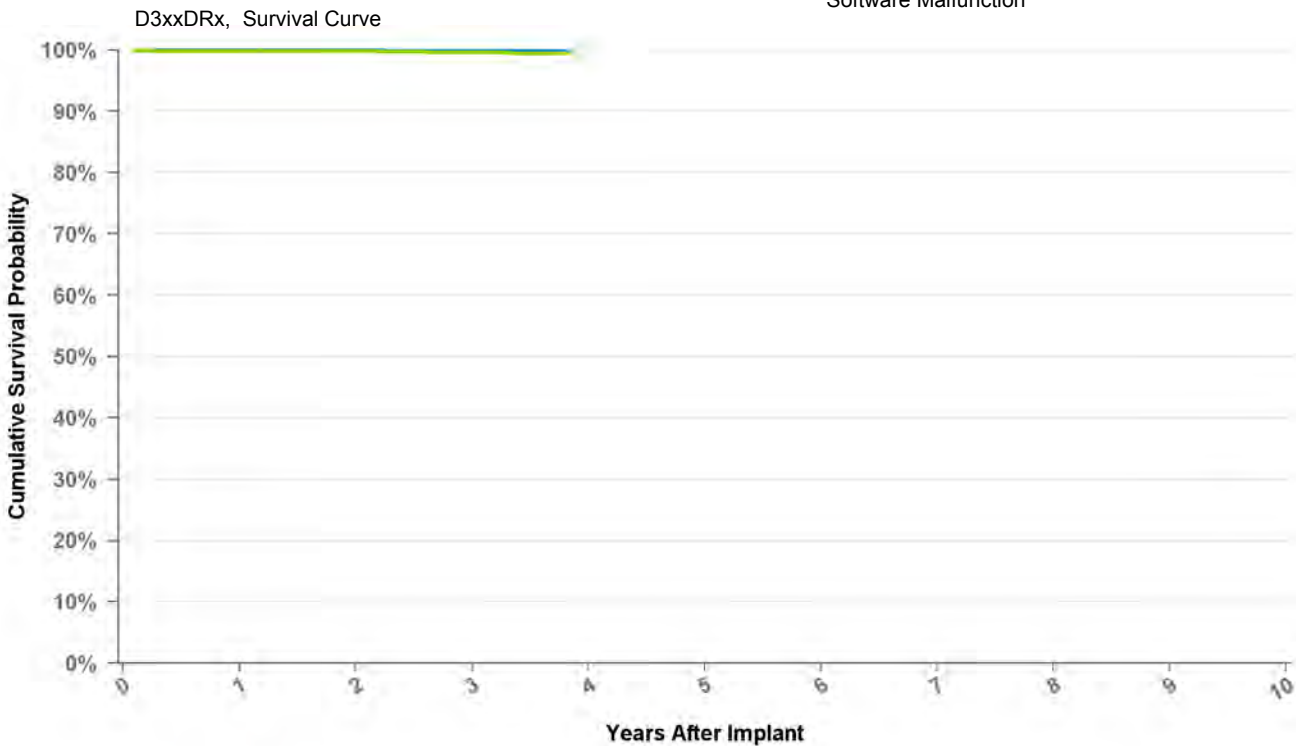

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.8% | 99.6% | 99.4% |
| Effective Sample Size | 57472 | 40632 | 13475 | 337 |

Implantable Cardioverter Defibrillator

D384VRG Cardia VR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 01/12/2011 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

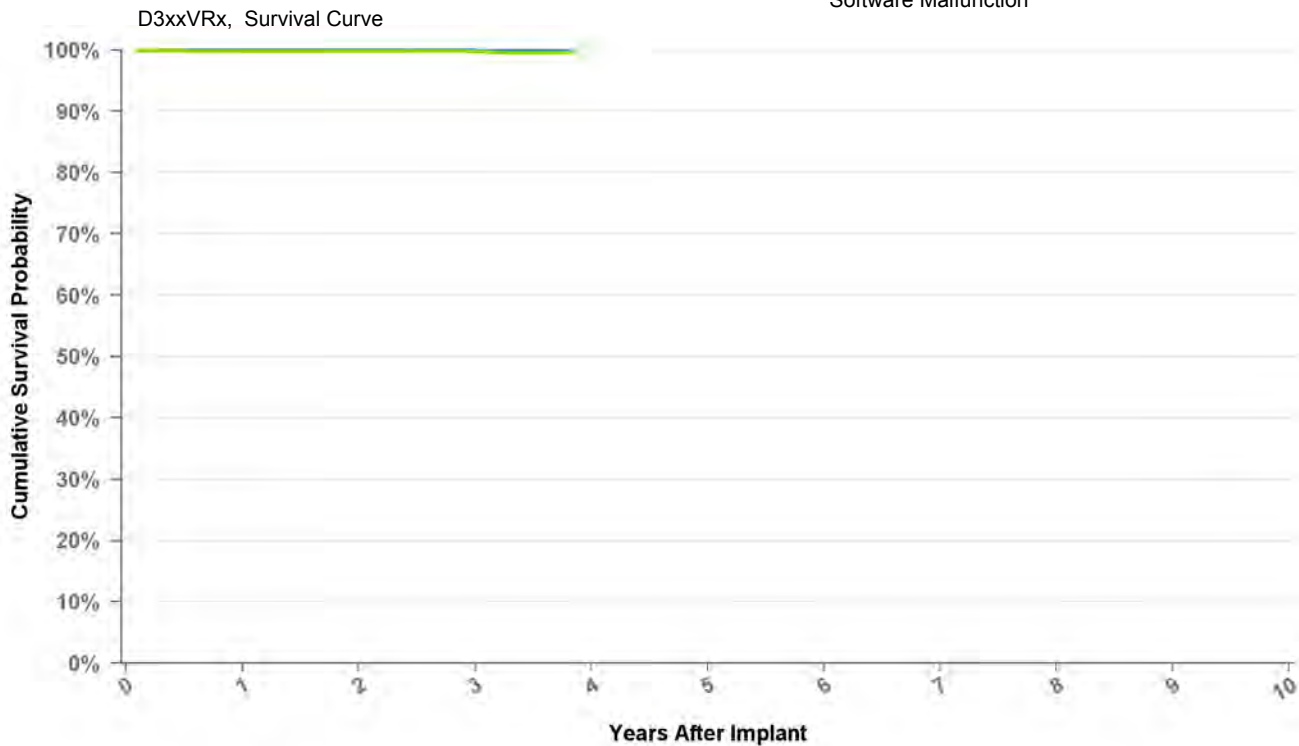

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.9% | 99.7% | 99.5% |
| Effective Sample Size | 27216 | 18397 | 5746 | 167 |

Implantable Cardioverter Defibrillator

D394DRG Egida DR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 01/12/2011 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-DDDR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

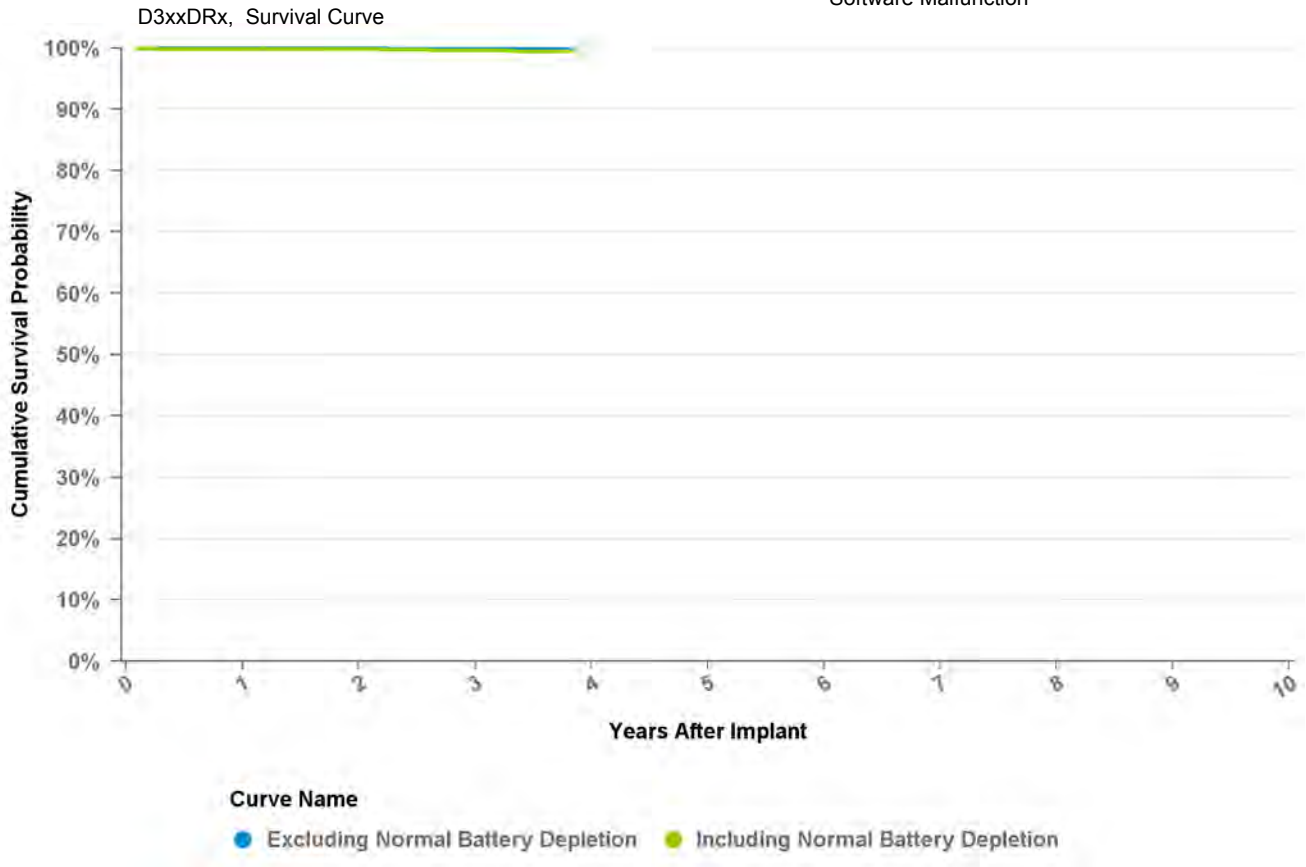


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.8% | 99.6% | 99.4% |
| Effective Sample Size | 57472 | 40632 | 13475 | 337 |

Implantable Cardioverter Defibrillator

D394VRG Egida VR

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 01/12/2011 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 35 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

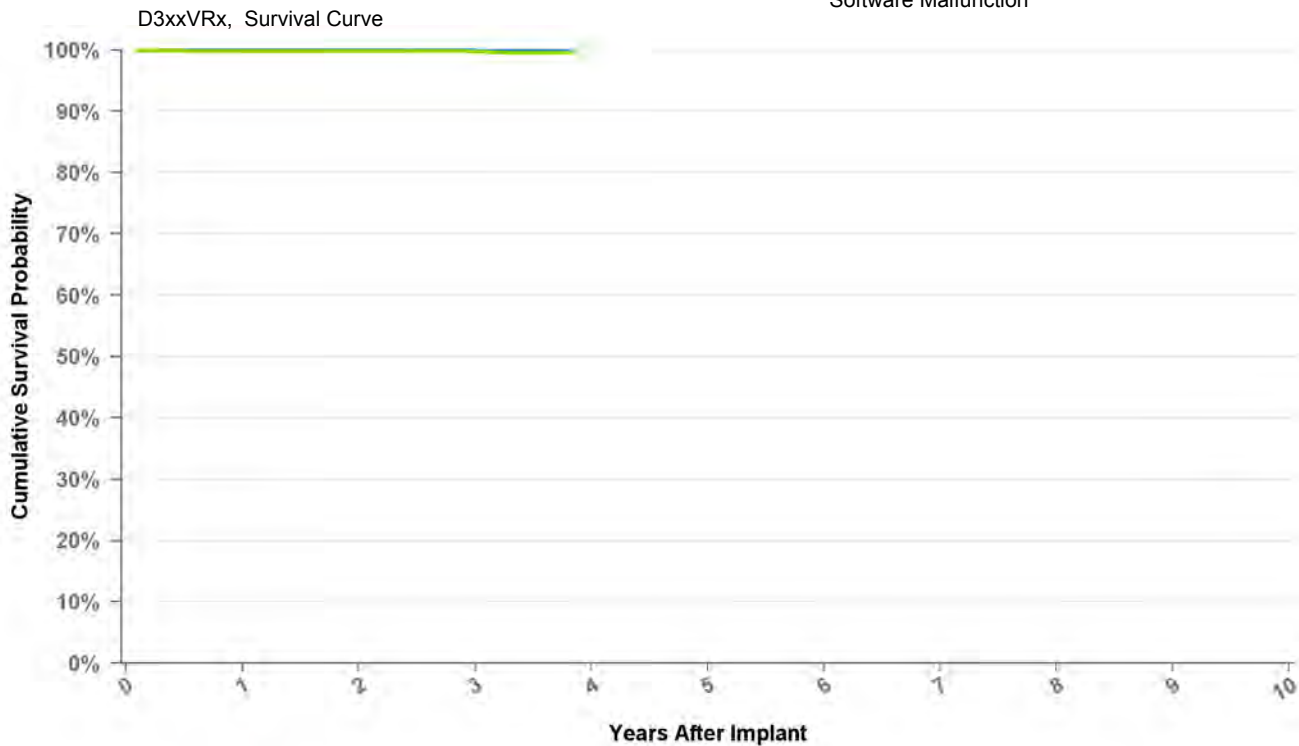

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | at 46 mo |
|------------------------------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 99.9% | 99.9% | 99.7% | 99.5% |
| Effective Sample Size | 27216 | 18397 | 5746 | 167 |

Implantable Cardioverter Defibrillator

DDBB1D1 Evera XT

| | |
|---------------------------------------|------------|
| US Market Release Date | 04/03/2013 |
| CE Market Approval Date | |
| Registered US Implants | 15,520 |
| Estimated Active US Implants | 14,994 |
| Normal Battery Depletions (US) | 1 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 1 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

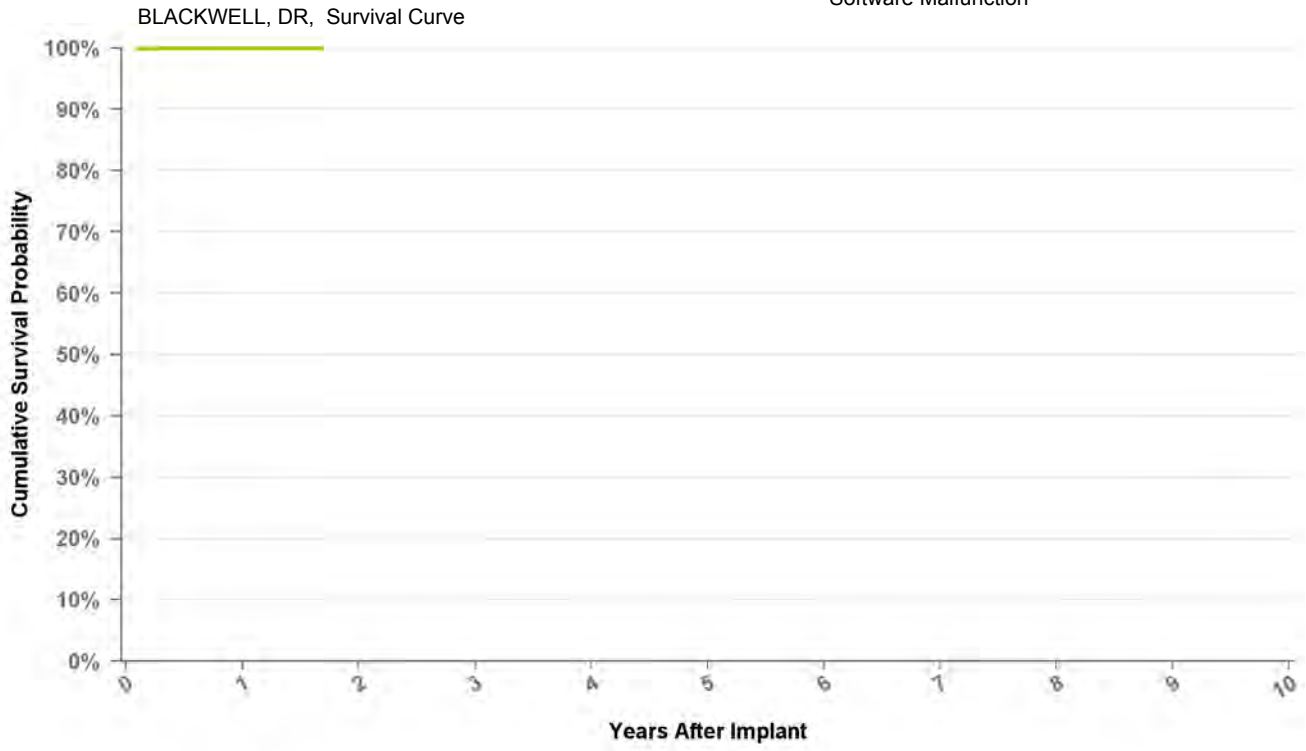

Curve Name
● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | at 20 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% |
| Effective Sample Size | 13934 | 335 |

Implantable Cardioverter Defibrillator

DDBB1D4 Evera XT

| | |
|---------------------------------------|------------|
| US Market Release Date | 04/03/2013 |
| CE Market Approval Date | |
| Registered US Implants | 16,056 |
| Estimated Active US Implants | 15,650 |
| Normal Battery Depletions (US) | 1 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 2 |
| Therapy Not Compromised Malfunctions | 2 |
| Battery Malfunction | 0 |
| Electrical Component | 2 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

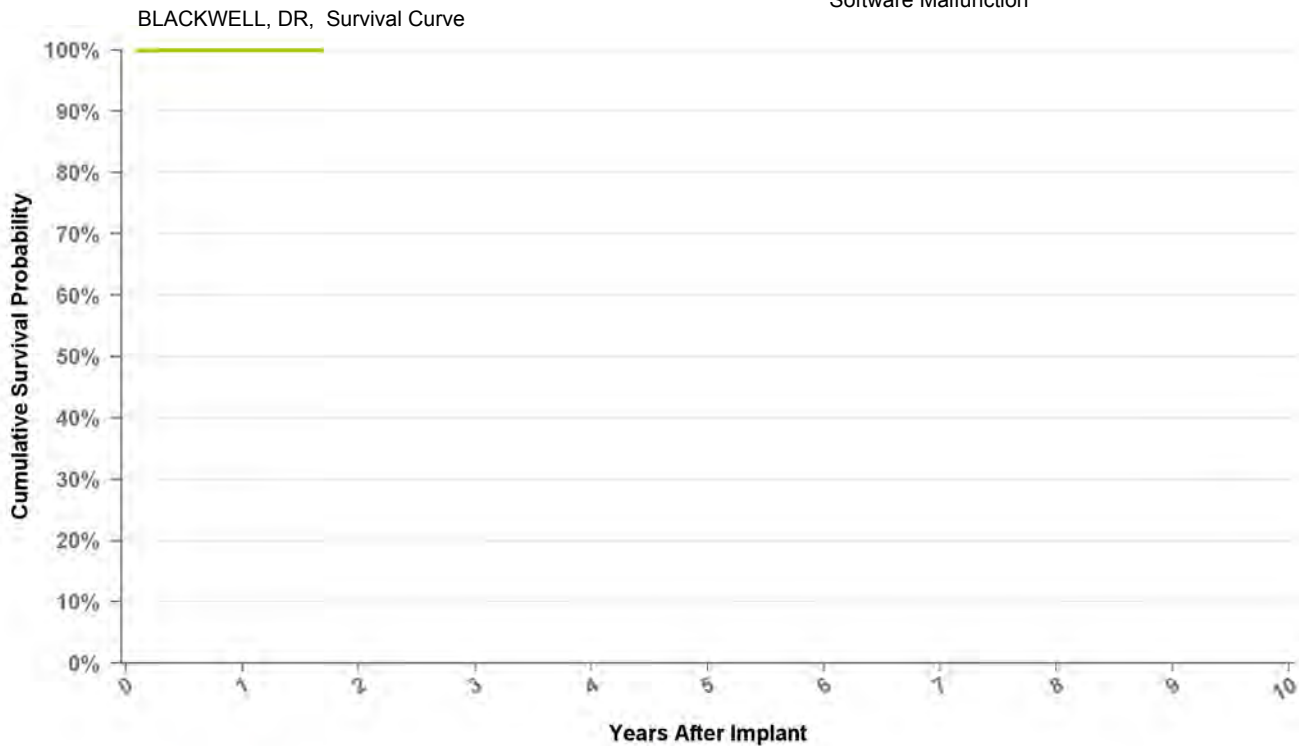

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 20 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% |
| Effective Sample Size | 13934 | 335 |

Implantable Cardioverter Defibrillator

DDBB2D1 Evera XT

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 12/17/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

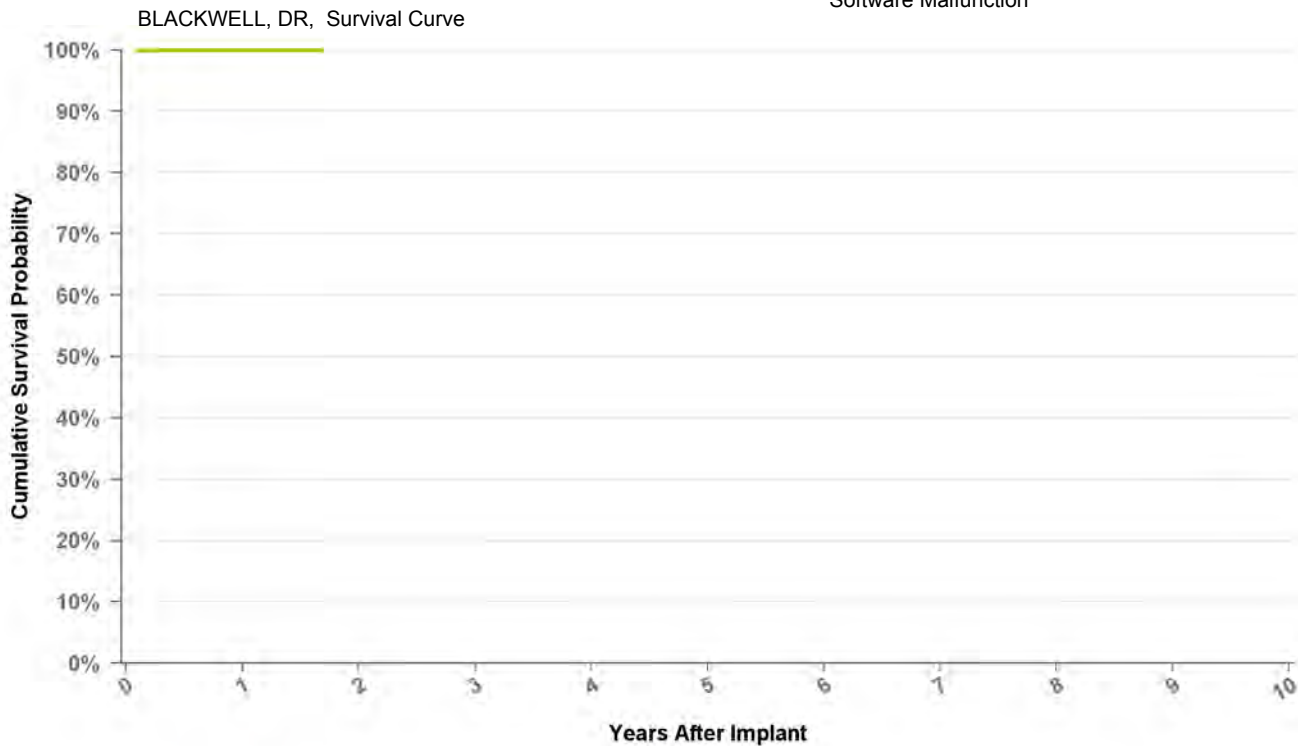

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 20 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% |
| Effective Sample Size | 13934 | 335 |

Implantable Cardioverter Defibrillator

DDBB2D4 Evera XT

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 12/17/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

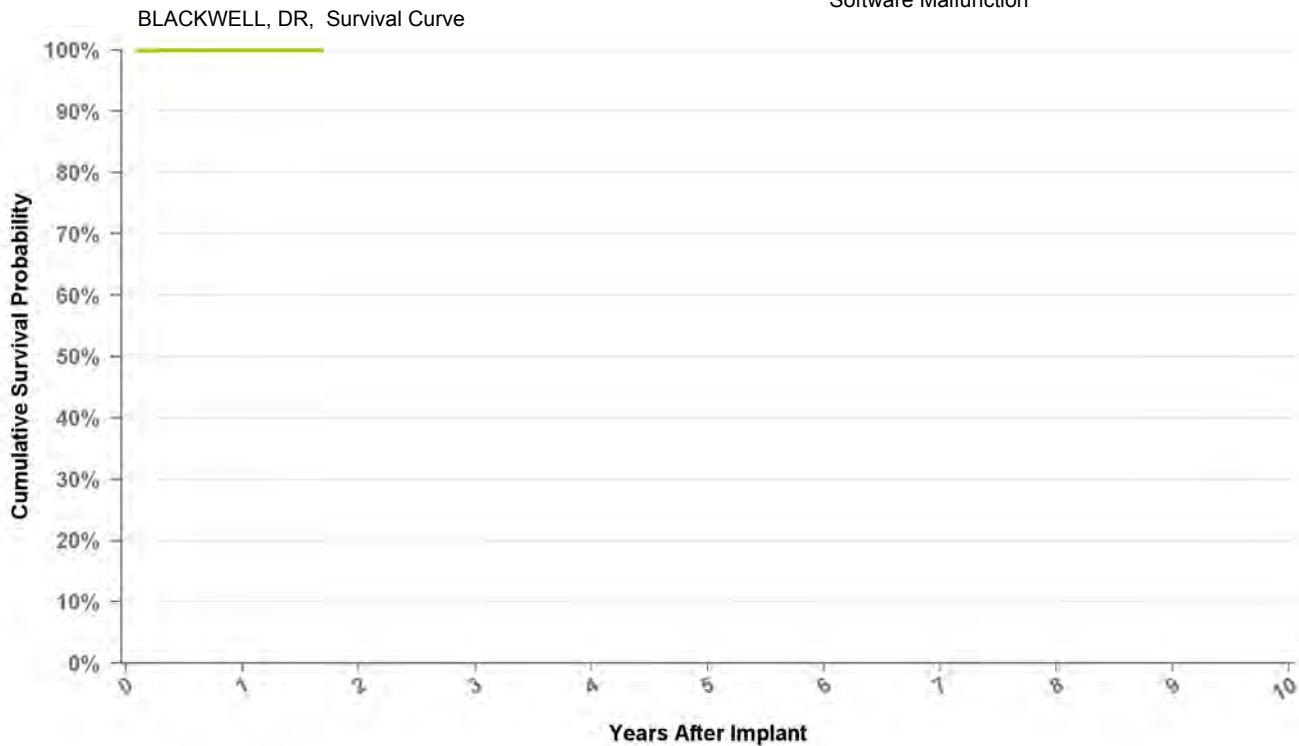

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 20 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% |
| Effective Sample Size | 13934 | 335 |

Implantable Cardioverter Defibrillator

DDBC3D1 Evera S

| | |
|---------------------------------------|------------|
| US Market Release Date | 04/03/2013 |
| CE Market Approval Date | 12/17/2012 |
| Registered US Implants | 3,455 |
| Estimated Active US Implants | 3,328 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 1 |
| Therapy Not Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

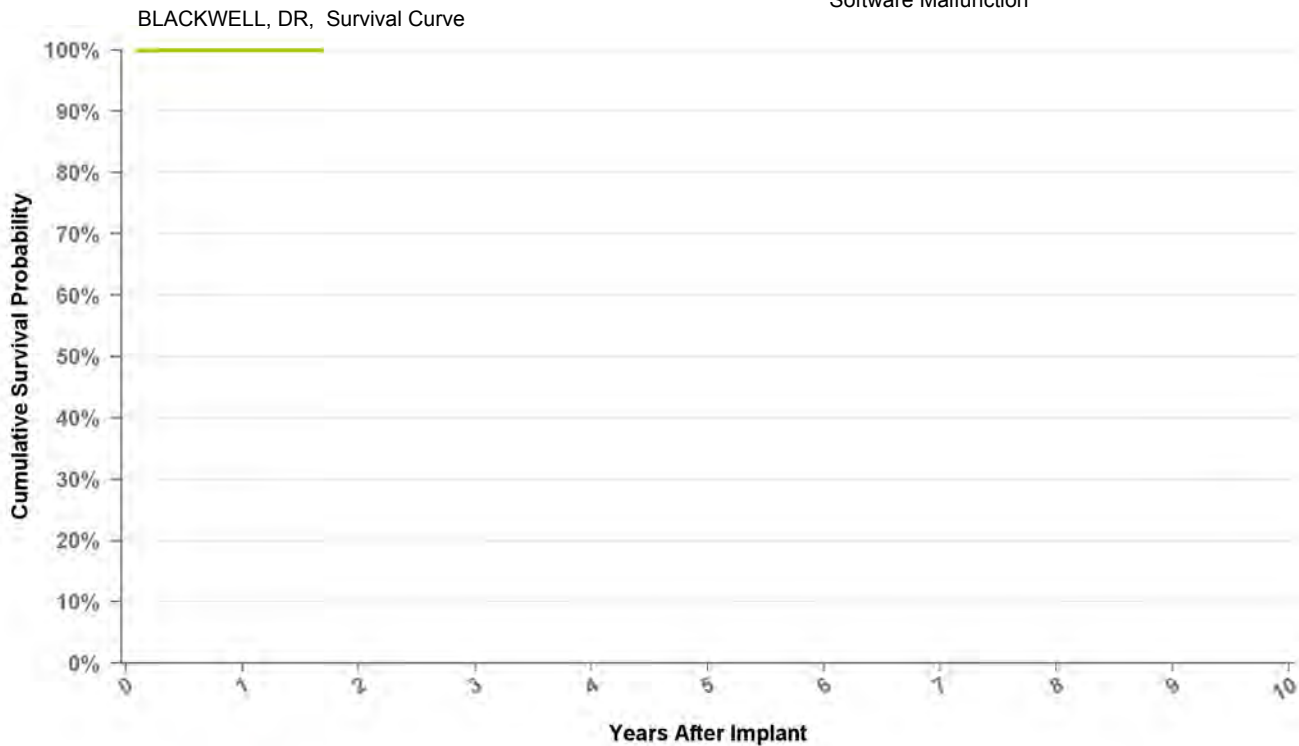

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 20 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% |
| Effective Sample Size | 13934 | 335 |

Implantable Cardioverter Defibrillator

DDBC3D4 Evera S

| | |
|---------------------------------------|------------|
| US Market Release Date | 04/03/2013 |
| CE Market Approval Date | 12/17/2013 |
| Registered US Implants | 3,050 |
| Estimated Active US Implants | 2,967 |
| Normal Battery Depletions (US) | 1 |
| NBG Code | DDE-DDDR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 1 |
| Therapy Not Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

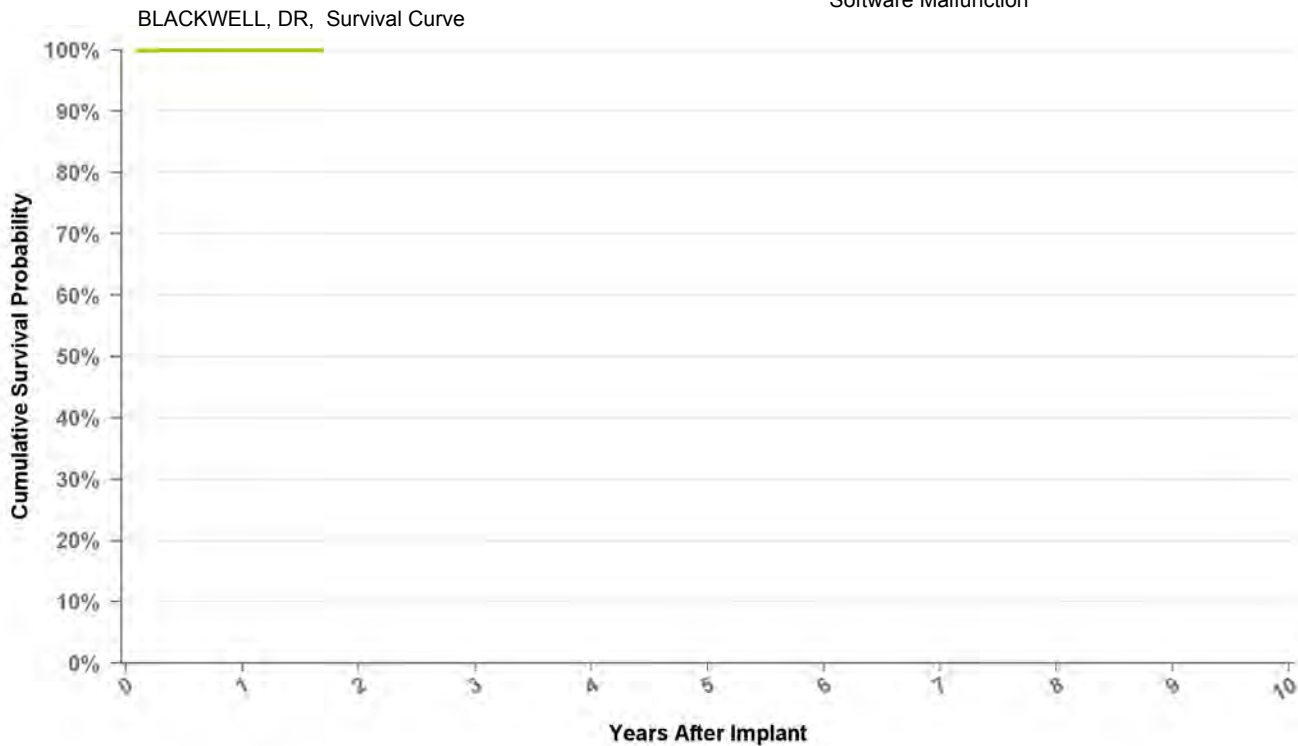

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | at 20 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% |
| Effective Sample Size | 13934 | 335 |

Implantable Cardioverter Defibrillator

DVBB1D1 Evera XT

US Market Release Date 04/03/2013

CE Market Approval Date

Registered US Implants 7,128

Estimated Active US Implants 6,903

Normal Battery Depletions (US) 0

NBG Code VVE-VVIR

Max Delivered Energy 36 J

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

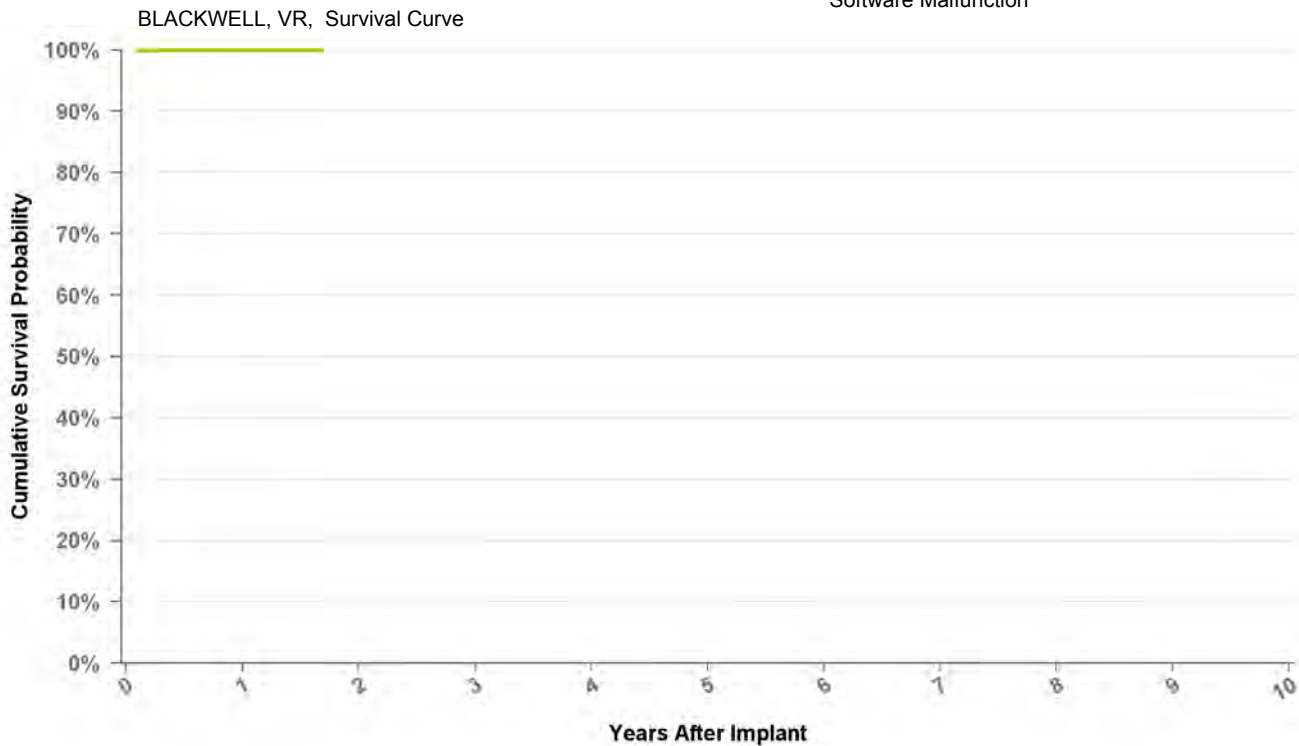

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | at 20 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% |
| Effective Sample Size | 7955 | 223 |

Implantable Cardioverter Defibrillator

DVBB1D4 Evera XT

US Market Release Date 04/03/2013

CE Market Approval Date

Registered US Implants 12,404

Estimated Active US Implants 12,086

Normal Battery Depletions (US) 1

NBG Code VVE-VVIR

Max Delivered Energy 36 J

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

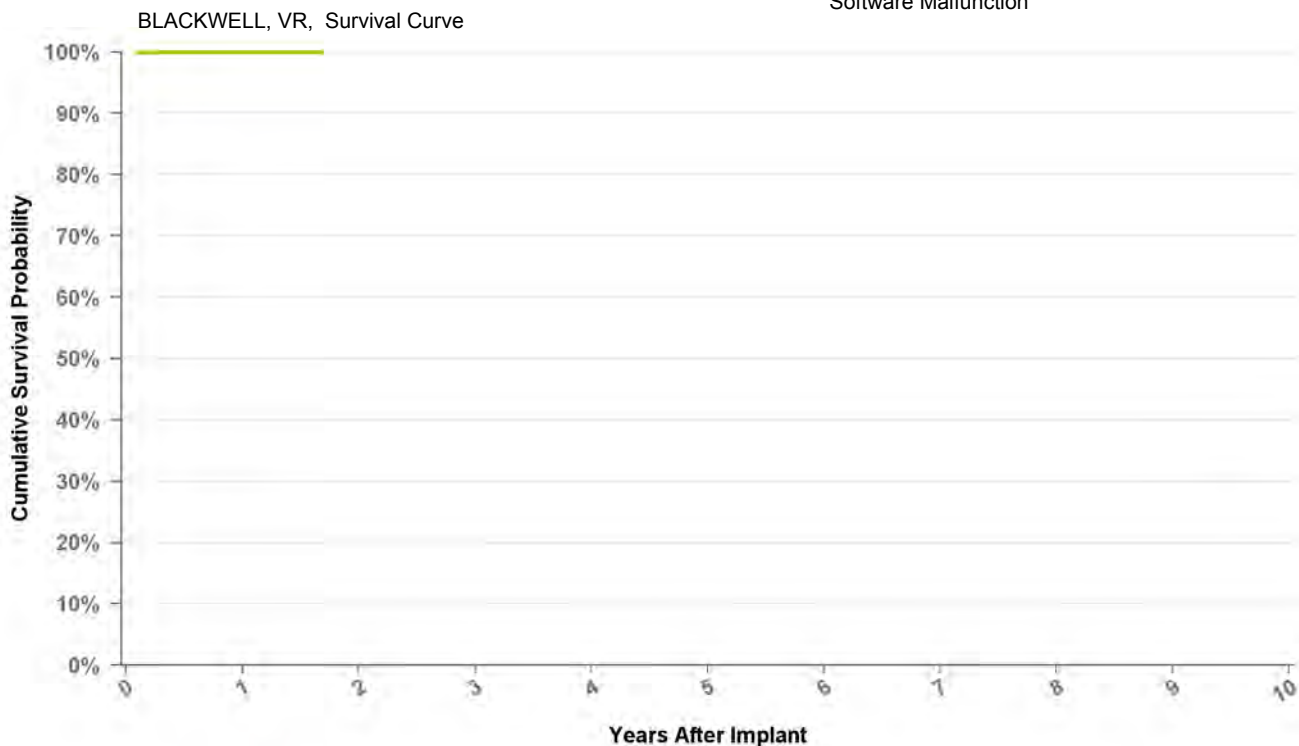

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 20 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% |
| Effective Sample Size | 7955 | 223 |

Implantable Cardioverter Defibrillator

DVBB2D1 Evera XT

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 12/17/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

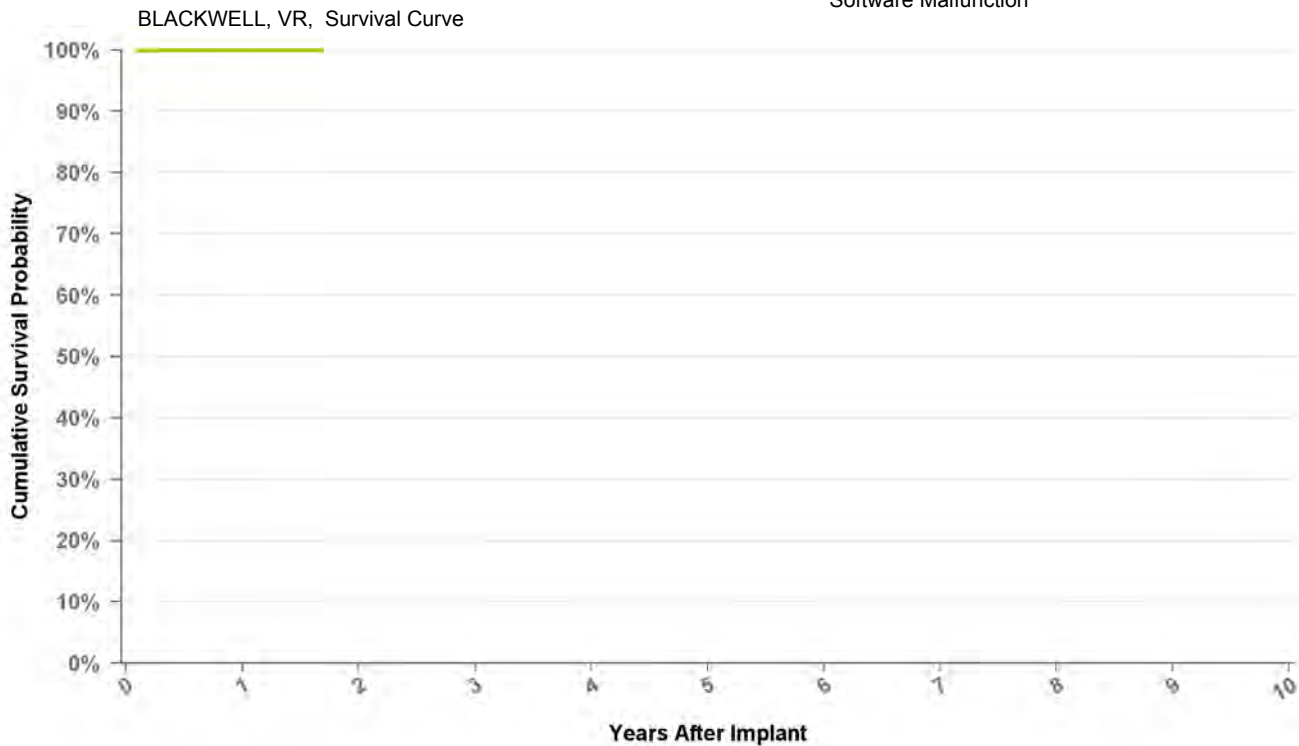

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 20 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% |
| Effective Sample Size | 7955 | 223 |

Implantable Cardioverter Defibrillator

DVBB2D4 Evera XT

| | |
|---------------------------------------|------------|
| US Market Release Date | |
| CE Market Approval Date | 12/17/2012 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

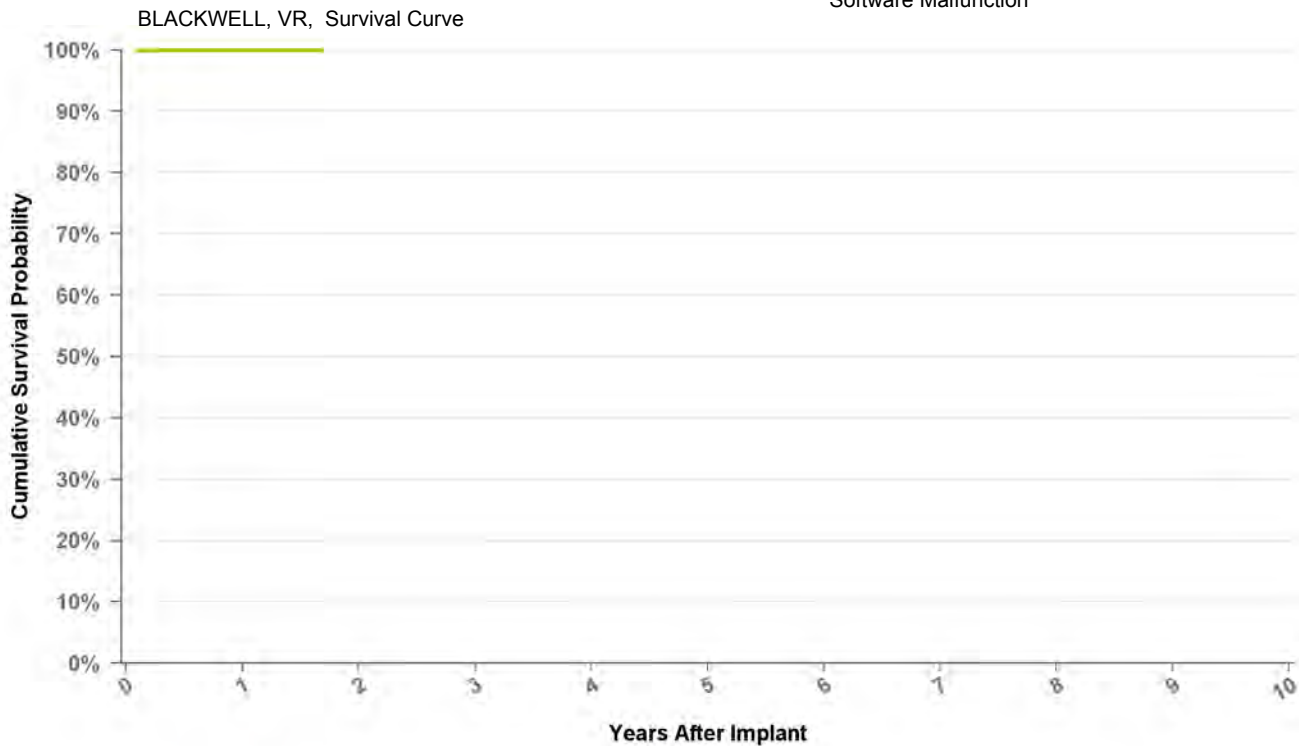

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 20 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% |
| Effective Sample Size | 7955 | 223 |

Implantable Cardioverter Defibrillator

DVBC3D1 Evera S

| | |
|---------------------------------------|------------|
| US Market Release Date | 04/03/2013 |
| CE Market Approval Date | 12/17/2012 |
| Registered US Implants | 1,803 |
| Estimated Active US Implants | 1,746 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

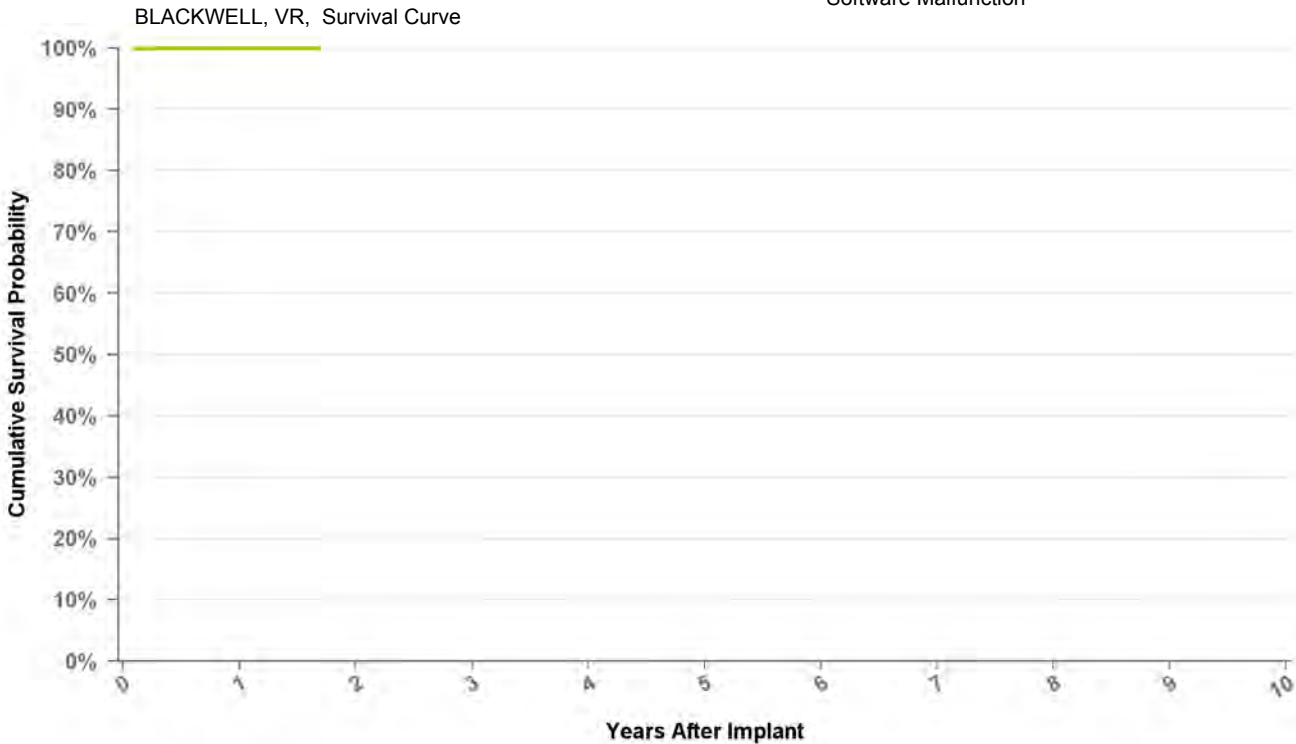

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | at 20 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% |
| Effective Sample Size | 7955 | 223 |

Implantable Cardioverter Defibrillator

DVBC3D4 Evera S

| | |
|---------------------------------------|------------|
| US Market Release Date | 04/03/2013 |
| CE Market Approval Date | 12/17/2012 |
| Registered US Implants | 2,758 |
| Estimated Active US Implants | 2,686 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | VVE-VVIR |
| Max Delivered Energy | 36 J |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

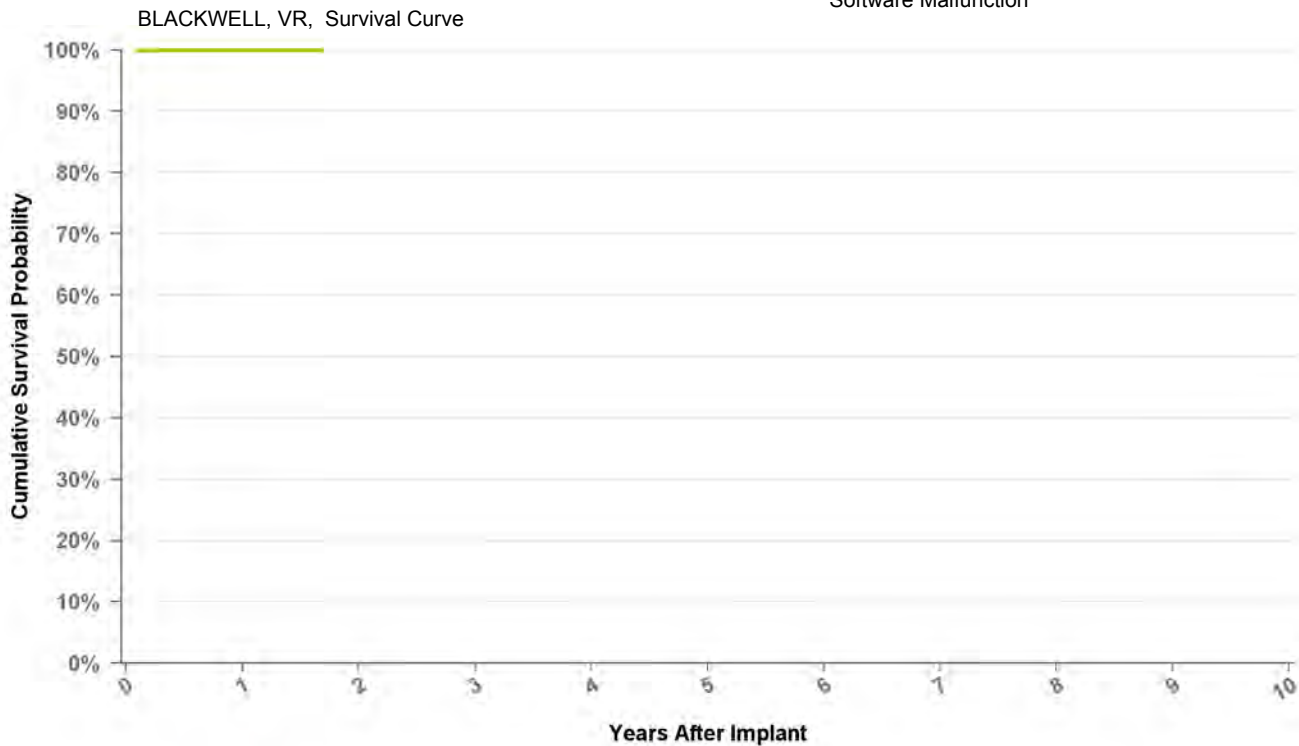

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | at 20 mo |
|------------------------------|--------|----------|
| Excluding NBD | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% |
| Effective Sample Size | 7955 | 223 |

Implantable Pulse Generator

A2DR01 Advisa DR MRI

US Market Release Date 01/15/2013

CE Market Approval Date

Registered US Implants 70,202

Estimated Active US Implants 68,669

Normal Battery Depletions (US) 1

NBG Code OAE-DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 4

Therapy Not Compromised Malfunctions 3

Battery Malfunction 0

Electrical Component 2

Electrical Interconnect 1

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 1


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

A2DR01, A3DR01, A5DR01, EN1DR01, Survival Curve

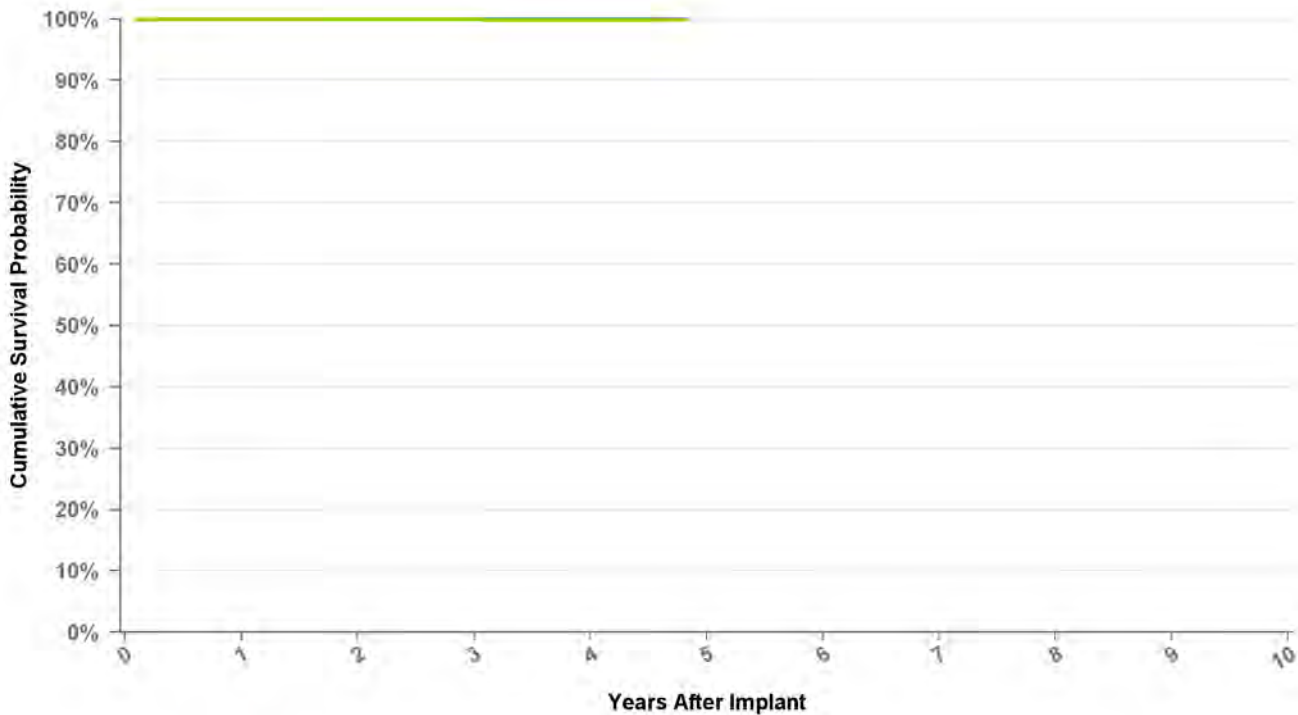

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | at 58 mo |
|-----------------------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% |
| Effective Sample Size | 40851 | 12039 | 6804 | 2770 | 161 |

Implantable Pulse Generator

A3DR01 Advisa DR MRI

US Market Release Date

CE Market Approval Date 06/02/2009

Registered US Implants 0

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code OAE-DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

A2DR01, A3DR01, A5DR01, EN1DR01, Survival Curve

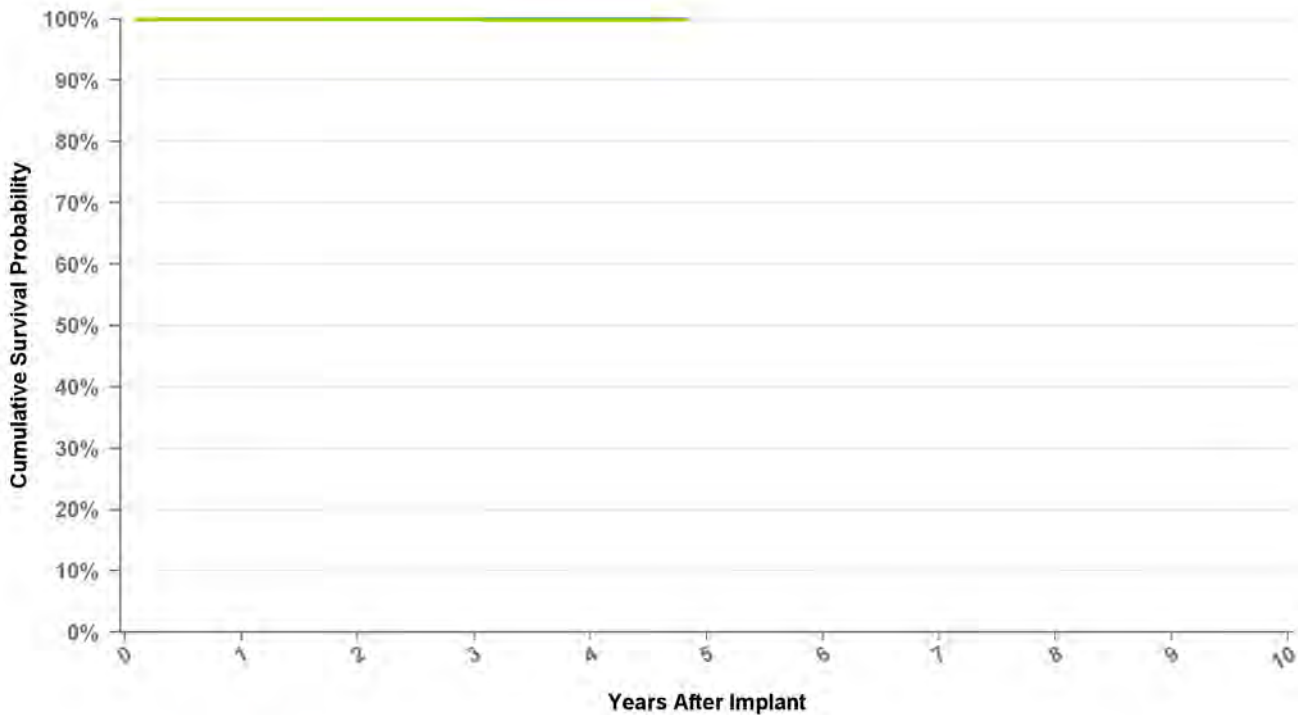

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | at 58 mo |
|------------------------------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% |
| Effective Sample Size | 40851 | 12039 | 6804 | 2770 | 161 |

Implantable Pulse Generator

A4DR01 Advisa DR

US Market Release Date 04/04/2011

CE Market Approval Date

Registered US Implants 1,536

Estimated Active US Implants 1,433

Normal Battery Depletions (US) 0

NBG Code OAE-DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

A2DR01, A3DR01, A5DR01, EN1DR01, Survival Curve

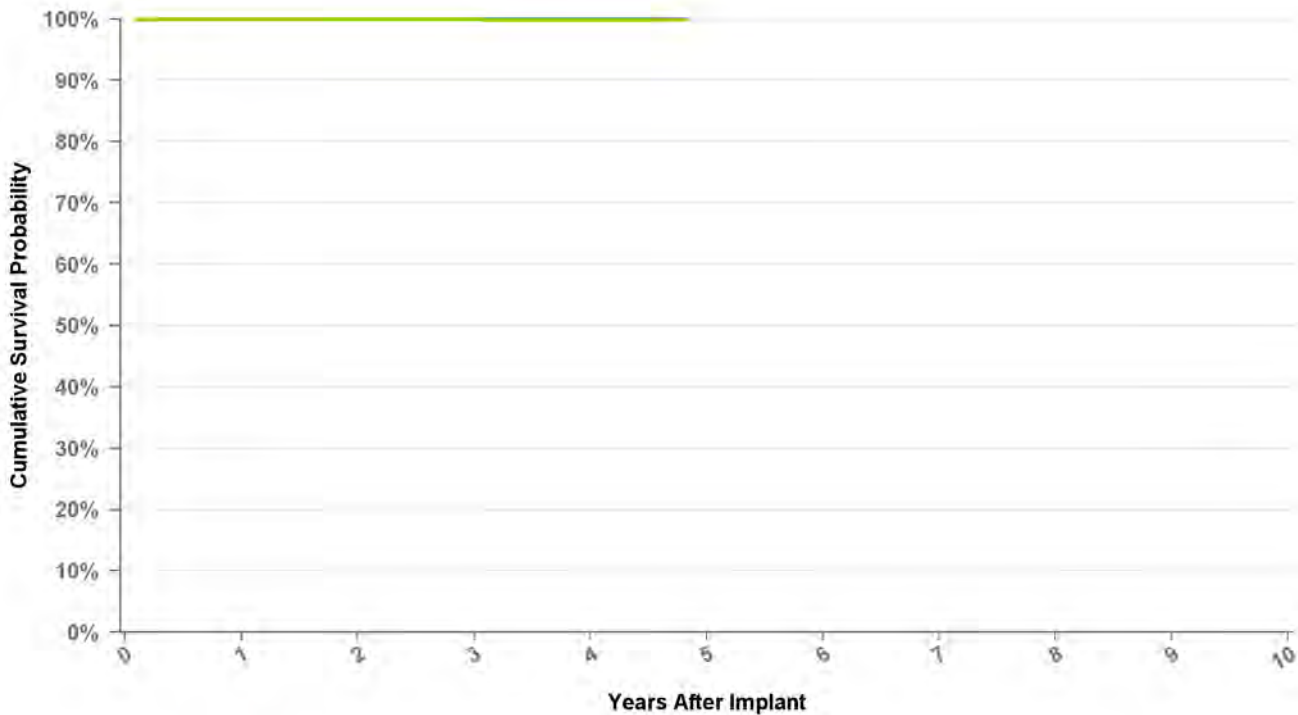

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | at 58 mo |
|------------------------------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% |
| Effective Sample Size | 40851 | 12039 | 6804 | 2770 | 161 |

Implantable Pulse Generator

A5DR01 Advisa DR

US Market Release Date

CE Market Approval Date 06/02/2009

Registered US Implants 0

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code OAE-DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

A2DR01, A3DR01, A5DR01, EN1DR01, Survival Curve

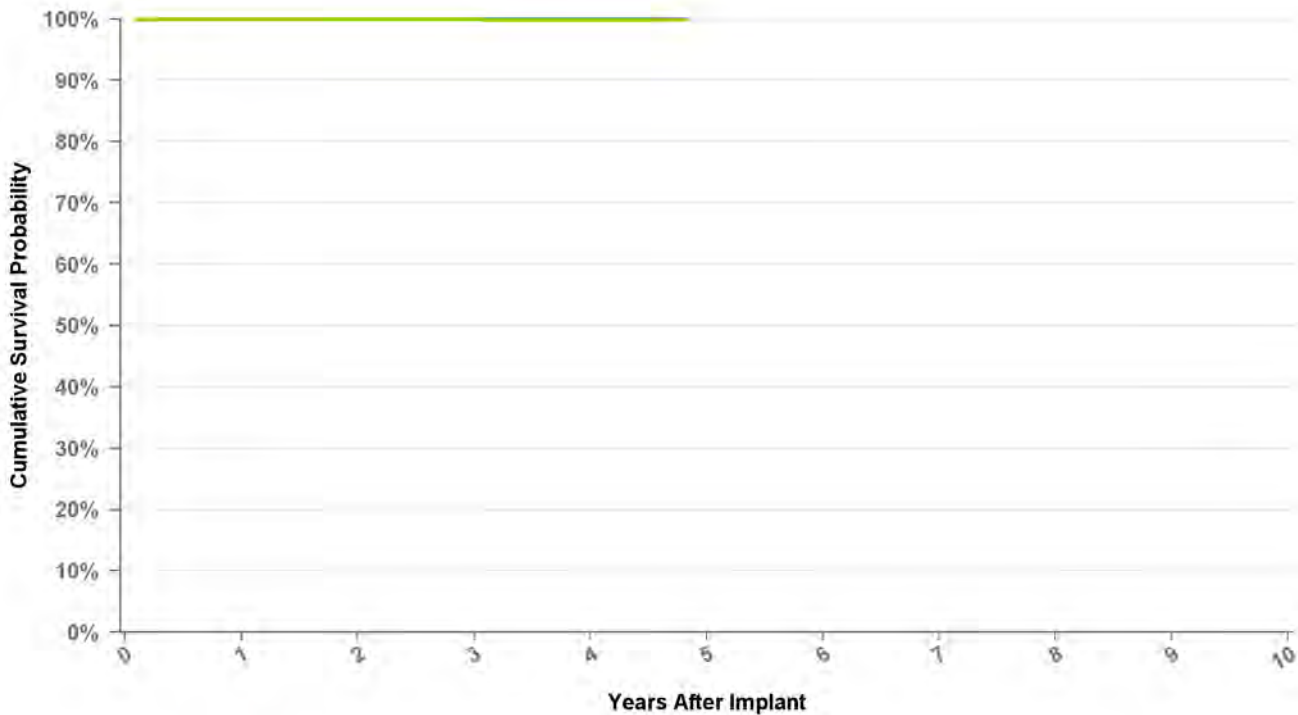

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | at 58 mo |
|------------------------------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% |
| Effective Sample Size | 40851 | 12039 | 6804 | 2770 | 161 |

Implantable Pulse Generator

ADD01 Adapta D

US Market Release Date 07/17/2006

CE Market Approval Date 09/20/2005

Registered US Implants 0

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code DDD

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

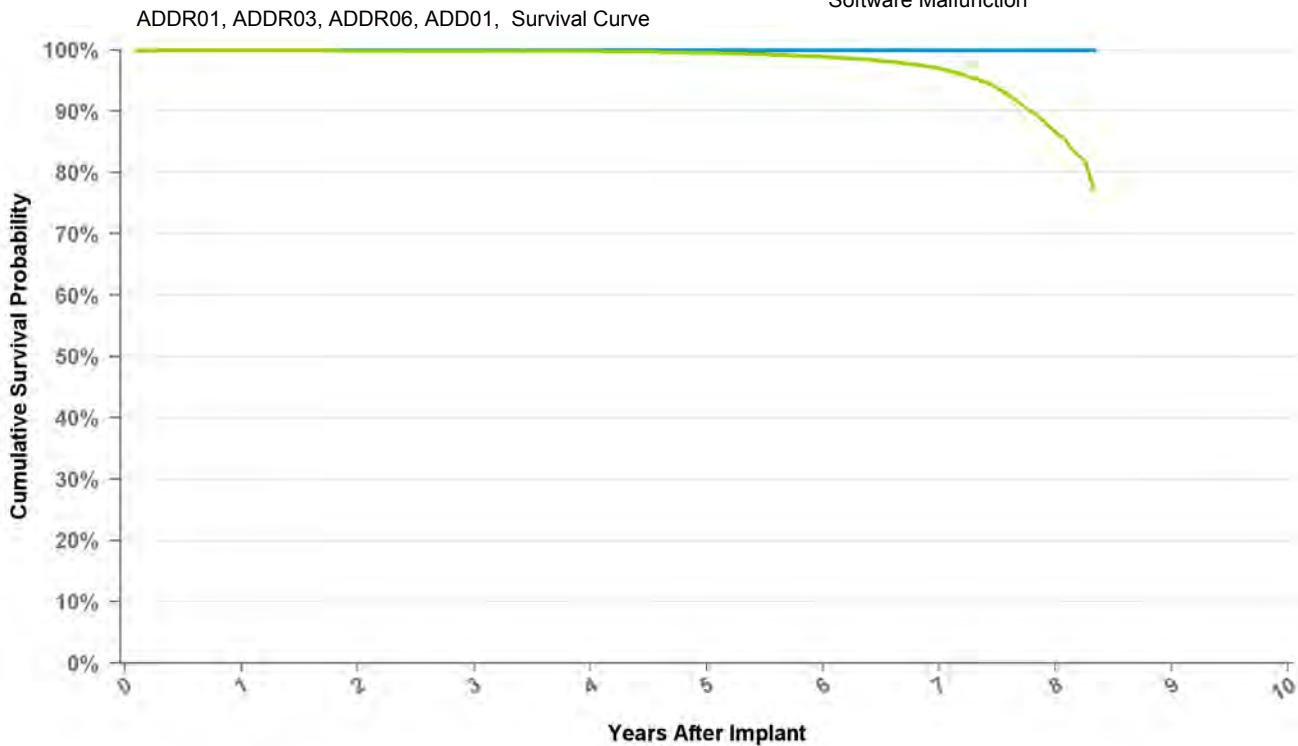

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 100 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% | 99.9% | 99.8% | 99.5% | 98.9% | 97.0% | 86.6% | 77.1% |
| Effective Sample Size | 368649 | 312517 | 254679 | 199788 | 143527 | 91801 | 46278 | 8301 | 494 |

Implantable Pulse Generator

ADDR01 Adapta DR

US Market Release Date 07/17/2006

CE Market Approval Date 09/20/2005

Registered US Implants 404,873

Estimated Active US Implants 320,831

Normal Battery Depletions (US) 2,704

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 68

Therapy Not Compromised Malfunctions 45

Battery Malfunction 0

Electrical Component 43

Electrical Interconnect 1

Other Malfunction 1

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 23

Battery Malfunction 0


Electrical Component 19

Electrical Interconnect 2

Other Malfunction 2

Poss Early Battery Depltn 0

Software Malfunction 0

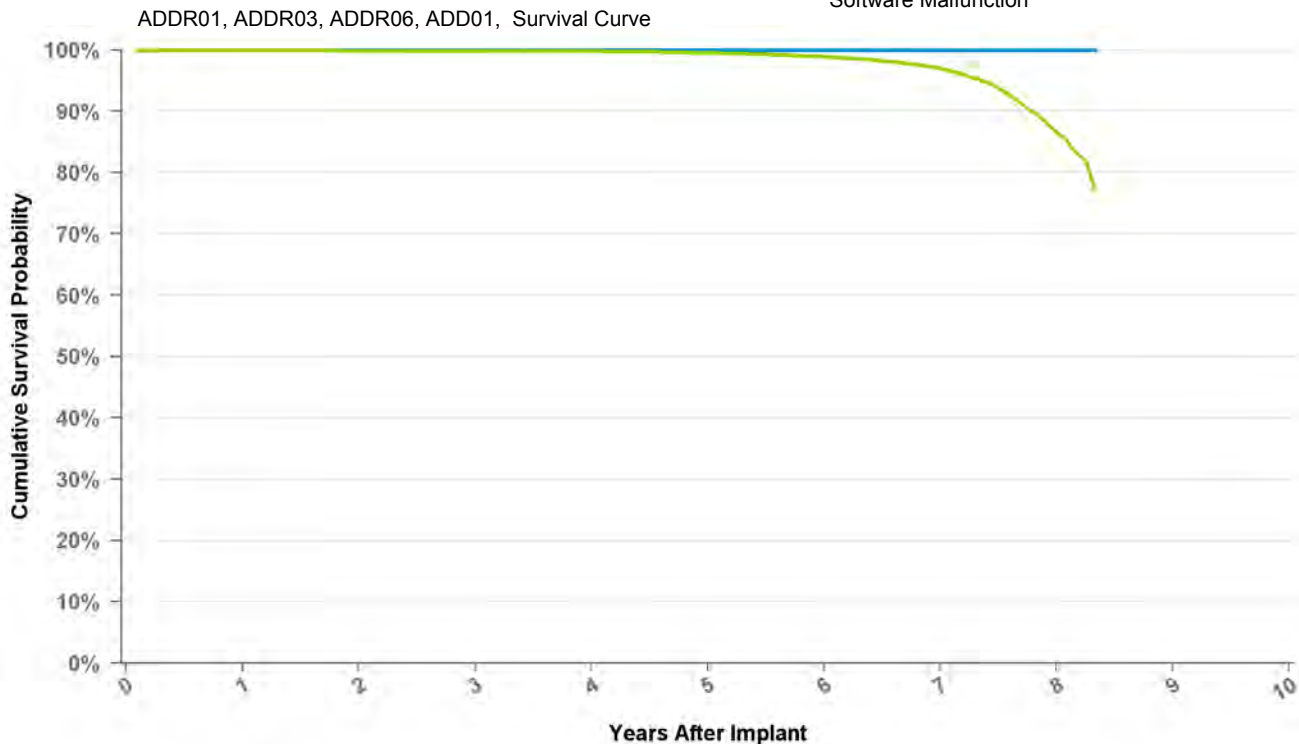

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 100 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% | 99.9% | 99.8% | 99.5% | 98.9% | 97.0% | 86.6% | 77.1% |
| Effective Sample Size | 368649 | 312517 | 254679 | 199788 | 143527 | 91801 | 46278 | 8301 | 494 |

Implantable Pulse Generator

ADDR03 Adapta DR

US Market Release Date 07/17/2006

CE Market Approval Date 09/20/2005

Registered US Implants 3,737

Estimated Active US Implants 2,761

Normal Battery Depletions (US) 59

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 2

Therapy Not Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 1

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 1

Battery Malfunction 0


Electrical Component 1

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

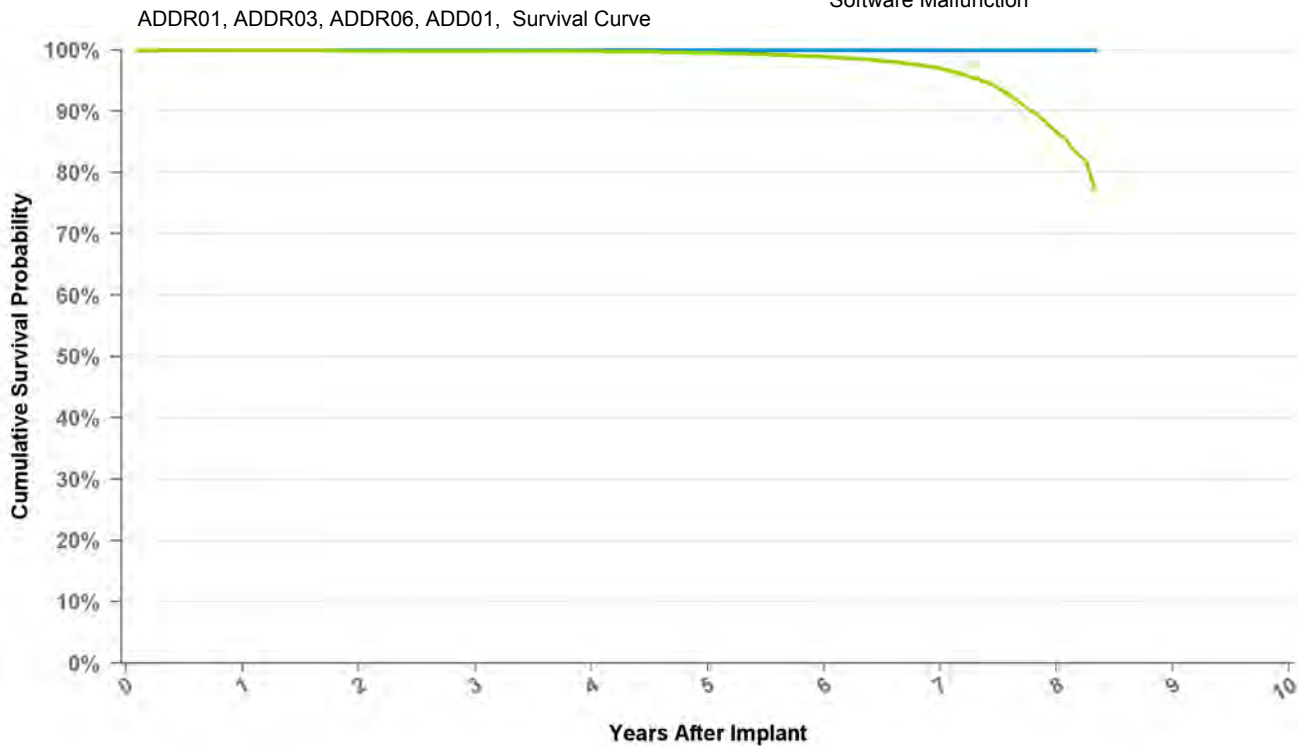

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 100 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% | 99.9% | 99.8% | 99.5% | 98.9% | 97.0% | 86.6% | 77.1% |
| Effective Sample Size | 368649 | 312517 | 254679 | 199788 | 143527 | 91801 | 46278 | 8301 | 494 |

Implantable Pulse Generator

ADDR06 Adapta DR

US Market Release Date 07/17/2006

CE Market Approval Date 09/20/2005

Registered US Implants 2,911

Estimated Active US Implants 1,842

Normal Battery Depletions (US) 94

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 1

Therapy Not Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 1

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

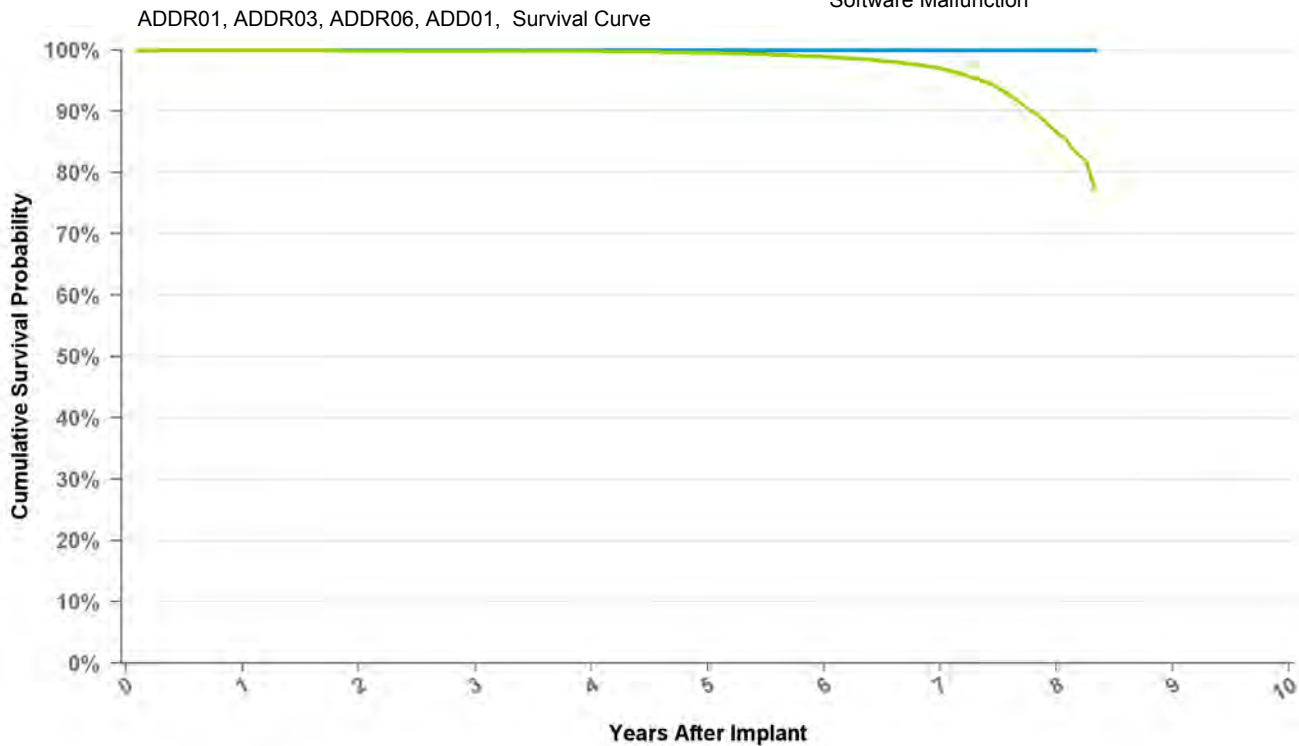

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 100 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% | 99.9% | 99.8% | 99.5% | 98.9% | 97.0% | 86.6% | 77.1% |
| Effective Sample Size | 368649 | 312517 | 254679 | 199788 | 143527 | 91801 | 46278 | 8301 | 494 |

Implantable Pulse Generator

ADDRL1 Adapta DR

US Market Release Date 07/17/2006

CE Market Approval Date 09/20/2005

Registered US Implants 106,991

Estimated Active US Implants 94,428

Normal Battery Depletions (US) 113

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 11

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 6

Electrical Interconnect 1

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0


Electrical Component 1

Electrical Interconnect 1

Other Malfunction 2

Poss Early Battery Depltn 0

Software Malfunction 0

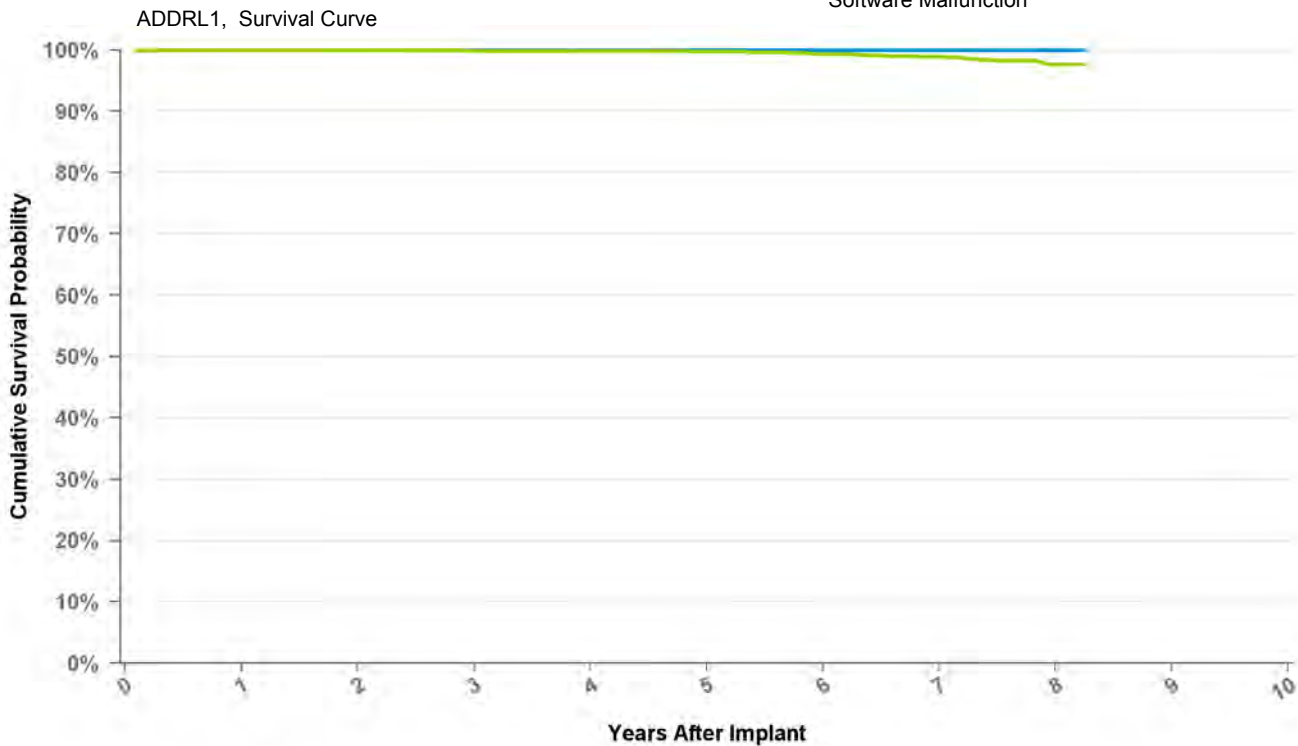

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 99 mo |
|-----------------------|--------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 99.9% | 99.8% | 99.7% | 99.3% | 98.9% | 97.7% | 97.7% |
| Effective Sample Size | 91147 | 71048 | 51522 | 35237 | 21396 | 10944 | 4307 | 607 | 180 |

Implantable Pulse Generator

ADDRS1 Adapta DR

US Market Release Date 07/17/2006

CE Market Approval Date 09/20/2005

Registered US Implants 41,421

Estimated Active US Implants 28,715

Normal Battery Depletions (US) 1,705

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 10

Therapy Not Compromised Malfunctions 6

Battery Malfunction 0

Electrical Component 5

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 1

Software Malfunction 0

Therapy Compromised Malfunctions 4

Battery Malfunction 0


Electrical Component 2

Electrical Interconnect 0

Other Malfunction 2

Poss Early Battery Depltn 0

Software Malfunction 0

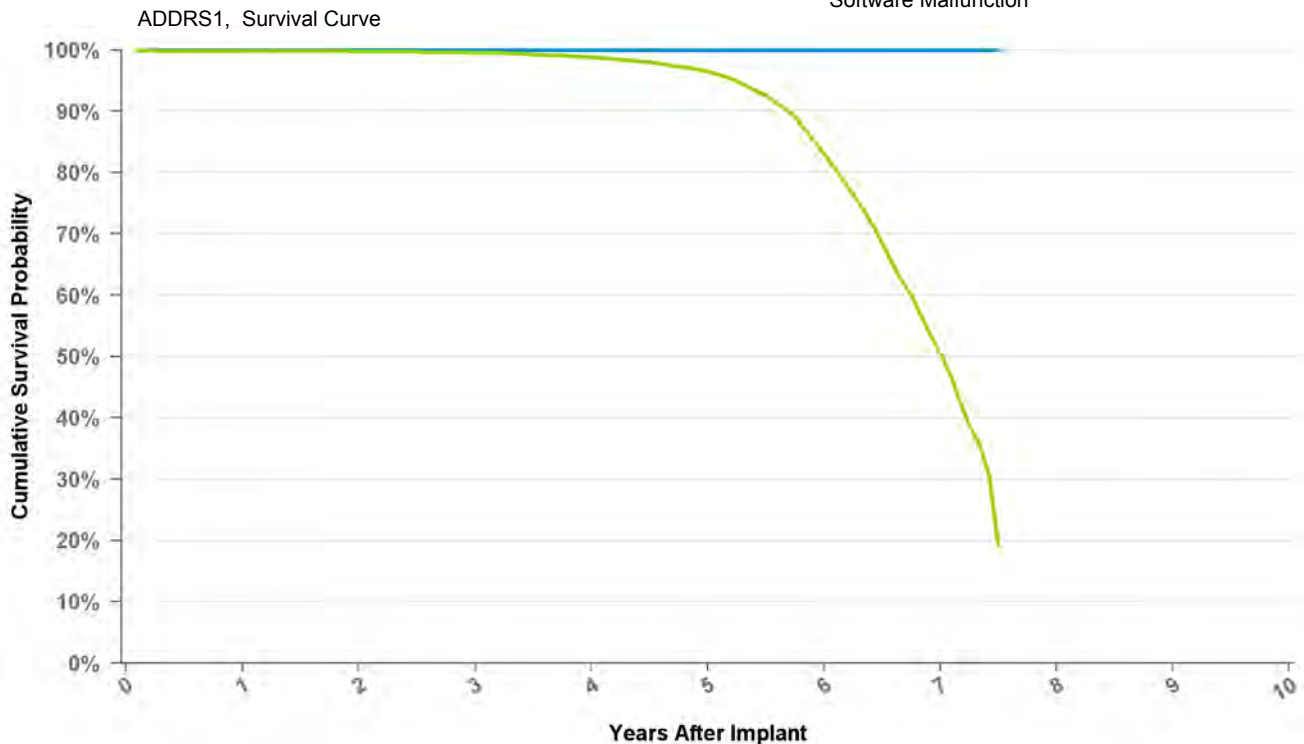

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 90 mo |
|-----------------------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.9% | 99.7% | 99.5% | 98.8% | 96.5% | 83.2% | 50.6% | 19.1% |
| Effective Sample Size | 35370 | 28688 | 22416 | 16720 | 11179 | 5692 | 1224 | 107 |

Implantable Pulse Generator

ADSR01 Adapta SR

| | |
|---------------------------------------|------------|
| US Market Release Date | 07/17/2006 |
| CE Market Approval Date | 09/20/2005 |
| Registered US Implants | 78,252 |
| Estimated Active US Implants | 54,282 |
| Normal Battery Depletions (US) | 707 |
| NBG Code | SSIR |
| Max Delivered Energy | N/A |

| | |
|---|----|
| Total Malfunctions (US) | 11 |
| Therapy Not Compromised Malfunctions | 6 |
| Battery Malfunction | 0 |
| Electrical Component | 4 |
| Electrical Interconnect | 1 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 5 |
| Battery Malfunction | 0 |
| Electrical Component | 4 |
| Electrical Interconnect | 1 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

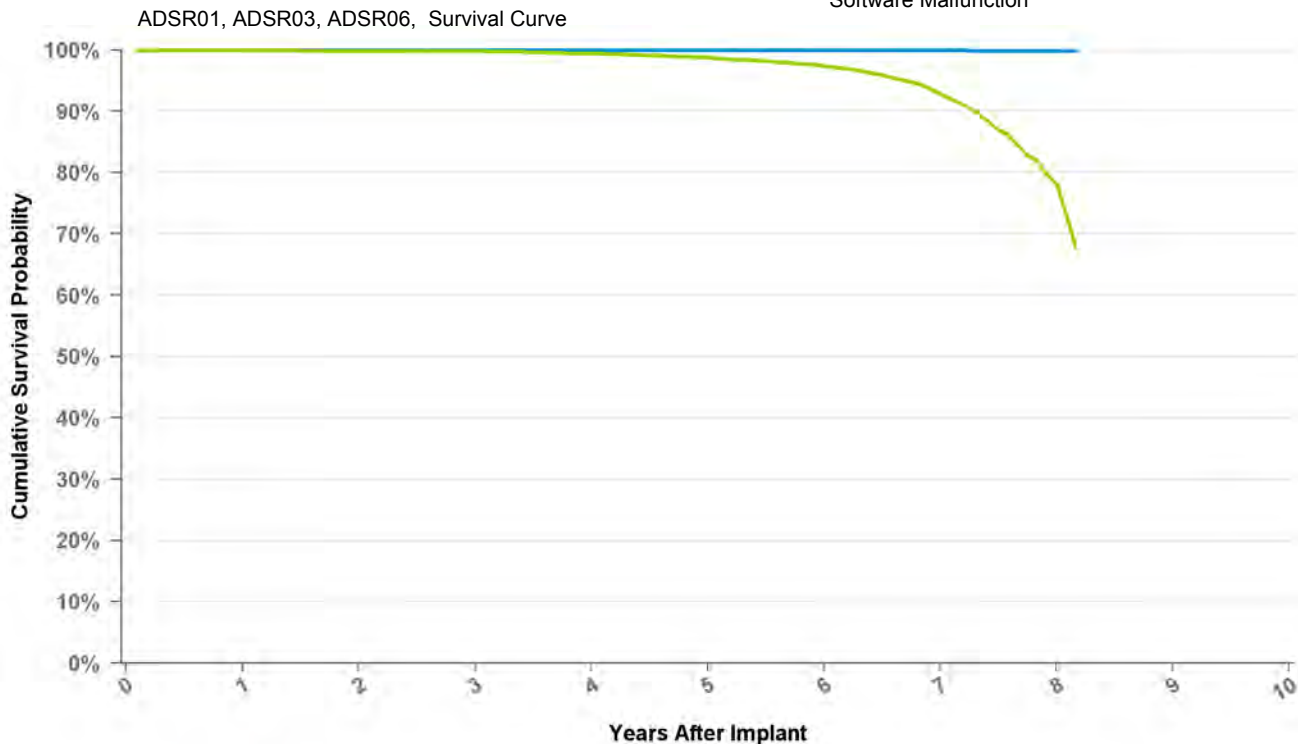

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 98 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 100.0% | 99.9% | 99.8% | 99.4% | 98.8% | 97.4% | 92.8% | 78.2% | 67.7% |
| Effective Sample Size | 71746 | 56696 | 43313 | 31904 | 22407 | 14042 | 6673 | 859 | 251 |

Implantable Pulse Generator

ADSR03 Adapta SR

US Market Release Date 07/17/2006

CE Market Approval Date 09/20/2005

Registered US Implants 1,808

Estimated Active US Implants 1,149

Normal Battery Depletions (US) 17

NBG Code SSIR

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

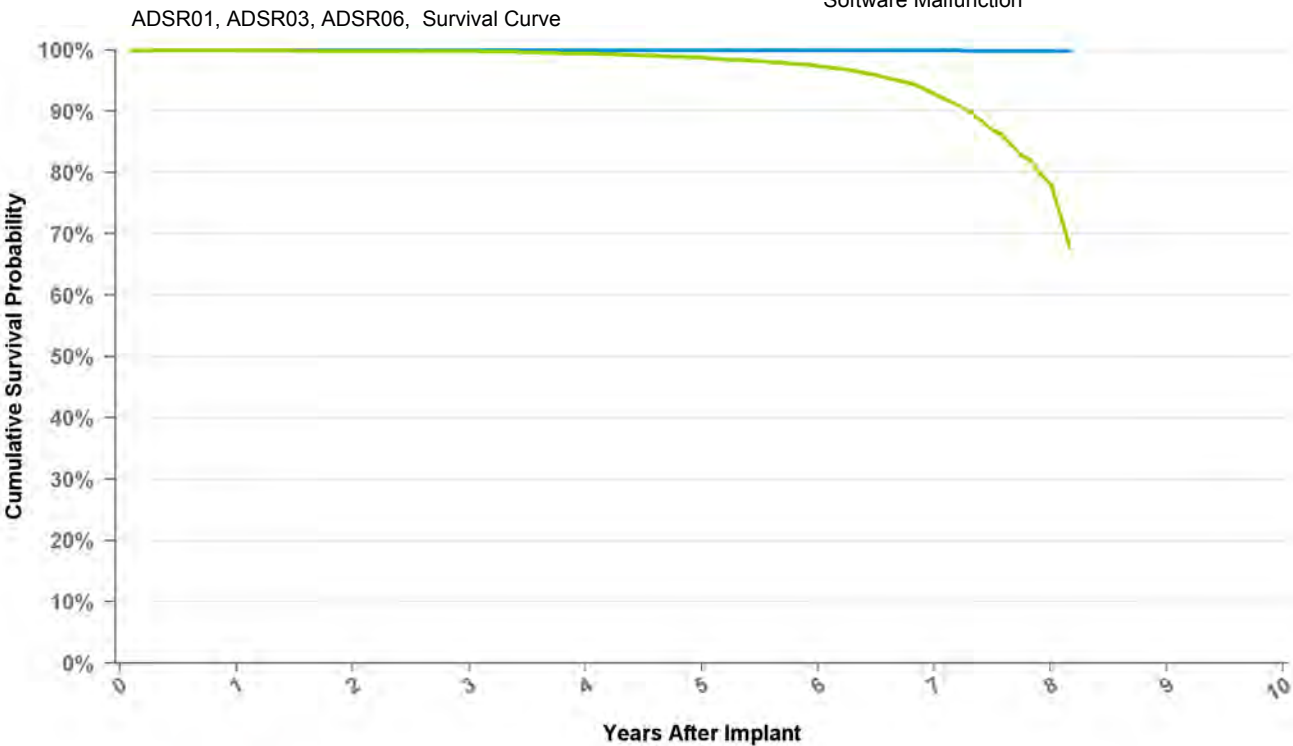

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 98 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 100.0% | 99.9% | 99.8% | 99.4% | 98.8% | 97.4% | 92.8% | 78.2% | 67.7% |
| Effective Sample Size | 71746 | 56696 | 43313 | 31904 | 22407 | 14042 | 6673 | 859 | 251 |

Implantable Pulse Generator

ADSR06 Adapta SR

US Market Release Date 07/17/2006

CE Market Approval Date 09/20/2005

Registered US Implants 2,469

Estimated Active US Implants 1,416

Normal Battery Depletions (US) 69

NBG Code SSIR

Max Delivered Energy N/A

Total Malfunctions (US) 2

Therapy Not Compromised Malfunctions 2

Battery Malfunction 0

Electrical Component 2

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

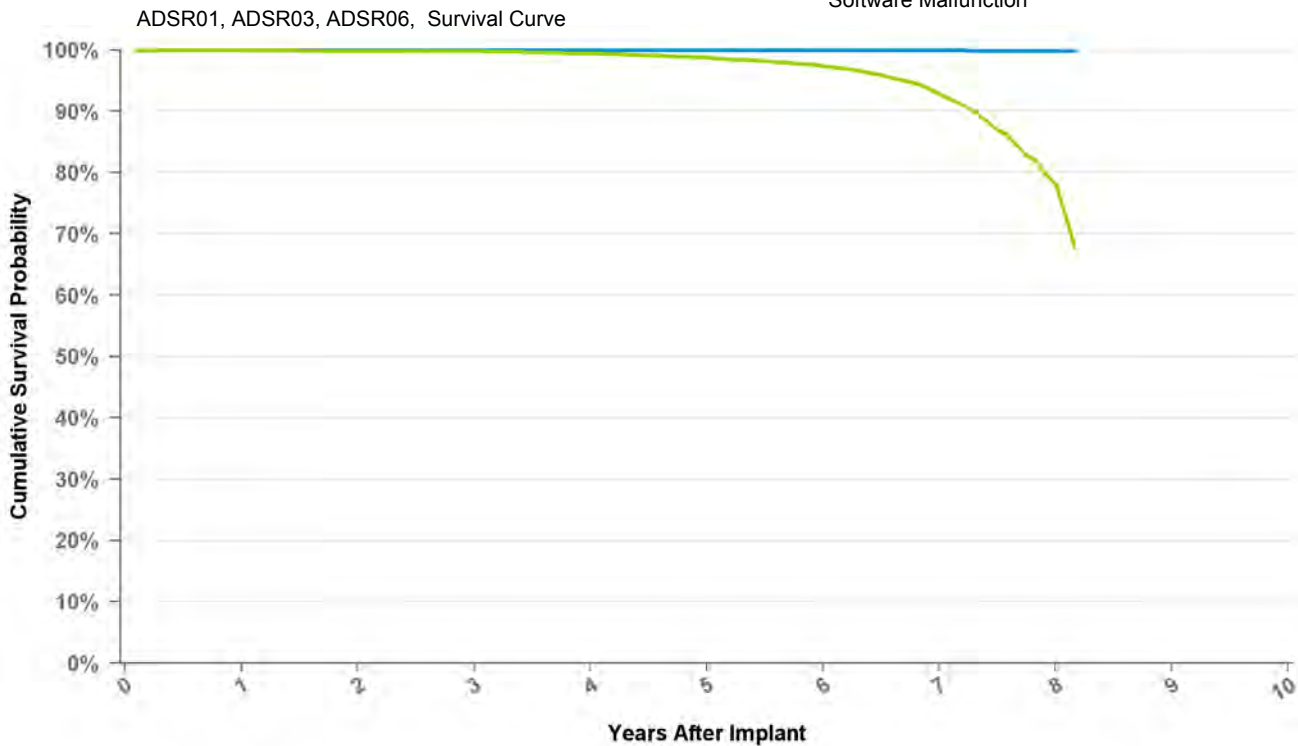

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 98 mo |
|-----------------------|--------|--------|--------|--------|--------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% |
| Including NBD | 100.0% | 99.9% | 99.8% | 99.4% | 98.8% | 97.4% | 92.8% | 78.2% | 67.7% |
| Effective Sample Size | 71746 | 56696 | 43313 | 31904 | 22407 | 14042 | 6673 | 859 | 251 |

Implantable Pulse Generator

ADVDD01 Adapta VDD

| | |
|---------------------------------------|------------|
| US Market Release Date | 07/17/2006 |
| CE Market Approval Date | 09/20/2005 |
| Registered US Implants | 1,014 |
| Estimated Active US Implants | 657 |
| Normal Battery Depletions (US) | 31 |
| NBG Code | VDD |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

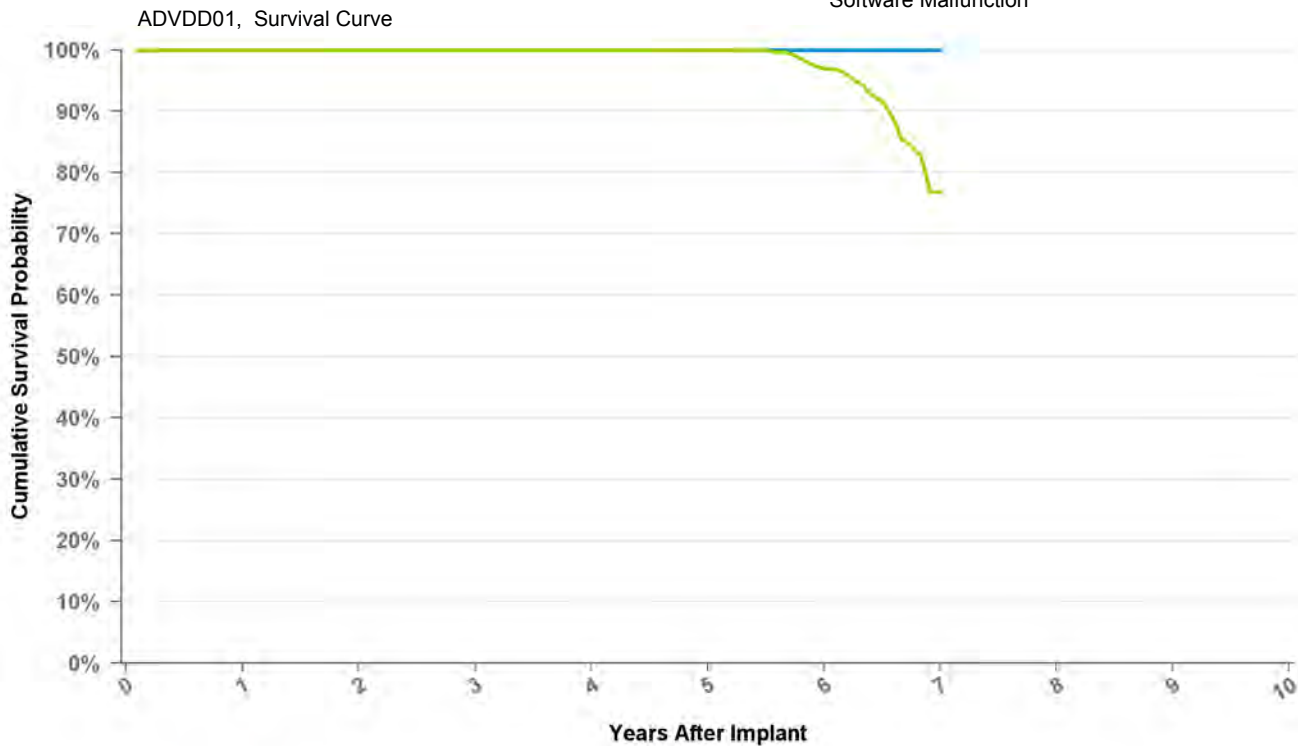

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 84 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 96.9% | 76.8% |
| Effective Sample Size | 1403 | 1172 | 951 | 776 | 598 | 383 | 110 |

Implantable Pulse Generator

E1DR01 EnPulse DR

US Market Release Date 12/18/2003

CE Market Approval Date

Registered US Implants 6,846

Estimated Active US Implants 739

Normal Battery Depletions (US) 1,688

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 1

Therapy Not Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 1

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

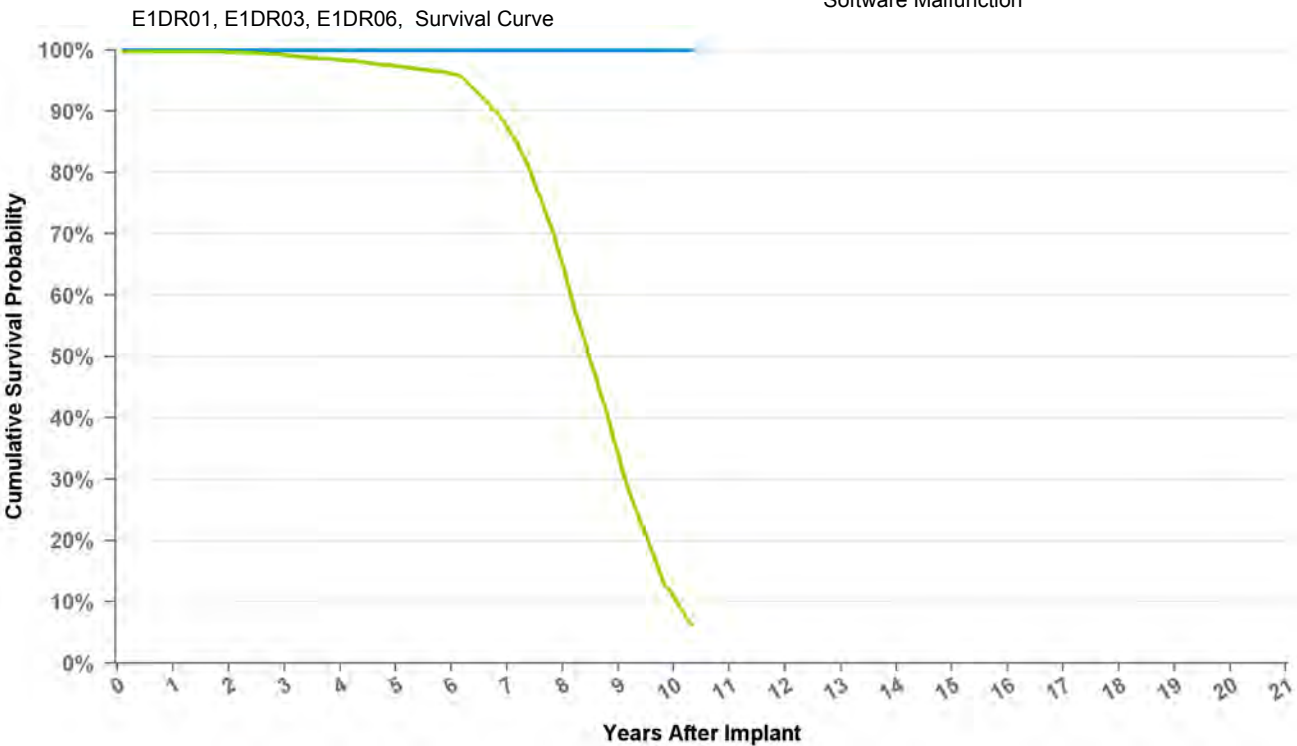

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 124 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.7% | 99.6% | 99.2% | 98.4% | 97.4% | 96.1% | 87.5% | 65.1% | 34.2% | 10.8% | 6.3% |
| Effective Sample Size | 6213 | 5761 | 5313 | 4845 | 4415 | 3985 | 3316 | 2224 | 1025 | 251 | 120 |

Implantable Pulse Generator

E1DR03 EnPulse DR

US Market Release Date 12/18/2003

CE Market Approval Date

Registered US Implants 0

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

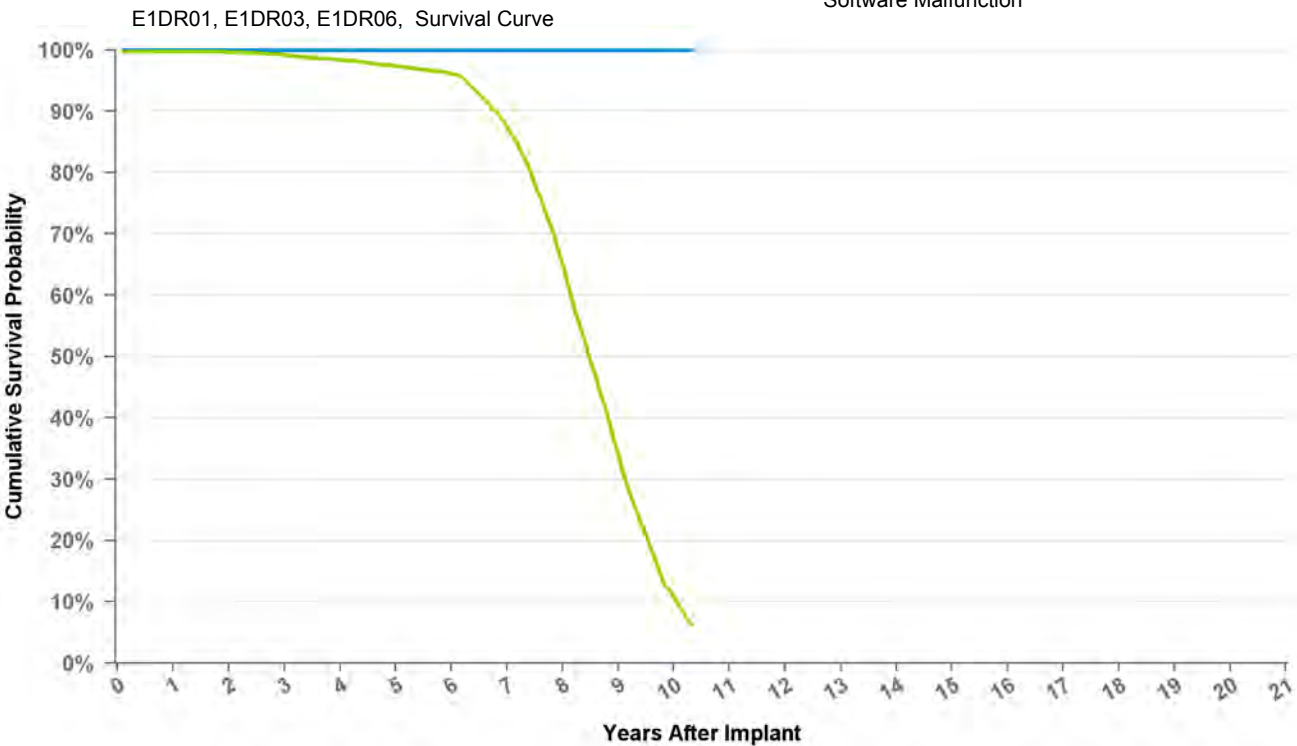

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 124 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.7% | 99.6% | 99.2% | 98.4% | 97.4% | 96.1% | 87.5% | 65.1% | 34.2% | 10.8% | 6.3% |
| Effective Sample Size | 6213 | 5761 | 5313 | 4845 | 4415 | 3985 | 3316 | 2224 | 1025 | 251 | 120 |

Implantable Pulse Generator

E1DR06 EnPulse DR

US Market Release Date 12/18/2003

CE Market Approval Date

Registered US Implants 0

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code DDDR

Max Delivered Energy

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

E1DR01, E1DR03, E1DR06, Survival Curve

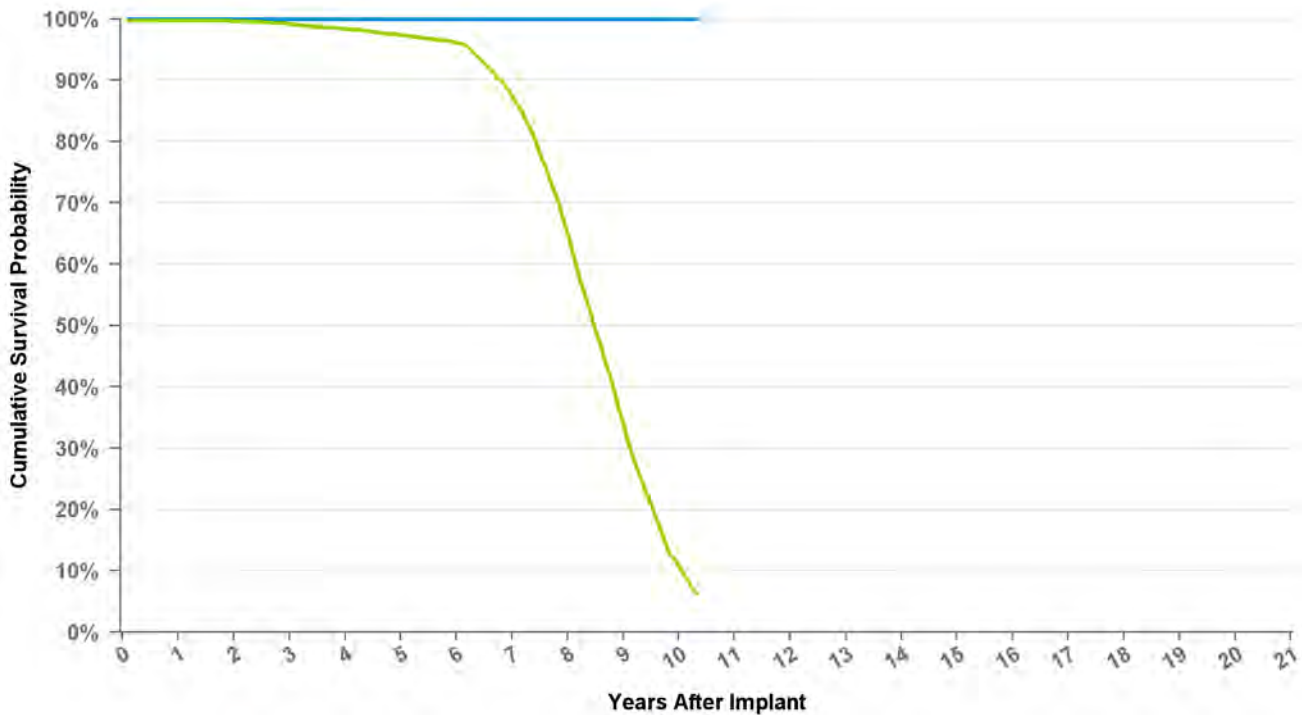

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 124 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.7% | 99.6% | 99.2% | 98.4% | 97.4% | 96.1% | 87.5% | 65.1% | 34.2% | 10.8% | 6.3% |
| Effective Sample Size | 6213 | 5761 | 5313 | 4845 | 4415 | 3985 | 3316 | 2224 | 1025 | 251 | 120 |

Implantable Pulse Generator

E1DR21 EnPulse DR

US Market Release Date 12/18/2003

CE Market Approval Date

Registered US Implants 1,856

Estimated Active US Implants 140

Normal Battery Depletions (US) 378

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

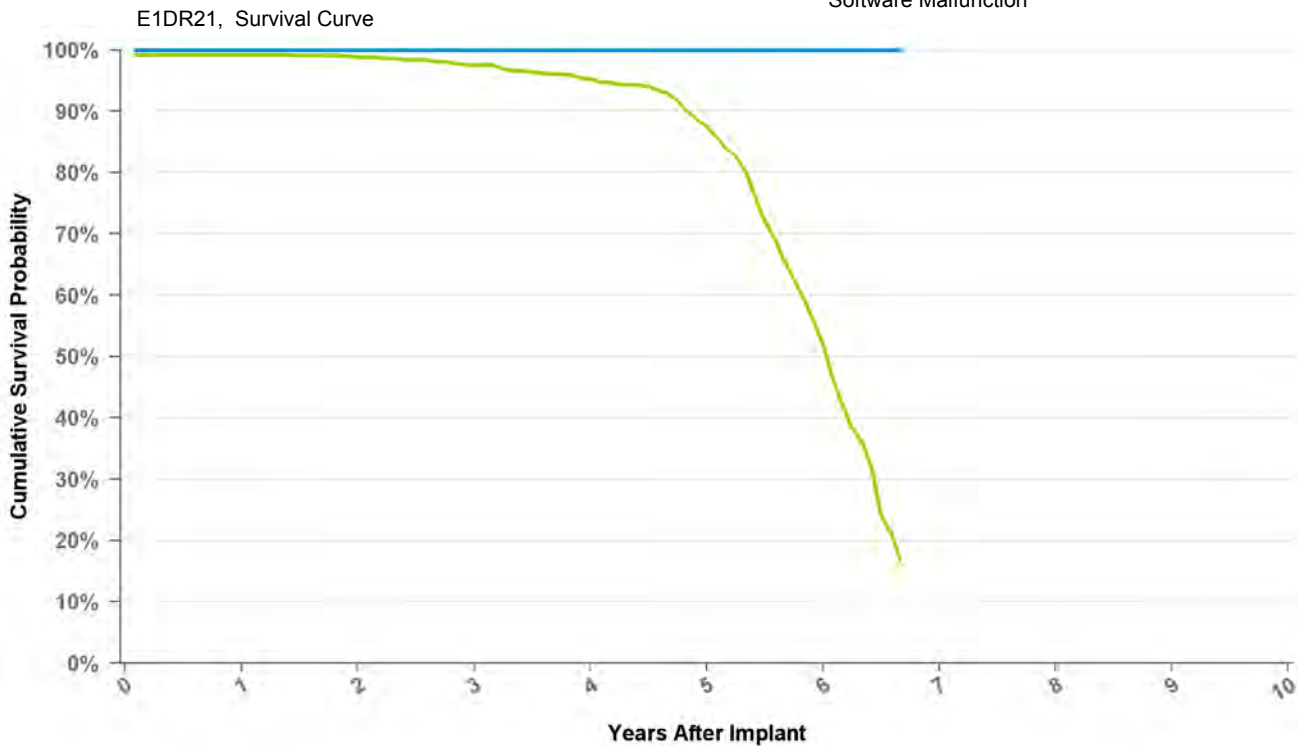

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 80 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.2% | 98.8% | 97.5% | 95.3% | 87.5% | 52.1% | 16.9% |
| Effective Sample Size | 1628 | 1476 | 1317 | 1155 | 945 | 449 | 117 |

Implantable Pulse Generator

E2D01

EnPulse 2

US Market Release Date 02/20/2004

CE Market Approval Date 09/08/2003

Registered US Implants 0

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code DDD

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

E2D01, E2D03, E2DR01, E2DR03, E2DR06, Survival Curve

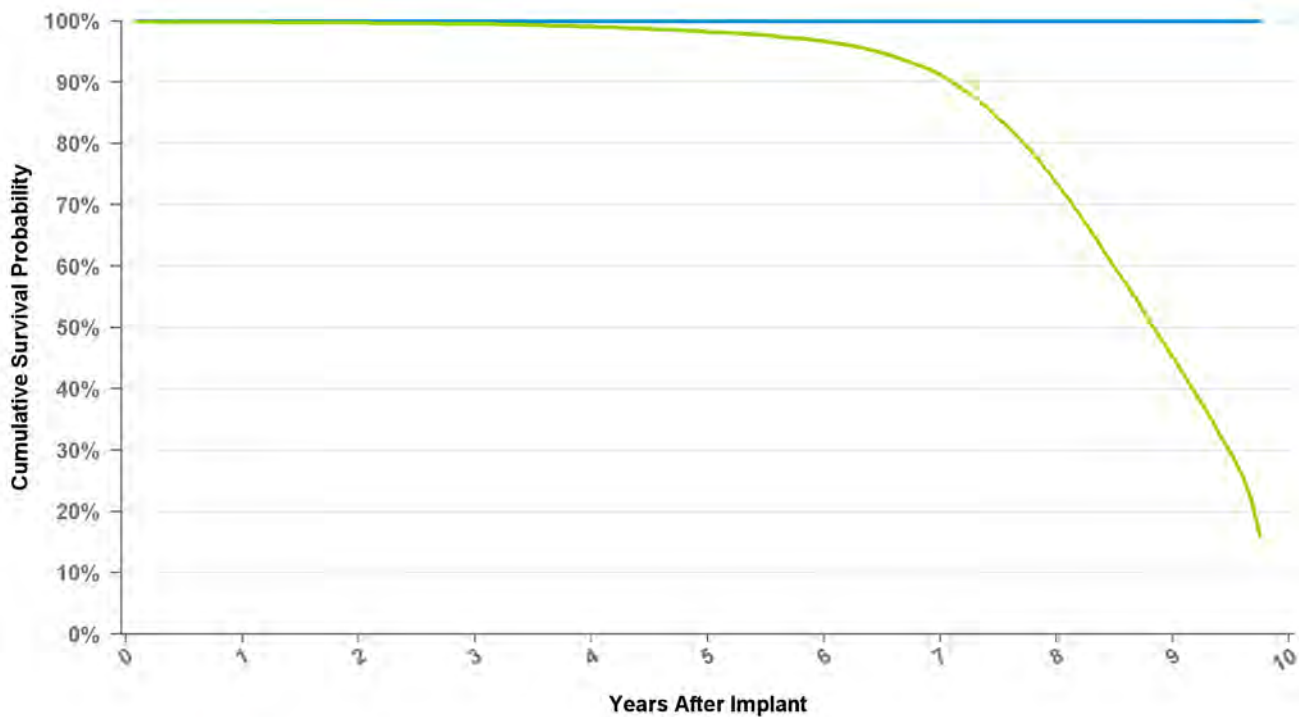

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 117 mo |
|-----------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.8% | 99.7% | 99.5% | 99.1% | 98.2% | 96.7% | 91.2% | 73.6% | 45.2% | 15.9% |
| Effective Sample Size | 94840 | 87664 | 80636 | 74009 | 67511 | 61334 | 54190 | 40500 | 14274 | 873 |

Implantable Pulse Generator


E2D03

EnPulse 2

| | |
|---------------------------------------|------------|
| US Market Release Date | 02/20/2004 |
| CE Market Approval Date | 09/08/2003 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDD |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

E2D01, E2D03, E2DR01, E2DR03, E2DR06, Survival Curve

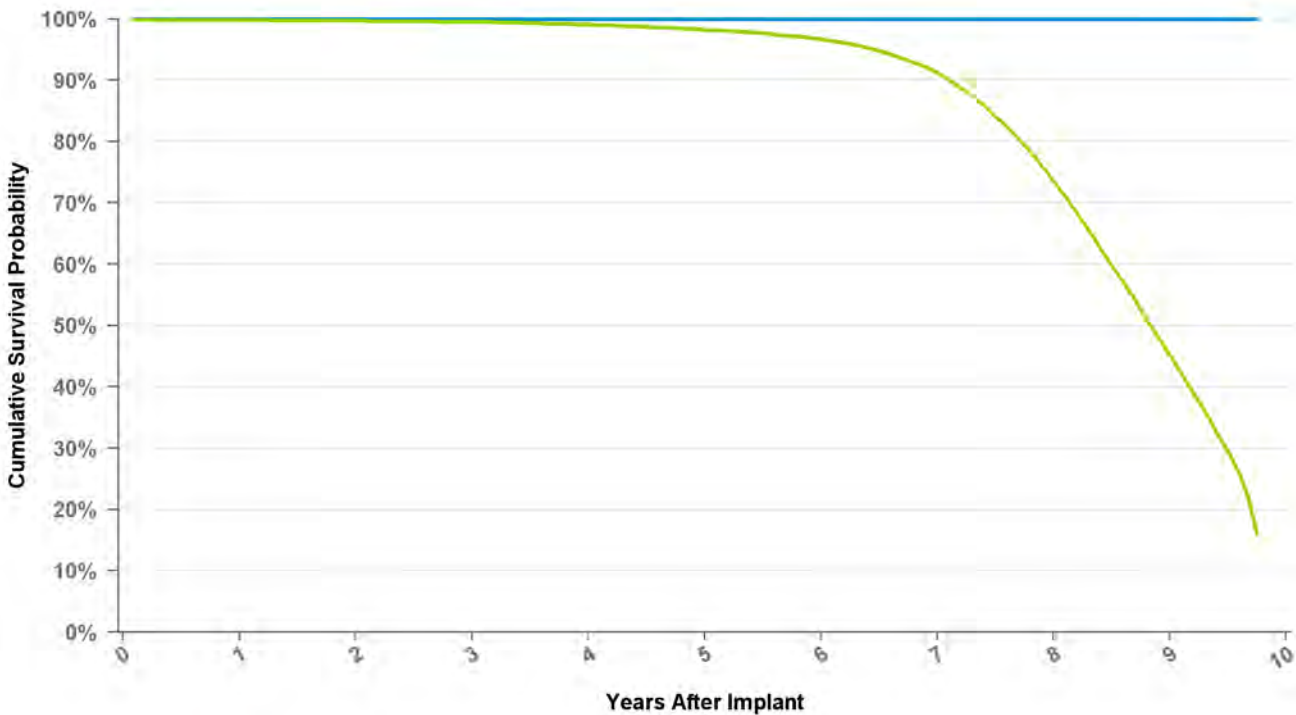

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 117 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.8% | 99.7% | 99.5% | 99.1% | 98.2% | 96.7% | 91.2% | 73.6% | 45.2% | 15.9% |
| Effective Sample Size | 94840 | 87664 | 80636 | 74009 | 67511 | 61334 | 54190 | 40500 | 14274 | 873 |


Implantable Pulse Generator

E2DR01 EnPulse 2 DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 02/20/2004 |
| CE Market Approval Date | 09/08/2003 |
| Registered US Implants | 97,093 |
| Estimated Active US Implants | 22,819 |
| Normal Battery Depletions (US) | 17,162 |
| NBG Code | DDDR |
| Max Delivered Energy | N/A |

| | |
|---|----|
| Total Malfunctions (US) | 27 |
| Therapy Not Compromised Malfunctions | 20 |
| Battery Malfunction | 0 |
| Electrical Component | 18 |
| Electrical Interconnect | 0 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 7 |
| Battery Malfunction | 1 |
| Electrical Component | 3 |
| Electrical Interconnect | 3 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

E2D01, E2D03, E2DR01, E2DR03, E2DR06, Survival Curve

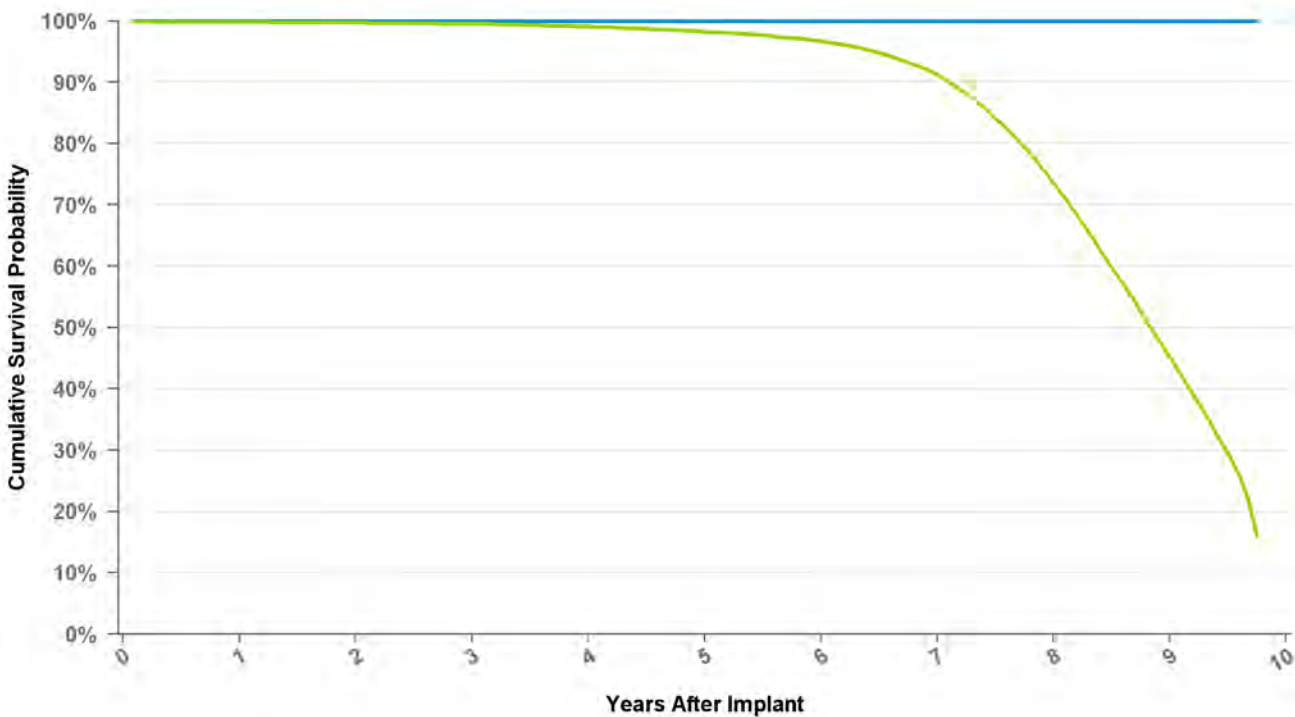

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 117 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.8% | 99.7% | 99.5% | 99.1% | 98.2% | 96.7% | 91.2% | 73.6% | 45.2% | 15.9% |
| Effective Sample Size | 94840 | 87664 | 80636 | 74009 | 67511 | 61334 | 54190 | 40500 | 14274 | 873 |

Implantable Pulse Generator

E2DR03 EnPulse 2 DR

US Market Release Date 02/20/2004

CE Market Approval Date 09/08/2003

Registered US Implants 2,050

Estimated Active US Implants 500

Normal Battery Depletions (US) 359

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

E2D01, E2D03, E2DR01, E2DR03, E2DR06, Survival Curve

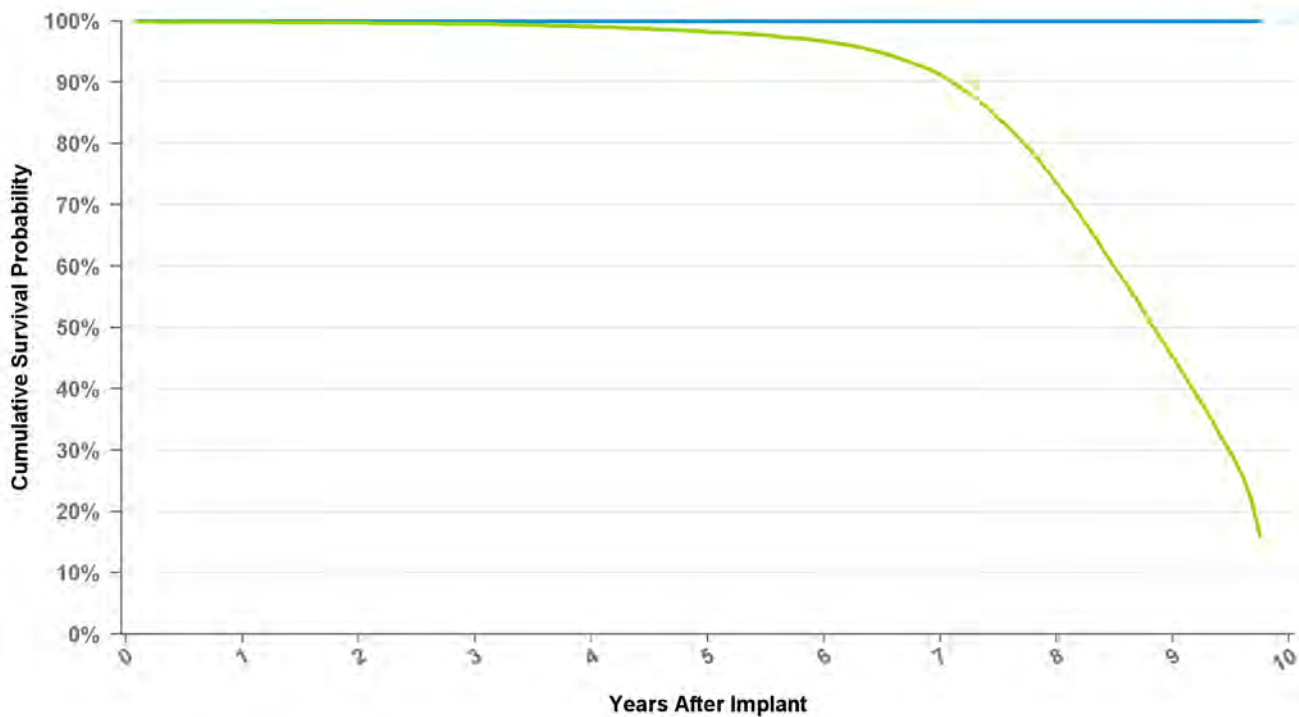

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 117 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.8% | 99.7% | 99.5% | 99.1% | 98.2% | 96.7% | 91.2% | 73.6% | 45.2% | 15.9% |
| Effective Sample Size | 94840 | 87664 | 80636 | 74009 | 67511 | 61334 | 54190 | 40500 | 14274 | 873 |

Implantable Pulse Generator

E2DR06 EnPulse 2 DR

US Market Release Date 02/20/2004

CE Market Approval Date 09/08/2003

Registered US Implants 1,626

Estimated Active US Implants 292

Normal Battery Depletions (US) 267

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 2

Therapy Not Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 1

Software Malfunction 0

Therapy Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 1

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

E2D01, E2D03, E2DR01, E2DR03, E2DR06, Survival Curve

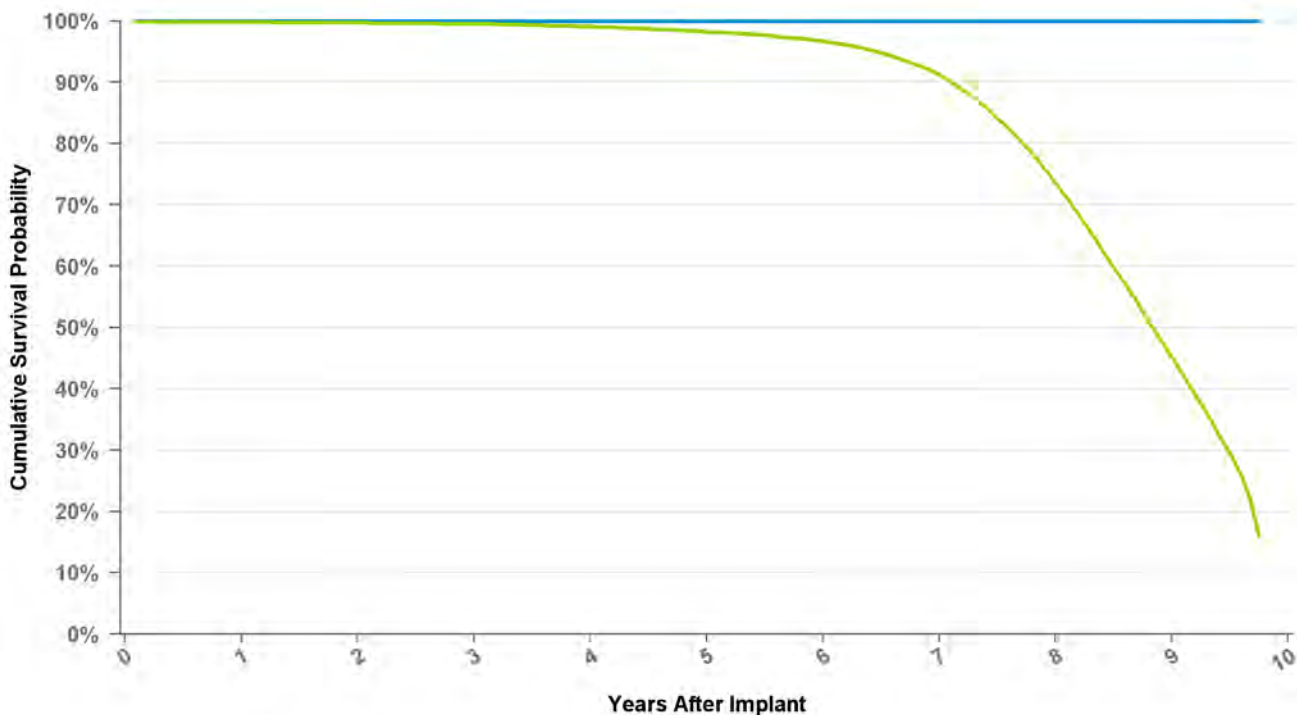

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 117 mo |
|-----------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.8% | 99.7% | 99.5% | 99.1% | 98.2% | 96.7% | 91.2% | 73.6% | 45.2% | 15.9% |
| Effective Sample Size | 94840 | 87664 | 80636 | 74009 | 67511 | 61334 | 54190 | 40500 | 14274 | 873 |

Implantable Pulse Generator

E2DR21 EnPulse 2 DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 02/20/2004 |
| CE Market Approval Date | 09/08/2003 |
| Registered US Implants | 12,199 |
| Estimated Active US Implants | 1,544 |
| Normal Battery Depletions (US) | 2,288 |
| NBG Code | DDDR |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 1 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

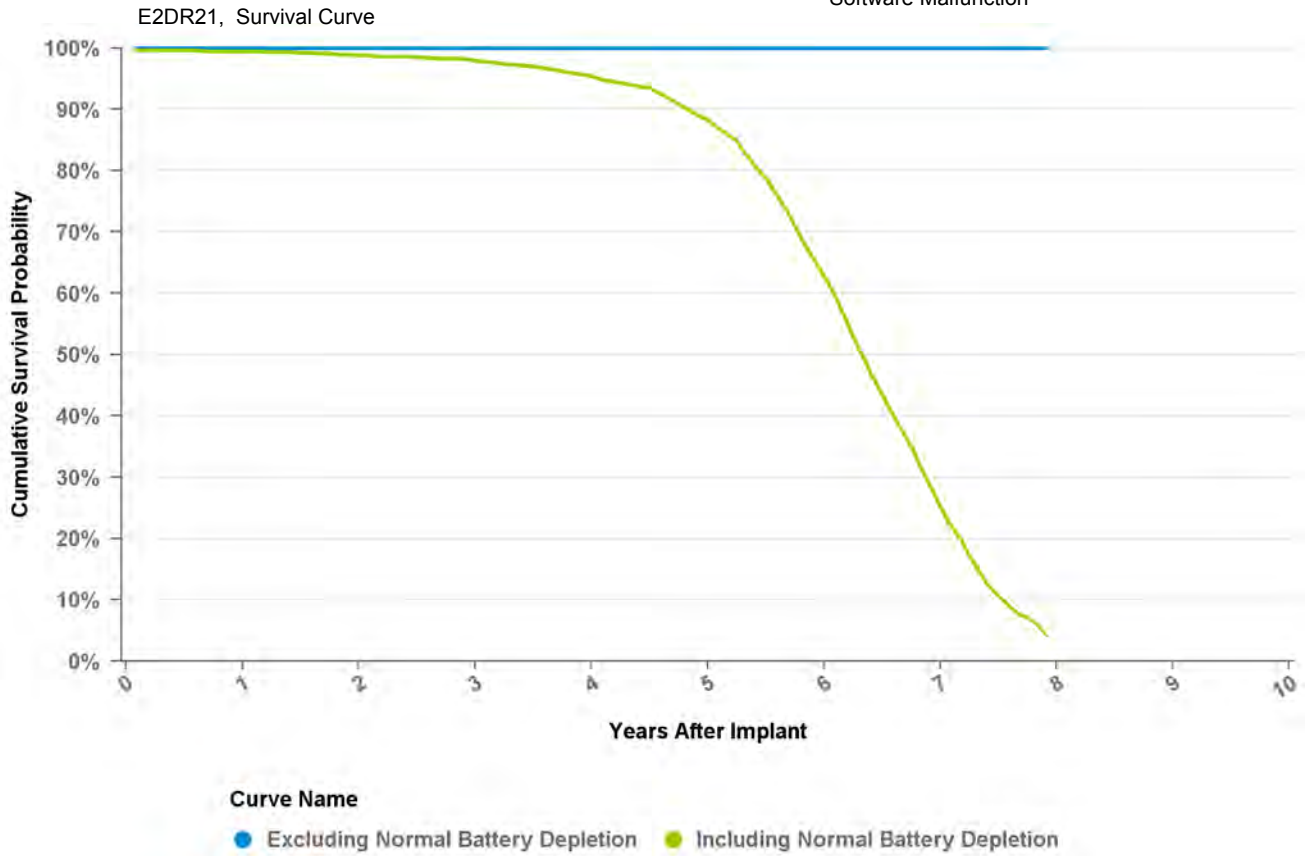


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 95 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.4% | 98.8% | 97.9% | 95.4% | 88.3% | 62.9% | 25.3% | 4.2% |
| Effective Sample Size | 10835 | 9715 | 8725 | 7611 | 6295 | 3860 | 1187 | 111 |

Implantable Pulse Generator

E2DR31 EnPulse 2 DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 02/20/2004 |
| CE Market Approval Date | 09/08/2003 |
| Registered US Implants | 587 |
| Estimated Active US Implants | 343 |
| Normal Battery Depletions (US) | 31 |
| NBG Code | DDDR |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

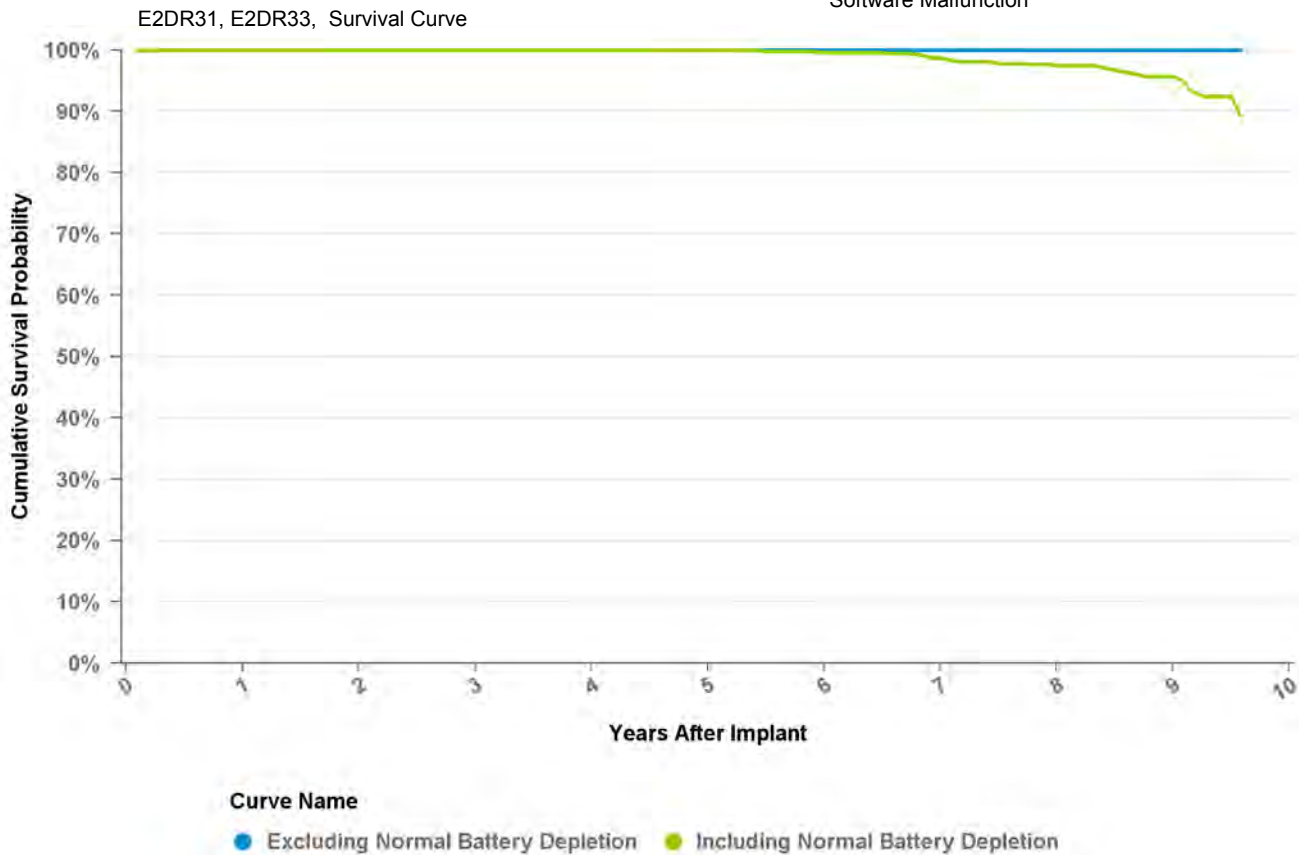


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 115 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.6% | 98.7% | 97.4% | 95.7% | 89.3% |
| Effective Sample Size | 1354 | 1276 | 1203 | 1129 | 1059 | 994 | 897 | 816 | 416 | 119 |

Implantable Pulse Generator

E2DR33 EnPulse 2 DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 02/20/2004 |
| CE Market Approval Date | 09/08/2003 |
| Registered US Implants | 5 |
| Estimated Active US Implants | 5 |
| Normal Battery Depletions (US) | 1 |
| NBG Code | DDDR |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

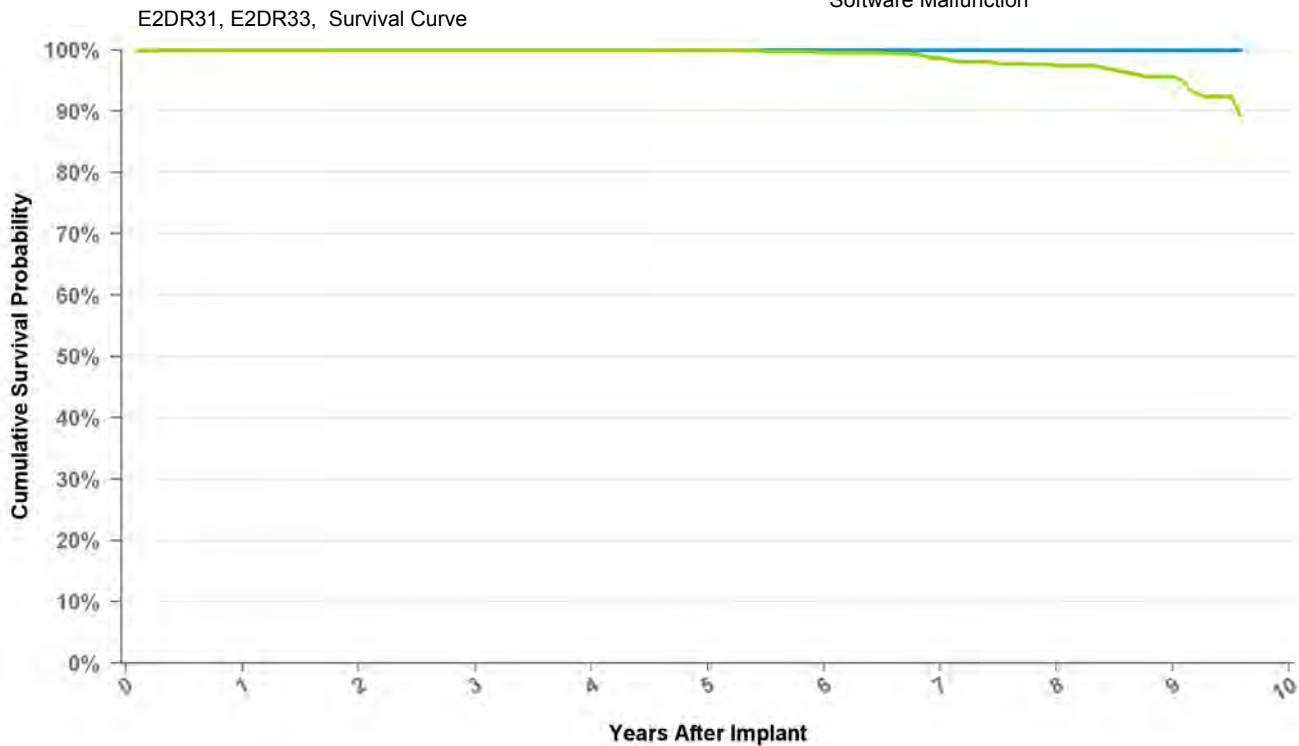

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 115 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.6% | 98.7% | 97.4% | 95.7% | 89.3% |
| Effective Sample Size | 1354 | 1276 | 1203 | 1129 | 1059 | 994 | 897 | 816 | 416 | 119 |

Implantable Pulse Generator

E2SR01 EnPulse 2 SR

US Market Release Date 12/18/2003

CE Market Approval Date 09/08/2003

Registered US Implants 22,528

Estimated Active US Implants 3,557

Normal Battery Depletions (US) 2,638

NBG Code SSIR

Max Delivered Energy N/A

Total Malfunctions (US) 4

Therapy Not Compromised Malfunctions 3

Battery Malfunction 0

Electrical Component 2

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 1

Software Malfunction 0

Therapy Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 1

Poss Early Battery Depltn 0

Software Malfunction 0

E2SR01, E2SR03, E2SR06, Survival Curve

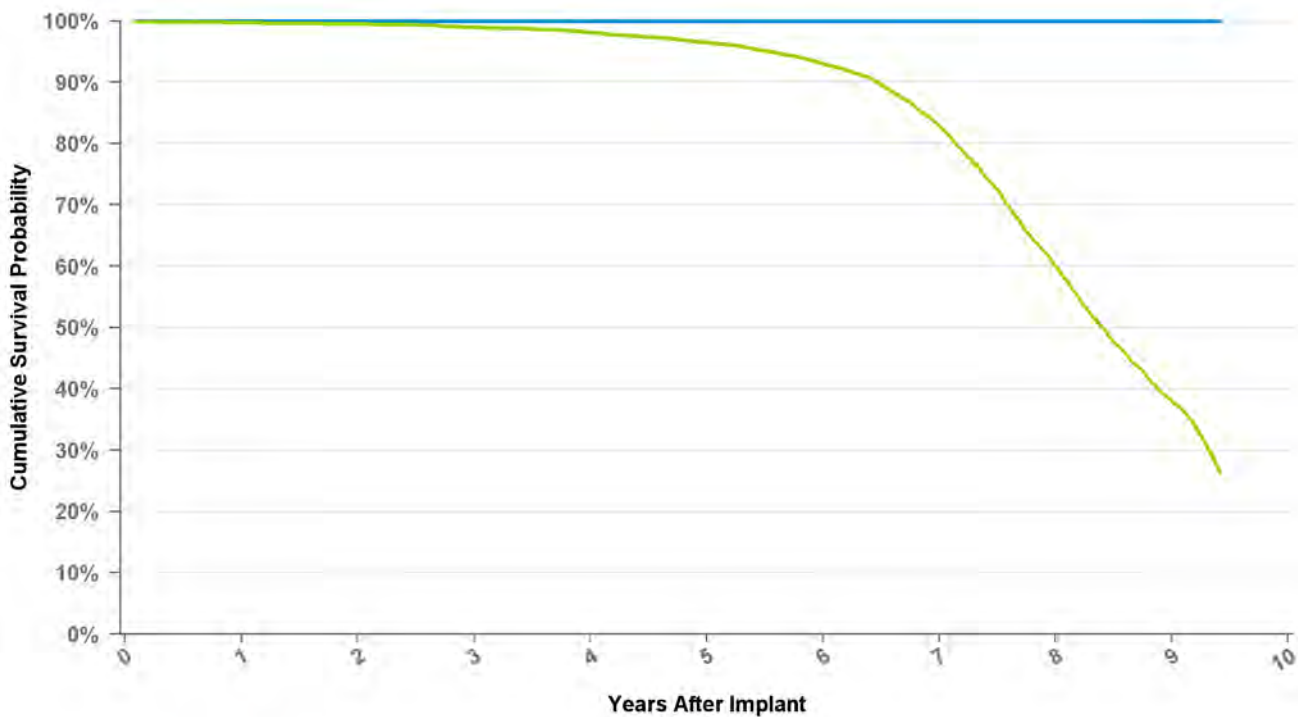

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 113 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.7% | 99.5% | 99.0% | 98.1% | 96.5% | 93.0% | 82.8% | 60.1% | 37.9% | 26.4% |
| Effective Sample Size | 22600 | 19616 | 17124 | 14986 | 12871 | 11059 | 8978 | 5680 | 1332 | 200 |

Implantable Pulse Generator

E2SR03 EnPulse 2 SR

| | |
|---------------------------------------|------------|
| US Market Release Date | 12/18/2003 |
| CE Market Approval Date | 09/08/2003 |
| Registered US Implants | 1,098 |
| Estimated Active US Implants | 185 |
| Normal Battery Depletions (US) | 130 |
| NBG Code | SSIR |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

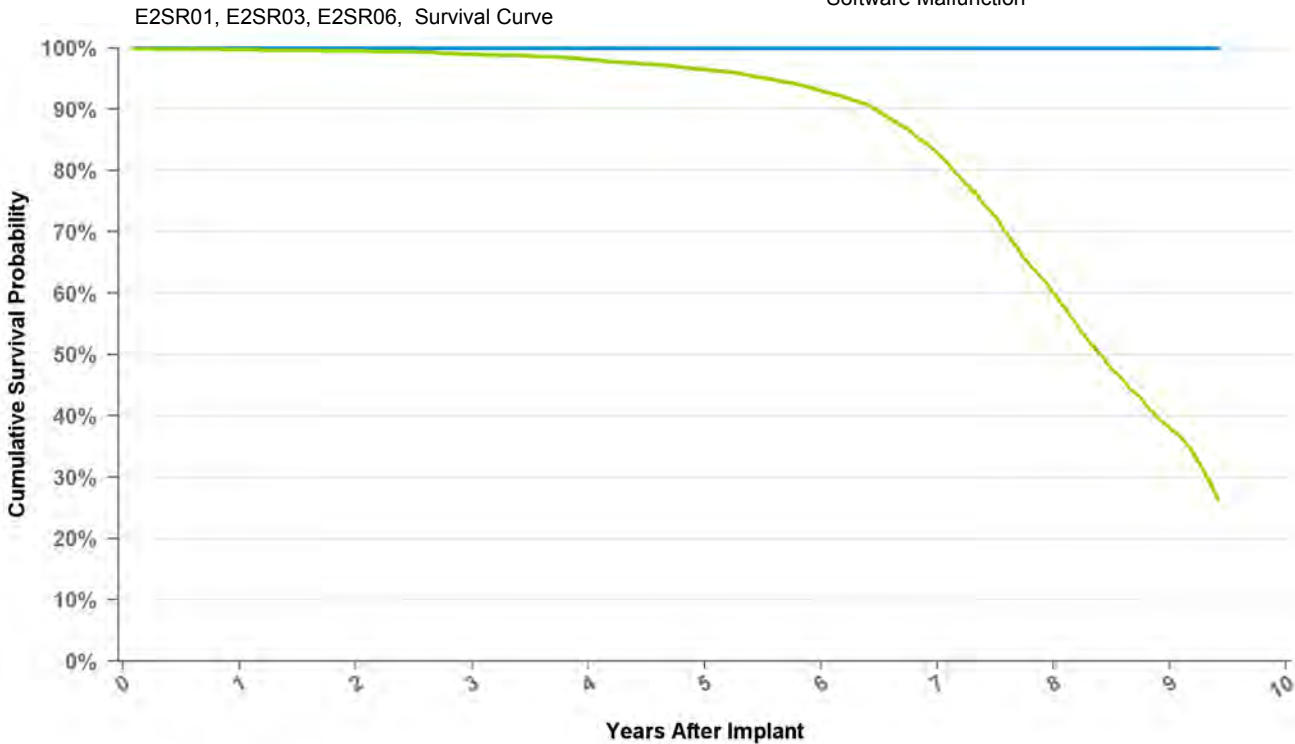

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 113 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.7% | 99.5% | 99.0% | 98.1% | 96.5% | 93.0% | 82.8% | 60.1% | 37.9% | 26.4% |
| Effective Sample Size | 22600 | 19616 | 17124 | 14986 | 12871 | 11059 | 8978 | 5680 | 1332 | 200 |

Implantable Pulse Generator

E2SR06 EnPulse 2 SR

US Market Release Date 12/18/2003

CE Market Approval Date 09/08/2003

Registered US Implants 1,749

Estimated Active US Implants 263

Normal Battery Depletions (US) 187

NBG Code SSIR

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

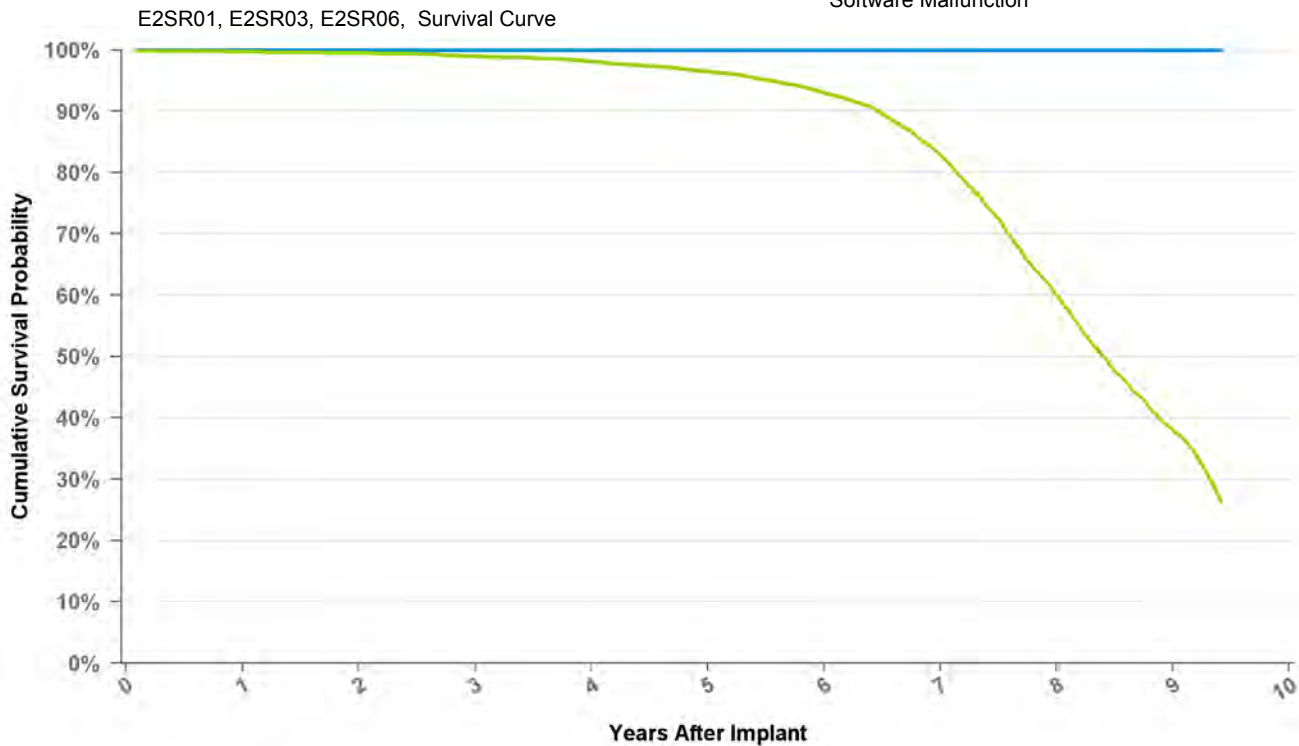

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 113 mo |
|-----------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.7% | 99.5% | 99.0% | 98.1% | 96.5% | 93.0% | 82.8% | 60.1% | 37.9% | 26.4% |
| Effective Sample Size | 22600 | 19616 | 17124 | 14986 | 12871 | 11059 | 8978 | 5680 | 1332 | 200 |

Implantable Pulse Generator

E2VDD01 EnPulse 2 VDD

| | |
|---------------------------------------|------------|
| US Market Release Date | 12/18/2003 |
| CE Market Approval Date | 09/08/2003 |
| Registered US Implants | 555 |
| Estimated Active US Implants | 89 |
| Normal Battery Depletions (US) | 93 |
| NBG Code | VDD |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

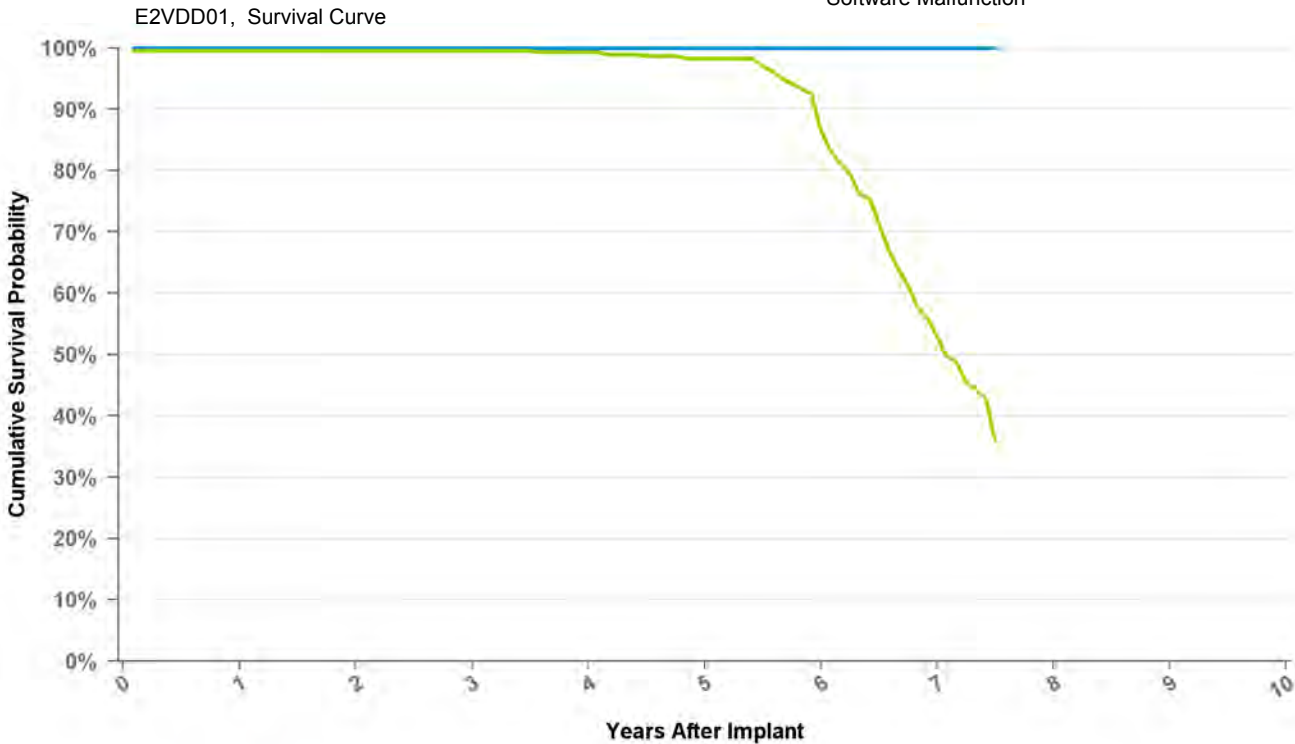

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 90 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.5% | 99.5% | 99.5% | 99.3% | 98.3% | 86.5% | 52.9% | 35.9% |
| Effective Sample Size | 705 | 649 | 595 | 543 | 489 | 406 | 189 | 113 |

Implantable Pulse Generator

EMDR01 EnRhythm MRI

US Market Release Date

CE Market Approval Date 09/30/2008

Registered US Implants 111

Estimated Active US Implants 57

Normal Battery Depletions (US) 3

NBG Code DDDRP

Max Delivered Energy N/A

Total Malfunctions (US) 17

Therapy Not Compromised Malfunctions

Battery Malfunction 17

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

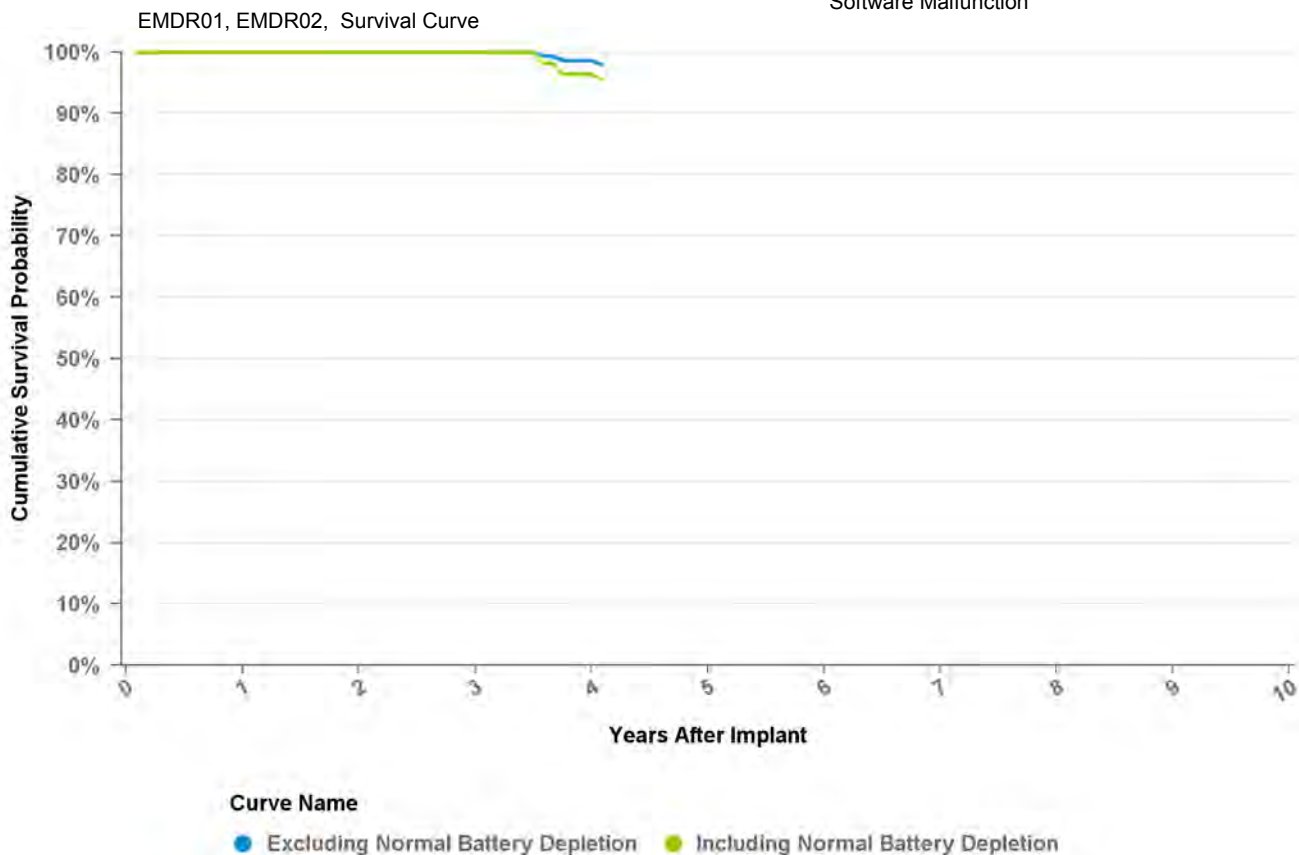

| Years | 1 | 2 | 3 | 4 | at 49 mo |
|-----------------------|--------|--------|--------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 98.6% | 97.9% |
| Including NBD | 100.0% | 100.0% | 100.0% | 96.4% | 95.5% |
| Effective Sample Size | 146 | 133 | 119 | 103 | 102 |

Implantable Pulse Generator

EN1DR01 Ensura MRI

US Market Release Date

CE Market Approval Date 06/23/2010

Registered US Implants 4

Estimated Active US Implants 4

Normal Battery Depletions (US) 0

NBG Code OOE-DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

A2DR01, A3DR01, A5DR01, EN1DR01, Survival Curve

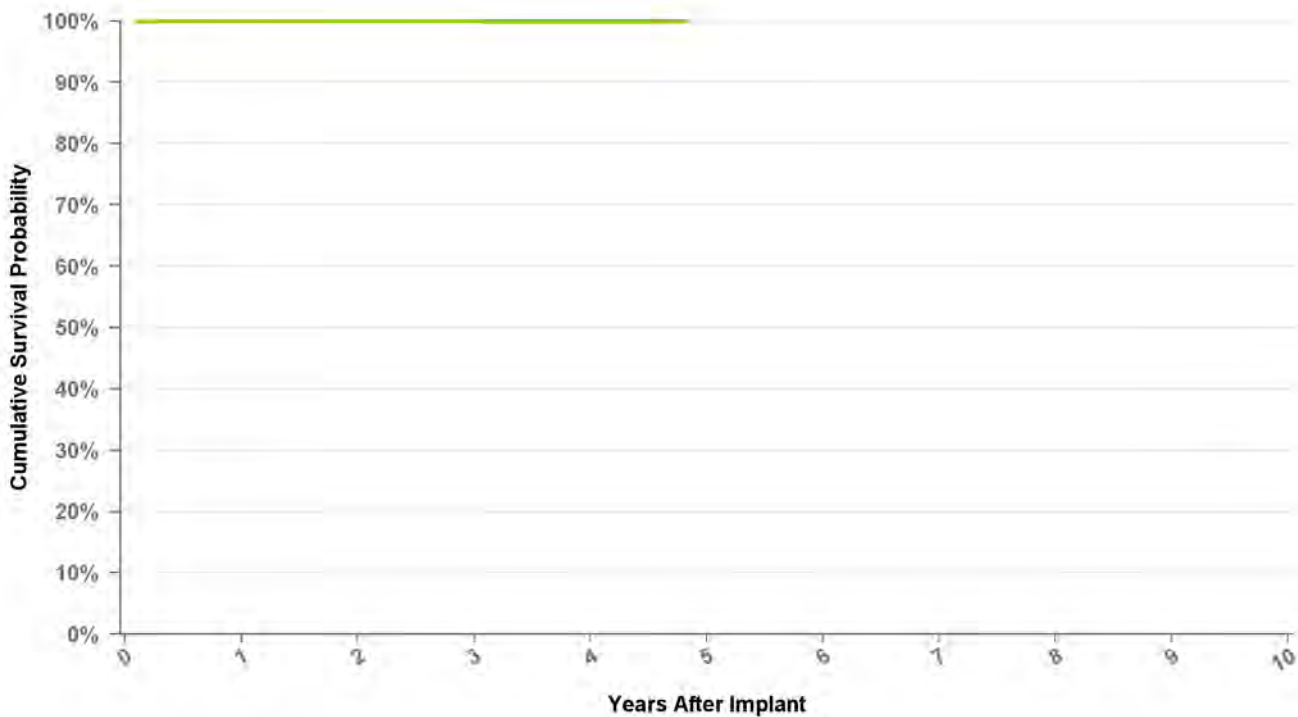

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | at 58 mo |
|-----------------------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% |
| Effective Sample Size | 40851 | 12039 | 6804 | 2770 | 161 |


Implantable Pulse Generator

KD700

Kappa 700 DR

| | |
|---------------------------------------|-----|
| US Market Release Date | |
| CE Market Approval Date | |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDD |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

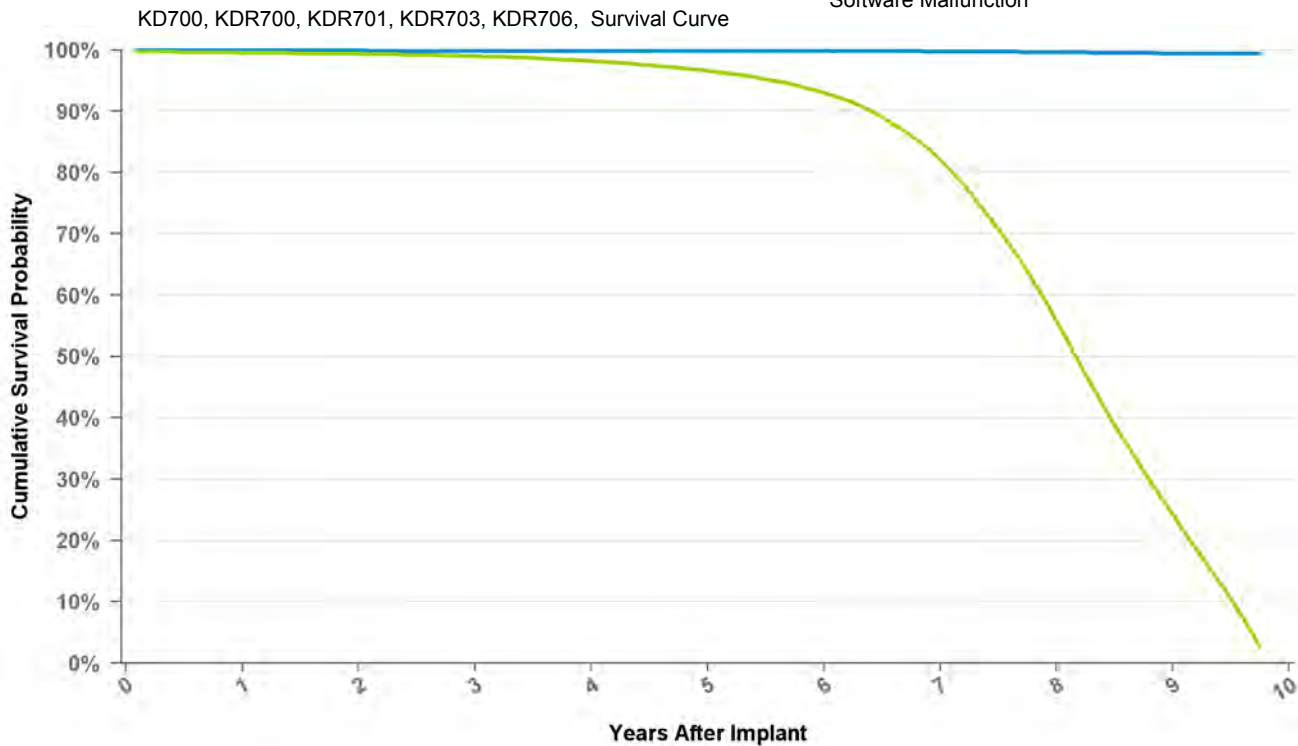

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 117 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.7% | 99.6% | 99.4% | 99.4% |
| Including NBD | 99.5% | 99.4% | 99.0% | 98.2% | 96.6% | 93.0% | 82.0% | 55.8% | 24.3% | 2.7% |
| Effective Sample Size | 180087 | 165060 | 150467 | 135831 | 121507 | 105911 | 83632 | 48446 | 14852 | 1091 |

Implantable Pulse Generator

KD701

Kappa 700 DR

US Market Release Date 01/29/1999

CE Market Approval Date 03/20/1998

Registered US Implants 242

Estimated Active US Implants 47

Normal Battery Depletions (US) 21

NBG Code DDD

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

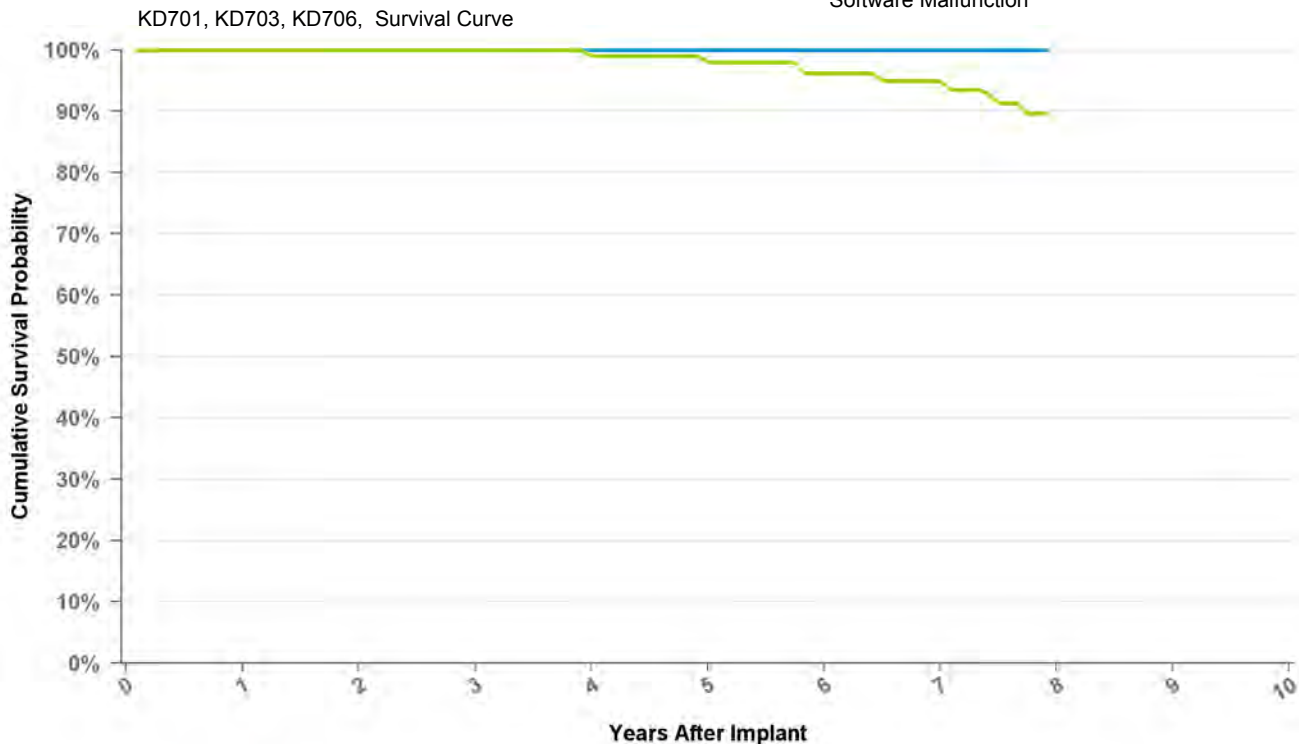

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 95 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 99.0% | 98.0% | 96.2% | 94.9% | 89.6% |
| Effective Sample Size | 289 | 260 | 229 | 206 | 186 | 162 | 137 | 100 |

Implantable Pulse Generator

KD703

Kappa 700 DR

US Market Release Date 01/29/1999

CE Market Approval Date 03/20/1998

Registered US Implants 1

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code DDD

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

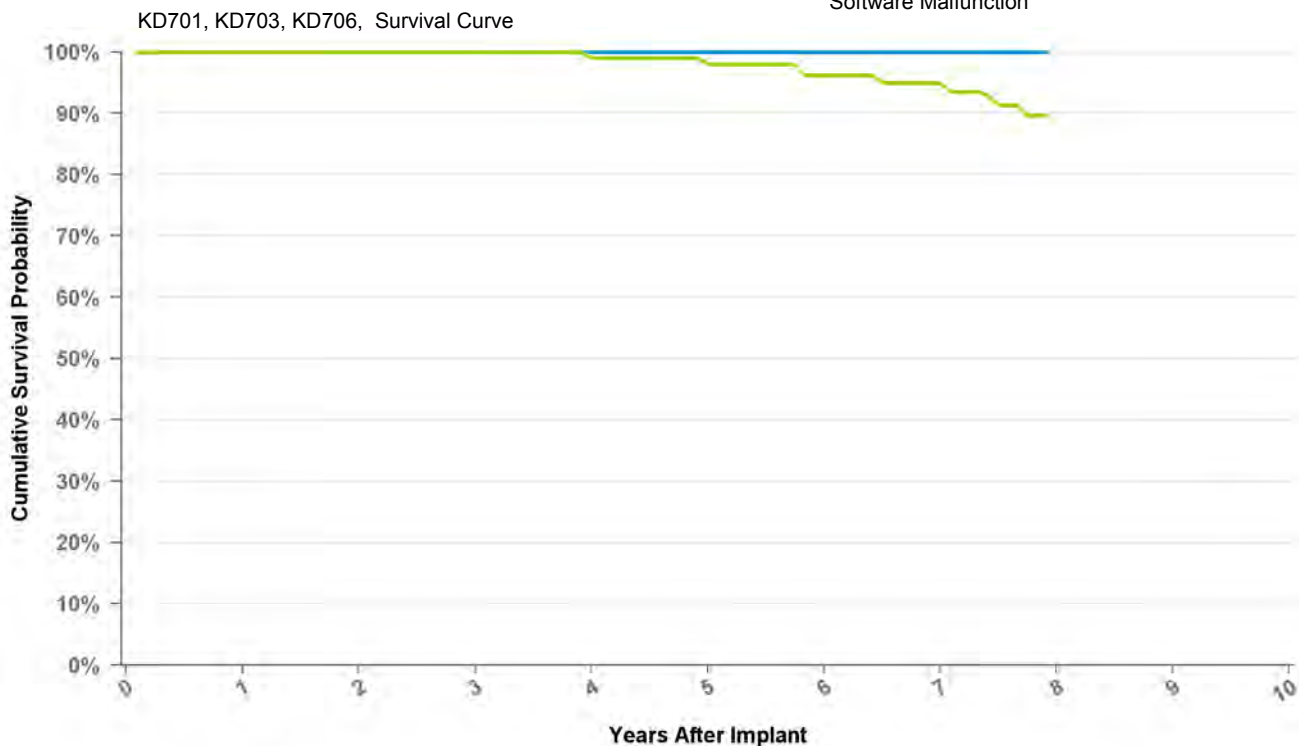

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 95 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 99.0% | 98.0% | 96.2% | 94.9% | 89.6% |
| Effective Sample Size | 289 | 260 | 229 | 206 | 186 | 162 | 137 | 100 |


Implantable Pulse Generator

KD706

Kappa 700 DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/29/1999 |
| CE Market Approval Date | 03/20/1998 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDD |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

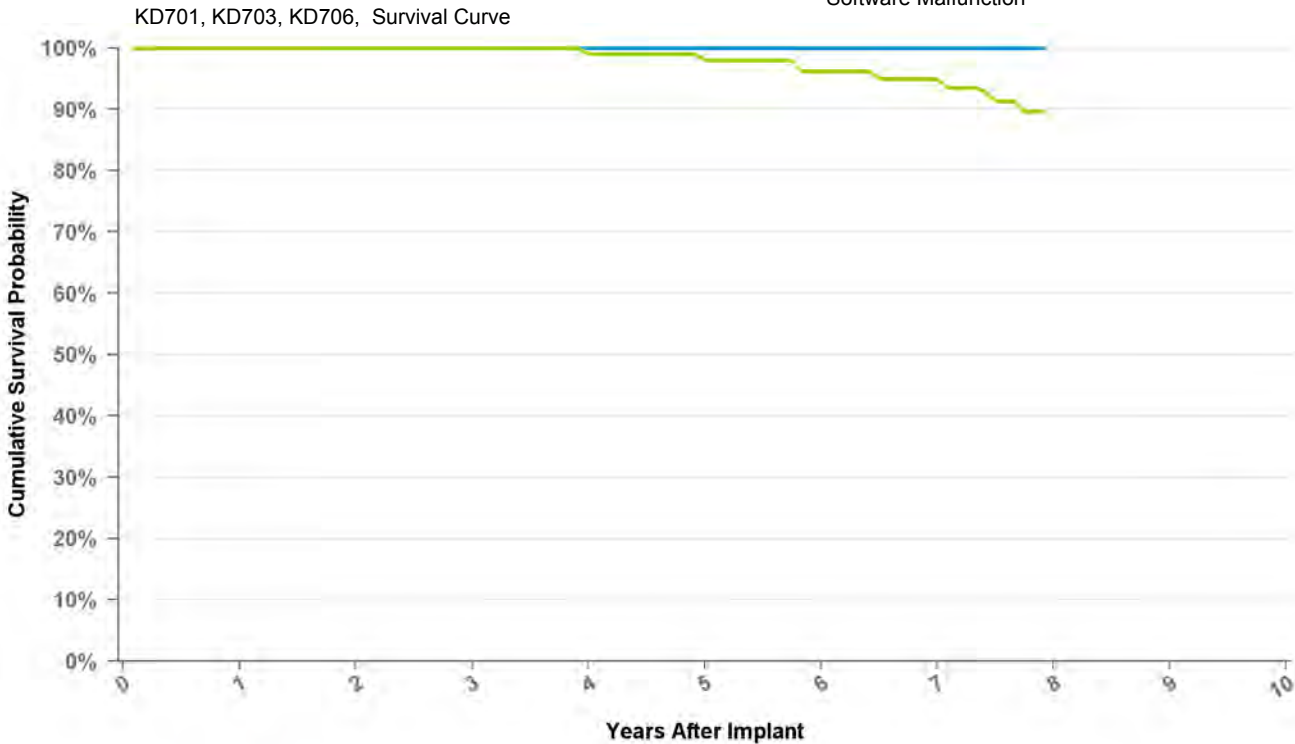

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 95 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 99.0% | 98.0% | 96.2% | 94.9% | 89.6% |
| Effective Sample Size | 289 | 260 | 229 | 206 | 186 | 162 | 137 | 100 |


Implantable Pulse Generator

KD901

Kappa 900 D

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/09/2002 |
| CE Market Approval Date | 09/28/2001 |
| Registered US Implants | 1 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDD |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

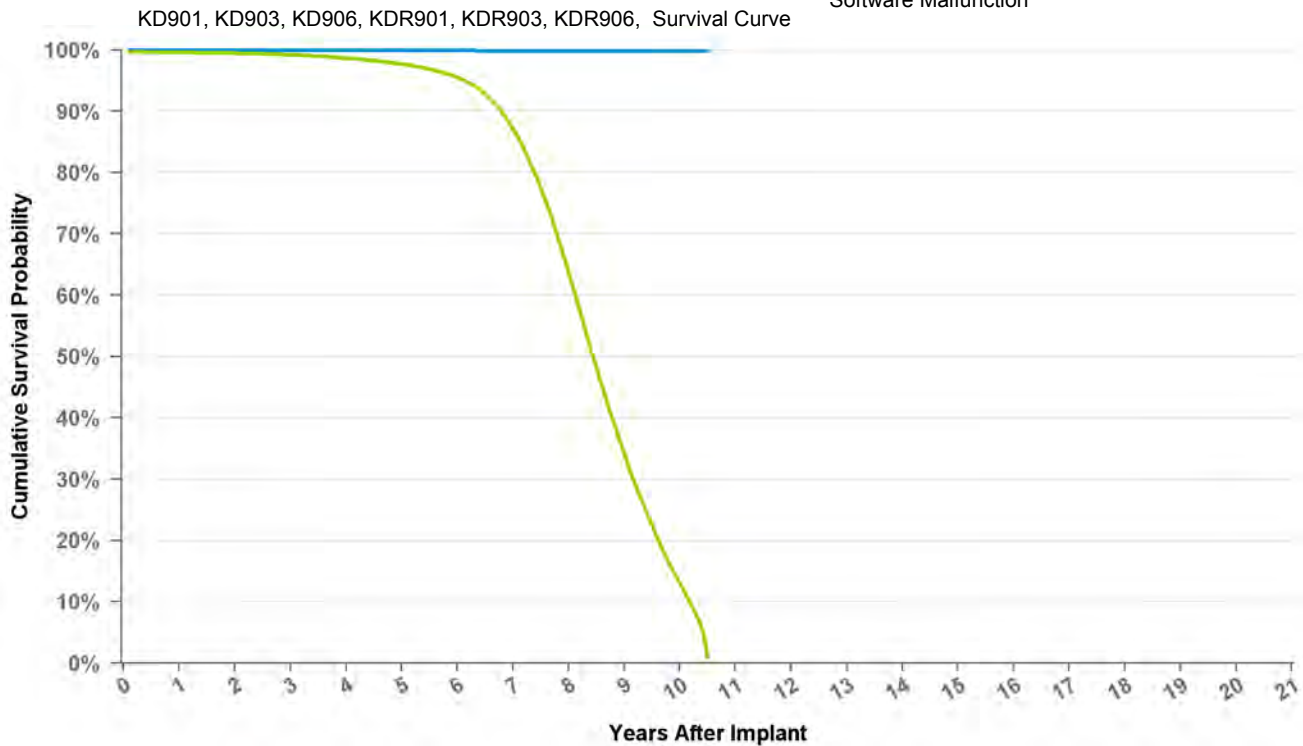

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.6% | 99.5% | 99.2% | 98.7% | 97.7% | 95.5% | 87.2% | 63.7% | 34.2% | 13.1% | 0.9% |
| Effective Sample Size | 117160 | 107791 | 98688 | 89956 | 81409 | 72845 | 61181 | 40024 | 15870 | 3015 | 175 |


Implantable Pulse Generator

KD903

Kappa 900 D

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/09/2002 |
| CE Market Approval Date | |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDD |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

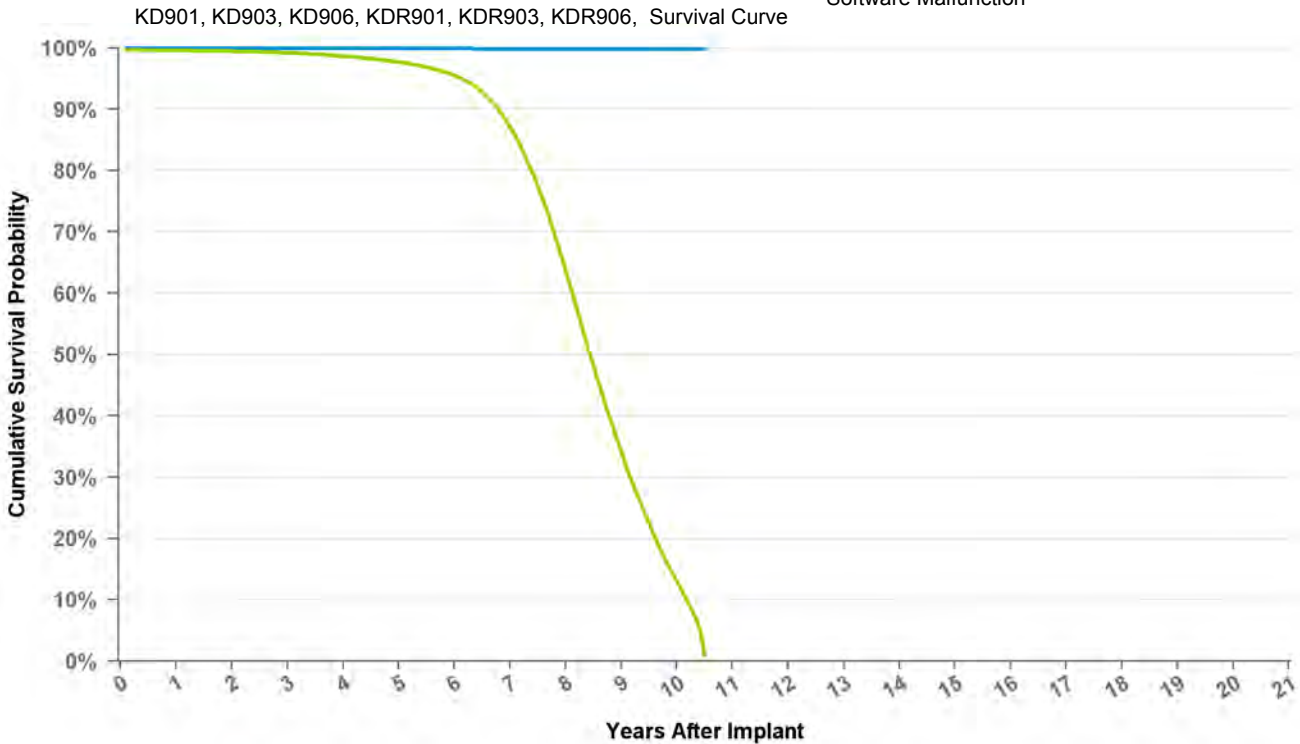

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.6% | 99.5% | 99.2% | 98.7% | 97.7% | 95.5% | 87.2% | 63.7% | 34.2% | 13.1% | 0.9% |
| Effective Sample Size | 117160 | 107791 | 98688 | 89956 | 81409 | 72845 | 61181 | 40024 | 15870 | 3015 | 175 |


Implantable Pulse Generator

KD906

Kappa 900 D

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/09/2002 |
| CE Market Approval Date | 09/28/2001 |
| Registered US Implants | 0 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | DDD |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

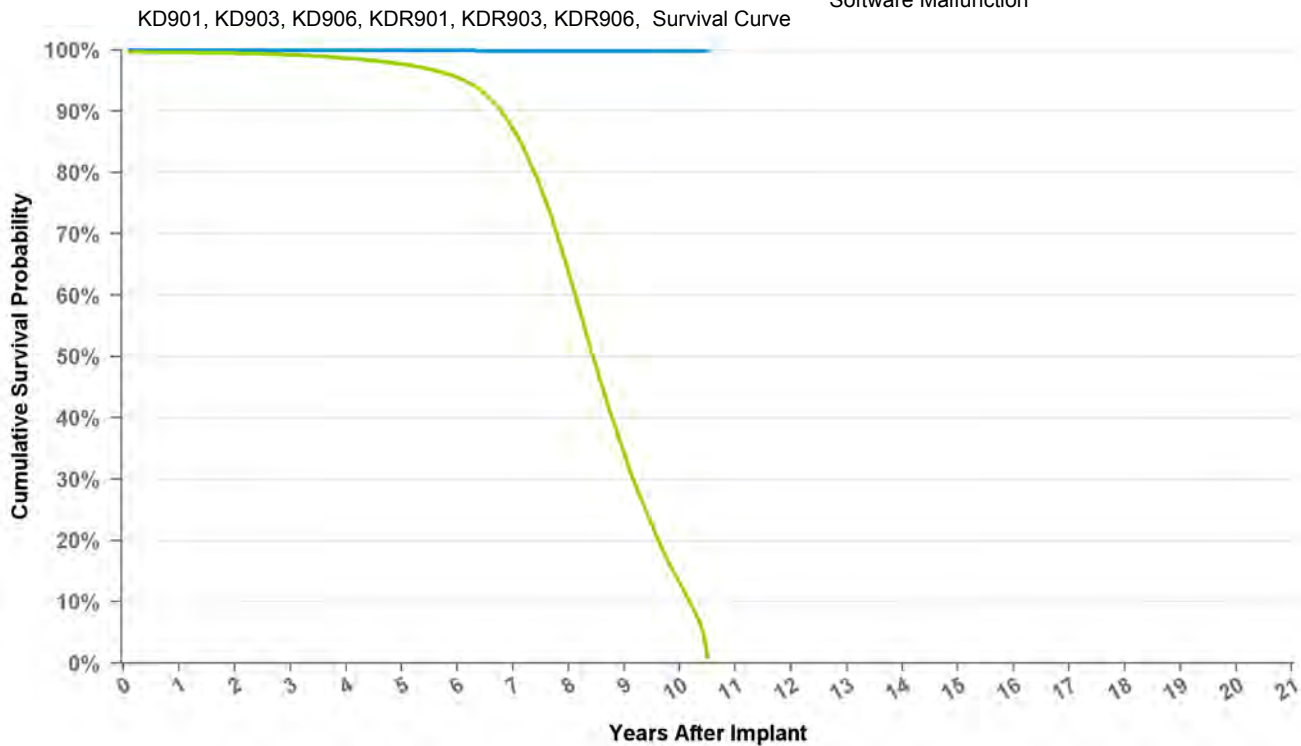

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.6% | 99.5% | 99.2% | 98.7% | 97.7% | 95.5% | 87.2% | 63.7% | 34.2% | 13.1% | 0.9% |
| Effective Sample Size | 117160 | 107791 | 98688 | 89956 | 81409 | 72845 | 61181 | 40024 | 15870 | 3015 | 175 |

Implantable Pulse Generator

KDR401 Kappa 400 DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/30/1998 |
| CE Market Approval Date | 11/12/1996 |
| Registered US Implants | 39,406 |
| Estimated Active US Implants | 2,787 |
| Normal Battery Depletions (US) | 7,178 |
| NBG Code | DDDR |
| Max Delivered Energy | N/A |

| | |
|---|----|
| Total Malfunctions (US) | 22 |
| Therapy Not Compromised Malfunctions | 13 |
| Battery Malfunction | 0 |
| Electrical Component | 9 |
| Electrical Interconnect | 1 |
| Other Malfunction | 2 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 9 |
| Battery Malfunction | 0 |
| Electrical Component | 6 |
| Electrical Interconnect | 3 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

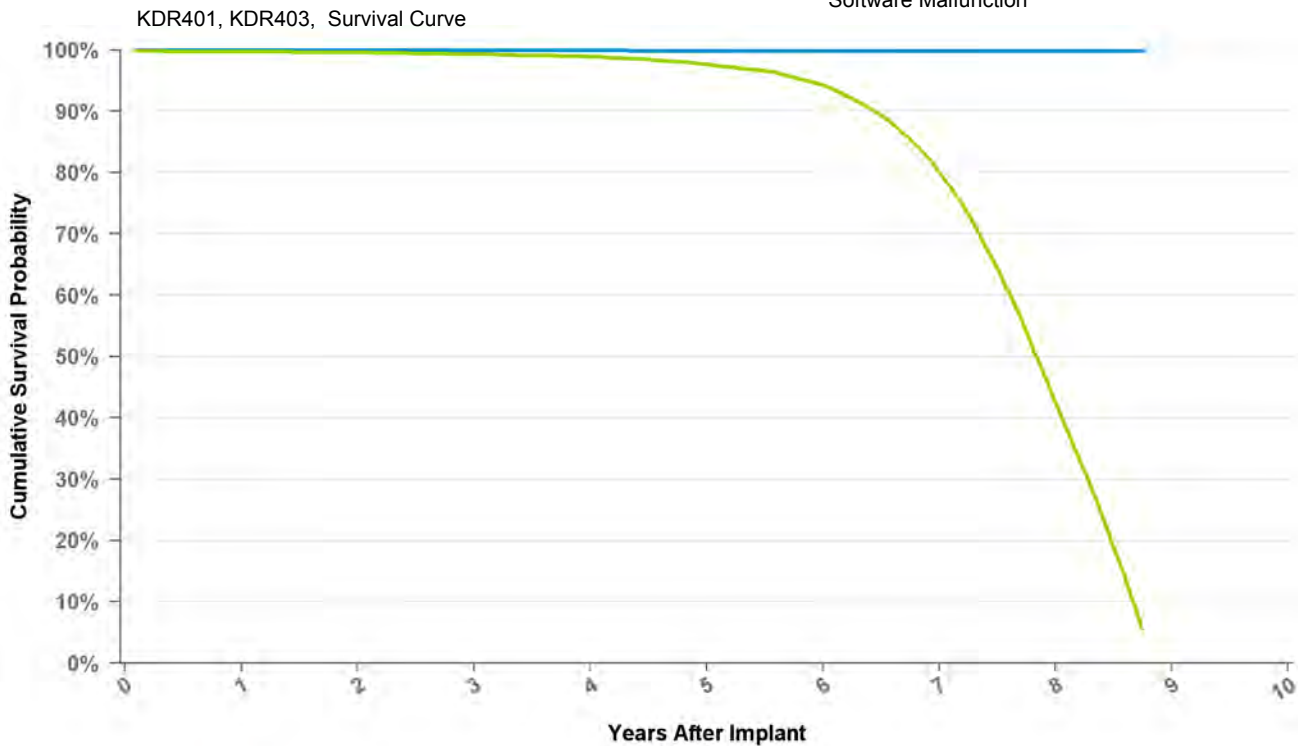

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 105 mo |
|------------------------------|--------|--------|--------|--------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.7% | 99.6% | 99.3% | 98.9% | 97.7% | 94.3% | 80.0% | 42.5% | 5.5% |
| Effective Sample Size | 44187 | 41058 | 37881 | 34829 | 31405 | 27423 | 20490 | 8453 | 888 |

Implantable Pulse Generator

KDR403 Kappa 400 DR

US Market Release Date 01/30/1998

CE Market Approval Date 11/12/1996

Registered US Implants 7,311

Estimated Active US Implants 827

Normal Battery Depletions (US) 1,114

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 6

Therapy Not Compromised Malfunctions 2

Battery Malfunction 0

Electrical Component 1

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 1

Software Malfunction 0

Therapy Compromised Malfunctions 4

Battery Malfunction 0


Electrical Component 1

Electrical Interconnect 3

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

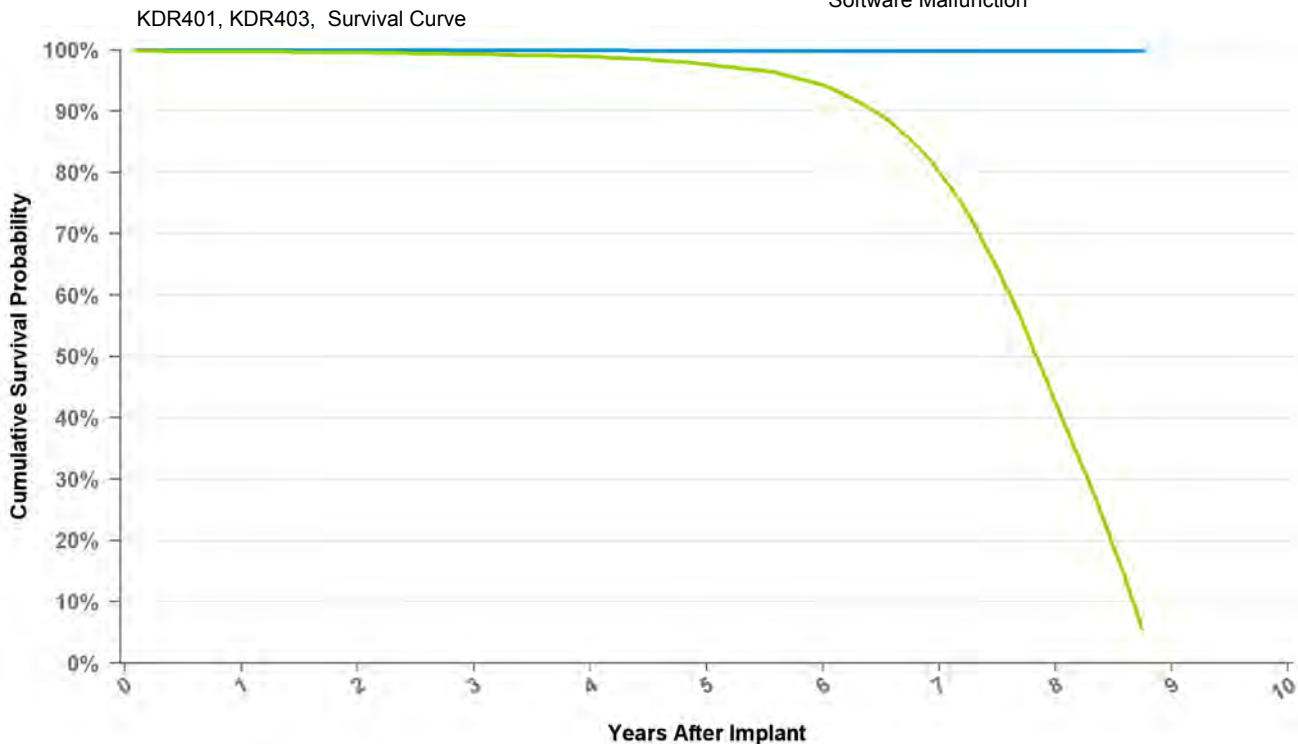

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 105 mo |
|------------------------------|--------|--------|--------|--------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.7% | 99.6% | 99.3% | 98.9% | 97.7% | 94.3% | 80.0% | 42.5% | 5.5% |
| Effective Sample Size | 44187 | 41058 | 37881 | 34829 | 31405 | 27423 | 20490 | 8453 | 888 |

Implantable Pulse Generator

KDR700

Kappa 700 DR

US Market Release Date

CE Market Approval Date

Registered US Implants 15

Estimated Active US Implants 1

Normal Battery Depletions (US) 4

NBG Code DDD/RO

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

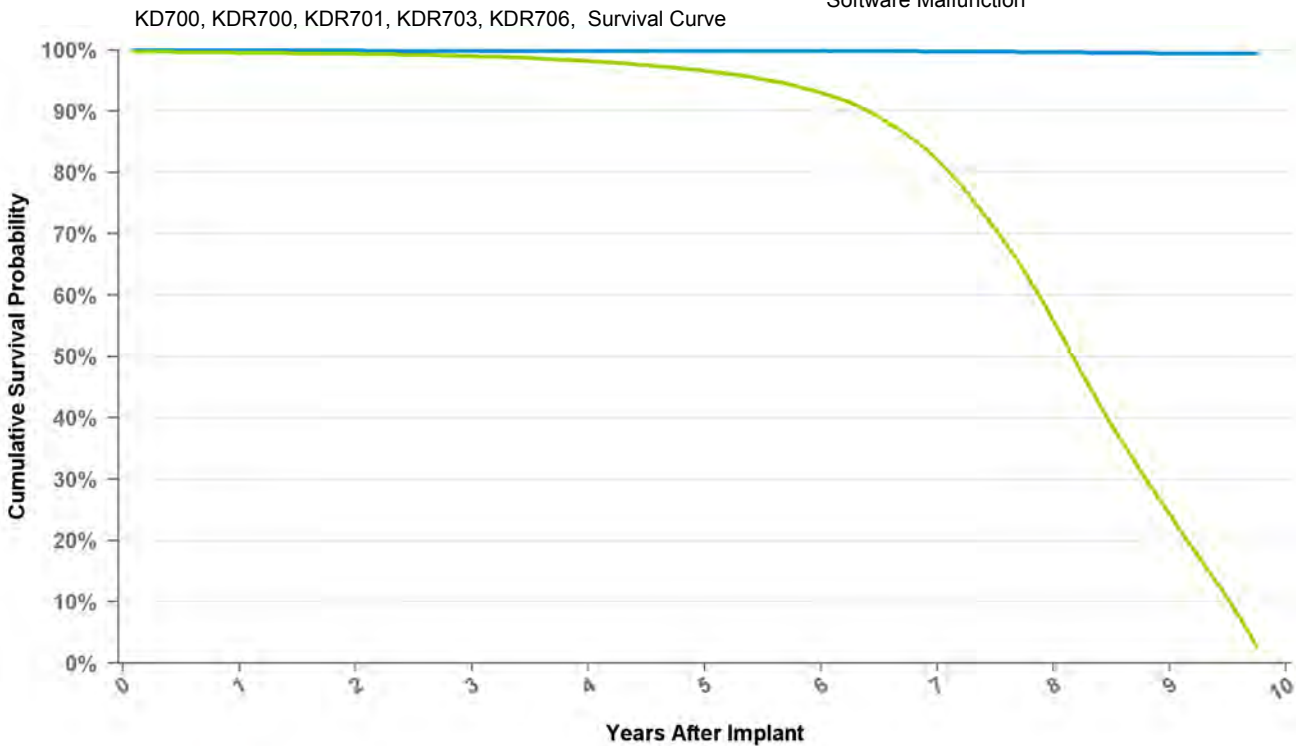

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 117 mo |
|-----------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.7% | 99.6% | 99.4% | 99.4% |
| Including NBD | 99.5% | 99.4% | 99.0% | 98.2% | 96.6% | 93.0% | 82.0% | 55.8% | 24.3% | 2.7% |
| Effective Sample Size | 180087 | 165060 | 150467 | 135831 | 121507 | 105911 | 83632 | 48446 | 14852 | 1091 |

Implantable Pulse Generator

KDR701 Kappa 700 DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/29/1999 |
| CE Market Approval Date | 03/20/1998 |
| Registered US Implants | 194,144 |
| Estimated Active US Implants | 17,293 |
| Normal Battery Depletions (US) | 36,299 |
| NBG Code | DDD/RO |
| Max Delivered Energy | N/A |

| | |
|---|-----|
| Total Malfunctions (US) | 702 |
| Therapy Not Compromised Malfunctions | 48 |
| Battery Malfunction | 1 |
| Electrical Component | 23 |
| Electrical Interconnect | 18 |
| Other Malfunction | 3 |
| Poss Early Battery Depltn | 3 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 654 |
| Battery Malfunction | 0 |
| Electrical Component | 16 |
| Electrical Interconnect | 637 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |

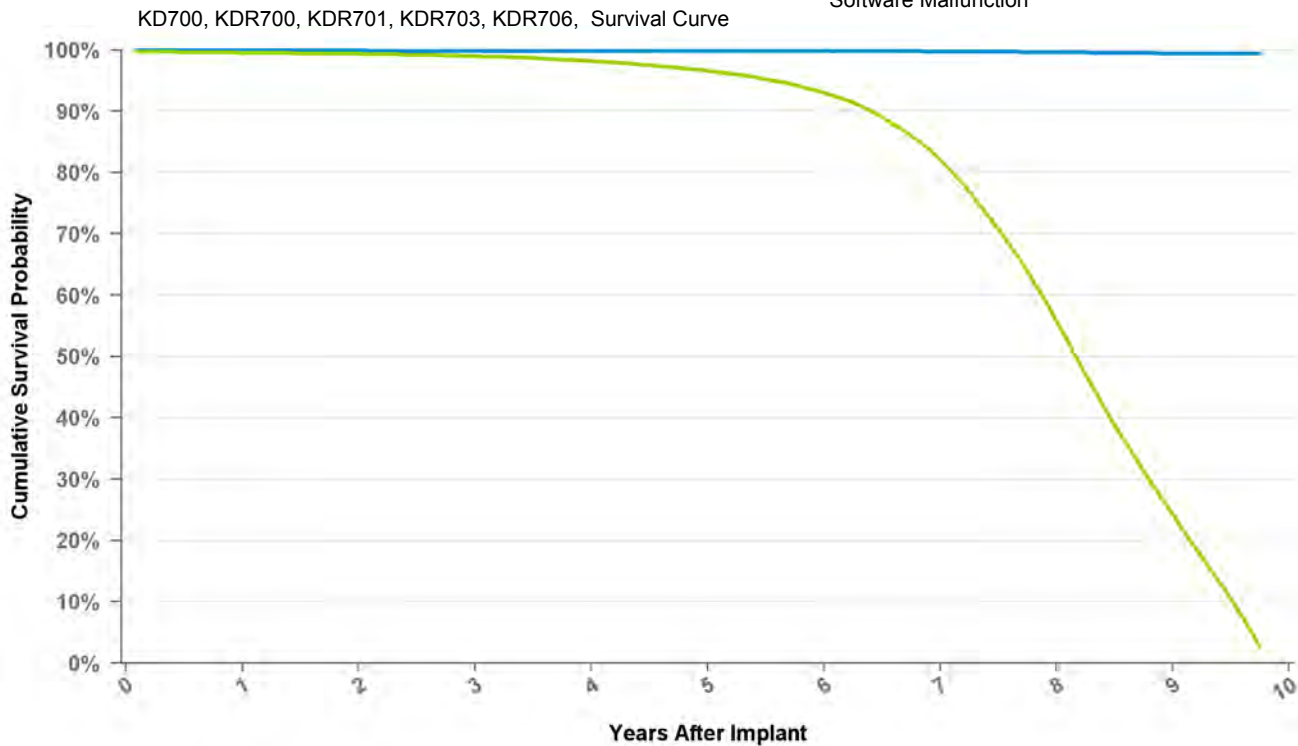

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 117 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.7% | 99.6% | 99.4% | 99.4% |
| Including NBD | 99.5% | 99.4% | 99.0% | 98.2% | 96.6% | 93.0% | 82.0% | 55.8% | 24.3% | 2.7% |
| Effective Sample Size | 180087 | 165060 | 150467 | 135831 | 121507 | 105911 | 83632 | 48446 | 14852 | 1091 |

Implantable Pulse Generator

KDR703 Kappa 700 DR

US Market Release Date 02/05/1999

CE Market Approval Date 03/20/1998

Registered US Implants 9,226

Estimated Active US Implants 774

Normal Battery Depletions (US) 1,531

NBG Code DDD/RO

Max Delivered Energy N/A

Total Malfunctions (US) 34

Therapy Not Compromised Malfunctions 4

Battery Malfunction 0

Electrical Component 3

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 1

Software Malfunction 0

Therapy Compromised Malfunctions 30

Battery Malfunction 0


Electrical Component 1

Electrical Interconnect 29

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

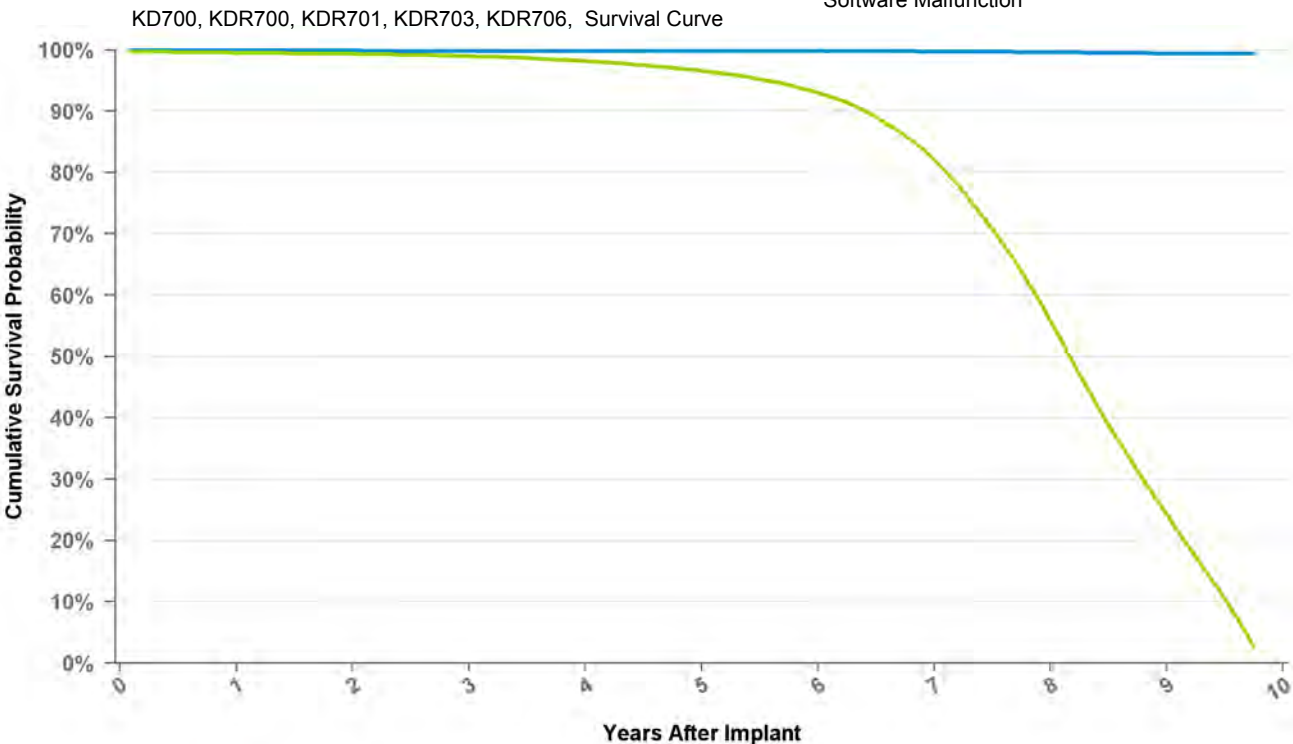

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 117 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.7% | 99.6% | 99.4% | 99.4% |
| Including NBD | 99.5% | 99.4% | 99.0% | 98.2% | 96.6% | 93.0% | 82.0% | 55.8% | 24.3% | 2.7% |
| Effective Sample Size | 180087 | 165060 | 150467 | 135831 | 121507 | 105911 | 83632 | 48446 | 14852 | 1091 |

Implantable Pulse Generator

KDR706 Kappa 700 DR

US Market Release Date 02/09/1999

CE Market Approval Date 03/20/1998

Registered US Implants 2,633

Estimated Active US Implants 176

Normal Battery Depletions (US) 402

NBG Code DDD/RO

Max Delivered Energy N/A

Total Malfunctions (US) 10

Therapy Not Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 1

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 9

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 9

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

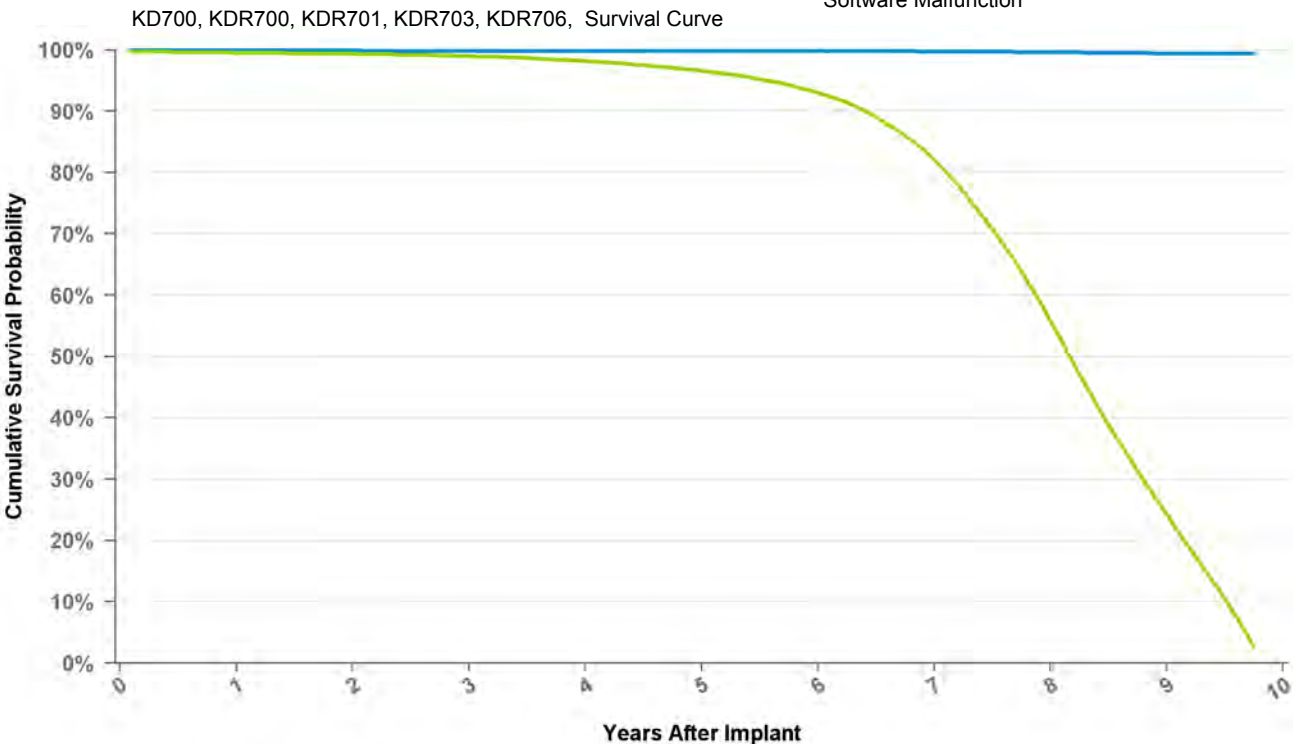

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 117 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.7% | 99.6% | 99.4% | 99.4% |
| Including NBD | 99.5% | 99.4% | 99.0% | 98.2% | 96.6% | 93.0% | 82.0% | 55.8% | 24.3% | 2.7% |
| Effective Sample Size | 180087 | 165060 | 150467 | 135831 | 121507 | 105911 | 83632 | 48446 | 14852 | 1091 |

Implantable Pulse Generator

KDR721 Kappa 700 DR

US Market Release Date 02/11/1999

CE Market Approval Date 03/20/1998

Registered US Implants 9,838

Estimated Active US Implants 721

Normal Battery Depletions (US) 1,361

NBG Code DDD/RO

Max Delivered Energy N/A

Total Malfunctions (US) 5

Therapy Not Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 1

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 4

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 4

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

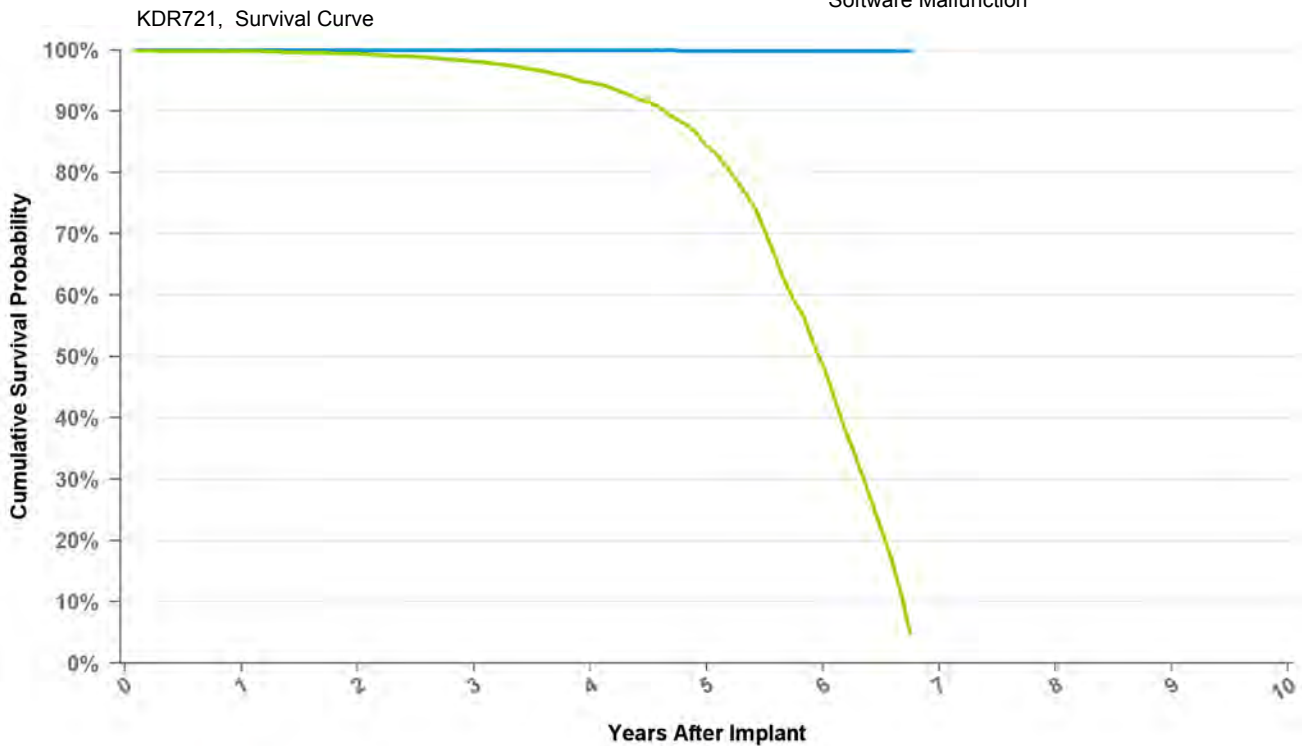

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 81 mo |
|------------------------------|--------|--------|--------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.8% | 99.4% | 98.1% | 94.7% | 84.4% | 48.7% | 4.8% |
| Effective Sample Size | 8623 | 7613 | 6639 | 5600 | 4305 | 1785 | 171 |

Implantable Pulse Generator

KDR901 Kappa 900 DR

US Market Release Date 01/09/2002

CE Market Approval Date 09/28/2001

Registered US Implants 120,696

Estimated Active US Implants 15,339

Normal Battery Depletions (US) 25,607

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 70

Therapy Not Compromised Malfunctions 21

Battery Malfunction 0

Electrical Component 16

Electrical Interconnect 4

Other Malfunction 1

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 49

Battery Malfunction 0


Electrical Component 10

Electrical Interconnect 39

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

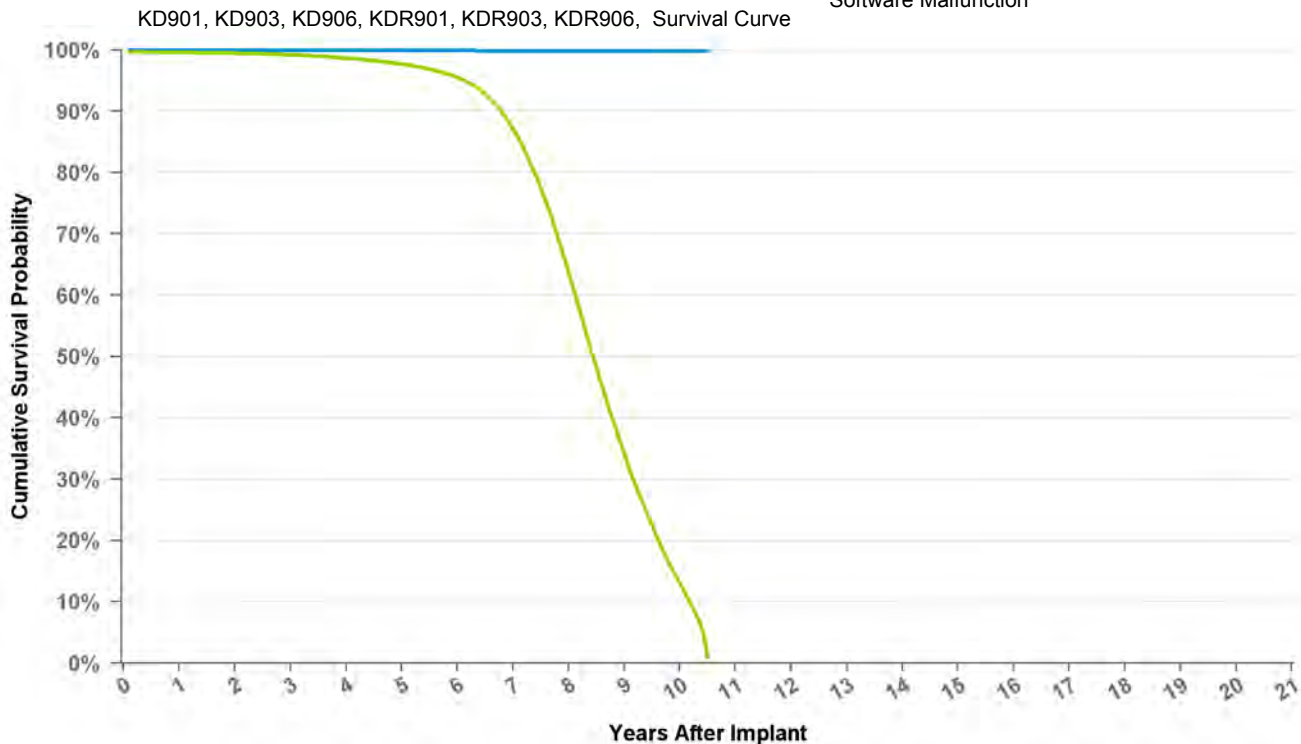

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.6% | 99.5% | 99.2% | 98.7% | 97.7% | 95.5% | 87.2% | 63.7% | 34.2% | 13.1% | 0.9% |
| Effective Sample Size | 117160 | 107791 | 98688 | 89956 | 81409 | 72845 | 61181 | 40024 | 15870 | 3015 | 175 |

Implantable Pulse Generator

KDR903 Kappa 900 DR

US Market Release Date 01/09/2002

CE Market Approval Date 09/28/2001

Registered US Implants 3,169

Estimated Active US Implants 326

Normal Battery Depletions (US) 612

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 3

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 3

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 3

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

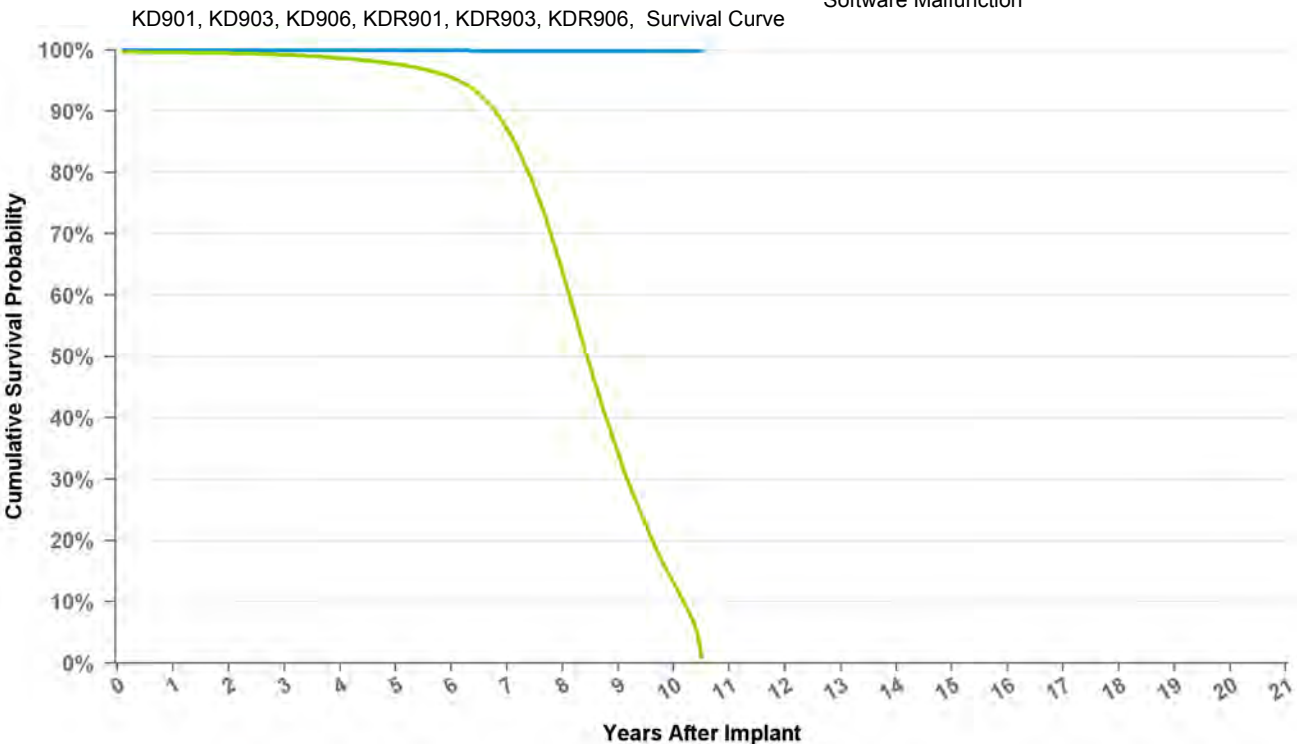

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.6% | 99.5% | 99.2% | 98.7% | 97.7% | 95.5% | 87.2% | 63.7% | 34.2% | 13.1% | 0.9% |
| Effective Sample Size | 117160 | 107791 | 98688 | 89956 | 81409 | 72845 | 61181 | 40024 | 15870 | 3015 | 175 |


Implantable Pulse Generator

KDR906

Kappa 900 DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/09/2002 |
| CE Market Approval Date | 09/28/2001 |
| Registered US Implants | 1,509 |
| Estimated Active US Implants | 116 |
| Normal Battery Depletions (US) | 298 |
| NBG Code | DDDR |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 2 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 2 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 2 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

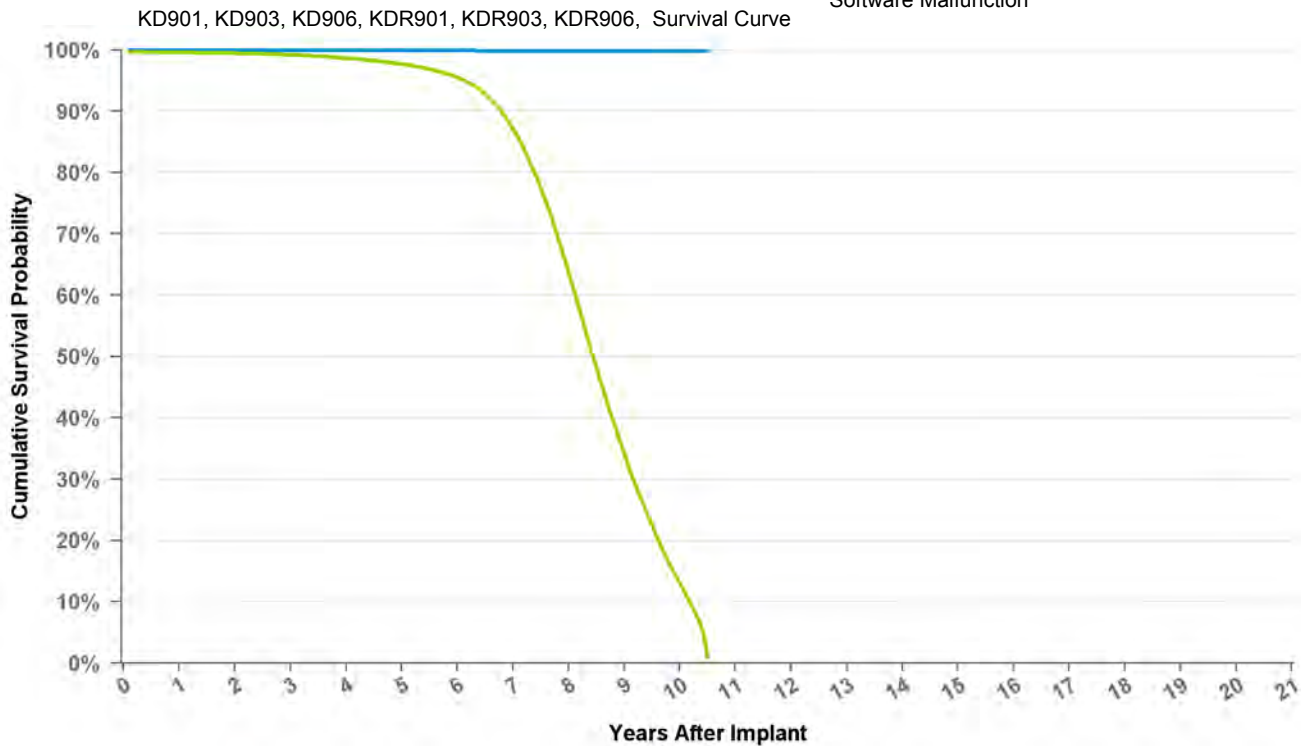

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.6% | 99.5% | 99.2% | 98.7% | 97.7% | 95.5% | 87.2% | 63.7% | 34.2% | 13.1% | 0.9% |
| Effective Sample Size | 117160 | 107791 | 98688 | 89956 | 81409 | 72845 | 61181 | 40024 | 15870 | 3015 | 175 |

Implantable Pulse Generator

KDR921 Kappa 900 DR

US Market Release Date 01/09/2002

CE Market Approval Date 09/28/2001

Registered US Implants 16,329

Estimated Active US Implants 1,319

Normal Battery Depletions (US) 2,886

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 4

Therapy Not Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 1

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 3

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 3

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

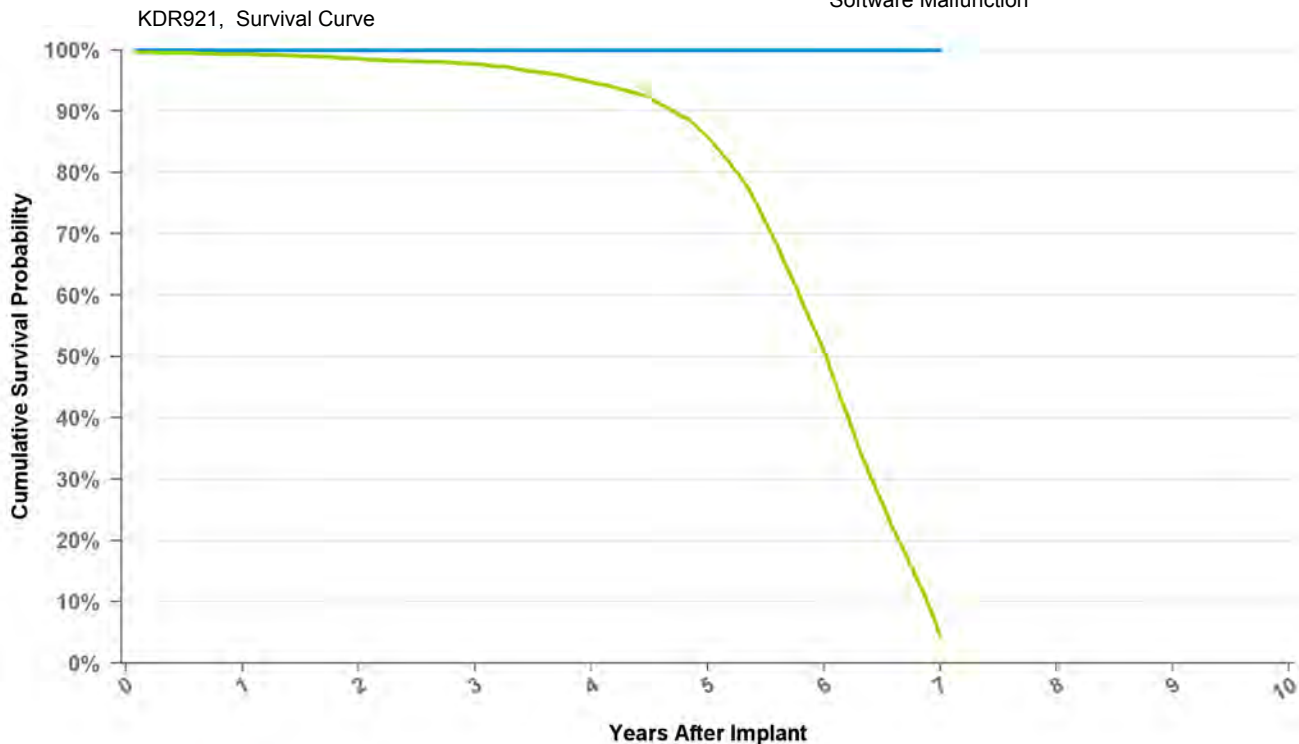

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 84 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.3% | 98.6% | 97.7% | 94.7% | 85.8% | 51.0% | 4.3% |
| Effective Sample Size | 14184 | 12614 | 11138 | 9597 | 7629 | 3534 | 235 |

Implantable Pulse Generator

KSR401

Kappa 400 SR

US Market Release Date 02/18/1998

CE Market Approval Date 11/12/1996

Registered US Implants 11,788

Estimated Active US Implants 866

Normal Battery Depletions (US) 1,278

NBG Code SSIR

Max Delivered Energy N/A

Total Malfunctions (US) 4

Therapy Not Compromised Malfunctions 4

Battery Malfunction 0

Electrical Component 3

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 1

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

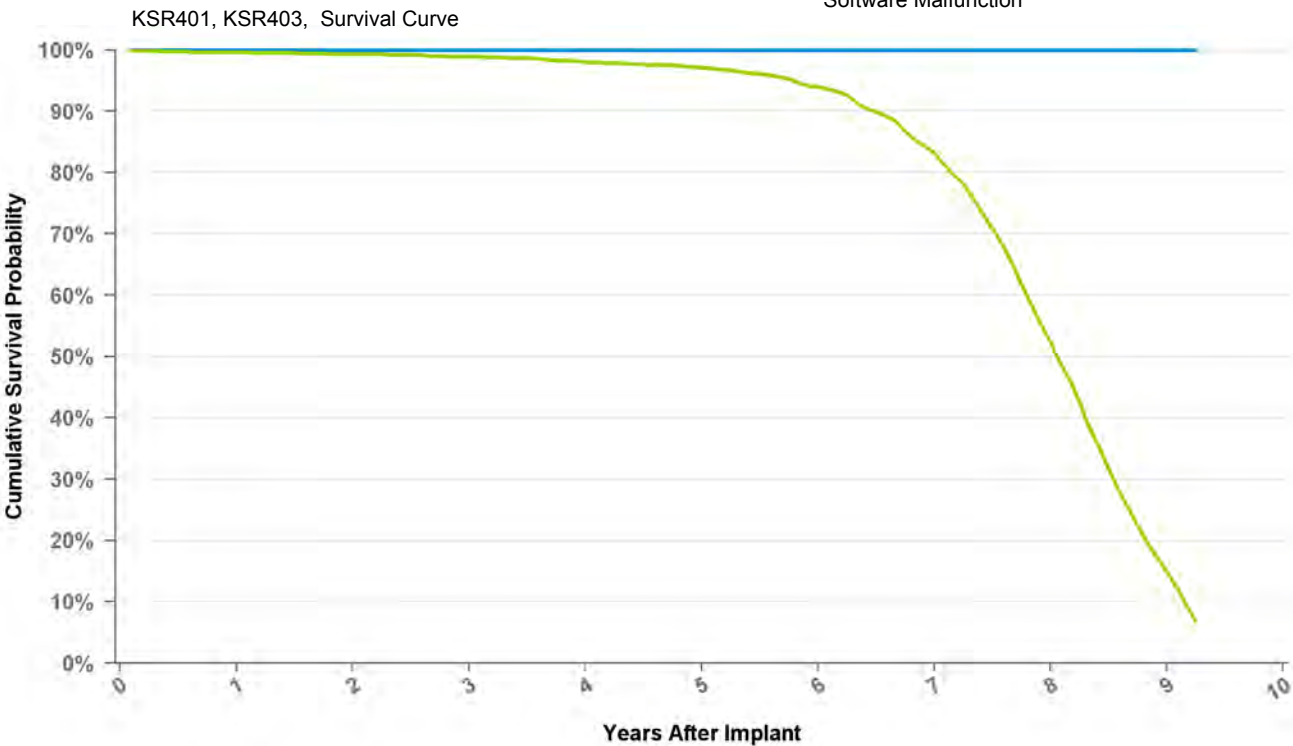

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 111 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.6% | 99.3% | 98.9% | 98.0% | 97.1% | 94.0% | 83.2% | 52.4% | 14.9% | 6.9% |
| Effective Sample Size | 13589 | 11932 | 10430 | 9156 | 7902 | 6630 | 5025 | 2448 | 393 | 147 |

Implantable Pulse Generator

KSR403 Kappa 400 SR

US Market Release Date 02/24/1998

CE Market Approval Date 11/12/1996

Registered US Implants 3,620

Estimated Active US Implants 407

Normal Battery Depletions (US) 376

NBG Code SSIR

Max Delivered Energy N/A

Total Malfunctions (US) 1

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 1

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 1

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

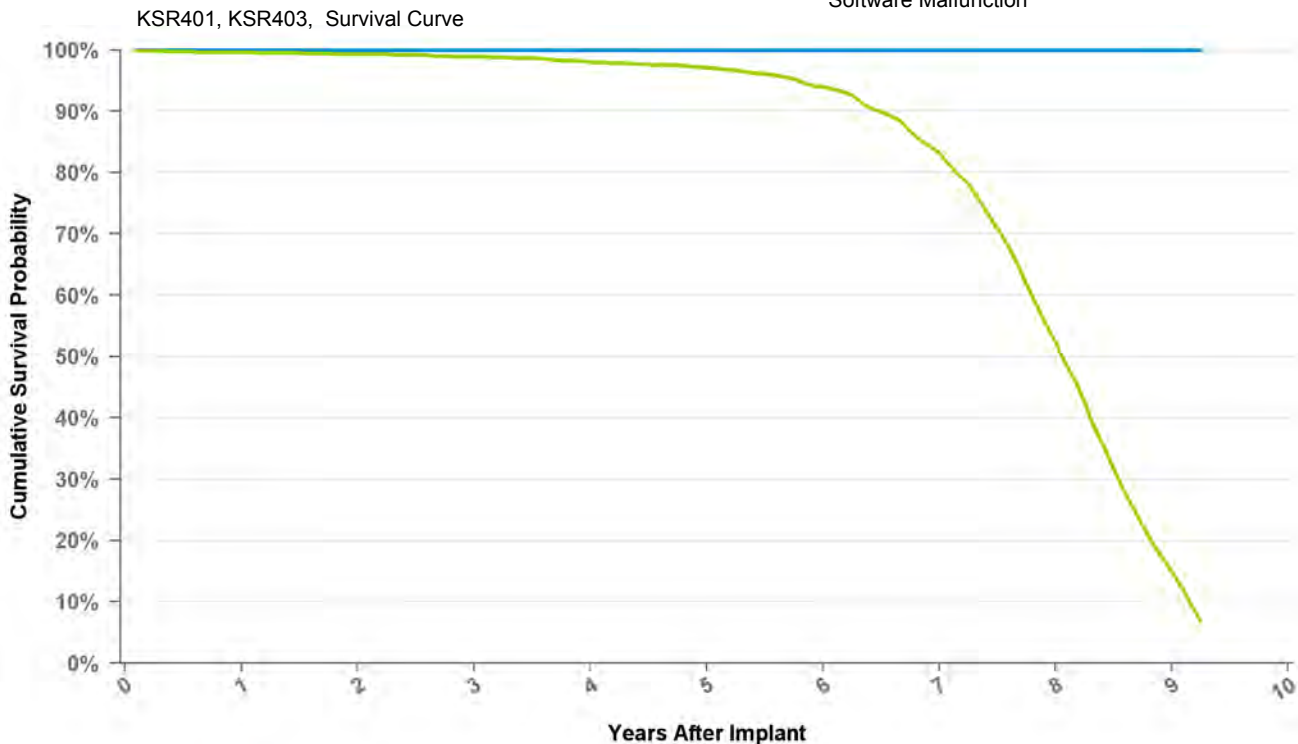

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 111 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.6% | 99.3% | 98.9% | 98.0% | 97.1% | 94.0% | 83.2% | 52.4% | 14.9% | 6.9% |
| Effective Sample Size | 13589 | 11932 | 10430 | 9156 | 7902 | 6630 | 5025 | 2448 | 393 | 147 |


Implantable Pulse Generator

KSR700

Kappa 700 SR

| | |
|---------------------------------------|------|
| US Market Release Date | |
| CE Market Approval Date | |
| Registered US Implants | 1 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | SSIR |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

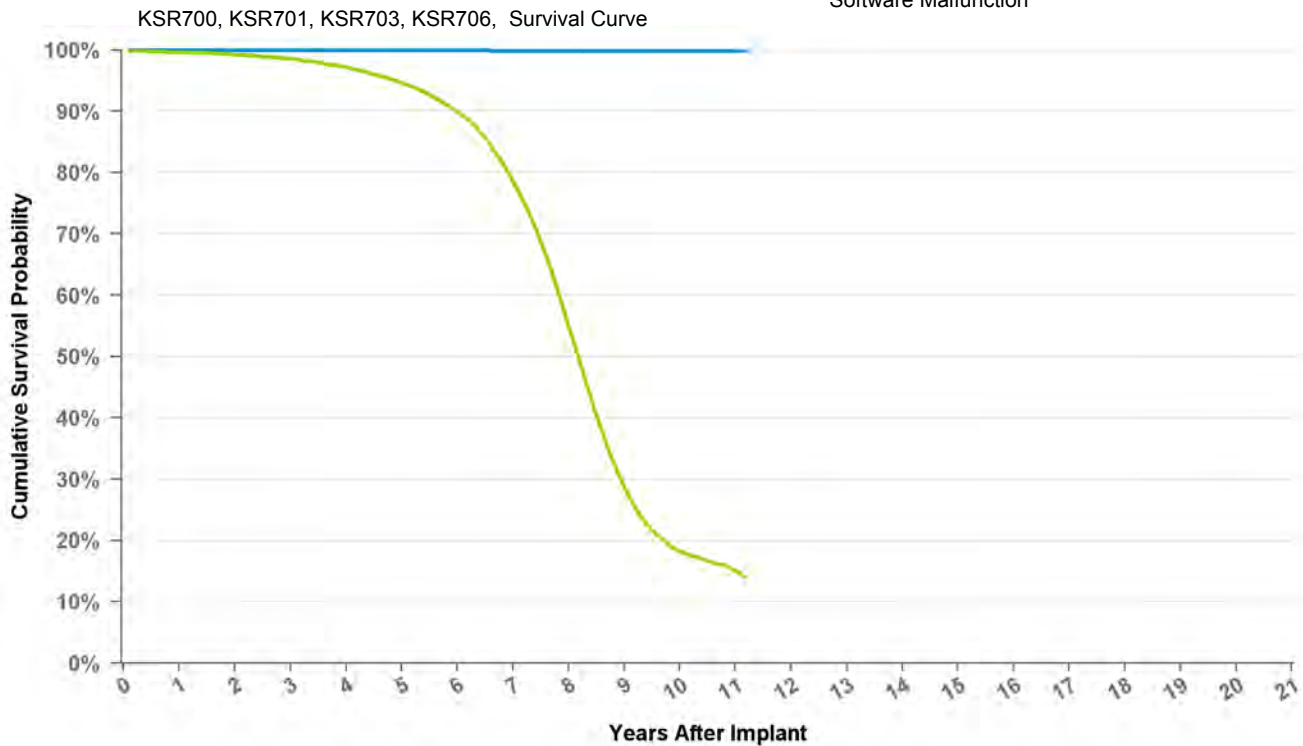

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 134 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.8% | 99.8% | 99.8% | 99.8% |
| Including NBD | 99.6% | 99.2% | 98.6% | 97.2% | 94.6% | 89.9% | 78.6% | 54.9% | 28.8% | 18.3% | 15.1% | 13.9% |
| Effective Sample Size | 48205 | 41529 | 35578 | 30377 | 25558 | 21008 | 15803 | 9014 | 3097 | 1041 | 245 | 135 |


Implantable Pulse Generator

KSR701

Kappa 700 SR

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/29/1999 |
| CE Market Approval Date | 03/20/1998 |
| Registered US Implants | 48,466 |
| Estimated Active US Implants | 4,309 |
| Normal Battery Depletions (US) | 5,041 |
| NBG Code | SSIR |
| Max Delivered Energy | N/A |

| | |
|---|----|
| Total Malfunctions (US) | 22 |
| Therapy Not Compromised Malfunctions | 3 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 1 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 19 |
| Battery Malfunction | 0 |
| Electrical Component | 2 |
| Electrical Interconnect | 17 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

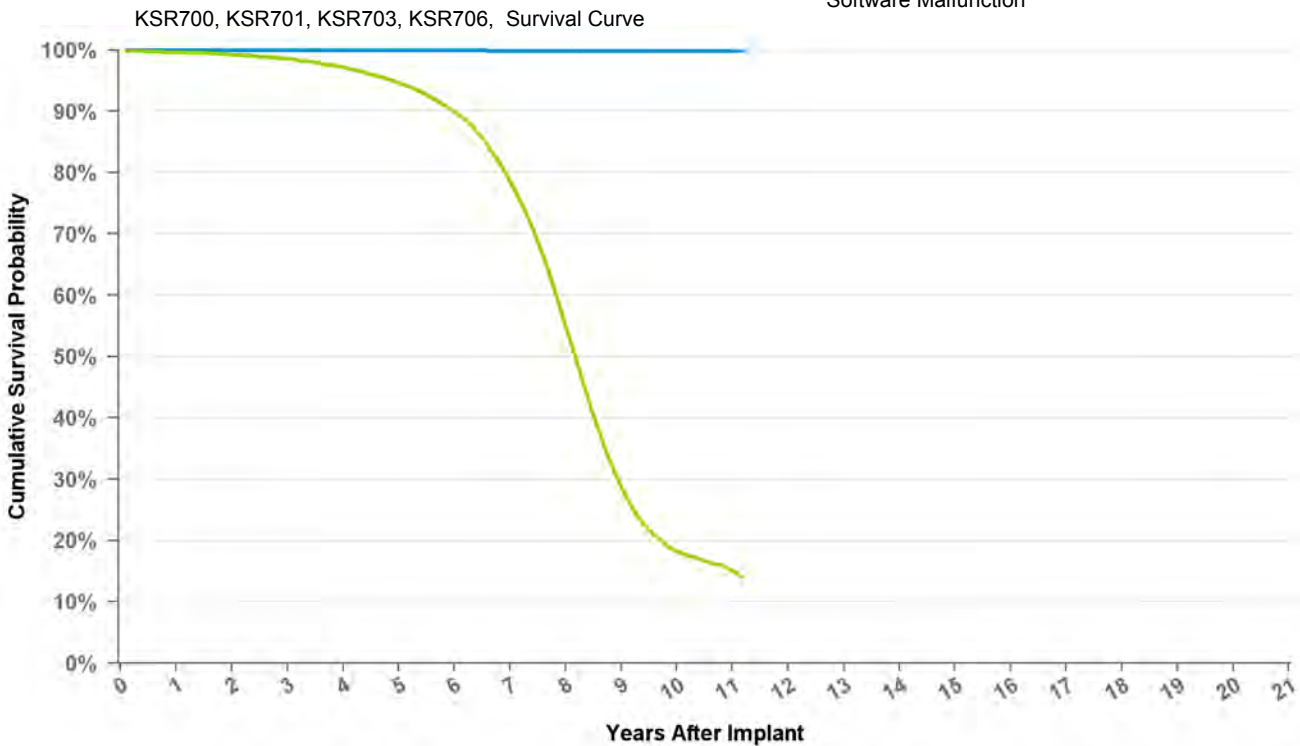

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 134 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.8% | 99.8% | 99.8% | 99.8% |
| Including NBD | 99.6% | 99.2% | 98.6% | 97.2% | 94.6% | 89.9% | 78.6% | 54.9% | 28.8% | 18.3% | 15.1% | 13.9% |
| Effective Sample Size | 48205 | 41529 | 35578 | 30377 | 25558 | 21008 | 15803 | 9014 | 3097 | 1041 | 245 | 135 |

Implantable Pulse Generator

KSR703 Kappa 700 SR

| | |
|---------------------------------------|------------|
| US Market Release Date | 02/08/1999 |
| CE Market Approval Date | 03/20/1998 |
| Registered US Implants | 3,607 |
| Estimated Active US Implants | 284 |
| Normal Battery Depletions (US) | 395 |
| NBG Code | SSIR |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 4 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 4 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 3 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

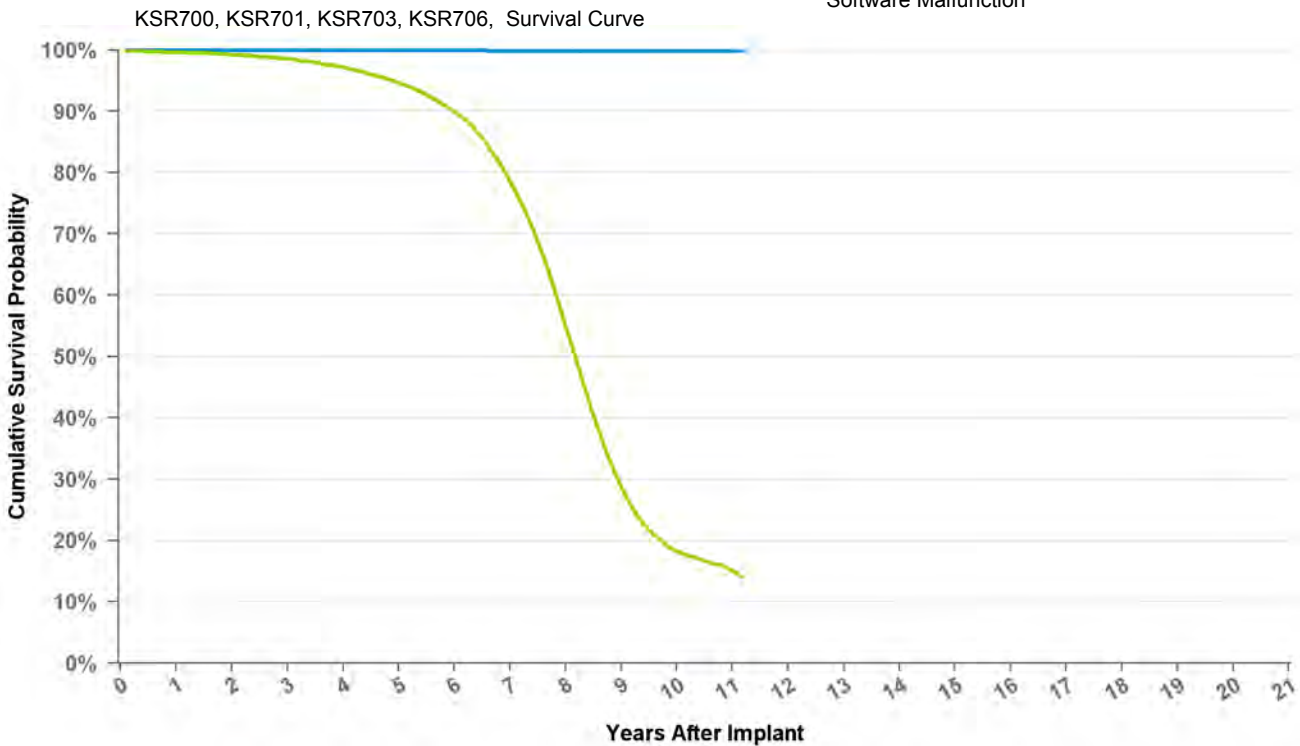

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 134 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.8% | 99.8% | 99.8% | 99.8% |
| Including NBD | 99.6% | 99.2% | 98.6% | 97.2% | 94.6% | 89.9% | 78.6% | 54.9% | 28.8% | 18.3% | 15.1% | 13.9% |
| Effective Sample Size | 48205 | 41529 | 35578 | 30377 | 25558 | 21008 | 15803 | 9014 | 3097 | 1041 | 245 | 135 |


Implantable Pulse Generator

KSR706

Kappa 700 SR

| | |
|---------------------------------------|------------|
| US Market Release Date | 02/09/1999 |
| CE Market Approval Date | 03/20/1998 |
| Registered US Implants | 2,920 |
| Estimated Active US Implants | 234 |
| Normal Battery Depletions (US) | 299 |
| NBG Code | SSIR |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 2 |
| Therapy Not Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

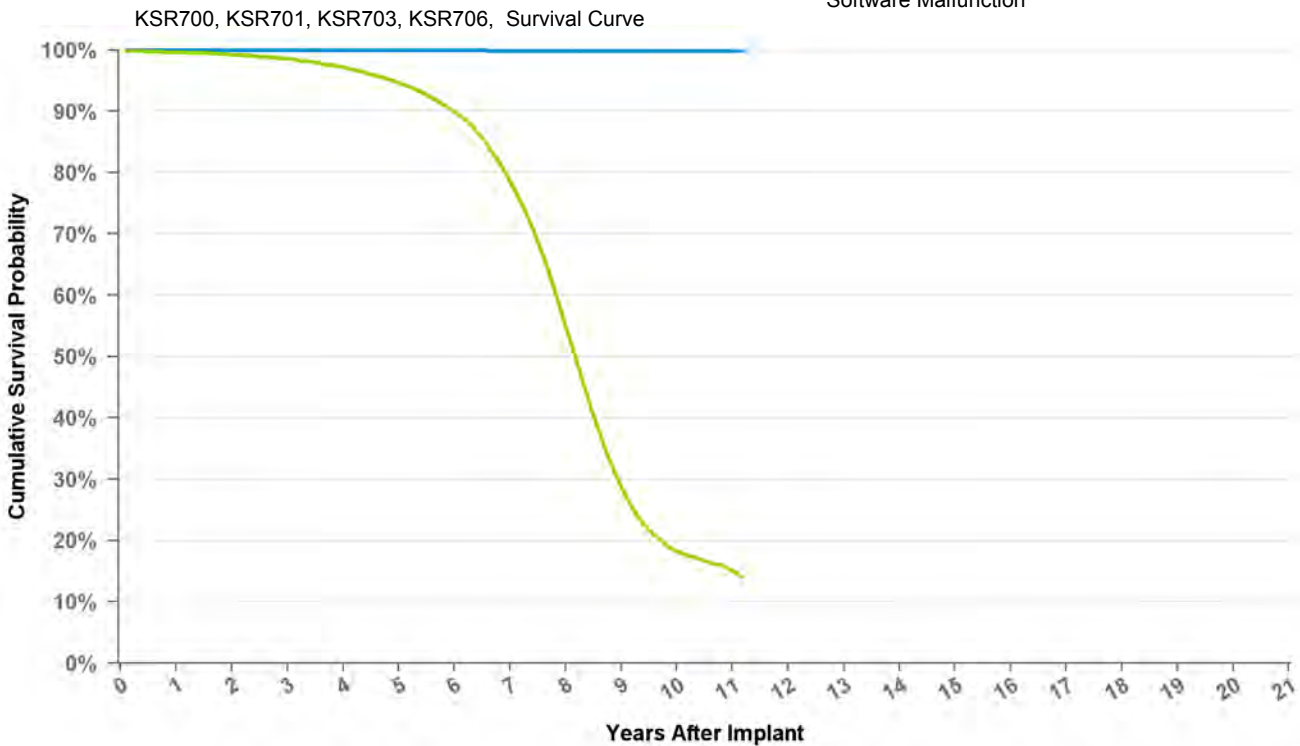

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 134 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.8% | 99.8% | 99.8% | 99.8% |
| Including NBD | 99.6% | 99.2% | 98.6% | 97.2% | 94.6% | 89.9% | 78.6% | 54.9% | 28.8% | 18.3% | 15.1% | 13.9% |
| Effective Sample Size | 48205 | 41529 | 35578 | 30377 | 25558 | 21008 | 15803 | 9014 | 3097 | 1041 | 245 | 135 |


Implantable Pulse Generator

KSR901

Kappa 900 SR

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/09/2002 |
| CE Market Approval Date | 09/28/2001 |
| Registered US Implants | 34,134 |
| Estimated Active US Implants | 3,984 |
| Normal Battery Depletions (US) | 3,988 |
| NBG Code | SSIR |
| Max Delivered Energy | N/A |

| | |
|---|----|
| Total Malfunctions (US) | 15 |
| Therapy Not Compromised Malfunctions | 7 |
| Battery Malfunction | 0 |
| Electrical Component | 6 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 8 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 8 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

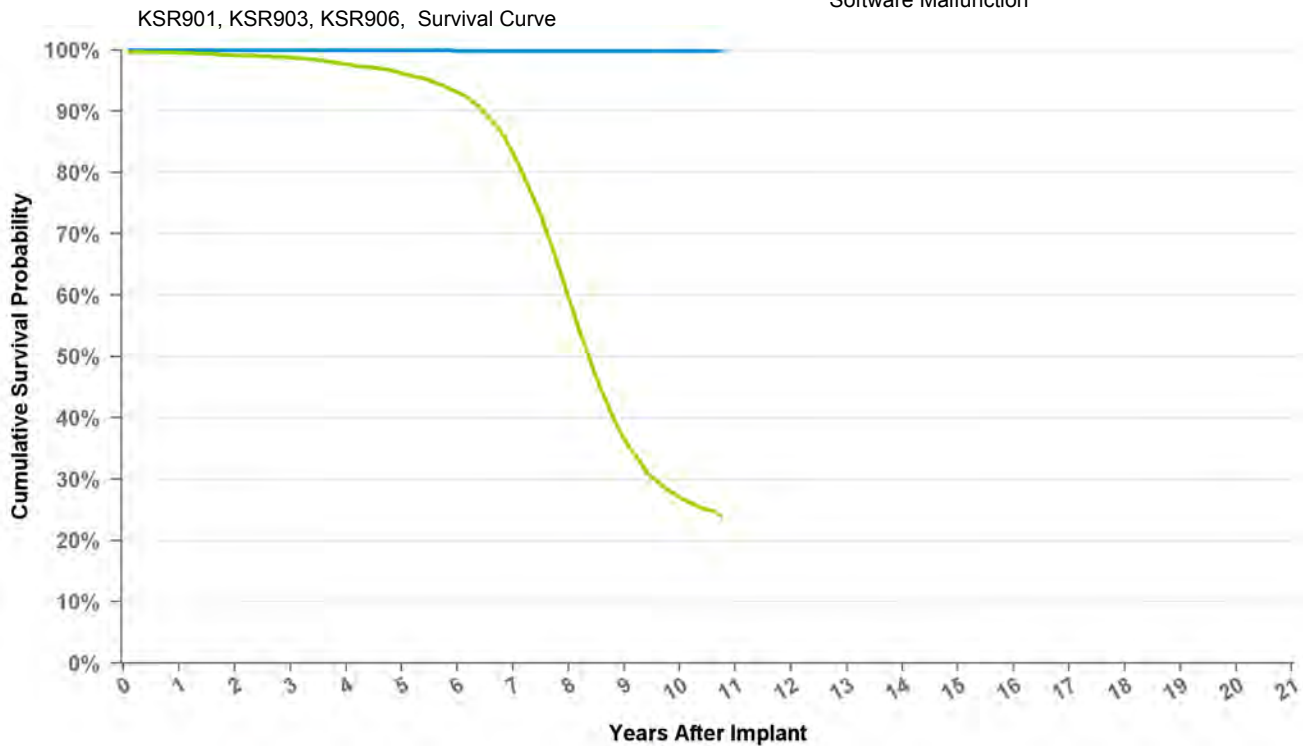

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 129 mo |
|------------------------------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.5% | 99.1% | 98.8% | 97.7% | 96.2% | 93.1% | 83.3% | 59.6% | 36.6% | 26.9% | 23.9% |
| Effective Sample Size | 31945 | 27507 | 23902 | 20586 | 17669 | 14997 | 11832 | 7300 | 2856 | 890 | 203 |

Implantable Pulse Generator

KSR903 Kappa 900 SR

US Market Release Date 01/09/2002

CE Market Approval Date 09/28/2001

Registered US Implants 1,372

Estimated Active US Implants 128

Normal Battery Depletions (US) 164

NBG Code SSIR

Max Delivered Energy N/A

Total Malfunctions (US) 1

Therapy Not Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 1

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

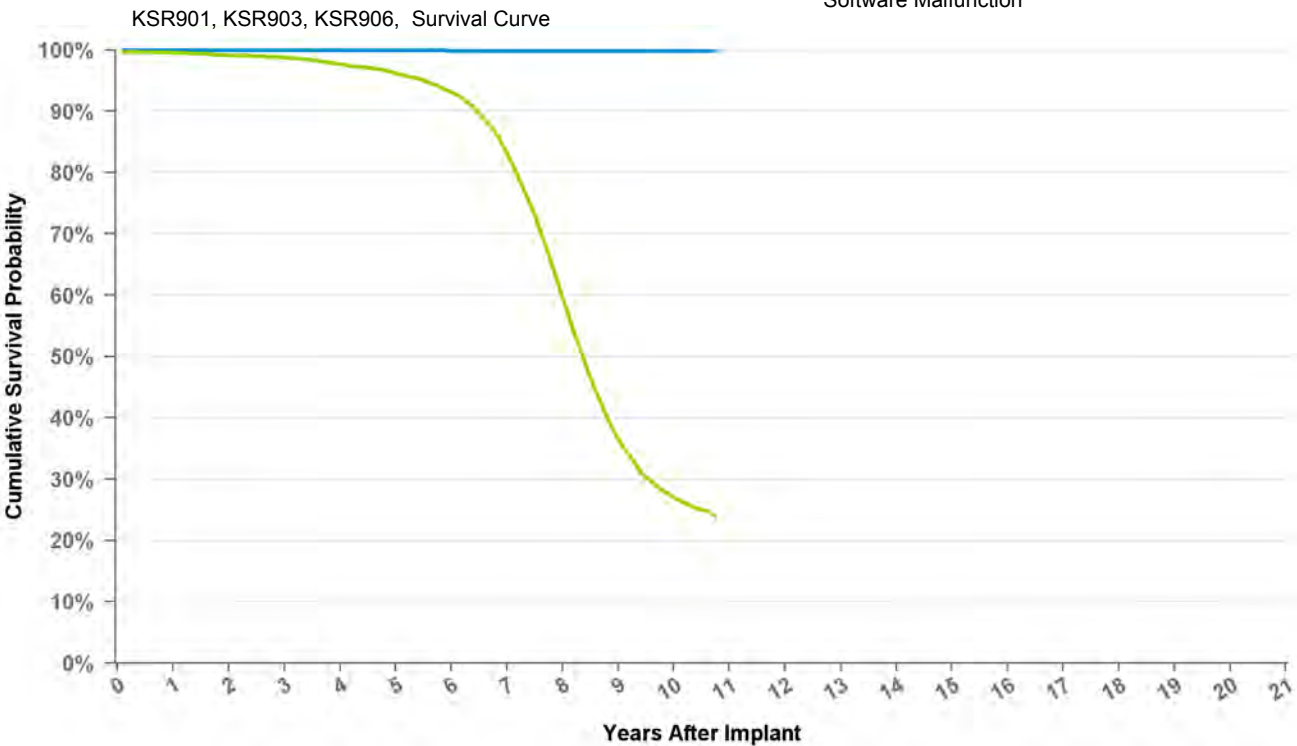

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 129 mo |
|------------------------------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.5% | 99.1% | 98.8% | 97.7% | 96.2% | 93.1% | 83.3% | 59.6% | 36.6% | 26.9% | 23.9% |
| Effective Sample Size | 31945 | 27507 | 23902 | 20586 | 17669 | 14997 | 11832 | 7300 | 2856 | 890 | 203 |


Implantable Pulse Generator

KSR906

Kappa 900 SR

| | |
|---------------------------------------|------------|
| US Market Release Date | 01/09/2002 |
| CE Market Approval Date | 09/28/2001 |
| Registered US Implants | 1,322 |
| Estimated Active US Implants | 125 |
| Normal Battery Depletions (US) | 179 |
| NBG Code | SSIR |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 1 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 1 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

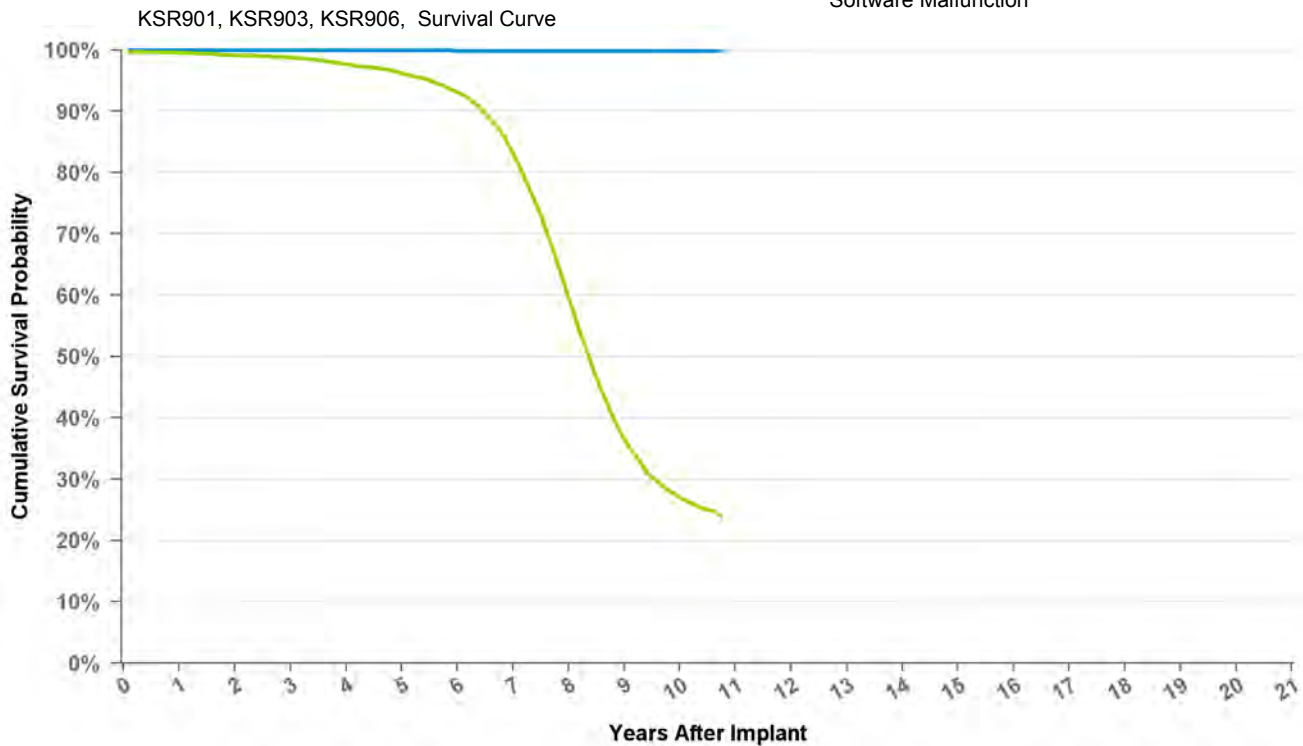

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 129 mo |
|------------------------------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% | 99.9% |
| Including NBD | 99.5% | 99.1% | 98.8% | 97.7% | 96.2% | 93.1% | 83.3% | 59.6% | 36.6% | 26.9% | 23.9% |
| Effective Sample Size | 31945 | 27507 | 23902 | 20586 | 17669 | 14997 | 11832 | 7300 | 2856 | 890 | 203 |

Implantable Pulse Generator

KVDD901 Kappa 900 VDD

US Market Release Date 01/09/2002

CE Market Approval Date 09/28/2001

Registered US Implants 566

Estimated Active US Implants 56

Normal Battery Depletions (US) 81

NBG Code VDD

Max Delivered Energy N/A

Total Malfunctions (US) 1

Therapy Not Compromised Malfunctions 1

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 1

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

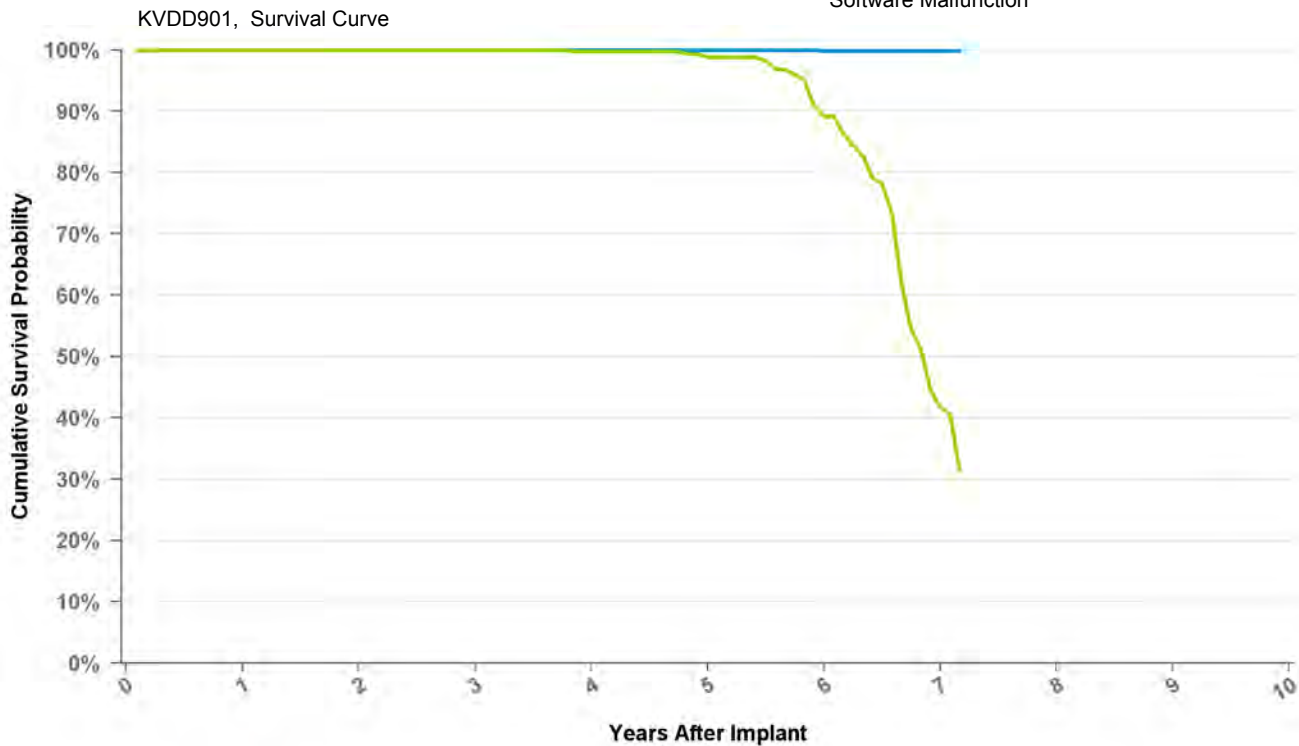

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 86 mo |
|------------------------------|--------|--------|--------|--------|--------|-------|-------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.8% | 99.8% | 99.8% |
| Including NBD | 100.0% | 100.0% | 100.0% | 99.7% | 98.8% | 89.2% | 41.8% | 31.5% |
| Effective Sample Size | 765 | 707 | 651 | 594 | 544 | 435 | 153 | 130 |

Implantable Pulse Generator

P1501DR EnRhythm DR

US Market Release Date 05/05/2005

CE Market Approval Date 08/13/2004

Registered US Implants 110,145

Estimated Active US Implants 48,385

Normal Battery Depletions (US) 5,088

NBG Code DDDRP

Max Delivered Energy N/A

Total Malfunctions (US) 12,000

Therapy Not Compromised Malfunctions 11,947

Battery Malfunction 11,833

Electrical Component 52

Electrical Interconnect 2

Other Malfunction 2

Poss Early Battery Depltn 58

Software Malfunction 0

Therapy Compromised Malfunctions 53

Battery Malfunction 5


Electrical Component 37

Electrical Interconnect 4

Other Malfunction 5

Poss Early Battery Depltn 2

Software Malfunction 0

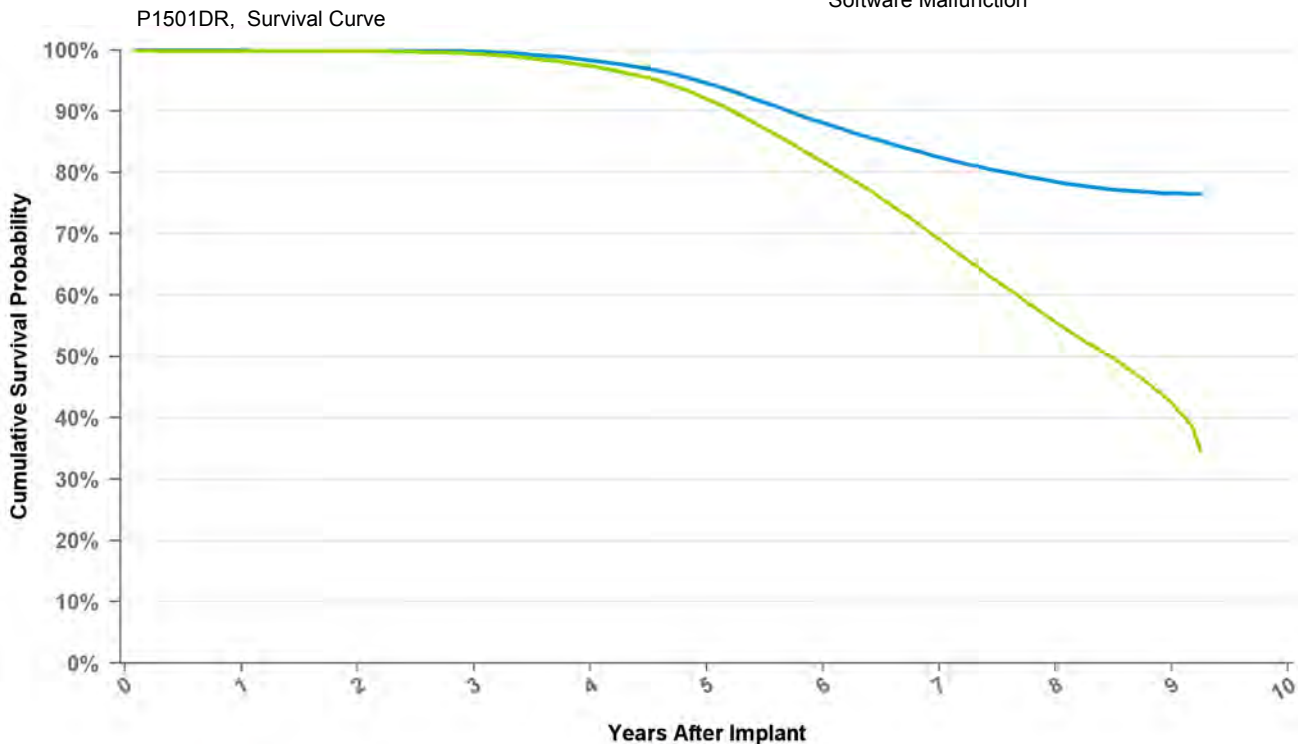

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 111 mo |
|------------------------------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 99.9% | 99.7% | 98.3% | 94.6% | 88.1% | 82.5% | 78.5% | 76.6% | 76.5% |
| Including NBD | 99.9% | 99.8% | 99.3% | 97.4% | 92.0% | 81.7% | 69.1% | 55.6% | 42.3% | 34.5% |
| Effective Sample Size | 104143 | 97728 | 91347 | 81128 | 63885 | 45134 | 29495 | 16173 | 3178 | 506 |

Implantable Pulse Generator

RED01 Relia D

US Market Release Date

CE Market Approval Date 05/07/2008

Registered US Implants 0

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code DDD

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

REDR01, RED01, Survival Curve

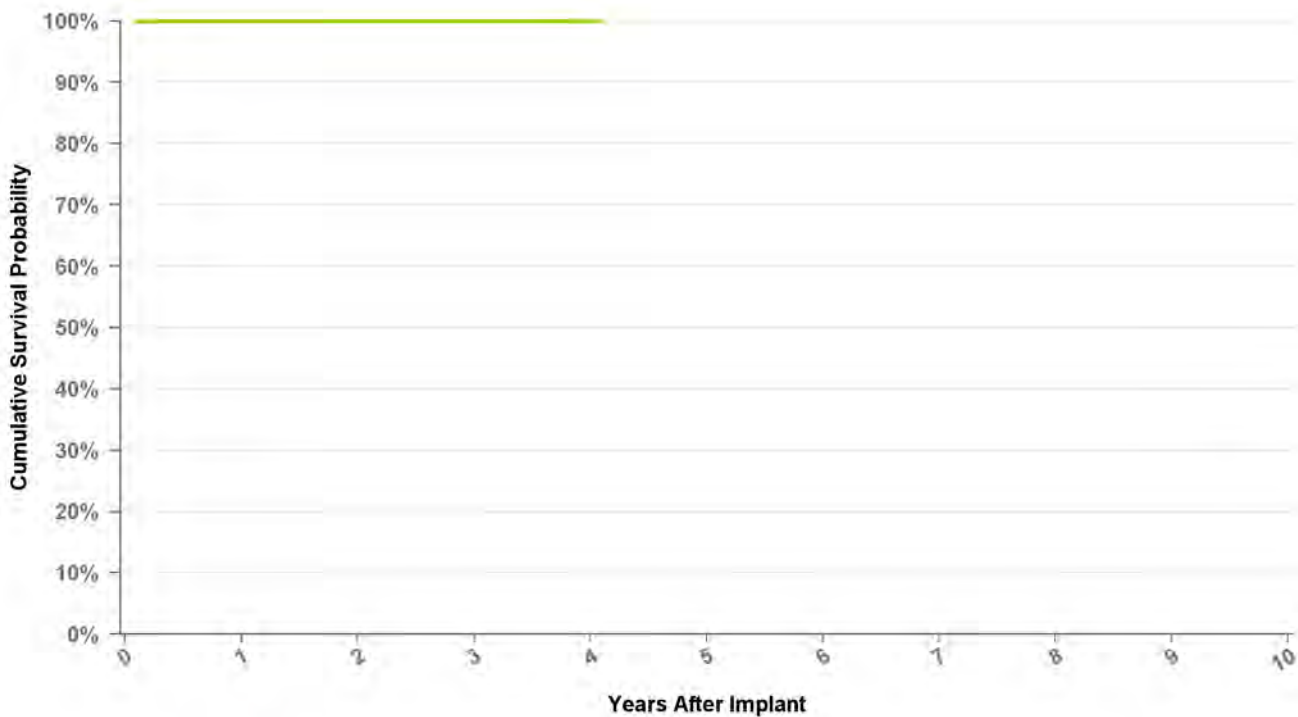

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | at 49 mo |
|------------------------------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Effective Sample Size | 280 | 244 | 191 | 110 | 105 |

Implantable Pulse Generator

REDR01 Relia DR

US Market Release Date

CE Market Approval Date 05/07/2008

Registered US Implants 0

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

REDR01, RED01, Survival Curve

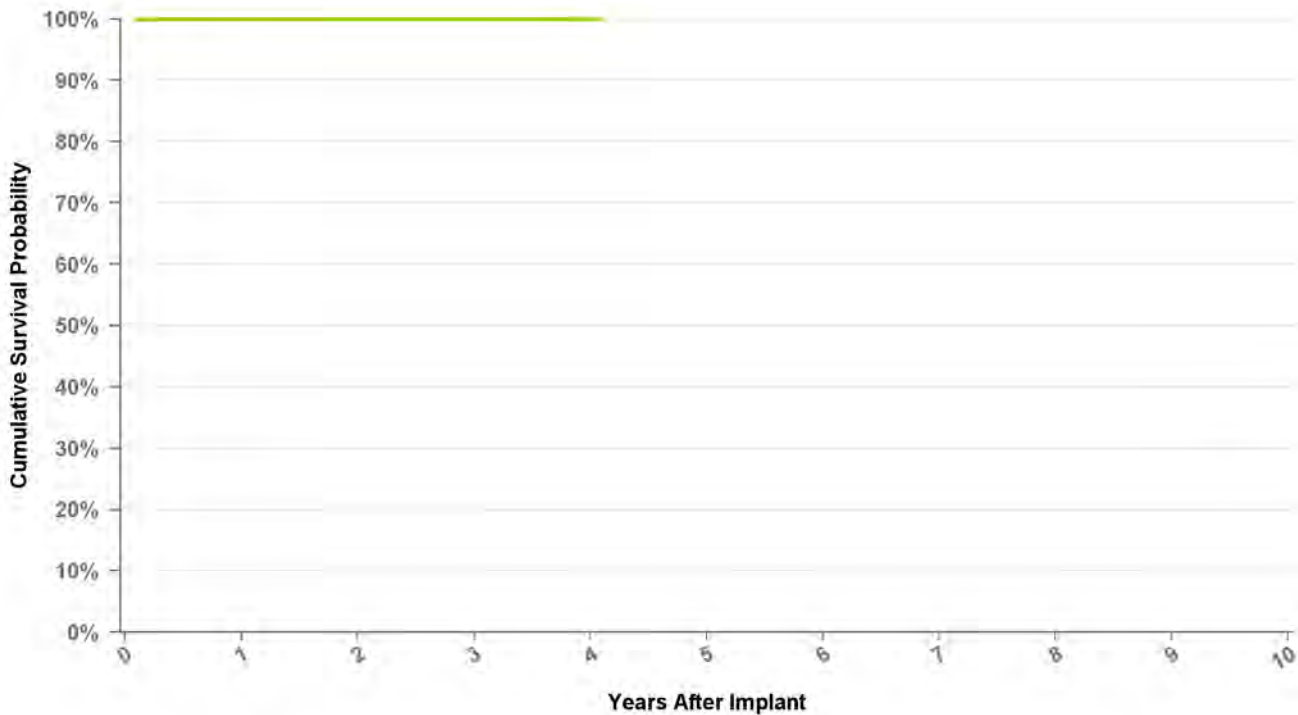

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | at 49 mo |
|-----------------------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Effective Sample Size | 280 | 244 | 191 | 110 | 105 |

Implantable Pulse Generator

RES01 Relia S

US Market Release Date

CE Market Approval Date 05/07/2008

Registered US Implants 2

Estimated Active US Implants 1

Normal Battery Depletions (US) 0

NBG Code AAI/VVI

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

RESR01, RES01, Survival Curve

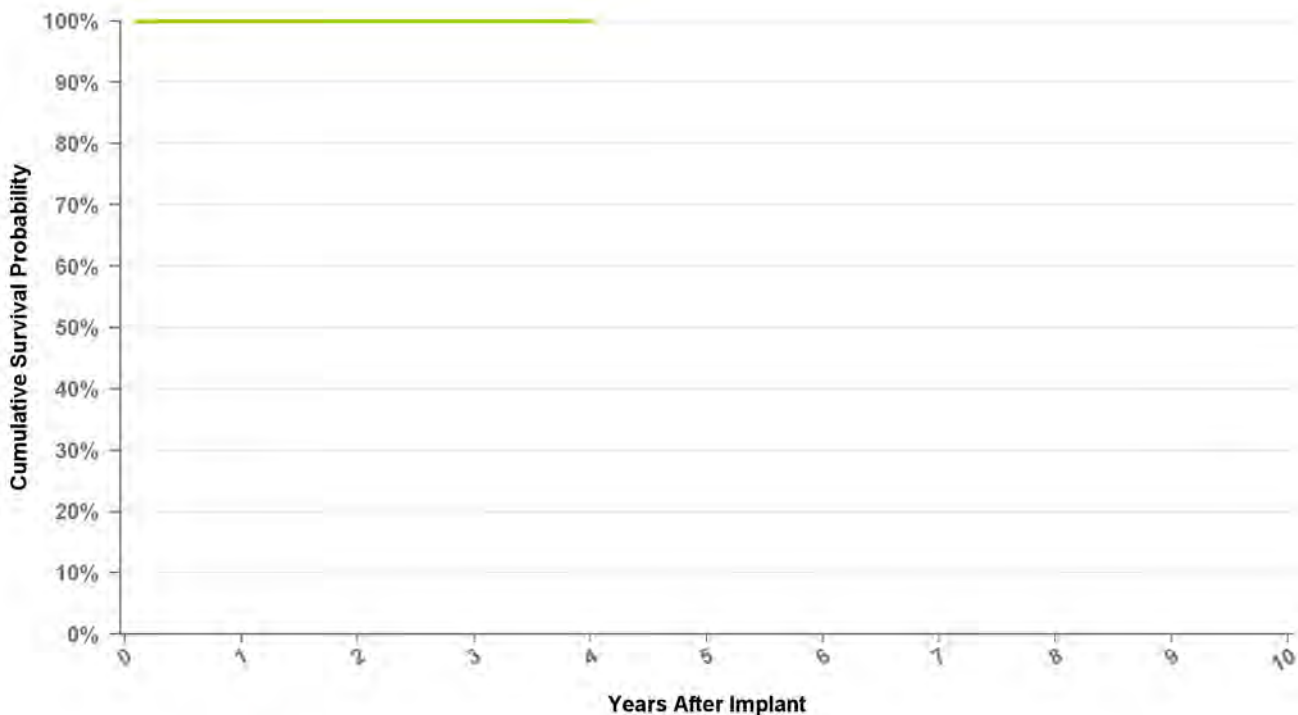

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 48 mo |
|-----------------------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 100.0% |
| Effective Sample Size | 299 | 249 | 182 | 102 |

Implantable Pulse Generator

RESR01 Relia SR

US Market Release Date

CE Market Approval Date 05/07/2008

Registered US Implants 0

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code AAIR/VVIR, AAI/VVI

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

RESR01, RES01, Survival Curve

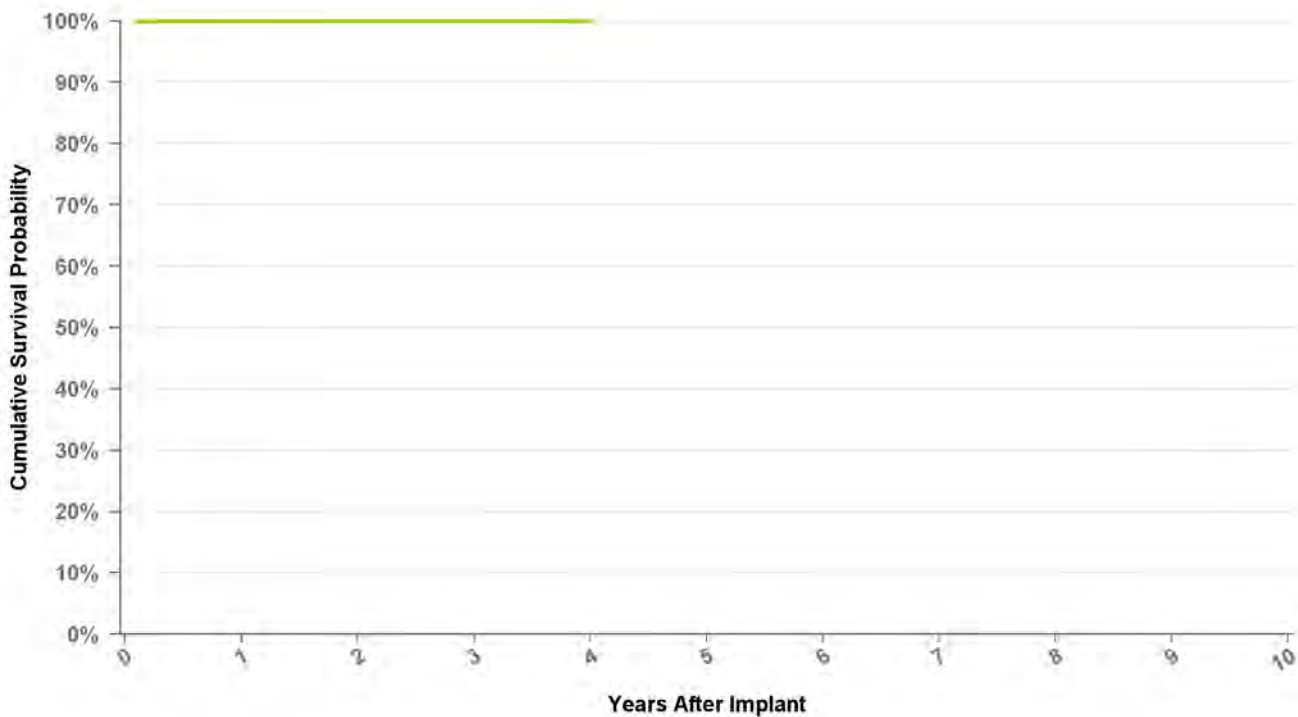

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 48 mo |
|-----------------------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 100.0% | 100.0% |
| Effective Sample Size | 299 | 249 | 182 | 102 |

Implantable Pulse Generator

REVDD01 Relia VDD

US Market Release Date

CE Market Approval Date 05/07/2008

Registered US Implants 0

Estimated Active US Implants 0

Normal Battery Depletions (US) 0

NBG Code VDD

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions

Battery Malfunction 0

Electrical Component 0


Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

REVDD01, Survival Curve

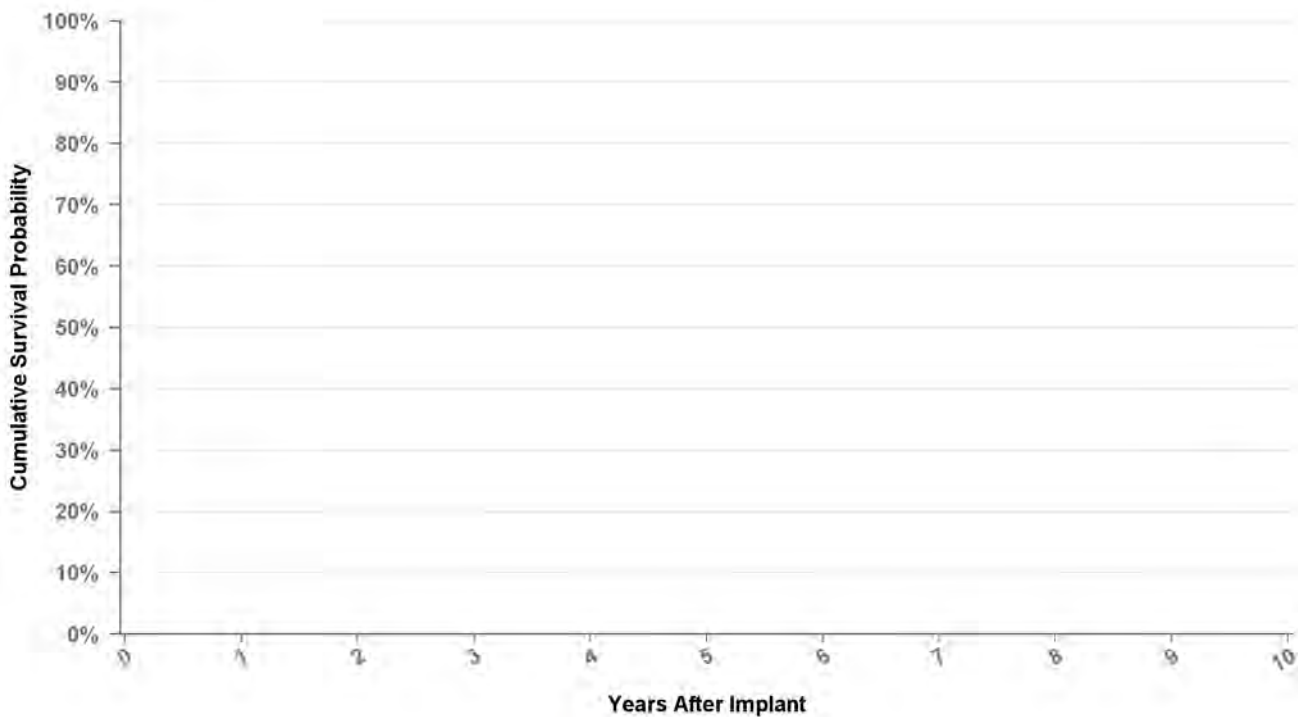

Curve Name



Years

Excluding NBD

Including NBD

Effective Sample Size

Implantable Pulse Generator

RVDR01 Revo MRI SureScan

US Market Release Date 02/08/2011

CE Market Approval Date

Registered US Implants 64,411

Estimated Active US Implants 60,005

Normal Battery Depletions (US) 7

NBG Code DDDRP

Max Delivered Energy N/A

Total Malfunctions (US) 22

Therapy Not Compromised Malfunctions 19

Battery Malfunction 1

Electrical Component 13

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 4

Software Malfunction 1

Therapy Compromised Malfunctions 3

Battery Malfunction 0


Electrical Component 3

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

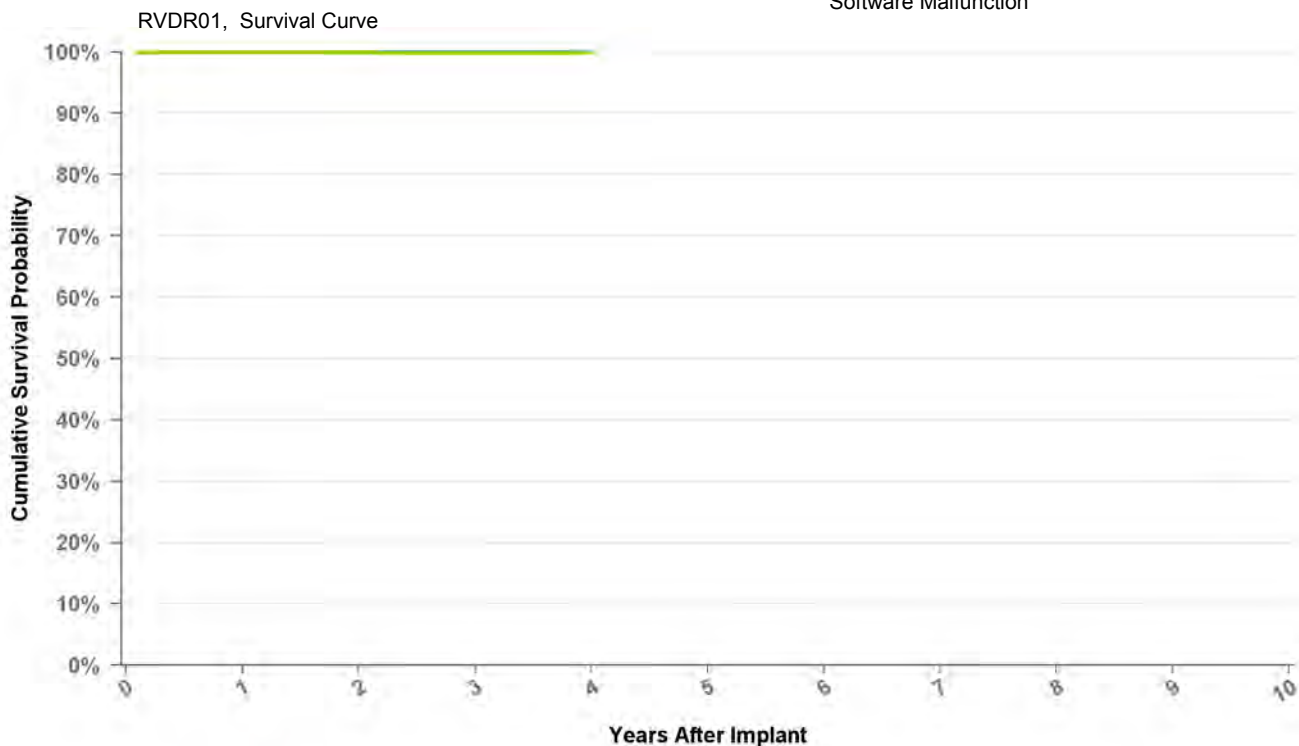

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | at 48 mo |
|------------------------------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 99.9% | 99.9% |
| Effective Sample Size | 59866 | 48475 | 22095 | 368 |

Implantable Pulse Generator


SD203

Sigma 200 D

| | |
|---------------------------------------|------------|
| US Market Release Date | 08/31/1999 |
| CE Market Approval Date | 12/17/1998 |
| Registered US Implants | 225 |
| Estimated Active US Implants | 27 |
| Normal Battery Depletions (US) | 18 |
| NBG Code | DDD |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 1 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 1 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

SDR203, SD203, Survival Curve

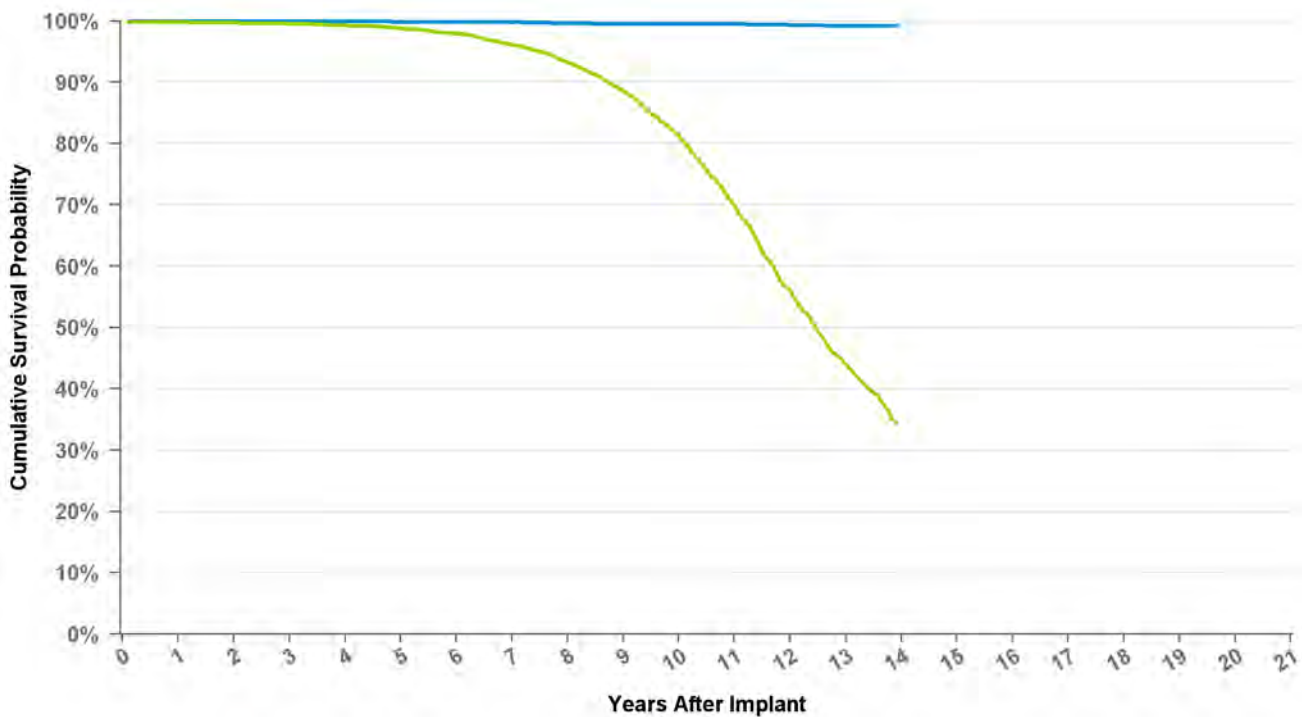

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | at 167 mo |
|------------------------------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.8% | 99.6% | 99.5% | 99.5% | 99.5% | 99.3% | 99.2% | 99.2% |
| Including NBD | 99.8% | 99.7% | 99.5% | 99.3% | 98.8% | 98.0% | 96.1% | 93.2% | 88.6% | 81.3% | 69.9% | 56.0% | 44.1% | 34.4% |
| Effective Sample Size | 14194 | 12721 | 11314 | 10128 | 8991 | 7953 | 6916 | 5993 | 5144 | 4175 | 2980 | 1730 | 821 | 102 |


Implantable Pulse Generator

SD303

Sigma 300 D

| | |
|---------------------------------------|------------|
| US Market Release Date | 08/26/1999 |
| CE Market Approval Date | 12/17/1998 |
| Registered US Implants | 122 |
| Estimated Active US Implants | 30 |
| Normal Battery Depletions (US) | 6 |
| NBG Code | DDD |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 1 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 1 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

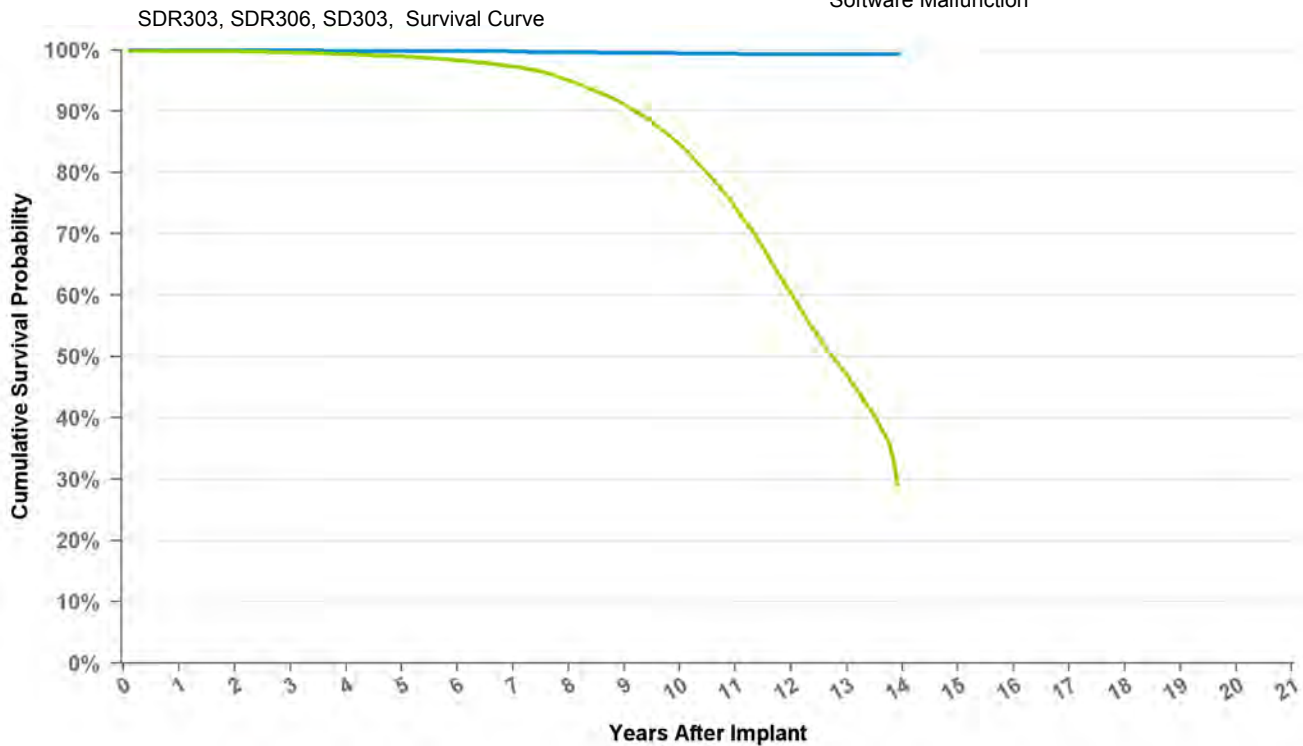

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | at 167 mo |
|------------------------------|--------|--------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.7% | 99.6% | 99.5% | 99.4% | 99.4% | 99.3% | 99.3% | 99.3% |
| Including NBD | 99.8% | 99.8% | 99.6% | 99.3% | 99.0% | 98.3% | 97.3% | 95.0% | 91.1% | 84.6% | 74.3% | 60.3% | 47.1% | 29.1% |
| Effective Sample Size | 96572 | 86490 | 77398 | 69020 | 61448 | 54755 | 48332 | 41257 | 33481 | 24956 | 16447 | 8493 | 3378 | 150 |

Implantable Pulse Generator

SDR203

Sigma 200 DR

US Market Release Date 08/31/1999

CE Market Approval Date 12/17/1998

Registered US Implants 15,644

Estimated Active US Implants 2,430

Normal Battery Depletions (US) 1,214

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 40

Therapy Not Compromised Malfunctions 10

Battery Malfunction 0

Electrical Component 1

Electrical Interconnect 9

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 30

Battery Malfunction 0

Electrical Component 2


Electrical Interconnect 27

Other Malfunction 1

Poss Early Battery Depltn 0

Software Malfunction 0

SDR203, SD203, Survival Curve

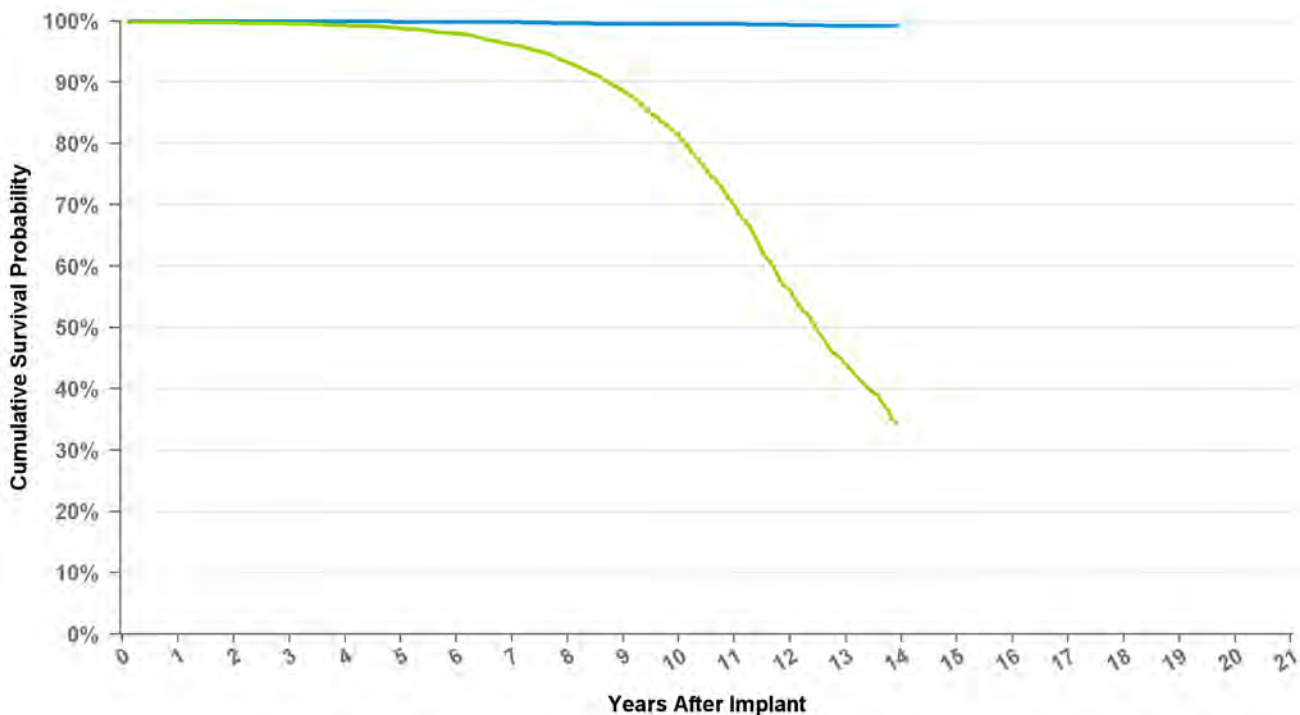

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | at 167 mo |
|-----------------------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.8% | 99.6% | 99.5% | 99.5% | 99.5% | 99.3% | 99.2% | 99.2% |
| Including NBD | 99.8% | 99.7% | 99.5% | 99.3% | 98.8% | 98.0% | 96.1% | 93.2% | 88.6% | 81.3% | 69.9% | 56.0% | 44.1% | 34.4% |
| Effective Sample Size | 14194 | 12721 | 11314 | 10128 | 8991 | 7953 | 6916 | 5993 | 5144 | 4175 | 2980 | 1730 | 821 | 102 |

Implantable Pulse Generator

SDR303 Sigma 300 DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 08/26/1999 |
| CE Market Approval Date | 12/17/1998 |
| Registered US Implants | 105,574 |
| Estimated Active US Implants | 23,077 |
| Normal Battery Depletions (US) | 6,791 |
| NBG Code | DDD/RO |
| Max Delivered Energy | N/A |

| | |
|---|-----|
| Total Malfunctions (US) | 277 |
| Therapy Not Compromised Malfunctions | 60 |
| Battery Malfunction | 0 |
| Electrical Component | 9 |
| Electrical Interconnect | 49 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 1 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 217 |
| Battery Malfunction | 0 |
| Electrical Component | 7 |
| Electrical Interconnect | 209 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

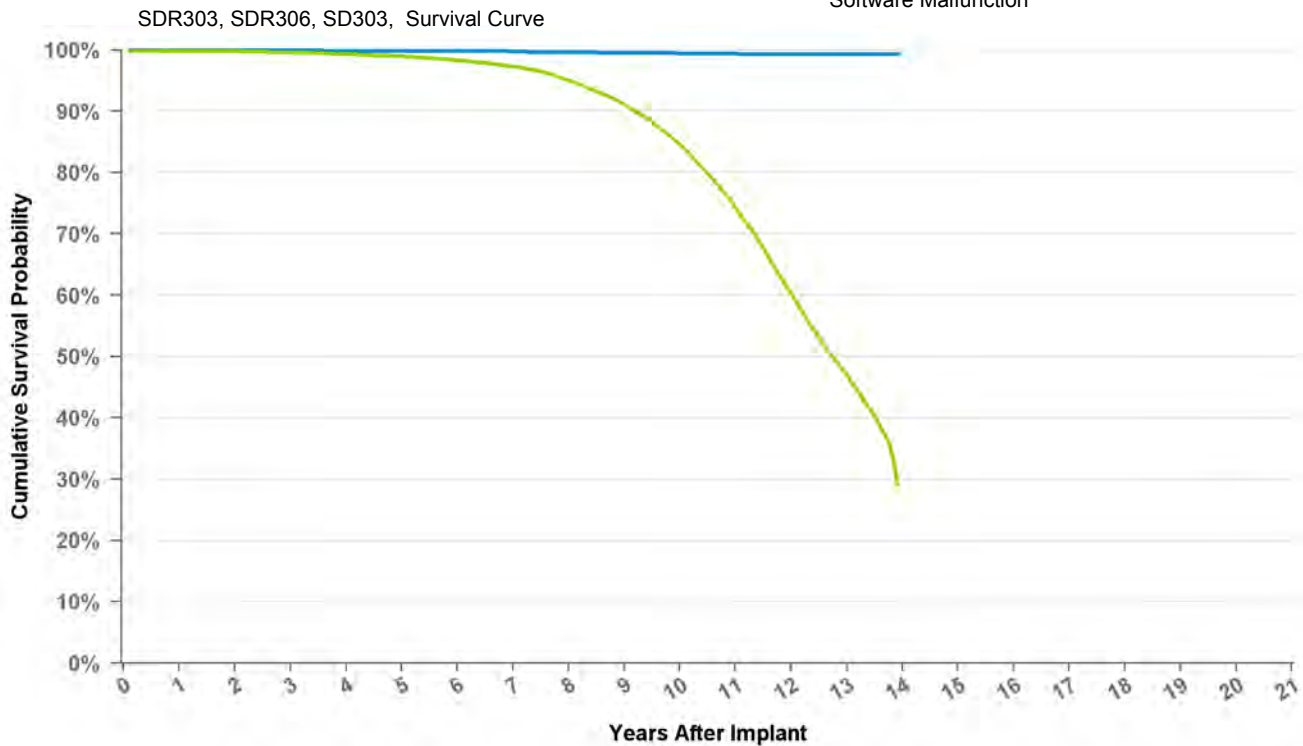

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | at 167 mo |
|------------------------------|--------|--------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.7% | 99.6% | 99.5% | 99.4% | 99.4% | 99.3% | 99.3% | 99.3% |
| Including NBD | 99.8% | 99.8% | 99.6% | 99.3% | 99.0% | 98.3% | 97.3% | 95.0% | 91.1% | 84.6% | 74.3% | 60.3% | 47.1% | 29.1% |
| Effective Sample Size | 96572 | 86490 | 77398 | 69020 | 61448 | 54755 | 48332 | 41257 | 33481 | 24956 | 16447 | 8493 | 3378 | 150 |

Implantable Pulse Generator

SDR306 Sigma 300 DR

| | |
|---------------------------------------|------------|
| US Market Release Date | 08/30/1999 |
| CE Market Approval Date | 12/17/1998 |
| Registered US Implants | 1,209 |
| Estimated Active US Implants | 149 |
| Normal Battery Depletions (US) | 144 |
| NBG Code | DDD/RO |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 5 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 5 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 5 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

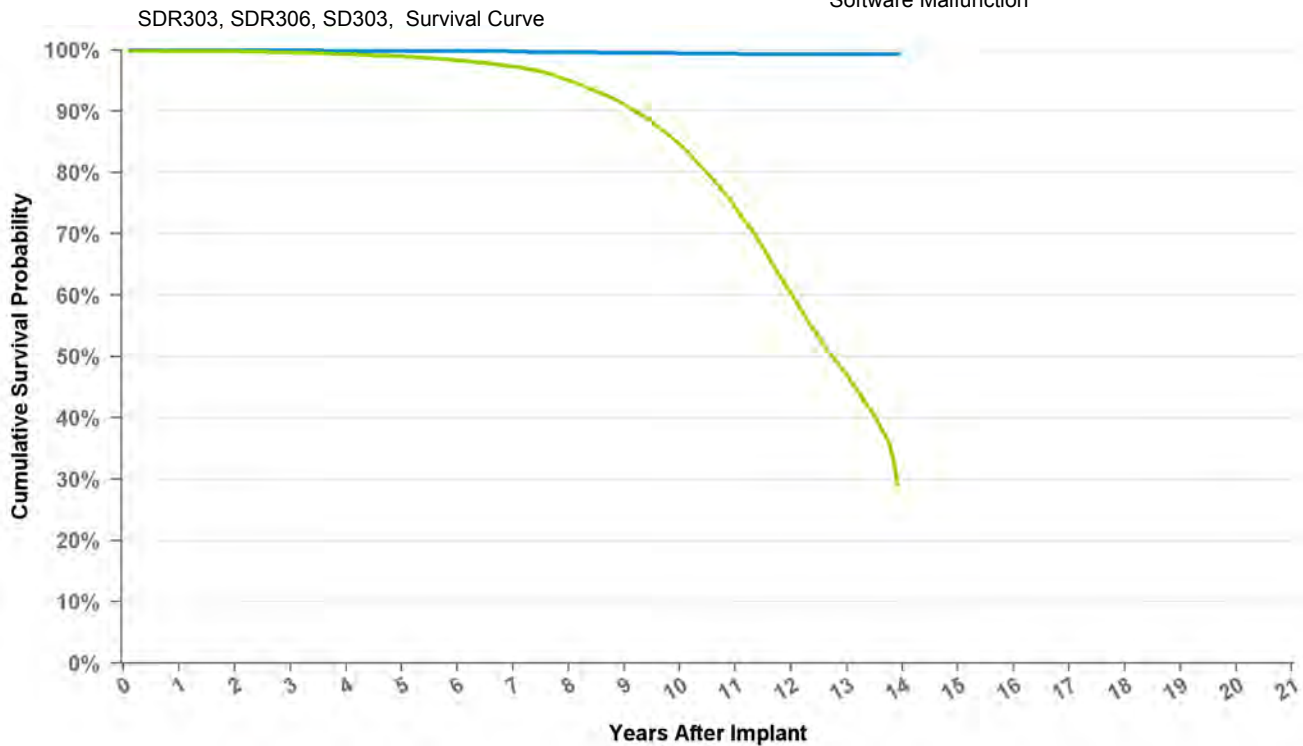

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | at 167 mo |
|------------------------------|--------|--------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.9% | 99.7% | 99.6% | 99.5% | 99.4% | 99.4% | 99.3% | 99.3% | 99.3% |
| Including NBD | 99.8% | 99.8% | 99.6% | 99.3% | 99.0% | 98.3% | 97.3% | 95.0% | 91.1% | 84.6% | 74.3% | 60.3% | 47.1% | 29.1% |
| Effective Sample Size | 96572 | 86490 | 77398 | 69020 | 61448 | 54755 | 48332 | 41257 | 33481 | 24956 | 16447 | 8493 | 3378 | 150 |

Implantable Pulse Generator

SED01

Sensia D

US Market Release Date 07/17/2006

CE Market Approval Date 09/20/2005

Registered US Implants 4

Estimated Active US Implants 3

Normal Battery Depletions (US) 0

NBG Code DDD

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

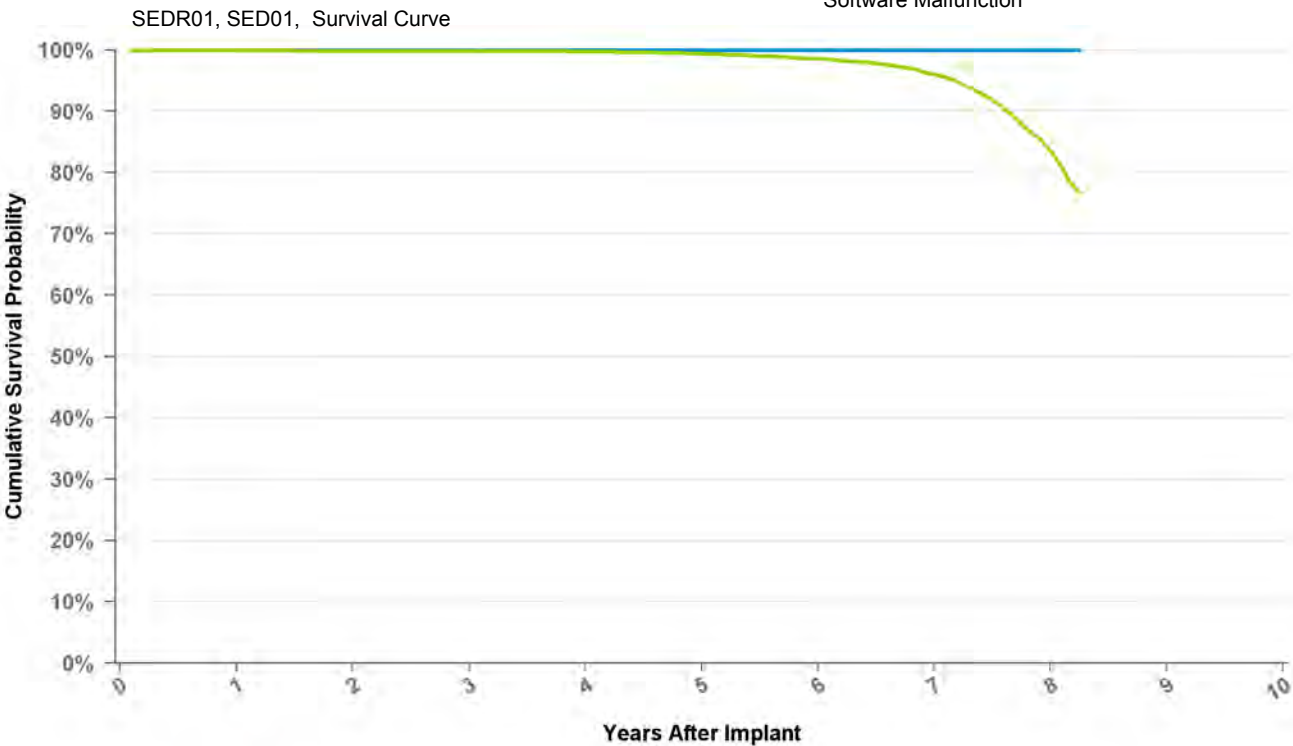

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 99 mo |
|-----------------------|--------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% | 99.9% | 99.7% | 99.4% | 98.6% | 96.0% | 83.6% | 76.8% |
| Effective Sample Size | 122225 | 102461 | 82943 | 63783 | 45604 | 28024 | 12770 | 1828 | 280 |

Implantable Pulse Generator

SEDR01 Sensia DR

US Market Release Date 07/17/2006

CE Market Approval Date 09/20/2005

Registered US Implants 139,942

Estimated Active US Implants 100,149

Normal Battery Depletions (US) 1,151

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 26

Therapy Not Compromised Malfunctions 15

Battery Malfunction 0

Electrical Component 12

Electrical Interconnect 2

Other Malfunction 1

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 11

Battery Malfunction 0


Electrical Component 4

Electrical Interconnect 2

Other Malfunction 5

Poss Early Battery Depltn 0

Software Malfunction 0

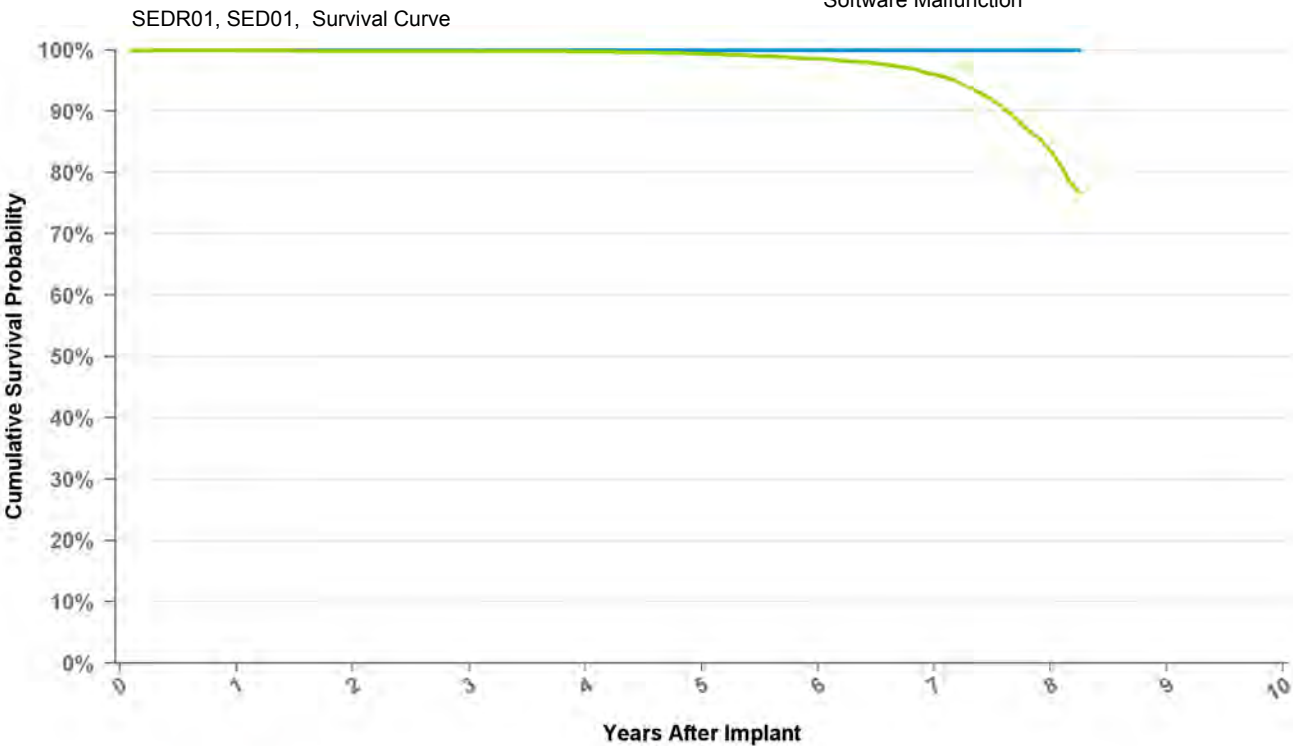

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 99 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% | 99.9% | 99.7% | 99.4% | 98.6% | 96.0% | 83.6% | 76.8% |
| Effective Sample Size | 122225 | 102461 | 82943 | 63783 | 45604 | 28024 | 12770 | 1828 | 280 |

Implantable Pulse Generator

SEDRL1 Sensia DR

US Market Release Date 07/17/2006

CE Market Approval Date 09/20/2005

Registered US Implants 1

Estimated Active US Implants 1

Normal Battery Depletions (US) 0

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

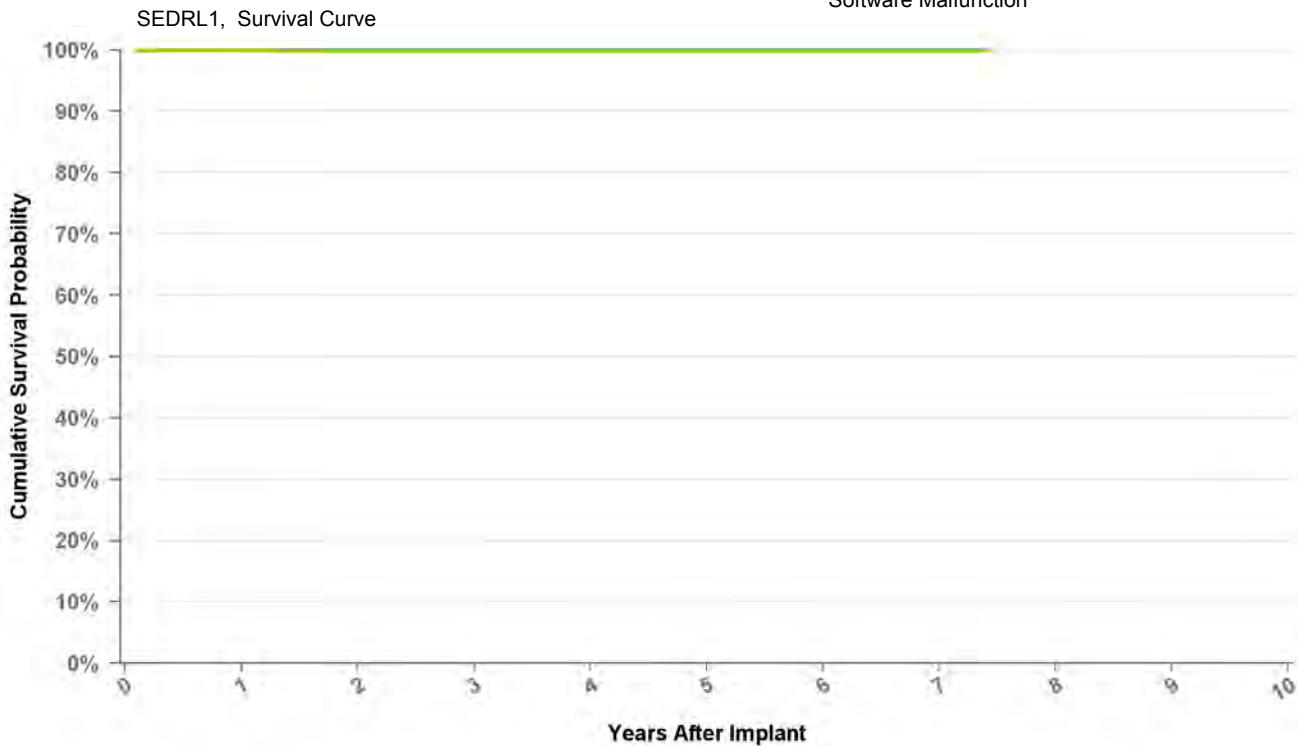

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 89 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.8% | 99.8% | 99.8% | 99.8% | 99.8% | 99.8% | 99.8% |
| Effective Sample Size | 3775 | 3208 | 2591 | 2007 | 1330 | 713 | 305 | 124 |


Implantable Pulse Generator

SES01

Sensia S

| | |
|---------------------------------------|------------|
| US Market Release Date | 07/17/2006 |
| CE Market Approval Date | 09/20/2005 |
| Registered US Implants | 4 |
| Estimated Active US Implants | 0 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | SSI |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

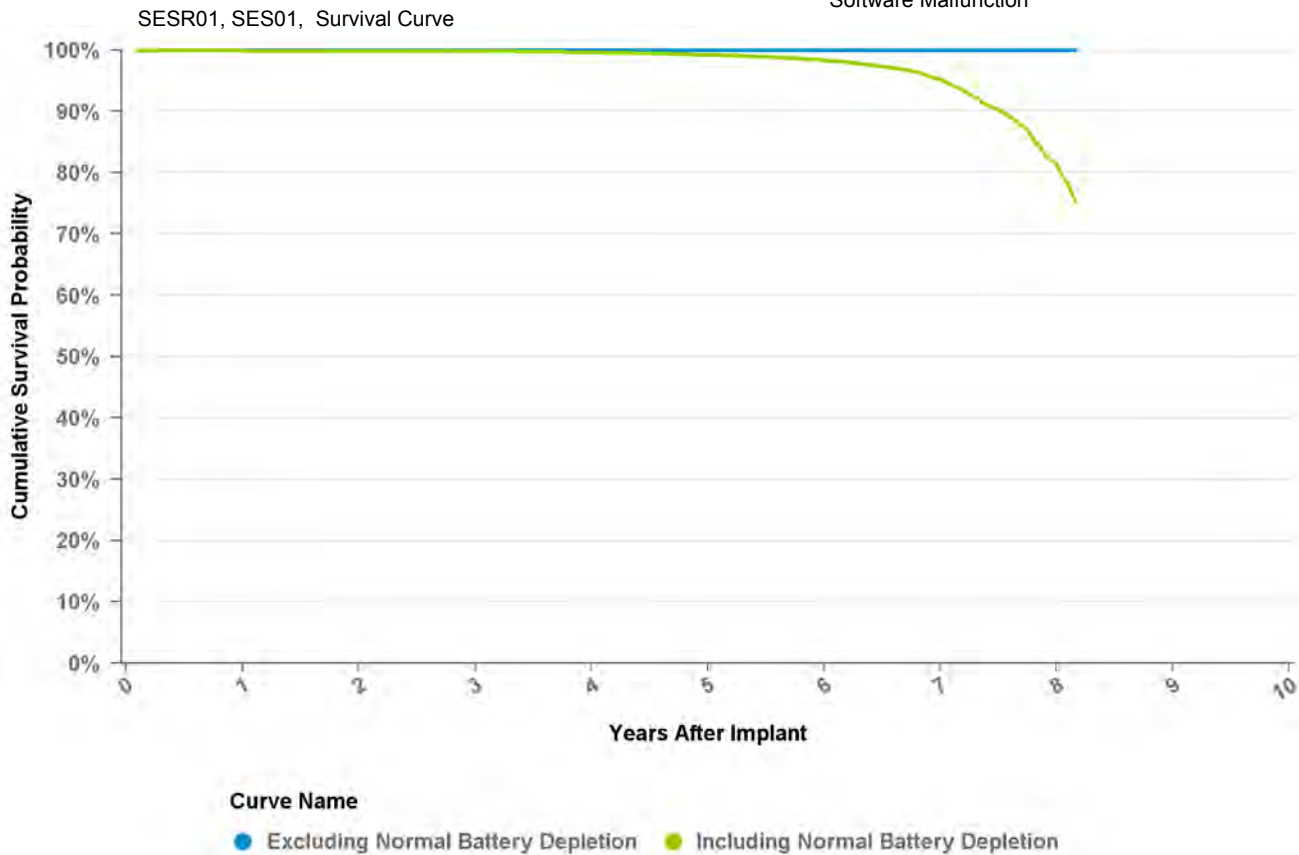


| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 98 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.9% | 99.9% | 99.8% | 99.6% | 99.2% | 98.3% | 95.2% | 81.1% | 75.2% |
| Effective Sample Size | 86855 | 69252 | 52668 | 38157 | 25923 | 15053 | 6387 | 717 | 188 |

Implantable Pulse Generator

SESR01 Sensia SR

| | |
|---------------------------------------|------------|
| US Market Release Date | 07/17/2006 |
| CE Market Approval Date | 09/20/2005 |
| Registered US Implants | 102,785 |
| Estimated Active US Implants | 69,355 |
| Normal Battery Depletions (US) | 710 |
| NBG Code | SSIR |
| Max Delivered Energy | N/A |

| | |
|---|----|
| Total Malfunctions (US) | 10 |
| Therapy Not Compromised Malfunctions | 7 |
| Battery Malfunction | 0 |
| Electrical Component | 6 |
| Electrical Interconnect | 0 |
| Other Malfunction | 1 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 3 |
| Battery Malfunction | 0 |
| Electrical Component | 2 |
| Electrical Interconnect | 1 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

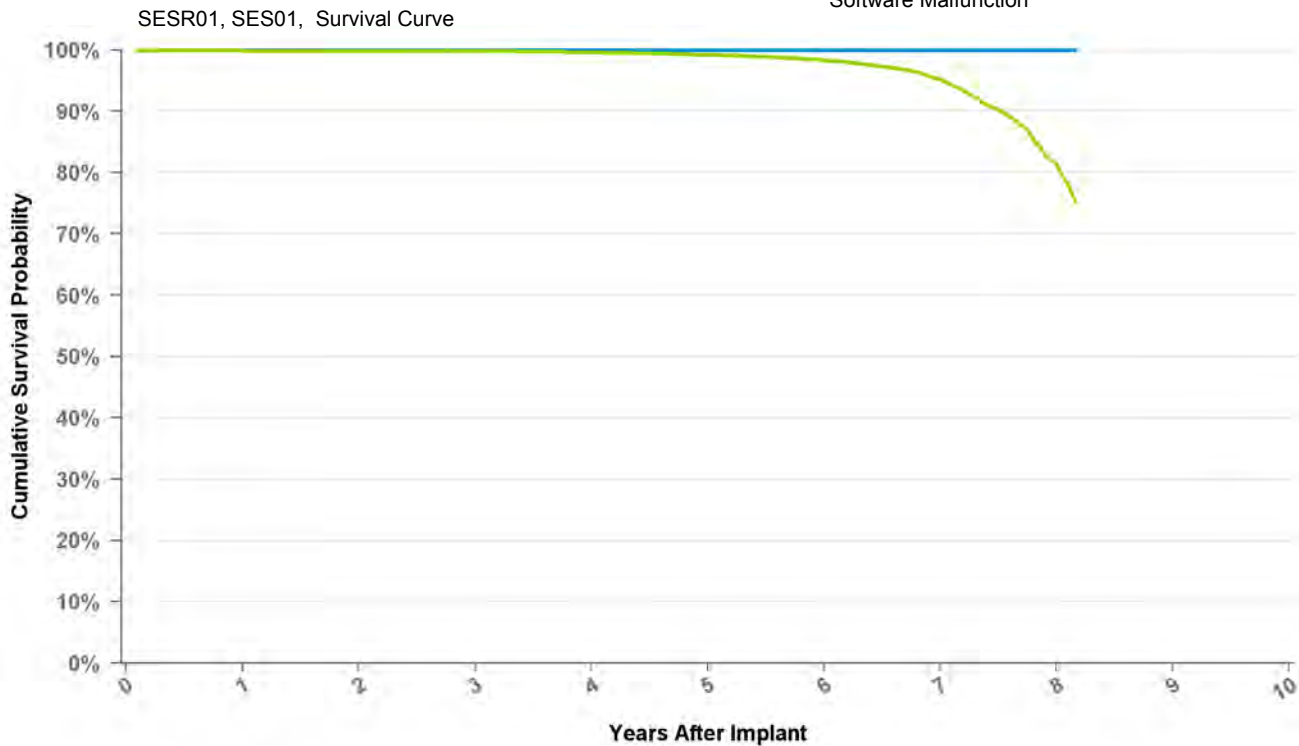

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 98 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 99.9% | 99.9% | 99.8% | 99.6% | 99.2% | 98.3% | 95.2% | 81.1% | 75.2% |
| Effective Sample Size | 86855 | 69252 | 52668 | 38157 | 25923 | 15053 | 6387 | 717 | 188 |


Implantable Pulse Generator

SS103

Sigma 100 S

| | |
|---------------------------------------|------------|
| US Market Release Date | 08/30/1999 |
| CE Market Approval Date | 12/17/1998 |
| Registered US Implants | 767 |
| Estimated Active US Implants | 92 |
| Normal Battery Depletions (US) | 27 |
| NBG Code | SSI |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

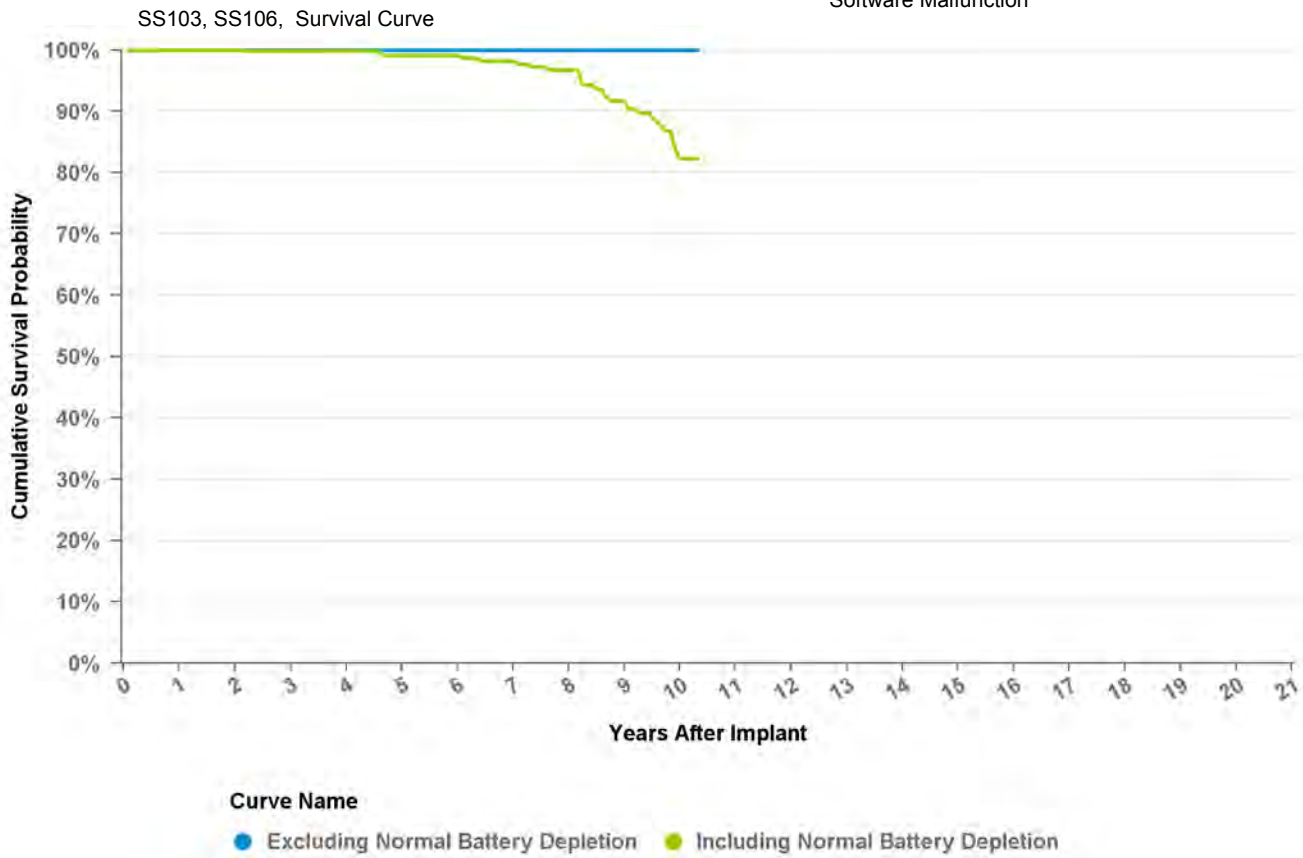

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 124 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 99.8% | 99.8% | 99.1% | 99.1% | 98.2% | 96.7% | 91.7% | 82.3% | 82.3% |
| Effective Sample Size | 634 | 507 | 406 | 331 | 263 | 234 | 201 | 171 | 138 | 109 | 101 |

Implantable Pulse Generator

SS106

Sigma 100 S

US Market Release Date 08/30/1999

CE Market Approval Date 12/17/1998

Registered US Implants 68

Estimated Active US Implants 4

Normal Battery Depletions (US) 7

NBG Code SSI

Max Delivered Energy N/A

Total Malfunctions (US) 0

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 0

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

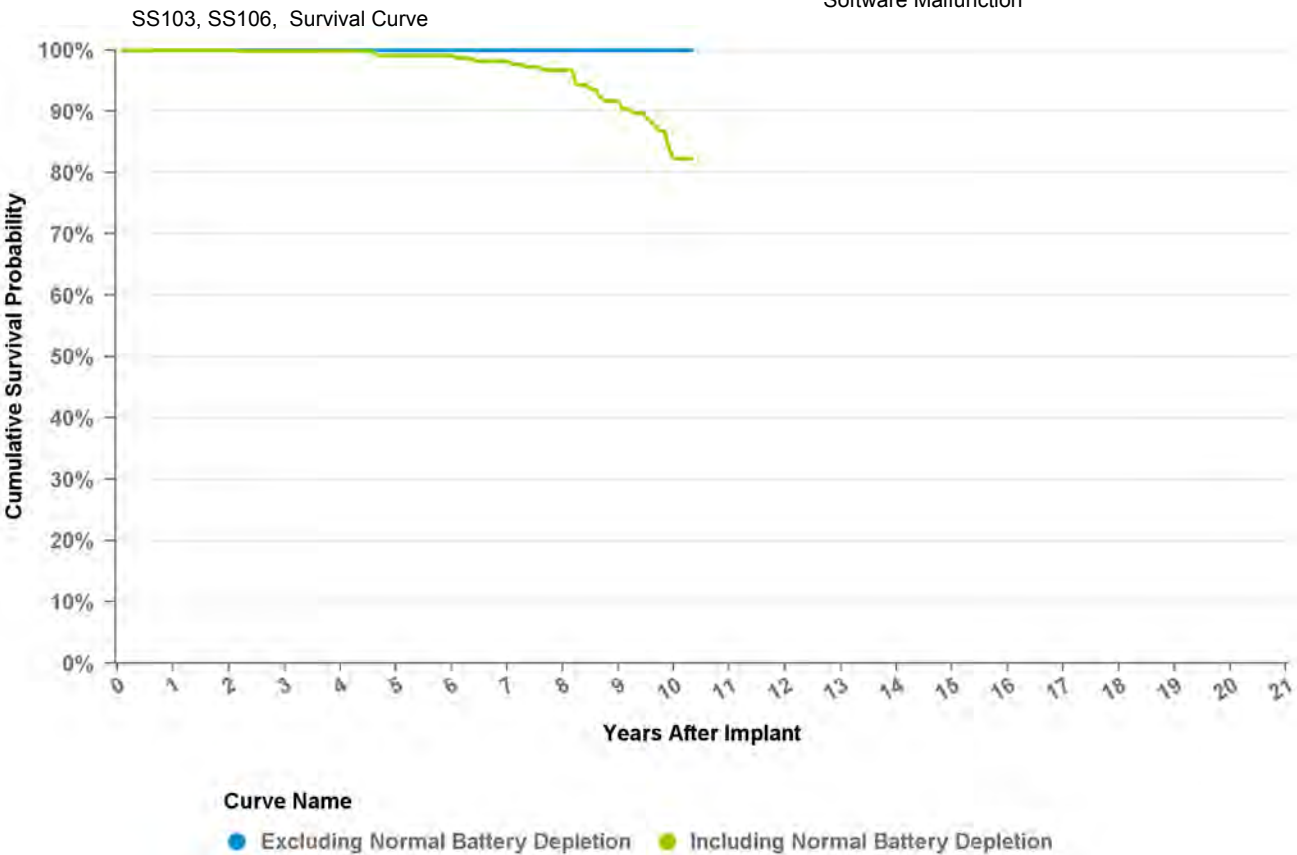

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 124 mo |
|-----------------------|--------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 100.0% | 99.8% | 99.8% | 99.1% | 99.1% | 98.2% | 96.7% | 91.7% | 82.3% | 82.3% |
| Effective Sample Size | 634 | 507 | 406 | 331 | 263 | 234 | 201 | 171 | 138 | 109 | 101 |


Implantable Pulse Generator

SS203

Sigma 200 S

| | |
|---------------------------------------|------------|
| US Market Release Date | 08/30/1999 |
| CE Market Approval Date | |
| Registered US Implants | 4 |
| Estimated Active US Implants | 1 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | SSI |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

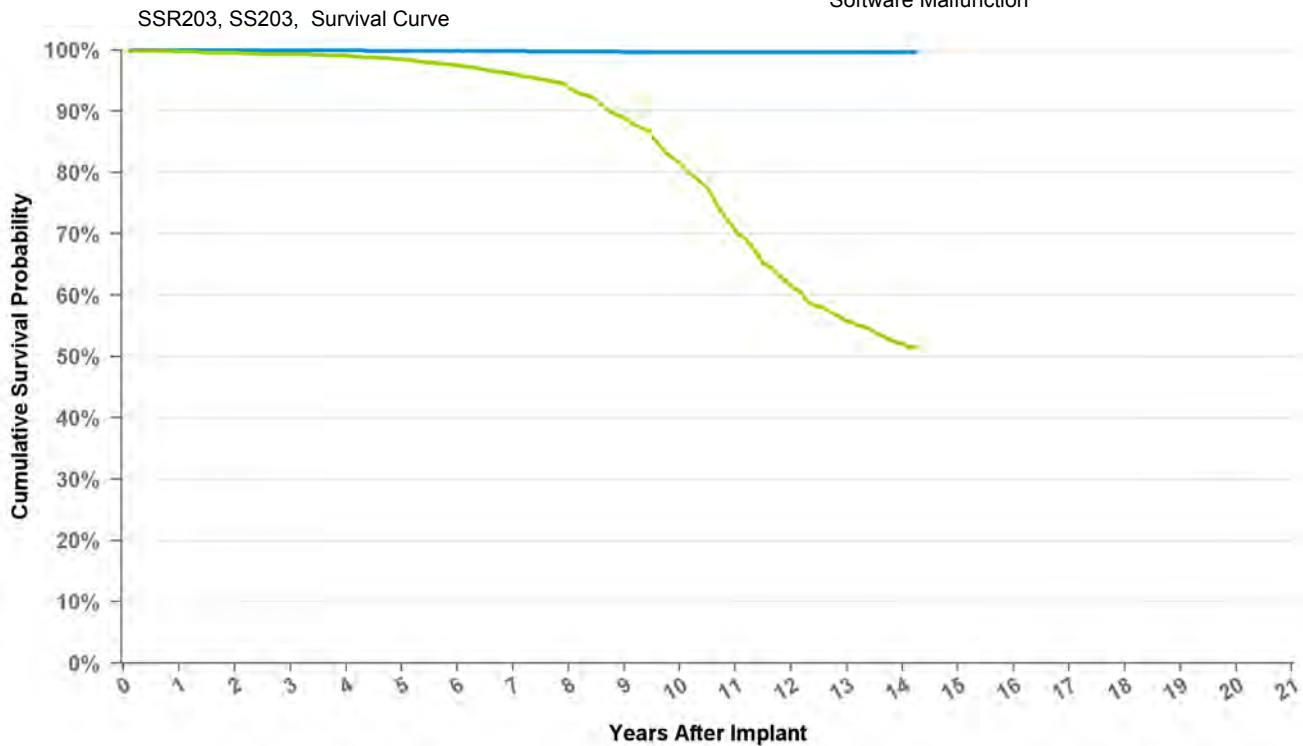

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | 14 | at 171 mo |
|------------------------------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.8% | 99.7% | 99.6% | 99.6% | 99.6% | 99.6% | 99.6% | 99.6% | 99.6% |
| Including NBD | 99.7% | 99.5% | 99.3% | 99.1% | 98.5% | 97.5% | 96.1% | 93.8% | 88.9% | 81.6% | 70.6% | 61.6% | 55.7% | 52.2% | 51.5% |
| Effective Sample Size | 10339 | 8716 | 7406 | 6354 | 5454 | 4722 | 4045 | 3562 | 3052 | 2493 | 1852 | 1252 | 788 | 267 | 133 |


Implantable Pulse Generator

SS303

Sigma 300 S

| | |
|---------------------------------------|------------|
| US Market Release Date | 09/15/1999 |
| CE Market Approval Date | 12/17/1998 |
| Registered US Implants | 221 |
| Estimated Active US Implants | 50 |
| Normal Battery Depletions (US) | 0 |
| NBG Code | SSI |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 0 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

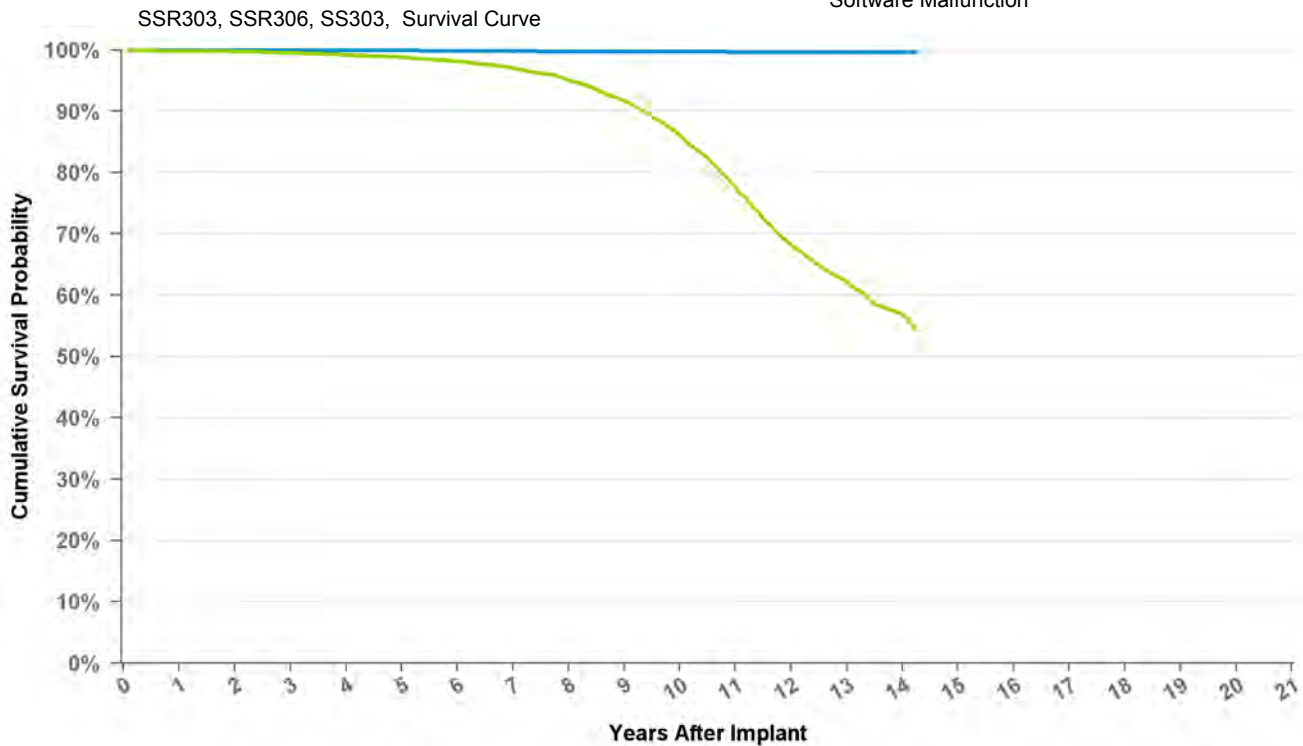

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | 14 | at 171 mo |
|------------------------------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.8% | 99.7% | 99.7% | 99.7% | 99.6% | 99.6% | 99.6% | 99.6% | 99.6% |
| Including NBD | 99.9% | 99.7% | 99.5% | 99.2% | 98.8% | 98.2% | 97.0% | 95.0% | 91.7% | 86.0% | 77.6% | 68.2% | 62.3% | 56.9% | 54.4% |
| Effective Sample Size | 47121 | 39977 | 34124 | 29348 | 25390 | 22076 | 19201 | 16101 | 13053 | 9933 | 6763 | 3868 | 2056 | 500 | 119 |


Implantable Pulse Generator

SSR203

Sigma 200 SR

| | |
|---------------------------------------|------------|
| US Market Release Date | 09/02/1999 |
| CE Market Approval Date | |
| Registered US Implants | 12,124 |
| Estimated Active US Implants | 1,483 |
| Normal Battery Depletions (US) | 584 |
| NBG Code | SSIR |
| Max Delivered Energy | N/A |

| | |
|---|----|
| Total Malfunctions (US) | 14 |
| Therapy Not Compromised Malfunctions | 0 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 14 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 14 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

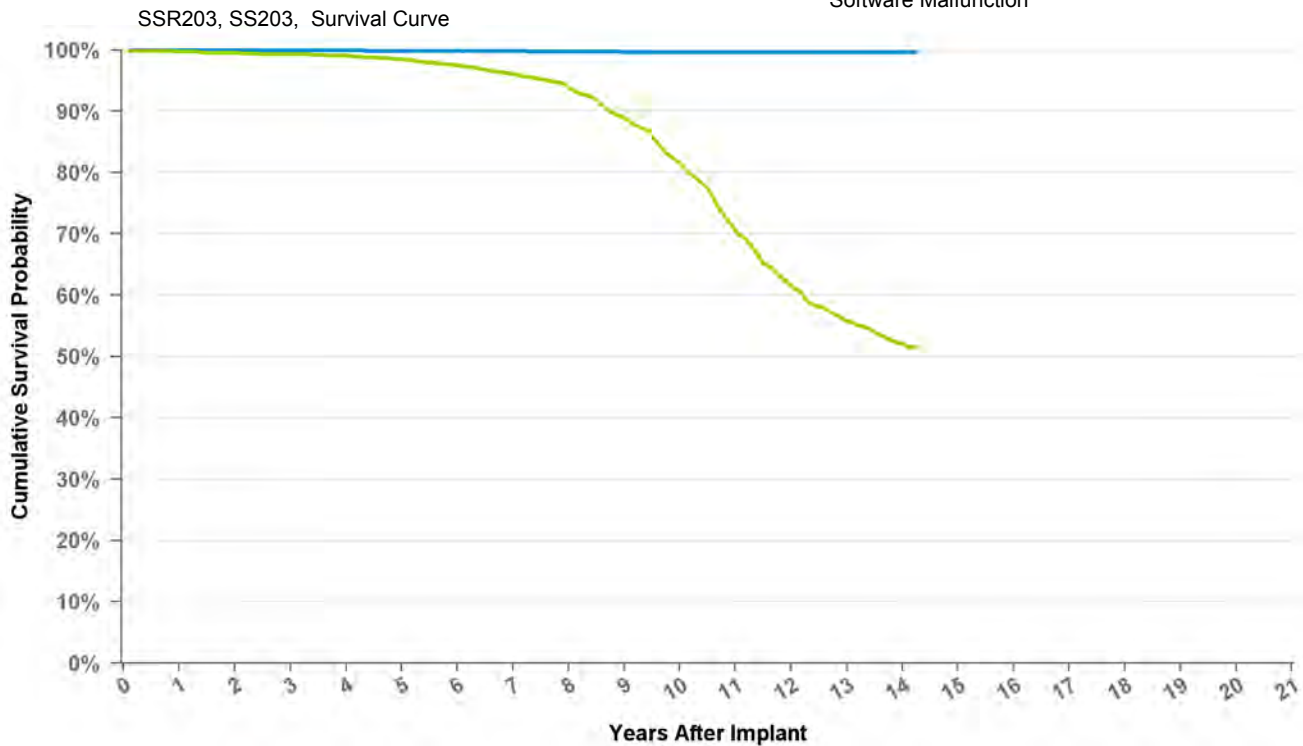

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | 14 | at 171 mo |
|------------------------------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.9% | 99.8% | 99.7% | 99.6% | 99.6% | 99.6% | 99.6% | 99.6% | 99.6% | 99.6% |
| Including NBD | 99.7% | 99.5% | 99.3% | 99.1% | 98.5% | 97.5% | 96.1% | 93.8% | 88.9% | 81.6% | 70.6% | 61.6% | 55.7% | 52.2% | 51.5% |
| Effective Sample Size | 10339 | 8716 | 7406 | 6354 | 5454 | 4722 | 4045 | 3562 | 3052 | 2493 | 1852 | 1252 | 788 | 267 | 133 |


Implantable Pulse Generator

SSR303

Sigma 300 SR

| | |
|---------------------------------------|------------|
| US Market Release Date | 08/30/1999 |
| CE Market Approval Date | 12/17/1998 |
| Registered US Implants | 51,699 |
| Estimated Active US Implants | 8,455 |
| Normal Battery Depletions (US) | 1,999 |
| NBG Code | SSIR |
| Max Delivered Energy | N/A |

| | |
|---|----|
| Total Malfunctions (US) | 57 |
| Therapy Not Compromised Malfunctions | 14 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 12 |
| Other Malfunction | 2 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 43 |
| Battery Malfunction | 0 |
| Electrical Component | 3 |
| Electrical Interconnect | 40 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

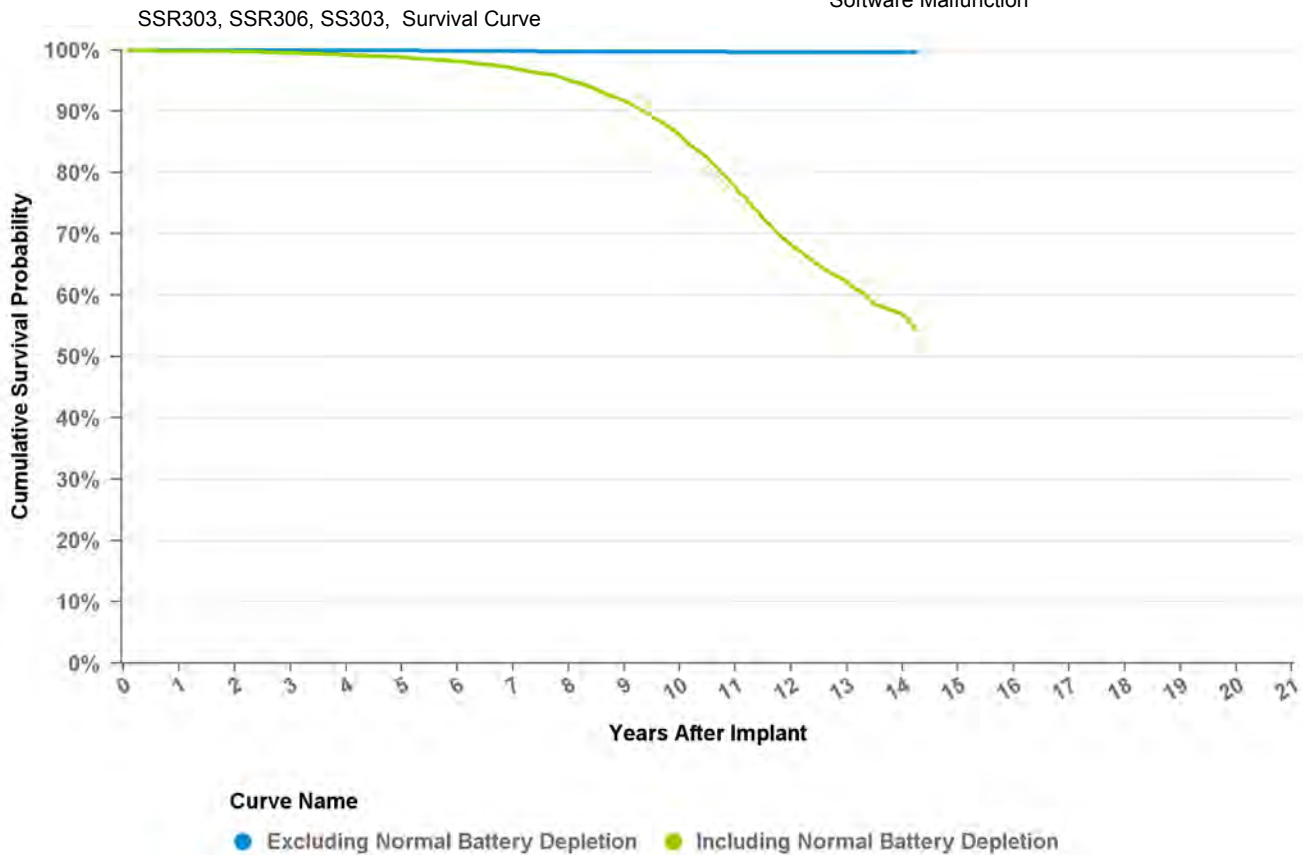

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | 14 | at 171 mo |
|------------------------------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.8% | 99.7% | 99.7% | 99.7% | 99.6% | 99.6% | 99.6% | 99.6% | 99.6% |
| Including NBD | 99.9% | 99.7% | 99.5% | 99.2% | 98.8% | 98.2% | 97.0% | 95.0% | 91.7% | 86.0% | 77.6% | 68.2% | 62.3% | 56.9% | 54.4% |
| Effective Sample Size | 47121 | 39977 | 34124 | 29348 | 25390 | 22076 | 19201 | 16101 | 13053 | 9933 | 6763 | 3868 | 2056 | 500 | 119 |


Implantable Pulse Generator

SSR306

Sigma 300 SR

| | |
|---------------------------------------|------------|
| US Market Release Date | 09/07/1999 |
| CE Market Approval Date | 12/17/1998 |
| Registered US Implants | 2,218 |
| Estimated Active US Implants | 276 |
| Normal Battery Depletions (US) | 136 |
| NBG Code | SSIR |
| Max Delivered Energy | N/A |

| | |
|---|---|
| Total Malfunctions (US) | 2 |
| Therapy Not Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 1 |
| Electrical Interconnect | 0 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |
| Therapy Compromised Malfunctions | 1 |
| Battery Malfunction | 0 |
| Electrical Component | 0 |
| Electrical Interconnect | 1 |
| Other Malfunction | 0 |
| Poss Early Battery Depltn | 0 |
| Software Malfunction | 0 |

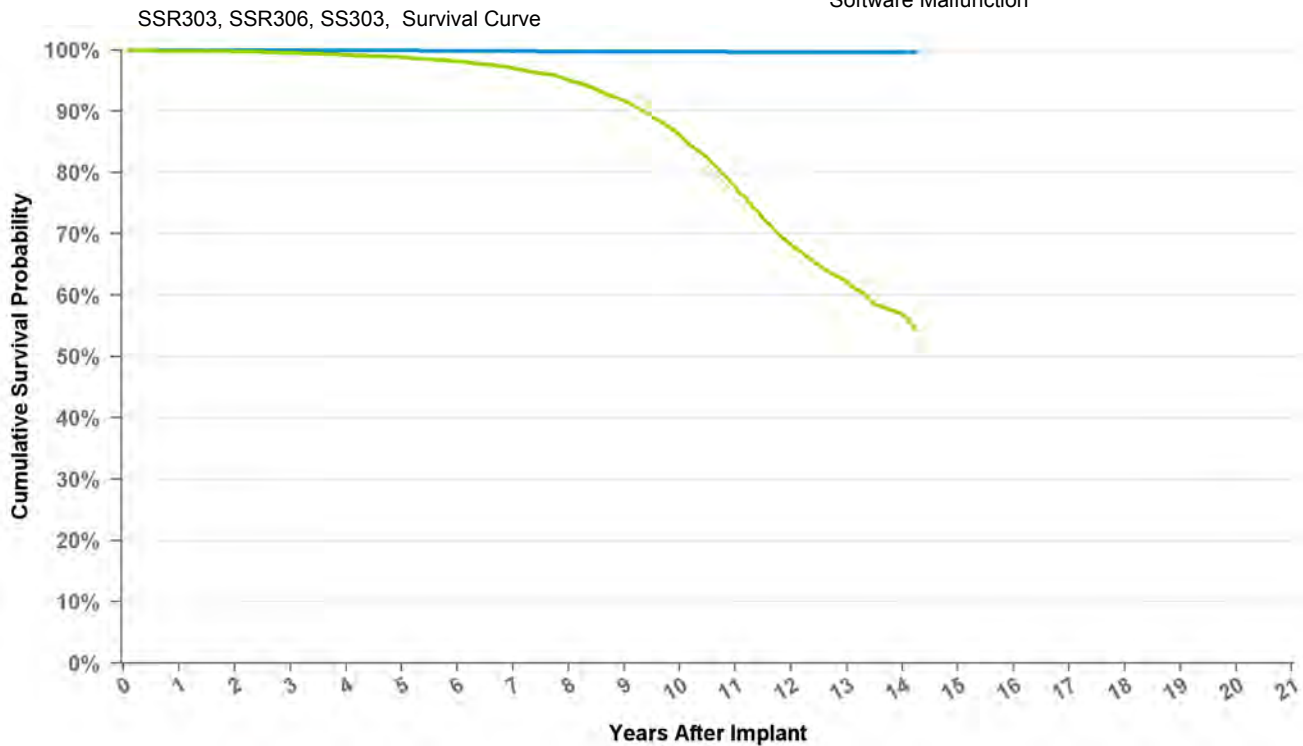

Curve Name

- Excluding Normal Battery Depletion
- Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | 14 | at 171 mo |
|------------------------------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.9% | 99.8% | 99.7% | 99.7% | 99.7% | 99.6% | 99.6% | 99.6% | 99.6% | 99.6% |
| Including NBD | 99.9% | 99.7% | 99.5% | 99.2% | 98.8% | 98.2% | 97.0% | 95.0% | 91.7% | 86.0% | 77.6% | 68.2% | 62.3% | 56.9% | 54.4% |
| Effective Sample Size | 47121 | 39977 | 34124 | 29348 | 25390 | 22076 | 19201 | 16101 | 13053 | 9933 | 6763 | 3868 | 2056 | 500 | 119 |

Implantable Pulse Generator

SVDD303 Sigma 300 VDD

US Market Release Date 09/15/1999

CE Market Approval Date 12/17/1998

Registered US Implants 650

Estimated Active US Implants 70

Normal Battery Depletions (US) 80

NBG Code VDD

Max Delivered Energy N/A

Total Malfunctions (US) 1

Therapy Not Compromised Malfunctions 0

Battery Malfunction 0

Electrical Component 0

Electrical Interconnect 0

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 1

Battery Malfunction 0


Electrical Component 0

Electrical Interconnect 1

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

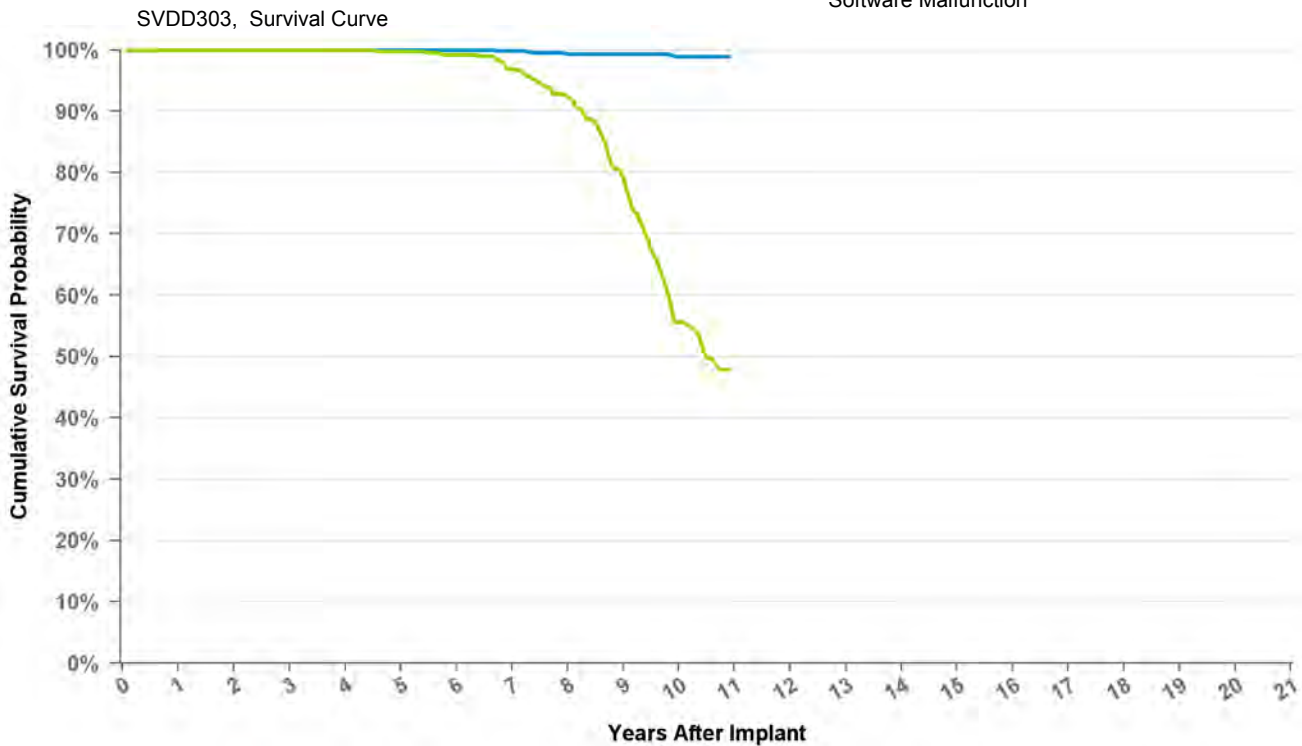

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 131 mo |
|-----------------------|--------|--------|--------|--------|--------|--------|-------|-------|-------|-------|-----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 99.8% | 99.3% | 99.3% | 98.9% | 98.9% |
| Including NBD | 100.0% | 100.0% | 100.0% | 100.0% | 99.7% | 99.2% | 96.9% | 92.4% | 79.2% | 55.6% | 47.9% |
| Effective Sample Size | 892 | 819 | 766 | 709 | 647 | 590 | 526 | 456 | 342 | 195 | 108 |

Implantable Pulse Generator

VEDR01 Versa DR

US Market Release Date 07/17/2006

CE Market Approval Date 09/20/2005

Registered US Implants 106,938

Estimated Active US Implants 76,935

Normal Battery Depletions (US) 1,208

NBG Code DDDR

Max Delivered Energy N/A

Total Malfunctions (US) 17

Therapy Not Compromised Malfunctions 9

Battery Malfunction 0

Electrical Component 7

Electrical Interconnect 2

Other Malfunction 0

Poss Early Battery Depltn 0

Software Malfunction 0

Therapy Compromised Malfunctions 8

Battery Malfunction 0


Electrical Component 4

Electrical Interconnect 0

Other Malfunction 4

Poss Early Battery Depltn 0

Software Malfunction 0

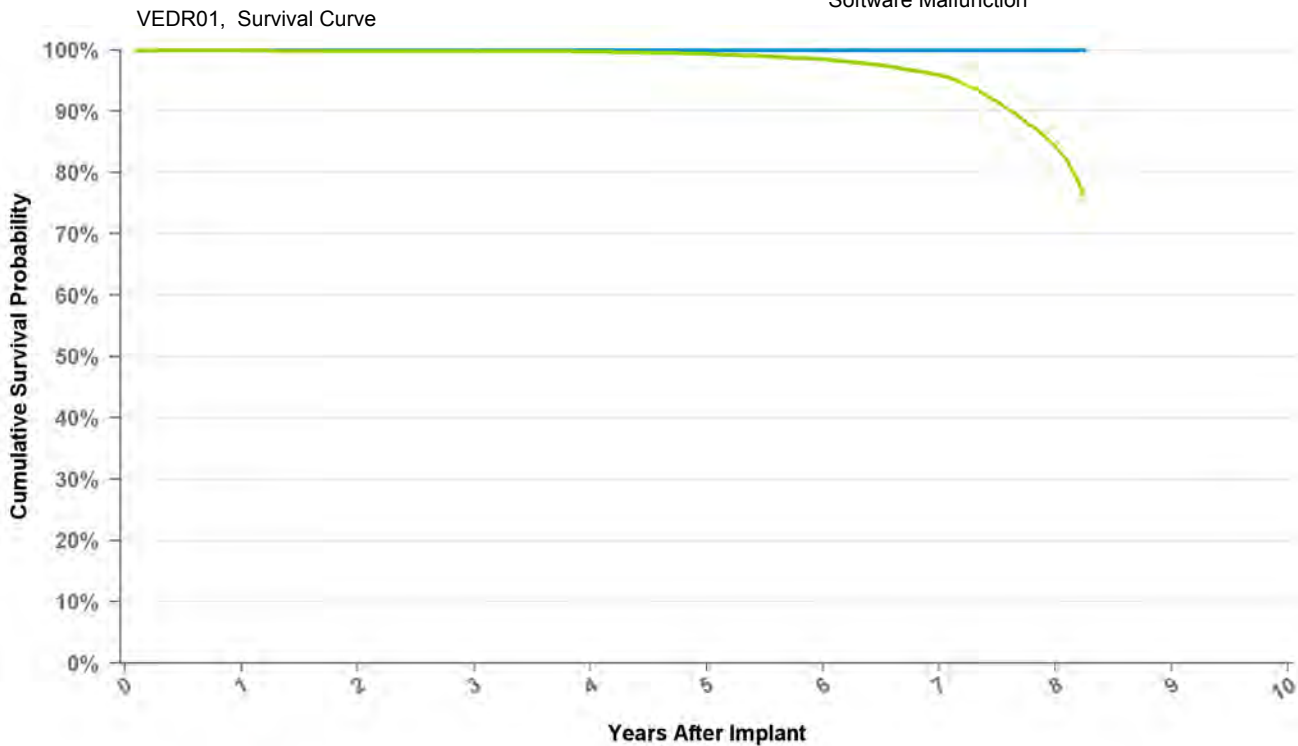

Curve Name

● Excluding Normal Battery Depletion ● Including Normal Battery Depletion

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 99 mo |
|------------------------------|--------|--------|--------|--------|--------|--------|--------|--------|----------|
| Excluding NBD | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% | 100.0% |
| Including NBD | 100.0% | 99.9% | 99.9% | 99.7% | 99.4% | 98.5% | 95.9% | 84.2% | 76.3% |
| Effective Sample Size | 97622 | 84249 | 69837 | 55425 | 40902 | 27087 | 13905 | 2455 | 450 |

Method for Estimating Lead Performance

Medtronic Cardiac Rhythm and Heart Failure (CRHF) has tracked lead survival for over 32 years with its multicenter, global chronic lead studies.

Leads Performance Analysis

Implanted leads operate in the challenging biochemical environment of the human body and the body's response to foreign objects. Implanted leads are also subject to mechanical stresses associated with heart motion, body motion, and patient anatomy.

In this environment, pacemaker and defibrillation leads cannot be expected to last forever. While IPGs and ICDs have a battery that will deplete after a predictable length of time, a lead's longevity cannot be predicted easily based on mechanical measurements, nor are there simple indicators that a lead is approaching the end of its service life. Therefore, regular monitoring while implanted, and evaluation of lead integrity upon IPG or ICD replacement, is necessary to determine if a lead may be approaching the end of its service life.

Shortfalls Of Using Returned Product And Complaints To Estimate Lead Performance

Leads and lead segments returned to Medtronic are analyzed to determine whether or not they meet performance limits established by Medtronic. Although returned product analyses are valuable for gaining insight into lead failure mechanisms, this data cannot be used by itself for determining the survival probability of leads because only a small fraction of leads are explanted and returned for analysis. Some leads are modified due to adverse device effect, however may not be explanted. Additionally, those leads that are returned cannot be assumed to be statistically representative of the performance of the total population for a given lead model. Partial or total lead extraction can result in significant damage to a lead, making a definitive analysis of a suspected failure, and its cause, impossible.

To account for the under reporting inherent with lead survival analysis based solely on returned product, some manufacturers add reported complaints where adverse product performance is evident but the product itself has not been returned. The improvement to the accuracy of survival estimates depends on the degree to which all complaints are actually communicated to the manufacturer. Since not all complaints are communicated to the manufacturer, adding complaints to the survival analysis does not completely solve the under reporting problem.

Lead survival probabilities are more appropriately determined through a prospective clinical surveillance study that includes active follow up with the patients. Although Medtronic monitors returned product analysis and complaints, these are not used to determine lead survival estimates.

Medtronic consolidated all cardiac rhythm surveillance registries into the PAN Registry. The PAN Registry is a patient centric surveillance platform which follows patients implanted with Medtronic cardiac rhythm product(s). The Product Performance Report (PPR) tracks PAN Registry enrolled patients to monitor lead performance status in vivo. The PAN Registry is designed to record clinical observations representative of the total clinical experience. Lead survival estimates include both lead hardware failure and lead-related clinical events that are classified as product performance events, and do not differentiate a lead hardware failure from other clinical events such as Failure to capture, perforation, dislodgement, or concurrent pulse generator failure.

PAN Registry

Medtronic has been monitoring the performance of its cardiac therapy products with a multicenter study since 1983 and has evaluated the performance of more than 95,000 leads, with data reported from countries around the world. Throughout this time period, Medtronic has continually worked to adapt systems and processes to more effectively monitor product performance following market release. The following summarizes current registry requirements.

Method for Estimating Lead Performance continued

Medtronic's product surveillance registry is a world-wide study that has a prospective, non-randomized, observational design. A key purpose of the registry is to provide continuing evaluation and periodic reporting of the long-term reliability and performance of Medtronic market-released cardiac rhythm therapy products. Product-related adverse events, indicating the status of the product, are collected to measure product survival probabilities. The data gathered may also be used to support the design and development of new cardiac therapy products. The registry is designed to continue indefinitely, encompassing new products as they become commercially available.

To ensure a sufficiently large and representative source of data, participating clinical sites must meet pre-specified selection criteria. Patients are enrolled upon implantation of a Medtronic Cardiac rhythm product. Every effort is made to ensure participants are representative of the range of clinical environments in which Medtronic cardiac rhythm products are used. Eligible products for enrollment include Medtronic market-released cardiac rhythm therapy products for which additional information to further characterize product performance following market release is desired. Number of enrollments is reviewed regularly to ensure adequate sample size is obtained for each individual product. Enrollment may be capped and follow-up discontinued when sufficient duration and precision is achieved to effectively characterize product survivability.

Enrolled patients are followed in accordance with the standard care practices of their care provider from their implant date until they can no longer be followed (e.g., death, lost to follow-up, etc.). However, to ensure regular patient status assessments are completed, follow-up windows consistent with typical care practices have been established with a minimum annual follow-up requirement. Product-related adverse events, system modifications and changes in patient status (e.g. death and withdrawal from the study) are required to be reported upon occurrence. This active surveillance model ensures a robust dataset for effectively monitoring product performance.

Patients are eligible for enrollment if:

- Patient is intended to be implanted or is within 30 days post-implant of a Medtronic market-released cardiac lead connected to a market-released CRT, ICD, or IPG device, and the lead is used for a pacing, sensing, or defibrillation application, or
- Patient participated in a qualifying investigational study of a Medtronic cardiac rhythm product that is now market-released; complete implant and follow-up data are available; and the data can be appropriately and legally released

Each site is required to inform Medtronic whenever a lead event has occurred, a lead is modified, or when a patient is no longer participating. Timely, accurate, and complete reporting and analysis of safety information for surveillance is crucial for the protection of patients, clinicians, and the sponsor Medtronic continually evaluates the quality and integrity of the data through a combination of on-site and centralized monitoring activities.

Lead Complications

Chronic lead performance is characterized by estimating lead related complication free survival probabilities. For analysis purposes, the complication criteria, which align with the AdvaMed 'Industry Guidance for Uniform Reporting of Clinical Performance of Cardiac Rhythm Management Pulse Generators and Leads', are defined below. These criteria do not, however, enable a lead integrity or "hardware" failure to be conclusively differentiated from other clinical events such as an undetected lead dislodgement, perforation, or concurrent pulse generator failure manifested as a sensing or capture problem.

Method for Estimating Lead Performance continued

All reported lead-related adverse events are classified by the reporting investigator and are adjudicated by an independent event adjudication committee¹. A lead-related event with at least one of the following classifications that is adjudicated by the committee as a complication and occurs more than 30 days after implant is considered a product performance event and will contribute to the survival analysis endpoint. Events with an onset date of 30 days or less after the implant are considered procedure related and therefore are not included as product performance events.

- Product performance events includes, but not limited to: Failure to capture
- Failure to sense/undersensing
- Oversensing
- Elevated pacing thresholds
- Abnormal pacing impedance (based on lead model, but normal range is typically 200 - 2,000 ohms)
- Abnormal defibrillation impedance (based on lead model, but normal range is typically 20 - 200 ohms)
- Lead Insulation breach
- Lead Conductor fracture, confirmed electrically, visually or radiographically
- Extracardiac stimulation
- Cardiac perforation
- Lead dislodgement
- Structural Lead Failure

Data Analysis Methods

The performance of leads is expressed in terms of lead survival estimates, where "survival" refers to the function of the lead, not the survival of the patient.. These survival estimates are intended to illustrate the probability that a lead will survive for a given number of years without a chronic lead-related complication.

Active surveillance normally begins at the time of implant and continues until a product performance or censoring event occurs. In some cases in the PAN Registry, active surveillance of a device starts after the device was implanted. The survival probability of such device is conditional on survival to the time when the device enters the Registry. This phenomenon is called Left-truncation². PPR lead survival analysis is estimated using the Kaplan-Meier method, a statistical method to incorporate data from these retrospectively enrolled devices, left-truncated data, was applied. The statistical technique uses data from existing devices while appropriately adjusting the device survival curves for the time the device was not actively followed in the registry. Thus, in some cases sample sizes may fluctuate from one time interval to the next interval.

On the following pages, each graph includes a survival curve for each lead model. The survival estimates is the probability that a lead is free of a product performance event at a given time point. For example, if a survival probability is 95% after 5 years of service, then the lead has a 5% chance of experiencing a lead-related complication in the first 5 years following implant.

The data in the tables is rounded to the nearest tenth of one percent. Occasionally, a graph may show 100% survival, but have one or more complications. This occurs because even with the complications, the data rounds to 100%.

The survival curves are statistical estimates. As sample size increases and performance experience accumulates, the estimation improves. Confidence intervals are provided as a way to indicate the degree of certainty of the estimates. Greenwood's formula is used to calculate the standard errors, and the log-log method is used to produce the 2-sided 95% confidence bounds.

Since the survival estimate can become very imprecise with small effective sample sizes, Medtronic truncates the survival curve when the number of leads entering an interval is less than 50 leads. When the number of leads entering an interval reaches 50, the next data point is added to the survival

Method for Estimating Lead Performance continued

curve. For those lead models that do not have sufficient sample size, a survival curve will not be presented.

Definition of Analysis Dataset

The survival estimates are derived from all device components successfully enrolled as of the data received cut-off date (e.g. date of data entry at a study site). The number of enrollments is listed for each lead model.

This sample is considered to be representative of the worldwide population, and therefore the survival estimates shown should be representative of the performance worldwide of these models.

Criteria for Model Inclusion

Performance information for a model or model family will be published when more than 100 leads have been enrolled and no fewer than 50 leads followed for at least 6 months. Medtronic, at its discretion, may stop providing updated performance information on lead models that received original US market-release approval 20 or more years ago.

Returned Product Analysis Results

Although the returned product analysis data is not used to generate the survival estimates, the data provides valuable insight into the causes of lead malfunction.

For reporting returned product analysis results, Medtronic CRHF considers a lead as having malfunctioned whenever the analysis shows that any parameter was outside the performance limits established by Medtronic while implanted and in service. To be considered a malfunction for returned product analysis reporting, the lead must have been returned to Medtronic and analyzed.

The results of the analysis is presented in four categories. The lead reporting categories are:

Conductor Fracture: Conductor malfunction with complete or intermittent loss of continuity that could interrupt current flow (e.g., fractured conductors), including those associated with clavicle flex fatigue or crush damage.

Insulation Breach: A malfunction of the insulation allowing inappropriate entry of body fluids or inappropriate current flow between the conductors, or between the conductor and the body. Examples include cuts, tears, depressions, abrasions, and material degradation.

Crimps/Welds/Bonds: Any malfunction in a conductor or lead body associated with a point of connection.

Other: Malfunctions of specific lead mechanical attributes, such as sensors, connectors, seal rings, or malfunction modes not included in the three categories above.

A lead subject to a safety advisory is not considered to have malfunctioned unless it has been returned to Medtronic CRHF and found, through analysis, to actually have performed outside the performance limits established by Medtronic.

For leads designed for either ventricular or atrial use, the numbers listed in the Returned Product Analysis tables include both.

The numbers of malfunctions listed in the Returned Product Analysis tables are the actual numbers confirmed in the returned product analysis. The numbers of complications listed in the complications tables are the actual numbers observed in the PSR centers around the world.

Method for Estimating Lead Performance continued

US Reports of Acute Lead Observations (Occurring within First Month of Service)

In the first weeks following lead implantation, physiologic responses and lead performance can vary until long-term lead stability is attained. Acute (defined as the first month after implant) lead performance may be subject to a number of factors, including patient-specific anatomy, clinical conditions and/or varying implant conditions/techniques. After a period of time, the implant and the lead performance stabilizes. It is for this reason that the Product Surveillance Registry results, which are intended to measure long-term performance, do not include complications that occur within the first 30 days after implant.

Information about the clinical experience in the first month of service is included in our reporting. The source for this information is Medtronic's complaint handling system database. The information is summarized in tables titled "US Reports of Acute Lead Observations."

Each Event Report received by Medtronic's complaint handling system is assigned one or more Reason for Report codes based on the information received. The Reason for Report codes have been grouped into Acute Lead Observation categories. The categories used for this product performance reporting are drawn from the "FDA Guidance for Submission of Research and Marketing Applications for Permanent Pacemaker Leads and for Pacemaker Lead Adapter 510(k) Submissions." The categories are:

1. Cardiac Perforation
2. Conductor Fracture
3. Lead Dislodgement
4. Failure to Capture
5. Oversensing
6. Failure to Sense
7. Insulation Breach
8. Impedance Abnormal
9. Extracardiac Stimulation
10. Unspecified

Although multiple observations are possible for any given lead, only one observation is reported per lead. The observation reported is the observation highest on the list. For example, if an Event Report includes observations for both Lead Dislodgement and Failure to Sense, Lead Dislodgement is reported.

The lead event reported to Medtronic may or may not have involved clinical action or product returned to Medtronic. The lead may have remained implanted and in service.

Estimated Number of Implanted and Active Leads in the United States

In addition to providing the number of leads enrolled in the PSR, we also provide the number of leads registered as implanted and the number remaining active in the United States based on the status recorded in the Medtronic Device and Registrant Tracking system.

Footnotes:

1: During the evolution of SLS, event adjudication was transitioned from a Medtronic technical review committee to an independent event adjudication committee in 2011. Data analyses include adjudication using both methods.

2: Klein, John P., Moeschberger, Melvin L. Survival Analysis Techniques for Censored and Truncated Data, New York: Springer-Verlag New York, Inc., 1997.

LEFT HEART PACING LEAD 2187

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 8/28/2001 |
| CE Approval Date | |
| Registered US Implants | 11,982 |
| Estimated Active US | 2,454 |

Product Characteristics

| | |
|---------------------|-------------------------------|
| Fixation Type | Distal Continuous Curve |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | None |
| Lead Placement | Transvenous |
| Lead Tip Location | Left Ventricular Cardiac Vein |
| Pace/Sense Polarity | Unipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|-------|
| Number of Leads Enrolled in Study | 138 |
| Cumulative Months of Follow-Up | 6,379 |
| Number of Leads Active in Study | 7 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 2 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |


US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 3 |
| Failure To Sense | 1 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 9 |
| Oversensing | 0 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 1 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 0 |
| Other | 4 |

2187, Survival Curve

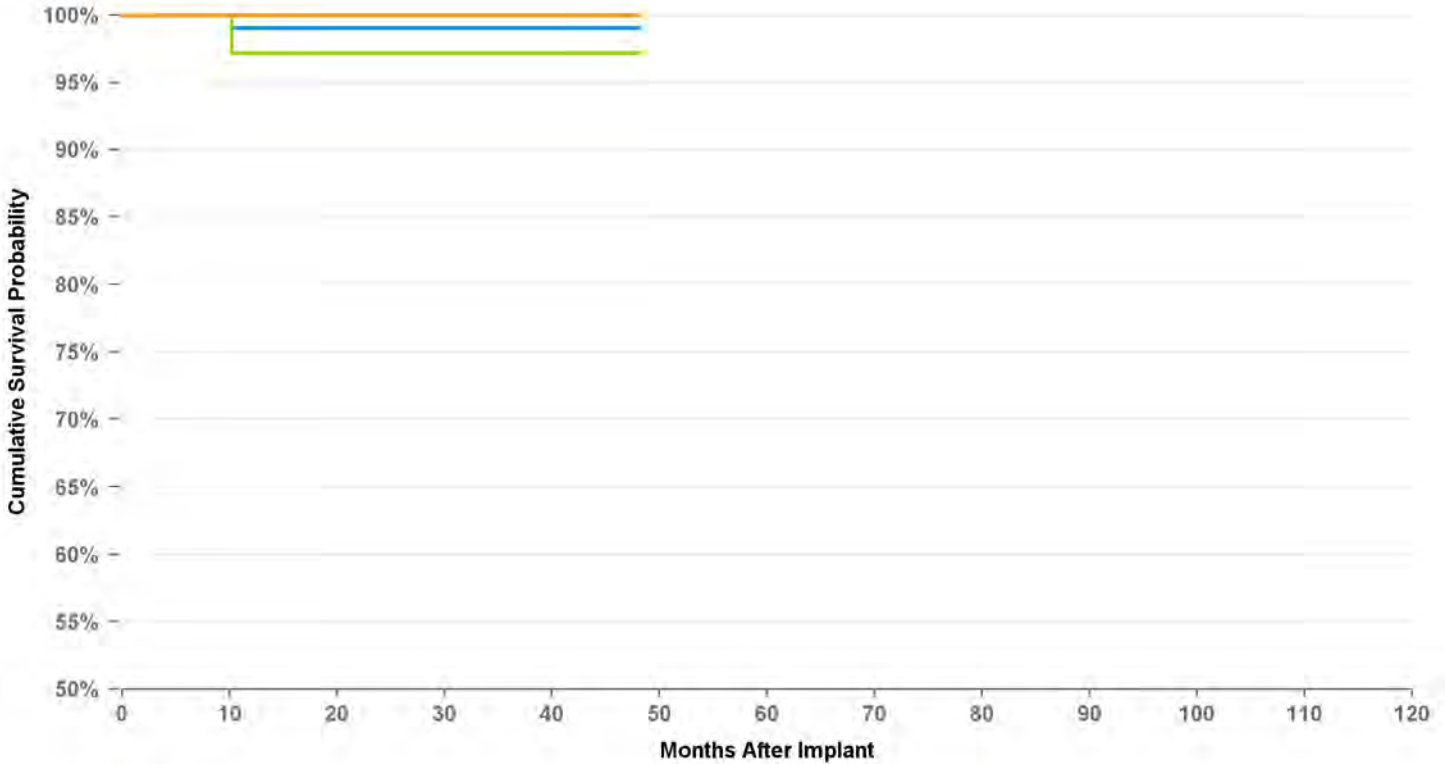

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | at 48 mo |
|-------|-------|-------|-------|----------|
| % | 99.0% | 99.0% | 99.0% | 99.0% |
| # | 100 | 84 | 64 | 52 |

LEFT HEART PACING LEAD

4193

Distribution Data

| | |
|------------------------|------------|
| US Market Release | 5/3/2002 |
| CE Approval Date | 12/22/2000 |
| Registered US Implants | 100,774 |
| Estimated Active US | 30,997 |

Product Characteristics

| | |
|---------------------|-------------------------------|
| Fixation Type | Distal Double Curve |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Left Ventricular Cardiac Vein |
| Pace/Sense Polarity | Unipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 739 |
| Cumulative Months of Follow-Up | 32,224 |
| Number of Leads Active in Study | 106 |

Product Surveillance Registry Qualifying Complications


| | |
|---|-----------|
| | 41 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 9 |
| Failure To Capture | 13 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 14 |
| Medical Judgment | 0 |
| Other Complication | 1 |
| Oversensing | 0 |
| Unspecified | 3 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 17 |
| Failure To Capture | 11 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 45 |
| Oversensing | 1 |
| Unspecified | 2 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 59 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 13 |
| Other | 48 |

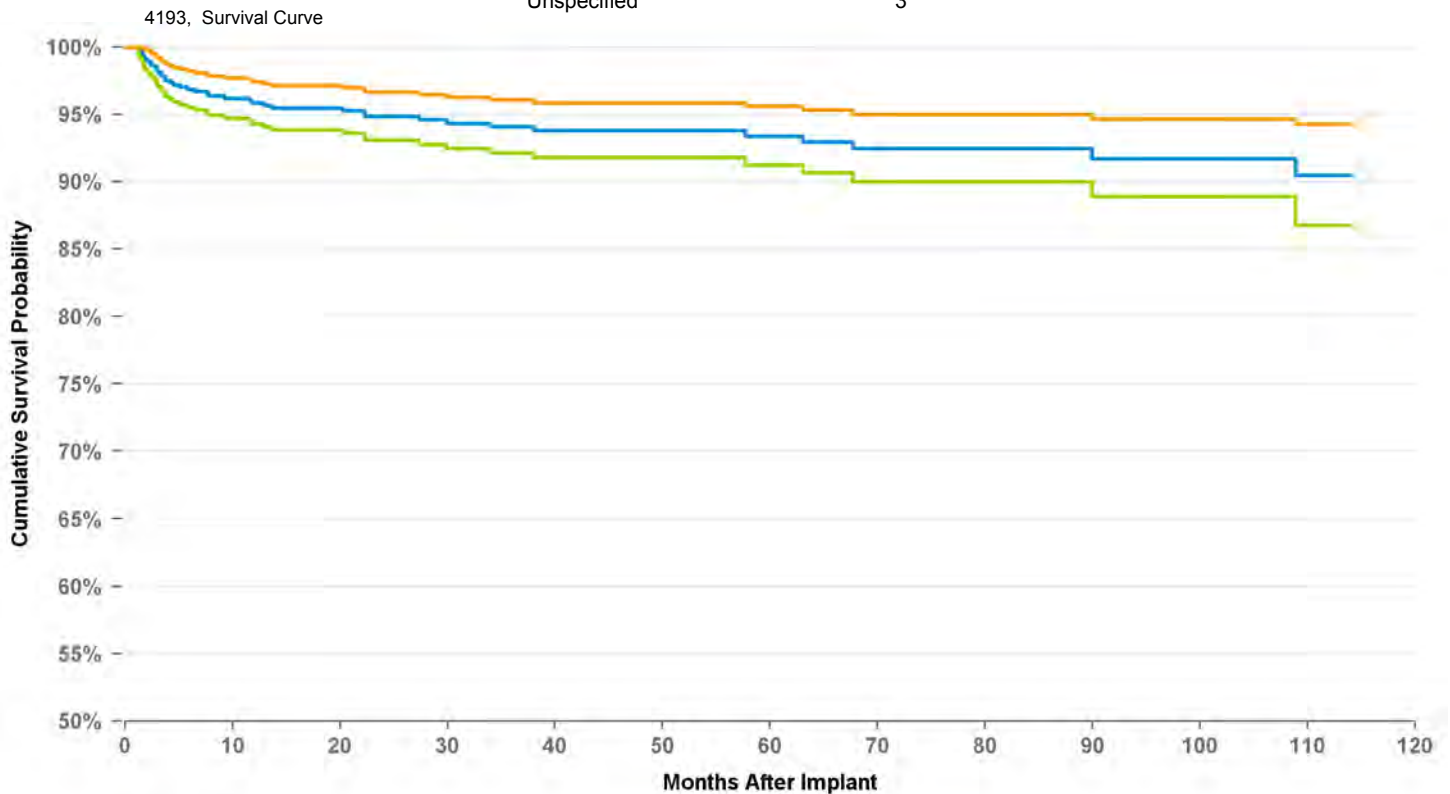

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 114 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 95.8% | 94.8% | 94.1% | 93.8% | 93.4% | 92.5% | 92.5% | 91.7% | 91.7% | 90.5% |
| # | 561 | 417 | 345 | 271 | 209 | 173 | 139 | 106 | 69 | 53 |

LEFT HEART PACING LEAD

4194

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 8/24/2004 |
| CE Approval Date | 7/14/2003 |
| Registered US Implants | 113,369 |
| Estimated Active US | 63,630 |

Product Characteristics

| | |
|---------------------|-------------------------------|
| Fixation Type | Distal Double Curve |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Left Ventricular Cardiac Vein |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,468 |
| Cumulative Months of Follow-Up | 52,175 |
| Number of Leads Active in Study | 686 |

Product Surveillance Registry Qualifying Complications


| | |
|---|-----------|
| | 43 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 8 |
| Failure To Capture | 11 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 1 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 2 |
| Lead Dislodgement | 21 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|-----|
| Cardiac Perforation | 2 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 41 |
| Failure To Capture | 39 |
| Failure To Sense | 0 |
| Impedance Abnormal | 6 |
| Insulation Breach | 0 |
| Lead Dislodgement | 144 |
| Oversensing | 2 |
| Unspecified | 5 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 18 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 68 |
| Other | 9 |

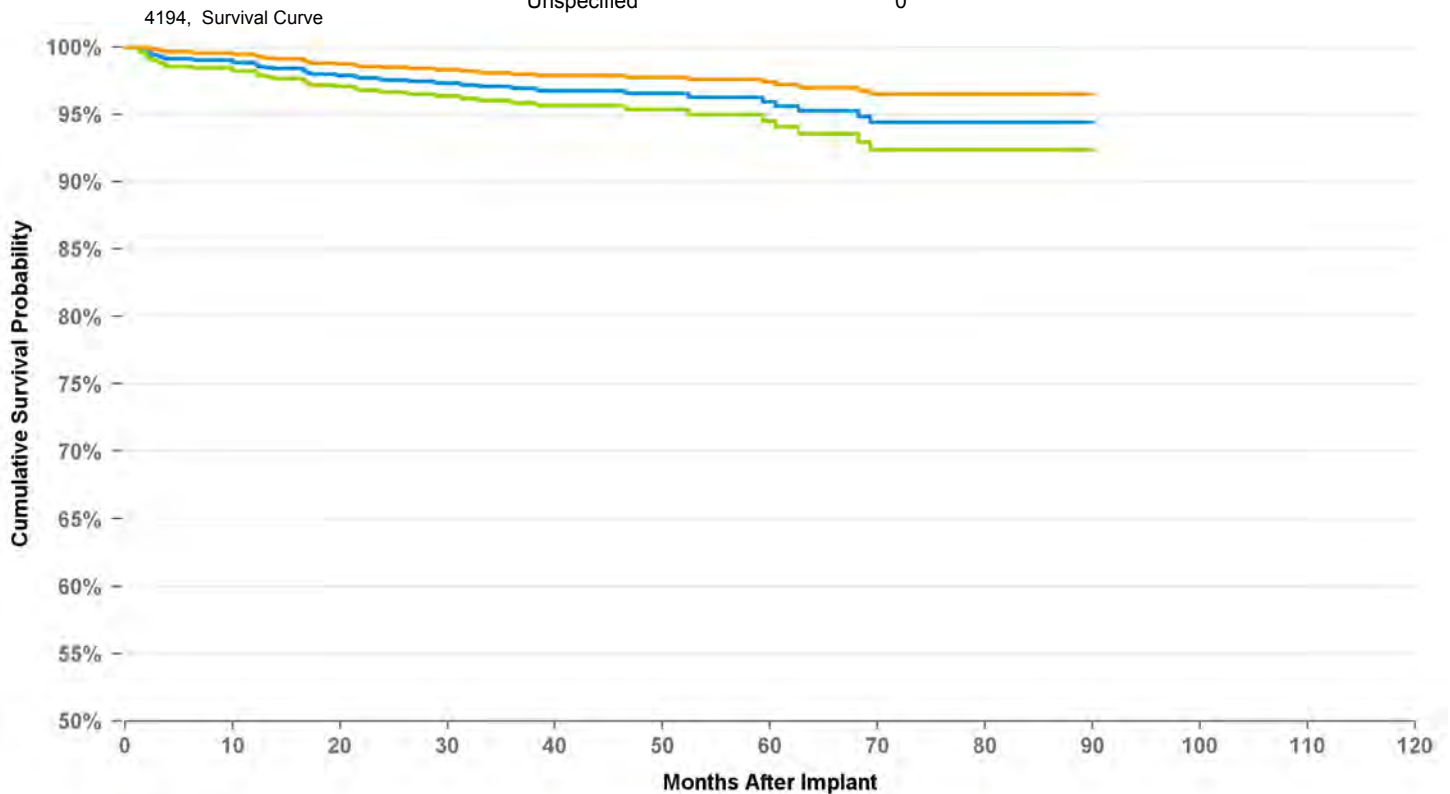

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 90 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|----------|
| % | 98.8% | 97.6% | 96.9% | 96.5% | 96.0% | 94.4% | 94.4% | 94.4% |
| # | 1,138 | 866 | 657 | 405 | 262 | 164 | 98 | 73 |

LEFT HEART PACING LEAD

4195

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 8/15/2008 |
| CE Approval Date | 5/13/2005 |
| Registered US Implants | 16,761 |
| Estimated Active US | 12,662 |

Product Characteristics

| | |
|---------------------|-------------------------------|
| Fixation Type | Deployable Lobe Fixation |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Left Ventricular Cardiac Vein |
| Pace/Sense Polarity | Unipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,441 |
| Cumulative Months of Follow-Up | 43,390 |
| Number of Leads Active in Study | 827 |

Product Surveillance Registry Qualifying Complications


| | |
|---|----|
| | 17 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 7 |
| Failure To Capture | 3 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 1 |
| Lead Dislodgement | 4 |
| Medical Judgment | 0 |
| Other Complication | 1 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 28 |
| Failure To Capture | 19 |
| Failure To Sense | 0 |
| Impedance Abnormal | 3 |
| Insulation Breach | 0 |
| Lead Dislodgement | 29 |
| Oversensing | 0 |
| Unspecified | 1 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 5 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 1 |
| Other | 4 |

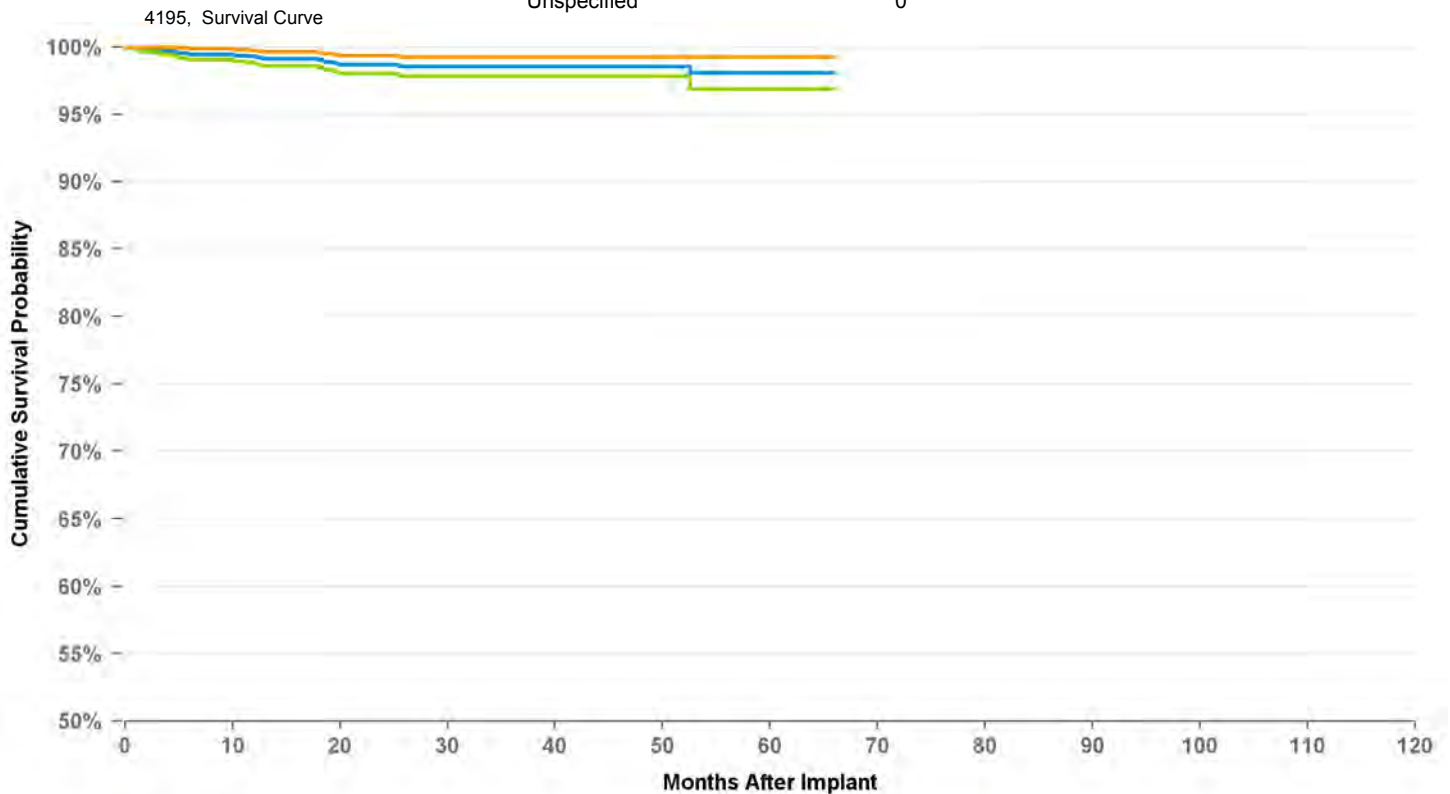

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | at 66 mo |
|-------|-------|-------|-------|-------|-------|----------|
| % | 99.3% | 98.7% | 98.6% | 98.6% | 98.1% | 98.1% |
| # | 1,136 | 825 | 527 | 279 | 89 | 55 |

LEFT HEART PACING LEAD

4196

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 5/15/2009 |
| CE Approval Date | 7/24/2007 |
| Registered US Implants | 61,607 |
| Estimated Active US | 49,366 |

Product Characteristics

| | |
|---------------------|-------------------------------|
| Fixation Type | Double Curve |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Left Ventricular Cardiac Vein |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 2,086 |
| Cumulative Months of Follow-Up | 58,184 |
| Number of Leads Active in Study | 939 |

Product Surveillance Registry Qualifying Complications

54


| | |
|---|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 12 |
| Failure To Capture | 18 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 20 |
| Medical Judgment | 0 |
| Other Complication | 2 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|-----|
| Cardiac Perforation | 1 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 78 |
| Failure To Capture | 50 |
| Failure To Sense | 1 |
| Impedance Abnormal | 7 |
| Insulation Breach | 1 |
| Lead Dislodgement | 168 |
| Oversensing | 1 |
| Unspecified | 3 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 13 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 0 |
| Other | 10 |

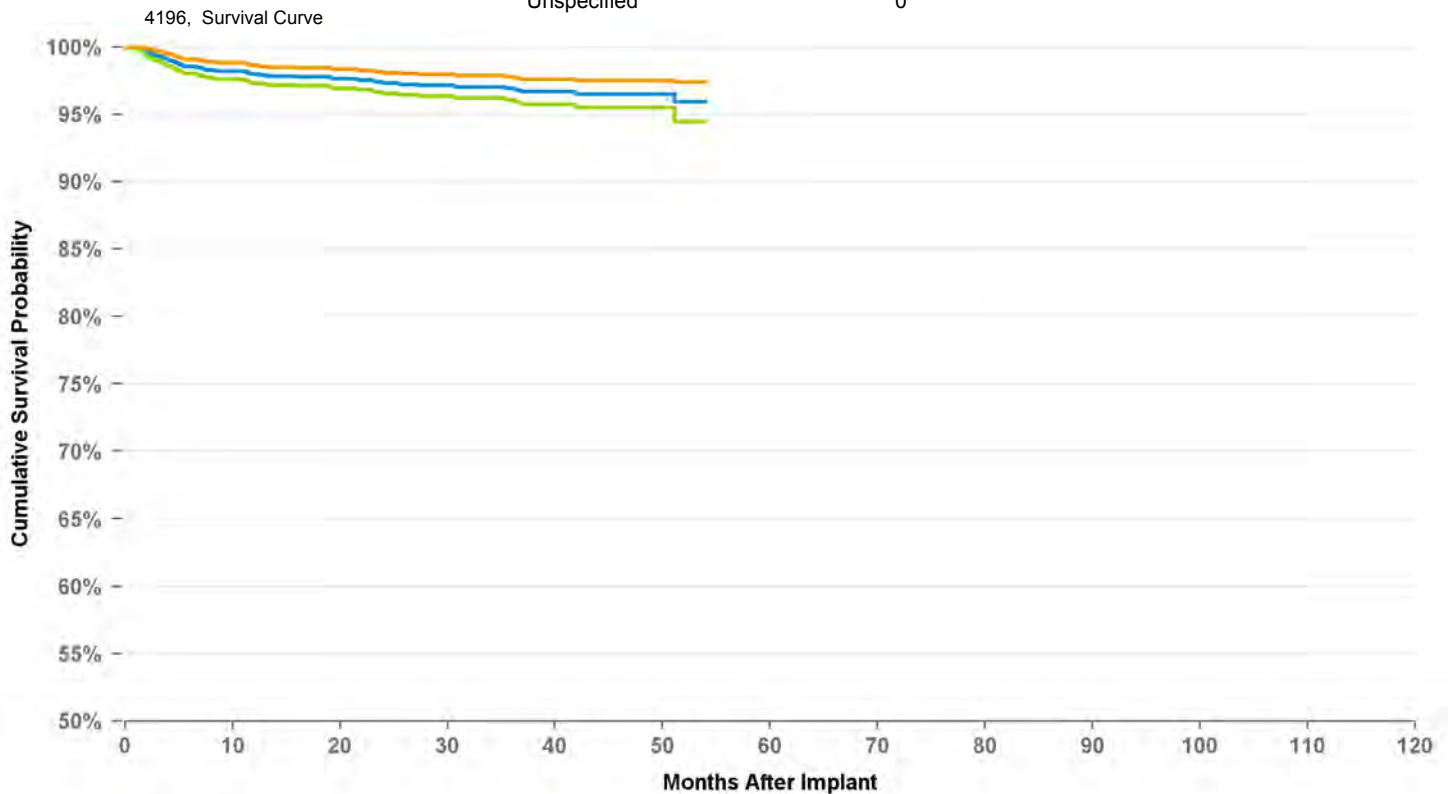

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | at 54 mo |
|-------|-------|-------|-------|-------|----------|
| % | 98.0% | 97.3% | 96.9% | 96.5% | 95.9% |
| # | 1,603 | 1,184 | 783 | 244 | 89 |

LEFT HEART PACING LEAD

4296

Distribution Data

| | |
|------------------------|------------|
| US Market Release | 4/1/2011 |
| CE Approval Date | 12/18/2009 |
| Registered US Implants | 28,068 |
| Estimated Active US | 25,563 |

Product Characteristics

| | |
|---------------------|-------------------------------|
| Fixation Type | Distal Double Curve |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Left Ventricular Cardiac Vein |
| Pace/Sense Polarity | Dual Electrodes |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,347 |
| Cumulative Months of Follow-Up | 18,385 |
| Number of Leads Active in Study | 971 |

Product Surveillance Registry Qualifying Complications


| | |
|---|-----------|
| | 10 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 3 |
| Failure To Capture | 2 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 5 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 2 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 42 |
| Failure To Capture | 18 |
| Failure To Sense | 0 |
| Impedance Abnormal | 8 |
| Insulation Breach | 4 |
| Lead Dislodgement | 93 |
| Oversensing | 0 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 2 |
| Crimp Weld Bond | 2 |
| Insulation Breach | 0 |
| Other | 3 |

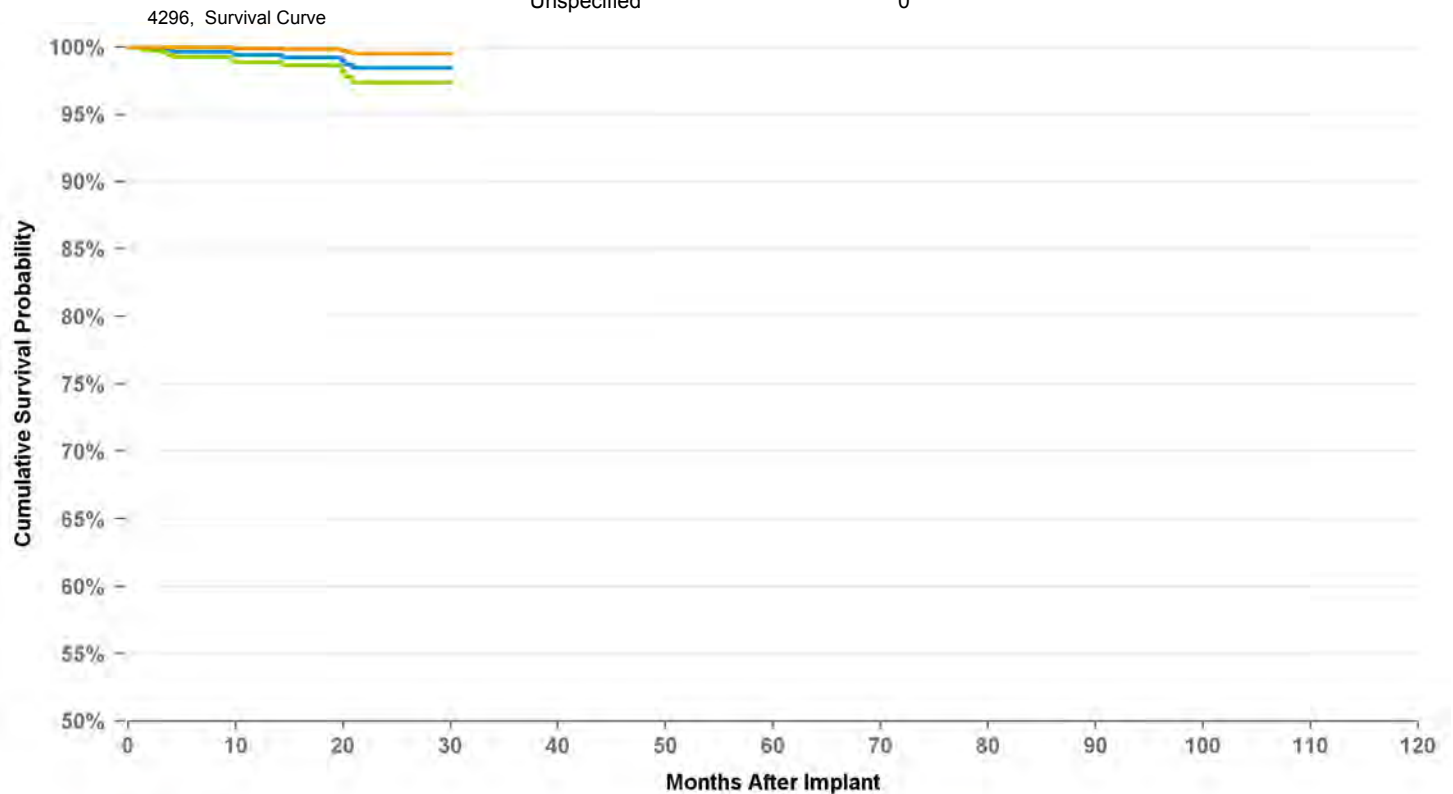

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | at 30 mo |
|-------|-------|-------|----------|
| % | 99.4% | 98.4% | 98.4% |
| # | 709 | 232 | 88 |

LEFT HEART PACING LEAD

4298

Distribution Data

| | |
|------------------------|----------|
| US Market Release | |
| CE Approval Date | 1/1/2013 |
| Registered US Implants | 7,796 |
| Estimated Active US | 7,664 |


Product Characteristics

| | |
|---------------------|-------------------------------|
| Fixation Type | Distal Double Curve |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Left Ventricular Cardiac Vein |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|---|
| Number of Leads Enrolled in Study | 0 |
| Cumulative Months of Follow-Up | 0 |
| Number of Leads Active in Study | 0 |

4298, Survival Curve

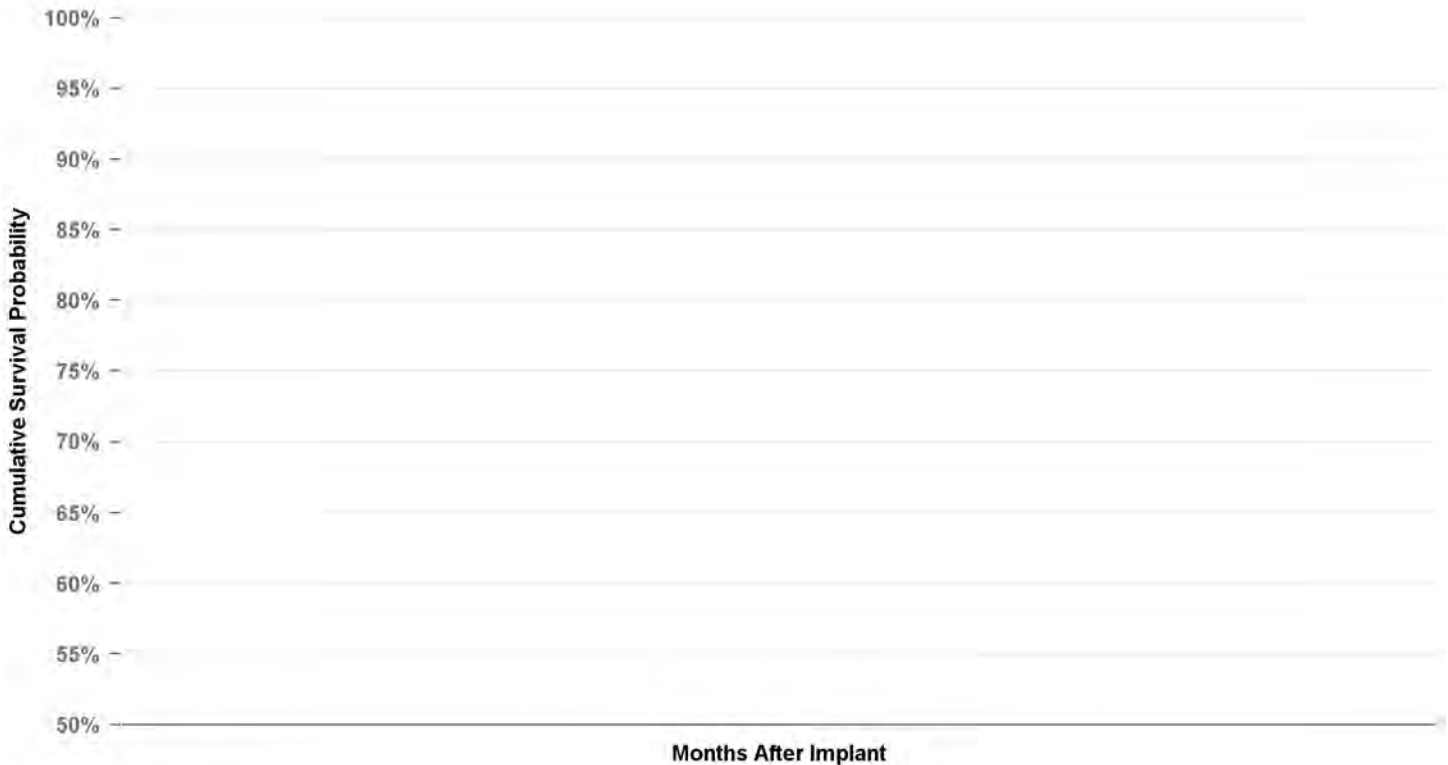

Graph Name

- Cumulative Survival Probability Graph
- Lower 95 Pct Confidence Graph
- Upper 95 Pct Confidence Graph

Years

%

#

Product Surveillance Registry Qualifying Complications

| | |
|---|----------|
| | 0 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 1 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 14 |
| Failure To Capture | 10 |
| Failure To Sense | 0 |
| Impedance Abnormal | 3 |
| Insulation Breach | 0 |
| Lead Dislodgement | 8 |
| Oversensing | 0 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 0 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 0 |
| Other | 4 |

LEFT HEART PACING LEAD

4396

Distribution Data

| | |
|------------------------|------------|
| US Market Release | 3/31/2011 |
| CE Approval Date | 12/18/2009 |
| Registered US Implants | 5,890 |
| Estimated Active US | 5,300 |

Product Characteristics

| | |
|---------------------|-------------------------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Left Ventricular Cardiac Vein |
| Pace/Sense Polarity | Dual Electrodes |

Product Surveillance Registry Results

| | |
|-----------------------------------|-------|
| Number of Leads Enrolled in Study | 361 |
| Cumulative Months of Follow-Up | 5,775 |
| Number of Leads Active in Study | 260 |

Product Surveillance Registry Qualifying Complications


| | |
|---|---|
| | 1 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 1 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 10 |
| Failure To Capture | 5 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 27 |
| Oversensing | 0 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 1 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 0 |
| Other | 1 |

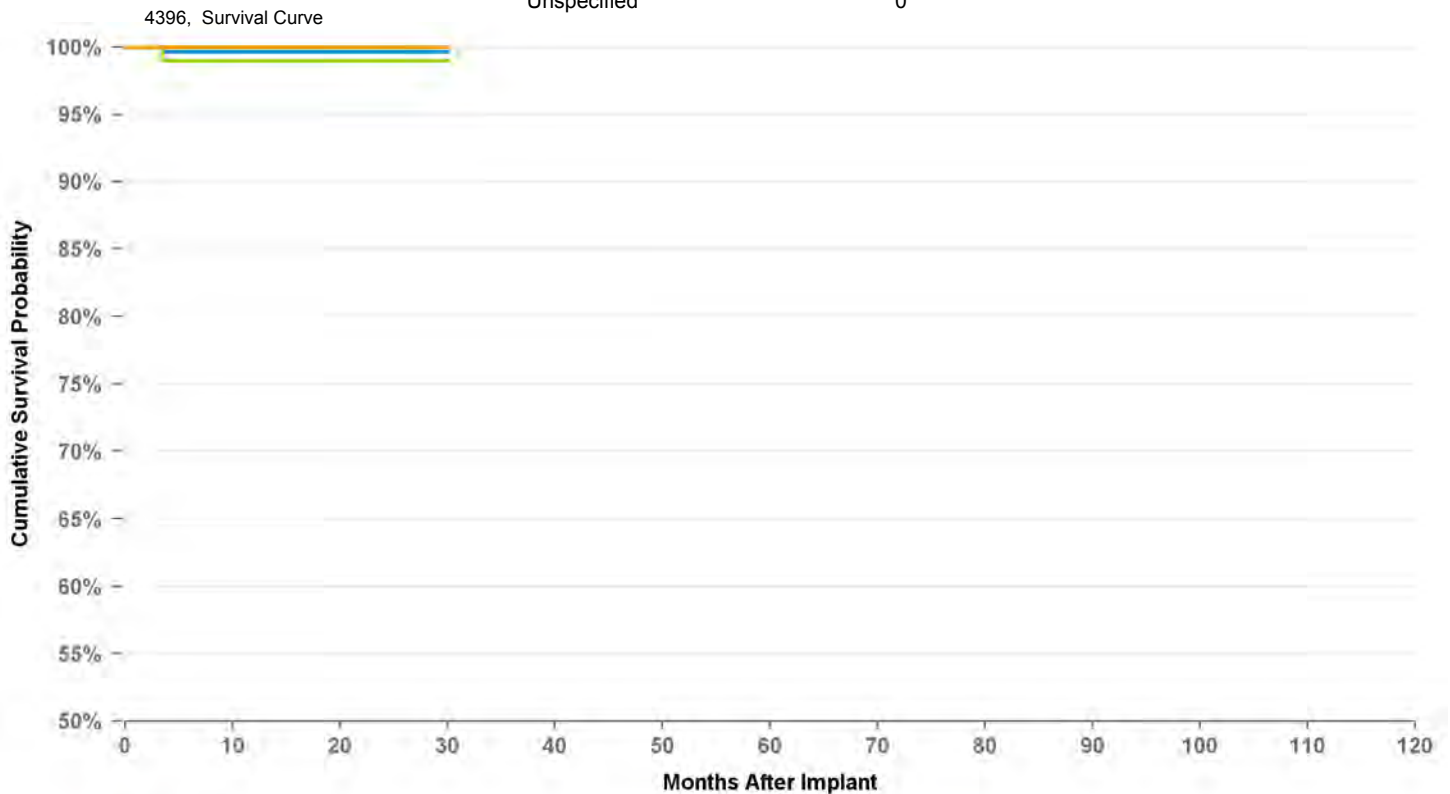

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | at 30 mo |
|-------|-------|-------|----------|
| % | 99.7% | 99.7% | 99.7% |
| # | 194 | 76 | 52 |

LEFT HEART PACING LEAD

4398

Distribution Data

| | |
|------------------------|----------|
| US Market Release | |
| CE Approval Date | 1/1/2013 |
| Registered US Implants | 395 |
| Estimated Active US | 379 |


Product Characteristics

| | |
|---------------------|-------------------------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Left Ventricular Cardiac Vein |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|---|
| Number of Leads Enrolled in Study | 0 |
| Cumulative Months of Follow-Up | 0 |
| Number of Leads Active in Study | 0 |

4398, Survival Curve

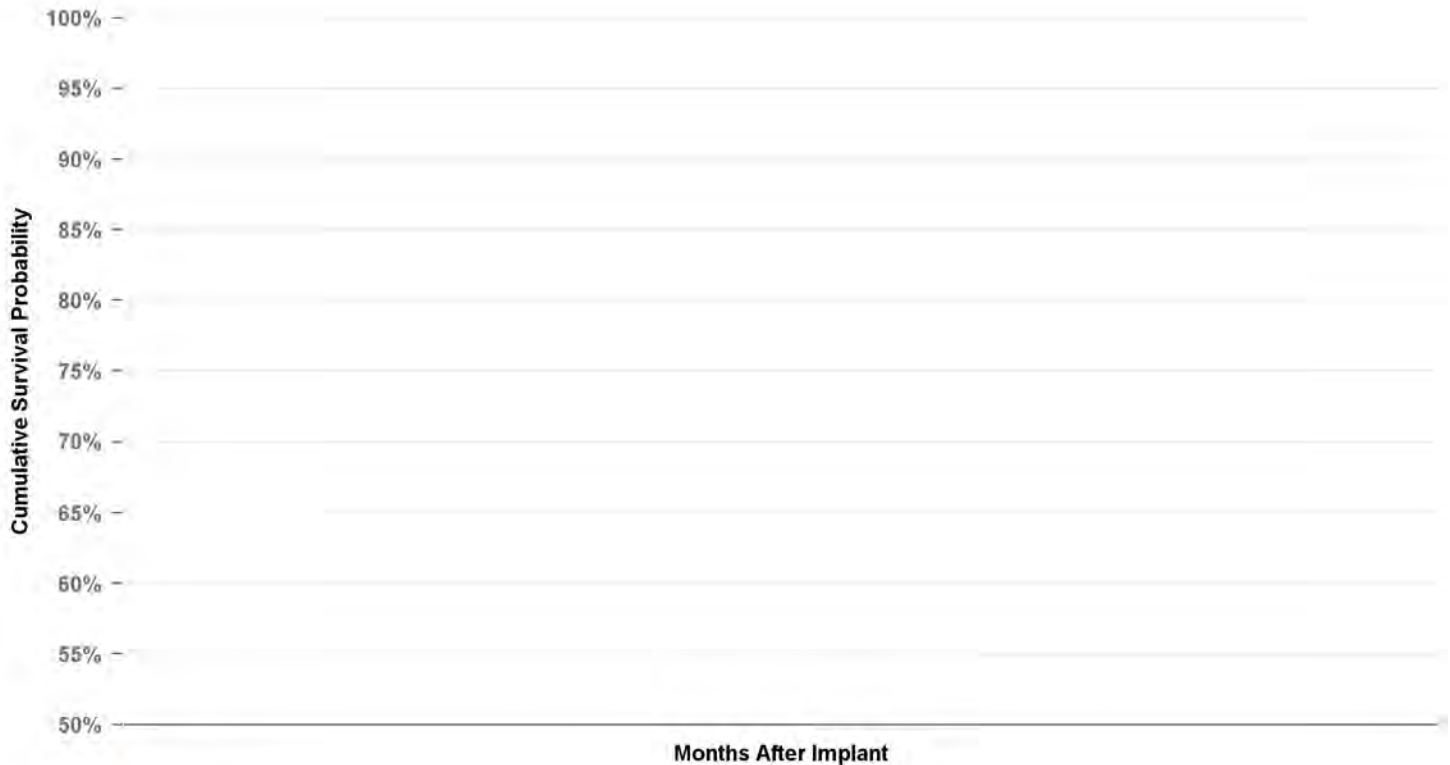

Graph Name

- Cumulative Survival Probability Graph
- Lower 95 Pct Confidence Graph
- Upper 95 Pct Confidence Graph

Years

%

#

Product Surveillance Registry Qualifying Complications

| | |
|---|----------|
| | 0 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 2 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 8 |
| Failure To Capture | 1 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 1 |
| Oversensing | 0 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 0 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 0 |
| Other | 1 |

DEFIBRILLATION LEAD

6721

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 3/31/1994 |
| CE Approval Date | 1/1/1993 |
| Registered US Implants | 2,973 |
| Estimated Active US | 1,125 |

Product Characteristics

| | |
|---------------------|----------------|
| Fixation Type | Suture |
| Lead Function | Defibrillation |
| Steroid Indicator | None |
| Lead Placement | Epi Patch |
| Lead Tip Location | Epicardial |
| Pace/Sense Polarity | n/a |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 410 |
| Cumulative Months of Follow-Up | 23,499 |
| Number of Leads Active in Study | 3 |

Product Surveillance Registry Qualifying Complications

47


| | |
|---|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 21 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 8 |
| Failure To Sense | 0 |
| Impedance Abnormal | 4 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 2 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 12 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 1 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 1 |
| Impedance Abnormal | 3 |
| Insulation Breach | 0 |
| Lead Dislodgement | 0 |
| Oversensing | 1 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 13 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 1 |
| Other | 0 |

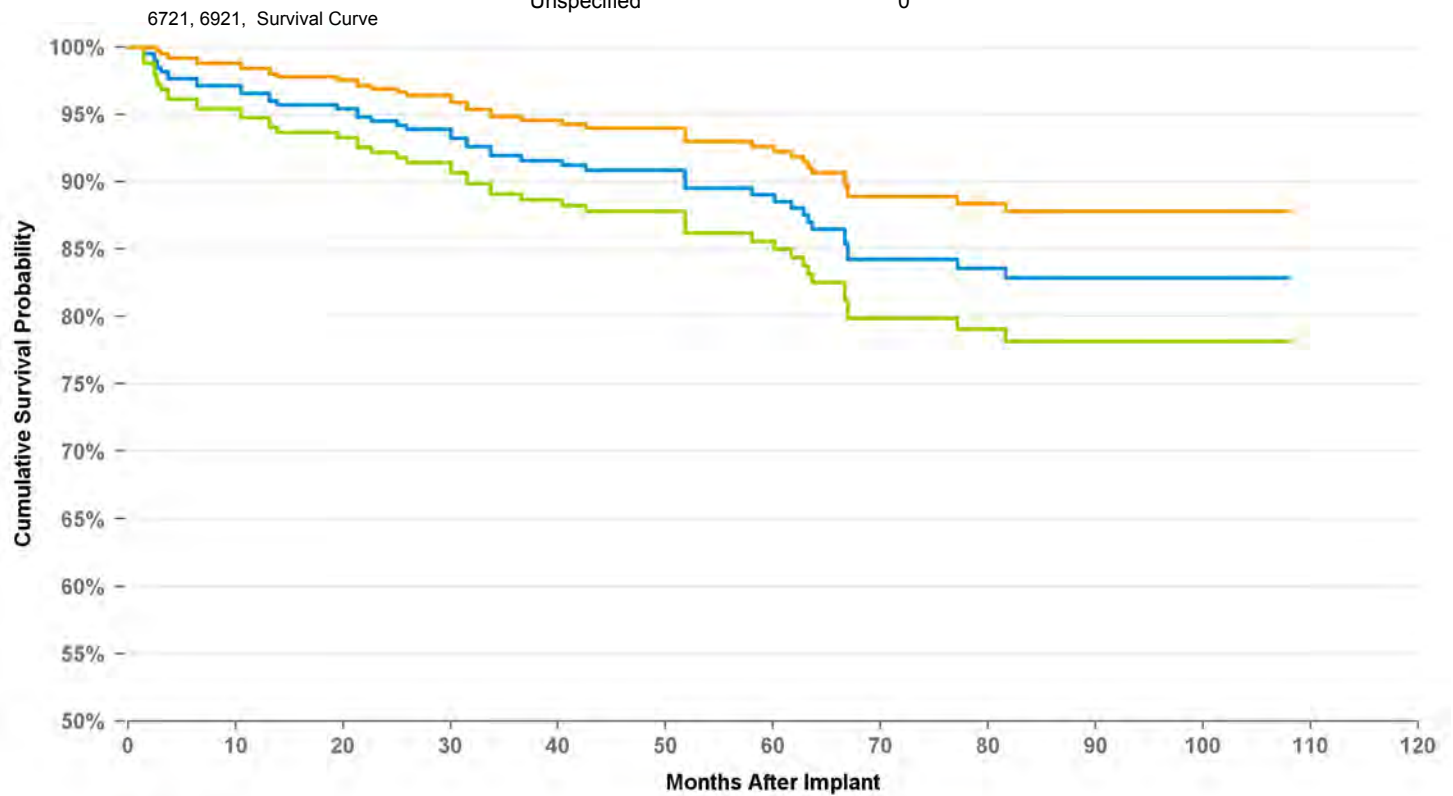

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 108 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 96.6% | 94.5% | 91.9% | 90.8% | 89.0% | 84.3% | 82.9% | 82.9% | 82.9% |
| # | 342 | 312 | 267 | 215 | 182 | 131 | 98 | 63 | 55 |

DEFIBRILLATION LEAD

6930

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 9/2/2004 |
| CE Approval Date | |
| Registered US Implants | 354 |
| Estimated Active US | 147 |


Product Characteristics

| | |
|---------------------|-----------------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | True Bipolar/One Coil |

Product Surveillance Registry Results

| | |
|-----------------------------------|-----|
| Number of Leads Enrolled in Study | 4 |
| Cumulative Months of Follow-Up | 211 |
| Number of Leads Active in Study | 2 |

6930, Survival Curve

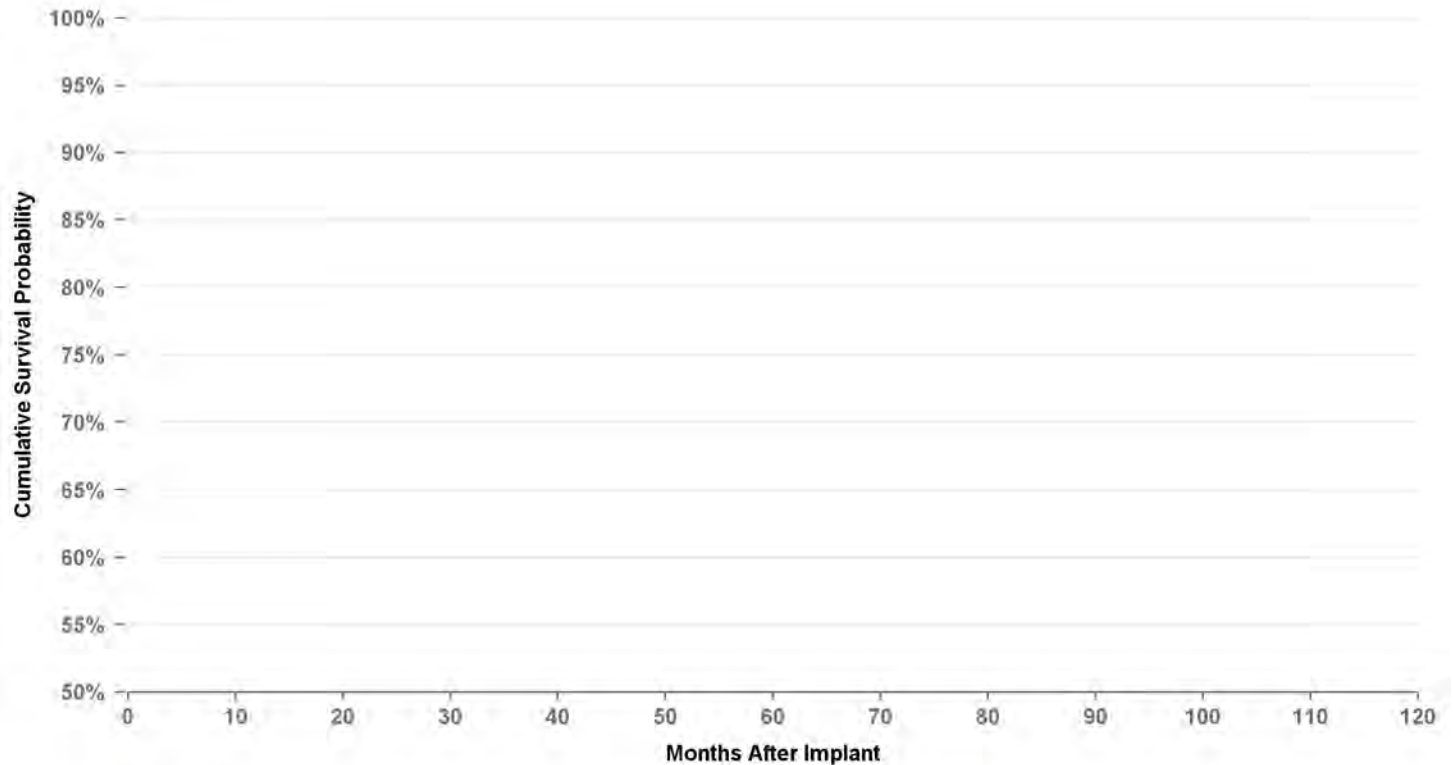

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

Years

%

#

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| | 0 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 0 |
| Oversensing | 0 |
| Unspecified | 1 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 5 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 0 |
| Other | 0 |

DEFIBRILLATION LEAD

6931

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 9/2/2004 |
| CE Approval Date | |
| Registered US Implants | 8,080 |
| Estimated Active US | 2,951 |

Product Characteristics

| | |
|---------------------|-----------------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | True Bipolar/One Coil |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 301 |
| Cumulative Months of Follow-Up | 15,661 |
| Number of Leads Active in Study | 50 |

Product Surveillance Registry Qualifying Complications


| | |
|---|-----------|
| | 55 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 33 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 3 |
| Failure To Sense | 1 |
| Impedance Abnormal | 9 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 2 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 7 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 1 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 1 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 1 |
| Oversensing | 3 |
| Unspecified | 1 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 586 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 1 |
| Other | 5 |

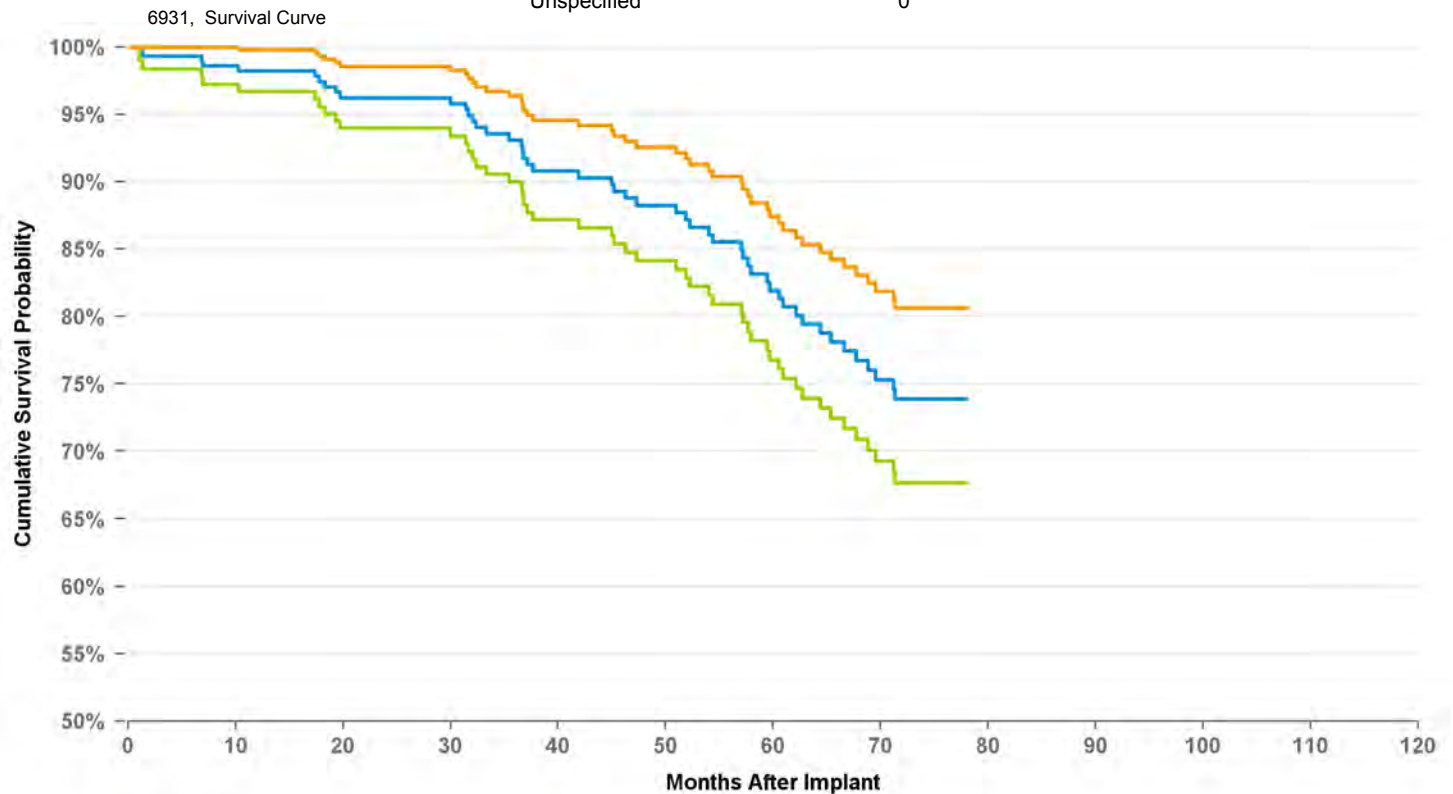

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 78 mo |
|-------|-------|-------|-------|-------|-------|-------|----------|
| % | 98.2% | 96.2% | 93.1% | 88.3% | 81.9% | 73.8% | 73.8% |
| # | 267 | 236 | 204 | 162 | 132 | 97 | 76 |

DEFIBRILLATION LEAD

6932

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 8/6/1996 |
| CE Approval Date | |
| Registered US Implants | 14,899 |
| Estimated Active US | 4,000 |

Product Characteristics

| | |
|---------------------|-----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | True Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 418 |
| Cumulative Months of Follow-Up | 25,621 |
| Number of Leads Active in Study | 34 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 2 |
| Failure To Sense | 2 |
| Impedance Abnormal | 2 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 4 |
| Unspecified | 0 |


11

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 2 |
| Failure To Sense | 2 |
| Impedance Abnormal | 1 |
| Insulation Breach | 0 |
| Lead Dislodgement | 4 |
| Oversensing | 0 |
| Unspecified | 2 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 23 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 26 |
| Other | 2 |

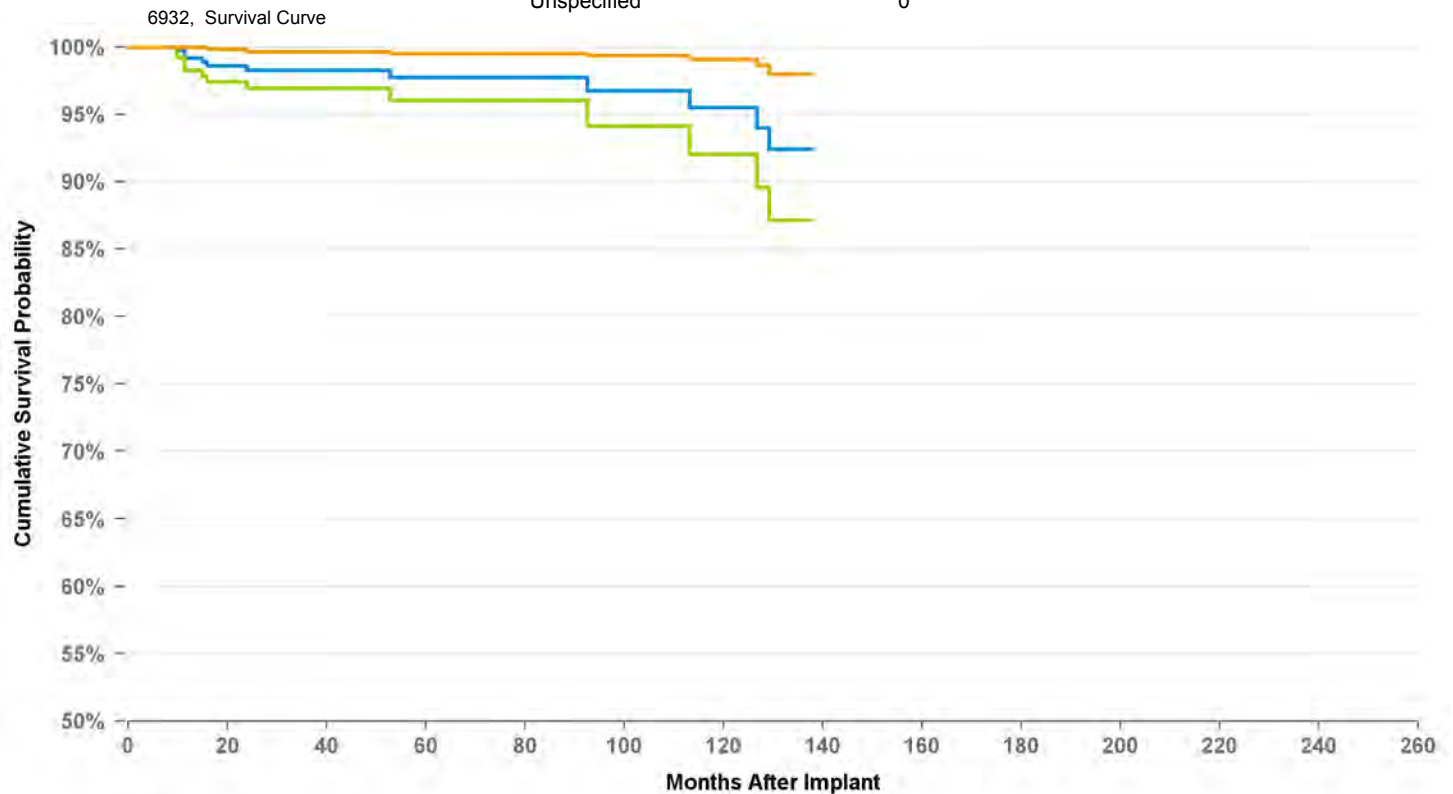

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 138 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.2% | 98.3% | 98.3% | 98.3% | 97.7% | 97.7% | 97.7% | 96.7% | 96.7% | 95.5% | 92.4% | 92.4% |
| # | 361 | 303 | 242 | 203 | 157 | 125 | 105 | 91 | 81 | 68 | 55 | 53 |

DEFIBRILLATION LEAD

6933

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 4/20/1994 |
| CE Approval Date | |
| Registered US Implants | 7,978 |
| Estimated Active US | 753 |

Product Characteristics

| | |
|---------------------|----------------|
| Fixation Type | Passive |
| Lead Function | Defibrillation |
| Steroid Indicator | None |
| Lead Placement | Transvenous |
| Lead Tip Location | SVC/CS |
| Pace/Sense Polarity | One Coil |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 968 |
| Cumulative Months of Follow-Up | 54,252 |
| Number of Leads Active in Study | 7 |

Product Surveillance Registry Qualifying Complications

| | |
|---|-----------|
| Total | 47 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 16 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 4 |
| Failure To Capture | 6 |
| Failure To Sense | 1 |
| Impedance Abnormal | 3 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 2 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 10 |
| Unspecified | 4 |


US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 0 |
| Oversensing | 0 |
| Unspecified | 3 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 105 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 16 |
| Other | 0 |

6933, 6937, 6937A, 6963, Survival Curve

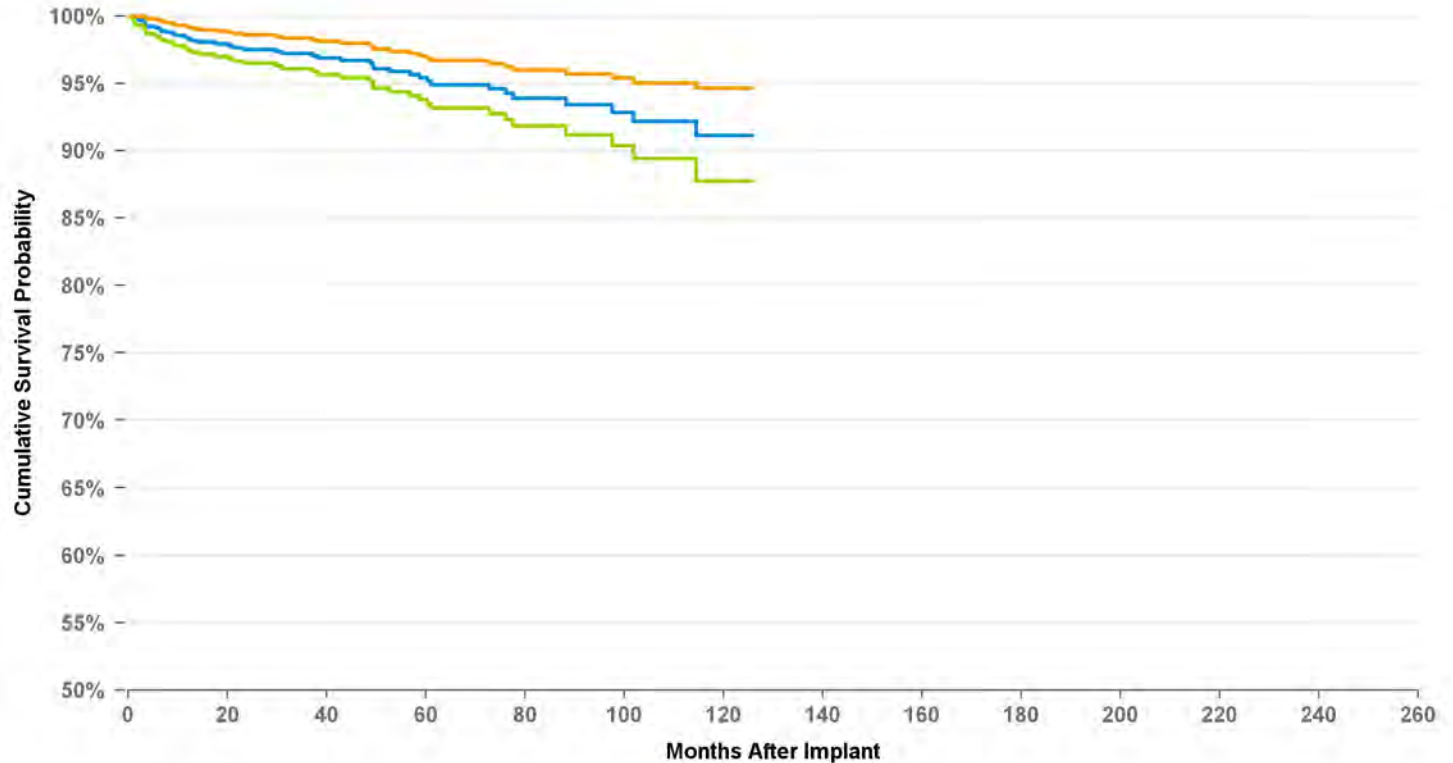

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 98.4% | 97.5% | 97.2% | 96.7% | 95.4% | 94.9% | 93.9% | 93.4% | 92.2% | 91.1% | 91.1% |
| # | 822 | 691 | 576 | 484 | 388 | 312 | 219 | 170 | 111 | 72 | 57 |

DEFIBRILLATION LEAD

6935

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 11/1/2008 |
| CE Approval Date | 3/31/2008 |
| Registered US Implants | 49,968 |
| Estimated Active US | 43,965 |

Product Characteristics

| | |
|---------------------|-----------------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | True Bipolar/One Coil |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 2,350 |
| Cumulative Months of Follow-Up | 61,342 |
| Number of Leads Active in Study | 1,438 |

Product Surveillance Registry Qualifying Complications

| | |
|---|-----------|
| | 23 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 7 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 2 |
| Failure To Sense | 1 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 7 |
| Medical Judgment | 0 |
| Other Complication | 1 |
| Oversensing | 4 |
| Unspecified | 0 |


US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 14 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 19 |
| Failure To Sense | 5 |
| Impedance Abnormal | 14 |
| Insulation Breach | 1 |
| Lead Dislodgement | 33 |
| Oversensing | 37 |
| Unspecified | 5 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 133 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 4 |
| Other | 37 |

6935, Survival Curve

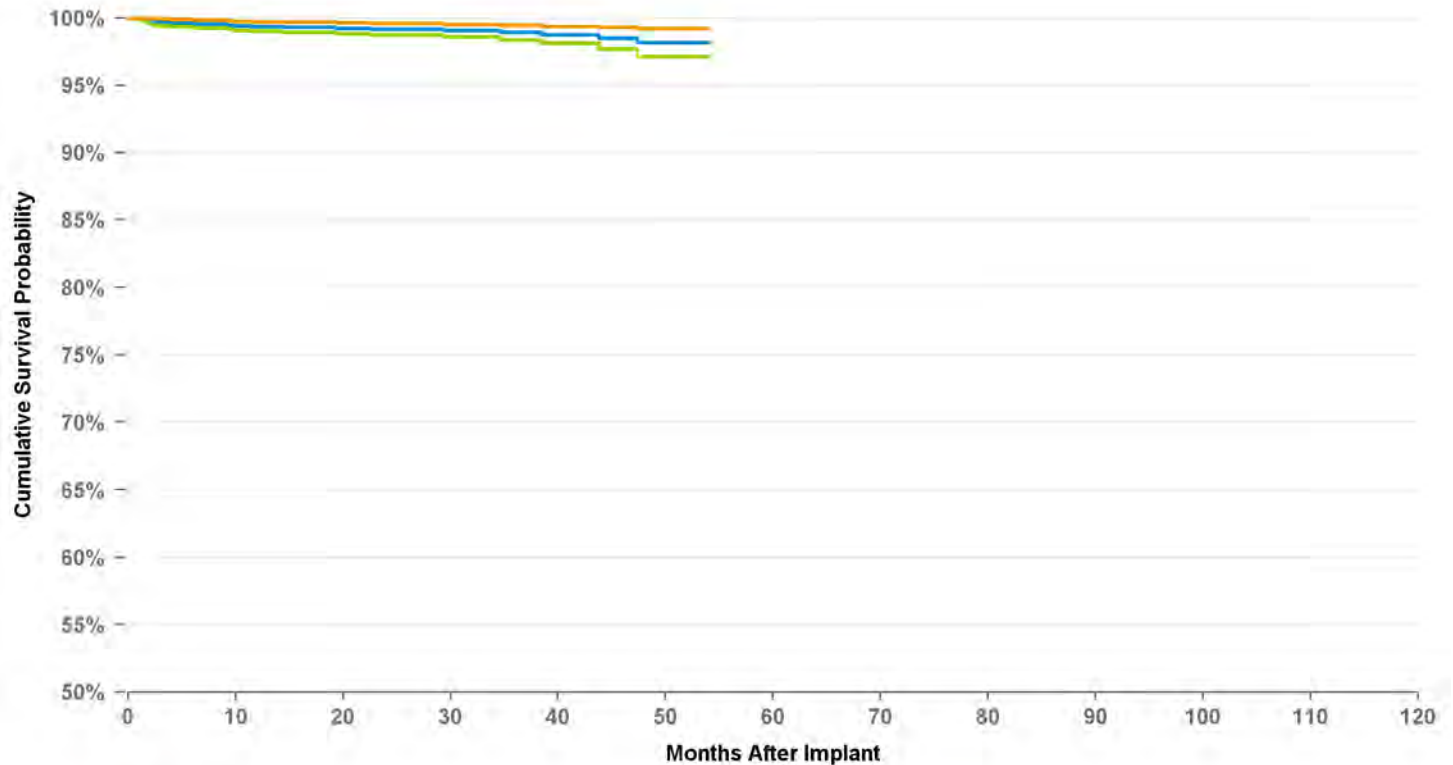

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | at 54 mo |
|-------|-------|-------|-------|-------|----------|
| % | 99.4% | 99.2% | 98.9% | 98.2% | 98.2% |
| # | 1,872 | 1,203 | 636 | 249 | 104 |

DEFIBRILLATION LEAD

6935M

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 8/2/2012 |
| CE Approval Date | 7/12/2012 |
| Registered US Implants | 45,858 |
| Estimated Active US | 44,333 |

Product Characteristics

| | |
|---------------------|-----------------------|
| Fixation Type | Active Screw in |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | True Bipolar/One Coil |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,709 |
| Cumulative Months of Follow-Up | 10,011 |
| Number of Leads Active in Study | 1,553 |

Product Surveillance Registry Qualifying Complications


| | |
|---|----------|
| | 5 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 2 |
| Medical Judgment | 0 |
| Other Complication | 1 |
| Oversensing | 1 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 12 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 4 |
| Failure To Capture | 38 |
| Failure To Sense | 6 |
| Impedance Abnormal | 7 |
| Insulation Breach | 1 |
| Lead Dislodgement | 57 |
| Oversensing | 33 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 10 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 1 |
| Other | 4 |

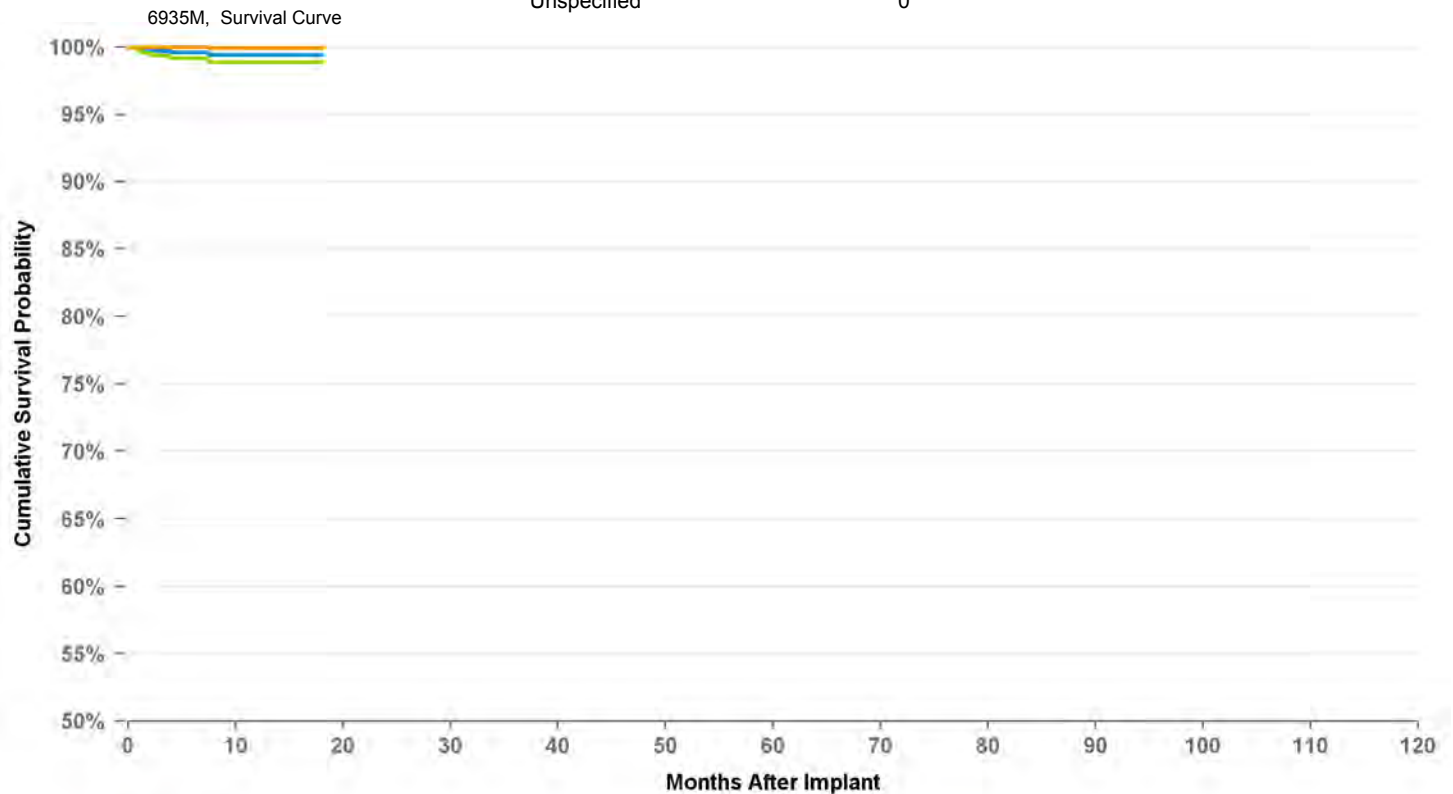

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| | | |
|-------|-------|----------|
| Years | 1 | at 18 mo |
| % | 99.4% | 99.4% |
| # | 329 | 116 |

DEFIBRILLATION LEAD

6937

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 3/22/1996 |
| CE Approval Date | 4/19/1994 |
| Registered US Implants | 2,056 |
| Estimated Active US | 380 |

Product Characteristics

| | |
|---------------------|----------------|
| Fixation Type | Passive |
| Lead Function | Defibrillation |
| Steroid Indicator | None |
| Lead Placement | Transvenous |
| Lead Tip Location | SVC/CS |
| Pace/Sense Polarity | One Coil |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 968 |
| Cumulative Months of Follow-Up | 54,252 |
| Number of Leads Active in Study | 7 |

Product Surveillance Registry Qualifying Complications

| | |
|---|-----------|
| Total | 47 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 16 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 4 |
| Failure To Capture | 6 |
| Failure To Sense | 1 |
| Impedance Abnormal | 3 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 2 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 10 |
| Unspecified | 4 |


US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 1 |
| Oversensing | 0 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 18 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 2 |
| Other | 1 |

6933, 6937, 6937A, 6963, Survival Curve

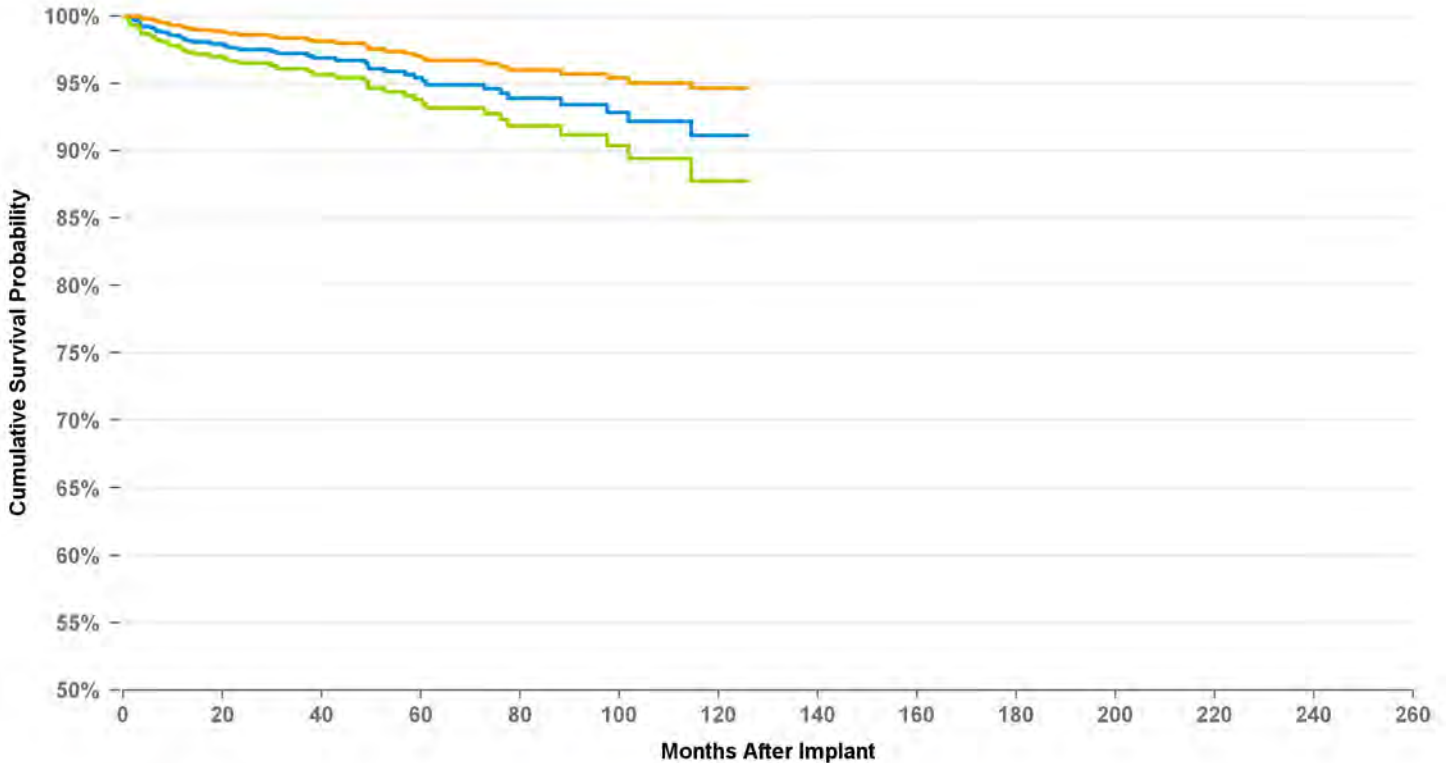

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 98.4% | 97.5% | 97.2% | 96.7% | 95.4% | 94.9% | 93.9% | 93.4% | 92.2% | 91.1% | 91.1% |
| # | 822 | 691 | 576 | 484 | 388 | 312 | 219 | 170 | 111 | 72 | 57 |

DEFIBRILLATION LEAD

6937A

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 4/6/2001 |
| CE Approval Date | |
| Registered US Implants | 2,072 |
| Estimated Active US | 1,315 |

Product Characteristics

| | |
|---------------------|----------------|
| Fixation Type | Passive |
| Lead Function | Defibrillation |
| Steroid Indicator | None |
| Lead Placement | Transvenous |
| Lead Tip Location | SVC/CS |
| Pace/Sense Polarity | One Coil |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 968 |
| Cumulative Months of Follow-Up | 54,252 |
| Number of Leads Active in Study | 7 |

Product Surveillance Registry Qualifying Complications

| | |
|---|-----------|
| Total | 47 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 16 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 4 |
| Failure To Capture | 6 |
| Failure To Sense | 1 |
| Impedance Abnormal | 3 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 2 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 10 |
| Unspecified | 4 |


US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 3 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 0 |
| Oversensing | 0 |
| Unspecified | 2 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 4 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 0 |
| Other | 0 |

6933, 6937, 6937A, 6963, Survival Curve

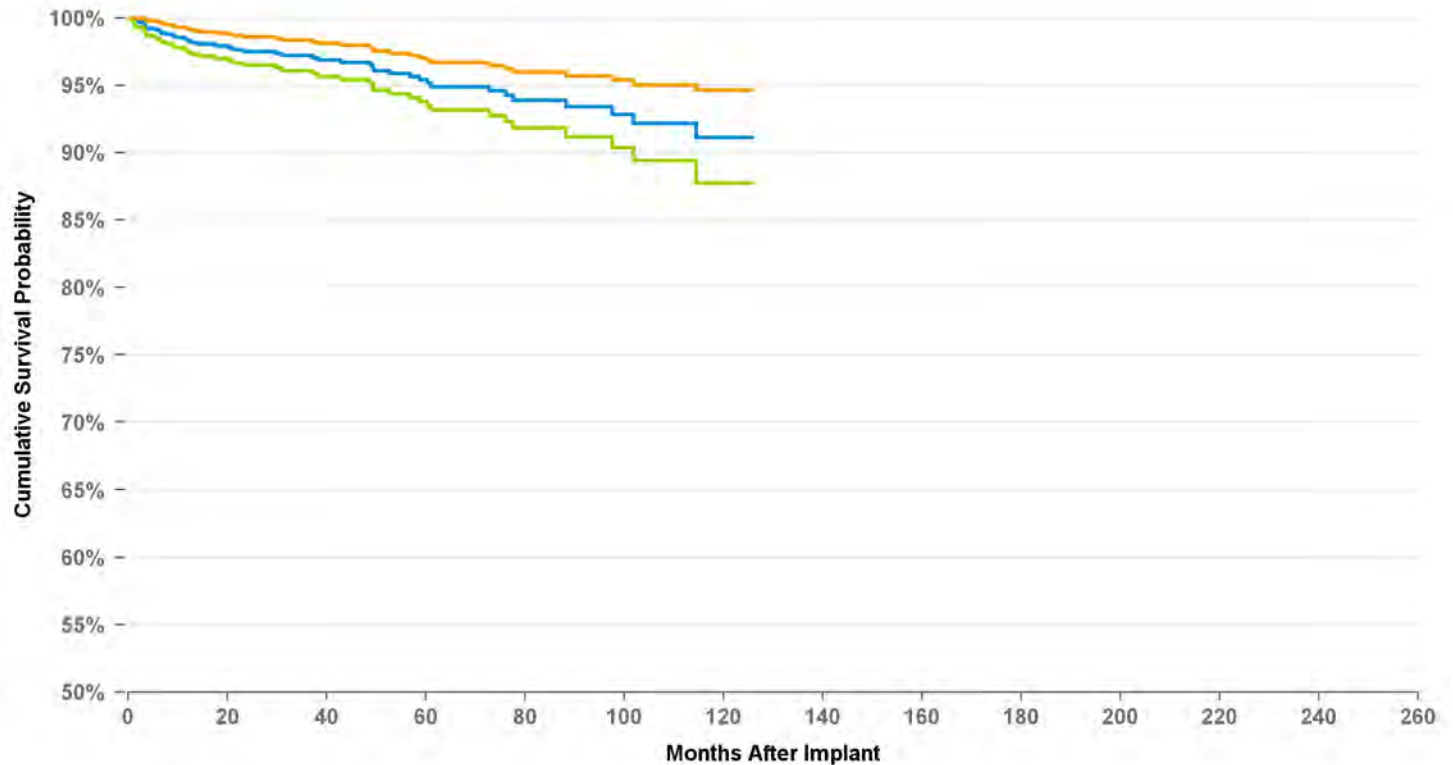

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 98.4% | 97.5% | 97.2% | 96.7% | 95.4% | 94.9% | 93.9% | 93.4% | 92.2% | 91.1% | 91.1% |
| # | 822 | 691 | 576 | 484 | 388 | 312 | 219 | 170 | 111 | 72 | 57 |

DEFIBRILLATION LEAD

6942

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 7/18/1997 |
| CE Approval Date | |
| Registered US Implants | 17,685 |
| Estimated Active US | 4,935 |

Product Characteristics

| | |
|---------------------|----------------------------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Integrated Bipolar/ Two Coils |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 358 |
| Cumulative Months of Follow-Up | 19,291 |
| Number of Leads Active in Study | 14 |

Product Surveillance Registry Qualifying Complications


| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 1 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 3 |
| Unspecified | 1 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 4 |
| Failure To Sense | 0 |
| Impedance Abnormal | 2 |
| Insulation Breach | 0 |
| Lead Dislodgement | 1 |
| Oversensing | 2 |
| Unspecified | 1 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 15 |
| Crimp Weld Bond | 1 |
| Insulation Breach | 25 |
| Other | 4 |

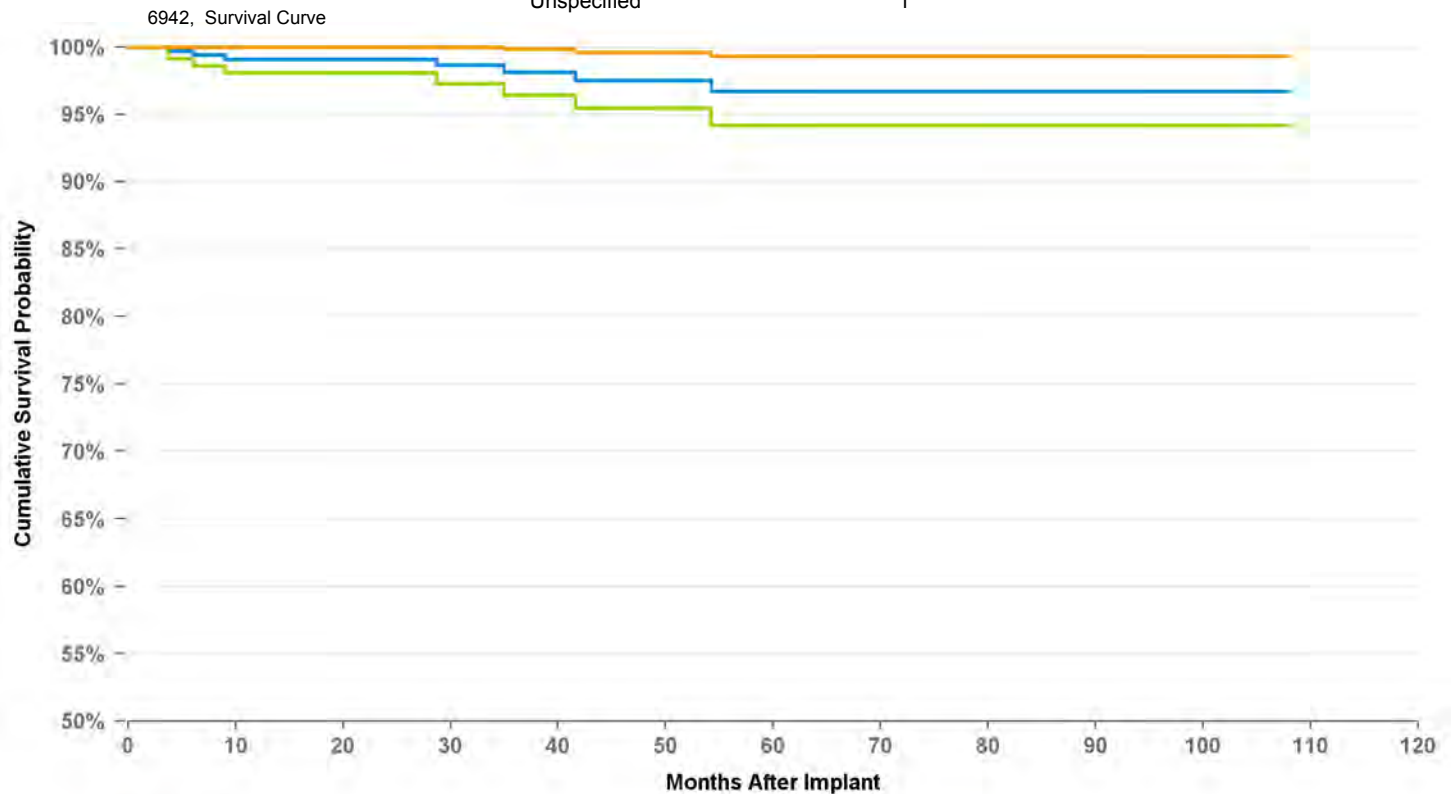

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 108 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.1% | 99.1% | 98.1% | 97.5% | 96.7% | 96.7% | 96.7% | 96.7% | 96.7% |
| # | 305 | 236 | 180 | 140 | 113 | 96 | 75 | 64 | 53 |

DEFIBRILLATION LEAD

6943

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 10/6/1997 |
| CE Approval Date | |
| Registered US Implants | 20,610 |
| Estimated Active US | 5,793 |

Product Characteristics

| | |
|---------------------|-----------------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | True Bipolar/One Coil |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,332 |
| Cumulative Months of Follow-Up | 83,939 |
| Number of Leads Active in Study | 151 |

Product Surveillance Registry Qualifying Complications


| | |
|---|------------|
| | 103 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 29 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 9 |
| Failure To Sense | 7 |
| Impedance Abnormal | 8 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 2 |
| Lead Dislodgement | 2 |
| Medical Judgment | 0 |
| Other Complication | 2 |
| Oversensing | 41 |
| Unspecified | 3 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 1 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 1 |
| Impedance Abnormal | 2 |
| Insulation Breach | 1 |
| Lead Dislodgement | 0 |
| Oversensing | 1 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 80 |
| Crimp Weld Bond | 1 |
| Insulation Breach | 31 |
| Other | 5 |

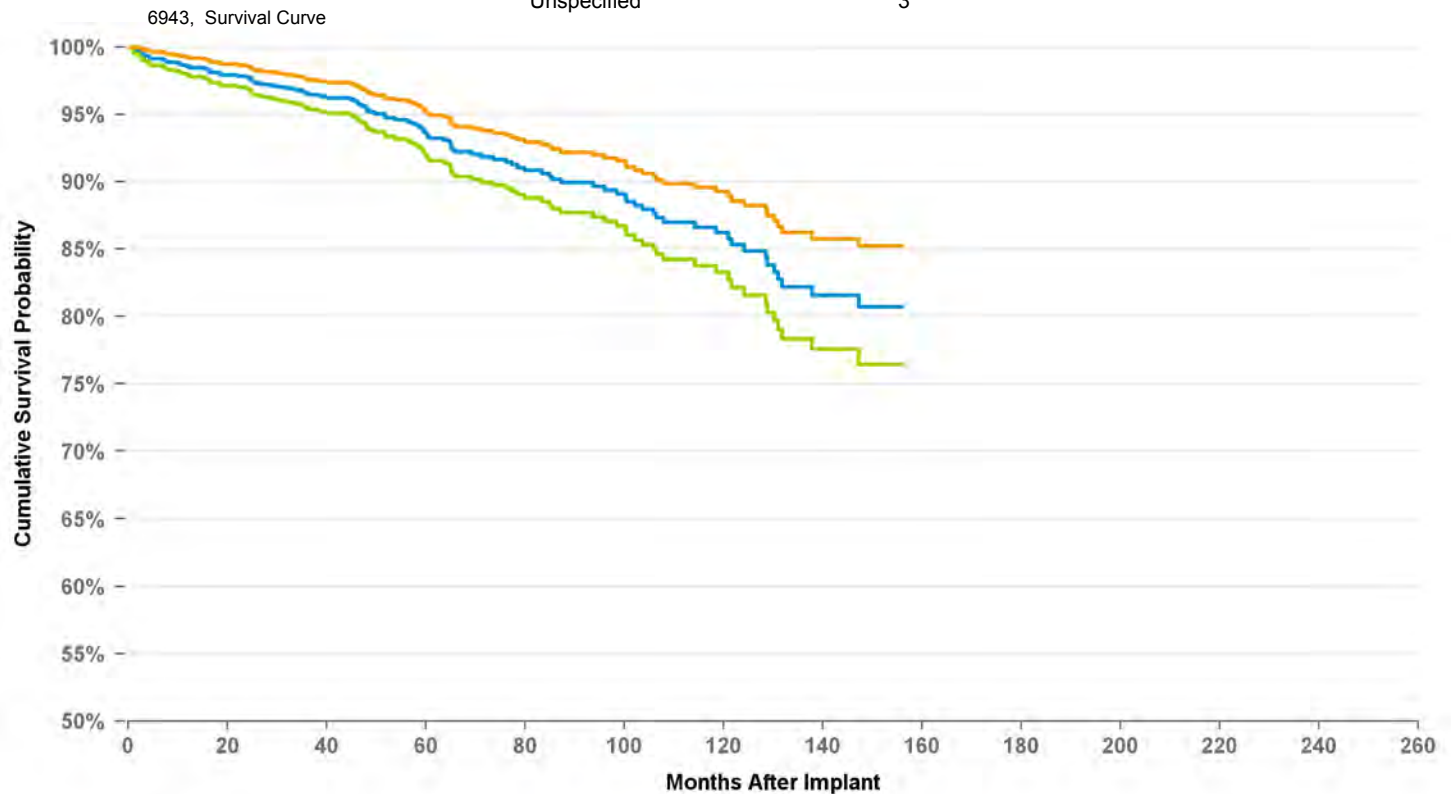

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | at 156 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 98.6% | 97.7% | 96.6% | 95.6% | 93.5% | 91.9% | 90.6% | 89.7% | 87.0% | 86.2% | 82.2% | 81.6% | 80.7% |
| # | 1,172 | 984 | 861 | 711 | 597 | 485 | 397 | 326 | 270 | 194 | 143 | 100 | 55 |

DEFIBRILLATION LEAD

6944

Distribution Data

| | |
|------------------------|------------|
| US Market Release | 12/13/2000 |
| CE Approval Date | 11/5/1999 |
| Registered US Implants | 43,462 |
| Estimated Active US | 22,097 |

Product Characteristics

| | |
|---------------------|------------------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | True Bipolar/Two Coils |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 566 |
| Cumulative Months of Follow-Up | 21,709 |
| Number of Leads Active in Study | 261 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 7 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 1 |
| Impedance Abnormal | 2 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 2 |
| Unspecified | 1 |


13

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 14 |
| Failure To Sense | 3 |
| Impedance Abnormal | 8 |
| Insulation Breach | 0 |
| Lead Dislodgement | 21 |
| Oversensing | 11 |
| Unspecified | 6 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 143 |
| Crimp Weld Bond | 1 |
| Insulation Breach | 4 |
| Other | 5 |

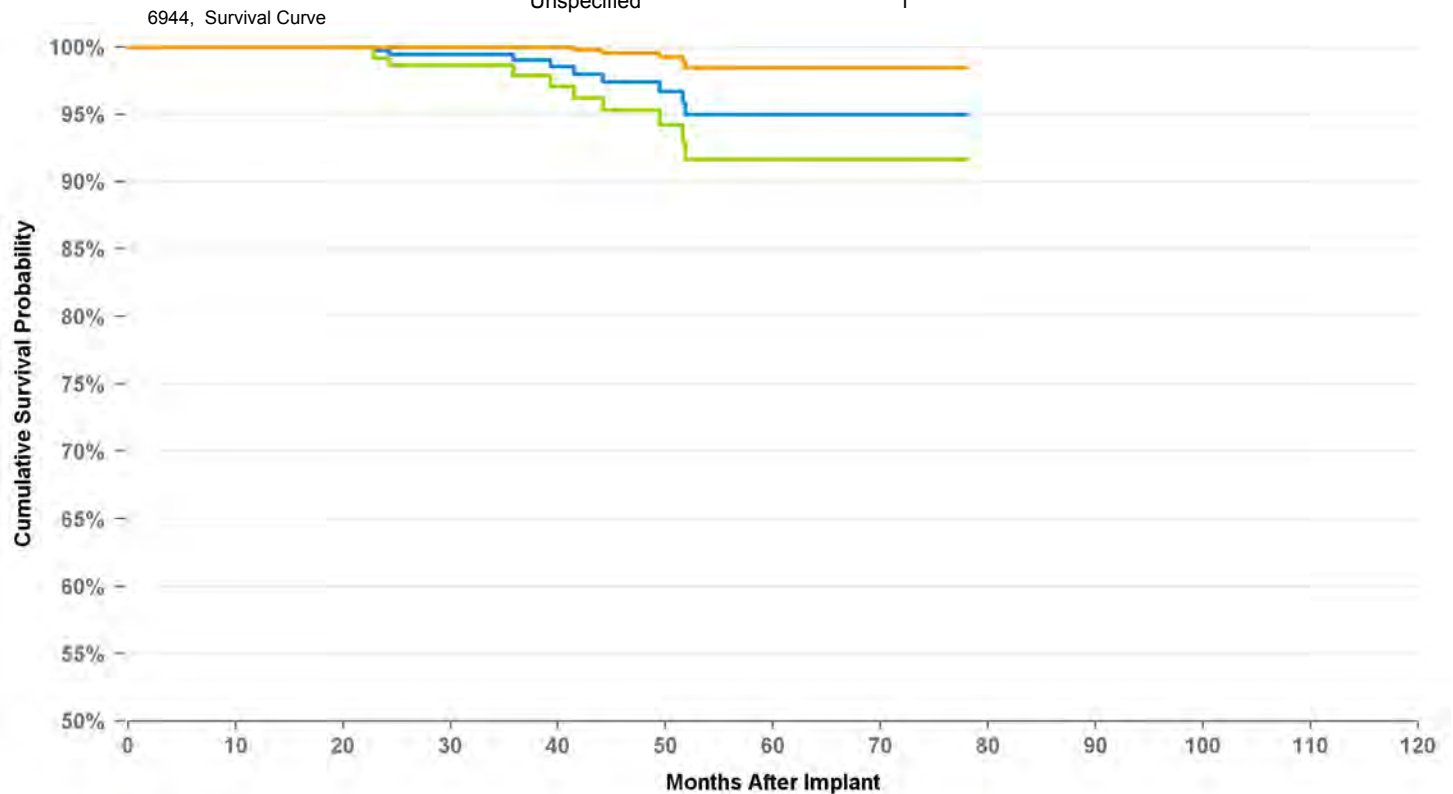

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 78 mo |
|-------|--------|-------|-------|-------|-------|-------|----------|
| % | 100.0% | 99.7% | 99.0% | 97.4% | 95.0% | 95.0% | 95.0% |
| # | 467 | 353 | 233 | 143 | 75 | 61 | 55 |

DEFIBRILLATION LEAD

6945

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 9/26/1997 |
| CE Approval Date | |
| Registered US Implants | 42,741 |
| Estimated Active US | 11,761 |

Product Characteristics

| | |
|---------------------|----------------------------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Integrated Bipolar/ Two Coils |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,186 |
| Cumulative Months of Follow-Up | 65,992 |
| Number of Leads Active in Study | 94 |

Product Surveillance Registry Qualifying Complications


| | |
|---|-----------|
| | 43 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 10 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 2 |
| Failure To Sense | 4 |
| Impedance Abnormal | 7 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 18 |
| Unspecified | 1 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 1 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 6 |
| Failure To Sense | 2 |
| Impedance Abnormal | 1 |
| Insulation Breach | 2 |
| Lead Dislodgement | 4 |
| Oversensing | 7 |
| Unspecified | 2 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 140 |
| Crimp Weld Bond | 1 |
| Insulation Breach | 43 |
| Other | 6 |

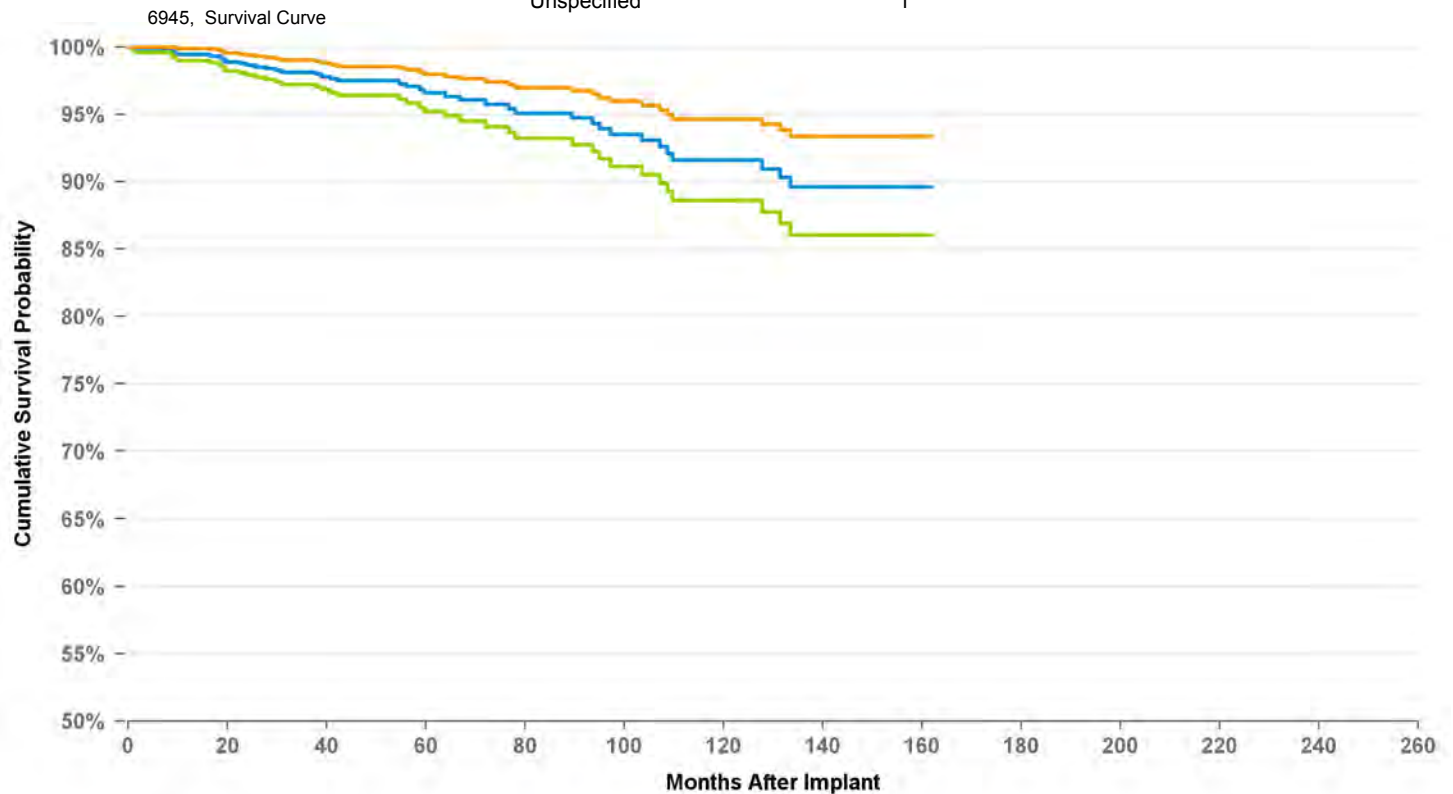

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | at 162 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.4% | 98.7% | 98.1% | 97.5% | 96.6% | 95.8% | 95.1% | 93.9% | 92.6% | 91.6% | 90.3% | 89.6% | 89.6% | 89.6% |
| # | 1,017 | 824 | 660 | 528 | 407 | 311 | 274 | 230 | 186 | 155 | 129 | 106 | 73 | 51 |

DEFIBRILLATION LEAD

6947

Distribution Data

| | |
|------------------------|------------|
| US Market Release | 11/12/2001 |
| CE Approval Date | 10/4/2001 |
| Registered US Implants | 369,050 |
| Estimated Active US | 235,704 |

Product Characteristics

| | |
|---------------------|------------------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | True Bipolar/Two Coils |

Product Surveillance Registry Results

| | |
|-----------------------------------|---------|
| Number of Leads Enrolled in Study | 3,608 |
| Cumulative Months of Follow-Up | 151,880 |
| Number of Leads Active in Study | 1,528 |

Product Surveillance Registry Qualifying Complications


| | |
|---|----|
| | 51 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 14 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 2 |
| Failure To Sense | 2 |
| Impedance Abnormal | 8 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 3 |
| Lead Dislodgement | 4 |
| Medical Judgment | 0 |
| Other Complication | 1 |
| Oversensing | 15 |
| Unspecified | 2 |

US Acute Lead Observations

| | |
|--------------------------|-----|
| Cardiac Perforation | 27 |
| Conductor Fracture | 19 |
| Extracardiac Stimulation | 2 |
| Failure To Capture | 74 |
| Failure To Sense | 30 |
| Impedance Abnormal | 54 |
| Insulation Breach | 4 |
| Lead Dislodgement | 108 |
| Oversensing | 119 |
| Unspecified | 22 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 673 |
| Crimp Weld Bond | 4 |
| Insulation Breach | 62 |
| Other | 215 |

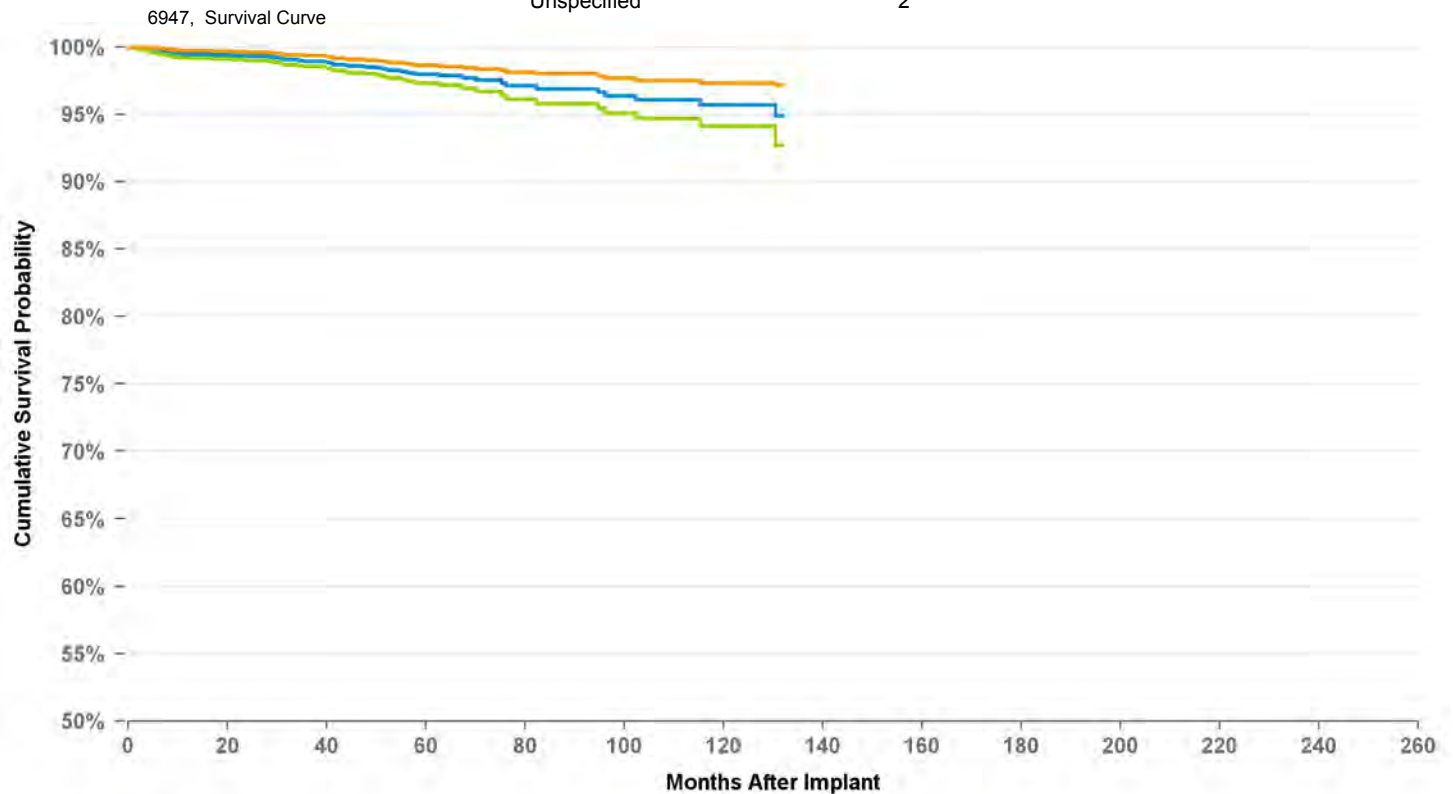

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 132 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.5% | 99.3% | 99.0% | 98.5% | 98.0% | 97.5% | 96.9% | 96.6% | 96.1% | 95.7% | 94.9% |
| # | 2,924 | 2,347 | 1,857 | 1,324 | 773 | 476 | 390 | 338 | 276 | 160 | 74 |

DEFIBRILLATION LEAD

6947M

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 2/13/2012 |
| CE Approval Date | 3/12/2010 |
| Registered US Implants | 57,035 |
| Estimated Active US | 54,254 |

Product Characteristics

| | |
|---------------------|------------------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | True Bipolar/Two Coils |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,698 |
| Cumulative Months of Follow-Up | 25,805 |
| Number of Leads Active in Study | 1,341 |

Product Surveillance Registry Qualifying Complications


| | |
|---|----------|
| | 3 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 3 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 11 |
| Conductor Fracture | 3 |
| Extracardiac Stimulation | 6 |
| Failure To Capture | 36 |
| Failure To Sense | 6 |
| Impedance Abnormal | 10 |
| Insulation Breach | 0 |
| Lead Dislodgement | 75 |
| Oversensing | 23 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 20 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 2 |
| Other | 8 |

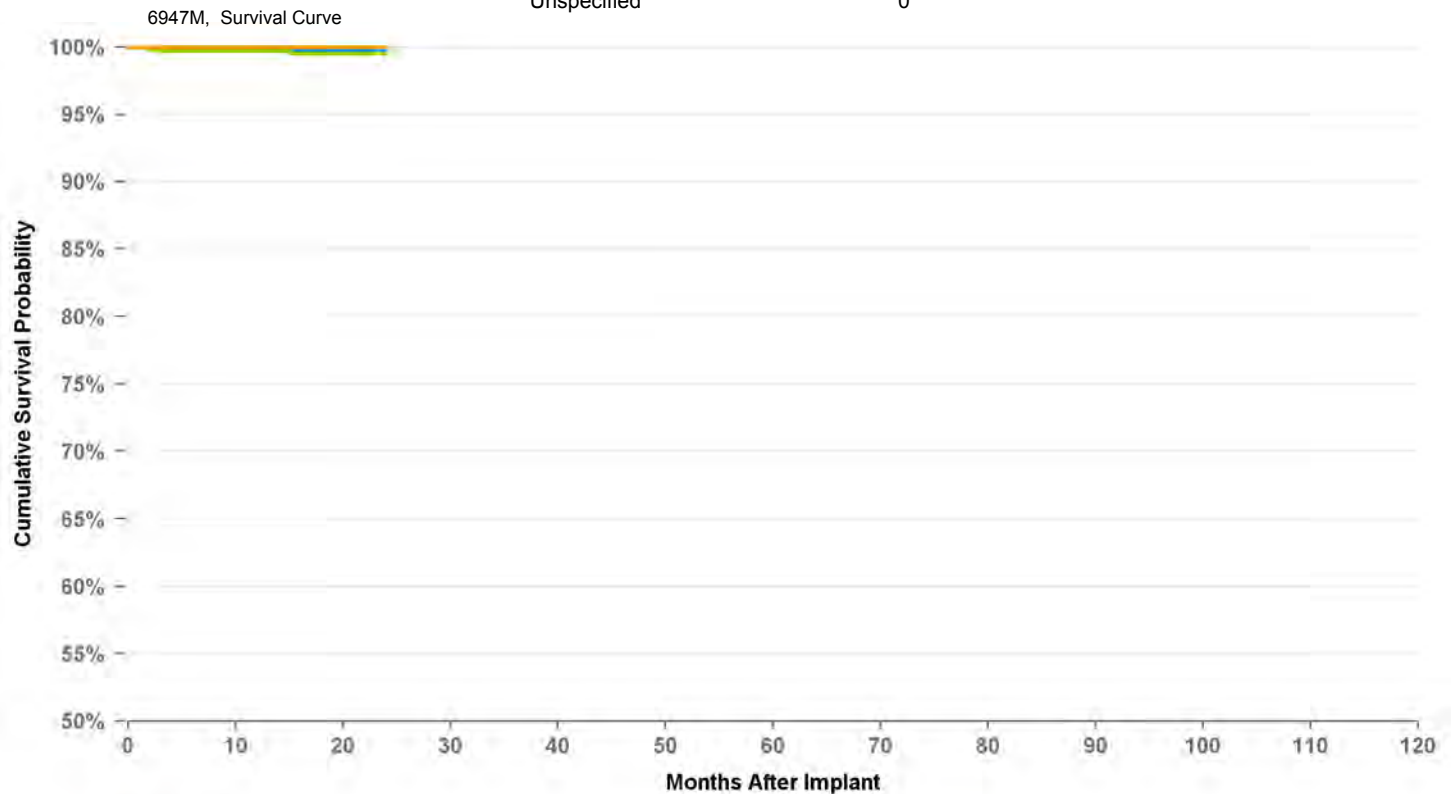

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| | | |
|-------|-------|----------|
| Years | 1 | at 24 mo |
| % | 99.9% | 99.8% |
| # | 1,103 | 273 |

DEFIBRILLATION LEAD

6948

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 9/2/2004 |
| CE Approval Date | |
| Registered US Implants | 10,379 |
| Estimated Active US | 4,218 |


Product Characteristics

| | |
|---------------------|------------------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | True Bipolar/Two Coils |

Product Surveillance Registry Results

| | |
|-----------------------------------|-------|
| Number of Leads Enrolled in Study | 37 |
| Cumulative Months of Follow-Up | 1,743 |
| Number of Leads Active in Study | 13 |

6948, Survival Curve

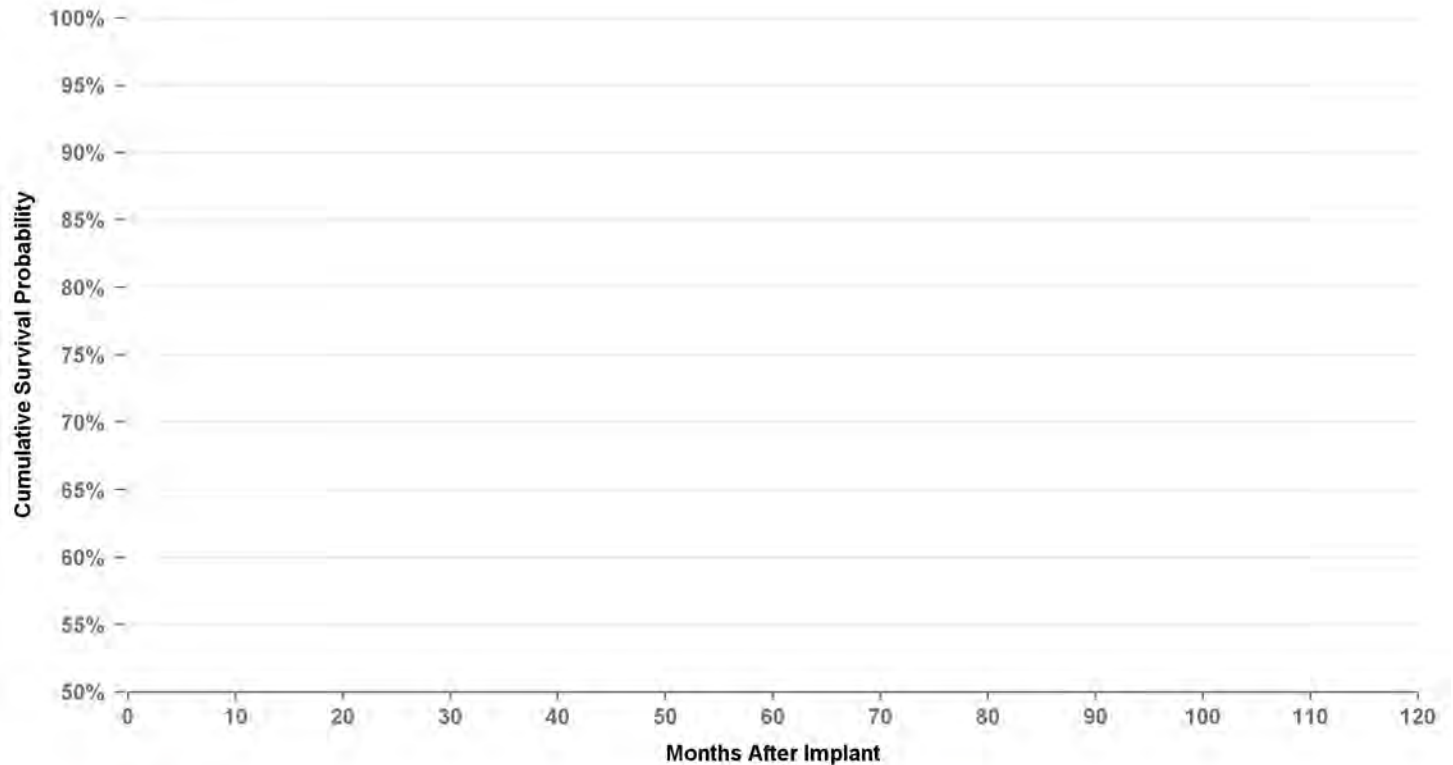

Graph Name

- Cumulative Survival Probability Graph
- Lower 95 Pct Confidence Graph
- Upper 95 Pct Confidence Graph

Years

%

#

Product Surveillance Registry Qualifying Complications

| | |
|---|----------|
| | 4 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 3 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 6 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 7 |
| Oversensing | 1 |
| Unspecified | 3 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 175 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 2 |
| Other | 2 |

DEFIBRILLATION LEAD

6949

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 9/2/2004 |
| CE Approval Date | |
| Registered US Implants | 186,784 |
| Estimated Active US | 65,386 |

Product Characteristics

| | |
|---------------------|------------------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | True Bipolar/Two Coils |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 923 |
| Cumulative Months of Follow-Up | 44,616 |
| Number of Leads Active in Study | 237 |

Product Surveillance Registry Qualifying Complications


| | |
|---|-----------|
| | 95 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 50 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 3 |
| Failure To Sense | 6 |
| Impedance Abnormal | 17 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 2 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 1 |
| Oversensing | 15 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 10 |
| Conductor Fracture | 45 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 31 |
| Failure To Sense | 19 |
| Impedance Abnormal | 17 |
| Insulation Breach | 6 |
| Lead Dislodgement | 22 |
| Oversensing | 30 |
| Unspecified | 25 |

USA Returned Product Analysis

| | |
|--------------------|-------|
| Conductor Fracture | 7,077 |
| Crimp Weld Bond | 3 |
| Insulation Breach | 32 |
| Other | 70 |

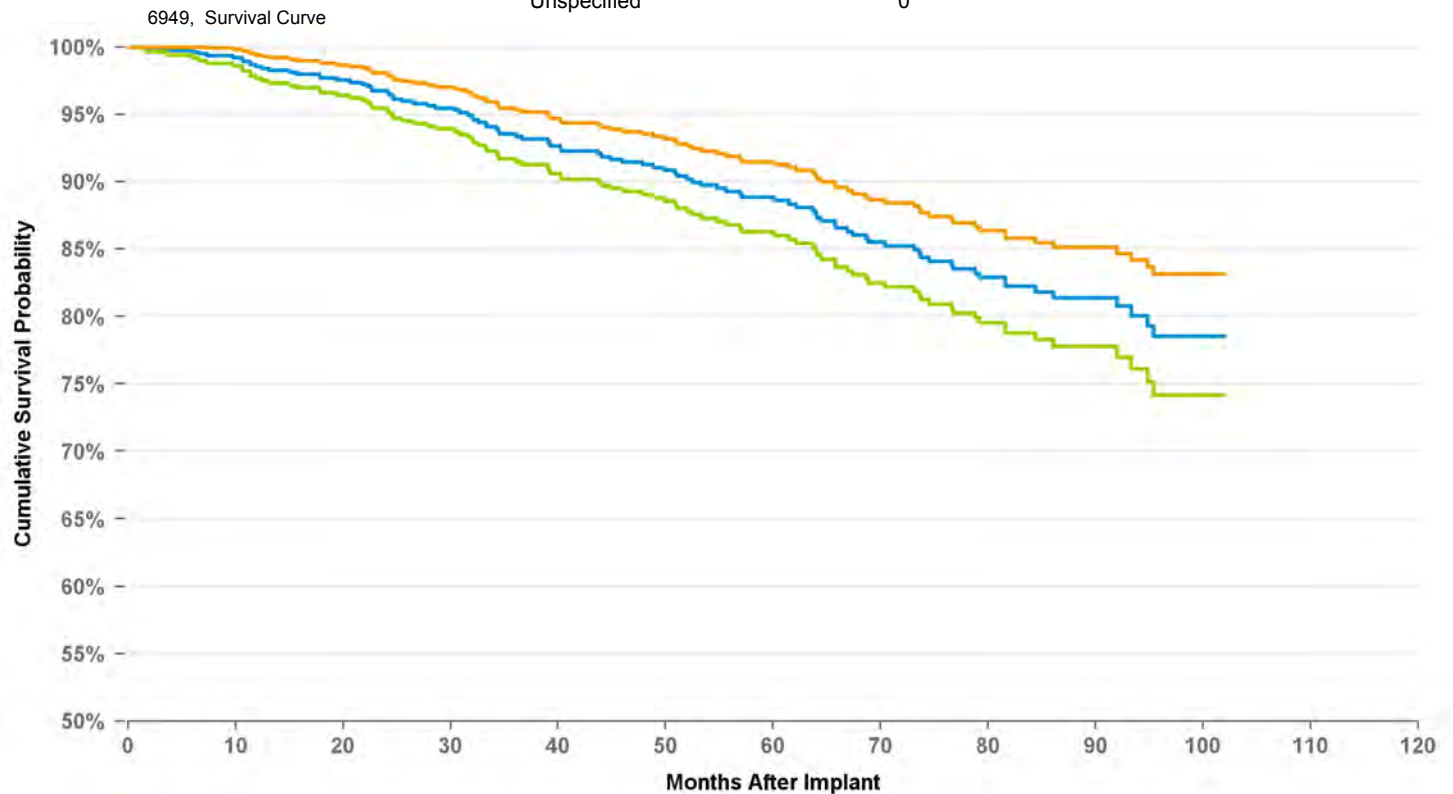

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 102 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 98.5% | 96.8% | 93.6% | 91.3% | 88.8% | 85.2% | 82.2% | 78.5% | 78.5% |
| # | 773 | 638 | 537 | 442 | 354 | 277 | 158 | 67 | 53 |

DEFIBRILLATION LEAD

6996

Distribution Data

| | |
|------------------------|------------|
| US Market Release | 6/11/2001 |
| CE Approval Date | 12/19/1997 |
| Registered US Implants | 4,248 |
| Estimated Active US | 2,483 |


Product Characteristics

| | |
|---------------------|-------------------------|
| Fixation Type | Suture on Anchor Sleeve |
| Lead Function | Defibrillation |
| Steroid Indicator | None |
| Lead Placement | Subcutaneous |
| Lead Tip Location | Defibrillation |
| Pace/Sense Polarity | One Coil |

Product Surveillance Registry Results

| | |
|-----------------------------------|-------|
| Number of Leads Enrolled in Study | 45 |
| Cumulative Months of Follow-Up | 1,420 |
| Number of Leads Active in Study | 16 |

6996, Survival Curve

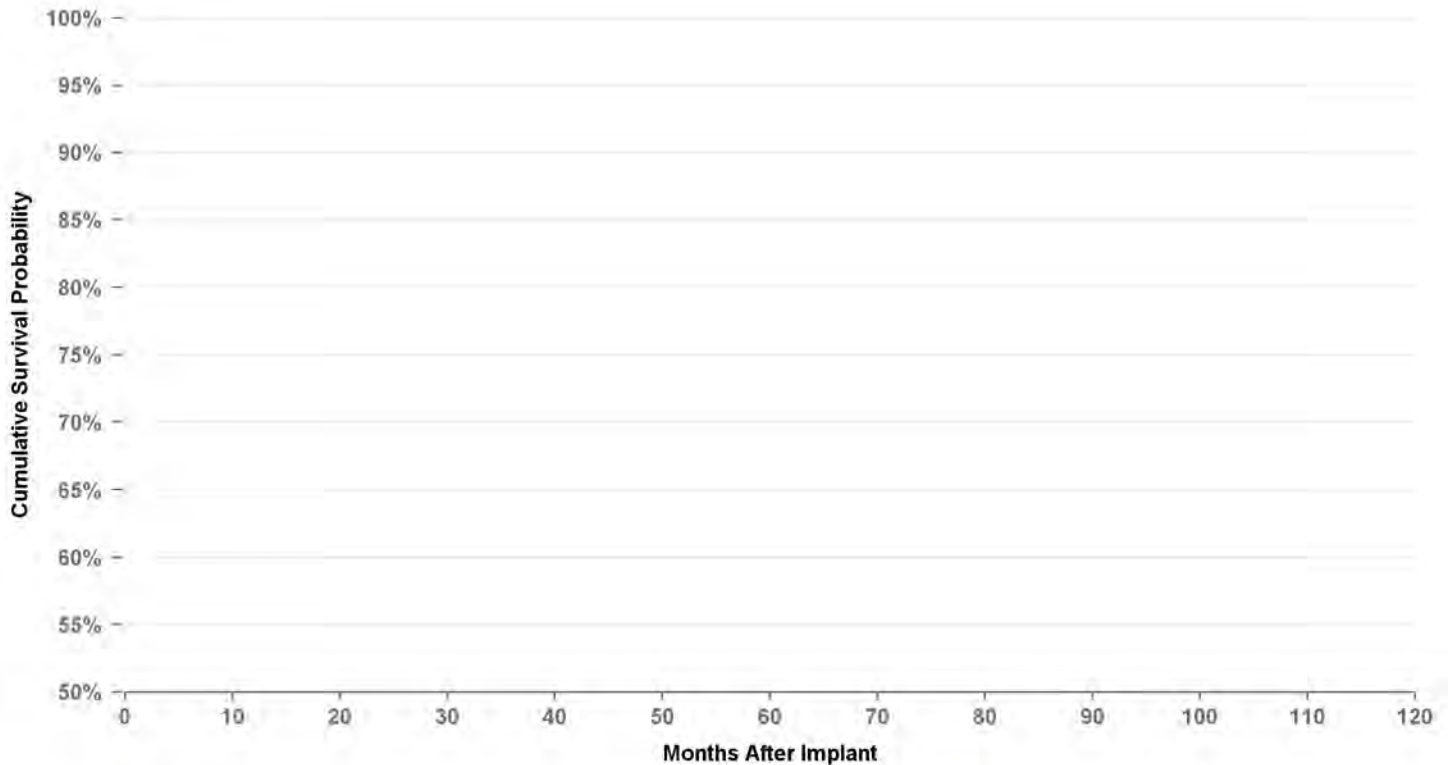

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

Years

%

#

Product Surveillance Registry Qualifying Complications

| | |
|---|----------|
| | 2 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 0 |
| Impedance Abnormal | 5 |
| Insulation Breach | 0 |
| Lead Dislodgement | 1 |
| Oversensing | 0 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 25 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 0 |
| Other | 0 |

PACING LEAD

3830

ATRIAL PLACEMENT

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 8/3/2005 |
| CE Approval Date | 1/31/2003 |
| Registered US Implants | 23,886 |
| Estimated Active US | 17,729 |

Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Fixed Screw |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 856 |
| Cumulative Months of Follow-Up | 31,736 |
| Number of Leads Active in Study | 492 |

Product Surveillance Registry Qualifying Complications

10


| | |
|---|---|
| Cardiac Perforation | 1 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 2 |
| Failure To Sense | 1 |
| Impedance Abnormal | 2 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 2 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 7 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 22 |
| Failure To Sense | 1 |
| Impedance Abnormal | 0 |
| Insulation Breach | 1 |
| Lead Dislodgement | 36 |
| Oversensing | 3 |
| Unspecified | 2 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 10 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 22 |
| Other | 3 |

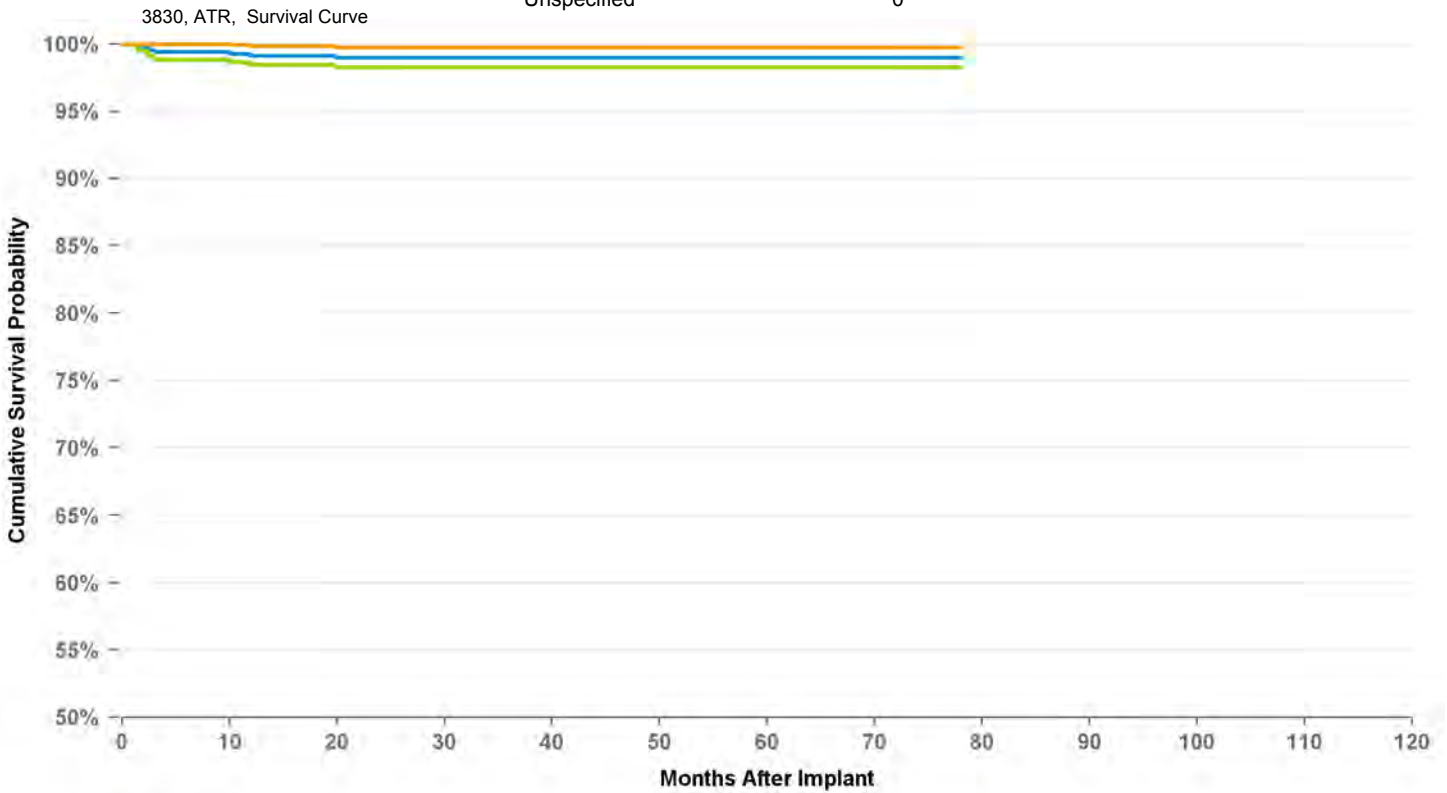

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 78 mo |
|-------|-------|-------|-------|-------|-------|-------|----------|
| % | 99.1% | 99.0% | 99.0% | 99.0% | 99.0% | 99.0% | 99.0% |
| # | 719 | 607 | 462 | 199 | 100 | 57 | 51 |

PACING LEAD

3830

VENTRICULAR PLACEMENT

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 8/3/2005 |
| CE Approval Date | 1/31/2003 |
| Registered US Implants | 23,886 |
| Estimated Active US | 17,729 |

Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Fixed Screw |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 560 |
| Cumulative Months of Follow-Up | 20,713 |
| Number of Leads Active in Study | 319 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 3 |
| Medical Judgment | 0 |
| Other Complication | 1 |
| Oversensing | 0 |
| Unspecified | 0 |


6

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 7 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 22 |
| Failure To Sense | 1 |
| Impedance Abnormal | 0 |
| Insulation Breach | 1 |
| Lead Dislodgement | 36 |
| Oversensing | 3 |
| Unspecified | 2 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 10 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 22 |
| Other | 3 |

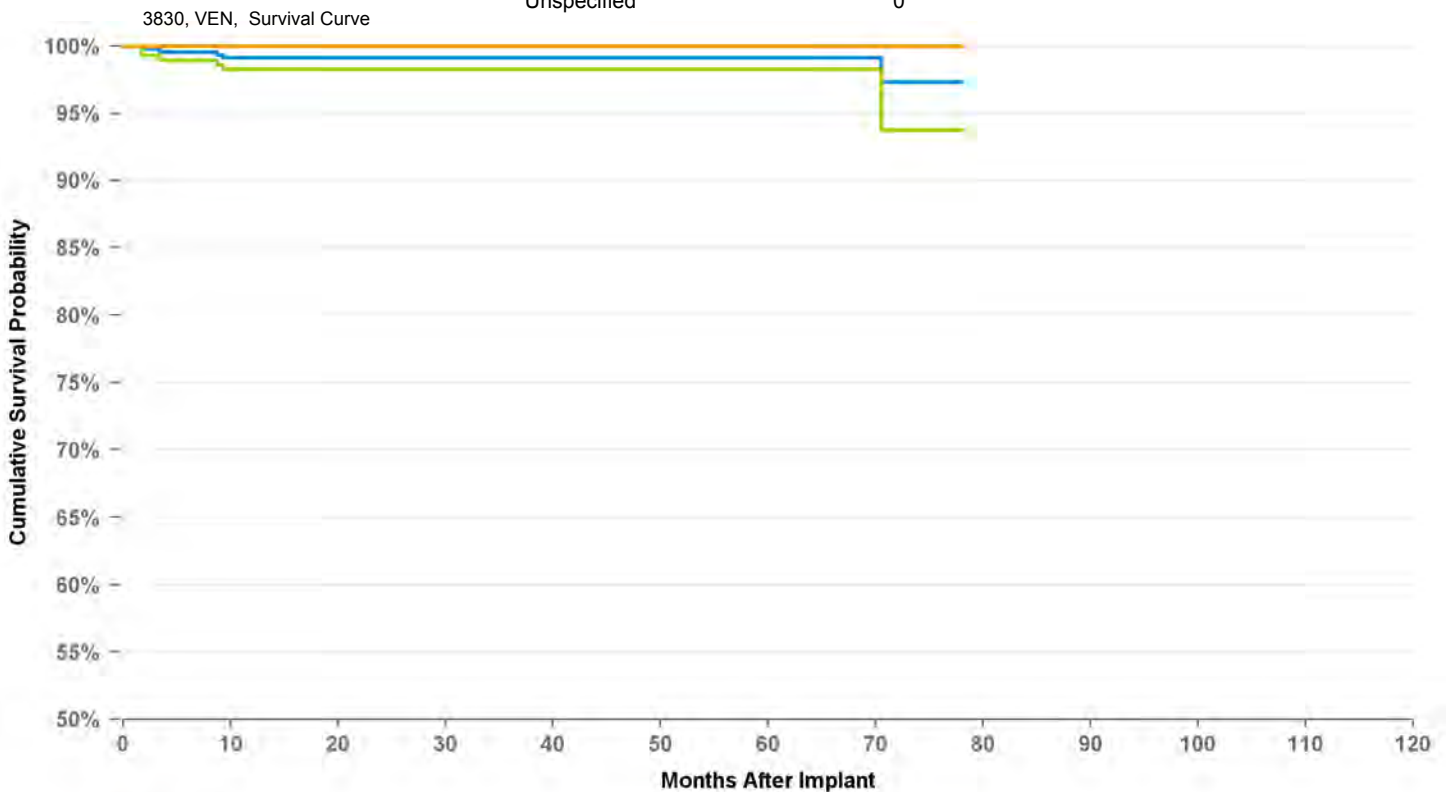

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 78 mo |
|-------|-------|-------|-------|-------|-------|-------|----------|
| % | 99.1% | 99.1% | 99.1% | 99.1% | 99.1% | 97.3% | 97.3% |
| # | 449 | 377 | 281 | 129 | 77 | 52 | 50 |

PACING LEAD

4024

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 10/1/1991 |
| CE Approval Date | |
| Registered US Implants | 218,566 |
| Estimated Active US | 37,917 |

Product Characteristics

| | |
|---------------------|-----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,219 |
| Cumulative Months of Follow-Up | 25,294 |
| Number of Leads Active in Study | 5 |

Product Surveillance Registry Qualifying Complications


| | |
|---|----------|
| | 4 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 3 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 1 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|-----|
| Cardiac Perforation | 13 |
| Conductor Fracture | 10 |
| Extracardiac Stimulation | 2 |
| Failure To Capture | 103 |
| Failure To Sense | 16 |
| Impedance Abnormal | 8 |
| Insulation Breach | 1 |
| Lead Dislodgement | 49 |
| Oversensing | 2 |
| Unspecified | 20 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 28 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 203 |
| Other | 12 |

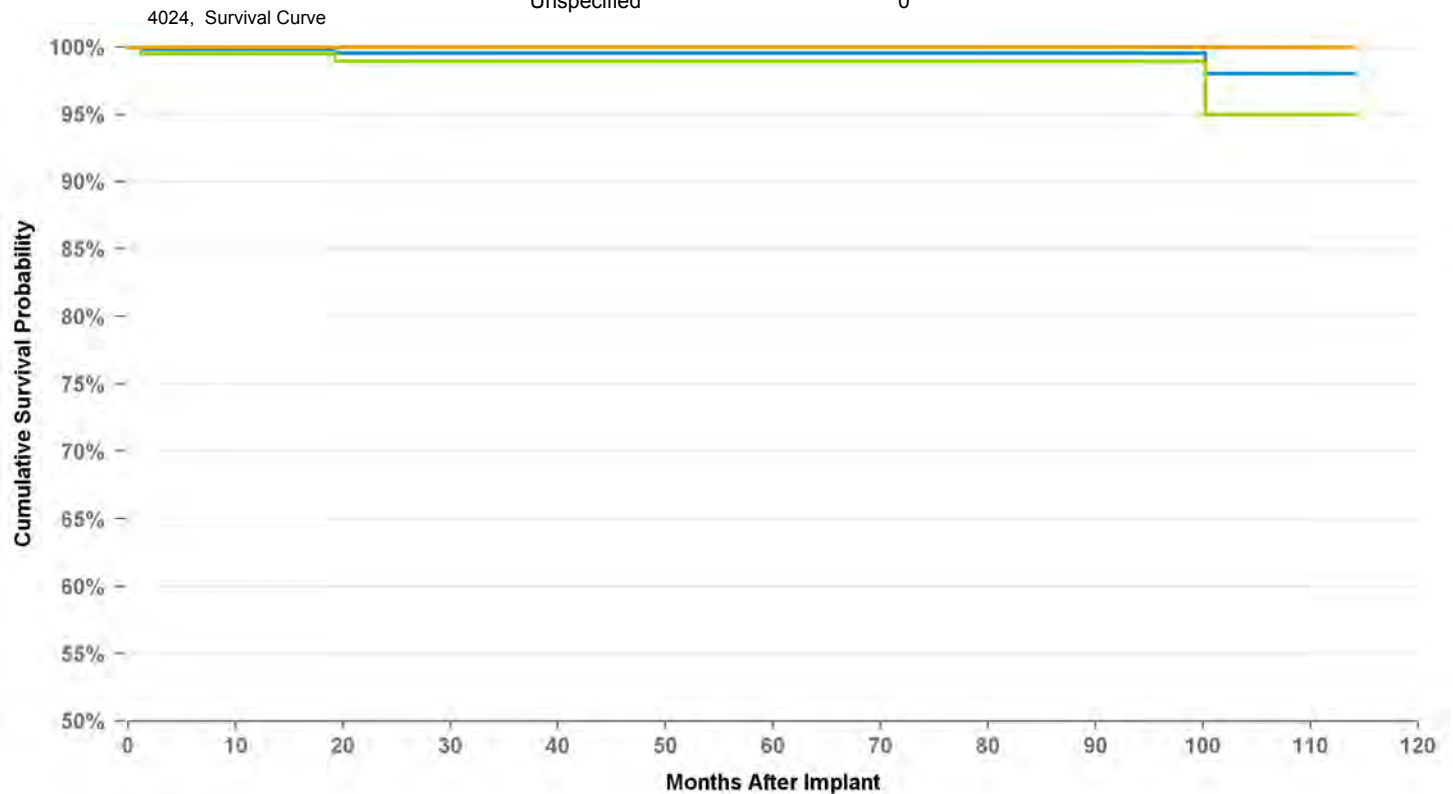

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 114 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.8% | 99.6% | 99.6% | 99.6% | 99.6% | 99.6% | 99.6% | 99.6% | 98.0% | 98.0% |
| # | 431 | 323 | 252 | 184 | 146 | 118 | 94 | 70 | 60 | 50 |

PACING LEAD

4068

ATRIAL PLACEMENT

Distribution Data

| | |
|--------------------------------|---------------------------|
| US Market Release | 3/29/1996 |
| CE Approval Date | |
| Registered US Implants | 124,260 |
| Estimated Active US | 27,694 |
| Product Characteristics | |
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|---------|
| Number of Leads Enrolled in Study | 2,429 |
| Cumulative Months of Follow-Up | 124,610 |
| Number of Leads Active in Study | 170 |

Product Surveillance Registry Qualifying Complications

| | |
|---|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 4 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 3 |
| Failure To Capture | 23 |
| Failure To Sense | 15 |
| Impedance Abnormal | 12 |
| Insulation Breach (ESC) | 2 |
| Insulation Breach (MIO) | 2 |
| Insulation Breach (not further defined) | 2 |
| Lead Dislodgement | 8 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 18 |
| Unspecified | 3 |


92

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 5 |
| Conductor Fracture | 3 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 23 |
| Failure To Sense | 5 |
| Impedance Abnormal | 2 |
| Insulation Breach | 1 |
| Lead Dislodgement | 31 |
| Oversensing | 0 |
| Unspecified | 4 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 53 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 207 |
| Other | 93 |

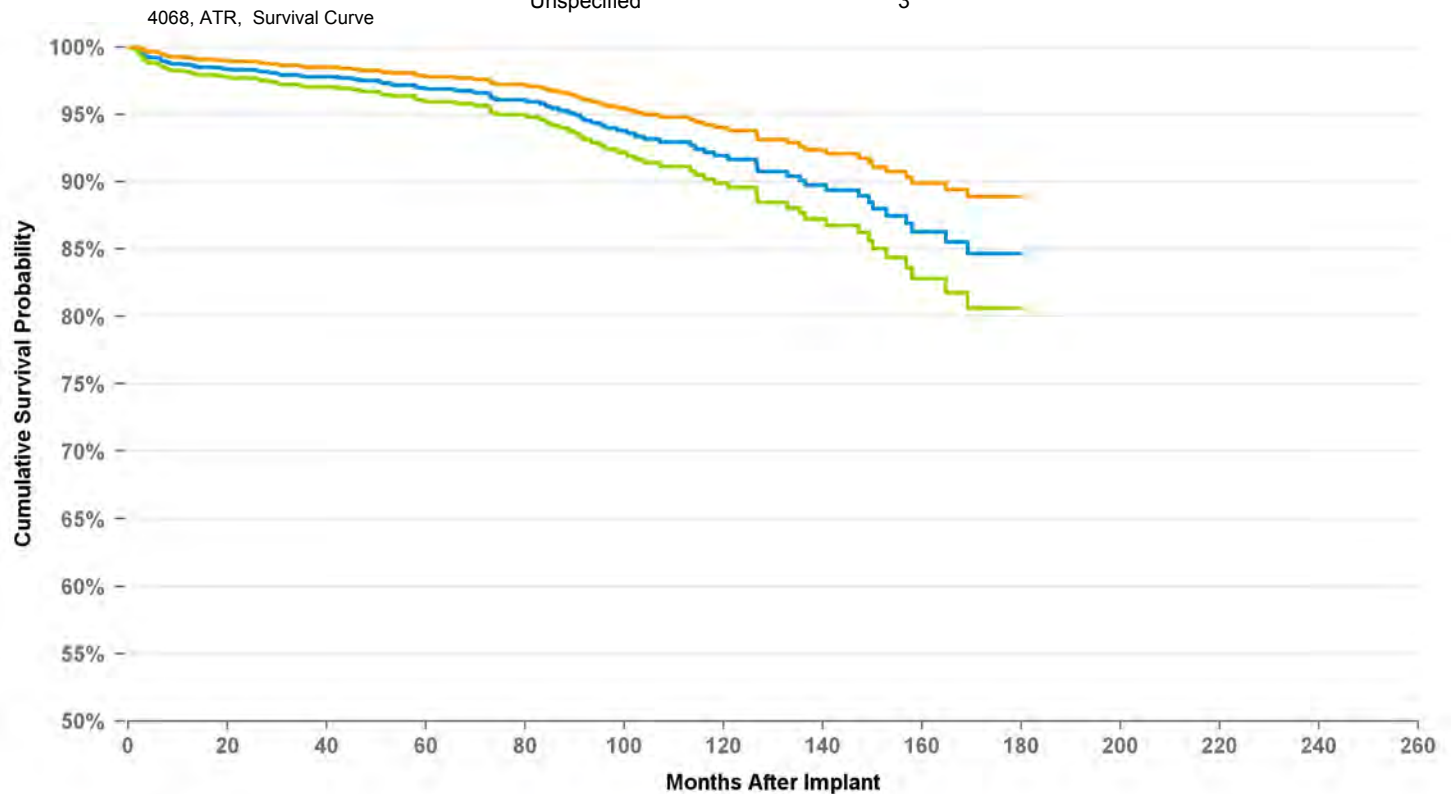

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | 14 | at 180 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 98.7% | 98.3% | 97.8% | 97.5% | 96.9% | 96.6% | 95.8% | 94.2% | 92.9% | 91.9% | 90.8% | 89.4% | 87.5% | 85.5% | 84.7% |
| # | 1,606 | 1,396 | 1,197 | 1,018 | 873 | 737 | 586 | 486 | 401 | 341 | 281 | 210 | 148 | 99 | 58 |

PACING LEAD

4068

VENTRICULAR PLACEMENT

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 3/29/1996 |
| CE Approval Date | |
| Registered US Implants | 124,260 |
| Estimated Active US | 27,694 |

Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,806 |
| Cumulative Months of Follow-Up | 91,664 |
| Number of Leads Active in Study | 78 |

Product Surveillance Registry Qualifying Complications

| | |
|---|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 3 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 2 |
| Failure To Capture | 24 |
| Failure To Sense | 4 |
| Impedance Abnormal | 21 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 1 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 2 |
| Oversensing | 10 |
| Unspecified | 2 |


69

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 5 |
| Conductor Fracture | 3 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 23 |
| Failure To Sense | 5 |
| Impedance Abnormal | 2 |
| Insulation Breach | 1 |
| Lead Dislodgement | 31 |
| Oversensing | 0 |
| Unspecified | 4 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 53 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 207 |
| Other | 93 |

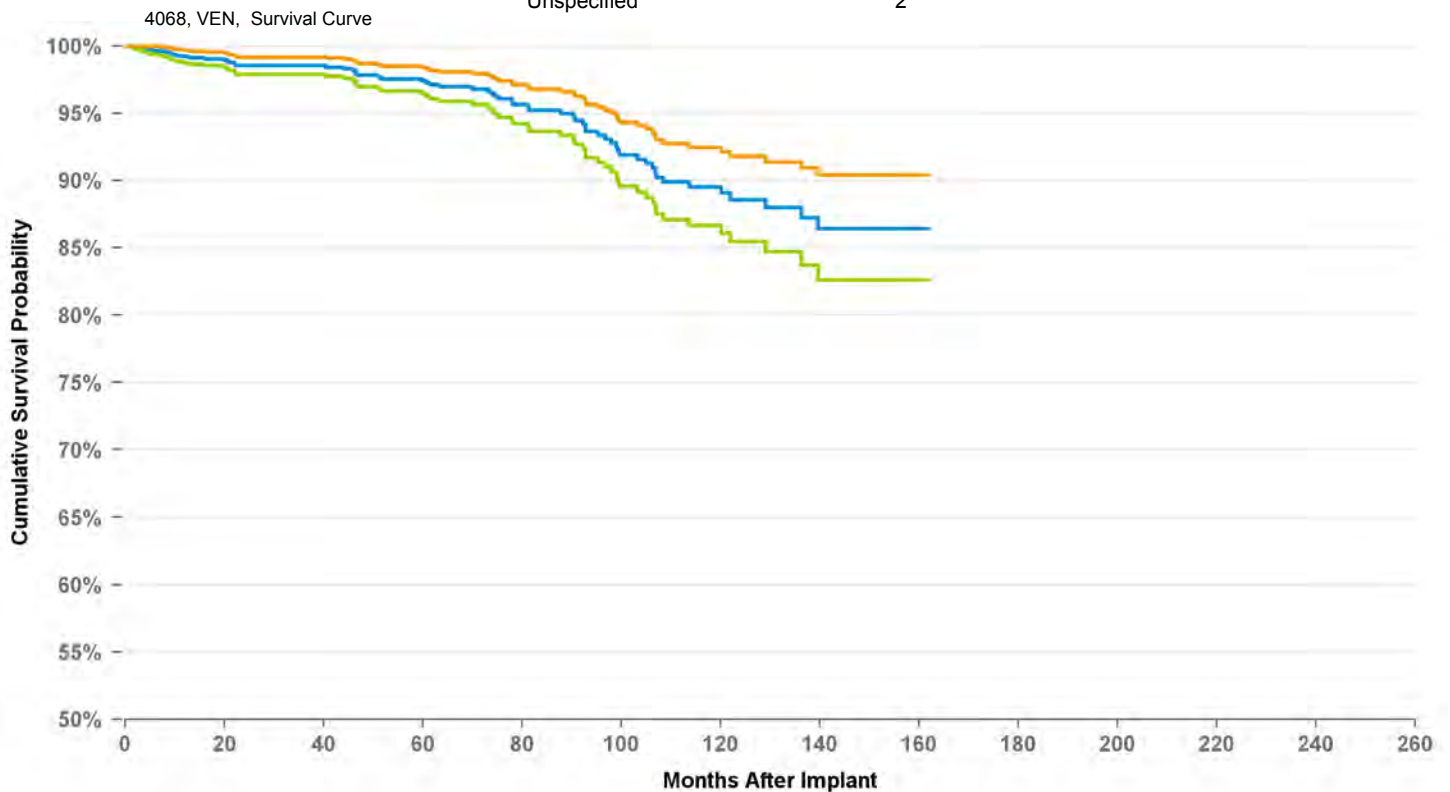

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | at 162 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.2% | 98.5% | 98.5% | 97.8% | 97.4% | 96.8% | 95.2% | 93.4% | 90.2% | 89.5% | 88.0% | 86.4% | 86.4% | 86.4% |
| # | 1,289 | 1,110 | 964 | 802 | 666 | 532 | 421 | 330 | 262 | 196 | 129 | 86 | 60 | 52 |

PACING LEAD

4074

ATRIAL PLACEMENT

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 6/23/2002 |
| CE Approval Date | 2/1/2002 |
| Registered US Implants | 100,394 |
| Estimated Active US | 61,976 |


Product Characteristics

| | |
|---------------------|-----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 214 |
| Cumulative Months of Follow-Up | 16,948 |
| Number of Leads Active in Study | 116 |

4074, ATR, Survival Curve

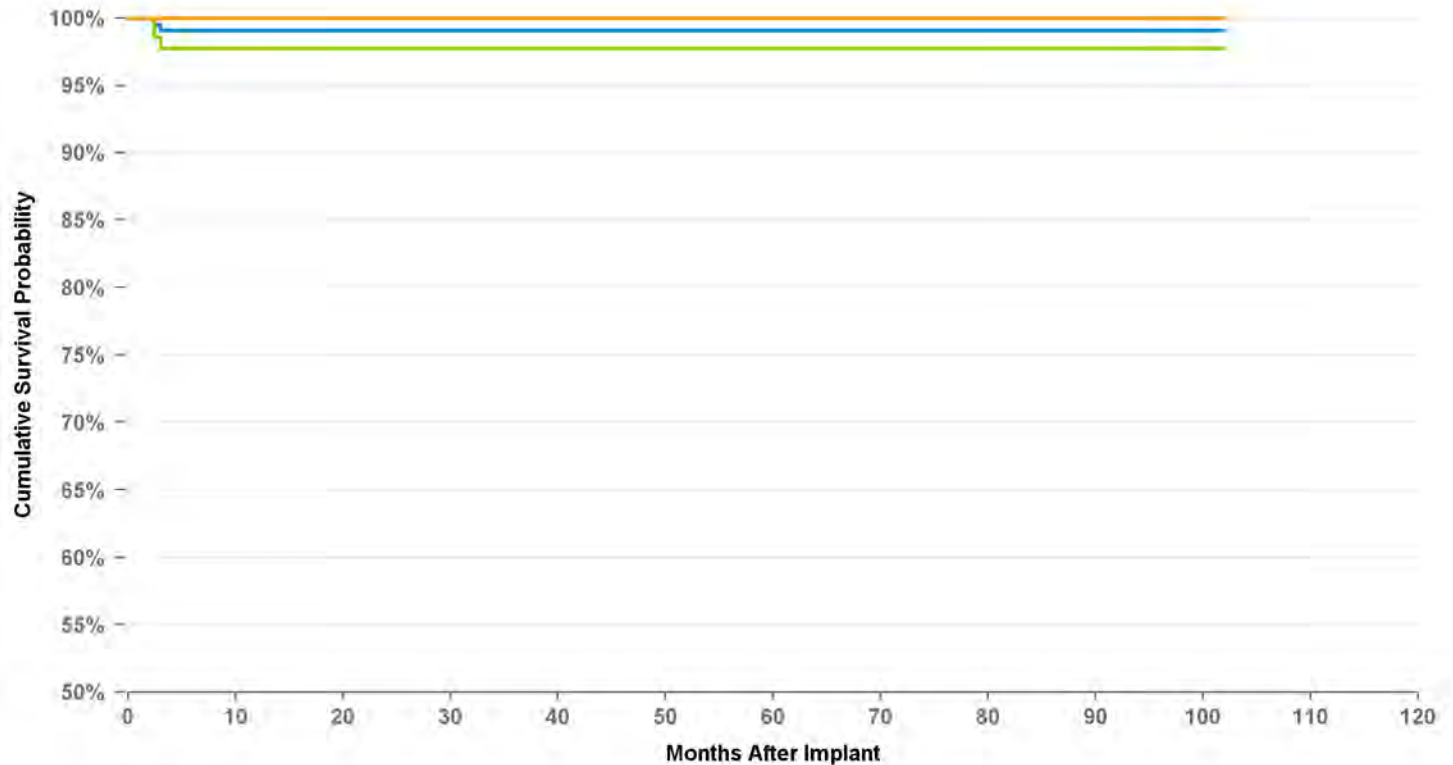

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 102 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.1% | 99.1% | 99.1% | 99.1% | 99.1% | 99.1% | 99.1% | 99.1% | 99.1% |
| # | 201 | 191 | 184 | 167 | 152 | 138 | 121 | 90 | 69 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 1 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

2

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 14 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 42 |
| Failure To Sense | 1 |
| Impedance Abnormal | 3 |
| Insulation Breach | 0 |
| Lead Dislodgement | 45 |
| Oversensing | 1 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 5 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 27 |
| Other | 0 |

PACING LEAD

4074

VENTRICULAR PLACEMENT

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 6/23/2002 |
| CE Approval Date | 2/1/2002 |
| Registered US Implants | 100,394 |
| Estimated Active US | 61,976 |

Product Characteristics

| | |
|---------------------|-----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,081 |
| Cumulative Months of Follow-Up | 42,369 |
| Number of Leads Active in Study | 578 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 2 |
| Failure To Sense | 0 |
| Impedance Abnormal | 2 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 2 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |


7

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 14 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 42 |
| Failure To Sense | 1 |
| Impedance Abnormal | 3 |
| Insulation Breach | 0 |
| Lead Dislodgement | 45 |
| Oversensing | 1 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 5 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 27 |
| Other | 0 |

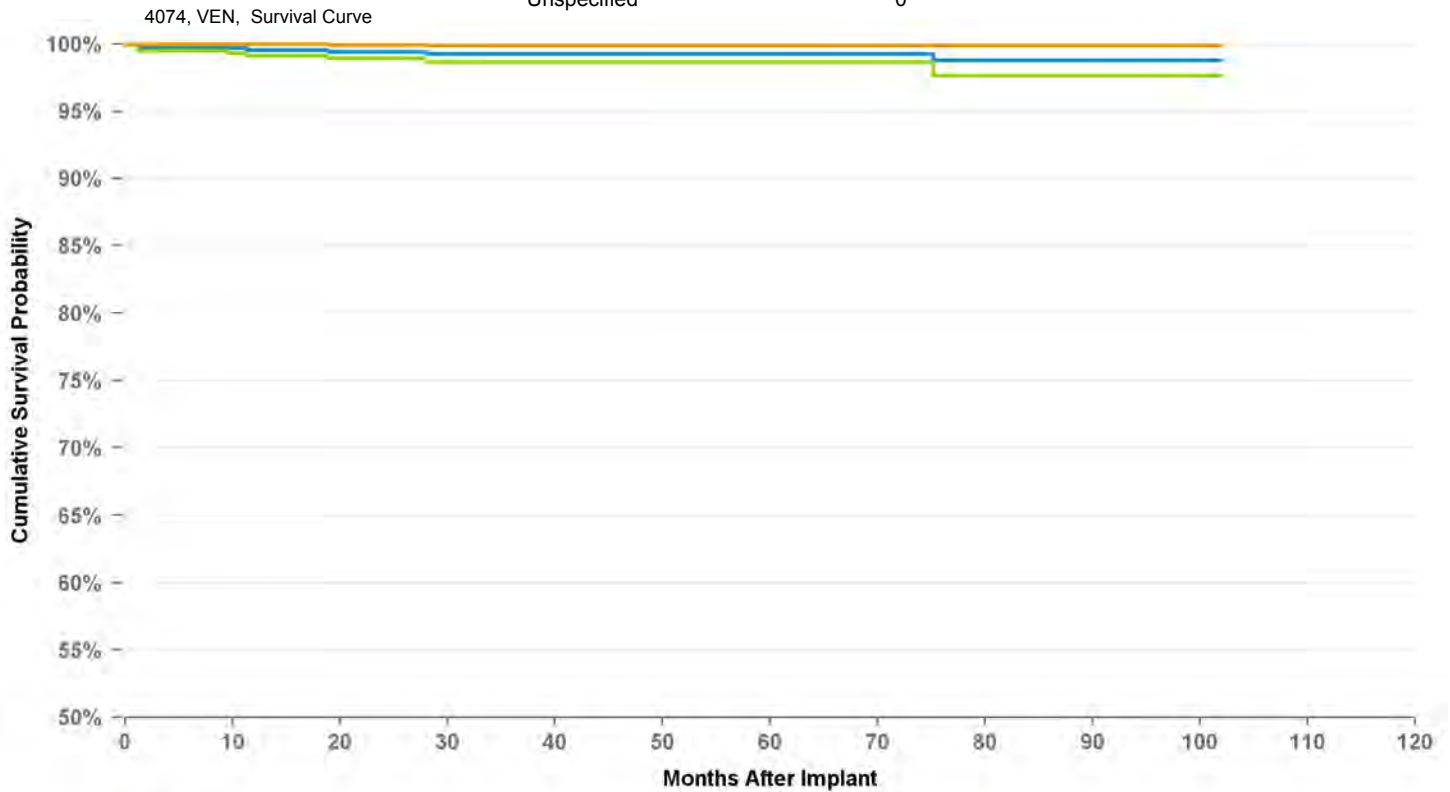

Graph Name

Cumulative Survival Probability Graph Lower 95 Pct Confidence Graph Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 102 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.6% | 99.4% | 99.3% | 99.3% | 99.3% | 99.3% | 98.8% | 98.8% | 98.8% |
| # | 851 | 630 | 423 | 315 | 262 | 215 | 156 | 93 | 68 |

PACING LEAD

4076

ATRIAL PLACEMENT

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 2/25/2004 |
| CE Approval Date | 6/14/2004 |
| Registered US Implants | 505,442 |
| Estimated Active US | 382,473 |


Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 2,502 |
| Cumulative Months of Follow-Up | 88,825 |
| Number of Leads Active in Study | 1,456 |

4076, ATR, Survival Curve

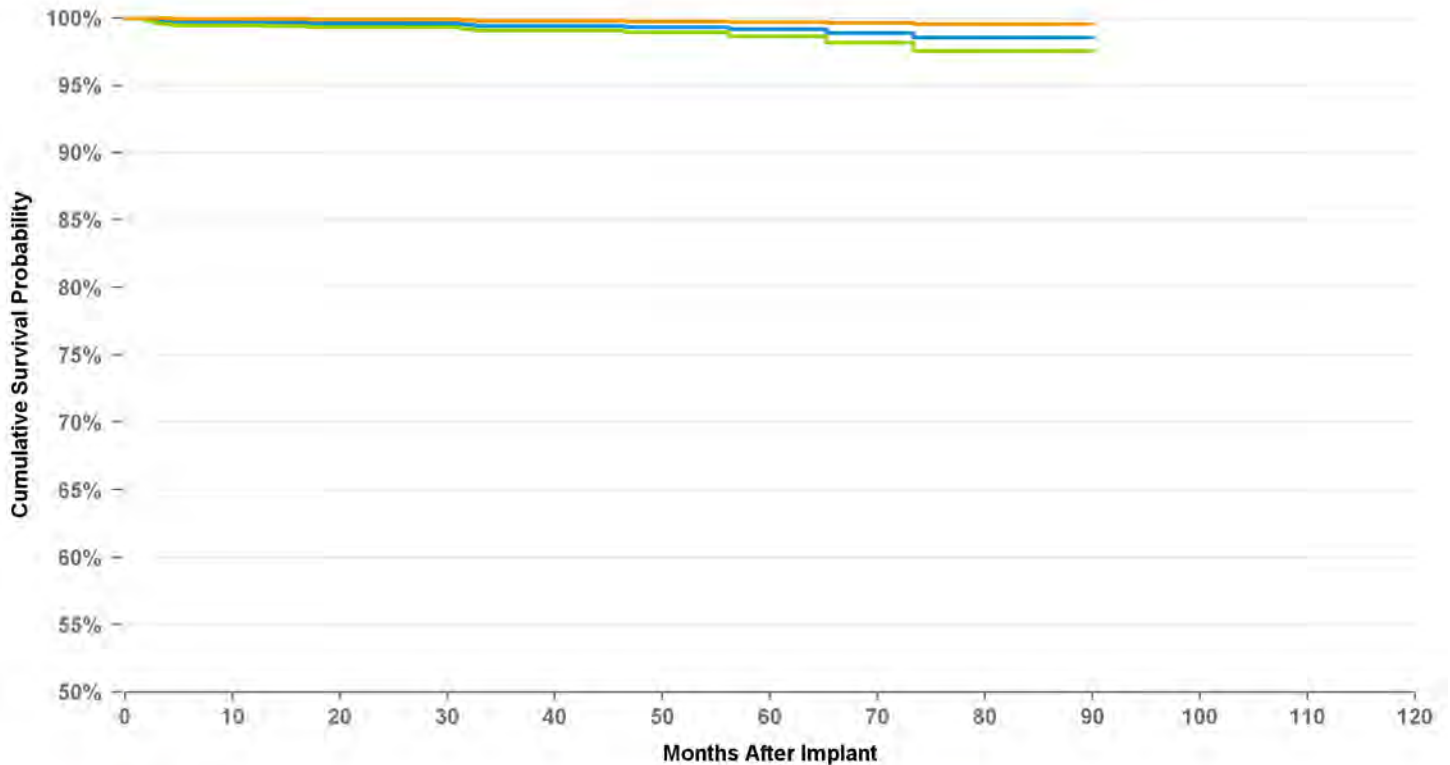

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 90 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|----------|
| % | 99.7% | 99.6% | 99.4% | 99.3% | 99.2% | 98.9% | 98.5% | 98.5% |
| # | 1,822 | 1,466 | 1,189 | 856 | 441 | 269 | 163 | 92 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 1 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 2 |
| Failure To Sense | 3 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 1 |
| Lead Dislodgement | 6 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 1 |
| Unspecified | 0 |

15

US Acute Lead Observations

| | |
|--------------------------|-----|
| Cardiac Perforation | 73 |
| Conductor Fracture | 4 |
| Extracardiac Stimulation | 11 |
| Failure To Capture | 92 |
| Failure To Sense | 25 |
| Impedance Abnormal | 12 |
| Insulation Breach | 1 |
| Lead Dislodgement | 215 |
| Oversensing | 12 |
| Unspecified | 12 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 57 |
| Crimp Weld Bond | 1 |
| Insulation Breach | 56 |
| Other | 20 |

PACING LEAD

4076

VENTRICULAR PLACEMENT

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 2/25/2004 |
| CE Approval Date | 6/14/2004 |
| Registered US Implants | 505,442 |
| Estimated Active US | 382,473 |

Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,401 |
| Cumulative Months of Follow-Up | 61,043 |
| Number of Leads Active in Study | 632 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 3 |
| Failure To Sense | 0 |
| Impedance Abnormal | 2 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |


7

US Acute Lead Observations

| | |
|--------------------------|-----|
| Cardiac Perforation | 73 |
| Conductor Fracture | 4 |
| Extracardiac Stimulation | 11 |
| Failure To Capture | 92 |
| Failure To Sense | 25 |
| Impedance Abnormal | 12 |
| Insulation Breach | 1 |
| Lead Dislodgement | 215 |
| Oversensing | 12 |
| Unspecified | 12 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 57 |
| Crimp Weld Bond | 1 |
| Insulation Breach | 56 |
| Other | 20 |

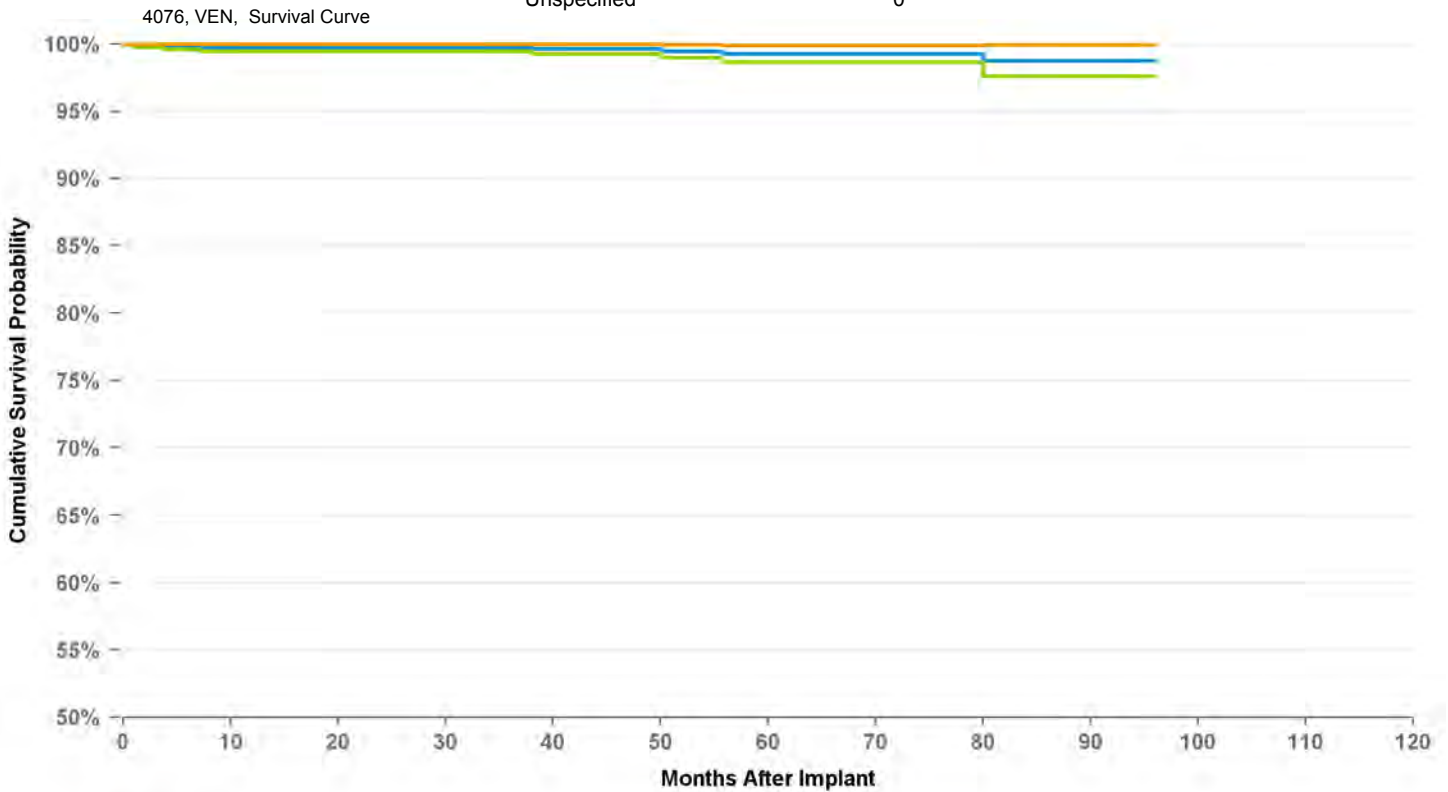

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 96 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|----------|
| % | 99.8% | 99.8% | 99.8% | 99.6% | 99.3% | 99.3% | 98.8% | 98.8% |
| # | 1,116 | 955 | 824 | 650 | 379 | 253 | 144 | 61 |

PACING LEAD

4092

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 9/17/1998 |
| CE Approval Date | 4/15/1998 |
| Registered US Implants | 183,321 |
| Estimated Active US | 79,201 |

Product Characteristics

| | |
|---------------------|-----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,178 |
| Cumulative Months of Follow-Up | 66,279 |
| Number of Leads Active in Study | 39 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 3 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 9 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 4 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |


18

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 3 |
| Conductor Fracture | 4 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 33 |
| Failure To Sense | 0 |
| Impedance Abnormal | 2 |
| Insulation Breach | 1 |
| Lead Dislodgement | 27 |
| Oversensing | 1 |
| Unspecified | 2 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 14 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 58 |
| Other | 2 |

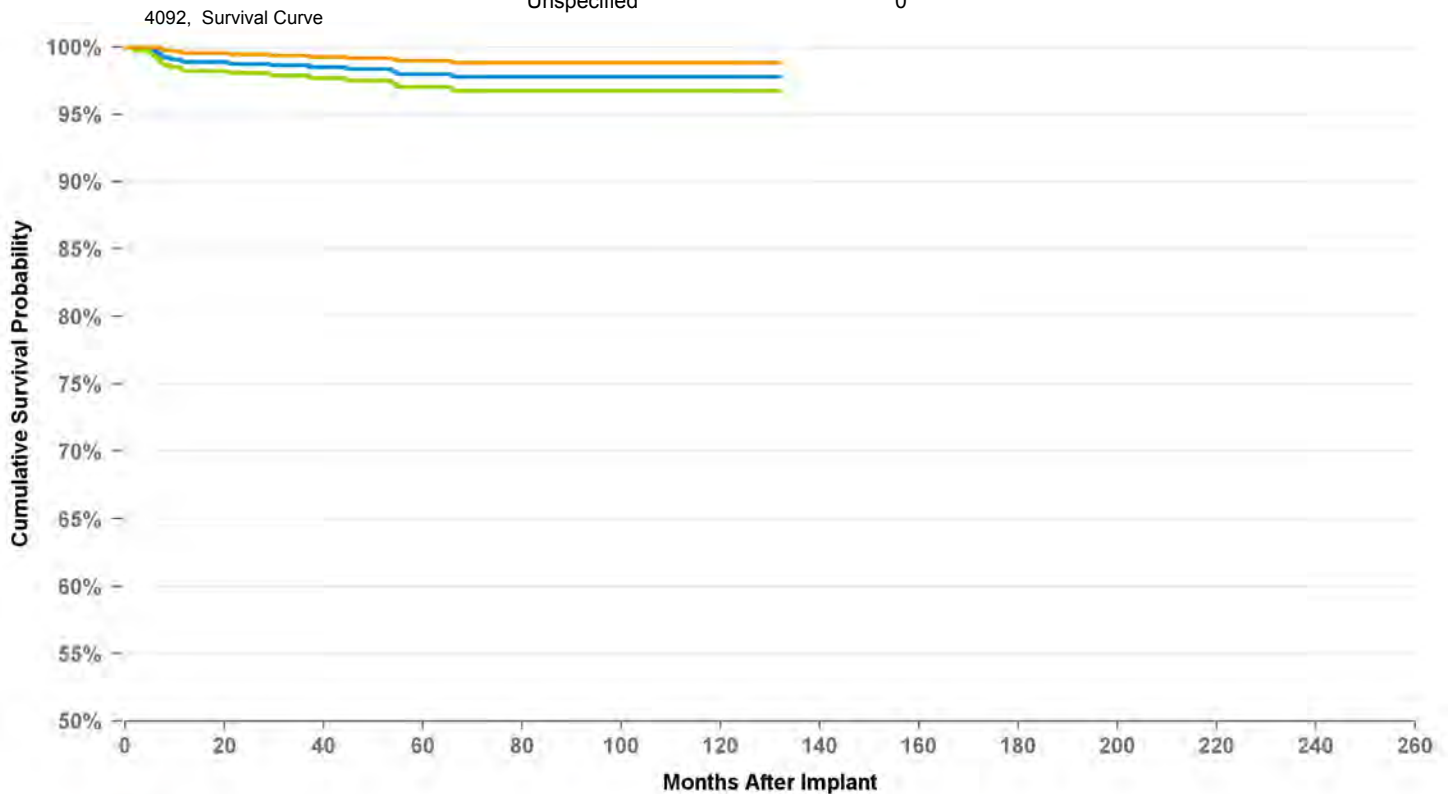

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 132 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 98.9% | 98.8% | 98.6% | 98.3% | 98.0% | 97.8% | 97.8% | 97.8% | 97.8% | 97.8% | 97.8% |
| # | 918 | 812 | 724 | 621 | 507 | 394 | 322 | 259 | 210 | 129 | 61 |

PACING LEAD

4524

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 10/1/1991 |
| CE Approval Date | |
| Registered US Implants | 100,268 |
| Estimated Active US | 21,638 |

Product Characteristics

| | |
|---------------------|----------------|
| Fixation Type | J-Shape, tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 918 |
| Cumulative Months of Follow-Up | 23,323 |
| Number of Leads Active in Study | 26 |

Product Surveillance Registry Qualifying Complications


| | |
|---|----------|
| | 6 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 3 |
| Failure To Sense | 2 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 2 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 15 |
| Failure To Sense | 4 |
| Impedance Abnormal | 1 |
| Insulation Breach | 2 |
| Lead Dislodgement | 23 |
| Oversensing | 0 |
| Unspecified | 12 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 1 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 79 |
| Other | 3 |

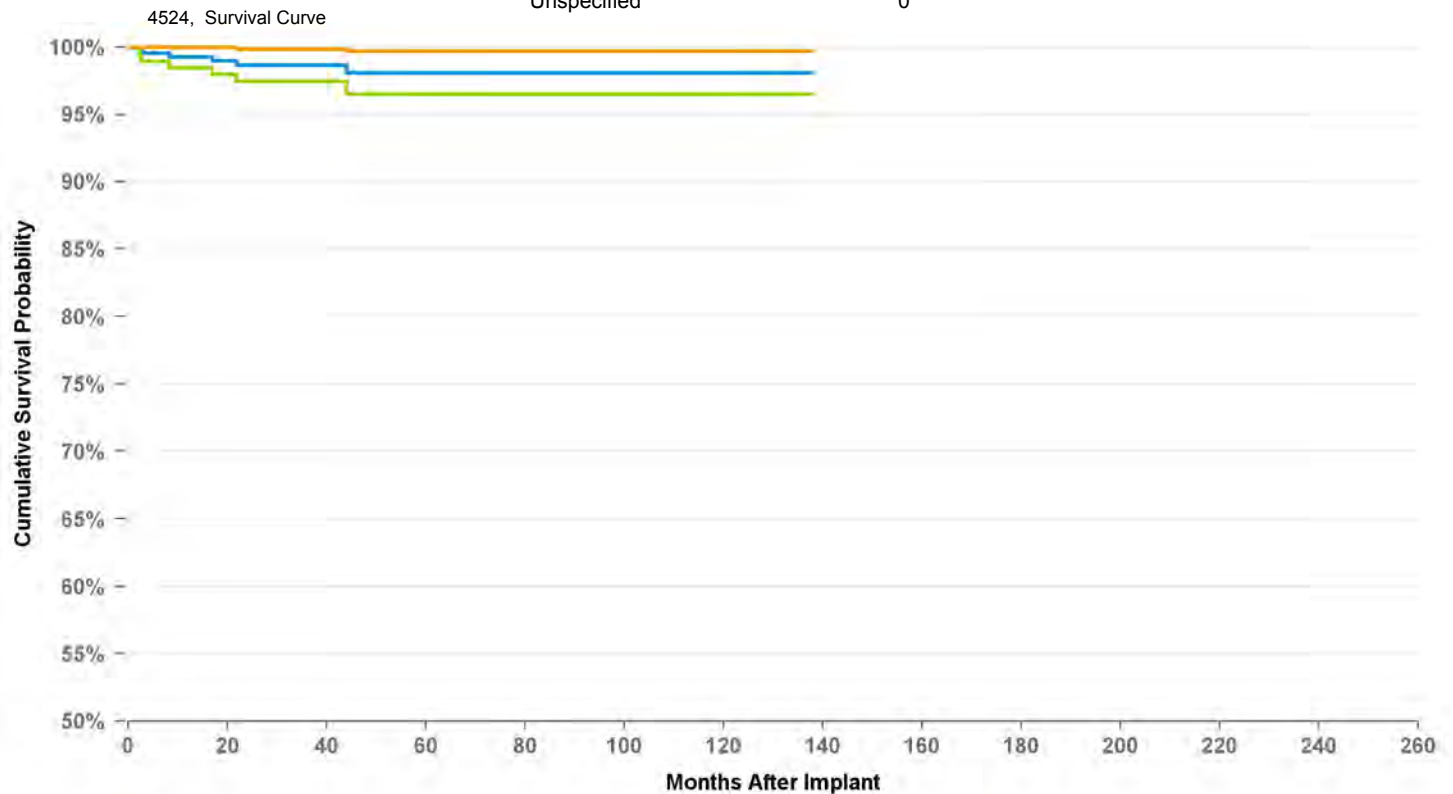

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 138 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.3% | 98.6% | 98.6% | 98.1% | 98.1% | 98.1% | 98.1% | 98.1% | 98.1% | 98.1% | 98.1% | 98.1% |
| # | 364 | 275 | 217 | 163 | 131 | 106 | 86 | 75 | 66 | 55 | 53 | 52 |

PACING LEAD

4558M

Distribution Data

| | |
|------------------------|------------|
| US Market Release | 11/14/1994 |
| CE Approval Date | |
| Registered US Implants | 19,566 |
| Estimated Active US | 3,542 |

Product Characteristics

| | |
|---------------------|-----------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | None |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium - J |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 540 |
| Cumulative Months of Follow-Up | 18,671 |
| Number of Leads Active in Study | 3 |

Product Surveillance Registry Qualifying Complications

| | |
|---|----|
| | 12 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 1 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 3 |
| Failure To Sense | 2 |
| Impedance Abnormal | 2 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 2 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 2 |
| Unspecified | 0 |


US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 2 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 2 |
| Failure To Sense | 1 |
| Impedance Abnormal | 1 |
| Insulation Breach | 0 |
| Lead Dislodgement | 2 |
| Oversensing | 0 |
| Unspecified | 1 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 1 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 24 |
| Other | 20 |

4558M, Survival Curve

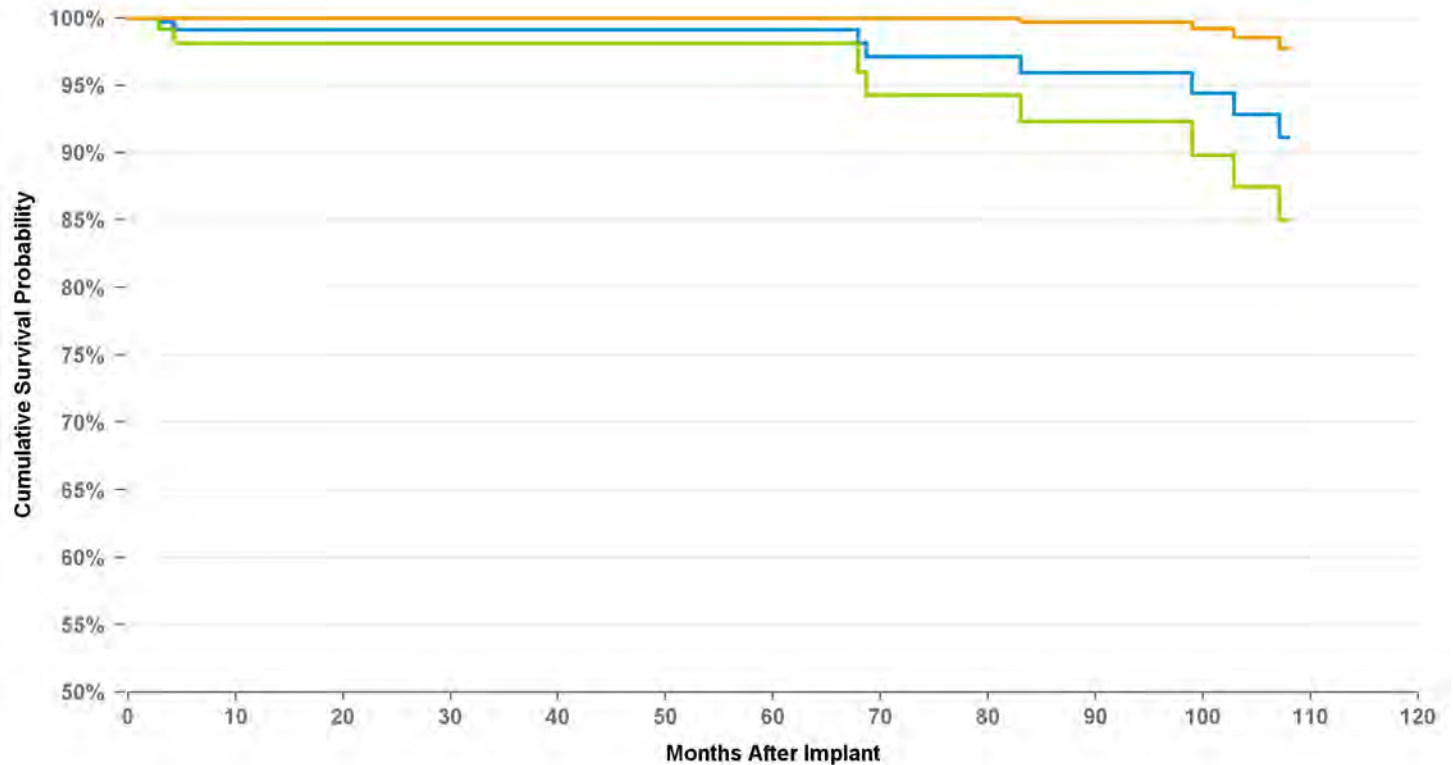

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | at 108 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.1% | 99.1% | 99.1% | 99.1% | 99.1% | 97.1% | 95.9% | 95.9% | 91.1% |
| # | 278 | 225 | 180 | 140 | 115 | 88 | 80 | 64 | 53 |

PACING LEAD

4568

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 1/2/1997 |
| CE Approval Date | |
| Registered US Implants | 69,208 |
| Estimated Active US | 19,145 |

Product Characteristics

| | |
|---------------------|-------------------|
| Fixation Type | J-shape, screw in |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 669 |
| Cumulative Months of Follow-Up | 31,663 |
| Number of Leads Active in Study | 15 |

Product Surveillance Registry Qualifying Complications

37


| | |
|---|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 19 |
| Failure To Sense | 4 |
| Impedance Abnormal | 3 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 9 |
| Medical Judgment | 1 |
| Other Complication | 1 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 3 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 6 |
| Failure To Sense | 1 |
| Impedance Abnormal | 2 |
| Insulation Breach | 0 |
| Lead Dislodgement | 4 |
| Oversensing | 1 |
| Unspecified | 1 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 7 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 101 |
| Other | 52 |

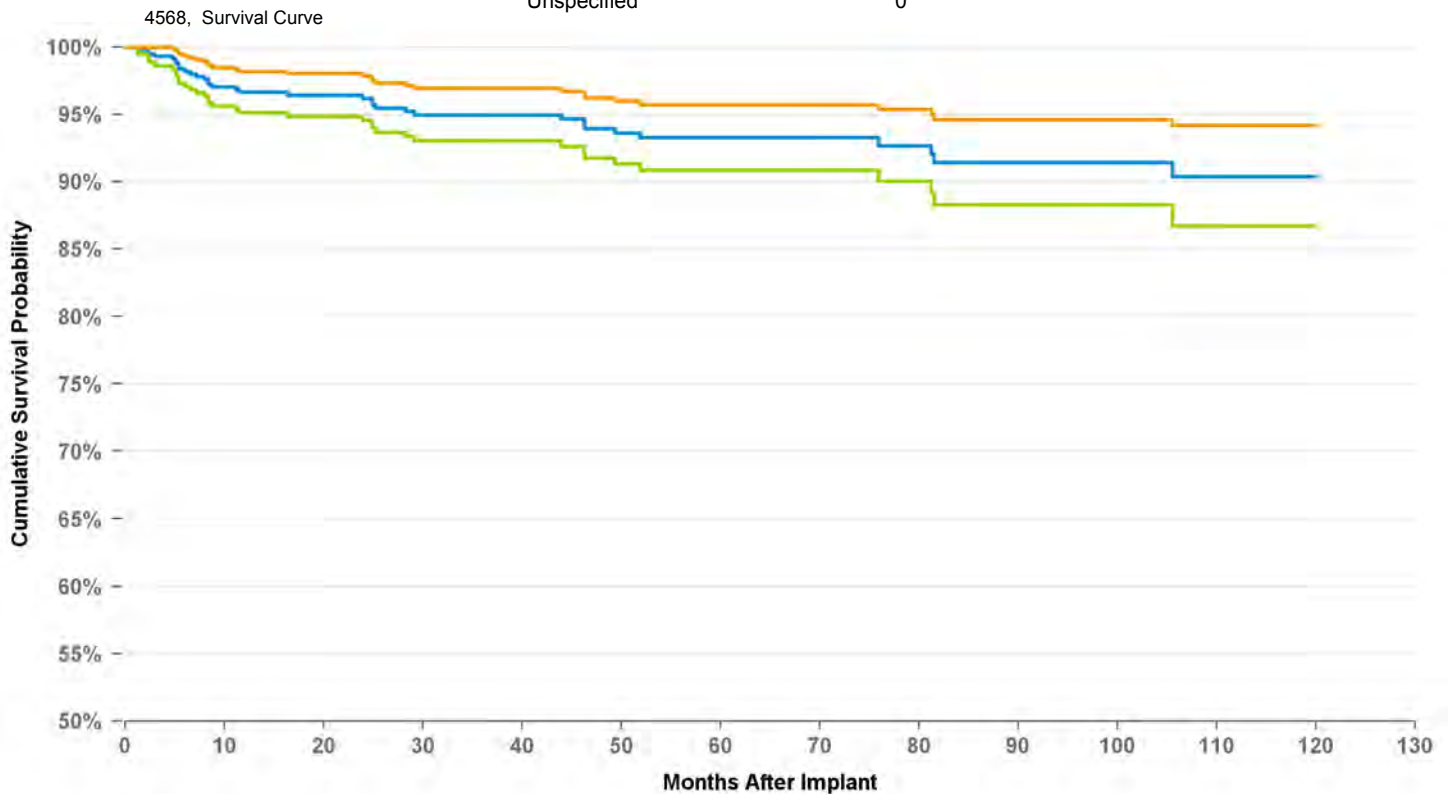

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 120 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 96.6% | 96.2% | 95.0% | 94.0% | 93.3% | 93.3% | 91.4% | 91.4% | 90.4% | 90.4% |
| # | 487 | 415 | 326 | 276 | 226 | 171 | 137 | 105 | 83 | 62 |

PACING LEAD

4574

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 6/23/2002 |
| CE Approval Date | 2/1/2002 |
| Registered US Implants | 68,263 |
| Estimated Active US | 45,020 |

Product Characteristics

| | |
|---------------------|----------------|
| Fixation Type | J-shape, tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 728 |
| Cumulative Months of Follow-Up | 13,890 |
| Number of Leads Active in Study | 515 |

Product Surveillance Registry Qualifying Complications


| | |
|---|----------|
| | 4 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 3 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 22 |
| Failure To Sense | 8 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 53 |
| Oversensing | 1 |
| Unspecified | 4 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 10 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 6 |
| Other | 0 |

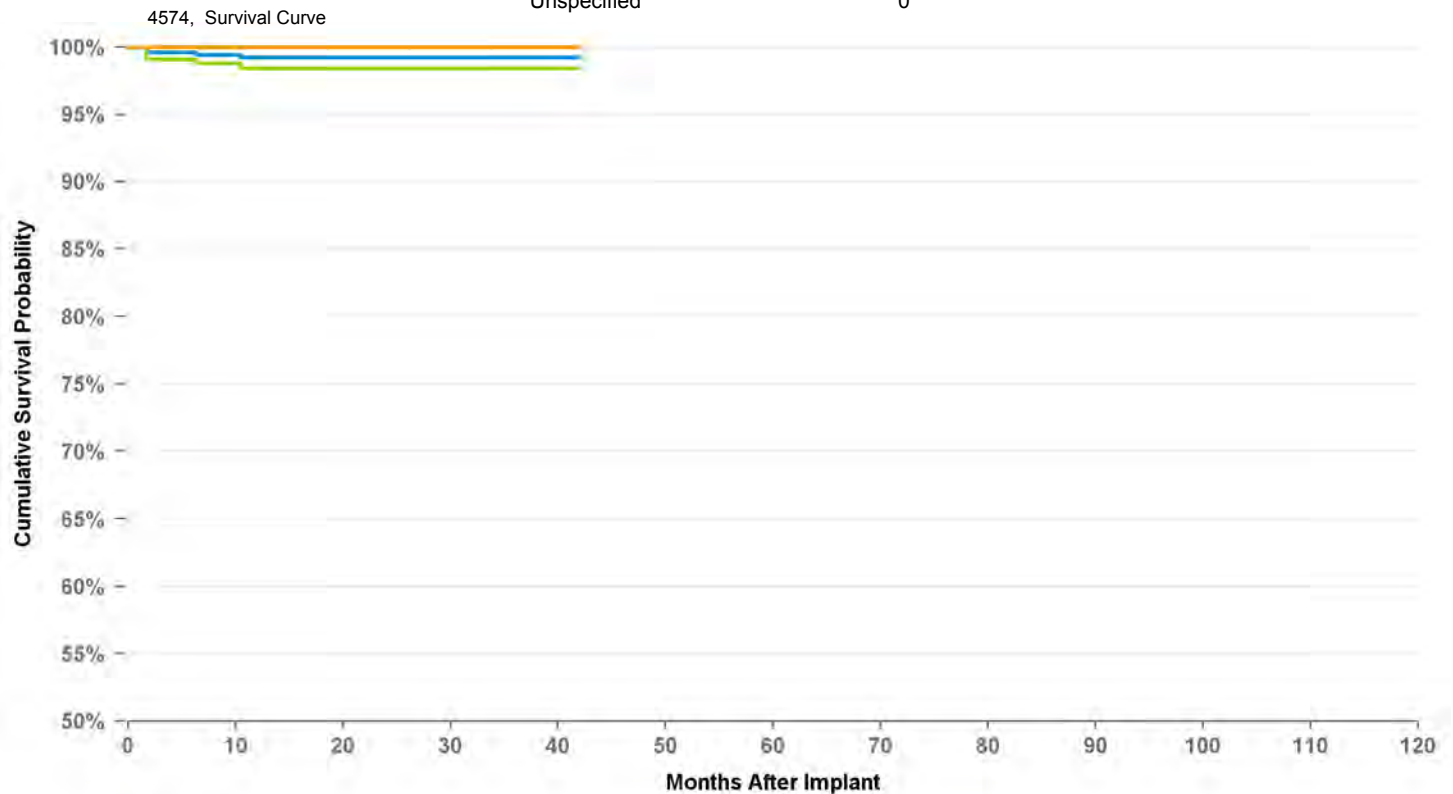

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | at 42 mo |
|-------|-------|-------|-------|----------|
| % | 99.2% | 99.2% | 99.2% | 99.2% |
| # | 446 | 244 | 94 | 58 |

PACING LEAD

4592

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 10/5/1998 |
| CE Approval Date | 4/15/1998 |
| Registered US Implants | 88,084 |
| Estimated Active US | 39,708 |

Product Characteristics

| | |
|---------------------|----------------|
| Fixation Type | J-shape, tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 324 |
| Cumulative Months of Follow-Up | 15,835 |
| Number of Leads Active in Study | 56 |

Product Surveillance Registry Qualifying Complications


| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 4 |
| Failure To Sense | 1 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 2 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 8 |
| Failure To Sense | 2 |
| Impedance Abnormal | 0 |
| Insulation Breach | 1 |
| Lead Dislodgement | 31 |
| Oversensing | 2 |
| Unspecified | 2 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 7 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 22 |
| Other | 1 |

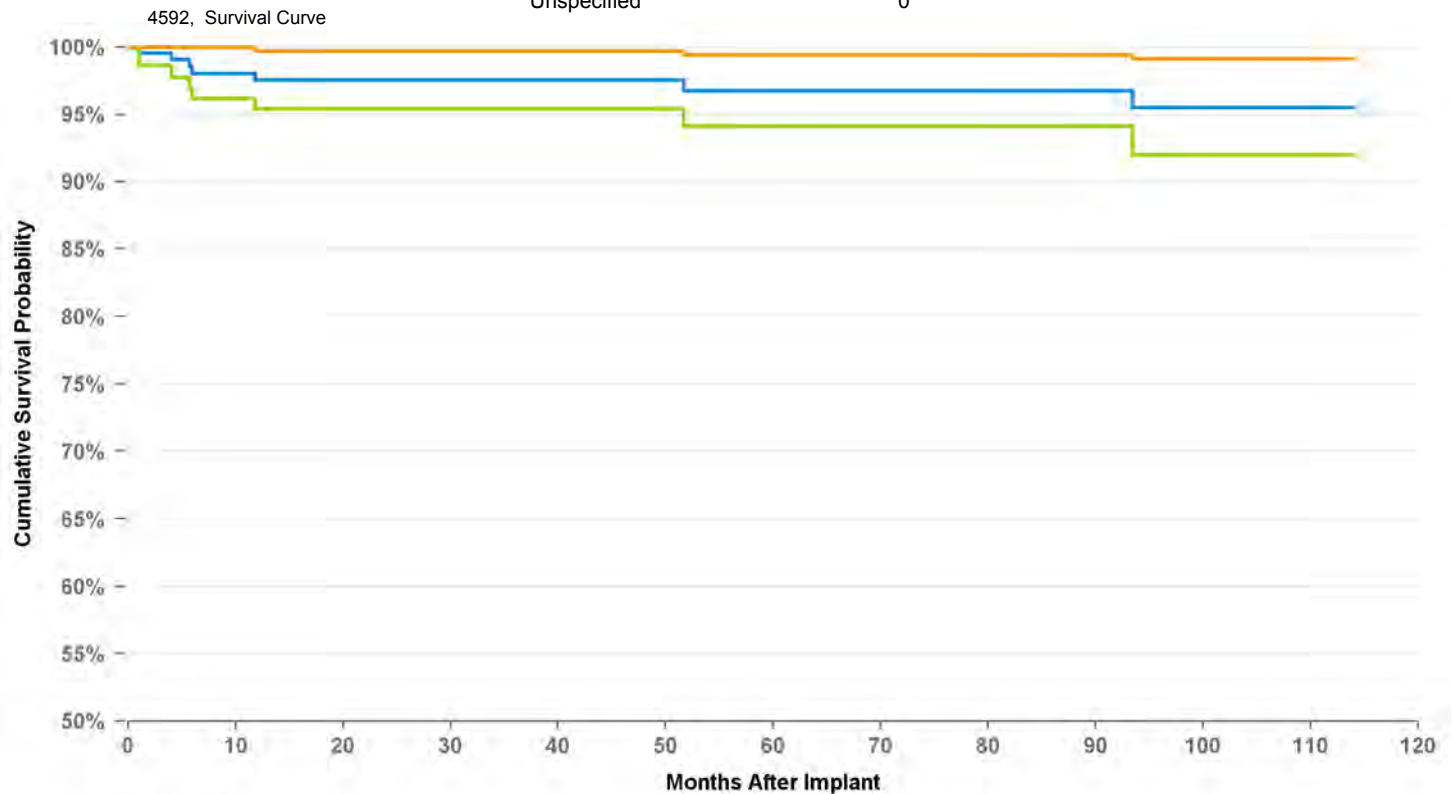

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | at 114 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 97.5% | 97.5% | 97.5% | 97.5% | 96.7% | 96.7% | 96.7% | 95.5% | 95.5% | 95.5% |
| # | 199 | 171 | 151 | 138 | 111 | 100 | 81 | 71 | 61 | 51 |

PACING LEAD

5033

Distribution Data

| | |
|--------------------------------|-----------------|
| US Market Release | 2/9/1996 |
| CE Approval Date | |
| Registered US Implants | 2,340 |
| Estimated Active US | 450 |
| Product Characteristics | |
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Unipolar |

Product Surveillance Registry Qualifying Complications

| | |
|---|-----------|
| | 32 |
| Cardiac Perforation | 1 |
| Conductor Fracture | 8 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 16 |
| Failure To Sense | 0 |
| Impedance Abnormal | 4 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 1 |
| Lead Dislodgement | 2 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations


| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 0 |
| Oversensing | 0 |
| Unspecified | 1 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 1 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 0 |
| Other | 3 |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,901 |
| Cumulative Months of Follow-Up | 77,308 |
| Number of Leads Active in Study | 30 |

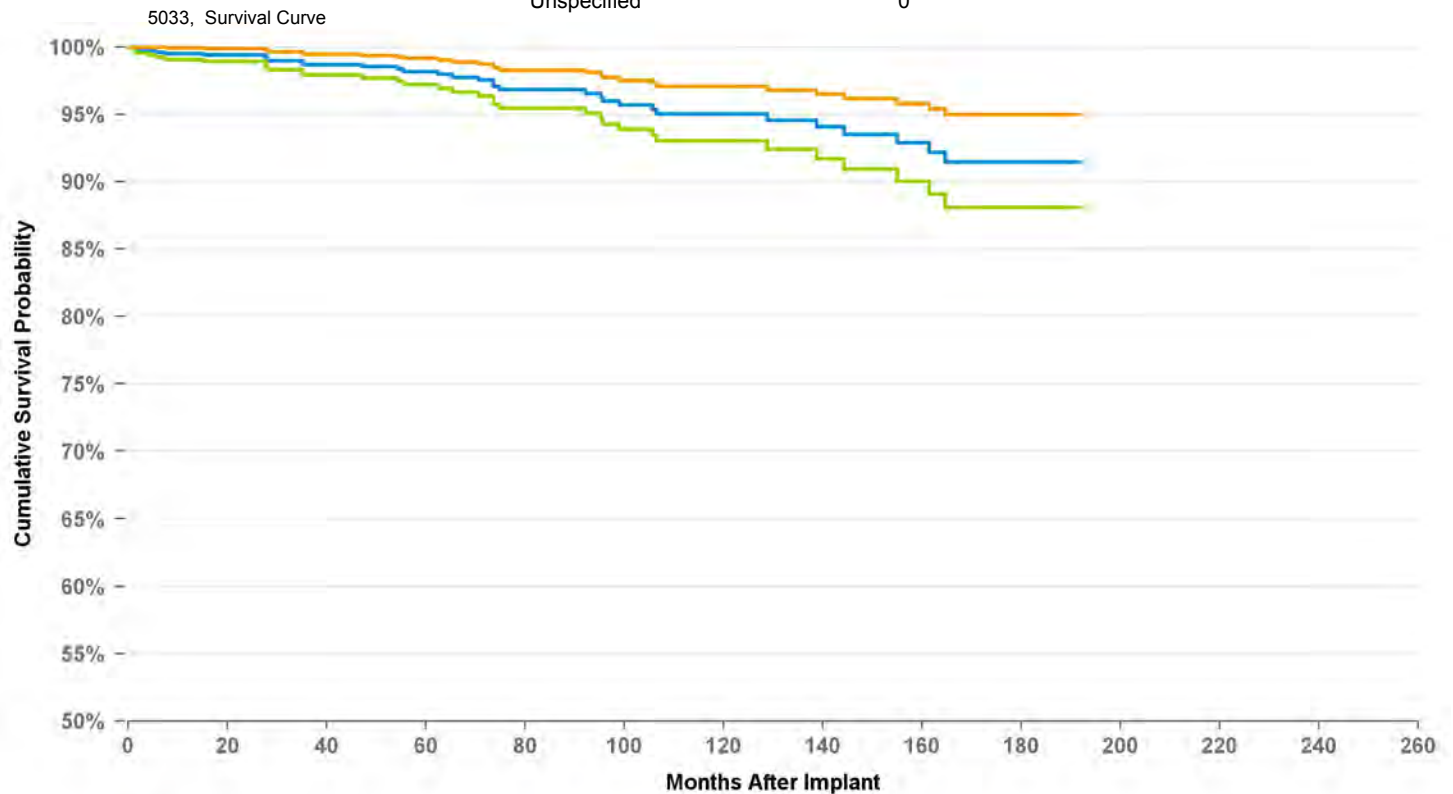

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | 14 | 15 | at 192 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.5% | 99.4% | 98.7% | 98.5% | 98.2% | 97.5% | 96.9% | 96.0% | 95.0% | 95.0% | 94.6% | 94.1% | 92.9% | 91.5% | 91.5% | 91.5% |
| # | 902 | 761 | 672 | 584 | 510 | 436 | 379 | 326 | 276 | 236 | 197 | 169 | 146 | 119 | 101 | 63 |

PACING LEAD

5034

ATRIAL PLACEMENT

Distribution Data

| | |
|--------------------------------|-----------------|
| US Market Release | 2/9/1996 |
| CE Approval Date | |
| Registered US Implants | 55,426 |
| Estimated Active US | 11,492 |
| Product Characteristics | |
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 2 |
| Failure To Sense | 1 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 1 |
| Oversensing | 0 |
| Unspecified | 0 |

6

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 2 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 28 |
| Failure To Sense | 3 |
| Impedance Abnormal | 0 |
| Insulation Breach | 3 |
| Lead Dislodgement | 14 |
| Oversensing | 0 |
| Unspecified | 12 |


Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 386 |
| Cumulative Months of Follow-Up | 46,774 |
| Number of Leads Active in Study | 83 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 16 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 15 |
| Other | 7 |

5034, ATR, Survival Curve

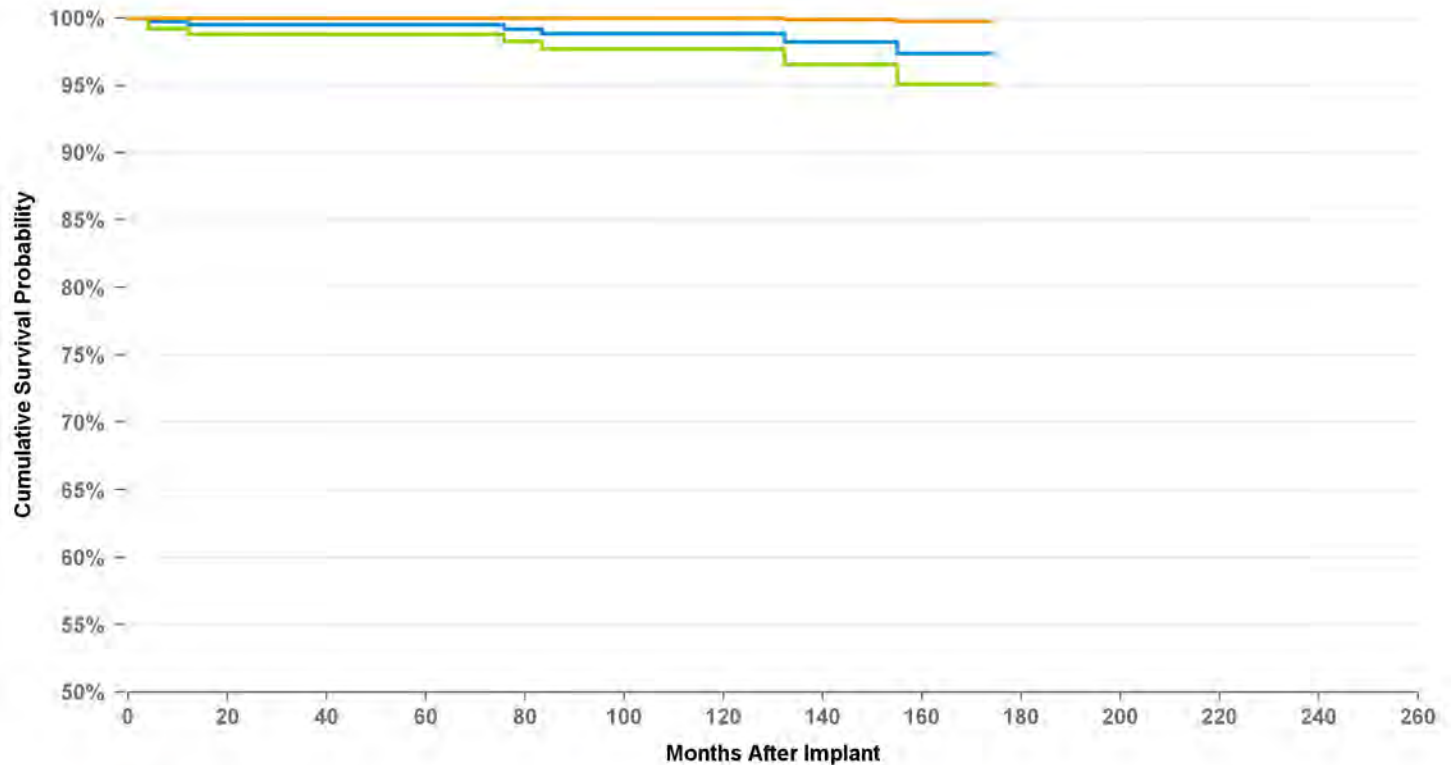

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | 14 | at 174 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.5% | 99.5% | 99.5% | 99.5% | 99.5% | 99.5% | 98.8% | 98.8% | 98.8% | 98.8% | 98.8% | 98.2% | 97.4% | 97.4% | 97.4% |
| # | 383 | 382 | 379 | 376 | 358 | 334 | 297 | 253 | 212 | 187 | 156 | 136 | 114 | 76 | 57 |

PACING LEAD

5034

VENTRICULAR PLACEMENT

Distribution Data

| | |
|--------------------------------|-----------------|
| US Market Release | 2/9/1996 |
| CE Approval Date | |
| Registered US Implants | 55,426 |
| Estimated Active US | 11,492 |
| Product Characteristics | |
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,213 |
| Cumulative Months of Follow-Up | 28,115 |
| Number of Leads Active in Study | 8 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 7 |
| Failure To Sense | 2 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |


11

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 2 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 28 |
| Failure To Sense | 3 |
| Impedance Abnormal | 0 |
| Insulation Breach | 3 |
| Lead Dislodgement | 14 |
| Oversensing | 0 |
| Unspecified | 12 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 16 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 15 |
| Other | 7 |

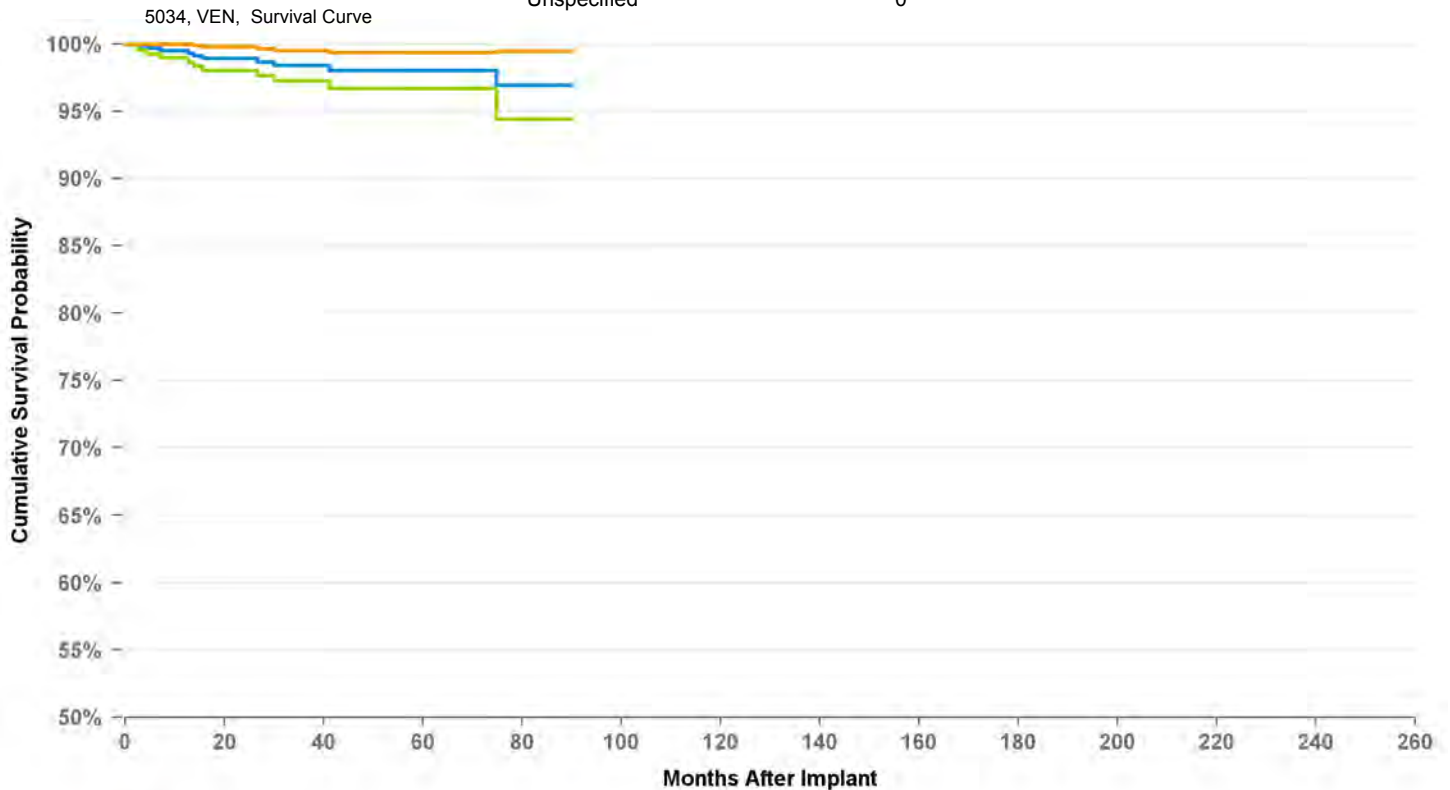

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | at 90 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|----------|
| % | 99.5% | 98.9% | 98.4% | 98.0% | 98.0% | 98.0% | 96.9% | 96.9% |
| # | 517 | 415 | 307 | 221 | 155 | 96 | 61 | 57 |

PACING LEAD

5054

ATRIAL PLACEMENT

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 6/3/1998 |
| CE Approval Date | 6/5/1997 |
| Registered US Implants | 98,325 |
| Estimated Active US | 40,420 |


Product Characteristics

| | |
|---------------------|-----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 424 |
| Cumulative Months of Follow-Up | 35,785 |
| Number of Leads Active in Study | 94 |

5054, ATR, Survival Curve

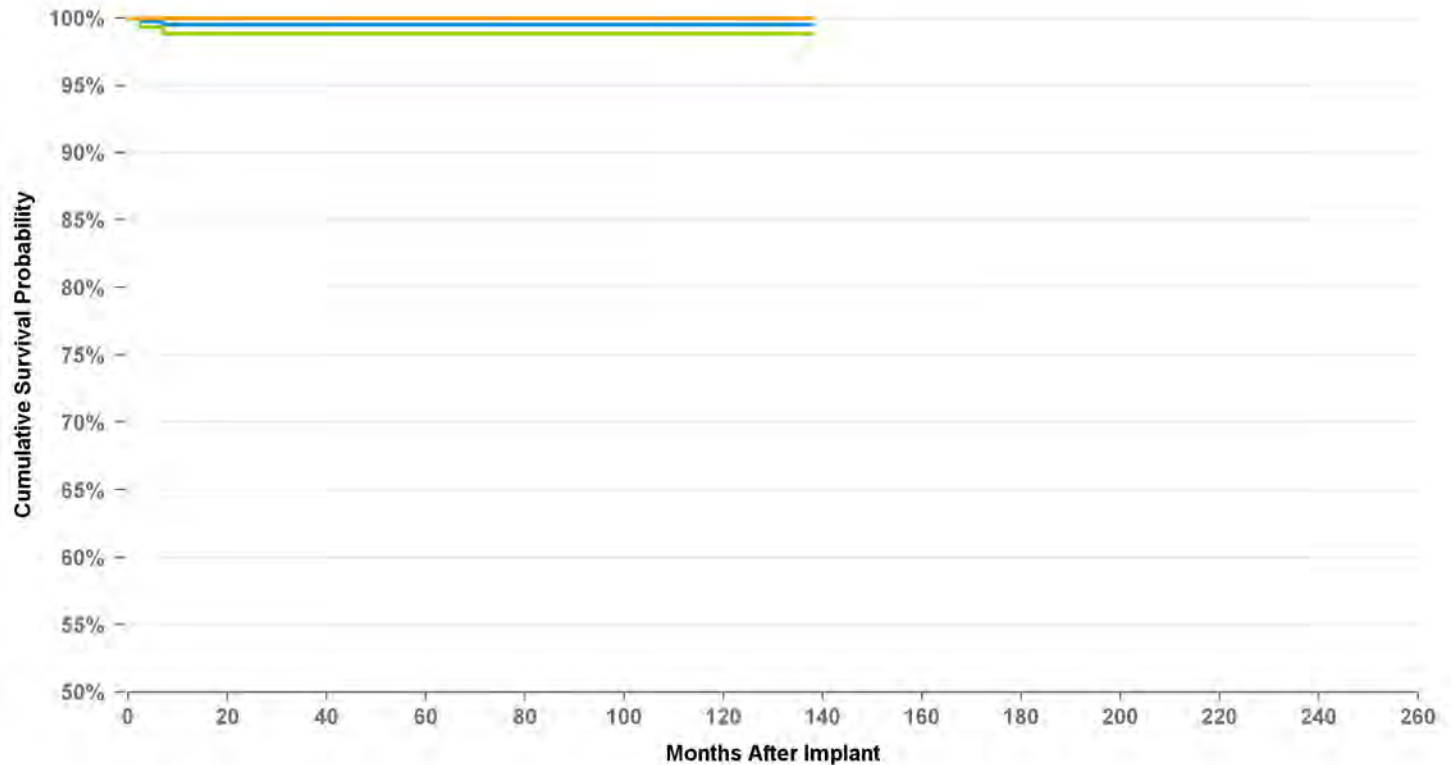

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 138 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.5% | 99.5% | 99.5% | 99.5% | 99.5% | 99.5% | 99.5% | 99.5% | 99.5% | 99.5% | 99.5% | 99.5% |
| # | 410 | 390 | 357 | 321 | 288 | 251 | 218 | 184 | 148 | 100 | 70 | 50 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

2

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 2 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 23 |
| Failure To Sense | 0 |
| Impedance Abnormal | 2 |
| Insulation Breach | 1 |
| Lead Dislodgement | 27 |
| Oversensing | 0 |
| Unspecified | 9 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 12 |
| Crimp Weld Bond | 1 |
| Insulation Breach | 31 |
| Other | 3 |

PACING LEAD

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 6/3/1998 |
| CE Approval Date | 6/5/1997 |
| Registered US Implants | 98,325 |
| Estimated Active US | 40,420 |

Product Characteristics

| | |
|---------------------|-----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 982 |
| Cumulative Months of Follow-Up | 31,734 |
| Number of Leads Active in Study | 57 |

5054

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 6 |
| Failure To Sense | 1 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |


VENTRICULAR PLACEMENT

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 2 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 23 |
| Failure To Sense | 0 |
| Impedance Abnormal | 2 |
| Insulation Breach | 1 |
| Lead Dislodgement | 27 |
| Oversensing | 0 |
| Unspecified | 9 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 12 |
| Crimp Weld Bond | 1 |
| Insulation Breach | 31 |
| Other | 3 |

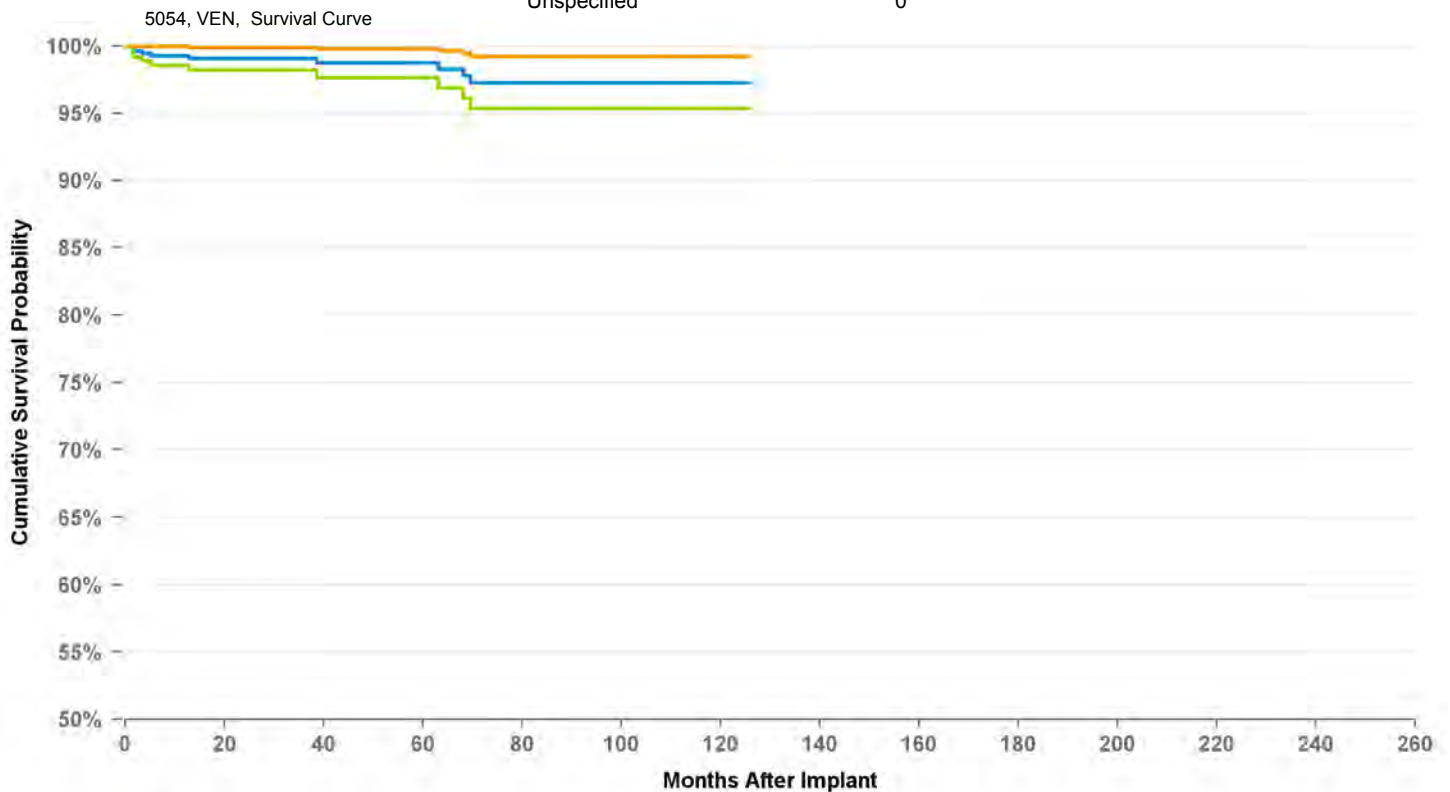

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.3% | 99.1% | 99.1% | 98.7% | 98.7% | 97.3% | 97.3% | 97.3% | 97.3% | 97.3% | 97.3% |
| # | 474 | 387 | 301 | 260 | 226 | 188 | 163 | 135 | 95 | 67 | 57 |

PACING LEAD

5068

ATRIAL PLACEMENT

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 1/2/1997 |
| CE Approval Date | |
| Registered US Implants | 102,406 |
| Estimated Active US | 27,024 |

Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Active Screw-in |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 979 |
| Cumulative Months of Follow-Up | 26,896 |
| Number of Leads Active in Study | 28 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 2 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 1 |
| Lead Dislodgement | 2 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 1 |
| Unspecified | 0 |


7

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 18 |
| Conductor Fracture | 4 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 31 |
| Failure To Sense | 5 |
| Impedance Abnormal | 1 |
| Insulation Breach | 1 |
| Lead Dislodgement | 20 |
| Oversensing | 1 |
| Unspecified | 7 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 42 |
| Crimp Weld Bond | 2 |
| Insulation Breach | 59 |
| Other | 83 |

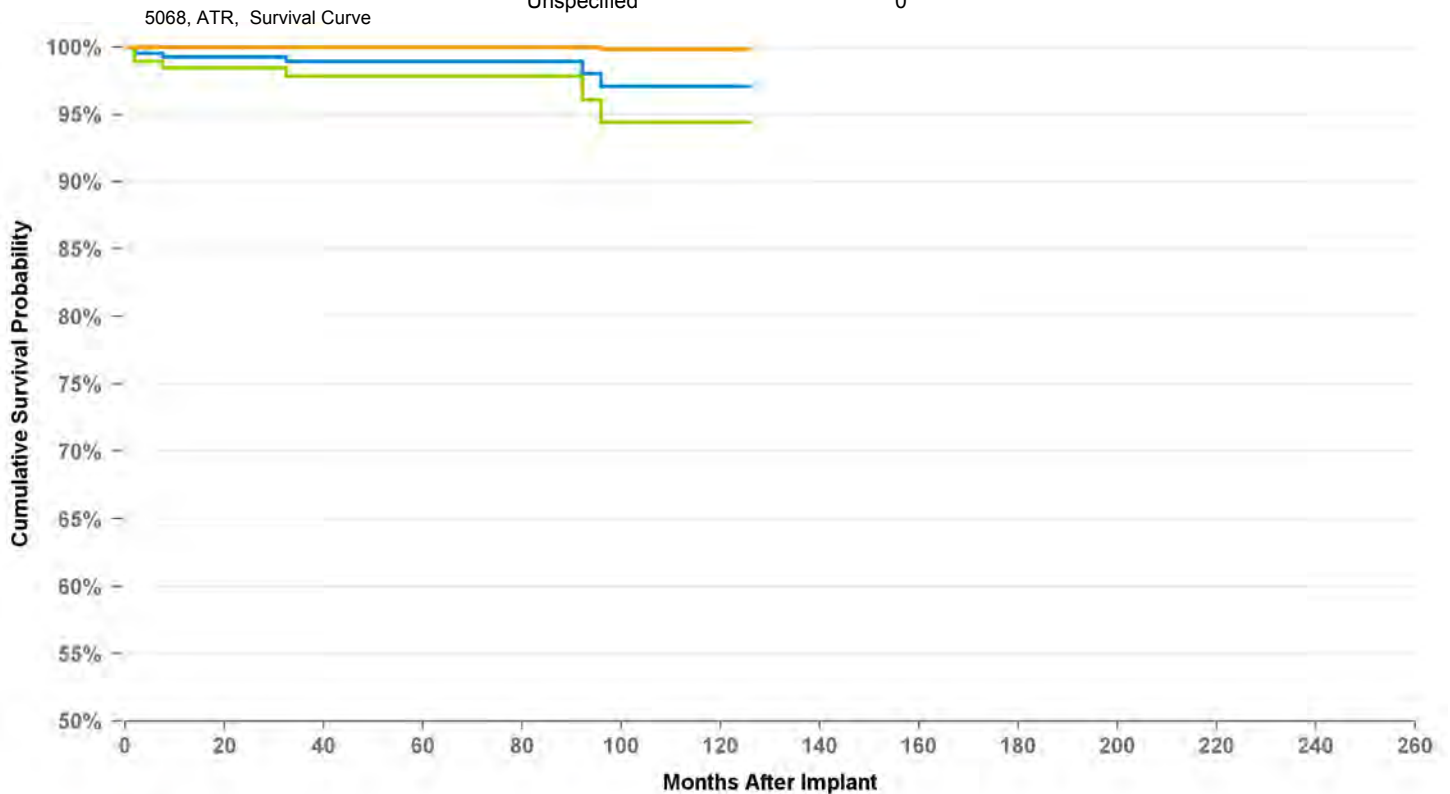

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.3% | 99.3% | 98.9% | 98.9% | 98.9% | 98.9% | 98.9% | 97.1% | 97.1% | 97.1% | 97.1% |
| # | 354 | 303 | 258 | 226 | 193 | 155 | 128 | 100 | 68 | 58 | 50 |

PACING LEAD

5068

VENTRICULAR PLACEMENT

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 1/2/1997 |
| CE Approval Date | |
| Registered US Implants | 102,406 |
| Estimated Active US | 27,024 |

Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Active Screw-in |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,371 |
| Cumulative Months of Follow-Up | 31,774 |
| Number of Leads Active in Study | 44 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 2 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 2 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 1 |
| Unspecified | 0 |


9

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 18 |
| Conductor Fracture | 4 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 31 |
| Failure To Sense | 5 |
| Impedance Abnormal | 1 |
| Insulation Breach | 1 |
| Lead Dislodgement | 20 |
| Oversensing | 1 |
| Unspecified | 7 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 42 |
| Crimp Weld Bond | 2 |
| Insulation Breach | 59 |
| Other | 83 |

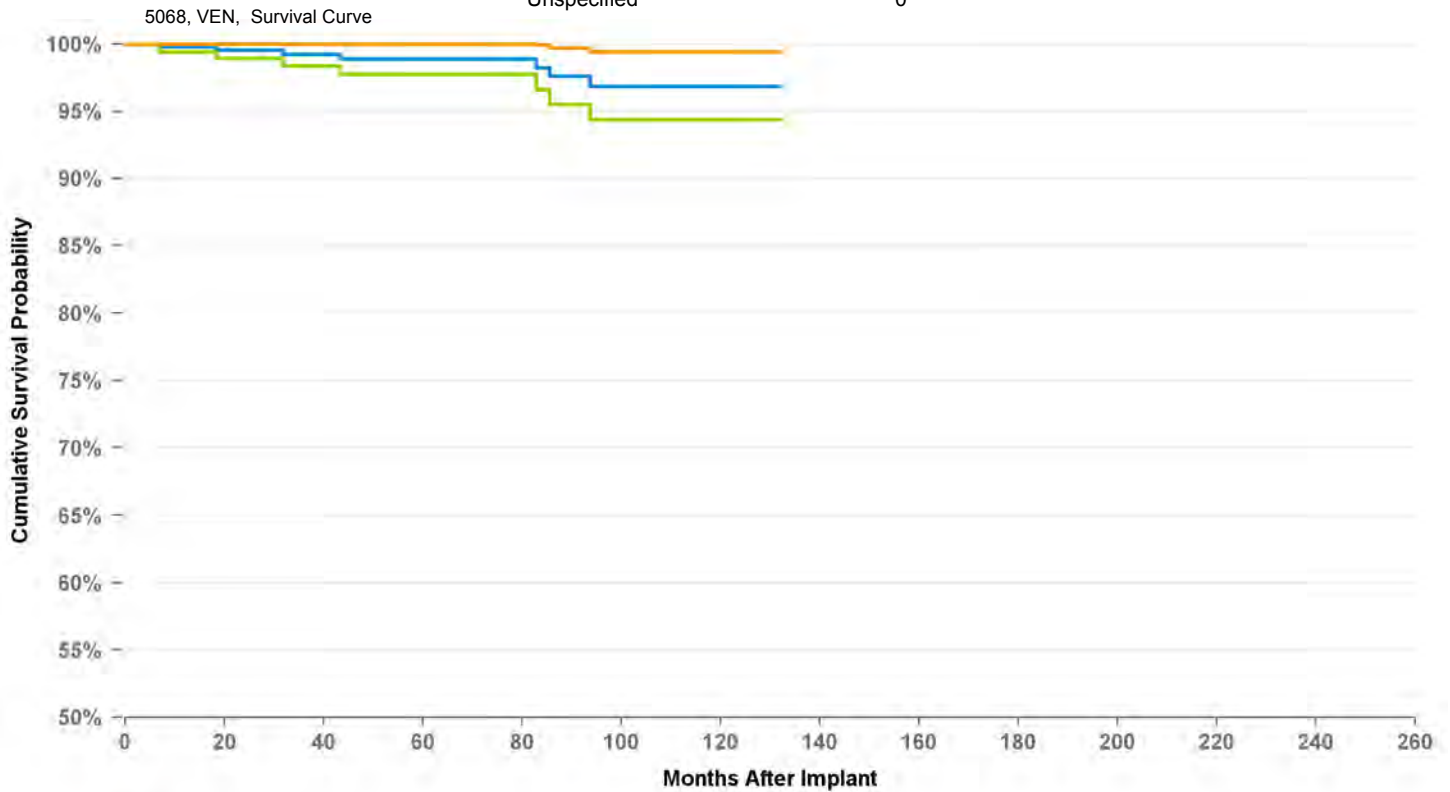

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 132 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.8% | 99.6% | 99.2% | 98.9% | 98.9% | 98.9% | 98.2% | 96.9% | 96.9% | 96.9% | 96.9% |
| # | 449 | 359 | 291 | 246 | 223 | 189 | 151 | 125 | 103 | 83 | 63 |

PACING LEAD

5072

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 6/5/1998 |
| CE Approval Date | 9/25/1997 |
| Registered US Implants | 10,054 |
| Estimated Active US | 3,807 |

Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Fixed Screw |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 514 |
| Cumulative Months of Follow-Up | 22,872 |
| Number of Leads Active in Study | 15 |

Product Surveillance Registry Qualifying Complications


| | |
|---|---|
| Cardiac Perforation | 1 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 1 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 2 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 2 |
| Oversensing | 0 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 3 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 9 |
| Other | 0 |

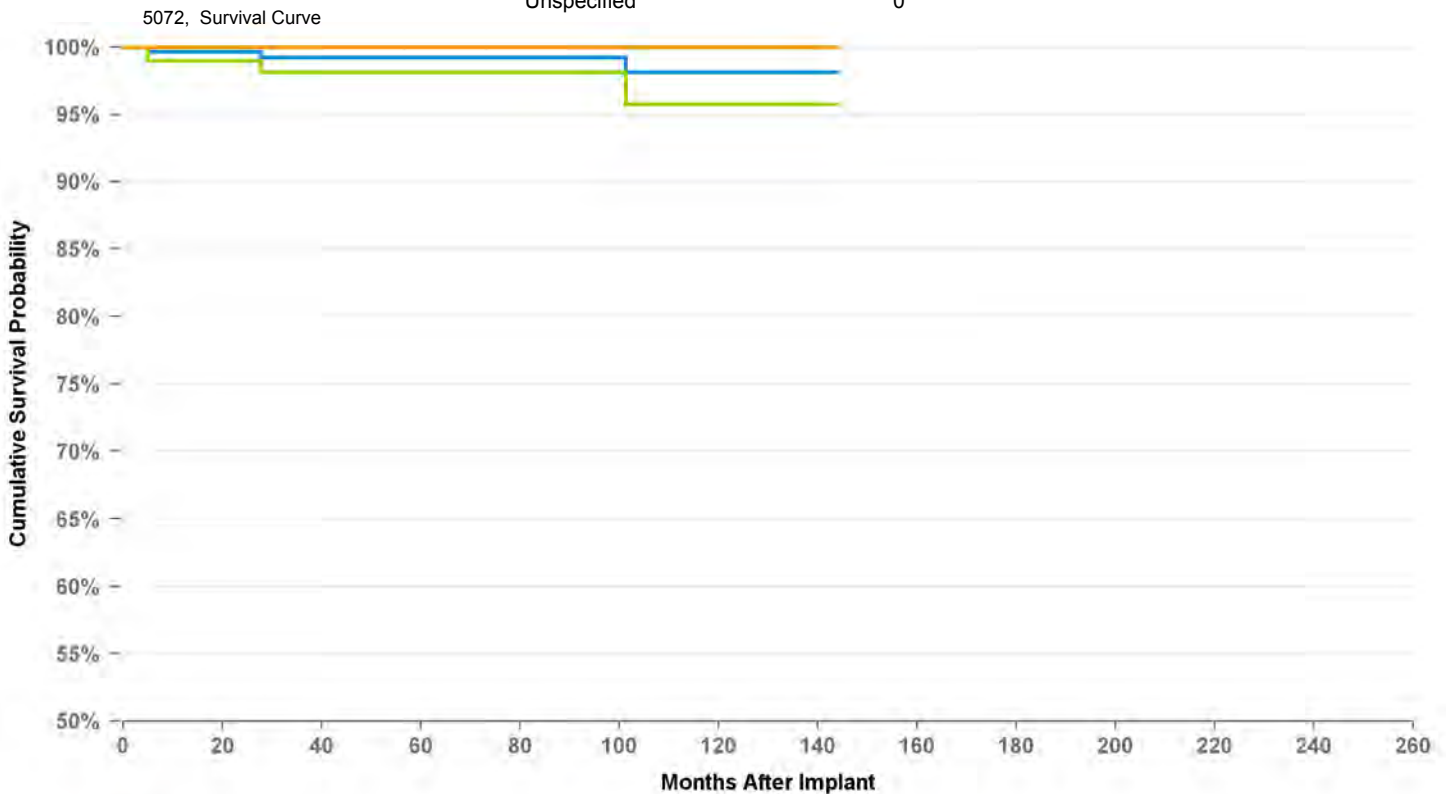

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 144 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.7% | 99.7% | 99.2% | 99.2% | 99.2% | 99.2% | 99.2% | 99.2% | 98.1% | 98.1% | 98.1% | 98.1% |
| # | 261 | 232 | 216 | 191 | 157 | 136 | 109 | 93 | 83 | 73 | 63 | 52 |

PACING LEAD

5076

ATRIAL PLACEMENT

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 8/31/2000 |
| CE Approval Date | 8/12/1999 |
| Registered US Implants | 1,720,845 |
| Estimated Active US | 1,089,008 |

Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Active Screw-in |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|---------|
| Number of Leads Enrolled in Study | 5,039 |
| Cumulative Months of Follow-Up | 182,831 |
| Number of Leads Active in Study | 2,490 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 1 |
| Conductor Fracture | 5 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 2 |
| Failure To Capture | 6 |
| Failure To Sense | 2 |
| Impedance Abnormal | 4 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 1 |
| Lead Dislodgement | 6 |
| Medical Judgment | 0 |
| Other Complication | 2 |
| Oversensing | 1 |
| Unspecified | 0 |


30

US Acute Lead Observations

| | |
|--------------------------|-----|
| Cardiac Perforation | 268 |
| Conductor Fracture | 15 |
| Extracardiac Stimulation | 21 |
| Failure To Capture | 331 |
| Failure To Sense | 54 |
| Impedance Abnormal | 20 |
| Insulation Breach | 8 |
| Lead Dislodgement | 799 |
| Oversensing | 47 |
| Unspecified | 31 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 570 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 577 |
| Other | 195 |

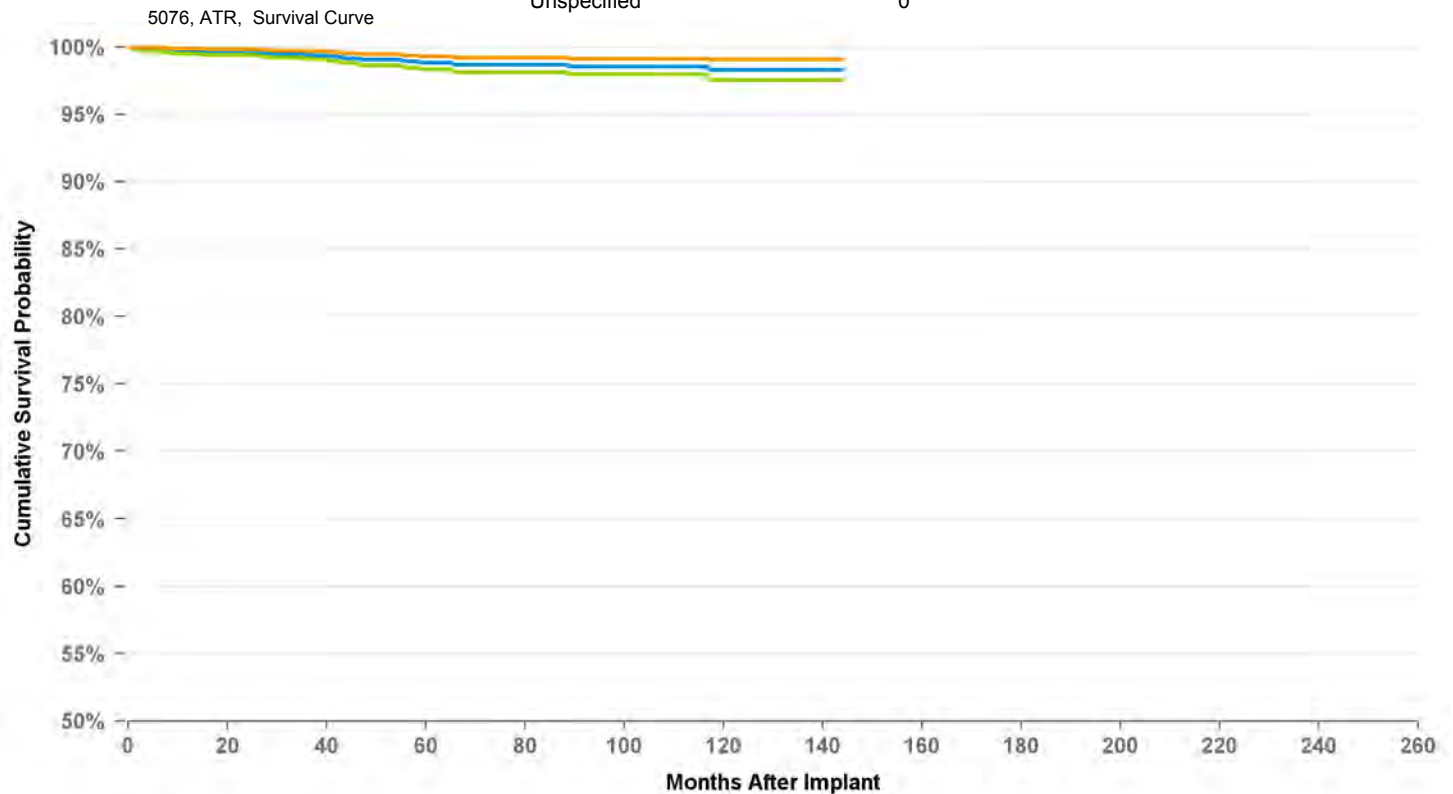

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 144 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.7% | 99.6% | 99.4% | 99.1% | 98.8% | 98.7% | 98.7% | 98.6% | 98.6% | 98.3% | 98.3% | 98.3% |
| # | 3,150 | 2,249 | 1,849 | 1,480 | 1,177 | 976 | 828 | 638 | 429 | 257 | 136 | 54 |

PACING LEAD

5076

VENTRICULAR PLACEMENT

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 8/31/2000 |
| CE Approval Date | 8/12/1999 |
| Registered US Implants | 1,720,845 |
| Estimated Active US | 1,089,008 |

Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Active Screw-in |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 2,133 |
| Cumulative Months of Follow-Up | 76,607 |
| Number of Leads Active in Study | 694 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 1 |
| Conductor Fracture | 4 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 9 |
| Failure To Sense | 1 |
| Impedance Abnormal | 4 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 3 |
| Medical Judgment | 0 |
| Other Complication | 1 |
| Oversensing | 0 |
| Unspecified | 0 |

23


US Acute Lead Observations

| | |
|--------------------------|-----|
| Cardiac Perforation | 268 |
| Conductor Fracture | 15 |
| Extracardiac Stimulation | 21 |
| Failure To Capture | 331 |
| Failure To Sense | 54 |
| Impedance Abnormal | 20 |
| Insulation Breach | 8 |
| Lead Dislodgement | 799 |
| Oversensing | 47 |
| Unspecified | 31 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 570 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 577 |
| Other | 195 |

5076, VEN, Survival Curve

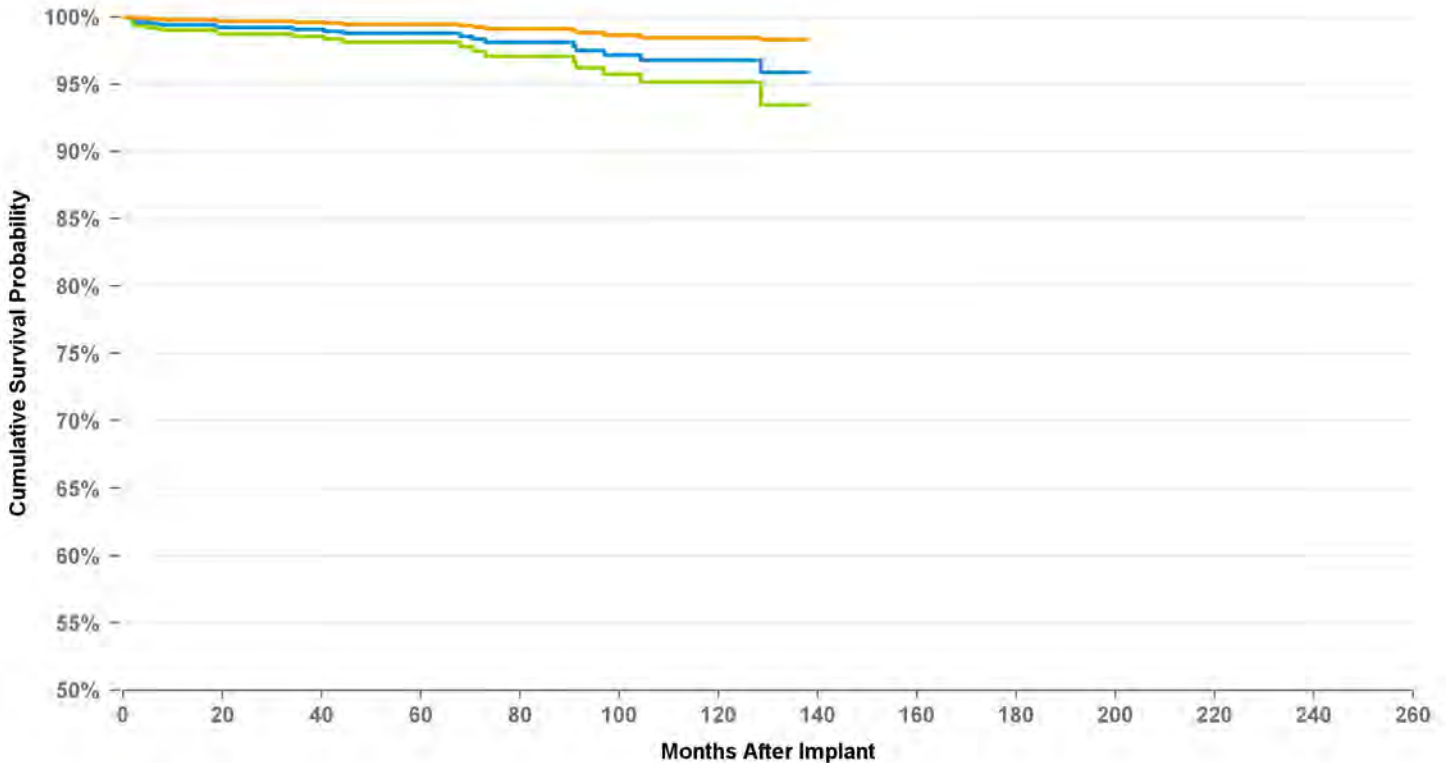

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 138 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.4% | 99.2% | 99.1% | 98.8% | 98.8% | 98.3% | 98.1% | 97.5% | 96.8% | 96.8% | 95.9% | 95.9% |
| # | 1,300 | 913 | 749 | 592 | 491 | 415 | 349 | 274 | 198 | 134 | 81 | 63 |

PACING LEAD

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 2/8/2011 |
| CE Approval Date | 1/21/2009 |
| Registered US Implants | 206,227 |
| Estimated Active US | 196,468 |


Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 2,961 |
| Cumulative Months of Follow-Up | 59,890 |
| Number of Leads Active in Study | 2,230 |

5086MRI, ATR, Survival Curve

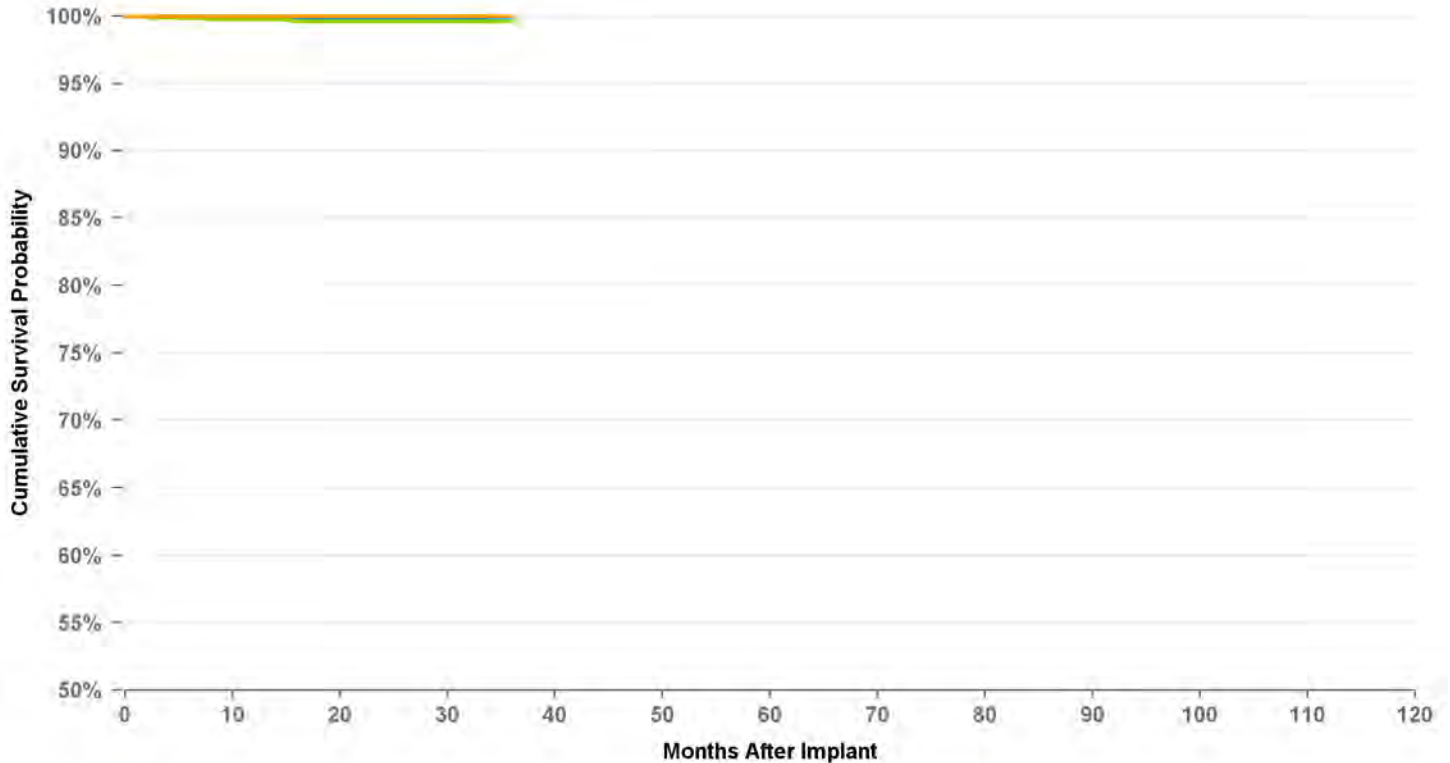

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | at 36 mo |
|-------|-------|-------|----------|
| % | 99.9% | 99.8% | 99.8% |
| # | 2,226 | 1,238 | 122 |

5086MRI

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 4 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

ATRIAL PLACEMENT

US Acute Lead Observations

| | |
|--------------------------|-----|
| Cardiac Perforation | 208 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 17 |
| Failure To Capture | 137 |
| Failure To Sense | 27 |
| Impedance Abnormal | 9 |
| Insulation Breach | 1 |
| Lead Dislodgement | 297 |
| Oversensing | 29 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 13 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 35 |
| Other | 10 |

PACING LEAD

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 2/8/2011 |
| CE Approval Date | 1/21/2009 |
| Registered US Implants | 206,227 |
| Estimated Active US | 196,468 |

Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Active Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 2,950 |
| Cumulative Months of Follow-Up | 59,779 |
| Number of Leads Active in Study | 2,222 |

5086MRI

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 2 |
| Failure To Sense | 1 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 3 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |


VENTRICULAR PLACEMENT

US Acute Lead Observations

| | |
|--------------------------|-----|
| Cardiac Perforation | 208 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 17 |
| Failure To Capture | 137 |
| Failure To Sense | 27 |
| Impedance Abnormal | 9 |
| Insulation Breach | 1 |
| Lead Dislodgement | 297 |
| Oversensing | 29 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 13 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 35 |
| Other | 10 |

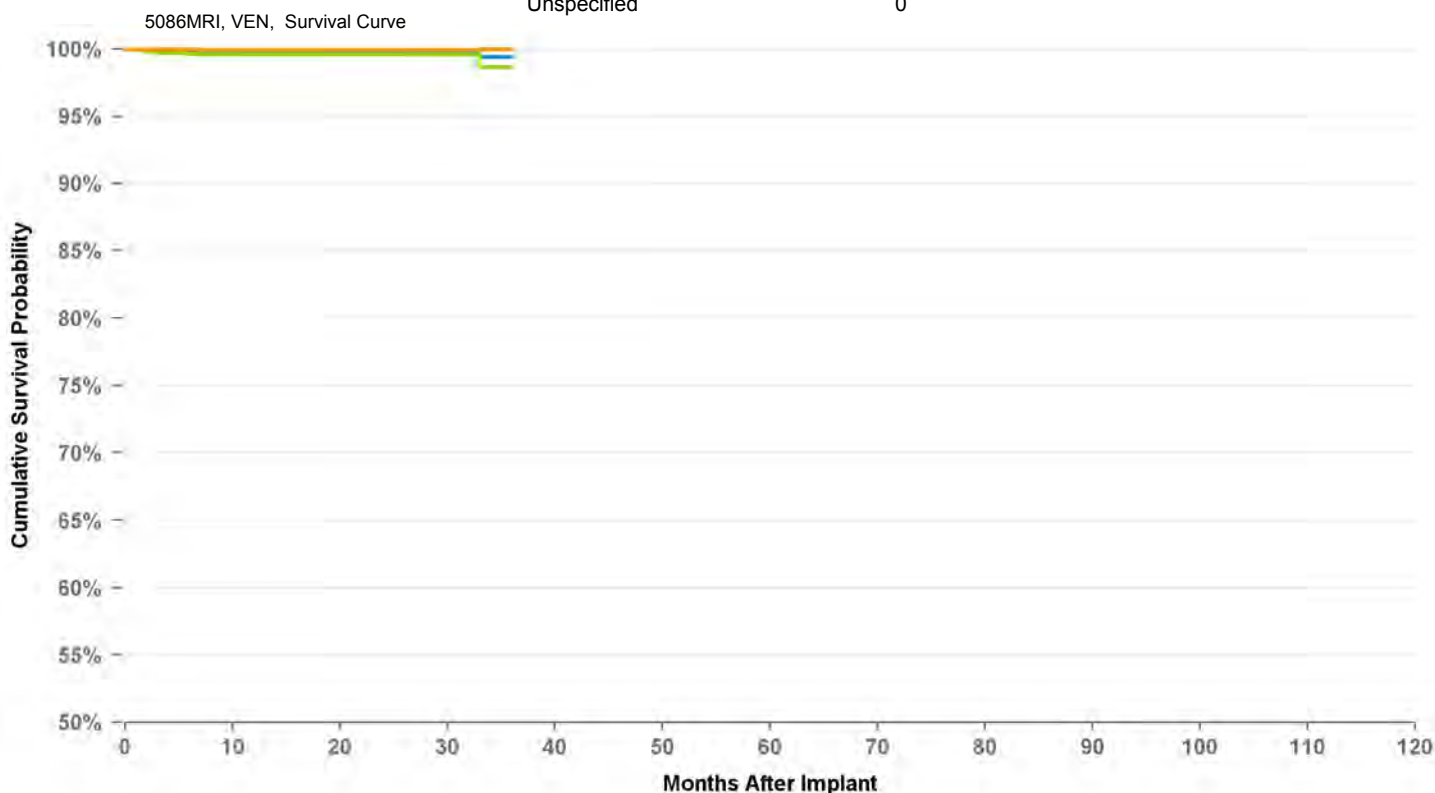

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | at 36 mo |
|-------|-------|-------|----------|
| % | 99.8% | 99.8% | 99.4% |
| # | 2,217 | 1,243 | 118 |

PACING LEAD

5092

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 6/3/1998 |
| CE Approval Date | 9/25/1997 |
| Registered US Implants | 138,380 |
| Estimated Active US | 61,159 |

Product Characteristics

| | |
|---------------------|-----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,195 |
| Cumulative Months of Follow-Up | 49,529 |
| Number of Leads Active in Study | 101 |

Product Surveillance Registry Qualifying Complications


| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 3 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 5 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 6 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 3 |
| Failure To Capture | 43 |
| Failure To Sense | 7 |
| Impedance Abnormal | 1 |
| Insulation Breach | 3 |
| Lead Dislodgement | 62 |
| Oversensing | 1 |
| Unspecified | 9 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 14 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 43 |
| Other | 3 |

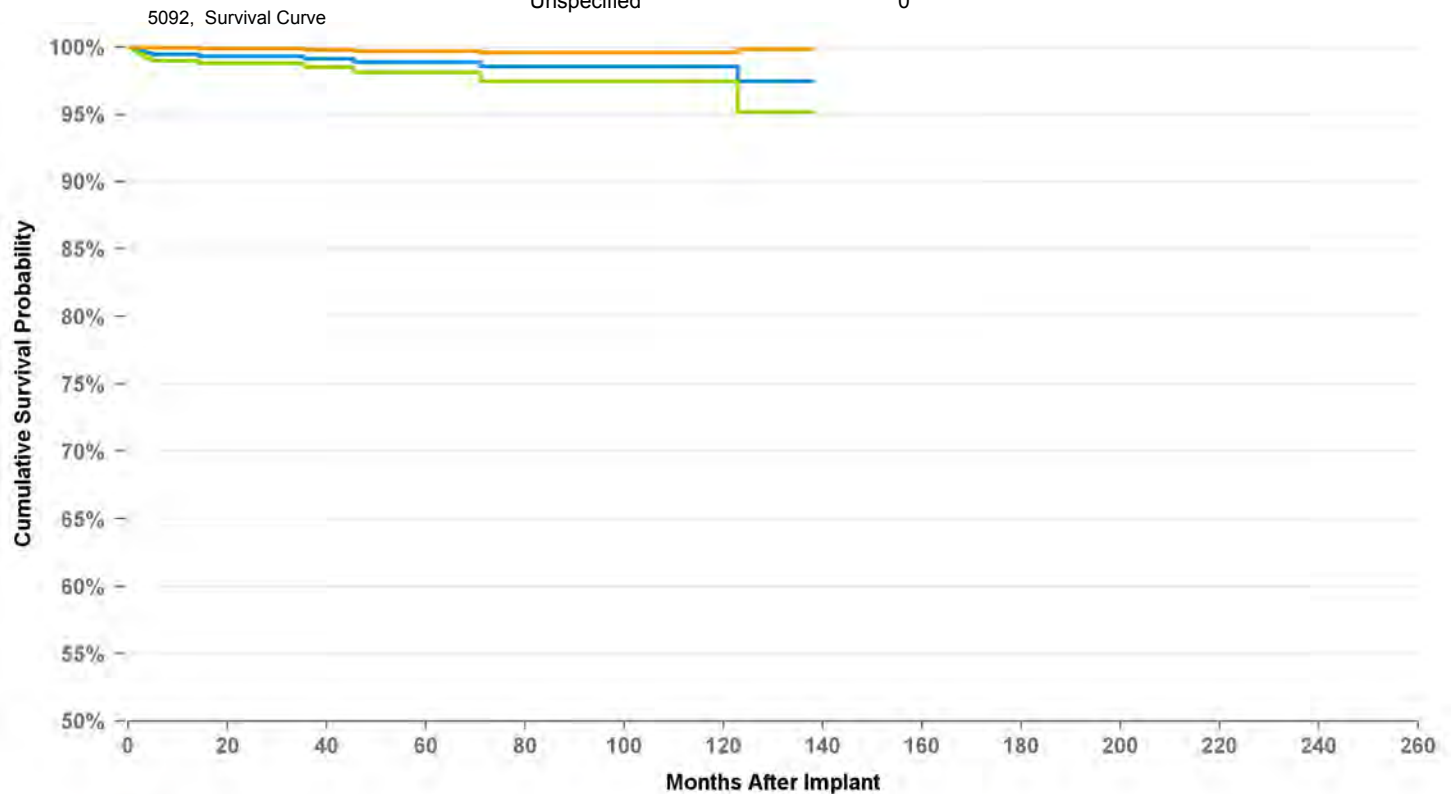

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 138 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.5% | 99.3% | 99.1% | 98.9% | 98.9% | 98.5% | 98.5% | 98.5% | 98.5% | 98.5% | 97.5% | 97.5% |
| # | 810 | 643 | 505 | 406 | 321 | 252 | 206 | 157 | 122 | 97 | 70 | 58 |

PACING LEAD

5534

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 2/9/1996 |
| CE Approval Date | |
| Registered US Implants | 25,846 |
| Estimated Active US | 6,322 |

Product Characteristics

| | |
|---------------------|----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium - J |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|-------|
| Number of Leads Enrolled in Study | 267 |
| Cumulative Months of Follow-Up | 9,609 |
| Number of Leads Active in Study | 3 |

Product Surveillance Registry Qualifying Complications


| | |
|---|----------|
| | 6 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 5 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 3 |
| Failure To Sense | 1 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 6 |
| Oversensing | 0 |
| Unspecified | 4 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 7 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 5 |
| Other | 4 |

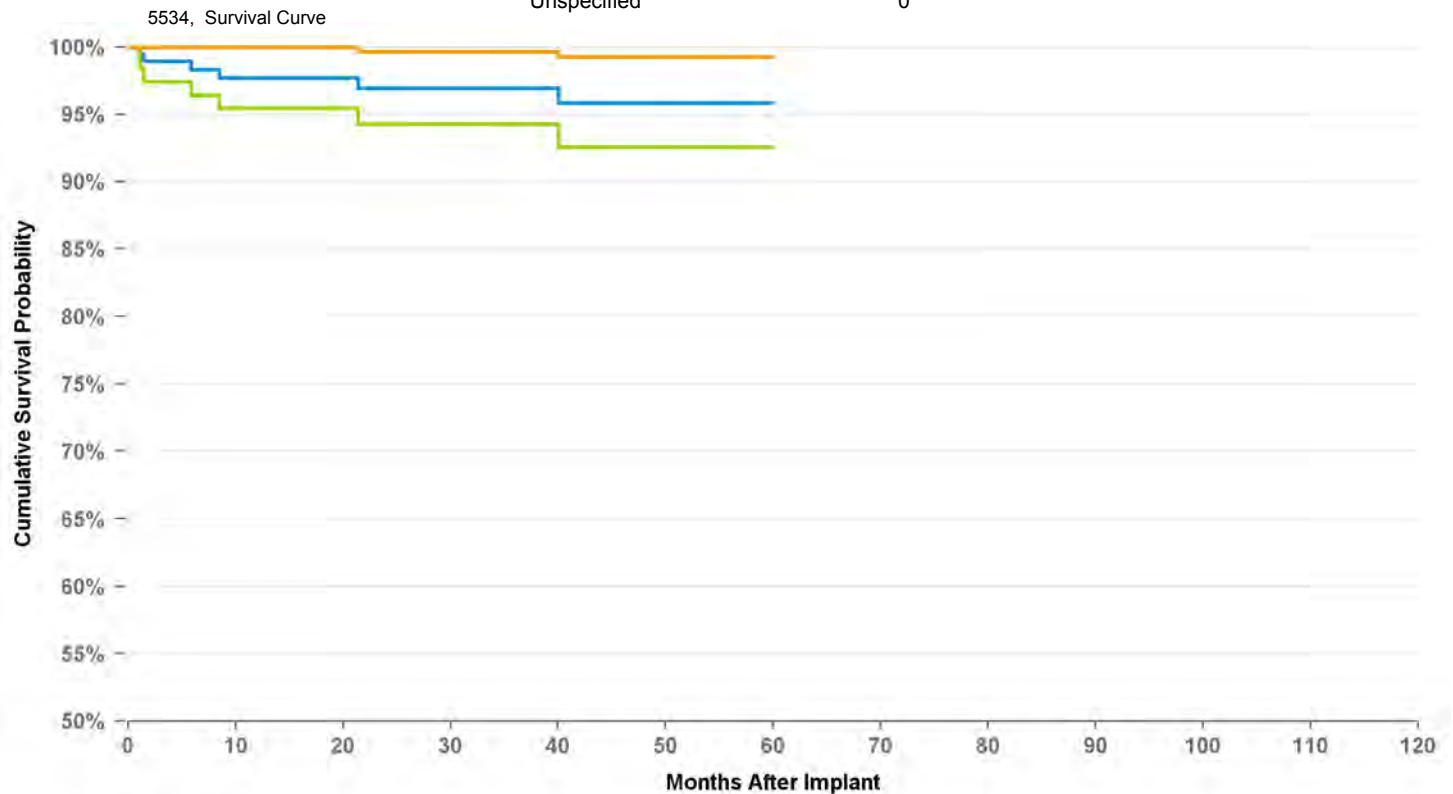

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | at 60 mo |
|-------|-------|-------|-------|-------|----------|
| % | 97.7% | 96.9% | 96.9% | 95.9% | 95.9% |
| # | 148 | 126 | 98 | 79 | 55 |

PACING LEAD

5554

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 6/3/1998 |
| CE Approval Date | 6/5/1997 |
| Registered US Implants | 63,584 |
| Estimated Active US | 28,307 |

Product Characteristics

| | |
|---------------------|----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium - J |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|-------|
| Number of Leads Enrolled in Study | 355 |
| Cumulative Months of Follow-Up | 8,287 |
| Number of Leads Active in Study | 10 |

Product Surveillance Registry Qualifying Complications


| | |
|---|----------|
| | 5 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 2 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 1 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 1 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 30 |
| Failure To Sense | 2 |
| Impedance Abnormal | 1 |
| Insulation Breach | 0 |
| Lead Dislodgement | 36 |
| Oversensing | 0 |
| Unspecified | 3 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 11 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 26 |
| Other | 2 |

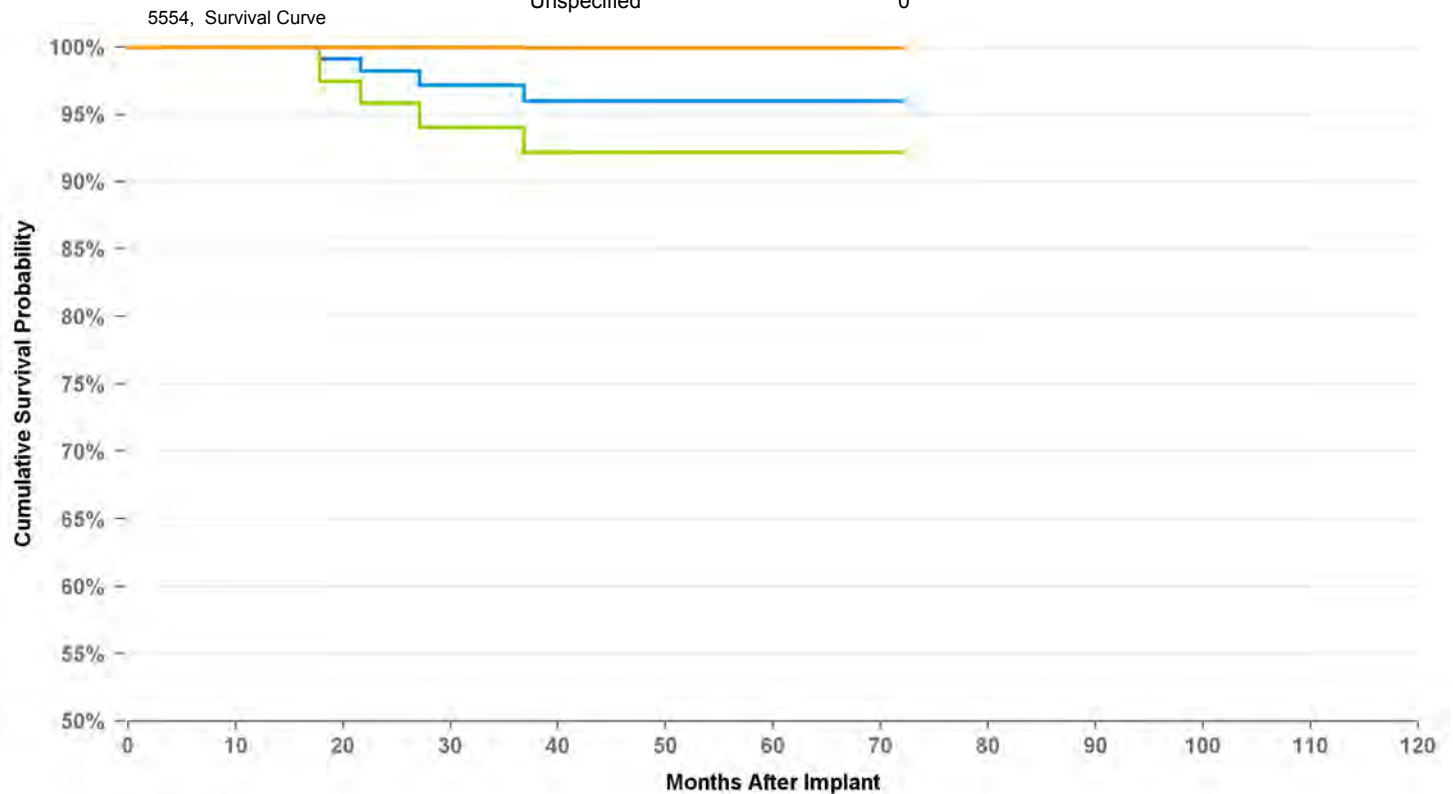

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | at 72 mo |
|-------|--------|-------|-------|-------|-------|----------|
| % | 100.0% | 98.2% | 97.2% | 96.0% | 96.0% | 96.0% |
| # | 146 | 107 | 82 | 74 | 59 | 50 |

PACING LEAD

5568

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 1/2/1997 |
| CE Approval Date | 8/14/1996 |
| Registered US Implants | 95,421 |
| Estimated Active US | 50,832 |

Product Characteristics

| | |
|---------------------|-----------------|
| Fixation Type | Active Screw-in |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium - J |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 1,129 |
| Cumulative Months of Follow-Up | 35,649 |
| Number of Leads Active in Study | 122 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 6 |
| Failure To Sense | 3 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 2 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 4 |
| Unspecified | 0 |


17

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 14 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 2 |
| Failure To Capture | 23 |
| Failure To Sense | 2 |
| Impedance Abnormal | 2 |
| Insulation Breach | 1 |
| Lead Dislodgement | 40 |
| Oversensing | 3 |
| Unspecified | 4 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 17 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 42 |
| Other | 37 |

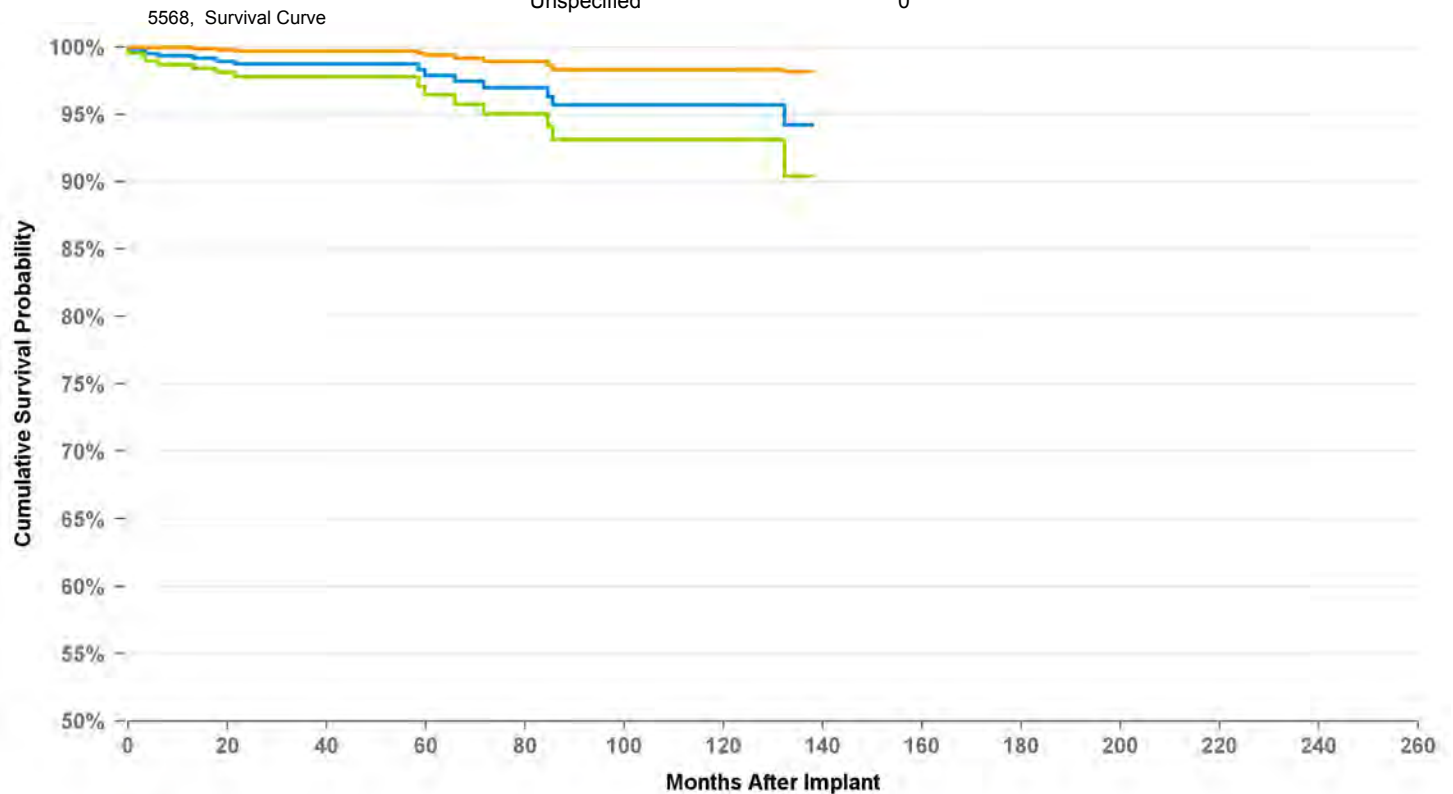

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | at 138 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.4% | 98.7% | 98.7% | 98.7% | 97.9% | 97.0% | 97.0% | 95.7% | 95.7% | 95.7% | 95.7% | 94.2% |
| # | 533 | 431 | 363 | 293 | 233 | 189 | 147 | 124 | 103 | 80 | 62 | 52 |

PACING LEAD

5592

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 6/3/1998 |
| CE Approval Date | 9/25/1997 |
| Registered US Implants | 36,220 |
| Estimated Active US | 19,077 |

Product Characteristics

| | |
|---------------------|----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium - J |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 696 |
| Cumulative Months of Follow-Up | 32,944 |
| Number of Leads Active in Study | 116 |

Product Surveillance Registry Qualifying Complications


| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 3 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 2 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 1 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 4 |
| Failure To Sense | 2 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 35 |
| Oversensing | 1 |
| Unspecified | 1 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 4 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 4 |
| Other | 0 |

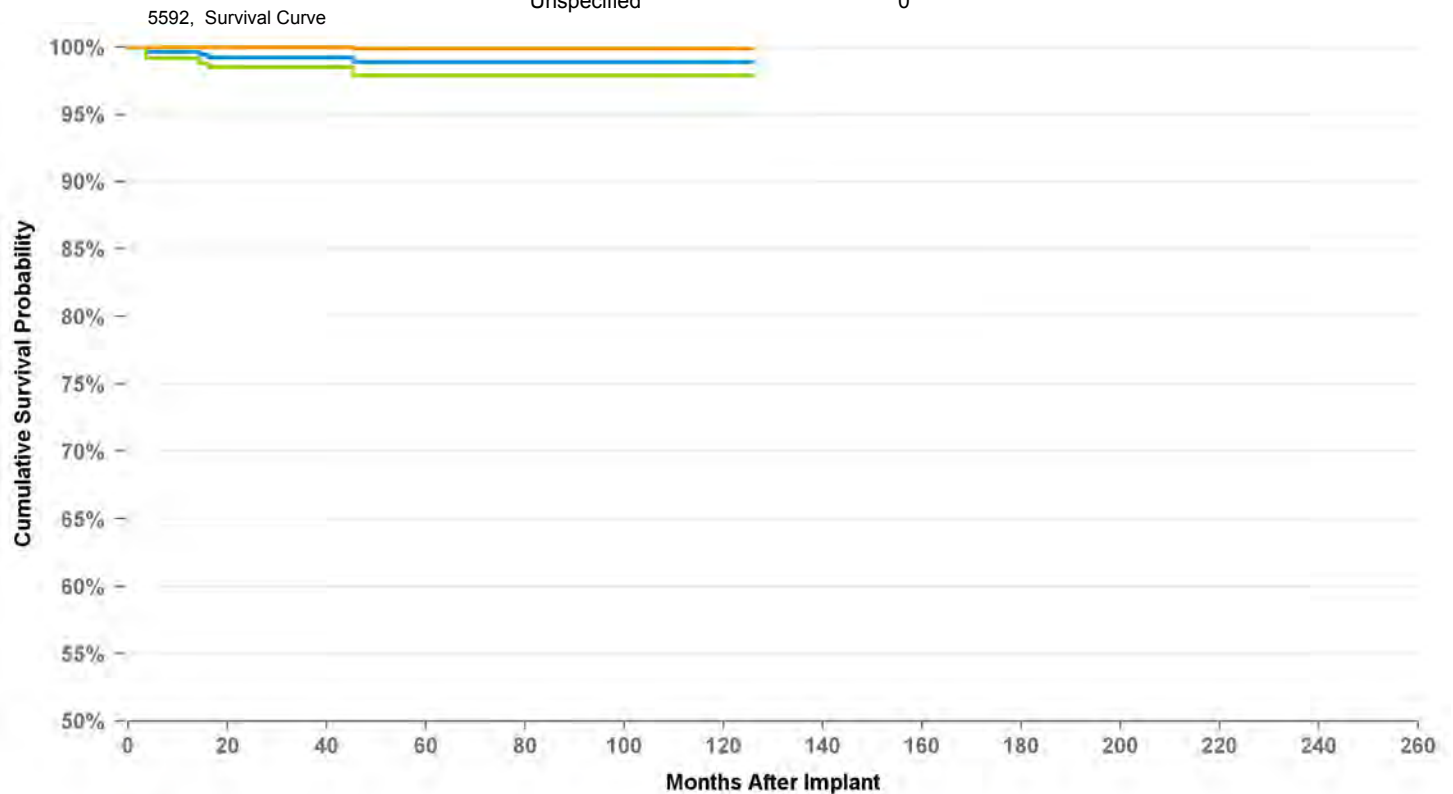

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.6% | 99.2% | 99.2% | 98.9% | 98.9% | 98.9% | 98.9% | 98.9% | 98.9% | 98.9% | 98.9% |
| # | 515 | 426 | 340 | 284 | 228 | 172 | 141 | 115 | 88 | 66 | 53 |

PACING LEAD

5594

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 6/25/2001 |
| CE Approval Date | 3/23/2001 |
| Registered US Implants | 17,009 |
| Estimated Active US | 10,648 |


Product Characteristics

| | |
|---------------------|----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium - J |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|-------|
| Number of Leads Enrolled in Study | 23 |
| Cumulative Months of Follow-Up | 1,635 |
| Number of Leads Active in Study | 9 |

5594, Survival Curve

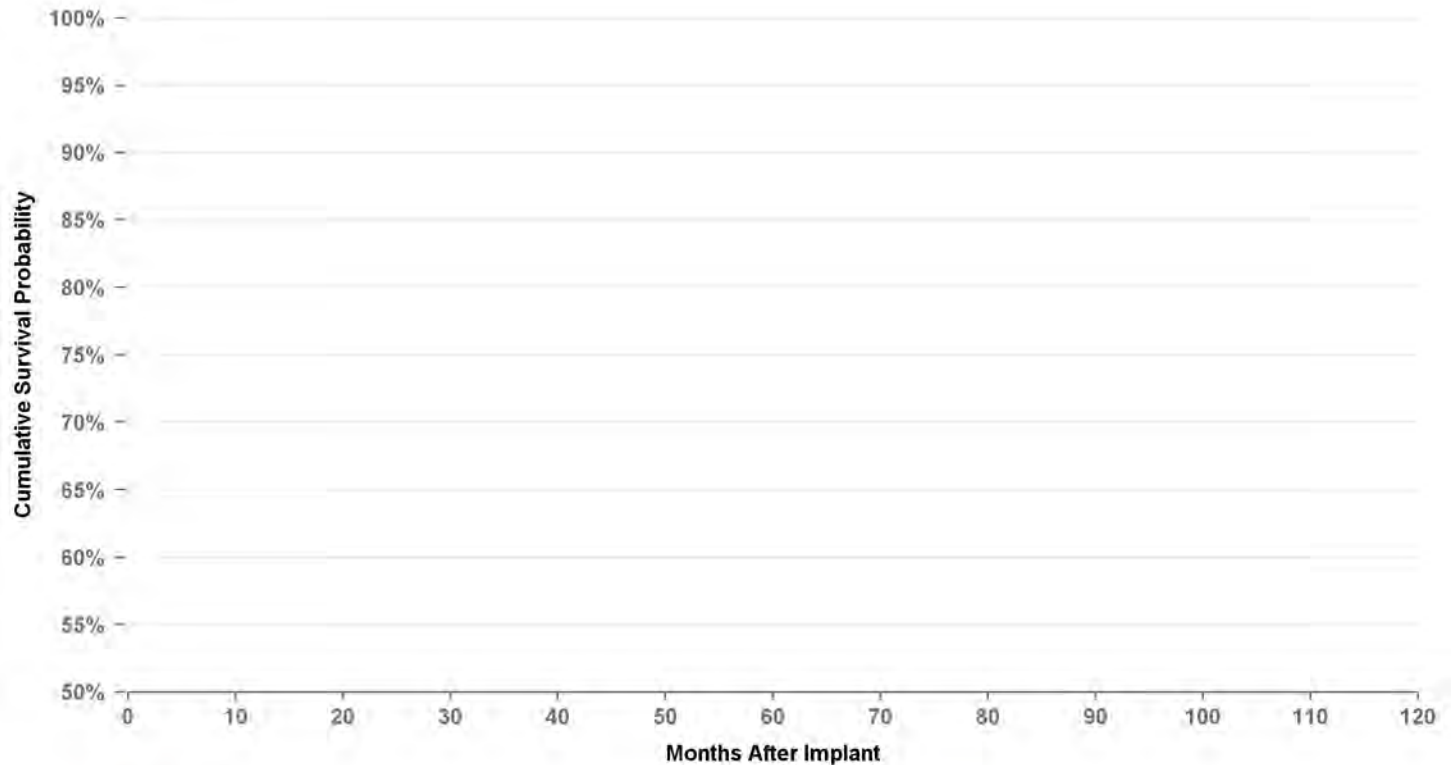

Graph Name

- Cumulative Survival Probability Graph
- Lower 95 Pct Confidence Graph
- Upper 95 Pct Confidence Graph

Years

%

#

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| | 0 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 0 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 12 |
| Oversensing | 0 |
| Unspecified | 2 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 9 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 10 |
| Other | 1 |

PACING LEAD

6940

Distribution Data

| | |
|--------------------------------|-----------------|
| US Market Release | 10/9/1998 |
| CE Approval Date | |
| Registered US Implants | 25,385 |
| Estimated Active US | 6,642 |
| Product Characteristics | |
| Fixation Type | Active Screw-in |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Atrium - J |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Qualifying Complications

| | |
|---|-----------|
| | 14 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 3 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 3 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 6 |
| Unspecified | 0 |

US Acute Lead Observations


| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach | 0 |
| Lead Dislodgement | 6 |
| Oversensing | 0 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 13 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 20 |
| Other | 12 |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 841 |
| Cumulative Months of Follow-Up | 42,929 |
| Number of Leads Active in Study | 48 |

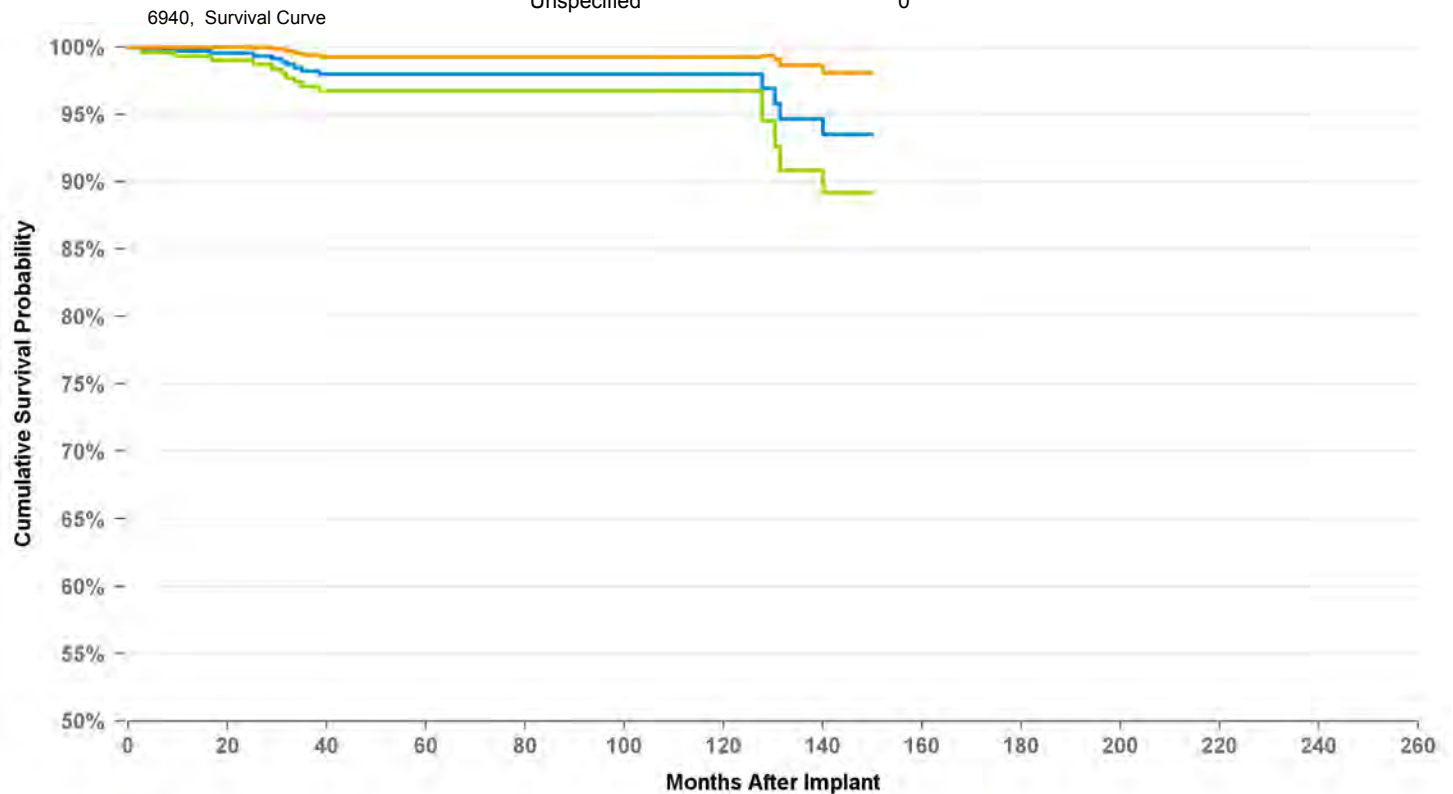

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | at 150 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.7% | 99.5% | 98.2% | 98.0% | 98.0% | 98.0% | 98.0% | 98.0% | 98.0% | 98.0% | 94.7% | 93.5% | 93.5% |
| # | 635 | 510 | 421 | 346 | 278 | 218 | 189 | 153 | 126 | 96 | 80 | 69 | 59 |

EPI MYOCARDIAL LEAD

4965

Distribution Data

| | |
|------------------------|----------|
| US Market Release | 9/6/1996 |
| CE Approval Date | 1/1/1993 |
| Registered US Implants | 21,855 |
| Estimated Active US | 9,290 |

Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Suture |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Myocardial |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Unipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|-------|
| Number of Leads Enrolled in Study | 228 |
| Cumulative Months of Follow-Up | 6,718 |
| Number of Leads Active in Study | 11 |

Product Surveillance Registry Qualifying Complications

13


| | |
|---|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 6 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 3 |
| Failure To Sense | 1 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 1 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 2 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 4 |
| Failure To Sense | 5 |
| Impedance Abnormal | 6 |
| Insulation Breach | 0 |
| Lead Dislodgement | 0 |
| Oversensing | 1 |
| Unspecified | 3 |

USA Returned Product Analysis

| | |
|--------------------|-----|
| Conductor Fracture | 199 |
| Crimp Weld Bond | 1 |
| Insulation Breach | 41 |
| Other | 0 |

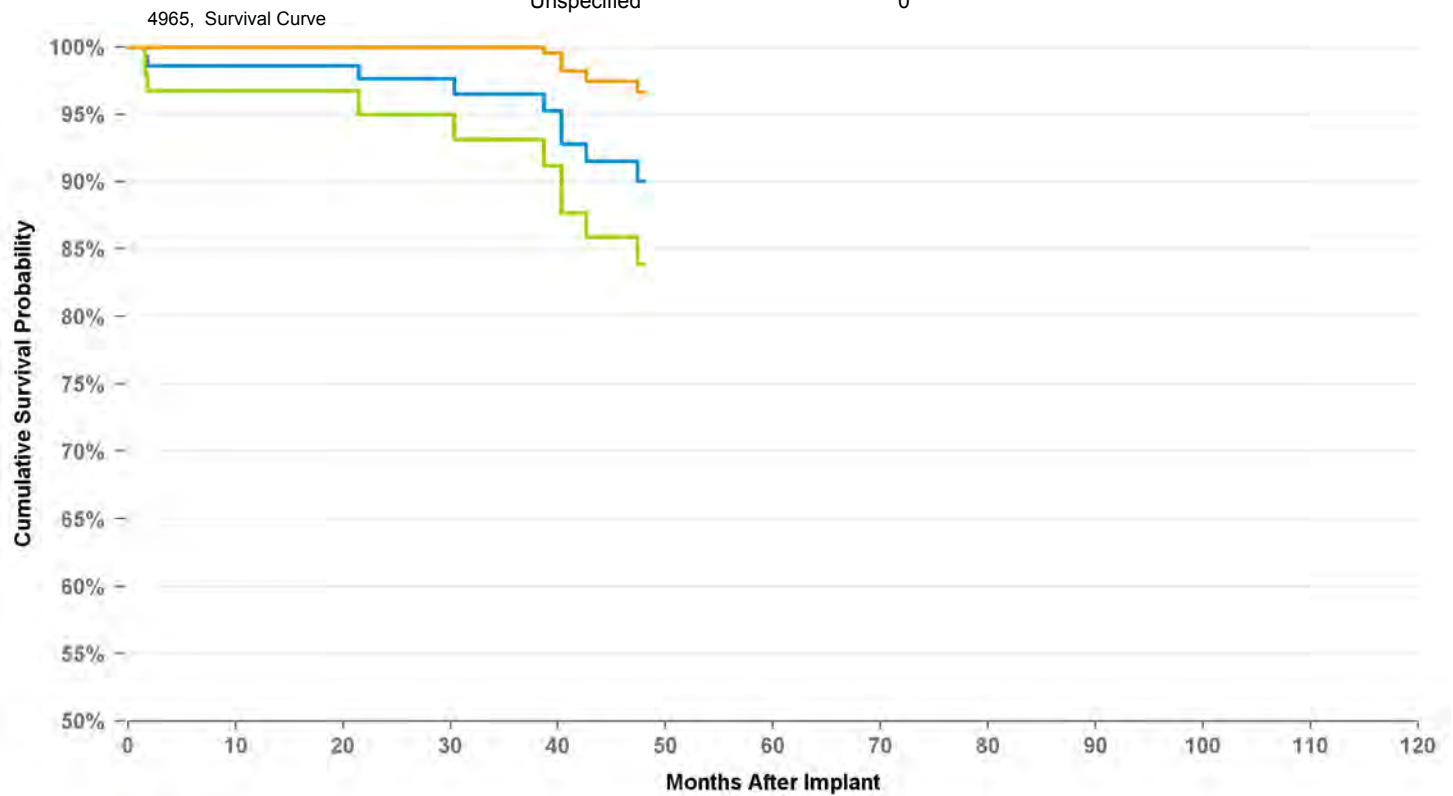

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | at 48 mo |
|-------|-------|-------|-------|----------|
| % | 98.6% | 97.6% | 96.5% | 90.0% |
| # | 125 | 104 | 84 | 61 |

EPI MYOCARDIAL LEAD

4968

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 9/16/1999 |
| CE Approval Date | 4/21/1998 |
| Registered US Implants | 33,661 |
| Estimated Active US | 20,822 |

Product Characteristics

| | |
|---------------------|---------------------------|
| Fixation Type | Suture |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Myocardial |
| Lead Tip Location | Atrium or Right Ventricle |
| Pace/Sense Polarity | Bipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 864 |
| Cumulative Months of Follow-Up | 43,771 |
| Number of Leads Active in Study | 297 |

Product Surveillance Registry Qualifying Complications


| | |
|---|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 14 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 2 |
| Failure To Capture | 20 |
| Failure To Sense | 3 |
| Impedance Abnormal | 4 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 3 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 2 |
| Oversensing | 13 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 0 |
| Conductor Fracture | 2 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 22 |
| Failure To Sense | 1 |
| Impedance Abnormal | 3 |
| Insulation Breach | 1 |
| Lead Dislodgement | 4 |
| Oversensing | 4 |
| Unspecified | 0 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 46 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 28 |
| Other | 1 |

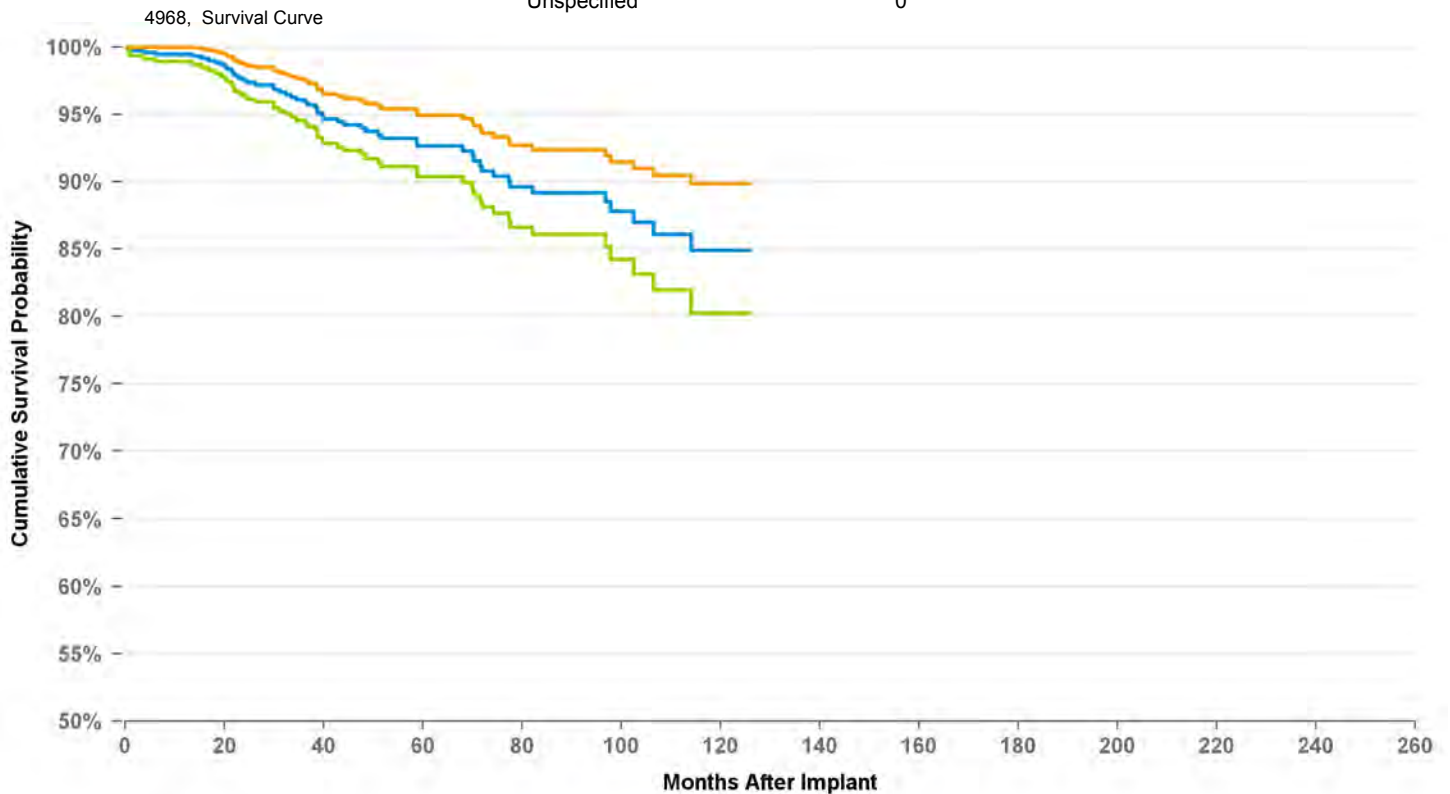

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | at 126 mo |
|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-----------|
| % | 99.5% | 97.5% | 96.1% | 94.0% | 92.6% | 90.8% | 89.2% | 89.2% | 86.1% | 84.9% | 84.9% |
| # | 679 | 588 | 501 | 382 | 305 | 234 | 181 | 131 | 82 | 59 | 50 |

EPI MYOCARDIAL LEAD

5071

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 12/3/1992 |
| CE Approval Date | 1/1/1993 |
| Registered US Implants | 47,810 |
| Estimated Active US | 16,066 |

Product Characteristics

| | |
|---------------------|-----------------|
| Fixation Type | Fixed Screw In |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | None |
| Lead Placement | Myocardial |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Unipolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|-------|
| Number of Leads Enrolled in Study | 365 |
| Cumulative Months of Follow-Up | 7,649 |
| Number of Leads Active in Study | 92 |

Product Surveillance Registry Qualifying Complications


| | |
|---|-----------|
| | 18 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 1 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 14 |
| Failure To Sense | 0 |
| Impedance Abnormal | 1 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 2 |
| Unspecified | 0 |

US Acute Lead Observations

| | |
|--------------------------|----|
| Cardiac Perforation | 1 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 5 |
| Failure To Capture | 44 |
| Failure To Sense | 2 |
| Impedance Abnormal | 2 |
| Insulation Breach | 0 |
| Lead Dislodgement | 0 |
| Oversensing | 0 |
| Unspecified | 1 |

USA Returned Product Analysis

| | |
|--------------------|----|
| Conductor Fracture | 15 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 2 |
| Other | 0 |

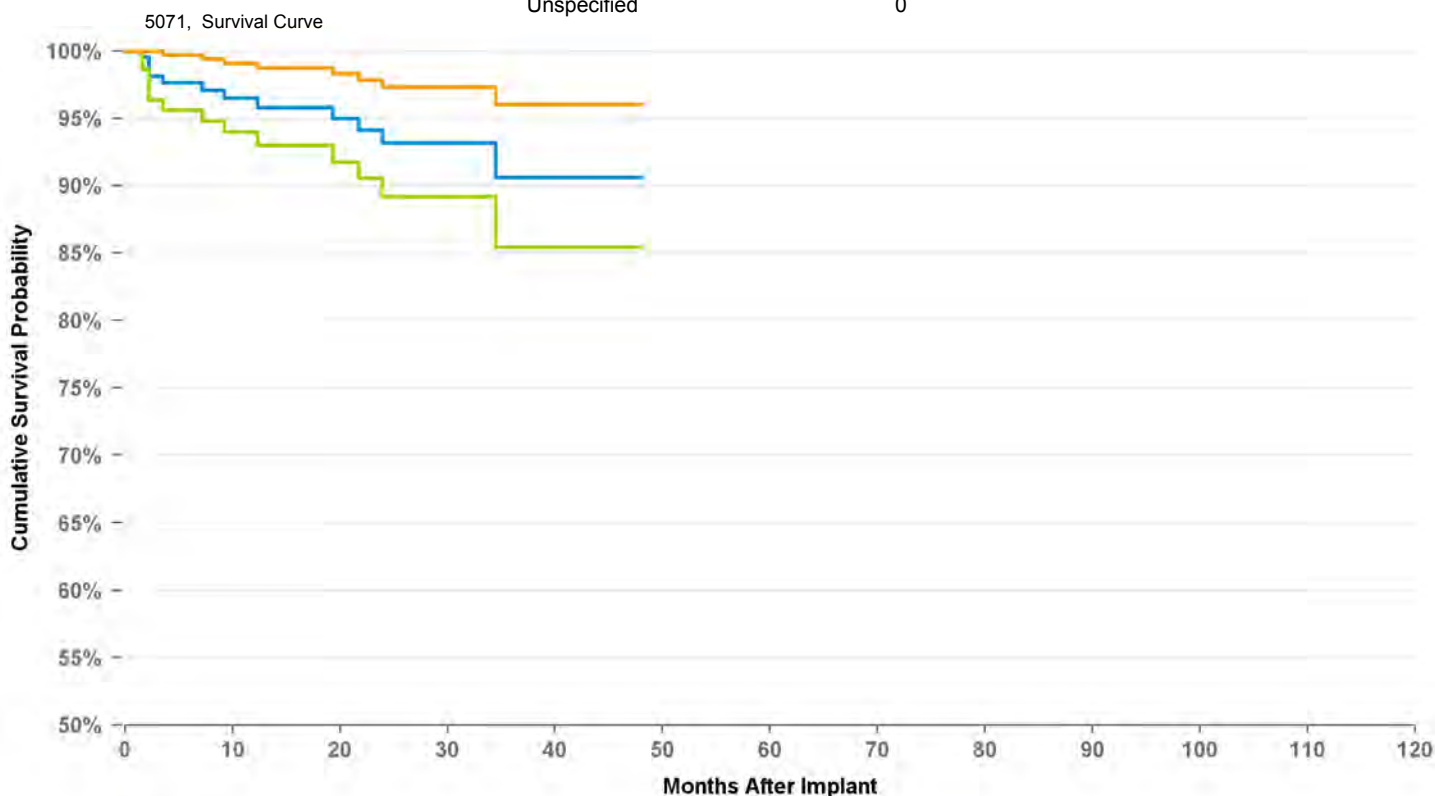

Graph Name

■ Cumulative Survival Probability Graph
 ■ Lower 95 Pct Confidence Graph
 ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | at 48 mo |
|-------|-------|-------|-------|----------|
| % | 96.5% | 93.2% | 90.6% | 90.6% |
| # | 146 | 99 | 71 | 55 |

VDD SINGLE PASS LEAD

5032

Distribution Data

| | |
|------------------------|-----------|
| US Market Release | 3/22/1996 |
| CE Approval Date | |
| Registered US Implants | 5,218 |
| Estimated Active US | 1,093 |

Product Characteristics

| | |
|---------------------|-----------------|
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Quadripolar |

Product Surveillance Registry Results

| | |
|-----------------------------------|-----|
| Number of Leads Enrolled in Study | 38 |
| Cumulative Months of Follow-Up | 287 |
| Number of Leads Active in Study | 0 |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| | 1 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 0 |
| Failure To Sense | 1 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |


US Acute Lead Observations

| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 1 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 1 |
| Oversensing | 0 |
| Unspecified | 1 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 7 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 6 |
| Other | 0 |

5032, Survival Curve

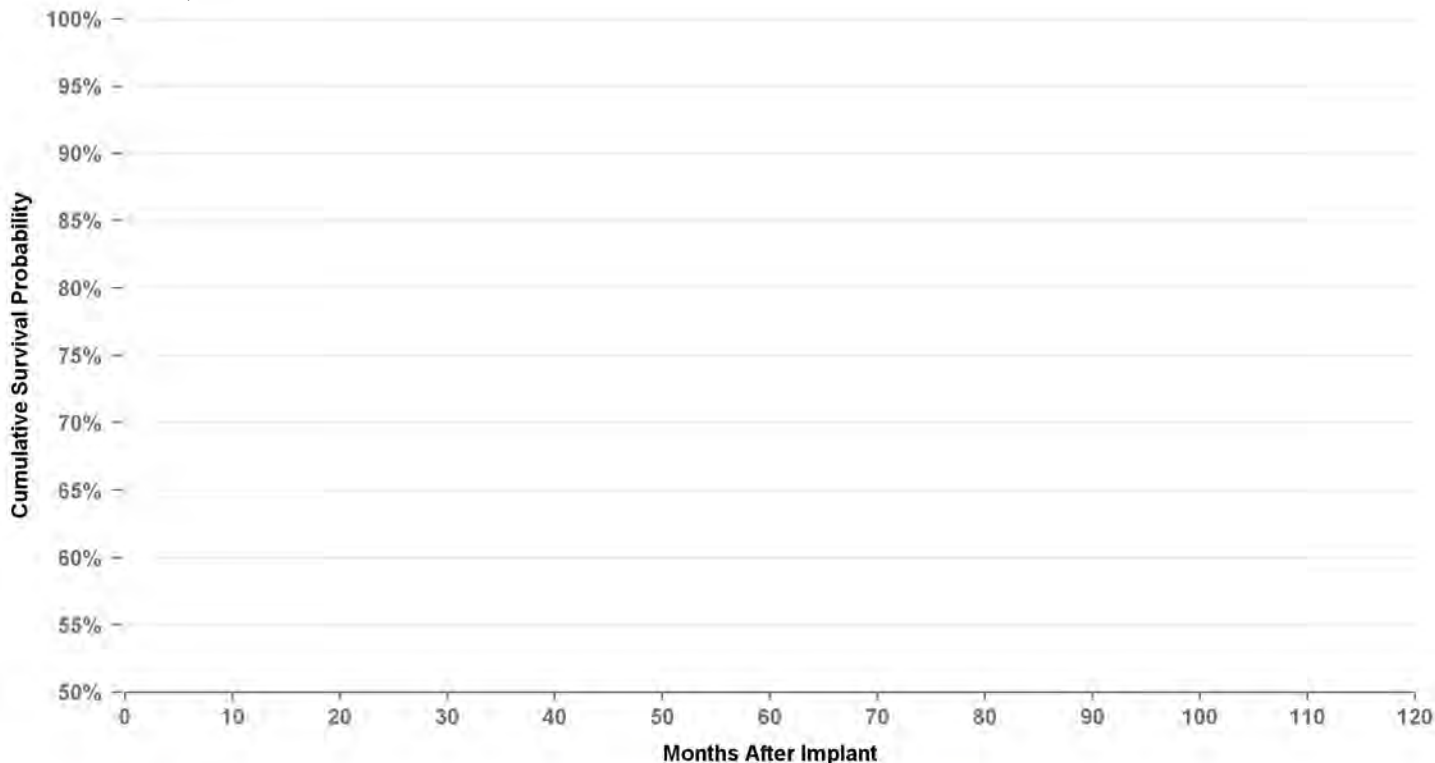

Graph Name

- Cumulative Survival Probability Graph
- Lower 95 Pct Confidence Graph
- Upper 95 Pct Confidence Graph

Years

%

#

VDD SINGLE PASS LEAD

5038

Distribution Data

| | |
|--------------------------------|-----------------|
| US Market Release | 9/10/1998 |
| CE Approval Date | 4/15/1997 |
| Registered US Implants | 9,154 |
| Estimated Active US | 3,448 |
| Product Characteristics | |
| Fixation Type | Tines |
| Lead Function | Pacing/Sensing |
| Steroid Indicator | Yes |
| Lead Placement | Transvenous |
| Lead Tip Location | Right Ventricle |
| Pace/Sense Polarity | Quadripolar |

Product Surveillance Registry Qualifying Complications

| | |
|---|---|
| | 7 |
| Cardiac Perforation | 0 |
| Conductor Fracture | 3 |
| Electrical Abandonment | 0 |
| Extracardiac Stimulation | 0 |
| Failure To Capture | 1 |
| Failure To Sense | 3 |
| Impedance Abnormal | 0 |
| Insulation Breach (ESC) | 0 |
| Insulation Breach (MIO) | 0 |
| Insulation Breach (not further defined) | 0 |
| Lead Dislodgement | 0 |
| Medical Judgment | 0 |
| Other Complication | 0 |
| Oversensing | 0 |
| Unspecified | 0 |

US Acute Lead Observations


| | |
|--------------------------|---|
| Cardiac Perforation | 0 |
| Conductor Fracture | 0 |
| Extracardiac Stimulation | 1 |
| Failure To Capture | 1 |
| Failure To Sense | 2 |
| Impedance Abnormal | 0 |
| Insulation Breach | 0 |
| Lead Dislodgement | 3 |
| Oversensing | 0 |
| Unspecified | 0 |

Product Surveillance Registry Results

| | |
|-----------------------------------|--------|
| Number of Leads Enrolled in Study | 567 |
| Cumulative Months of Follow-Up | 15,624 |
| Number of Leads Active in Study | 6 |

USA Returned Product Analysis

| | |
|--------------------|---|
| Conductor Fracture | 4 |
| Crimp Weld Bond | 0 |
| Insulation Breach | 1 |
| Other | 0 |

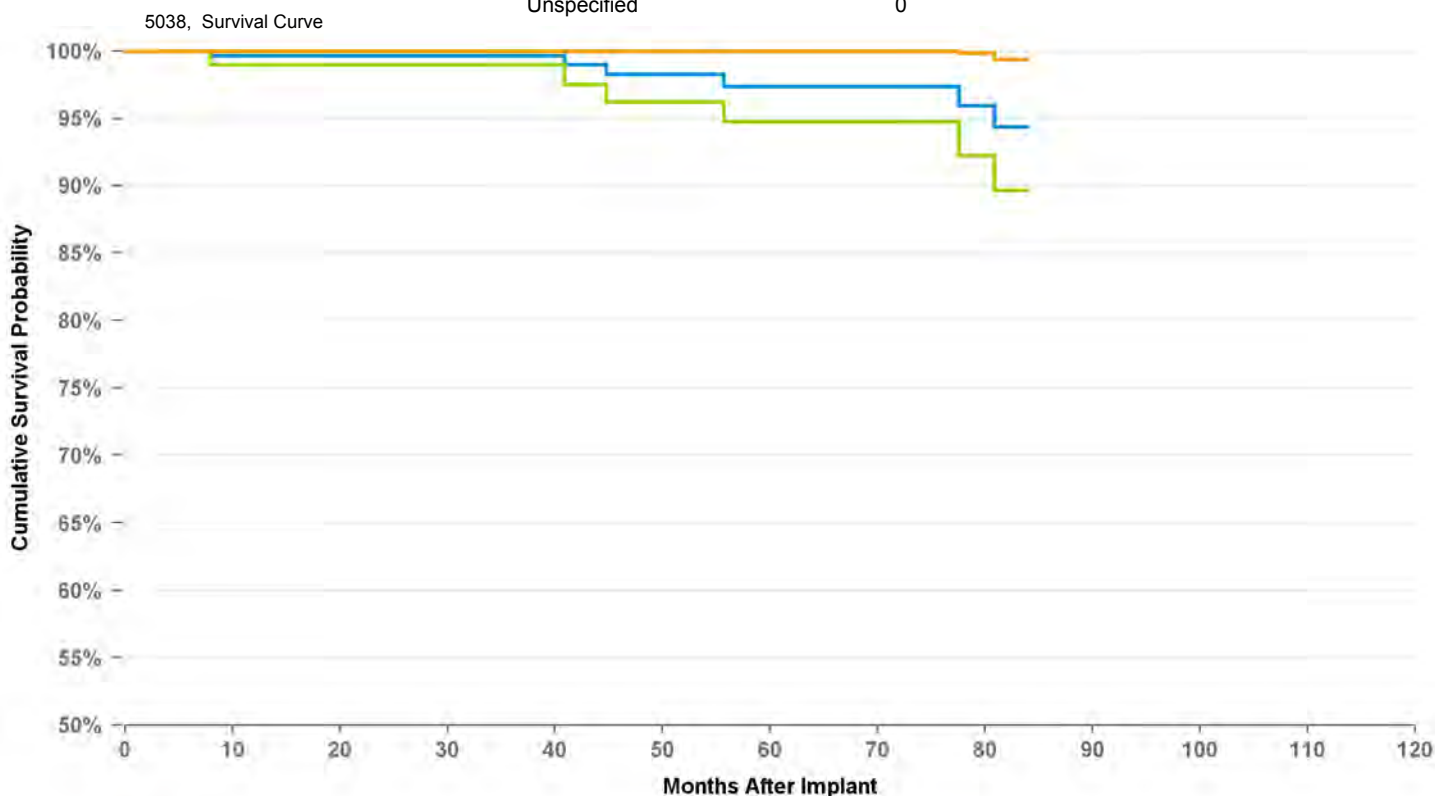

Graph Name

■ Cumulative Survival Probability Graph ■ Lower 95 Pct Confidence Graph ■ Upper 95 Pct Confidence Graph

| Years | 1 | 2 | 3 | 4 | 5 | 6 | at 84 mo |
|-------|-------|-------|-------|-------|-------|-------|----------|
| % | 99.7% | 99.7% | 99.7% | 98.2% | 97.4% | 97.4% | 94.4% |
| # | 289 | 219 | 161 | 130 | 106 | 77 | 55 |

ICD and CRT-D Charge Time Performance

Medtronic continues its commitment to providing updated information on charge time performance.

Introduction

Information on charge time performance of Medtronic products is presented in this section of the CRHF Product Performance Report. Medtronic implemented the collection of charge time data on July 1, 1999. The data are collected via our ongoing active clinical study of long-term system performance called the Product Surveillance Registry. The study protocol requests device data be routinely taken and sent to Medtronic at no more than 6-month intervals.


In our analysis performed for this report, only charge times resulting from full energy charges are considered. To ensure consistent reporting across devices, the charge time reported at implant represents the last charge time available from date of implant. When more than one charge time is available in a 6-month interval, a conservative approach has been adopted whereby only the maximum charge time in each 6-month interval is reported. As charge time is directly proportional to the time elapsed since the last capacitor reformation, charges occurring within 15 days of a previous charge are excluded. This precludes the reporting of overly optimistic results.

Data from over 20,000 devices contribute to the charge time data in this report. By tracking and reporting this charge time data, Medtronic is able to ascertain the actual performance of its charging circuitry. The insight gained through this information is applied to Medtronic's ongoing efforts to provide charge times that are short and consistent over the life of the product.

Charge time data for ICD and CRT-D models are presented using boxplots at 6-month intervals. The shaded box on the plots represents the middle half of the data – the Interquartile Range (IQR). The white line in the middle of each box is the median charge time. The top of the box representing the IQR is the third quartile or the 75th percentile (i.e., 75% of all charge times fall below this line), whereas the bottom of the box represents the first quartile or the 25th percentile. Vertical lines are drawn from the quartiles to the farthest value not more than 1.5 times the interquartile range. Any values more extreme than the vertical lines are considered outliers.


7230 Charge Time

| Model Number | Brand |
|--------------|------------|
| 7230B | Marquis VR |
| 7230Cx | Marquis VR |
| 7230E | Marquis VR |

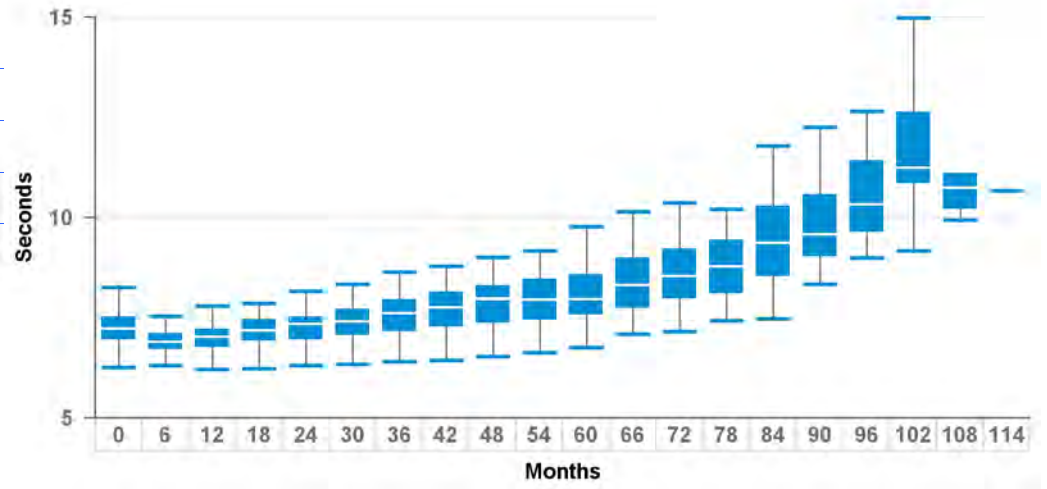


7231 Charge Time

| Model Number | Brand |
|--------------|------------|
| 7231Cx | GEM III VR |

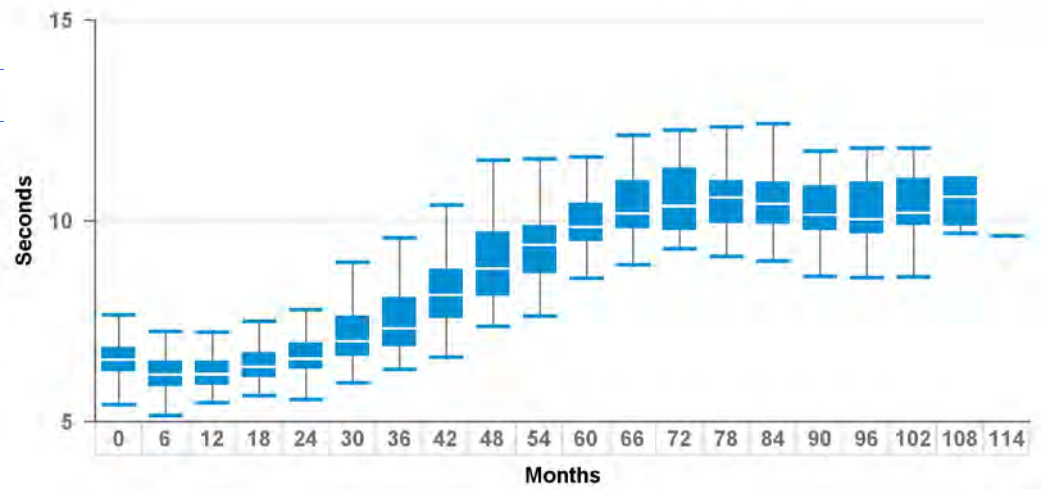


7232 Charge Time

| Model Number | Brand |
|--------------|-----------|
| 7232B | Maximo VR |
| 7232Cx | Maximo VR |
| 7232E | Maximo VR |

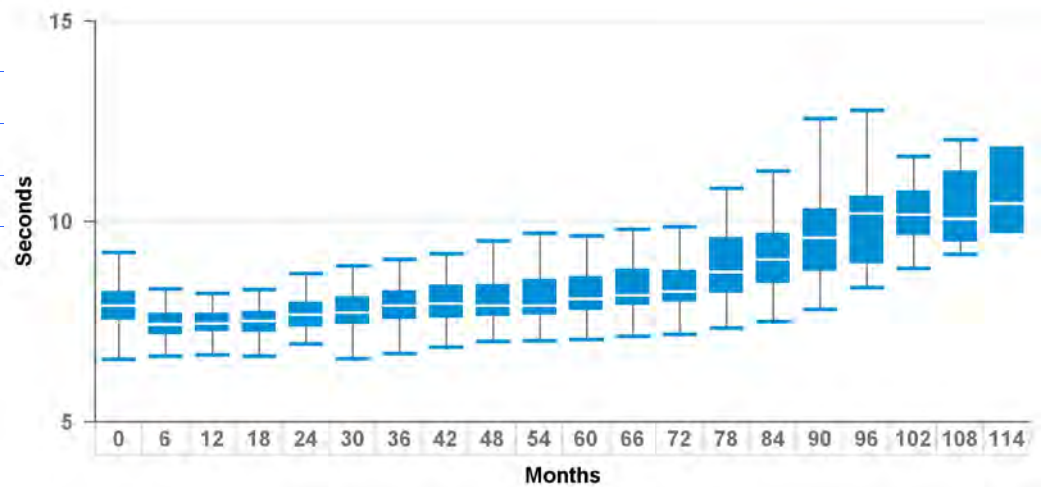


7274 Charge Time

| Model Number | Brand |
|--------------|------------|
| 7274 | Marquis DR |

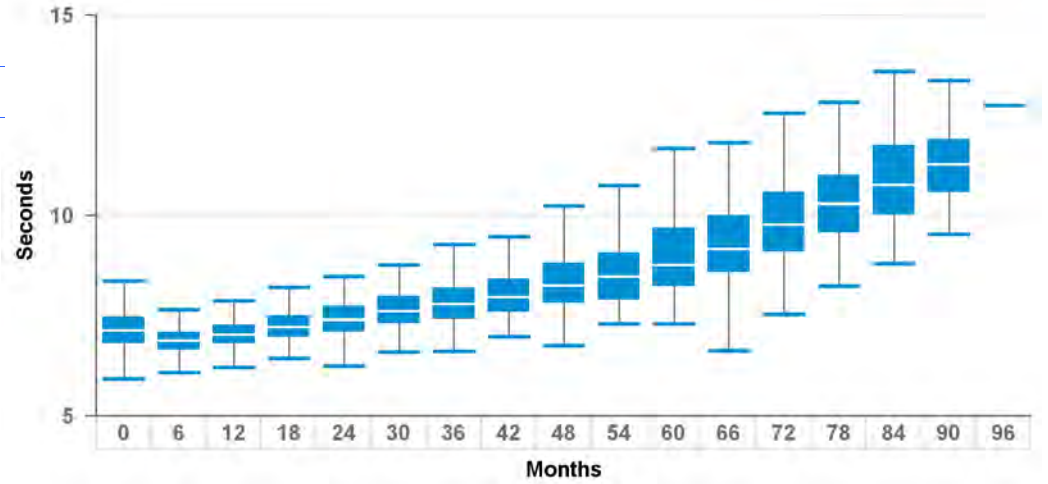

7278 Charge Time

| Model Number | Brand |
|--------------|-----------|
| 7278 | Maximo DR |

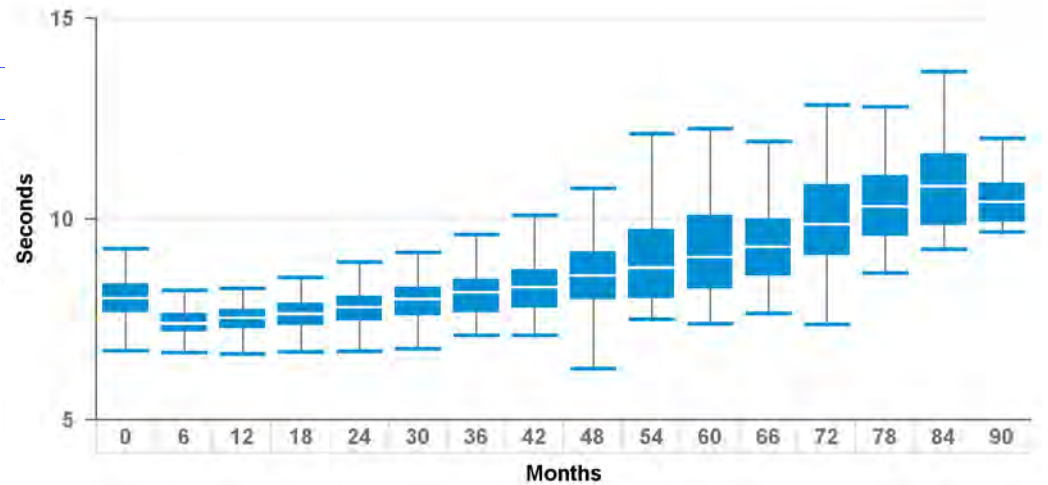


7285, 7295 Charge Time

| Model Number | Brand |
|--------------|--------------------|
| 7285 | InSync III Protect |
| 7295 | InSync II Protect |




7288 Charge Time

| Model Number | Brand |
|--------------|-----------|
| 7288 | Intrinsic |

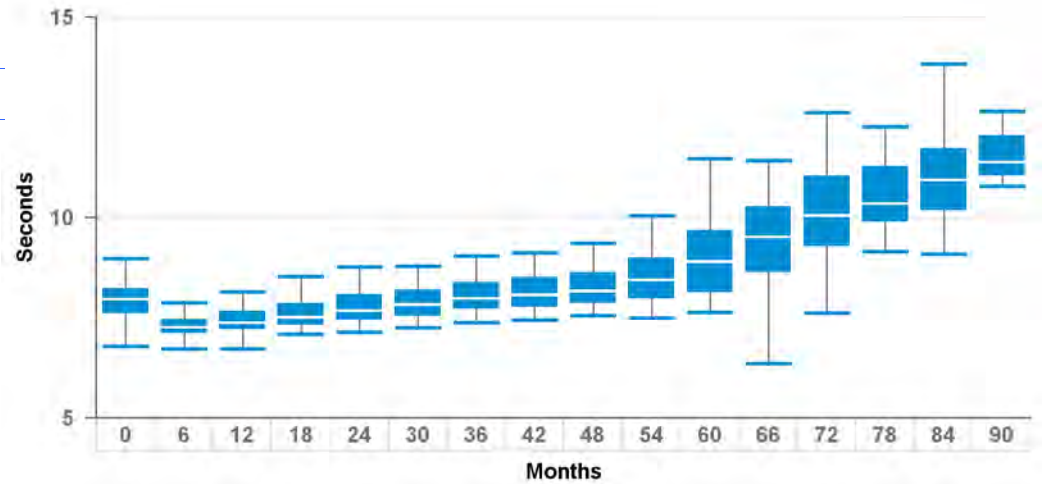


7299 Charge Time

| Model Number | Brand |
|--------------|---------------|
| 7299 | InSync Sentry |

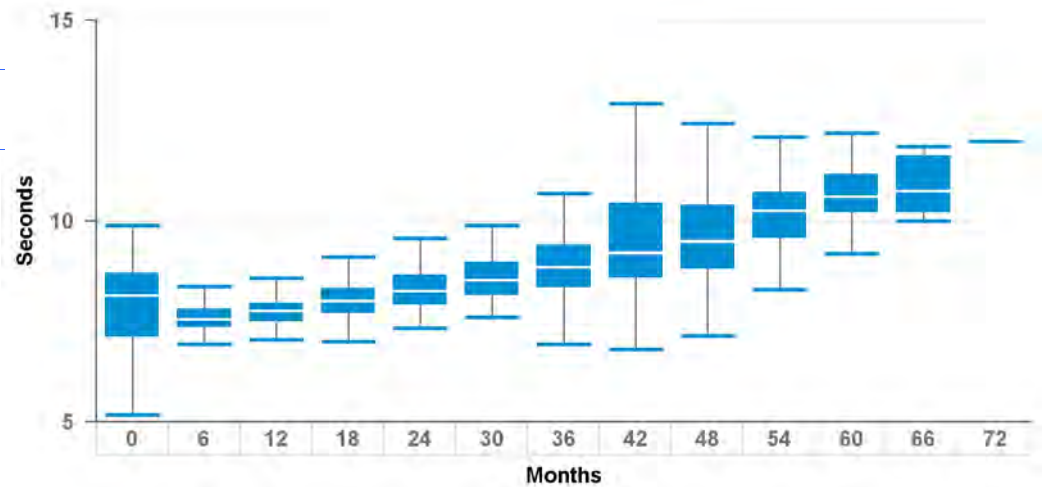


7304 Charge Time

| Model Number | Brand |
|--------------|---------------|
| 7304 | InSync Maximo |

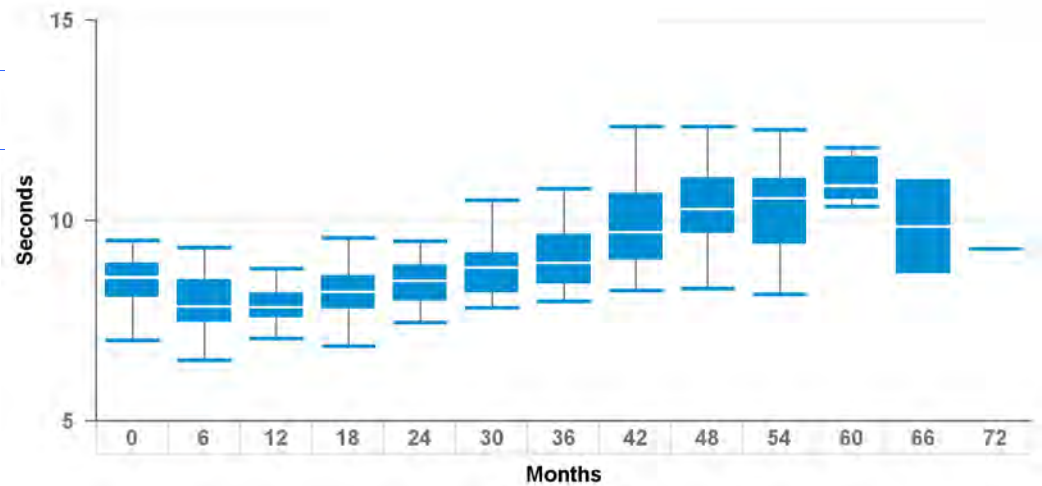


BLACKWELL, CRT-D Charge Time

| Model Number | Brand |
|--------------|--------------|
| DTBA1D1 | Viva XT |
| DTBA1D4 | Viva XT |
| DTBA1Q1 | Viva Quad XT |
| DTBA1QQ | Viva Quad XT |
| DTBA2D1 | Viva XT |
| DTBA2D4 | Viva XT |
| DTBA2Q1 | Viva Quad XT |
| DTBA2QQ | Viva Quad XT |
| DTBB1D1 | Viva S |
| DTBB1D4 | Viva S |
| DTBB1Q1 | Viva Quad S |
| DTBB1QQ | Viva Quad S |
| DTBB2D1 | Viva S |
| DTBB2D4 | Viva S |
| DTBB2QQ | Viva Quad S |
| DTBC2D1 | Brava |
| DTBC2D4 | Brava |
| DTBC2Q1 | Brava Quad |
| DTBC2QQ | Brava Quad |

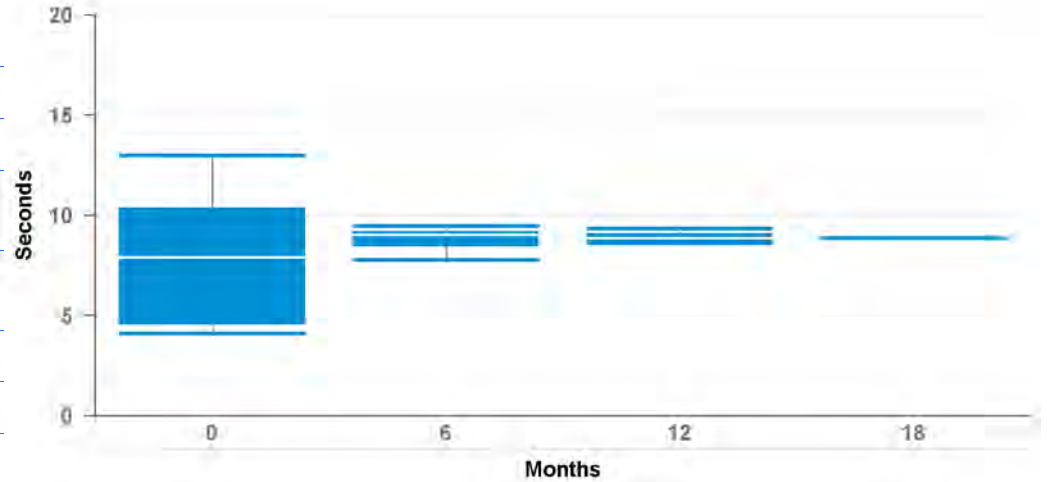


C154DWK, C164AWK, C174AWK Charge Time

| Model Number | Brand |
|--------------|----------------|
| C154DWK | Concerto CRT-D |
| C164AWK | Concerto CRT-D |
| C174AWK | Concerto CRT-D |

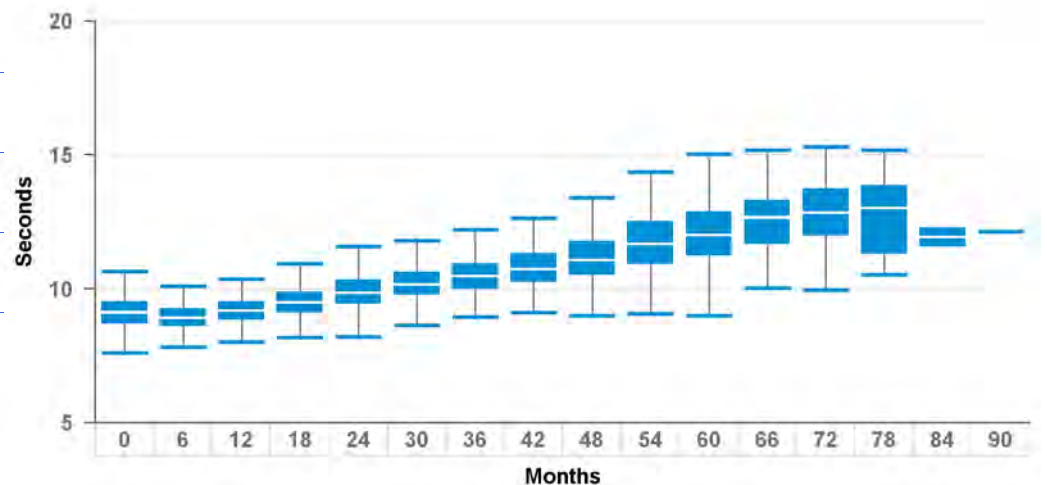


D144DRG, D154ATG, D154DRG Charge Time

| Model Number | Brand |
|--------------|----------------|
| D144DRG | Entrust Escudo |
| D154ATG | Entrust AT |
| D154DRG | Entrust DR |

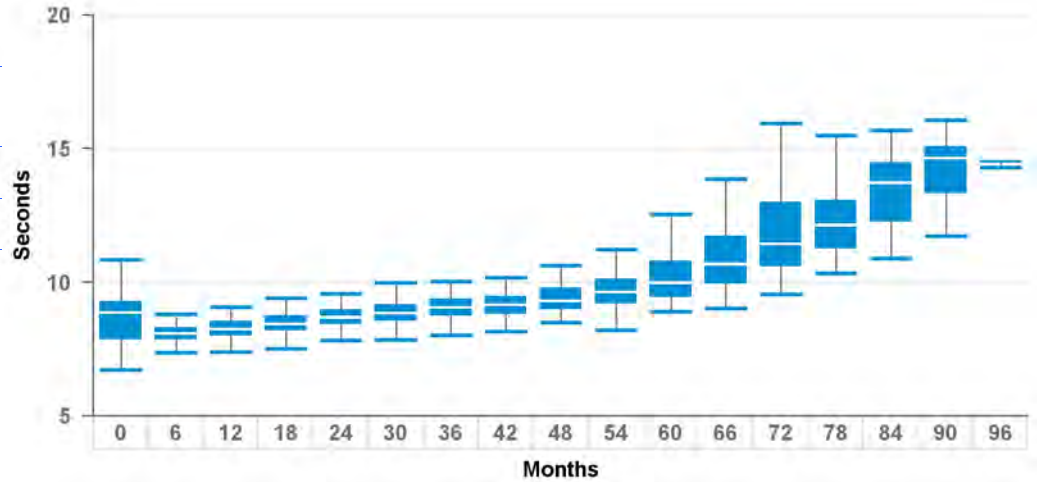


D144VRC, D154VRC Charge Time

| Model Number | Brand |
|--------------|----------------|
| D144VRC | Entrust Escudo |
| D154VRC | Entrust VR |

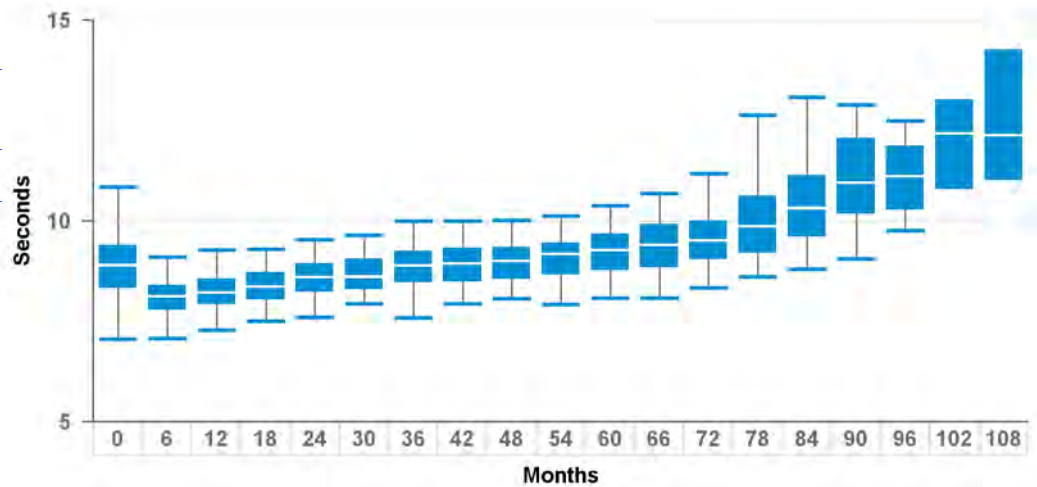


D154AWG, D164AWG Charge Time

| Model Number | Brand |
|--------------|-------------|
| D154AWG | Virtuoso DR |
| D164AWG | Virtuoso DR |

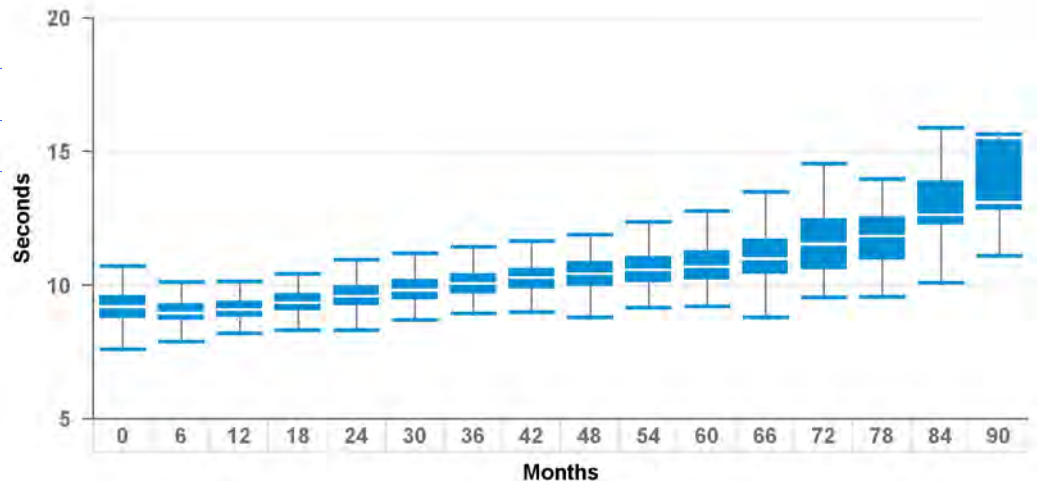


D154VWC, D164VWC Charge Time

| Model Number | Brand |
|--------------|-------------|
| D154VWC | Virtuoso VR |
| D164VWC | Virtuoso VR |

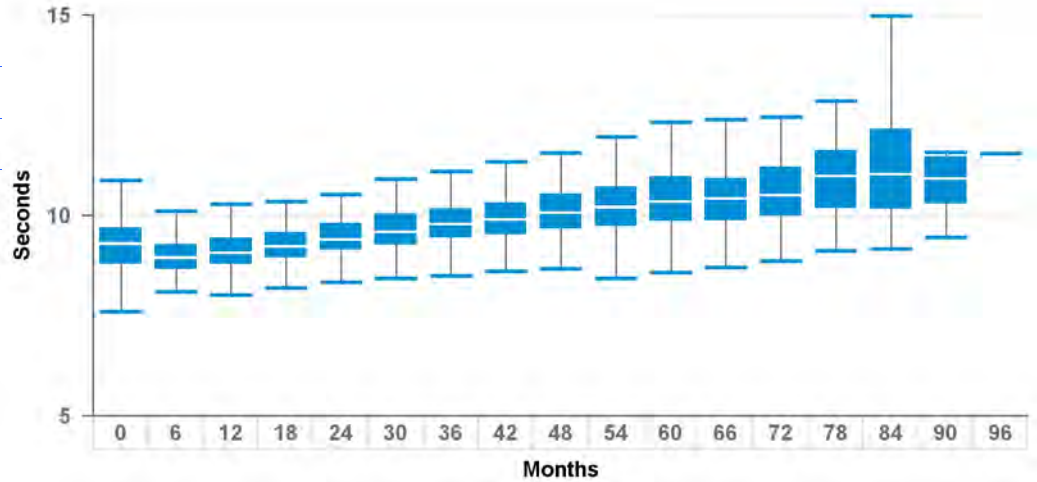


D204DRM, D214DRM, D224DRG, D234DRG Charge Time

| Model Number | Brand |
|--------------|-----------|
| D204DRM | Secura DR |
| D214DRM | Secura DR |
| D224DRG | Secura DR |
| D234DRG | Secura DR |

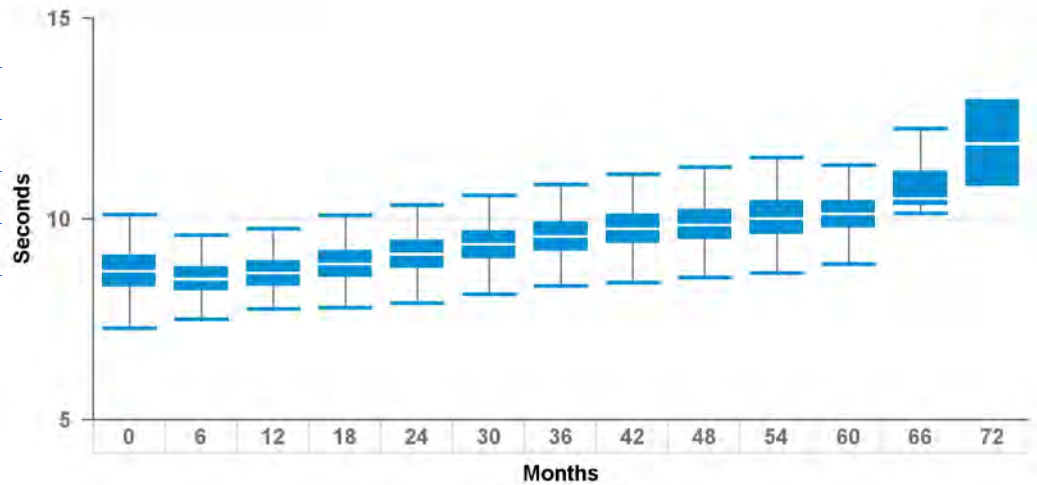


D204TRM, D214TRM, D224TRK, D234TRK Charge Time

| Model Number | Brand |
|--------------|----------------|
| D204TRM | Consulta CRT-D |
| D214TRM | Consulta CRT-D |
| D224TRK | Consulta CRT-D |
| D234TRK | Consulta CRT-D |

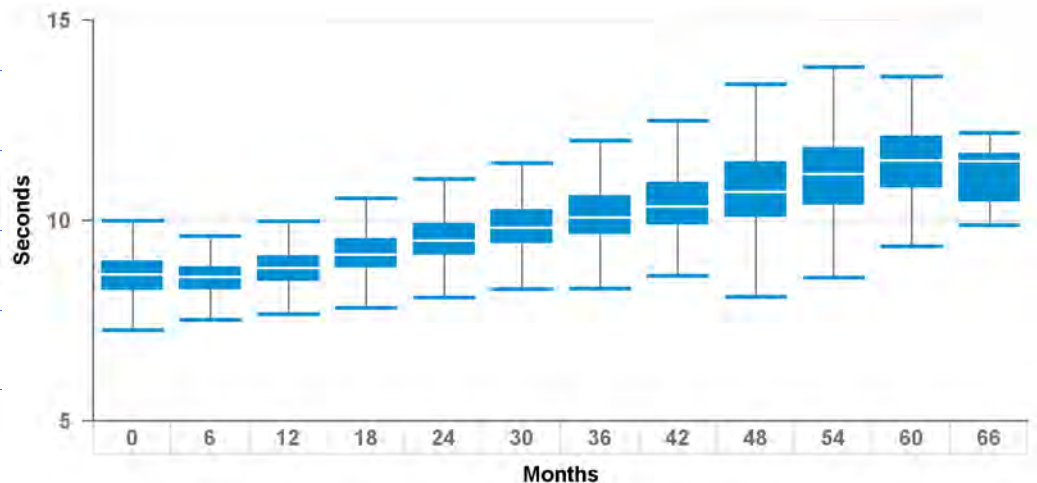


D204VRM, D214VRM, D224VRC, D234VRC Charge Time

| Model Number | Brand |
|--------------|-----------|
| D204VRM | Secura VR |
| D214VRM | Secura VR |
| D224VRC | Secura VR |
| D234VRC | Secura VR |

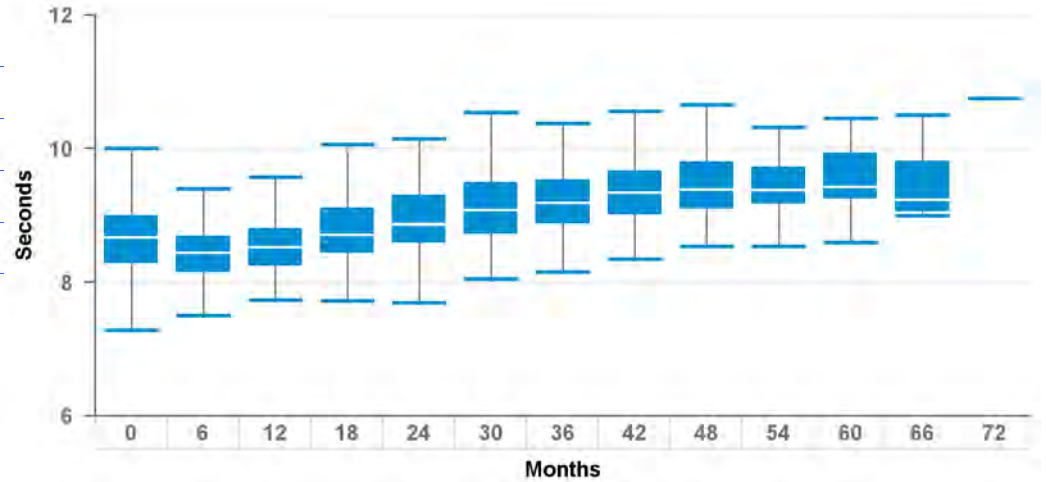


D264DRG, D284DRG, D384DRx, D394DRx Charge Time

| Model Number | Brand |
|--------------|--------------|
| D264DRM | Maximo II DR |
| D284DRG | Maximo II DR |
| D384DRG | Cardia DR |
| D394DRG | Egida DR |

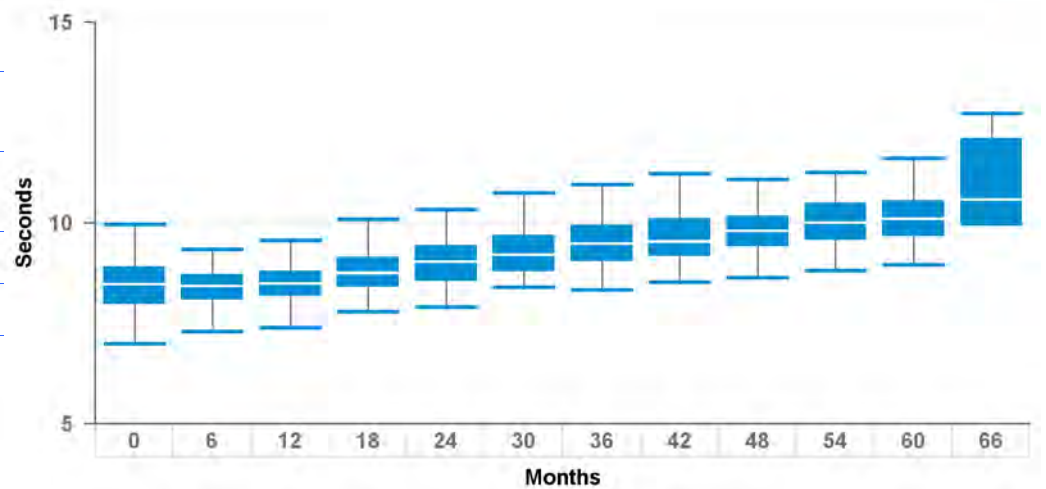


D264TRM, D284TRK, D384TRx, D394TRx Charge Time

| Model Number | Brand |
|--------------|-----------------|
| D264TRM | Maximo II CRT-D |
| D284TRK | Maximo II CRT-D |
| D384TRG | Cardia CRT-D |
| D394TRG | Egida CRT-D |

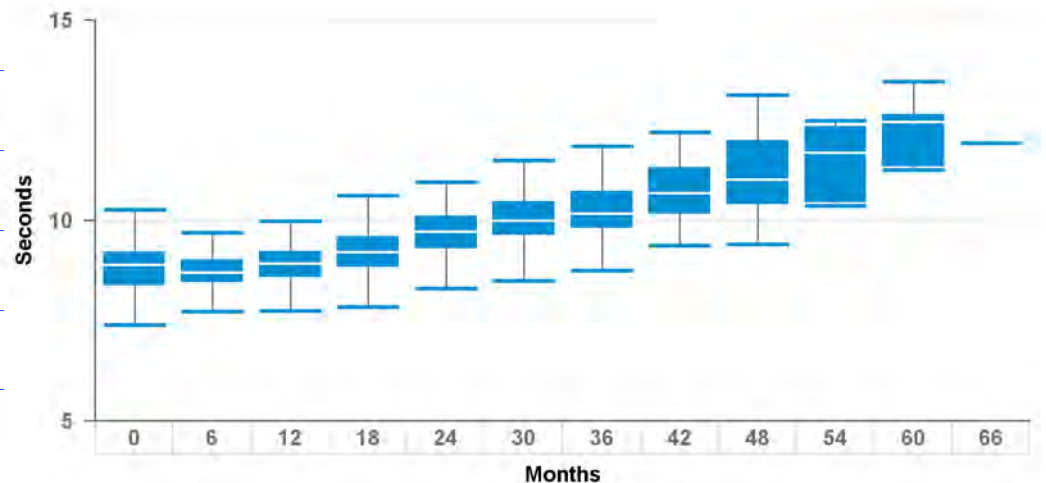


D264VRM, D284VRC, D384VRx, D394VRx Charge Time

| Model Number | Brand |
|--------------|--------------|
| D264VRM | Maximo II VR |
| D284VRC | Maximo II VR |
| D384VRG | Cardia VR |
| D394VRG | Egida VR |

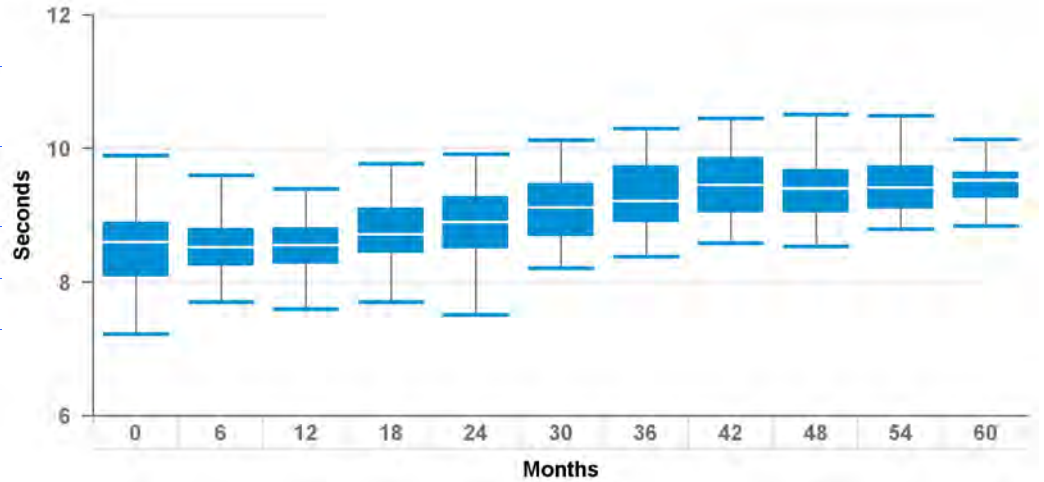


D274DRG, D294DRG Charge Time

| Model Number | Brand |
|--------------|----------------|
| D274DRG | Virtuoso II DR |
| D294DRG | Virtuoso II DR |

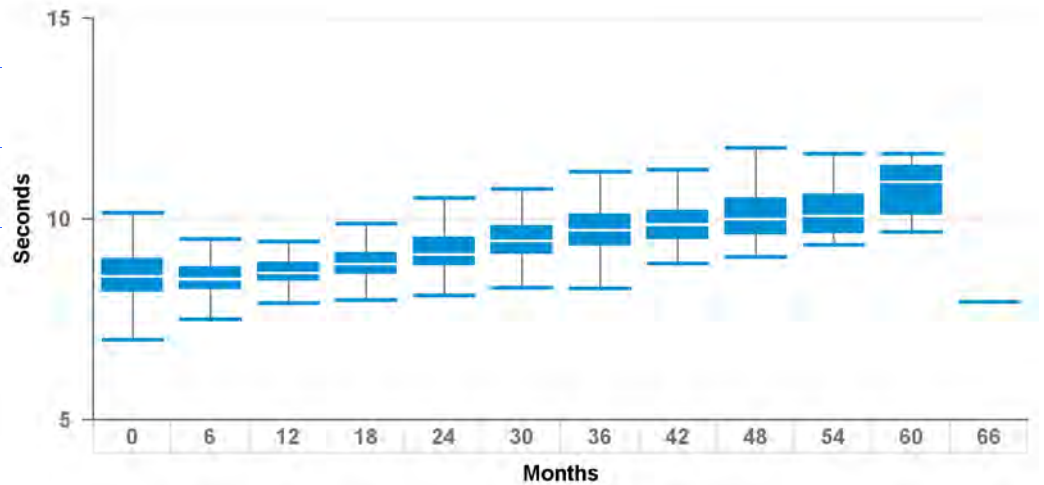


D274TRK, D294TRK Charge Time

| Model Number | Brand |
|--------------|-------------------|
| D274TRK | Concerto II CRT-D |
| D294TRK | Concerto II CRT-D |

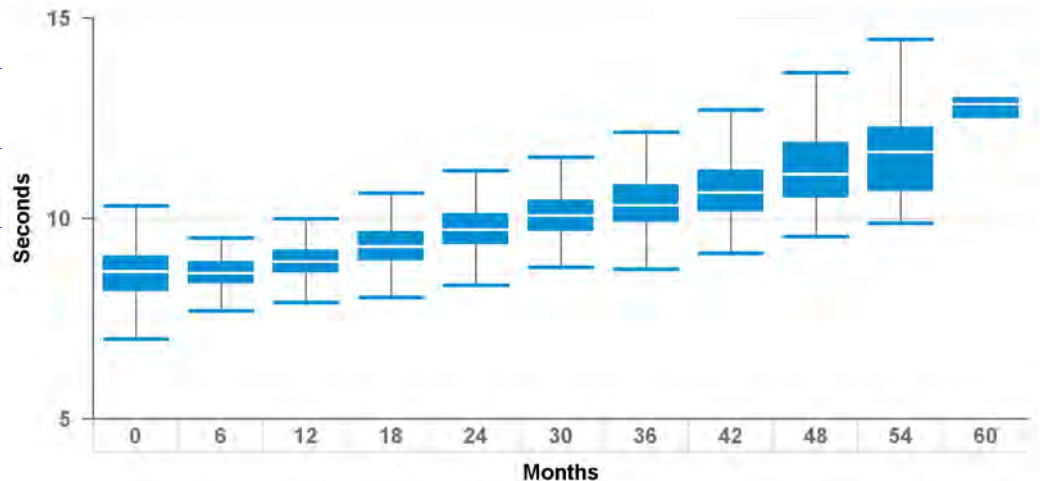


D274VRC, D294VRC Charge Time

| Model Number | Brand |
|--------------|----------------|
| D274VRC | Virtuoso II VR |
| D294VRC | Virtuoso II VR |

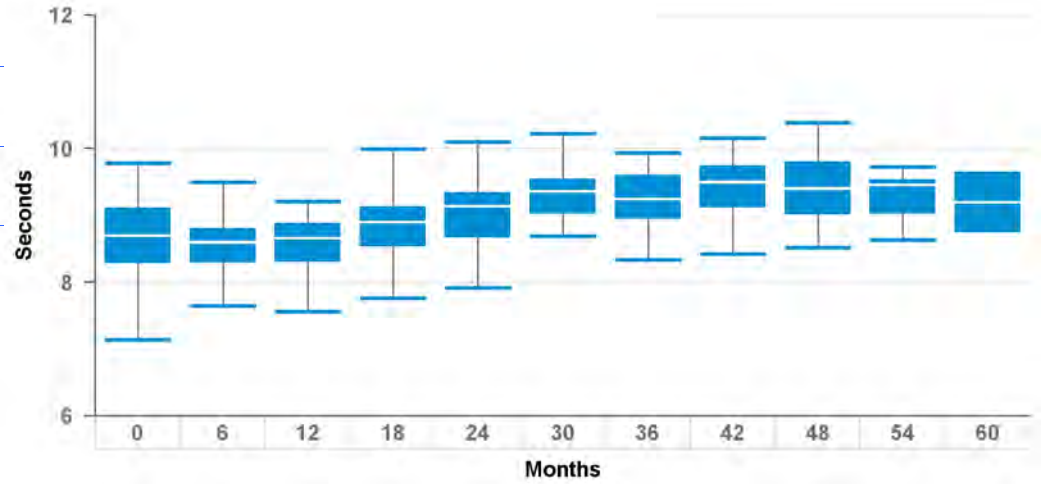


D314DRx Charge Time

| Model Number | Brand |
|--------------|----------------|
| D314DRG | Protecta XT DR |
| D314DRM | Protecta XT DR |

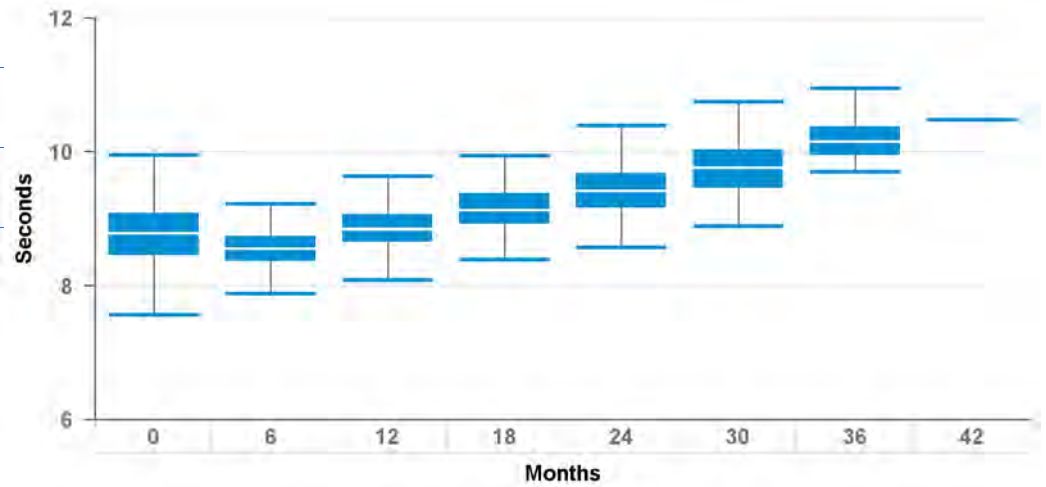


D314TRx Charge Time

| Model Number | Brand |
|--------------|-------------------|
| D314TRG | Protecta XT CRT-D |
| D314TRM | Protecta XT CRT-D |

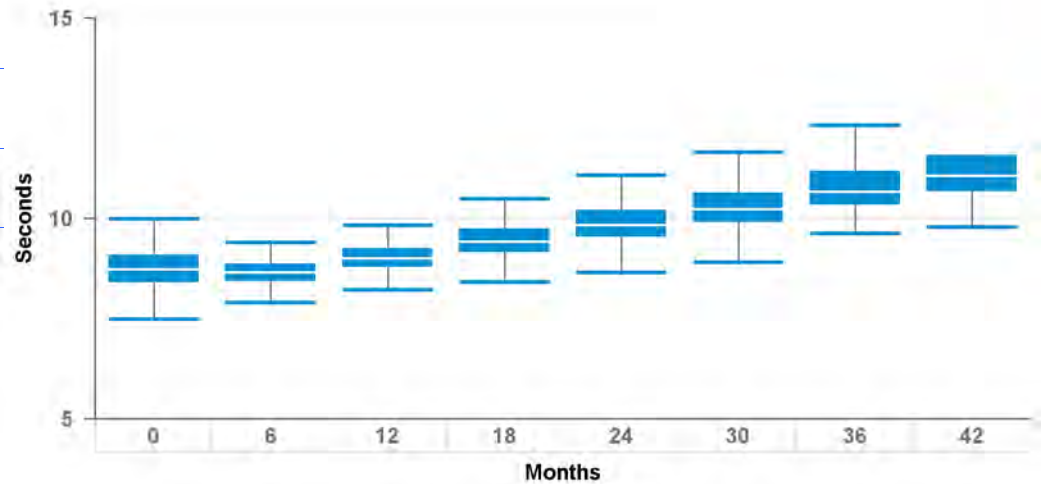


D314VRx Charge Time

| Model Number | Brand |
|--------------|----------------|
| D314VRG | Protecta XT VR |
| D314VRM | Protecta XT VR |

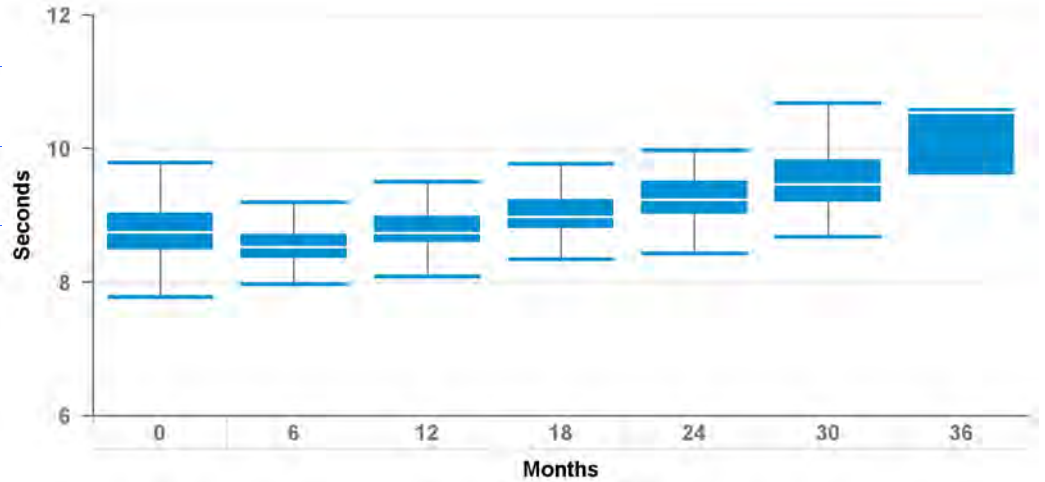


D334DRx, D364DRx Charge Time

| Model Number | Brand |
|--------------|-------------|
| D334DRG | Protecta DR |
| D334DRM | Protecta DR |
| D364DRG | Protecta DR |
| D364DRM | Protecta DR |

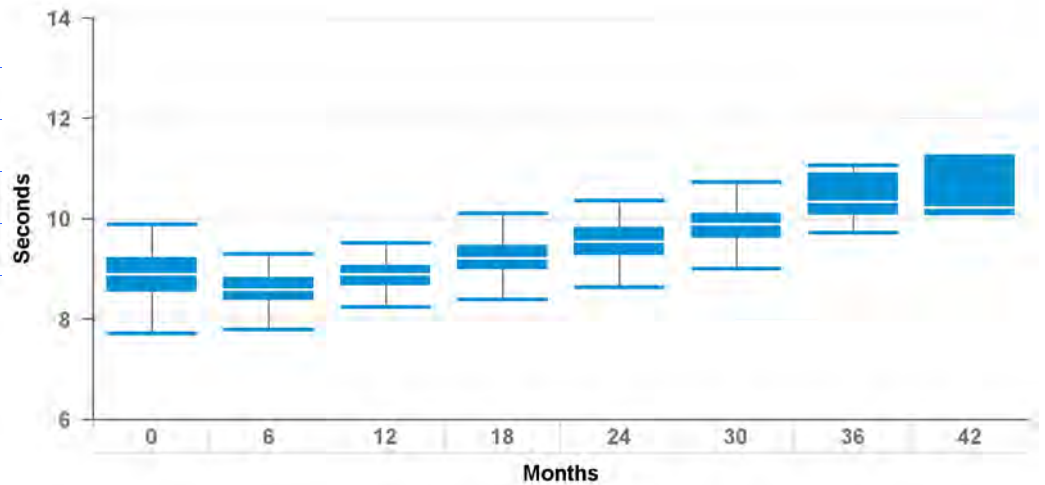


D334TRx, D364TRx Charge Time

| Model Number | Brand |
|--------------|----------------|
| D334TRG | Protecta CRT-D |
| D334TRM | Protecta CRT-D |
| D364TRG | Protecta CRT-D |
| D364TRM | Protecta CRT-D |

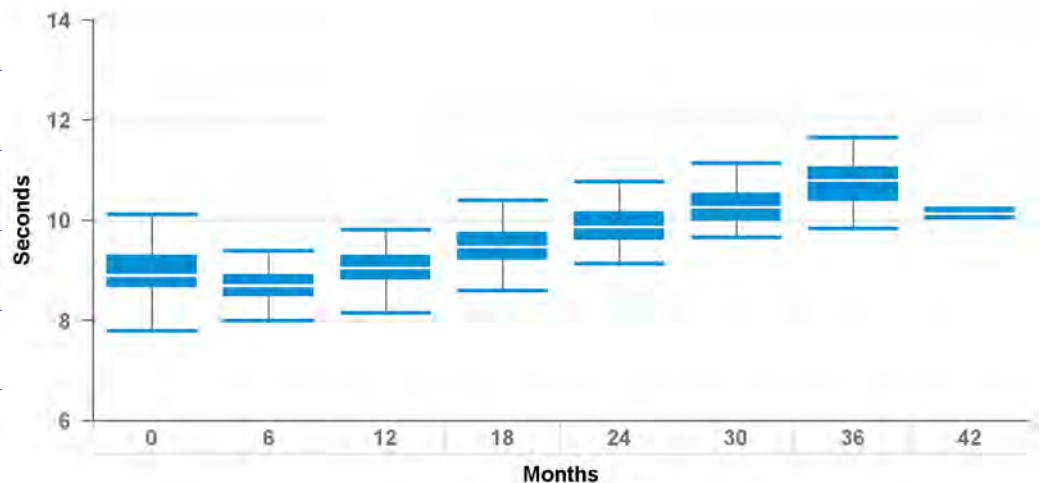


D334VRx, D364VRx Charge Time

| Model Number | Brand |
|--------------|-------------|
| D334VRG | Protecta VR |
| D334VRM | Protecta VR |
| D364VRG | Protecta VR |
| D364VRM | Protecta VR |

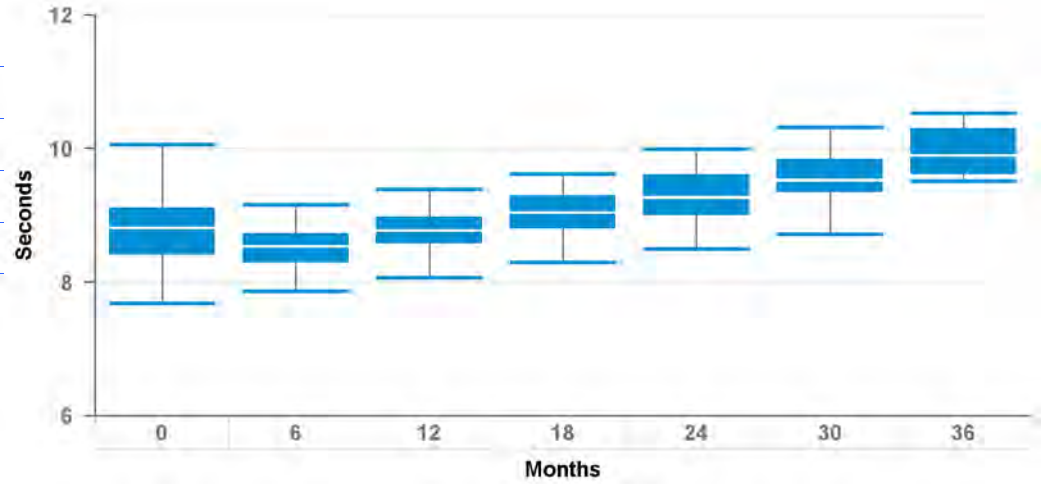


D354DRx Charge Time

| Model Number | Brand |
|--------------|----------------|
| D354DRG | Protecta XT DR |
| D354DRM | Protecta XT DR |

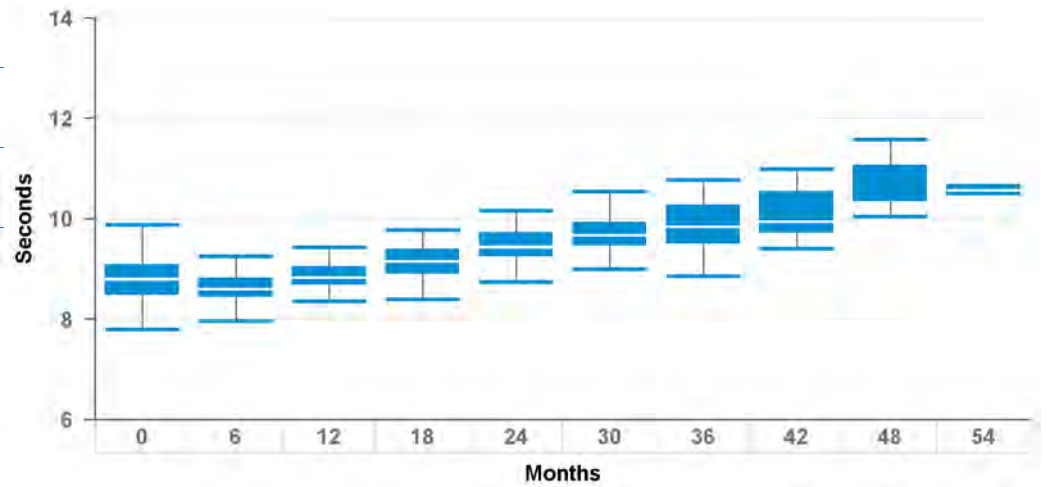


D354TRx Charge Time

| Model Number | Brand |
|--------------|-------------------|
| D354TRG | Protecta XT CRT-D |
| D354TRM | Protecta XT CRT-D |

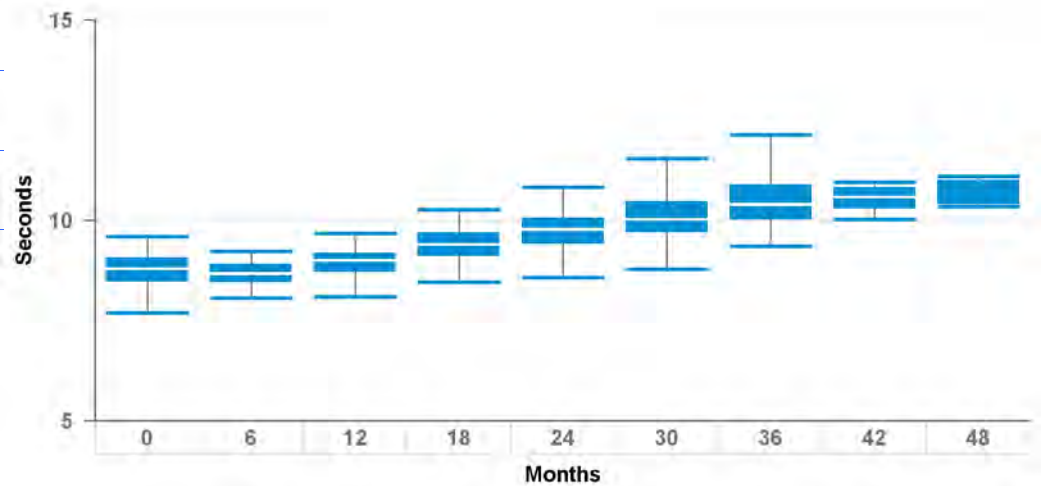

D354VRx Charge Time

| Model Number | Brand |
|--------------|-------------------|
| D354VRG | Protecta XT VR |
| D354VRM | Protecta XT VR |

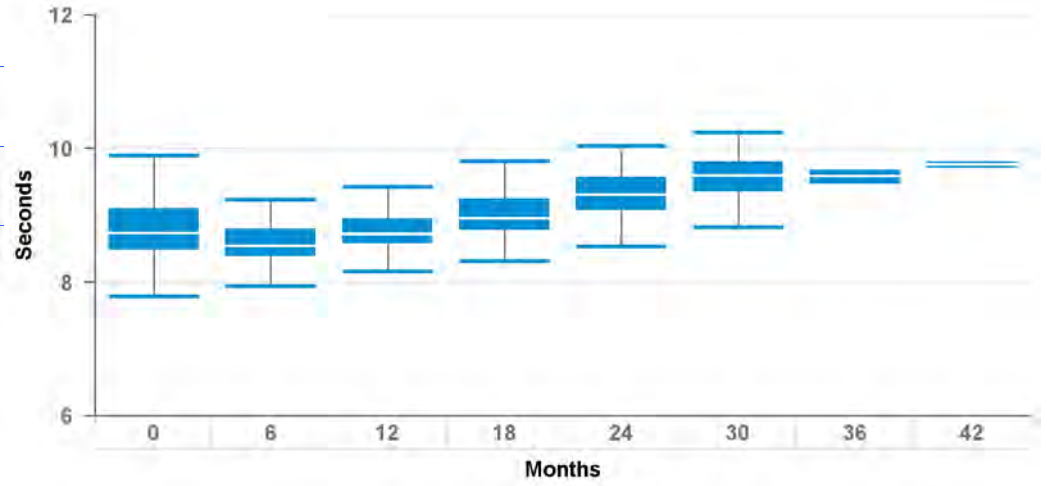

Advisories

Potential Loss Of Device Hermeticity

Consulta® CRT-P and Syncra® CRT-P Original Date of Advisory: June 2013

Product

Consulta® CRT-P and Syncra® CRT-P. Go to <http://wwwp.medtronic.com/productperformance/> to determine if a specific device is affected.

Advisory

Medtronic has identified an issue with a connector bracket weld on a subset of Consulta CRT-P models and Syncra CRT-P devices manufactured between April 1 and May 13, 2013. This type of connector bracket weld is unique to Consulta and Syncra CRT-P devices and no other Medtronic device models are affected.

An out-of-specification weld could result in a loss of device hermeticity and compromised device functionality. **There have been no reported or confirmed device failures or patient injuries.** Medtronic estimates the rate of out-of-specification welds to be 1-2% in this subset of devices.

Non-implanted devices from this subset have been recalled to Medtronic for re-inspection with additional controls to ensure that the weld meets specification. In June 2013, Medtronic communicated to impacted physicians that up to 779 devices worldwide (43 in the U.S.) may have been implanted from this subset. The Physician Letter is available at <http://www.medtronic.com/for-healthcare-professionals/consulta-syncracrt-p/index.htm>

Patient Management Recommendations (As of June 2013)

As a result of on-going investigation and consultation with Medtronic's Independent Physician Quality Panel, Medtronic offers the following patient management recommendations:

- Physicians should advise their patients to seek medical attention immediately if they experience a return of symptoms related to bradycardia or heart failure.
- If considering prophylactic device replacement for pacemaker-dependent patients with a device in the identified subset, physicians should carefully assess individual patient circumstances against the known risk of a device replacement.
- Physicians should continue routine follow up in accordance with standard practice

Status Update

As of January 31, 2015, 536 of the 779 devices have been returned from field inventory. Medtronic estimates the remaining 242 devices (44 in the U.S.) have been implanted. **There have been no reported or confirmed device failures or patient injuries.**

| Initial Affected Population | Number of Confirmed Advisory Related Events | Estimated Remaining Active Population | Current Malfunction Rate (confirmed malfunctions over total population) |
|---|--|---|---|
| Up to 779 Worldwide (44 United States) | 0 Worldwide (0 United States) | 190 Worldwide (37 United States) | 0% Worldwide (0% United States) |

Advisories

Potential Rapid Battery Depletion

EnTrust® VR/DR/AT ICDs

Original Date of Advisory: March 2012

Product

All EnTrust ICDs.

Advisory

A small percentage of EnTrust ICDs may not meet expected longevity or provide at least three months of device operation between the Elective Replacement Indicator (ERI) and End of Life (EOL) due to a more-rapid-than-expected drop in battery voltage. No patient deaths or serious injuries have been reported as a result of this issue.

The reported events have involved a drop in battery voltage from ~3.0 V to ERI (2.61 V) over a time period ranging from approximately one week to six months. All reported events have occurred at least 30 months after implant.

Medtronic has identified the cause of these occurrences to be an internal battery short that develops as the battery capacity is consumed. The Physician Letter is available at <http://www.medtronic.com/product-advisories/entrust/physician/index.htm>

Patient Management Recommendations (As of March 2012)

After consultation with Medtronic's Independent Physician Quality Panel, Medtronic offers the following patient management recommendations:

- Physicians should continue routine follow-up sessions at least every three months in accordance with product labeling.
- Physicians should program the audible patient alerts for "Low Battery Voltage ERI" and "Excessive Charge Time EOL" to ON.
- Physicians should replace devices promptly after they reach ERI if the decline in voltage is more rapid than expected.
- Prophylactic replacement of EnTrust ICDs is not recommended.

Status Update

As of January 31, 2015, there have been 91 confirmed events. No patient deaths have been reported due to this issue. No reports have been made of a failure to deliver high voltage therapy.

| Initial Affected Population | Number of Confirmed Advisory Related Events | Estimated Remaining Active Population | Current Malfunction Rate (confirmed malfunctions over total population) |
|--|--|--|---|
| 69,200 Worldwide (44,300 United States) | 91 Worldwide (71 United States) | 15,700 Worldwide (10,000 United States) | 0.13% Worldwide (0.16% United States) |

Advisories

Low Battery Voltage Displayed at Device Interrogation

EnRhythm and EnRhythm MRI Pacemakers

Original Date of Advisory: February 2010

Product

All EnRhythm and EnRhythm MRI pacemakers.

Original Advisory Information (February 2010)

Two specific battery issues with EnRhythm pacemakers were identified. The risks to patients for both issue have been addressed by a Medtronic software update. The Physician Letter is available at <http://www.medtronic.com/enrhythm-advisory/physician.html>

First Issue

In February 2010, Medtronic had received 62 reports (out of approximately 110,000 devices worldwide) indicating that the battery voltage at device interrogation was lower than the battery voltage that is tracked by the device to provide data for the elective replacement indicator (ERI) notification.

Medtronic's investigation found that none of these reports resulted in loss of therapy. Importantly, the original ERI notification, which uses the nightly battery voltage measurement, was unaffected and accurate. Medtronic identified the root cause as higher than expected battery impedance.

Medtronic's internal testing showed there was no current risk for compromised therapy delivery. If the software update referenced above is not implemented, there will be a potential risk of loss of device functionality in a small percent (less than 0.08% 6 years post-implant) of devices. The software update obviates this risk.

Second Issue

Through internal accelerated testing, Medtronic identified a second issue that projects battery voltage could decrease sooner than expected due to a slightly increased rate of lithium depletion near end of device life. This issue has not been clinically observed and is not expected to occur until approximately 9 years post-implant. If the software update referenced above is not implemented, there may be a potential risk for loss of therapy at or near ERI in a small number of devices. The software eliminates this issue by changing ERI criteria.

Software Update (As of October 2010)

The battery issues described above and subsequent software update are summarized in the table below. When a device receives the software update, if battery impedance is greater than the new ERI threshold ERI will be triggered shortly thereafter. Therefore, clinicians may observe an ERI/EOL indicator at the next patient follow-up. When ERI is triggered by battery impedance, additional battery capacity remains and can support device function at ERI parameters for at least one year. Medtronic is not aware of any reports of loss of therapy due to this issue.

As a reminder, when ERI is triggered, EnRhythm devices revert to VVI pacing at 65 ppm at the programmed output settings. EOL is declared 90 days after ERI or at a battery voltage of 2.69V, whichever comes sooner.

Advisories

| Battery Issue | Software Update |
|---|---|
| Battery voltage could decrease sooner than expected due to a slightly increased rate of lithium depletion | Changed ERI battery voltage threshold from 2.59V to 2.81V to ensure 90 days of therapy from ERI to EOL |
| Higher than expected battery impedance | <p>Added a secondary ERI trigger based on battery impedance. This new criteria will identify devices with increased battery impedance before device performance is impacted.</p> <p>If triggered, displayed battery voltage is reset to 2.81 V to ensure alignment with ERI battery voltage threshold</p> |

Updated Performance Information (as of August 2011)

We now have access to battery impedance and ERI performance on more than 5000 EnRhythm devices that have received the EnRhythm software update. Our modeling based on these data shows that approximately 6-10% of devices will reach ERI within 5 years post-implant. Consistent with our previous communications, we continue to expect average device longevity to be reduced by approximately 10 –15%, with the expected average longevity remaining at 8.5 to 10.5 years, depending on device settings.

Updated Patient Management Recommendations (as of August 2011)

After consultation with Medtronic's Independent Physician Quality Panel, we recommend:

- Performing a device follow-up within 90 days after the software download to identify devices that triggered ERI shortly after the software update. Subsequent follow up can be performed per standard practice. During programmer interrogation of a device at ERI, there is a slight possibility a transient drop in pacing amplitude could occur. If this is noted, either remove the programmer head or temporarily program to a higher output voltage.
- If an unanticipated ERI/EOL is declared, it is likely due to battery impedance. In such cases, additional battery capacity remains and can support device function at ERI parameters for at least one year. However, when ERI or EOL (typically 90 days after ERI) declaration is seen, schedule device replacement.

Status Update

First Issue

Included in the August 2011 Performance Update was information about the projected percentage of devices that would encounter an early ERI due to unexpected high battery impedance. As of January 31, 2015, percentage of devices that encountered ERI due to battery impedance has not exceeded the rate of 6-10% within 5 years of post-implant as communicated with our August 2011 Performance Update. Only devices using the updated software can trigger ERI due to impedance.

| Initial Affected Population | Number of Confirmed ERIs due to impedance | Number of Confirmed ERIs due to impedance within 5 years post-implant | Estimated ERI rate due to impedance within 5 years post-implant ² | Confirmed events of loss of therapy due to battery impedance | Estimated Remaining Active Population |
|---|---|---|--|--|---------------------------------------|
| All EnRhythm pacemakers (146,500 Worldwide) | 13,690 Worldwide | 5,103 | 5.5% | 0 | 65,400 Worldwide |

Advisories

Second Issue

| Initial Affected Population | Number of Events of Loss of Therapy Due to Increased Rate of Lithium Depletion | Estimated Remaining Active Population |
|---|--|---------------------------------------|
| All EnRhythm pacemakers (146,500 Worldwide) | 0 Worldwide | 65,400 Worldwide |

¹The 8.5 year estimate represents a high use scenario (DDD, 100% pacing in atrium and ventricle with 3.0 V output in both chambers). The 10.5 year estimate represents a typical use scenario for a sinus node dysfunction patient with the MVP function ON (AAI(R) \Leftrightarrow DDD(R), 50% pacing in atrium and 5% pacing in ventricle with 3.0 V output in both chambers). Projections are based on modeling and not actual field returns, due to limited availability of implant experience beyond 6 years. Field performance will continue to be monitored and modeling updated to reflect actual data.

²Accounts for underreporting of impedance ERIs based on the fraction of replaced devices in the U.S. registration system that are subsequently returned.

Advisories

Potential Separation of Interconnect Wires (2009)

Kappa 600/700/900 and Sigma 100/200/300 Pacemakers Original Date of Advisory: May 2009

Product

A specific subset of Kappa and Sigma series pacemakers may fail due to separation of interconnect wires from the hybrid circuit. You may use the "Search for Information by Serial Number" tool at <http://wwwp.medtronic.com/productperformance/> to determine if a specific device is affected. The Physician Letter is available at <http://www.medtronic.com/kappasigma/physician.html>

Advisory Population

Specific subsets of Kappa and Sigma series pacemakers may fail at a higher than expected rate due to separation of wires that connect the electronic circuit to other pacemaker components (e.g., battery, connector). This may present clinically as loss of rate response, premature battery depletion, loss of telemetry, or no output.

Some patients, whose devices experience a wire separation resulting in a loss of pacing output, will experience a return of bradycardia symptoms (e.g., fainting or lightheadedness). In rare cases involving pacemaker dependent patients, loss of pacing output may result in death or serious injury.

Since 1997, there have been over 1.7 million Kappa and Sigma devices implanted worldwide. . At the time of the original advisory communication, an estimated 15,200 Kappa and 6,100 Sigma devices affected by the advisory remained implanted and active. These devices were manufactured primarily between November 2000 and November 2002. Most of these devices have been implanted in patients for five years or longer and may be nearing normal elective replacement time.

There is no provocative testing that can predict which specific devices may fail, and no device programming can mitigate this issue if it occurs.

Patient Management Recommendations

We realize that each patient requires unique clinical consideration and we support your judgment in caring for your patients. After consultation with Medtronic's Independent Physician Quality Panel, Medtronic offers the following recommendations for patients:

- Physicians should advise their patients to seek medical attention immediately if they experience symptoms (e.g., fainting or lightheadedness).
- Physicians should consider device replacement for patients who are both pacemaker dependent and who have been implanted with a device in the affected subsets. Medtronic will offer a supplemental device warranty if the device is not already at elective replacement time.
- Physicians should continue routine follow-up in accordance with standard practice for those patients who are not pacemaker dependent.

Status Update

Advisory Population

Patient management recommendations remain unchanged. As of January 31, 2015, Medtronic has observed 459 Kappa devices and 309 Sigma devices with this failure mechanism from the Kappa and new Sigma device subsets. This represents 0.79% (Kappa) and 2% (Sigma) of the original affected implant population.

Advisories

Four hundred twenty-two (422) of the Kappa devices (0.72%) and 241 of the Sigma devices (1.60%) were returned with information indicating a problem with the patient's pacing system prior to explant. The remaining 37 Kappa devices (0.06%) and 68 Sigma devices (0.45%) were returned with no information indicating a potential malfunction while implanted or with insufficient information to determine the state of the device at explant. Lacking definite information indicating proper operation until explant, these remaining devices are conservatively categorized as having experienced interconnect wire separation while implanted.

As of May 2009, our modeling predicts failure rates due to this issue of 1.1% (Kappa) and 4.8% (Sigma) over the remaining lifetime of those pacemakers still in service at that time.

Out of the initial advisory population of 58,300 Kappa devices and 14,900 Sigma devices worldwide, approximately 300 Sigma devices remain implanted worldwide. Of these, less than 100 Sigma devices are in the United States.

Continued Vigilance

Included in the advisory communication was information about an additional subset of Kappa devices where we have observed a much lower rate of occurrence of this issue. We estimate that none of these devices remain active.

| Initial Affected Population | Number of Confirmed Advisory Related Events | Estimated Remaining Active Population | Current Malfunction Rate (confirmed malfunctions over total population) | Predicted Malfunction Rate Over the Remaining Life of the Devices Still Implanted |
|---|--|---|---|---|
| Kappa Pacemakers | | | | |
| 58,300 Implanted Worldwide (est.) (17,600 United States) | 410 Worldwide (211 United States) with information indicating a clinical presentation. An additional 36 worldwide (24 US) without information indicating a clinical presentation or with insufficient information to determine the state of the device at explant. | No active population remains | 0.70% Worldwide (1.19% United States) | N/A |
| Sigma Pacemakers | | | | |
| 14,900 Implanted Worldwide (est.) (3,700 United States) | 241 Worldwide (52 United States) with information indicating a clinical presentation. An additional 68 worldwide (17 US) without information indicating a clinical presentation or with insufficient information to determine the state of the device at explant. | 300 Worldwide (< 100 United States) | 2% Worldwide (1.6% United States) | 4.8% |

Advisories

Potential Conductor Wire Fracture

6930, 6931, 6948, 6949 Sprint Fidelis Defibrillation Leads Original Date of Advisory: October 2007

Product

All Model 6930, 6931, 6948, and 6949 implantable defibrillation leads.

Advisory

There are two primary locations where chronic conductor fractures have occurred on Sprint Fidelis leads: 1) the distal portion of the lead, affecting the anode (ring electrode) and 2) near the anchoring sleeve tie-down, predominantly affecting the cathode (helix tip electrode), and occasionally the high voltage conductor. These two locations account for approximately 90% of the chronic fractures identified in Returned Product Analysis (RPA). The remaining 10% of chronic fractures occurred in the DF-1 connector leg and the proximal portion of the RV coil. High voltage conductor fractures could result in the inability to deliver defibrillation therapy. Anode or cathode conductor fractures (at either location) may present clinically as increased impedance, oversensing, increased interval counts, multiple inappropriate shocks, and/or loss of pacing output.

Patient Management Recommendations (Updated April 2011)

The Lead Integrity Alert (LIA) provides three days advance notice prior to inappropriate therapy to 76% of patients with lead fractures¹. As a result, we strongly recommend that all Sprint Fidelis patients who have the ability to upgrade to Lead Integrity Alert do so promptly. Also ensure that high voltage lead impedance alerts (maximum of 100 ohms) are programmed. When a lead fracture is suspected or confirmed, immediate patient attention is strongly recommended. Physicians should inform their patients to seek medical attention without delay if they experience unexpected shocks.

- **If a Fidelis lead fracture of any type has occurred, we recommend implanting a new high voltage lead with or without extraction of the Fidelis lead.**
- In patients with normal device function and no manifestation of lead fracture, no action is recommended. The risk of prophylactic intervention appears to be greater than serious injury resulting from lead fracture even for pacemaker dependent patients, except in select individual patient circumstances as determined by the physician.
- In the event of a device change-out or upgrade procedure, with no manifestation of lead fracture, consider the patient age and lead model data above, as well as patient life expectancy, co-morbidities, ease of extraction related to implant time, patient preference, etc., for the following options:
 - Leave a properly performing lead intact.
 - Implant a new ICD lead without extraction of the existing lead.
 - Carefully consider all factors before prophylactic placement of a pace-sense lead. Data shows an increased risk of high voltage conductor fracture if a pace-sense conductor fracture has previously occurred. This data is available at www.medtronic.com/fidelis
 - Individual patient circumstances may warrant extracting and implanting a new ICD lead. If warranted, Medtronic's Independent Physician Quality Panel recommends the lead extraction procedure be performed by a physician with extensive lead extraction experience.²

Advisories

Status Update

As of January 31, 2015, of the initial implant population of 205,600 in the United States, approximately 72,700 remain implanted. According to Product Surveillance Registry results, lead survival is estimated to be 78.5% (+4.6/-4.3%) at 102 months. As the implanted population ages and the sample size increases for each time interval, the accuracy of the estimated survival probability will increase as shown by tighter confidence intervals.

Keeping Physicians Informed

The most recent Sprint Fidelis lead performance information, including survival curves, physician letters, and subpopulation data, can be found at www.medtronic.com/fidelis and will be updated annually. Medtronic's website also has a selected list of peer-reviewed publications related to Fidelis lead performance and extraction. Medtronic is committed to answering your questions and keeping you informed. If you have any questions or concerns, please contact your Medtronic Representative or Medtronic Technical Services at 1-800-723-4636 (US).

| Initial Affected Population | Number of Confirmed Advisory Related Events | Estimated Remaining Active Population | Additional information about the Sprint Fidelis lead is available at www.medtronic.com/fidelis . |
|---|---|---|---|
| 279,500 Worldwide(205,600 United States) | 6,763 Worldwide(4,821 United States) | 96,300 Worldwide(72,700 United States) | |

Footnotes:

1: Swerdlow C, Gunderson, B, et al. "Downloadable Algorithm to Reduce Inappropriate Shocks Caused by Fractures of Implantable Cardioverter-Defibrillator Leads", Circulation, November 2008, 118: 2122-2129.

2: "Transvenous Lead Extraction: Heart Rhythm Society Expert Consensus on Facilities, Training, Indications, and Patient Management", Heart Rhythm, Vol 6, No 7, July 2009.

Advisories

Potential Separation of Interconnect Wires (2005)

Sigma Implantable Pulse Generators Original Date of Advisory: November 2005

Product

A specific subset of Sigma series pacemakers may fail due to separation of interconnect wires from the hybrid circuit. You may use the "Search for Information by Serial Number" tool at <http://wwwp.medtronic.com/productperformance/> to determine if a specific device is affected.

Advisory

This subset of Sigma series pacemakers that may fail due to separation of interconnect wires from the hybrid circuit may present clinically as loss of rate response, premature battery depletion, intermittent or total loss of telemetry, or no output.

Separation of redundant interconnect wires has been observed on hybrid terminal blocks. Device failure occurs only where both interconnect wires separate from a hybrid terminal block. In October 2005, testing and analysis identified the root cause of these failures and the affected population. Hybrid circuits used in this subset of devices were cleaned during manufacturing with a particular cleaning solvent that could potentially reduce the strength of the interconnect wire bond over time.

No provocative testing can predict which devices may fail.

Patient Management Recommendations

Recommendation for the management of patients who have pacemakers affected by this advisory were changed in May 2009. Current recommendations are:

We realize that each patient requires unique clinical consideration and we support your judgment in caring for your patients. After consultation with Medtronic's Independent Physician Quality Panel, Medtronic offers the following recommendations for patients in the 2005 Sigma advisory:

- Physicians should advise their patients to seek medical attention immediately if they experience symptoms (e.g., fainting or lightheadedness).
- Physicians should consider device replacement for patients who are both pacemaker dependent and who have been implanted with a device in the affected subsets. Medtronic will offer a supplemental device warranty if the device is not already at elective replacement time.
- Physicians should continue routine follow-up in accordance with standard practice for those patients who are not pacemaker dependent.

Status Update

Patient management recommendations remain unchanged. As of January 31, 2015, 839 devices out of approximately 40,000 devices worldwide have been confirmed as having experienced interconnect wire separation.

Four hundred seventy-four(474) of the Sigma devices (1.1%) were returned with information indicating a problem with the patient's pacing system prior to explant. The remaining 365 Sigma devices (0.90%) were returned with no information indicating a potential malfunction while implanted or with insufficient information to determine the state of the device at explant. Lacking definite information indicating proper operation until explant, these remaining devices are conservatively categorized as having experienced interconnect wire separation while implanted.

Advisories

Our original modeling predicted a failure rate from 0.17% to 0.30% over the remaining lifetime of these pacemakers. However, as of May 2009 updated modeling now predicts a failure rate of 3.9% over the remaining device life of those devices still in service at that time.

Out of the initial advisory population of 40,000 worldwide, approximately 4,000 remain implanted. Approximately 900 of these are in the United States.

| Initial Affected Population | Number of Confirmed Advisory Related Events | Estimated Remaining Active Population | Current Malfunction Rate (confirmed malfunctions over total population) | Predicted Malfunction Rate Over the Remaining Life of the Devices Still Implanted |
|--|--|--|---|---|
| 40,000 Implanted Worldwide (est.) (9,900 United States) | 474 Worldwide (96 United States) with information indicating a clinical presentation. An additional 365 Worldwide (66 US) without information indicating a clinical presentation or with insufficient information to determine the state of the device at explant. | 4,000 Worldwide (900 United States) | 101% Worldwide (1.0% United States) | 3.9% |

Performance Notes

Dual Chamber Pacemakers with Measurement Lock-up ERI

Kappa 600, 700, 800, 900, EnPulse, Adapta, Versa, Sensia, Relia, and Vitatron Models E50A1, E60A1, and G70A1

Purpose of this Information

This Performance Note describes a rare measurement lock-up issue that impacts the Medtronic dual chamber pacemakers listed above. If this measurement lock-up occurs, the device will trigger a false Elective Replacement Indicator (ERI). A reset is available to clear this condition and there is no need to explant the device. This issue does not impact battery longevity.

Background

If this rare measurement lock-up occurs in the pacemaker, it causes the device to read a value of zero for battery voltage. After four measurements of zero, the device will trigger ERI and revert to a VVI pacing mode at 65 bpm. There is no loss of ventricular pacing and the output voltage will remain the same.

Programmer Software Reset Method (Adapta, Versa, Sensia, Relia, Vitatron Series E and G)

Programmer software is available which can differentiate a regular ERI and an ERI caused by the measurement lock-up issue. Upon interrogation of a device with the measurement

lock-up ERI, the programmer software recognizes the issue and guides the clinician to clear the ERI (Example 1). Following an ERI reset, the device parameters should be reviewed and reprogrammed to clinician specifications.

Reset Method for Kappa and EnPulse


A service tool continues to be available through Medtronic Technical Services to clear the measurement lock-up issue for Kappa and EnPulse devices.

The issue can be identified using the programmer or via CareLink transmission; the battery voltage measurements and remaining longevity will appear as blank values (Example 2). If this measurement lock-up occurs, contact Medtronic Brady Technical Services at 1-800-505-4636 for assistance.

Example 1 – Programmer Software Detects Measurement Lock-up ERI



Example 2 – Programmer Screens for Measurement Lock-up ERI (Kappa and EnPulse)

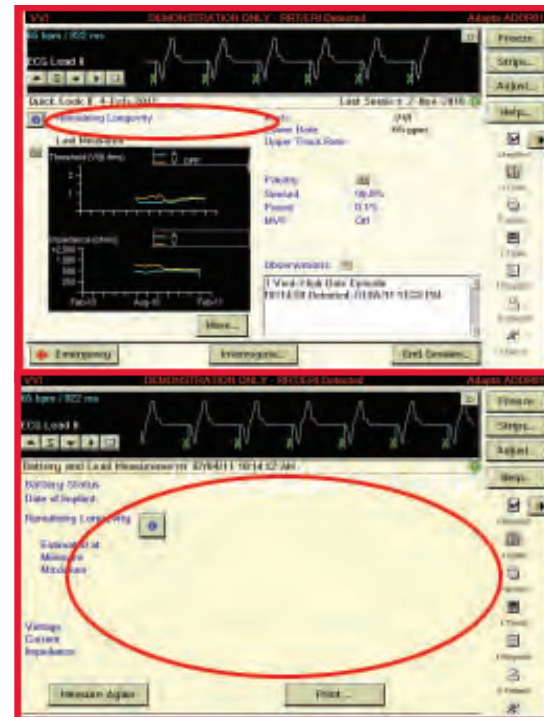

Clinical Management of VCM near Elective Replacement

Background

Medtronic Technical Services has received reports of devices going to ERI or end of life (EOL) sooner than expected after a normal follow-up in which the device longevity was projected to be approximately 18 months. It has been noted that these cases typically involve Kappa 700 devices where Ventricular Capture Management set the ventricular lead to high output (5 V, 1 ms), which occurs by device design when a high threshold is measured. It is important for physicians and allied professionals to understand VCM behavior as it relates to longevity so that they can, in turn, understand how this affects management of the device and follow-up visits as VCM equipped IPGs near the end of their expected longevity.

Device Longevity and VCM Behavior

Ventricular Capture Management is a feature that uses evoked response sensing to determine the stimulation threshold needed to capture the ventricular chamber. Proper detection of the evoked response is crucial to the VCM algorithm determining an accurate capture threshold. There are rare conditions, however, during which the VCM algorithm will not be able to measure the evoked response accurately.¹ When this occurs, for safety reasons the VCM algorithm will reprogram the output to 5 V, 1 ms until the subsequent VCM measurement.

If the device has considerable remaining longevity, these occasional excursions to high output do not substantially affect remaining longevity. However, if the device has less than approximately 18 months remaining longevity, there is the possibility that the high output condition caused by the 5 V, 1 ms output will drain the battery and trigger ERI.

When ERI is declared by the device, VCM is disabled and the outputs are left at 5 V, 1 ms until the device is reprogrammed at an in-office follow-up. This increased current drain of a high output condition will speed depletion of the device, possibly resulting in the device getting to the EOL (battery voltage ≤ 2.15 V).

Please note that the following parameter changes occur when the device goes to ERI:

Table: IPG Therapy Parameter Changes at ERI

| Parameter | Value |
|--------------------------------|--------|
| Pacing Mode | VVI |
| Lower Rate | 65 bpm |
| Single Chamber Hysteresis | OFF |
| Sleep Function | OFF |
| Ventricular Capture Management | OFF |
| Atrial Sensing Assurance | OFF |
| Ventricular Sensing Assurance | OFF |

Kappa 700 is Medtronic's first-generation VCM algorithm, which has a relatively higher incidence of evoked response undersensing compared to subsequent algorithms, resulting in more frequent high output conditions. Therefore, Kappa 700 products are the primary focus of this note. It should be noted that IPGs equipped with the second-generation VCM algorithm (Kappa 900, EnPulse, Adapta/Versa/Sensia, and Relia) have not been observed with evoked response undersensing in the general population, though the items listed in "Follow-Up Considerations" may also be used on these devices.

Follow-Up Considerations

- Estimated longevity in the event the device goes to high output can be determined by the following steps. This allows the clinician to determine follow-up frequency if he or she is concerned the device may go to ERI due to high output.
 - Program the ventricular channel to 5 V, 1 ms
 - Navigate to Data/Battery and Lead Measurements
 - When the message stating "Warning – Old Data" is displayed, select "Yes" to measure battery voltage and lead impedance at the new ventricular outputs
 - An updated remaining longevity estimate will be calculated on the elevated outputs. Note the "Minimum Remaining Longevity." Clinical decisions can be based on this value.
 - Program the Amplitude and Pulse Widths back to their original values before leaving the session
- If the capture trends and lead impedance trends are stable, VCM can be programmed to "Monitor Only" for the remaining device life. This should be considered only if remaining longevity is 18 months or less.
- Follow-up frequency can be increased for those patients who do not have stable capture or lead impedance trends. This can be done via a CareLink Home Monitor, or in-office.

¹ Medtronic, Inc. (2001). Medtronic Kappa 700/600 Series Pacemaker Reference Guide (Chapter 4, p. 27). Can be retrieved from <http://manuals.medtronic.com>.

Performance Notes

General Follow-Up and Replacement of ICD Leads

Implanted leads operate in the challenging biochemical environment of the human body and the body's response to foreign objects. Implanted leads are also subject to mechanical stresses associated with heart motion, body motion, and patient anatomy.

In this environment, pacemaker and defibrillation leads cannot be expected to last forever. Unlike implantable cardioverter defibrillators (ICDs), a lead's longevity cannot be predicted nor are there simple indicators that a lead is approaching the end of its service life. The determination that a lead may be approaching end of service life requires follow-up of the chronically implanted lead and thorough evaluation of lead integrity at ICD replacement.

Follow-Up of Chronically Implanted Leads

The frequency of follow-up for ICD patients will depend on a number of factors including the patient's medical condition, ICD system implant time, hospital/clinic follow-up practice, and Medicare guidelines. In all cases, it is important to assess the functionality of the ICD system and the integrity. For newly implanted leads, it is beneficial to establish a baseline of chronic performance parameters once the lead has stabilized, generally within 6 to 12 months after implant. These performance parameters should include pacing and sensing thresholds and impedance. During routine patient follow-up, these procedures can be used to evaluate lead integrity.

- Measure pacing and sensing threshold and compare to the chronic baseline. Significant increases or decreases may be indicative of lead failure, dislodgement, perforation, exit block, etc.
- Measure pacing impedance where possible and compare to the chronic baseline. Decreases of 30% or more or pacing impedances below 200-250 ohms may be indicative of insulation failure. Sudden and significant increases in pacing impedance may be indicative of conductor fracture.
- High voltage lead circuit impedance should be between 10-75 ohms at system implant. Chronic measurements below 10 and above 200 ohms may be indicative of high voltage lead circuit failure.
- Carefully review ECGs or the nonsustained detection log on Medtronic ICDs for indications of pacing and/or sensing abnormalities such as oversensing, undersensing, and loss of capture
- Elicit and investigate any patient complaints/symptoms that may be suggestive of potential lead failure

Where routine follow-up indicates, additional tools should be used to further evaluate performance. Tools include radiographic data, ICD electrograms, ICD Patient Alert and performance information from the Product Surveillance Registry (PSR).

The final decision on the functional integrity and continued use of an implanted lead must be a matter of medical judgment based on these factors as well as specific patient conditions.

General Criteria for Lead Replacement

The evaluation of a chronically implanted lead is an important part of the decision to continue to use the lead with a new ICD. However, these results alone do not necessarily predict the future integrity of that lead. With the expected longevity of today's ICDs varying between approximately 5 and 10 years, a physician replacing a device should consider a number of factors, including those listed below.

Factors that should be considered in a decision to replace or continue to use include:

- Pacing and sensing thresholds should be evaluated for the potential to maintain acceptable levels
- Pacing impedance should be measured. Bear in mind that pacing impedance below 250 ohms results in excessive battery current drain, which may seriously compromise ICD longevity, regardless of lead integrity.
- The physical appearance of the lead should be examined for insulation cracks, breaches, or other indications of lead wear or degradation
- Medtronic System Longevity Study data should be referenced. Actuarial survival of the lead and the observed lead failure mechanisms are specific factors to consider. Use of a new lead should be considered if failure mechanisms suggest an increased time dependency as suggested in the shape of performance curve for the specific lead model.
- Current publications may provide additional information on the clinical management of leads.¹⁻³ Ultimately, the decision to replace an implanted lead involves medical judgment.

¹ Hauser RG, Cannom D, Hayes DL, et al. Long-term structural failure of coaxial polyurethane implantable cardioverter defibrillator leads. *PACE*. June 2002;25(6):879-882.

² Ellenbogen KA, Wood MA, Shepard RK, et al. Detection and management of an implantable cardioverter defibrillator lead failure: incidence and clinical implications. *J Am Coll Cardiol*. January 1, 2003;41(1):73-80.

³ Hauser RG, Kallinen LM, Almquist AK, Gornick CC, Katsiyannis WT. Early failure of a small-diameter high-voltage implantable cardioverter-defibrillator lead. *Heart Rhythm*. July 2007;4(7):892-896.

Clinical Management of High-Voltage Lead System Oversensing

Appropriate sensing by an ICD system refers to the sensing of cardiac events that may or may not require therapy delivery. ICD systems must sense relatively large QRS complexes while avoiding sensing of smaller T waves, yet continue to sense often small variable amplitude ventricular fibrillation. Thus, ICD systems attempt to dynamically adjust sensing of electrical events and discriminate between them based on detection algorithms and programmed settings.

Inappropriate sensing can occur when an ICD system classifies events of non-cardiac origin as QRS/VF events, or senses and counts T and far-field P waves as ventricular depolarizations. This is often referred to as “oversensing,” and may result in delivery of inappropriate high-voltage therapies. This is due, in part, to the desire to err on the side of delivering lifesaving high voltage therapy rather than withholding

it. Thus, an ICD system that is experiencing oversensing issues will continue to deliver therapeutic shocks as required, but may also subject the patient to unnecessary shocks.

Oversensing can be difficult to manage, in that the precipitating cause of the oversensing can be problematic to isolate. Oversensing can be caused by many factors, including myopotentials/far-field sensing, electromagnetic interference, T wave sensing, connector issues, incomplete or complete conductor fractures, and insulation breaches. While the individual physician must exercise medical judgment in determination of appropriate clinical management of ICD systems, the chart below may assist in the process of causal factor differentiation and possible intervention.

| Phenomenon | Causal Factors | Characteristics | Management/Comments |
|---|--|--|---|
| Myopotentials/ Far-field sensing | Diaphragmatic muscle potentials in breathing, wide tip-to-ring (coil on integrated bipolar leads) spacing | Nonphysiological sensed event on EGM, which may confuse detection potentially resulting in false positive shocks | Check R waves for deterioration. Reprogram sensitivity. Try repositioning lead. Consider change-out to true bipolar lead, or if true bipolar lead in use, one with closer tip-to-ring spacing than current lead. |
| EMI (Electro-Magnetic Interference) | Arc welders, electrical generators, store walk-through security scanners, poorly insulated electrical equipment | Multiple and consecutive short intervals (< 140 ms) independent of underlying sinus beats. Associated with proximity to the EMI source. | Avoid EMI areas. True bipolar leads less susceptible. |
| T-wave sensing | Drugs, ischemic tissue, exercise, Long QT syndrome, electrolyte imbalance | Sense markers seen on EGM related to T wave. False positive detection. | Check for R wave deterioration and characteristics. If R wave > 3.0 mV, reprogram sensitivity. If R wave < 3.0 mV, reposition/replace lead. Address causal factor (e.g., drugs [if appropriate/medically viable]). |
| Connector problems | Loose setscrew, cross-threaded setscrew, incomplete lead insertion into header | This is an acute phenomenon seen within 6 months of implant (usually sooner) | Requires invasive check of connections. May be reproducible with pocket manipulation. |
| Incomplete conductor fracture | One or more filars of a multifilar conductor fracturing while leaving enough filars intact to provide a conduction circuit | Characterized by chaotic oversensing related to motion of the fracture site | Check EGMs and x-rays. Manipulate lead at suspected fracture site if possible as a provocative test. If confirmed, replace lead. |
| Lead insulation breach | Cuts, tears, metal ion oxidization, abrasion, cold flow, environmental stress cracking | Characterized by cyclical and/or erratic, intermittent, spontaneous oversensing; often post-pace or post-shock can cause false positives | Replace lead. If acute, usually secondary to implant damage/replacement damage. If late, material characteristic. |
| Oversensing during interrogation with programming head (not wireless telemetry) with complete lead fracture | Interrogation with a programming head in combination with complete lead fracture that creates an open circuit can induce noise on the sensing circuitry inside the ICD can | Nonphysiologic sensed event on EGM. If detection is enabled during interrogation, oversensing may result in inappropriate therapy. | Quickly remove the programming head. CANCEL the interrupted interrogation and manually load the software for the specific device model. Reposition the programmer head over the device and immediately select SUSPEND. Device will resume detection when programming head is removed, or when RESUME is selected. Replace lead. |

Technical Services is available at all times to advise clinicians in the troubleshooting and management of Medtronic products. For assistance in the United States, please call 1 (800) 723-4636. In other countries, please contact your local Medtronic representative.

Performance Notes

Tests and Observations for Clinical Assessment of Chronic Pacing Leads

| Test/Observation | Possible Insulation Failure | Possible Conductor Failure | Possible Other System Failure | Effect on Test/Observation |
|---|--|---|---|--|
| Pacing Impedance (Telemetered or Measured Invasively) | Sudden and Significant Decrease | Sudden and Significant Increase | Dislodgement. Perforation. Electrolyte Imbalance. Improper IPG/Lead Connection. . . | Decrease Increase or Decrease Increase or Decrease Increase or Decrease |
| Pacing Thresholds (Telemetered/Programmed or Measured Invasively) | Sudden and Significant Increase, Especially in Bipolar System | Sudden and Significant Increase | Dislodgement. Exit Block. Infarct at Electrode Site. Perforation. Improper IPG/Lead Connection. . . | Increase Increase Increase Increase Increase |
| Electrograms (Telemetered or Measured Invasively) | Sudden and Significant Decrease in Amplitudes and/or Slew Rates for P and/or R Waves | Sudden and Significant Decrease or Disappearance of Amplitudes and/or Slew Rates for P and/or R Waves | Dislodgement. Perforation Infarct at Electrode Site. Electrolyte Imbalance. Improper IPG/Lead Connection. . . | Decrease Decrease Decrease Decrease Decrease |
| Waveform Analysis (Oscillographs of Pacer Artifact from ECG Electrodes) | Sudden Increase in Ratios of Leading-Edge Voltages to Trailing-Edge Voltages (i.e., over 25% increase) | Intermittent or No Pacer Artifacts (Even in Asynchronous Mode) | Improper IPG/Lead Connection | Intermittent or No Pacer Artifacts (Even in Asynchronous Mode) |
| Radiographs (Post-Implant, Recent, Current) | Not Discernible | Visual Observation of Conductor/Connector/ Electrode Fracture (Sometimes Discernible) | Dislodgement or Perforation. Improper IPG/Lead Connection. | Sometimes Discernible |
| Visual Inspection (Invasive) | Insulation Breach and/or Degradation, or Ligature Cut-Through | Not Easily Discernible | Connector Defect or Connector Pulled Apart. Improper IPG/Lead Connection. | Sometimes Discernible |
| Pectoral Muscle Stimulation | Sudden Onset, Especially in Bipolar System | | Connector Defect in Bipolar or Unipolar. Hypersensitivity to Unipolar Pulse Generator Can. Anti-Stim Coating or Protection Deficient. | |
| Phrenic Nerve/ Diaphragmatic Stimulation | Sudden Onset in Bipolar or Unipolar Systems | | Perforation or Displacement of Atrial Lead (Phrenic Nerve) | |
| Pacemaker ECG Stimulus Artifact Size and Morphology Change (May Not Be Possible with Digital ECG) | Sudden Onset and Significant Change, Especially in Bipolar System (Increase in Size) | Sudden Changes, Usually a Decrease in Size | Perforation or Dislodgement. Connector Defect. Improper IPG/Lead Connection. | Sometimes Discernible |
| Oversensing (Intermittent or Continuous) | Sudden Onset, Especially in Bipolar Systems | | Physical Contact between the Electrode(s) on the Lead and that of Another Lead. Inappropriate IPG Parameter Setting. Improper IPG/Lead Connection. | Sometimes Discernible |
| Undersensing (Intermittent or Continuous) | Sudden Onset in Either Unipolar or Bipolar Systems | Sudden Onset in Either Unipolar or Bipolar Systems | Dislodgement or Perforation. Infarct at Electrode Site. Electrolyte Imbalance. Inappropriate IPG Parameter Setting. Improper IPG/Lead Connection. | Sometimes Discernible |
| Loss of Capture | See "Pacing Thresholds" Above | See "Pacing Thresholds" Above | See "Pacing Thresholds" Above | |

Mailer Kits Available for Returning Product

Medtronic urges all physicians to return explanted products and to notify Medtronic when a product is no longer in use, regardless of reason for explant or removal from use. The procedures for returning products vary by geographic location.

Mailer kits with prepaid US postage are available for use within the United States to send CRT, ICD, IPG, and leads to Medtronic's CRHF Returned Product Analysis Lab. These mailers are sized to accommodate the devices and leads from a single patient or clinical event and are designed to meet US postal regulations for mailing biohazard materials.

If the product being returned is located outside the United States, please contact your local Medtronic representative for instructions.

Medtronic also requests the return of devices from non-clinical sources, such as funeral homes, and will assume responsibility for storage and disposal of the product once received.

Mailer kits can be obtained by contacting the Returned Product Lab.

CRHF Returned Product Analysis Laboratory
Phone: 1 (800) 328-2518, ext. 44800
Email: crdm.returnedproduct@medtronic.com



www.medtronic.com

World Headquarters

Medtronic, Inc.
710 Medtronic Parkway
Minneapolis, MN
55432-5604 USA
Tel: (763) 514-4000
Fax: (763) 514-4879

Medtronic USA, Inc.
Toll-free: 1 (800) 328-2518
(24-hour technical support
for physicians and medical
professionals)

Europe

Medtronic International Trading
Sàrl Route du Molliau 31
CH-1131 Tolochenaz Switzerland
Tel: (41 21) 802 7000
Fax: (41 21) 802 7900

Canada

Medtronic of Canada Ltd.
6733 Kitimat Road Mississauga,
Ontario L5N 1W3 Canada
Tel: (905) 826-6020
Fax: (905) 826-6620
Toll-free: 1 (800) 268-5346

Asia Pacific

Medtronic International, Ltd.
16/F Manulife Plaza
The Lee Gardens, 33 Hysan
Avenue Causeway Bay
Hong Kong
Tel: (813)-6430-7026
Fax: (852) 2891 6830
enquiryap@medtronic.com

Latin America

Medtronic USA, Inc.
Doral Corporate Center II
3750 NW 87th Avenue Suite 700
Miami, FL 33178 USA
Tel: (305) 500-9328
Fax: (786) 709-4244



Medtronic