

CARDIAC RHYTHM DISEASE MANAGEMENT

Product Performance Report

Important Patient Management Information for Physicians

2008

First Edition
Issue 58



**25TH
YEAR**

- Tracking Performance with multicenter active studies
- Publishing standard, unbiased, consistent, and externally reviewed performance information

A Message from the Vice President

Dear Customer,

Every six months for the last 25 years, Medtronic has compiled and produced product performance reports with one primary goal, to provide you with the product information you need to best care for your patients.

Enclosed in this report is an update on Sprint Fidelis® lead performance and our ongoing vigilance efforts (page 144). Important Sprint Fidelis lead information is summarized as follows:

- **Sprint Fidelis lead performance continues to be in line with the information provided in October 2007.**
- **In consultation with the Independent Physician Quality Panel, our patient management recommendations remain unchanged.**
 - The risk of prophylactic intervention appears to be greater than the risk of serious injury resulting from lead fracture even for pacemaker dependent patients, except in select individual patient circumstances as determined by the physician.
 - When a lead fracture is suspected or confirmed, we strongly recommend prompt patient attention. Patients should contact their physician without delay if they experience unexpected shocks.
 - Implementation of our patient management recommendations is expected to provide two days advance notice prior to inappropriate therapy to 49% of the patients with lead fractures. The remainder will receive less than two days advance notice or no notice. This percentage may vary by implanted device.
- **Future plans include device enhancements and additional information to improve patient management.**
 - We are developing new software that can be downloaded into approximately 93% of Medtronic implanted devices worldwide (98% in the US) to increase the likelihood of fracture detection prior to inappropriate therapy. Approximately 75% of patients should get three or more days notice with the new software. The software will be available later this year, subject to regulatory approval.
 - Quarterly performance updates will be posted on the Medtronic website beginning in August at www.medtronic.com/fidelis.

Consistent with other product advisories, we will continue to communicate updated and in-depth Sprint Fidelis lead data in future product performance reports.

As we mark our 25th Anniversary of product performance reporting, we sincerely thank all our physician customers who have contributed to this important work through:

- Documenting the performance of over 15 million devices and leads implanted across the globe (7.7 million in the US).
- Tracking over 400 different product models with over 70 million accumulated patient-years of experience worldwide (34 million in the US).
- Enrolling over 75,000 patients across 50 centers in chronic lead and system longevity studies. Currently monitoring more than 15,000 leads in over 30 centers in 14 countries and 4 continents.

Far beyond performance reporting, your efforts have clearly proven the efficacy and reliability of cardiac rhythm devices and established their place in medicine as powerful tools to save and improve the lives of those suffering from cardiac disorders.

With appreciation and warm regards,



Reggie Groves
Vice President, Quality and Regulatory
Medtronic Cardiac Rhythm Disease Management
Medtronic, Inc.

Contact Information

We invite our customers to use these telephone numbers to call with suggestions, inquiries, or specific problems related to our products.

US Technical Services Department

Phone: 1 (800) 723-4636 (Tachy)
1 (800) 505-4636 (Brady)
Fax: 1 (800) 824-2362
www.medtronic.com/corporate/contact.jsp

International Technical Centers

Europe (Heerlen NL) +31-45-566-8844
Japan (Tokyo) +81-3-5753-4116

For questions related to this CRDM Product Performance Report, please call US Technical Services at the number above, or write to:

Timothy Smith
Medtronic, Inc.
8200 Coral Sea Street NE MS MVN61
Mounds View, MN 55112 USA
email: tim.smith@medtronic.com

For questions related to returning explanted product or returning product that shows signs of malfunction, please contact:

Outside the United States:
Your Medtronic representative or international technical center at the number above.

Within the United States:
Your Medtronic representative or
CRDM Returned Product Analysis Laboratory
Medtronic, Inc.
7000 Central Avenue NE MS RCE172
Minneapolis, MN 55432-3576 USA
Phone: 1 (800) 328-2518, ext. 44800
email: crdm.returnedproduct@medtronic.com

Editorial Staff

Editor

Reggie Groves, *Vice President, CRDM Quality and Regulatory*

Authors

Timothy Smith, *Senior Principal Product Performance Engineer, CRDM, Trending and Data Analysis*
Sheri Halverson, *MPH, Principal Clinical Research Specialist, CRDM*
Hongyan Qiao, *Statistician, CRDM*
Scott McRae, *Statistician, CRDM*
Tim Hamann, *Graphic Designer, CRDM*

Medtronic Review Board

David Steinhaus, MD, *Vice President and Medical Director, CRDM*
Lonny Stormo, *Vice President, CRDM, Therapy Delivery*
Tim Samsel, *Vice President, CRDM, Regulatory Affairs*
Susan Alpert, PhD, MD, *Senior Vice President, Medtronic Chief Quality and Regulatory Officer*
Subu Mangipudi, *Director, Product Vigilance and Reliability*

Trademarks of Medtronic, Inc.

Adapta®	InSync II	Patient Alert™
AT500®	Protect™	Preva®
Attain®	InSync III	Prevail®
CapSure®	Protect™	Prodigy®
CapSure Sense®	InSync Sentry®	Quick Look™
CapSureFix®	Intrinsic®	SelectSecure®
CareLink™	Jewel®	Sensia®
Concerto®	Kappa®	Sigma®
EnPulse®	Legend®	Spectraflex™
EnRhythm®	Marquis®	Sprint™
EnTrust®	Maximo®	Sprint Fidelis®
GEM®	Medtronic	Sprint Quattro®
InSync®	CareAlert®	Sprint Quattro
InSync ICD®	Medtronic	Secure®
InSync Marquis™	CareLink®	SureFix®
InSync II	Micro Jewel®	Target Tip®
Marquis™	Micro Minix®	Tenax™
InSync III	Minix®	Thera®-i
Marquis™	Minuet®	Transvene™
InSync Maximo®	MVP®	Versa®
	Onyx®	Virtuoso®

CRDM Product Performance Report

2008 First Edition
Issue 58

Date cutoff for this edition is
January 31, 2008

This report is available online at
www.CRDMPPR.medtronic.com

Introduction 4
Method for Estimating CRT, ICD, and IPG Device Performance 9

CRT Cardiac Resynchronization Therapy 13

CRT Survival Summary 18
CRT Reference Chart 20

ICD Implantable Cardioverter Defibrillators 21

ICD Survival Summary 30
ICD Reference Chart 33
ICD Connector Styles 35

IPG Implantable Pulse Generators 36

IPG Survival Summary 63
IPG Reference Chart 71

Leads

Method for Estimating Lead Performance 74

Left-Heart Leads 77

Lead Survival Summary 79
US Returned Product Analysis Summary 79
Reference Chart 79

Defibrillation Leads 80

Lead Survival Summary 88
US Returned Product Analysis Summary 89
Reference Chart 90

Pacing Leads 91

Lead Survival Summary 123
US Returned Product Analysis Summary 127
Reference Chart 129

Epi/Myocardial Pacing Leads 131

Lead Survival Summary 134
US Returned Product Analysis Summary 135
Reference Chart 135

VDD Single Pass Pacing Leads 136

Lead Survival Summary 137
US Returned Product Analysis Summary 137
Reference Chart 137

ICD and CRT-D Charge Time Performance 138

Advisories 144

(in order of communication date, from most recent to oldest)

Performance Notes 153

Ensuring the Accuracy of Battery Longevity Estimates 153
Interactions between Cardiac Pacing and Ventricular Arrhythmia Initiation 154
AT500 Pacing System Follow-Up Protocol 155
Insertion of the Lead into the Device 156
GEM II DR/VR and GEM III DR/VR/AT ICD Battery Discharge Behavior 157
General Follow-Up and Replacement of ICD Leads 158
Clinical Management of High Voltage Lead System Oversensing 159
Tests and Observations for Clinical Assessment of Chronic Pacing Leads 160

Index 161

CRT

ICD

IPG

Leads

ICD Charge Times

Advisories

Performance
Notes

Index

Introduction

All product performance reports are not created equal. For 25 years, Medtronic has monitored performance via both returned product analysis and multicenter clinical studies.

This Product Performance Report (PPR) presents device survival estimates, advisory summaries, performance notes, and other information pertinent to assessing the performance of Medtronic implantable pulse generators (IPGs), implantable cardioverter defibrillators (ICDs), Cardiac Resynchronization Therapy (CRT) devices, and implantable pacing and defibrillation leads.

This Product Performance Report has been prepared in accordance with International Standard ISO 5841- 2:2000(E).

The survival estimates provided in this report are considered to be representative of worldwide performance.

Survival Estimates

Medtronic Cardiac Rhythm Disease Management (CRDM) uses both returned product analysis and multicenter clinical studies to monitor performance.

Medtronic, like other companies, monitors CRT, ICD, and IPG device performance using returned product analysis. We also monitor CRT, ICD, and IPG device performance using an active multicenter clinical study. Medtronic CRDM is unique in the industry in that we track CRT, ICD, and IPG device survival using both methods.

Returned product analysis is a passive approach to assessing product performance. This approach provides a suitable measure of product performance only when a significant number of explanted products are returned to the manufacturer. Returned product analysis provides a measure of hardware performance, but not necessarily the total clinical performance (e.g., the incidence of complications such as infection, erosion, muscle stimulation, etc. are not estimated).

The survival estimates provided in this report for CRT, ICD, and IPG devices are based on returned product analysis. This approach is suitable because a significant number of explanted generators are returned for analysis.

Lead performance is monitored differently. In contrast to CRT, ICD, and IPG devices, a very small percentage of leads are returned to the manufacturer due to the difficulty of explanting them. For leads, an active clinical study provides more accurate survival estimates compared to estimates based solely on returned product analysis.

Survival estimates for leads are based on clinical observations recorded via Medtronic CRDM's System Longevity Study. This multicenter clinical study is

designed to record clinical observations representative of the total clinical experience. Therefore, the lead survival estimates include both lead hardware failure and lead related medical complications, and do not differentiate a lead hardware failure from other clinical events such as exit block, perforation, dislodgement, or concurrent pulse generator failure.

The actuarial life table method is applied to the data collected for CRT, ICD, and IPG devices and leads to provide the survival estimates included in this report. A general introduction to understanding this method of survival analysis is given later in this introduction.

ICD Charge Times

Since May 2000, Medtronic has provided important information on charge time performance of ICDs. The information provided in this report shows how ICD charge time can vary during the time a device is implanted. The information is presented in graphical format showing charge time as a function of implant time. The data for charge times are collected from devices enrolled in the System Longevity Study.

Advisory Summaries

This Product Performance Report includes summaries of all advisories applicable to the performance of the products included in the report. An advisory is added to the report when any product affected by the advisory remains in service and at risk of experiencing the behavior described in the advisory. The advisory will remain in the report until Medtronic estimates no product affected by the advisory remains active, or the risk of experiencing the behavior described in the advisory has passed.

For most advisories, the products subject to the advisory retain essentially the same survival probability as the products of the same model(s) not affected by the advisory. For those advisories where the survival probabilities of the affected and non-affected populations do differ significantly Medtronic will provide separate survival data for each population. The separate survival data will remain in the report until Medtronic estimates no affected product remains in active service.

Performance Notes

This report concludes with a number of Performance Notes developed by Medtronic to provide additional product performance information relevant to follow-up practice and patient management.

continued

Medtronic urges all physicians to return explanted product and to notify Medtronic when a product is no longer in use, regardless of reason for explant or removal from use.

How You Can Help

Medtronic urges all physicians to return explanted product and to notify Medtronic when a product is no longer in use, regardless of the reason for explant or removal from use. The procedures for returning product vary by geographic location.

Mailer kits with prepaid US postage are available for use within the United States to send CRTs, ICDs, IPGs, and leads to Medtronic's CRDM Returned Product Analysis Lab. These mailers are sized to accommodate the devices and leads from a single patient or clinical event and are designed to meet postal regulations for mailing biohazard materials.

If the product being returned is located outside the United States, please contact your local Medtronic representative for instructions.

Medtronic also requests the return of explanted product from non-clinical sources such as funeral homes, and will assume responsibility for storage and disposal of the product once received. For return of larger quantities of explanted products than the mailer can accommodate, Medtronic has handling and shipping guidelines available upon request.

Both mailers and guidelines can be requested by contacting the Returned Product Lab. For information on how to contact the Lab, refer to Contact Information on page 2 of this report.

We continually strive to improve this CRDM Product Performance Report. In keeping with this philosophy, we ask for your suggestions on the content and format of this report, as well as any information you have regarding the performance of Medtronic products. For information on how to comment on this report, see Contact Information on page 2 of this report.

Overview of Survival Analysis

Medtronic uses the Cutler-Ederer actuarial life table method to estimate the length of time over which devices and leads will perform within performance limits established by Medtronic. This probability to perform within performance limits over time is called the *survival probability*.

Devices and leads are followed until an *event* occurs where the device or lead ceases to operate within performance limits. The length of time from implant to the event is recorded for each individual device and lead in the *population sample*. The population sample for CRT, ICD, and IPG devices is made up of patients whose devices are registered as implanted in the United States. For leads, the population sample is the patients enrolled in our multicenter, international prospective System Longevity Study.

For IPGs and ICDs, the events can be normal battery depletion or a device malfunction. For leads, the events are complications as defined for the study.

The actuarial life table method allows Medtronic to account for devices and leads removed from service for reasons unrelated to performance. Devices and leads removed for these reasons are said to be *suspended*. Examples include devices and leads:

- still in service at the time the analysis is performed
- removed to upgrade the device or lead
- no longer in service due to the death of the patient for reasons unrelated to the device or leads, or
- implanted in patients who are lost to follow-up.

For each suspension, the device or lead has performed within performance limits for a period of time, after which its performance is unknown.

An Example

The following example describes the survival analysis method used to establish the survival probability estimates for Medtronic CRDM devices and leads. The example is intended to provide an overview of the analysis process. The definitions of malfunctions and complications, and other details specific to calculating device and lead survival estimates, are provided in the articles *Method for Estimating CRT, ICD, and IPG Device Performance* (page 9) and *Method for Estimating Lead Performance* (page 74).

continued

This simple example describes the survival analysis method used to establish the survival probability estimates for Medtronic CRDM devices and leads.

Figure 1

Implant times for devices of 16 patients. Gray bars with an orange X indicate devices removed from service due to an event. Blue bars indicate suspended devices.

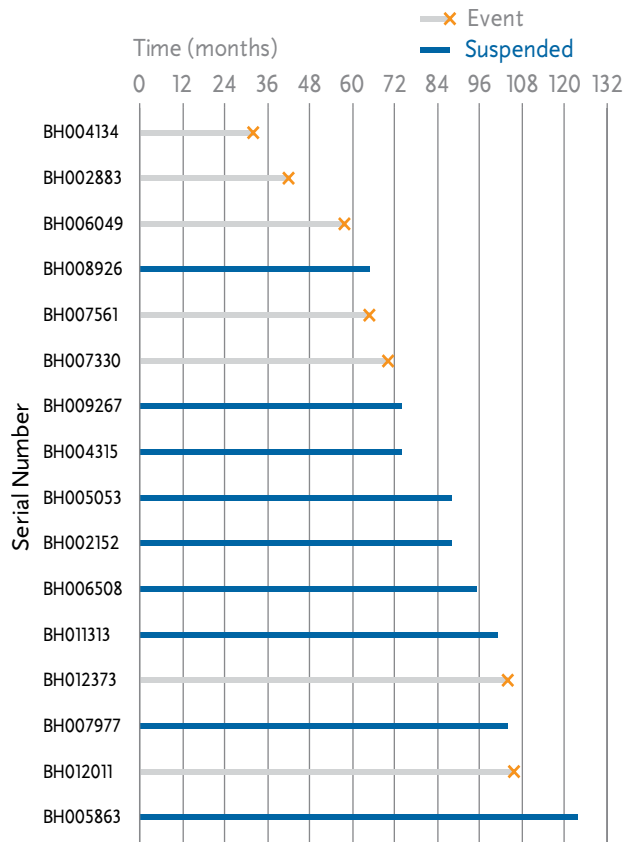


Figure 1 illustrates 16 patients who have implanted devices. The first patient’s device (serial number BH004134) operated within performance limits for 32 months. At that time an event occurred. The fourth patient’s device (serial number BH008926) did not have an event but is suspended, perhaps because it was still in service at the time of the analysis. This patient had 66 months of implant experience. In this example, Figure 1 shows that 7 of the 16 devices suffered events, and 9 are suspended.

The first step in the life table method is to divide the implant time into intervals of a specific length. This example will use 12-month intervals.

The number of devices entered, suspended, and removed due to an event are counted and summarized as shown in Table 1. For the first two intervals, all 16 devices survived and none were removed. In the interval (24-36 months), device BH004134 was removed due to an event. Therefore the table entries show that 16 entered the interval, none were suspended, and one was removed due to an event.

For interval from 36-48 months, only 15 devices entered the interval and one was removed for an event. The remaining intervals are examined and the data entered in columns A, B, and C in like manner. The rest of the columns are filled in using calculations on the data in columns A, B, and C.

The *Effective Sample Size (D)* is the number of devices with full opportunity to experience a qualifying event in the interval. This is computed by subtracting one half the number suspended in the interval from the number that entered the interval. This calculation more accurately reflects the number of devices that could have experienced a qualifying event than simply using the number that entered the interval. Using the number of devices that enter an interval over-estimates the sample size because the suspended devices do not complete the interval. Ignoring the suspended devices under-estimates the sample size because suspended devices are not credited with their full service time. Using one half the number of suspended devices effectively splits the difference.

The next column in the table is the *Proportion with Event (E)*. This is the proportion of devices that had an event in the interval. It is calculated by dividing the *Number of Events (C)* by the *Effective Sample Size (D)*. The number can be interpreted as the estimated rate at which events occur in the time interval.

The *Interval Survival Probability (F)* is the estimate of probability of surviving to the end of the interval assuming the device was working at the beginning of the interval. It is calculated as 1 minus the *Proportion With Event (E)*. This number can be interpreted as the estimated rate at which events **do not** occur in the time interval.

continued

The **Cumulative Survival Probabilities** from (G) the last column of the life table can be plotted versus time intervals in the first column to give a survival curve. Figure 2 shows the survival curve for the data shown in Table 1.

Table 1 Life Table for Figure 1

	A	B	C	D	E	F	G
Interval in Months	Number Entered	Number Suspended	Number of Events	Effective Sample Size	Proportion with Event	Interval Survival Probability	Cumulative Survival Probability
0	16	0	0	16	0.000	1.000	1.000
0-12	16	0	0	16	0.000	1.000	1.000
12-24	16	0	0	16	0.000	1.000	1.000
24-36	16	0	1	16	0.063	0.938	0.938
36-48	15	0	1	15	0.067	0.933	0.875
48-60	14	0	1	14	0.071	0.929	0.813
60-72	13	1	2	12.5	0.160	0.840	0.683
72-84	10	2	0	9	0.000	1.000	0.683
84-96	8	3	0	6.5	0.000	1.000	0.683
96-108	5	2	2	4	0.500	0.500	0.341
108-120	1	0	0	1	0.000	1.000	0.341
120-132	1	1	0	0.5	0.000	1.000	0.341

Definitions:


A	B	C	D	E	F	G
Number Entered	Number Suspended	Number of Events	Effective Sample Size	Proportion with Event	Interval Survival Probability	Cumulative Survival Probability
Number of devices active at the start of the interval	Number of devices removed from service for reasons other than an event	Number of units removed from service due to an event	Number of units with full opportunity to experience a qualifying event in the interval. Computed by subtracting one half the Number Suspended from the Number Entered	Proportion of devices that had an event in the interval. Computed by dividing the Number of Events by the Effective Sample Size	The probability of surviving to the end of the interval, assuming the device was working at the beginning of the interval. Computed as 1 minus the Proportion With Event	The overall probability of surviving to the end of the interval. Computed by multiplying the Interval Survival Probability by the previous interval's Cumulative Survival Probability

Cumulative Survival Probability (G) is the estimate of the unconditional probability of surviving to the end of the interval. It is computed by multiplying the *Interval Survival Probability* (F) by the previous interval's Cumulative Survival Probability. The probability of surviving to 132 months in the example is estimated for the table to be 0.341, or 34.1%.

The *Cumulative Survival Probabilities* (G) of the life table can be plotted versus time intervals in the first column to give a survival curve. Figure 2 shows the survival curve for the data in Table 1.

continued

Figure 2 Survival Curve for Data Given in Table 1

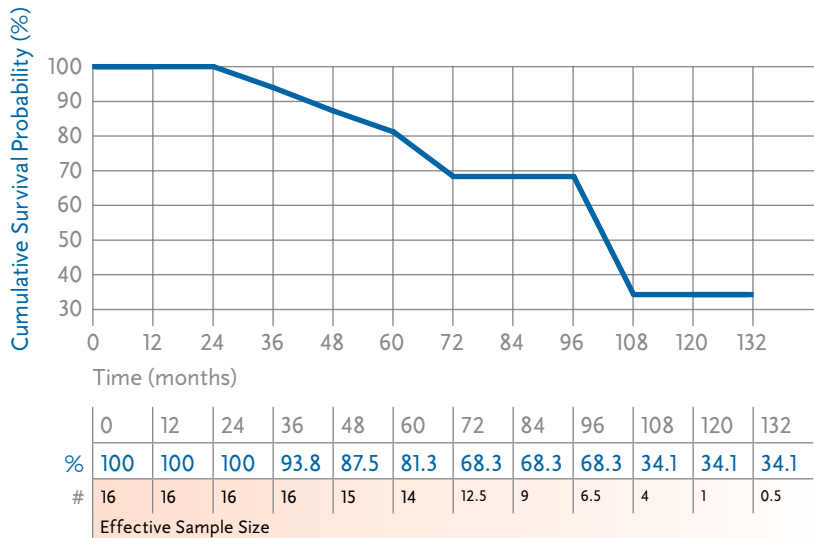

Confidence Intervals

Since survival curves are based on a sample of the device and lead population, they are only estimates of survival. The larger the effective sample size, the more confident the estimate. A confidence interval can be calculated to assess the confidence in an estimate. In the Product Performance Report, Medtronic provides a 95% confidence interval. This can be interpreted as meaning that 95% of the time, the true survival of the device will fall somewhere in the interval.

Survival Curves in the Product Performance Report

Since the survival estimate can become very imprecise with small effective sample sizes, Medtronic truncates the survival curve when the effective sample size is less than 100 for CRTs, ICDs, and IPGs, and when the number entered is less than 50 for leads. The survival charts in the Product Performance Report show the effective sample size for each year interval where Medtronic has experience. When the effective sample size reaches 100 for CRTs, ICDs, and IPGs or when the number entered reaches 50 for leads, the next data point is added to the survival curve.

Although the report provides tabular data in one-year intervals, the curves are actually computed and plotted using one-month intervals (for CRT, ICD, and IPG devices) or three-month intervals (for leads).

A number of references are available for additional information on survival analysis using the Cutler-Ederer life table method¹

¹ Lee, Elisa T.(2003) Statistical Methods for Survival Data Analysis – 3rd Edition (Wiley Series in Probability and Statistics)

Method for Estimating CRT, ICD, and IPG Device Performance

Medtronic urges all physicians to return explanted product and to notify Medtronic when a product is no longer in use, regardless of reason for explant or removal from use.

The performance of CRT, ICD, and IPG devices is expressed in terms of device survival estimates, where “survival” refers to the function of the device, not the survival of the patient. These survival estimates are intended to illustrate the probability that a device will survive for a given number of years with neither malfunction nor battery depletion.

The survival estimates are determined from the analysis of Medtronic CRDM’s United States device registration data and United States returned product analysis data. These data are presented graphically and numerically.

Because this analysis is based on returned product analysis, the performance data does not reflect any device-related medical complications, such as erosion, infection, muscle stimulation, or muscle inhibition.

Categorization of Depleted and Malfunctioning Devices for Survival Analysis

For survival estimation, every device returned to Medtronic CRDM and analyzed in the CRDM Returned Product Analysis laboratory is assigned to one of three categories. The device 1) has functioned normally, 2) has reached normal battery depletion, or 3) has malfunctioned. This categorization is combined with data from our device registry for the total number of implants and the implant durations to create the survival curves presented on the following pages.

Definition of Malfunction

Medtronic CRDM considers a device as having malfunctioned whenever the analysis shows that any parameter was outside the performance limits established by Medtronic while implanted and in service. To be considered a malfunction or battery depletion, the device must have been returned to Medtronic and analyzed.

Devices damaged after explant, damaged due to failure to heed warnings or contraindications in the labeling, or damaged due to interaction with other implanted devices (including leads) are not considered device malfunctions.

A device subject to a safety advisory is not considered to have malfunctioned unless it has been returned to Medtronic CRDM and found, through analysis, to actually have performed outside the performance limits established by Medtronic.

Not all malfunctions expose the patient to a loss of pacing or defibrillation therapy. Some malfunctions included in the following survival estimates may not have been detected at all by the physician or the patient. These malfunctions, however, are included in the survival estimates and provide important feedback to our product development organization.

To provide insight into the nature of malfunctions, each malfunction is categorized as Malfunction with Compromised Therapy Function or Malfunction without Compromised Therapy Function. A summary of these malfunctions is presented for the most recently market-released models.

For this report, Normal Battery Depletion, Malfunction with Compromised Therapy Function and Malfunction without Compromised Therapy Function are defined as follows:

Normal Battery Depletion – The condition when

- (a) A device is returned with no associated complaint and the device has reached its elective replacement indicator(s) with implant time that meets or exceeds the nominal (50 percentile) predicted longevity at default (labeled) settings, or
- (b) A device is returned and the device has reached its elective replacement indicator(s) with implant time exceeding 80% of the expected longevity calculated using the available device setting information.

Medtronic CRDM establishes expected longevity by statistically characterizing the power consumed by the device and the power available from the device battery. This characterization is applied to a number of parameter configurations to derive a statistical mean longevity value and standard deviation for each parameter configuration. The statistical mean value minus three standard deviations is used as the expected longevity for determining if a battery depleted normally.

continued

The Standard Actuarial Method is used to estimate IPG and ICD survival. This product performance report has been prepared in accordance with International Standard ISO 5841-2:2000(E).

For reference purposes, the following pages include estimated longevity for each model. The actual longevity achieved for any device while implanted will depend on the actual programmed parameters and patient factors, and may differ significantly from these estimates.

Malfunction with Compromised Therapy Function

The condition when a device is found to have malfunctioned in a manner that compromised pacing or defibrillation therapy (including complete loss or partial degradation), while implanted and in service, as confirmed by returned product analysis.

Examples: Sudden loss of battery voltage; accelerated current drain such that low battery was not detected before loss of therapy; sudden malfunction during defibrillation therapy resulting in aborted delivery of therapy, intermittent malfunction where therapy is compromised while in the malfunction state.

Malfunction without Compromised Therapy Function

The condition when a device is found to have malfunctioned in a manner that *did not* compromise pacing or defibrillation therapy, while implanted and in service, as confirmed by returned product analysis.

Examples: Error affecting diagnostic functions, telemetry function, data storage; malfunction of a component that causes battery to lose power quickly enough to cause premature battery depletion, but slowly enough that the condition is detected through normal follow-up before therapy is lost; mechanical problems with connector header that do not affect therapy.

Expanded Malfunction Detail

The malfunctions are further divided into categories that identify the subject area of the malfunction. The malfunctions are divided into the following subject areas:

Electrical Component – findings linked to electrical components such as integrated circuits, resistors, capacitors, diodes, etc.

Electrical Interconnect – findings linked to the connections between electrical components such as wires, solder joints, wire bonds, etc.

Battery – findings linked to the battery and its components

Software/Firmware – findings linked to software or firmware function

Possible Early Battery Depletion – findings where the actual reported implant time is less than 80% of the expected longevity calculated using the available device setting information with no device malfunction observed. There may not be sufficient device setting information to determine conclusively if battery depletion was normal or premature in the absence of a specific root cause finding. However, returned devices meeting the above criteria are conservatively classified as Possible Early Battery Depletion malfunctions.

Other – findings related to other components such as insulators, grommets, setscrews, and packaging, and findings where analysis is inconclusive.

Returned Product Analysis Process

Analysis of returned product is performed according to written procedures. These procedures determine the minimum analysis required. The analysis required varies depending on the type of device, age of the device, the associated information received with the device, actual experience with models of similar design, and other factors. Additional analysis is performed as necessary to investigate a performance concern from a customer, or to collect specific reliability data.

When a device is returned with a performance concern from a customer, the general analysis process includes a preliminary analysis of the device in its as-received condition, followed by an automated functional test using test equipment equivalent to the equipment used in manufacturing.

When a malfunction is identified, failure analysis is performed to provide the detailed information necessary to investigate possible causes and actions. Medtronic CRDM maintains in-house expertise and performs its failure analysis using facilities it owns and supports. This capability permits detailed failure analysis.

continued

Medtronic CRDM adjusts all-cause survival estimates to account for underreporting. While this lowers our all-cause survival estimates, we feel it gives a more accurate perspective on real performance.

Statistical Methods for Survival Analysis

Of the several different statistical methods available for survival analysis, the Standard Actuarial Method, with suspensions assumed distributed across the intervals (Cutler-Ederer Method), is used to determine estimates of IPG and ICD survival. This method is commonly used by medical researchers and clinicians.

Implant times are calculated from the implant date to the earlier of the explant date or the cutoff date of the report. From this data an estimate of the probability of device survival is calculated at each monthly interval.

On the following pages, each graph includes a survival curve where events include malfunctions and normal battery depletions. This survival curve is a good representation of the probability a device will survive a period of time without malfunction and without battery depletion. For example, if a device survival probability is 95% after 5 years of service, then the device has a 5% chance of being removed due to battery depletion or malfunction in the first five years following implant.

In addition, a second curve is included to show survival excluding normal battery depletion. This curve is a good representation of the probability for a device to survive without malfunction. This curve includes only malfunctions as events and excludes normal battery depletion.

Since the survival estimate can become very imprecise with small effective sample sizes, Medtronic truncates the survival curve when the effective sample size is less than 100 for CRT, ICD, and IPG devices. The survival charts in the Product Performance Report show the effective sample size for each year interval where we have experience. When the effective sample size reaches 100, the next data point is added to the survival curve.

Although the report provides tabular data in one-year intervals, the curves are actually computed and plotted using one-month intervals.

The data in the tables is rounded to the nearest tenth of one percent. Occasionally, a graph may show 100% survival, but have 1 or more malfunctions or battery depletions. This occurs because even with the malfunctions or battery depletions, the data rounds to 100%.

The survival curves are statistical estimates. As performance experience accumulates, the estimation improves. Confidence intervals are provided as a way to indicate the degree of certainty of the estimates. Greenwood's formula is used to calculate corresponding 95% confidence intervals for the standard errors and the complementary log-log method is used to produce the confidence bounds.

Sample Size and How the Population and Population Samples Are Defined

The population sample from which the survival estimates are derived is comprised of the devices registered as implanted in the United States as of the report cutoff date. The number of registered implants, as well as an estimate of the number that remain in active service, is listed for each model. To be included in the population, the device must have been registered with Medtronic's registration system and implanted for at least one day.

This sample based on US implants is considered to be representative of the worldwide population, and therefore the survival estimates shown in this report should be representative of the performance worldwide of these models.

A CRT, ICD, or IPG model or model family will be included in this report when it has accumulated at least 10,000 implant months, and will remain in the report as long as at least 500 devices remain active.

Methods Used to Adjust for Underreporting of Malfunction and Battery Depletion

The tables on the following pages show the actual number of malfunctions and battery depletions recorded by the analysis lab for US registered devices. Since not all devices are returned to Medtronic CRDM for analysis, these numbers underestimate the true number of malfunctions and battery depletions. To more accurately estimate the all-cause device survival probabilities, the number of malfunctions and battery depletions used to plot each interval of the all-cause survival curves is adjusted (multiplied) by a factor that is based on an estimate of the magnitude of underreporting. The magnitude of underreporting is estimated by analyzing experience in clinical studies (including the System Longevity Study) and the device registration system.

continued

However, at this time, no adjustment for underreporting is applied to the malfunction-free survival curve because a method for estimating malfunction-only underreporting has not been developed.

Adjustments to Registered Implants to Compensate for Unreported Devices Removed from Service

Devices are at times removed from service for reasons other than device malfunction or battery depletion. Examples are devices removed from service due to non-device related patient mortality and devices removed due to changes in the patient's medical condition. Because an accurate estimate of device survival depends on an accurate estimate of the number of devices in service, it is important not to overstate the number of devices in service.

To ensure the number of devices in service is not overstated, the patient mortality rate derived from our device registration system is monitored and compared to published mortality rates for comparable patient populations. If, during calculation of the survival curves, the patient mortality indicated by the data in our device registration is significantly different from published rates, an adjustment is applied to correct the difference.


7272 InSync ICD

Product Characteristics

US Market Release	Jul-02
Registered US Implants	13,000
Estimated Active US Implants	3,000
Normal Battery Depletions (US)	420
Advisories	None

Malfunctions (US)	188
Therapy Function Not Compromised	174
Battery	2
Electrical Component	23
Software/Firmware	3
Possible Early Battery Depletion	146
Therapy Function Compromised	14
Battery	1
Electrical Component	13

NBD Code	VVED
Serial Number Prefix	PJP
Max Delivered Energy	34 J
Estimated Longevity	See page 20

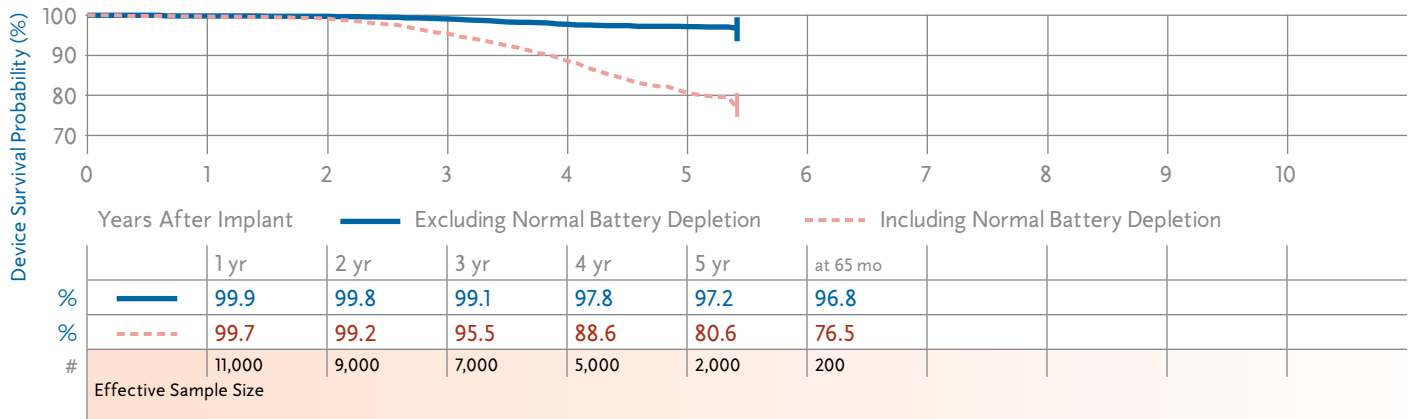


7277 InSync Marquis

Product Characteristics

US Market Release	Mar-03
Registered US Implants	7,000
Estimated Active US Implants	1,000
Normal Battery Depletions (US)	196
Advisories: See page 146 – 2005 Potential Premature Battery Depletion Due to Battery Short	

Malfunctions (US)	72
Therapy Function Not Compromised	62
Battery	1
Electrical Component	8
Software/Firmware	1
Possible Early Battery Depletion	52
Therapy Function Compromised	10
Battery (9 malfunctions related to advisory)	9
Electrical Component	1


NBD Code	VVED
Serial Number Prefix	PLT
Max Delivered Energy	30 J
Estimated Longevity	See page 20

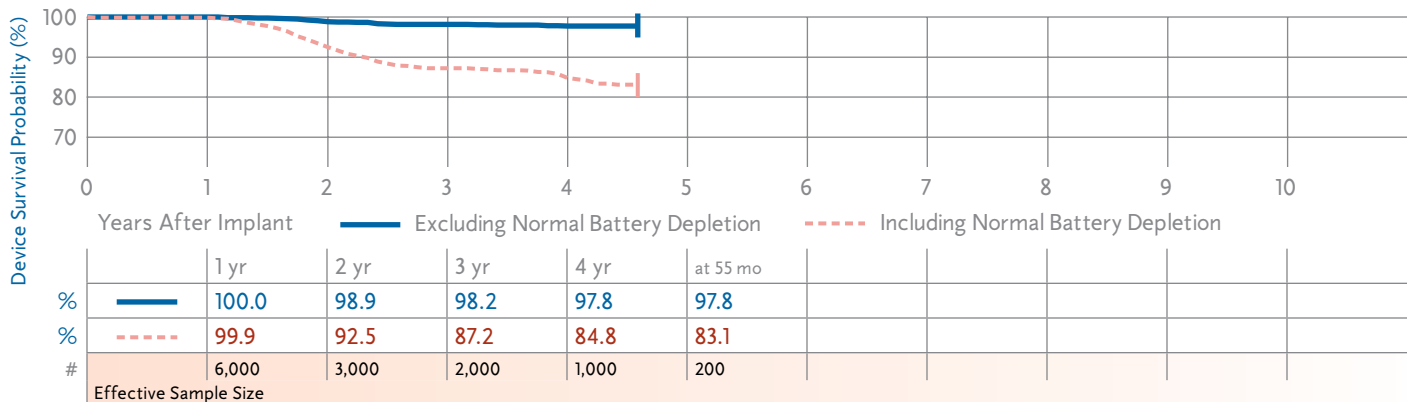

7289 InSync II Marquis

Product Characteristics


US Market Release	Jul-03	Malfunctions (US)	169	NBD Code	VVED
Registered US Implants	28,000	Therapy Function Not Compromised	141	Serial Number Prefix	PRJ
Estimated Active US Implants	9,000	Electrical Component	13	Max Delivered Energy	30 J
Normal Battery Depletions (US)	744	Software/Firmware	1	Estimated Longevity	See page 20
Advisories: See page 146 – 2005 Potential Premature Battery Depletion Due to Battery Short		Possible Early Battery Depletion	127		
		Therapy Function Compromised	28		
		Battery (<i>8 malfunctions related to advisory</i>)	9		
		Electrical Component	19		

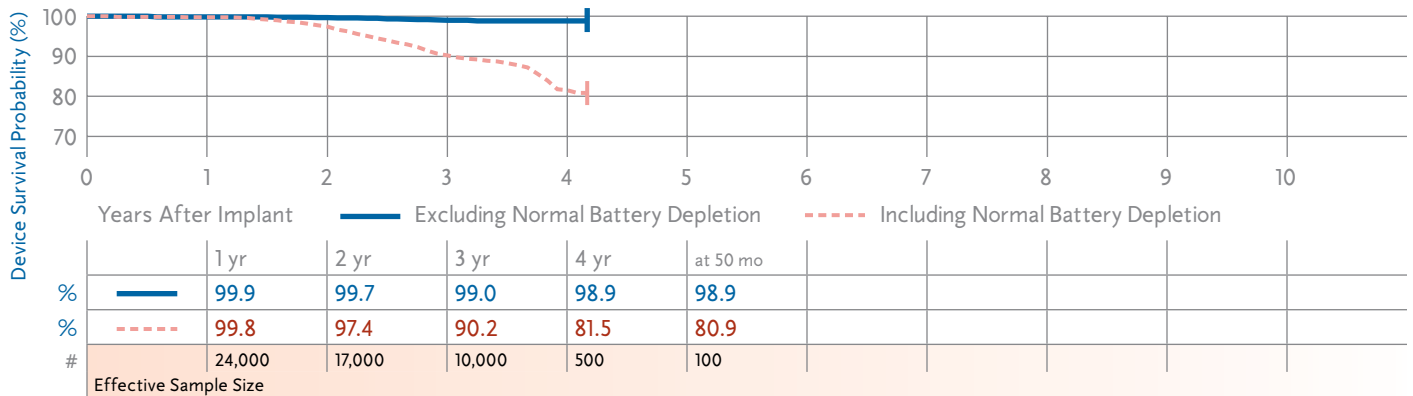

7297 InSync Sentry

Product Characteristics


US Market Release	Nov-04	Malfunctions (US)	14	NBD Code	VVED
Registered US Implants	9,000	Therapy Function Not Compromised	13	Serial Number Prefix	PRK
Estimated Active US Implants	6,000	Battery	1	Max Delivered Energy	35 J
Normal Battery Depletions (US)	50	Electrical Component	4	Estimated Longevity	See page 20
Advisories	None	Possible Early Battery Depletion	8		
		Therapy Function Compromised	1		
		Electrical Component	1		

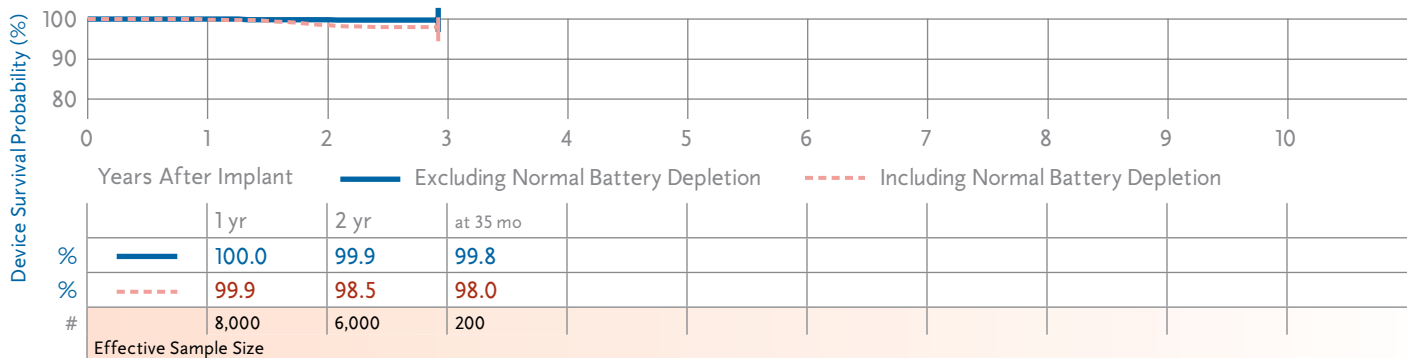

7299 InSync Sentry

Product Characteristics


US Market Release	Apr-05	Malfunctions (US)	13	NBD Code	VVED
Registered US Implants	30,000	Therapy Function Not Compromised	9	Serial Number Prefix	PRK
Estimated Active US Implants	23,000	Electrical Component	4	Max Delivered Energy	35 J
Normal Battery Depletions (US)	17	Software/Firmware	2	Estimated Longevity	See page 20
Advisories	None	Possible Early Battery Depletion	3		
		Therapy Function Compromised	4		
		Electrical Component	4		

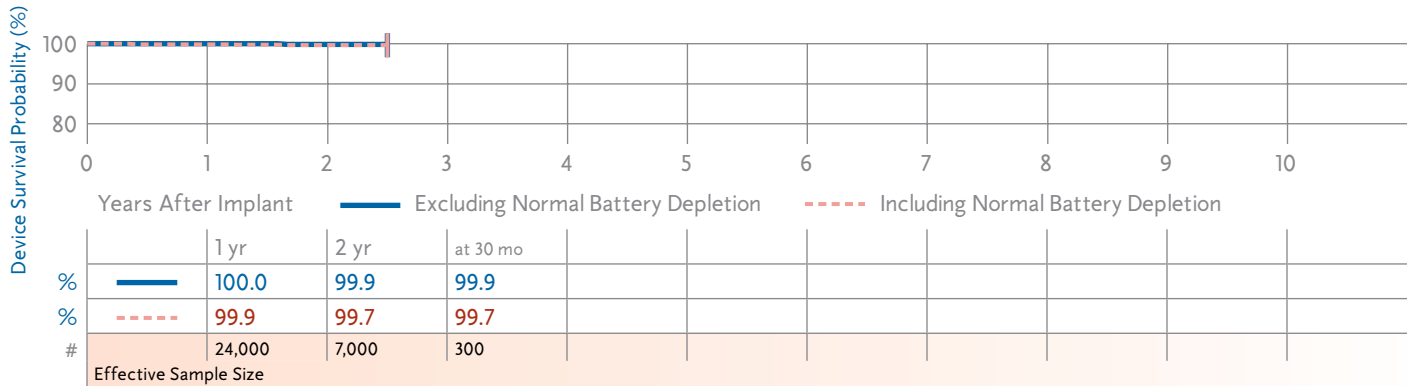

7303 InSync Maximo

Product Characteristics


US Market Release	Jun-04	Malfunctions (US)	34	NBD Code	VVED
Registered US Implants	17,000	Therapy Function Not Compromised	29	Serial Number Prefix	PRL
Estimated Active US Implants	10,000	Electrical Component	5	Max Delivered Energy	35 J
Normal Battery Depletions (US)	193	Software/Firmware	1	Estimated Longevity	See page 20
Advisories	None	Possible Early Battery Depletion	23		
		Therapy Function Compromised	5		
		Electrical Component	5		

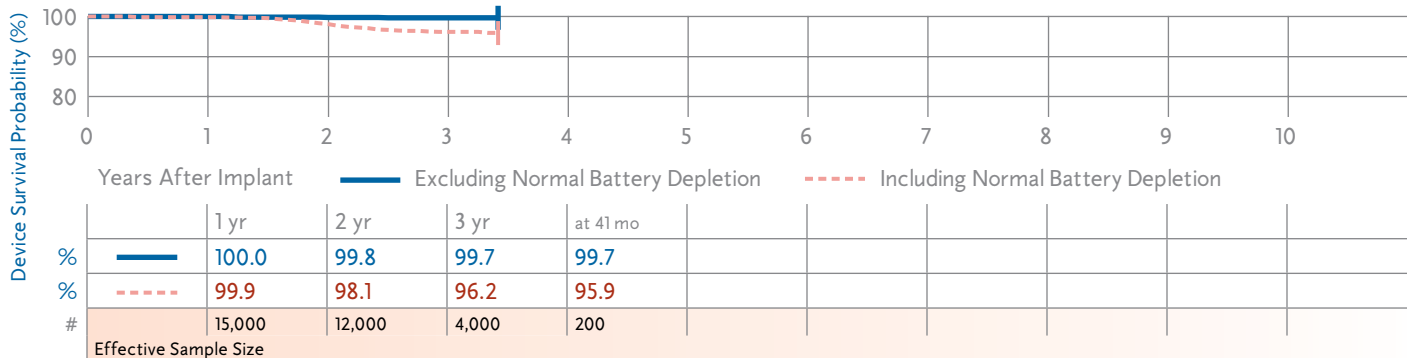

7304 InSync Maximo

Product Characteristics


US Market Release	Apr-05	Malfunctions (US)	4	NBD Code	VVED
Registered US Implants	17,000	Therapy Function Not Compromised	3	Serial Number Prefix	PRL
Estimated Active US Implants	13,000	Battery	1	Max Delivered Energy	35 J
Normal Battery Depletions (US)	9	Electrical Component	2	Estimated Longevity	See page 20
Advisories	None	Therapy Function Compromised	1		
		Electrical Component	1		

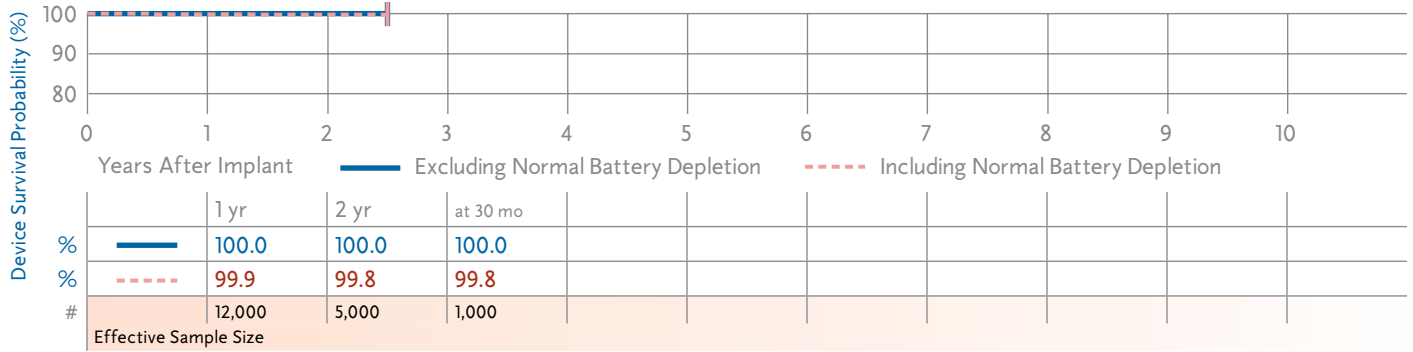

8040 InSync

Product Characteristics


US Market Release	Aug-01	Malfunctions (US)	28	NBD Code	DDDR
Registered US Implants	15,000	Therapy Function Not Compromised	8	Serial Number Prefix	PIN
Estimated Active US Implants	4,000	Electrical Component	4	Estimated Longevity	See page 20
Normal Battery Depletions (US)	248	Electrical Interconnect	1		
Advisories	None	Possible Early Battery Depletion	3		
		Therapy Function Compromised	20		
		Electrical Interconnect	20		

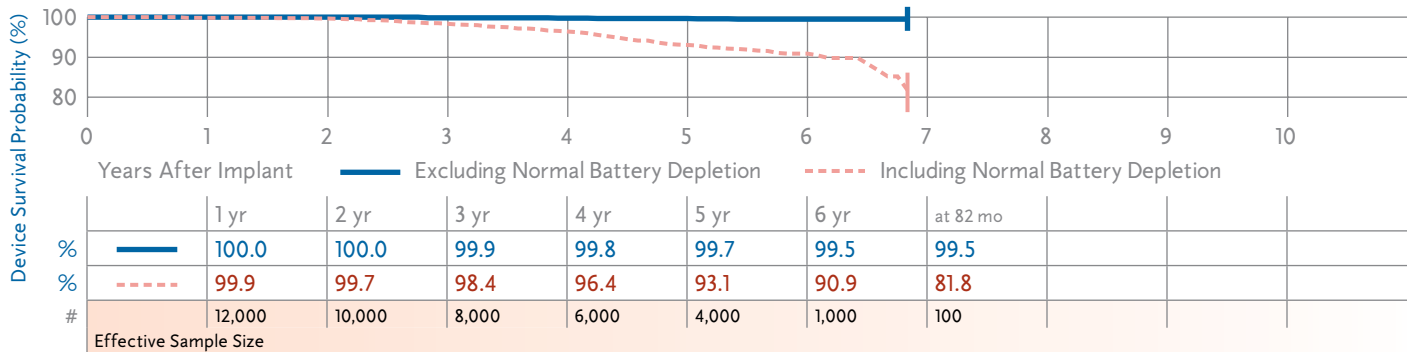

8042 InSync III

Product Characteristics


US Market Release	Feb-03	Malfunctions (US)	5	NBD Code	DDDR
Registered US Implants	25,000	Therapy Function Not Compromised	3	Serial Number Prefix	PKF
Estimated Active US Implants	15,000	Electrical Component	2	Estimated Longevity	See page 20
Normal Battery Depletions (US)	62	Possible Early Battery Depletion	1		
Advisories	None	Therapy Function Compromised	2		
		Electrical Interconnect	2		

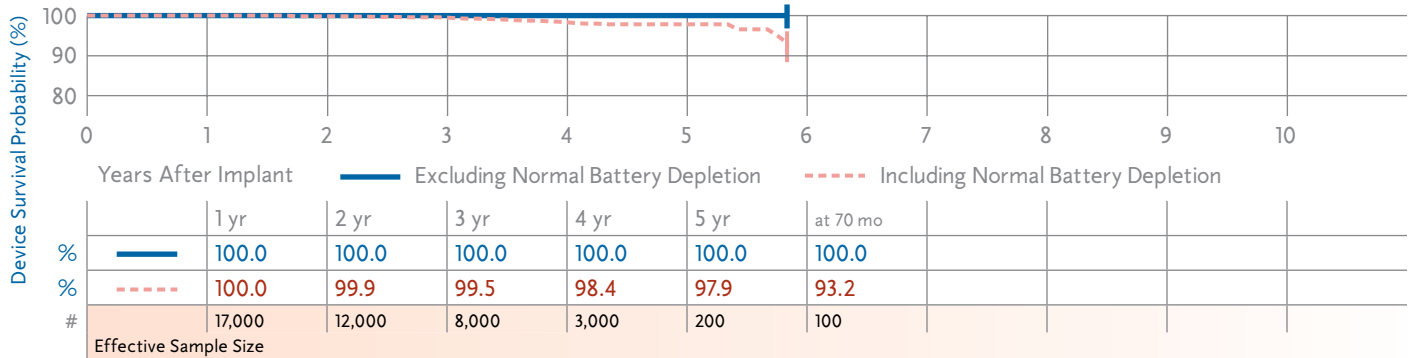

C154DWK, C164AWK, C174AWK Concerto

Product Characteristics

US Market Release	May-06	Malfunctions (US)	13	NBD Code	VVED
Registered US Implants	35,000	Therapy Function Not Compromised	6	Serial Number Prefix	PVU, PVT, PVR
Estimated Active US Implants	32,000	Electrical Component	2	Max Delivered Energy	35 J
Normal Battery Depletions (US)	2	Possible Early Battery Depletion	4	Estimated Longevity	See page 20
Advisories	None	Therapy Function Compromised	7		
		Electrical Component	6		
		Electrical Interconnect	1		

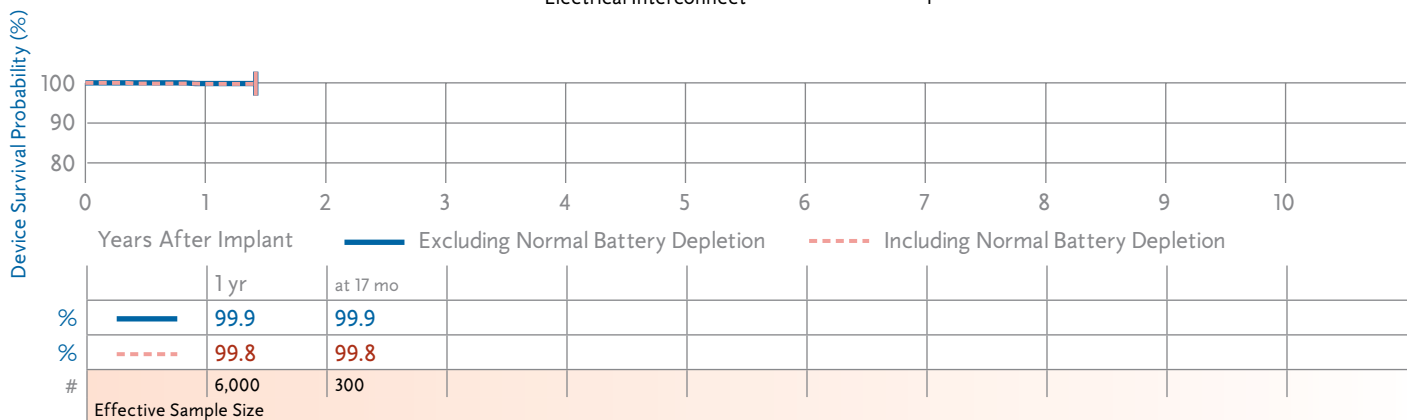

Device Survival Summary (95% Confidence Interval)
 The following table shows CRT device survival estimates with 95% confidence intervals. Estimates are shown both with and without normal battery depletions included.

Model Number	Family	US Market Release	Registered US Implants	Estimated Active US Implants	Normal Battery Depletions (US)	Malfunctions (US)		Device Survival Probability (%)										
						Therapy Function Compromised	Therapy Function Not Compromised	Years After Implant										
						14 + 174 =	188	1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr		
7272	InSync ICD	Jul-02	13,000	3,000	420	14 + 174 =	188	Excluding Normal Battery Depletion	99.9 +0.0/-0.1	99.8 +0.1/-0.1	99.1 +0.2/-0.2	97.8 +0.3/-0.4	97.2 +0.4/-0.4	96.8 +0.7/-0.9 at 65 mo				
								Including Normal Battery Depletion	99.7 +0.1/-0.1	99.2 +0.2/-0.2	95.5 +0.4/-0.5	88.6 +0.7/-0.8	80.6 +1.1/-1.1 at 65 mo					
7277	InSync Marquis	Mar-03	7,000	1,000	196	10 + 62 =	72	Excluding Normal Battery Depletion	100.0 +0.0/-0.1	98.9 +0.3/-0.4	98.2 +0.4/-0.5	97.8 +0.5/-0.6	97.8 +0.5/-0.6 at 55 mo					
								Including Normal Battery Depletion	99.9 +0.1/-0.1	92.5 +0.7/-0.8	87.2 +1.1/-1.2	84.8 +1.3/-1.4	83.1 +1.5/-1.6 at 55 mo					
7289	InSync II Marquis	Jul-03	28,000	9,000	744	28 + 141 =	169	Excluding Normal Battery Depletion	99.9 +0.0/-0.0	99.7 +0.1/-0.1	99.0 +0.1/-0.2	98.9 +0.2/-0.2	98.9 +0.2/-0.2 at 50 mo					
								Including Normal Battery Depletion	99.8 +0.0/-0.1	97.4 +0.2/-0.2	90.2 +0.5/-0.5	81.5 +1.4/-1.5	80.9 +1.6/-1.7 at 50 mo					
7297	InSync Sentry	Nov-04	9,000	6,000	50	1 + 13 =	14	Excluding Normal Battery Depletion	100.0 +0.0/-0.1	99.9 +0.1/-0.1	99.8 +0.1/-0.1 at 35 mo							
								Including Normal Battery Depletion	99.9 +0.1/-0.1	98.5 +0.3/-0.3	98.0 +0.3/-0.4 at 35 mo							
7299	InSync Sentry	Apr-05	30,000	23,000	17	4 + 9 =	13	Excluding Normal Battery Depletion	100.0 +0.0/-0.0	99.9 +0.0/-0.0	99.9 +0.0/-0.0 at 30 mo							
								Including Normal Battery Depletion	99.9 +0.0/-0.0	99.7 +0.1/-0.1	99.7 +0.1/-0.1 at 30 mo							
7303	InSync Maximo	Jun-04	17,000	10,000	193	5 + 29 =	34	Excluding Normal Battery Depletion	100.0 +0.0/-0.0	99.8 +0.1/-0.1	99.7 +0.1/-0.1	99.7 +0.1/-0.1 at 41 mo						
								Including Normal Battery Depletion	99.9 +0.0/-0.1	98.1 +0.2/-0.3	96.2 +0.3/-0.4 at 41 mo							
7304	InSync Maximo	Apr-05	17,000	13,000	9	1 + 3 =	4	Excluding Normal Battery Depletion	100.0 +0.0/-0.0	100.0 +0.0/-0.1	100.0 +0.0/-0.1 at 30 mo							
								Including Normal Battery Depletion	99.9 +0.0/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1 at 30 mo							

continued

Device Survival Summary continued

Model Number	Family	US Market Release	Registered US Implants	Estimated Active US Implants	Normal Battery Depletions (US)	Malfunctions (US)		Device Survival Probability (%)									
						Therapy Function Compromised	Therapy Function Not Compromised	Years After Implant									
								1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	
8040	InSync	Aug-01	15,000	4,000	248	20 + 8 = 28	28	100.0 +0.0/-0.0	100.0 +0.0/-0.1	99.9 +0.0/-0.1	99.8 +0.1/-0.1	99.7 +0.1/-0.2	99.5 +0.2/-0.2	99.5 +0.2/-0.2 at 82 mo			
						Excluding Normal Battery Depletion	Including Normal Battery Depletion	99.9 +0.0/-0.1	96.4 +0.4/-0.4	93.1 +0.6/-0.6	90.9 +0.8/-0.9	81.8 +4.4/-5.5 at 82 mo					
8042	InSync III	Feb-03	25,000	15,000	62	2 + 3 = 5	5	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.1	100.0 +0.0/-0.1	100.0 +0.0/-0.1	100.0 +0.0/-0.1 at 70 mo				
						Excluding Normal Battery Depletion	Including Normal Battery Depletion	99.9 +0.0/-0.1	98.4 +0.3/-0.4	97.9 +0.4/-0.4	93.2 +2.9/-4.9 at 70 mo						
C154DWK, C164AWK, C174AWK	Concerto	May-06	35,000	32,000	2	7 + 6 = 13	13	99.9 +0.0/-0.1	99.9 +0.0/-0.1 at 17 mo								
						Excluding Normal Battery Depletion	Including Normal Battery Depletion	99.8 +0.1/-0.1									

Reference Chart

The longevity estimates provided are mean values calculated for the parameters given. The actual longevity achieved for any device while implanted will depend on the actual programmed parameters and patient factors, and may differ significantly from these estimates.

Model Number	Family	Connector Style	Volume/ Mass*	Delivered Energy	Estimated Longevity					Elective Replacement (ERI)**		End of Life (EOL) Battery Voltage
					Charging Frequency**	100% Pacing†	50% Pacing†	15% Pacing†	100% Sensing	Battery Voltage	Charge Time	
7272	InSync ICD	DR+LV	66 cc 117 g	34 J	Monthly Quarterly Semiannual	5.4 6.5 6.9	6.3 8.0 8.5	7.3 9.4 10.3	7.8 10.3 11.2	≤ 4.91 V	—	≤ 4.57 V
7277	InSync Marquis	DR+LV split	38 cc 77 g	30 J	Monthly Quarterly Semiannual	3.7 5.0 5.5	4.3 6.0 6.7	4.7 7.0 8.0	4.9 7.5 8.6	≤ 2.62 V	> 16 second charge time	3 months after ERI
7289	InSync II Marquis	DR+LV true	38 cc 76 g	30 J	Monthly Quarterly Semiannual	3.3 4.2 4.5	3.6 4.9 5.4	4.0 5.5 6.1	4.2 5.8 6.6	≤ 2.62 V	> 16 second charge time	3 months after ERI
7295	InSync II Protect	DR+LV true	38 cc 77 g	30 J	Monthly Quarterly Semiannual	3.3 4.2 4.5	3.7 4.9 5.4	4.0 5.5 6.2	4.2 5.9 6.6	≤ 2.62 V	> 16 second charge time	3 months after ERI
7297	InSync Sentry	DR+LV true	40 cc 78 g	35 J	Monthly Quarterly Semiannual	3.3 4.5 5.0	3.7 5.3 6.0	4.1 6.2 7.1	4.3 6.6 7.7	≤ 2.62 V	> 16 second charge time	3 months after ERI
7299	InSync Sentry	DR+LV true	40 cc 78 g	35 J	Monthly Quarterly Semiannual	3.3 4.5 5.0	3.7 5.3 6.0	4.1 6.2 7.1	4.3 6.6 7.7	≤ 2.62 V	> 16 second charge time	3 months after ERI
7303	InSync Maximo	DR+LV true	40 cc 78 g	35 J	Monthly Quarterly Semiannual	3.3 4.5 5.0	3.7 5.3 6.0	4.1 6.2 7.1	4.3 6.6 7.7	≤ 2.62 V	> 16 second charge time	3 months after ERI
7304	InSync Maximo	DR+LV true	40 cc 78 g	35 J	Monthly Quarterly Semiannual	3.3 4.5 5.0	3.7 5.3 6.0	4.1 6.2 7.1	4.3 6.6 7.7	≤ 2.62 V	> 16 second charge time	3 months after ERI

Family	Model Number	Estimated Longevity			Elective Replacement Time Indicators
		Amplitude Setting	500 Lead Ω	1000 Lead Ω	
InSync	8040	Low 2.5 V (A, RV)	11.9	13.7	**
		Nominal 3.5 V (A, RV)	8.9	11.4	
		High 5.0 V (A, RV)	6.6	9.1	
InSync III	8042	Low 2.5 V (A, RV, LV)	8.3	9.9	**
		Nominal 3.5 V (A, RV, LV)	5.9	7.8	
		High 5.0 V (A, RV, LV)	4.1	6.0	

Model Number	Family	Connector Style	Volume/ Mass*	Delivered Energy	Estimated Longevity					Recommended Replacement (RRT)***		End of Service (EOS)
					Charging Frequency**	100% Pacing†	50% Pacing†	15% Pacing†	100% Sensing	Battery Voltage	Charge Time	
C154DWK, C164AWK, C174AWK	Concerto	DR+LV true	38 cm 68 g	35 J	Monthly Quarterly Semiannual	3.8 5.5 6.3	4.3 6.8 8.0	4.8 8.0 9.8	5.0 8.8 11.0	≤ 2.62 V	—	3 month after RRT or > 16-second charge time

* Volume and mass differ by connector style.

** A full charge is a full energy therapeutic shock or capacitor reformation.

*** The minimum time between ERI and EOL (or RRT and EOS) is 3 months (100% pacing, two charges per month).

† Pacing mode is DDD for CRT models. Parameter settings; lower rate at 60 ppm, sensing rate at 70 bpm, (A, RV, LV) 3.0 V amplitude, 0.4 ms pulse width, and 510 ohm pace load per applicable channel. CRT models with shared biventricular pacing; InSync Marquis 7277 (LV impedance set to 510 ohms), InSync ICD 7272 (RV amplitude set to 4.0 V).

7227 GEM


Product Characteristics

US Market Release	Oct-98
Registered US Implants	22,000
Estimated Active US Implants	6,000
Normal Battery Depletions (US)	749

Malfunctions (US) 140

NBD Code	VVEV
Serial Number Prefix	PIP, PLN, PLP, PLR
Max Delivered Energy	35 J
Estimated Longevity	See page 33

Advisories: [See page 148](#) – 1999 Potential Circuit Overload

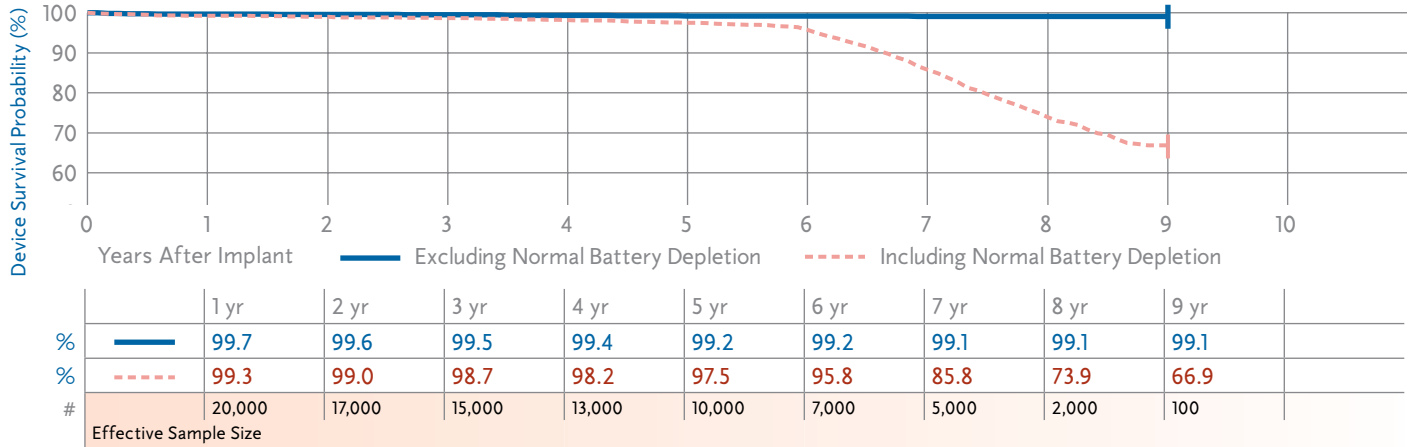

7229 GEM II VR


Product Characteristics

US Market Release	Jul-99
Registered US Implants	11,000
Estimated Active US Implants	1,000
Normal Battery Depletions (US)	994

Malfunctions (US) 26

NBD Code	VVEV
Serial Number Prefix	PJJ
Max Delivered Energy	30 J
Estimated Longevity	See page 33


Advisories: [See page 148](#) – 1999 Potential Circuit Overload
[also see page 157](#) – Performance note on ICD Battery Discharge Behavior

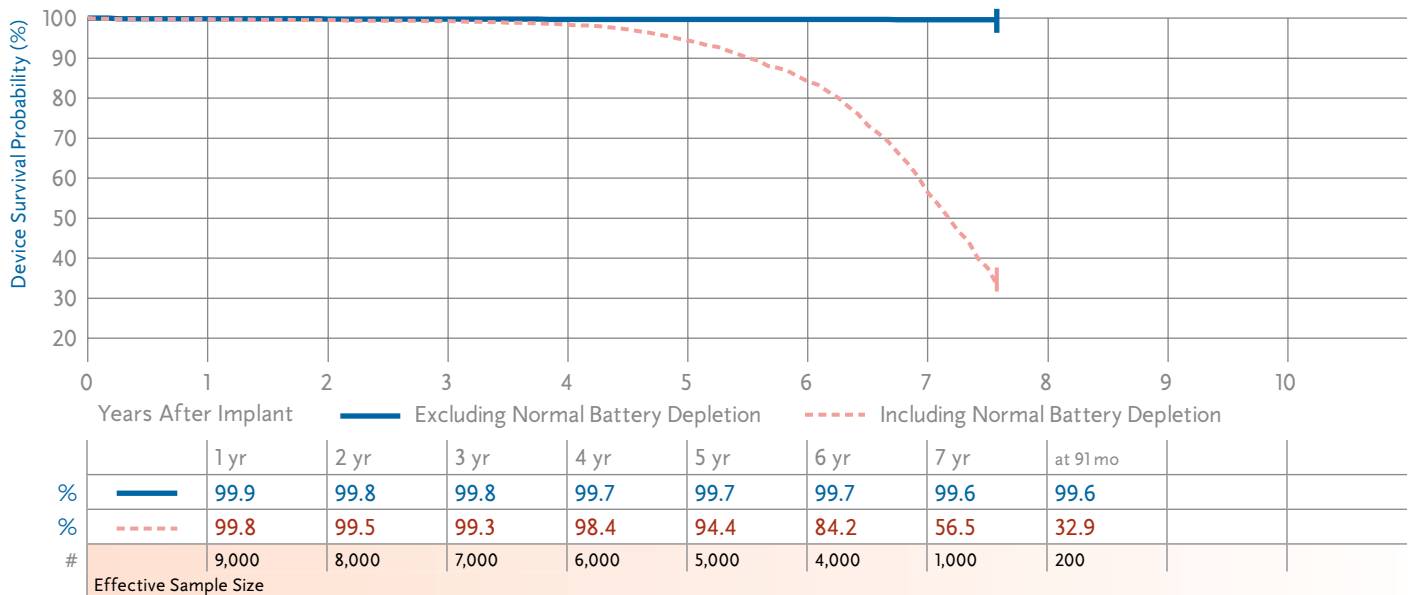

7230 Marquis VR

Product Characteristics


US Market Release	Dec-02	Malfunctions (US)	21	NBD Code	VVEV
Registered US Implants	19,000	Therapy Function Not Compromised	15	Serial Number Prefix	PKD, PLW, PLY
Estimated Active US Implants	10,000	Electrical Component	10	Max Delivered Energy	30 J
Normal Battery Depletions (US)	8	Possible Early Battery Depletion	4	Estimated Longevity	See page 33
Advisories: See page 146 – 2005 Potential Premature Battery Depletion Due to Battery Short		Other	1		
		Therapy Function Compromised	6		
		Battery	1		
		Electrical Component	5		

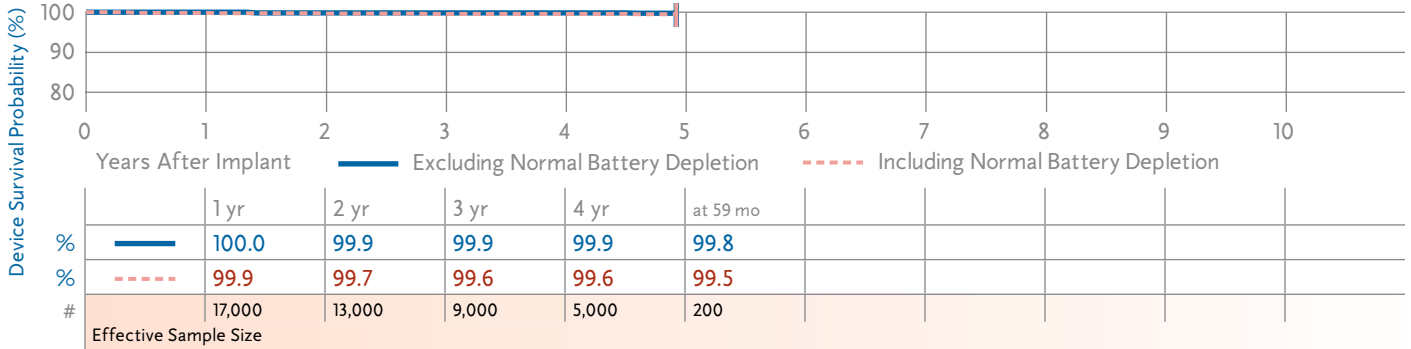

7231 GEM III VR

Product Characteristics

US Market Release	Dec-00	Malfunctions (US)	31	NBD Code	VVEV
Registered US Implants	17,000	Therapy Function Not Compromised	23	Serial Number Prefix	PJL
Estimated Active US Implants	9,000	Battery	1	Max Delivered Energy	30 J
Normal Battery Depletions (US)	223	Electrical Component	18	Estimated Longevity	See page 33
Performance Note: see page 157 – Performance note on ICD Battery Discharge Behavior		Possible Early Battery Depletion	4		
		Therapy Function Compromised	8		
		Battery	1		
		Electrical Component	7		

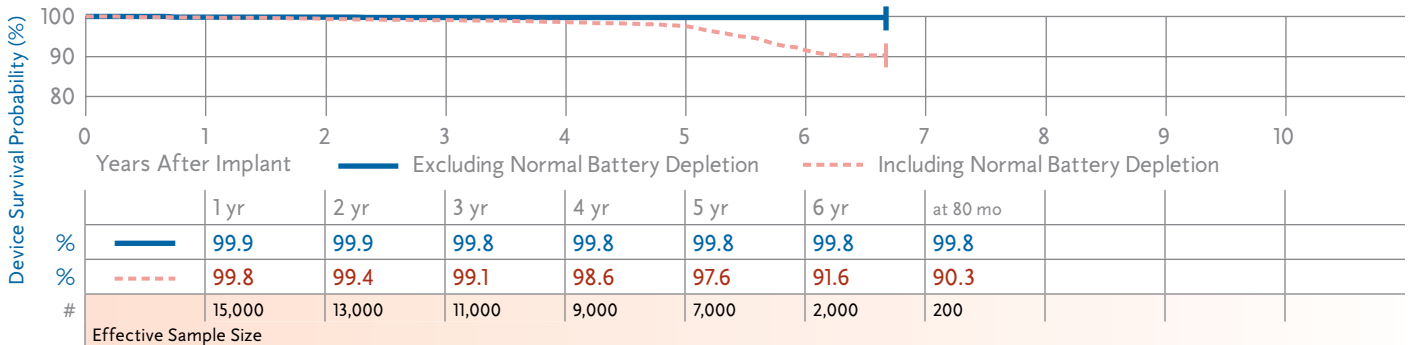


7232 Maximo VR

Product Characteristics

US Market Release	Oct-03
Registered US Implants	41,000
Estimated Active US Implants	33,000
Normal Battery Depletions (US)	7
Advisories: See page 146 – 2005 Potential Premature Battery Depletion Due to Battery Short	

Malfunctions (US)	18
Therapy Function Not Compromised	12
Electrical Component	6
Possible Early Battery Depletion	6
Therapy Function Compromised	6
Electrical Component	5
Possible Early Battery Depletion	1

NBD Code	VVED
Serial Number Prefix	PRN
Max Delivered Energy	35 J
Estimated Longevity	See page 33

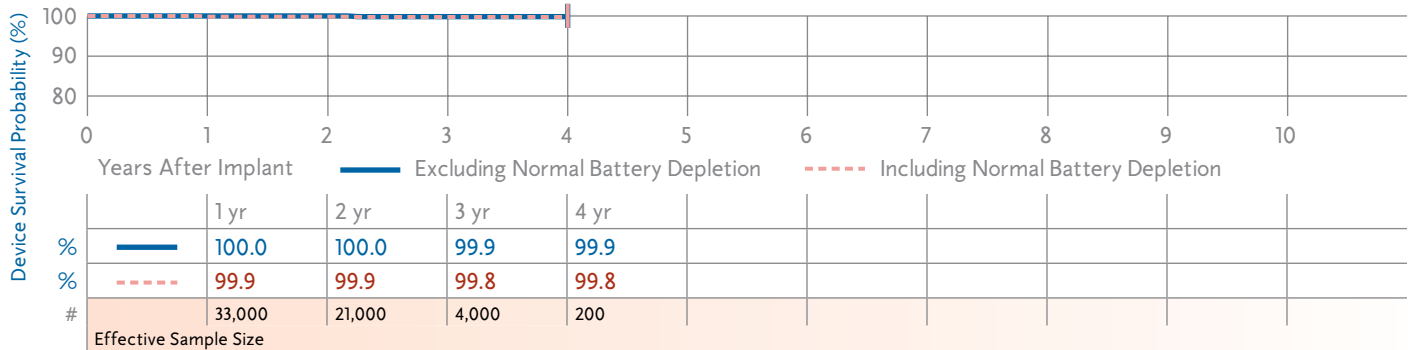


7271 GEM DR

Product Characteristics

US Market Release	Oct-98
Registered US Implants	15,000
Estimated Active US Implants	3,000
Normal Battery Depletions (US)	652
Advisories	None

Malfunctions (US)	88
-------------------	----

NBD Code	VVED
Serial Number Prefix	PIM
Max Delivered Energy	27 J
Estimated Longevity	See page 33

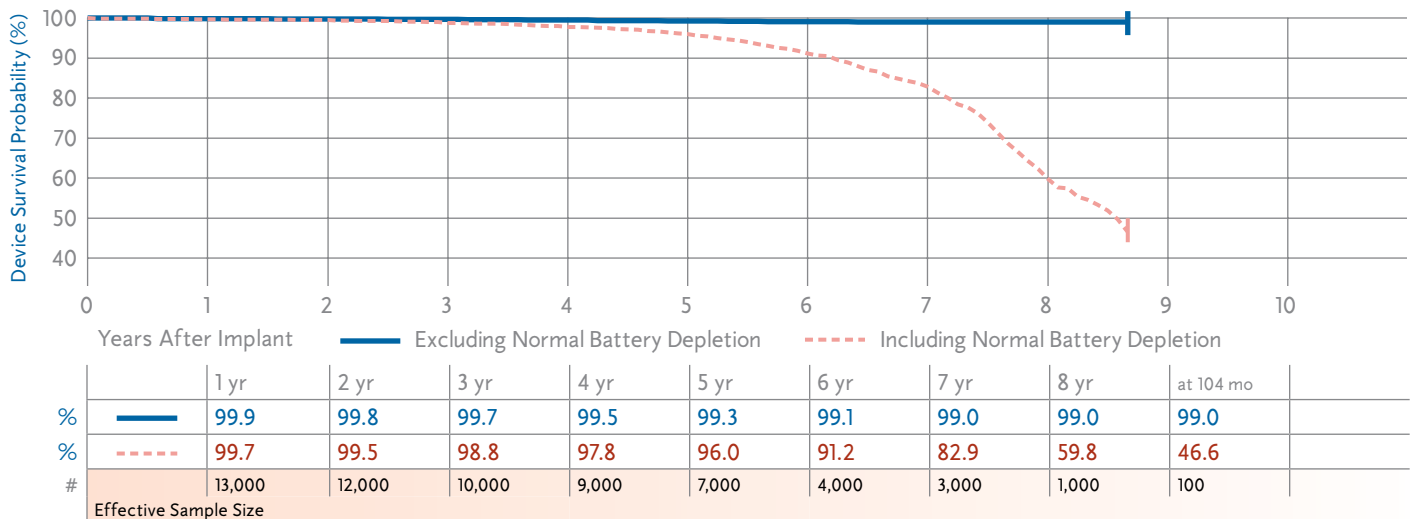


7274 Marquis DR

Product Characteristics

US Market Release	Mar-02
Registered US Implants	48,000
Estimated Active US Implants	21,000
Normal Battery Depletions (US)	203
Advisories: See page 146 – 2005 Potential Premature Battery Depletion Due to Battery Short	

Malfunctions (US)	118
Therapy Function Not Compromised	55
Battery (2 malfunctions related to advisory)	4
Electrical Component	22
Possible Early Battery Depletion	29
Therapy Function Compromised	63
Battery (35 malfunctions related to advisory)	42
Electrical Component	21

NBD Code	VVED
Serial Number Prefix	PKC
Max Delivered Energy	30 J
Estimated Longevity	See page 33

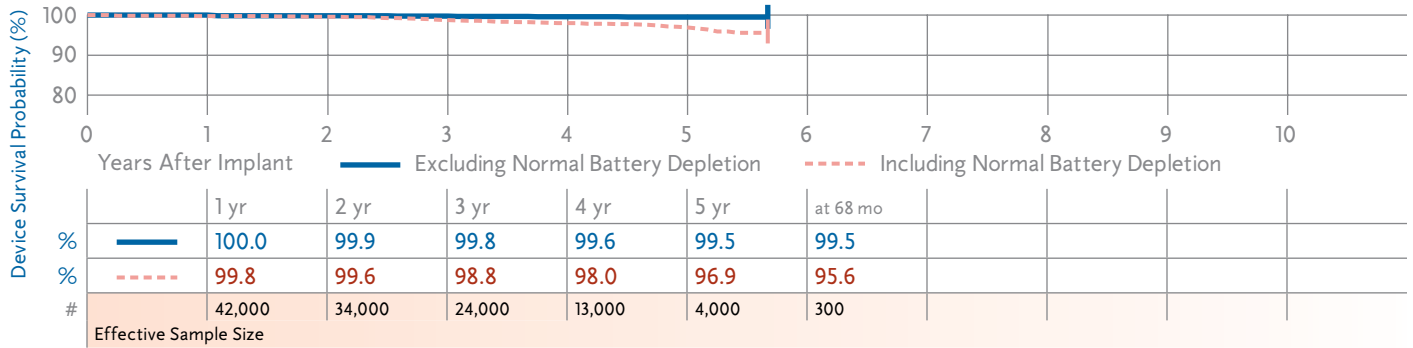


7275 GEM III DR

Product Characteristics

US Market Release	Nov-00
Registered US Implants	20,000
Estimated Active US Implants	3,000
Normal Battery Depletions (US)	1,980
Performance Note: see page 157 – Performance note on ICD Battery Discharge Behavior	

Malfunctions (US)	39
Therapy Function Not Compromised	28
Battery	1
Electrical Component	11
Software/Firmware	1
Possible Early Battery Depletion	15
Therapy Function Compromised	11
Battery	2
Electrical Component	8
Electrical Interconnect	1


NBD Code	VVED
Serial Number Prefix	PJM
Max Delivered Energy	30 J
Estimated Longevity	See page 33

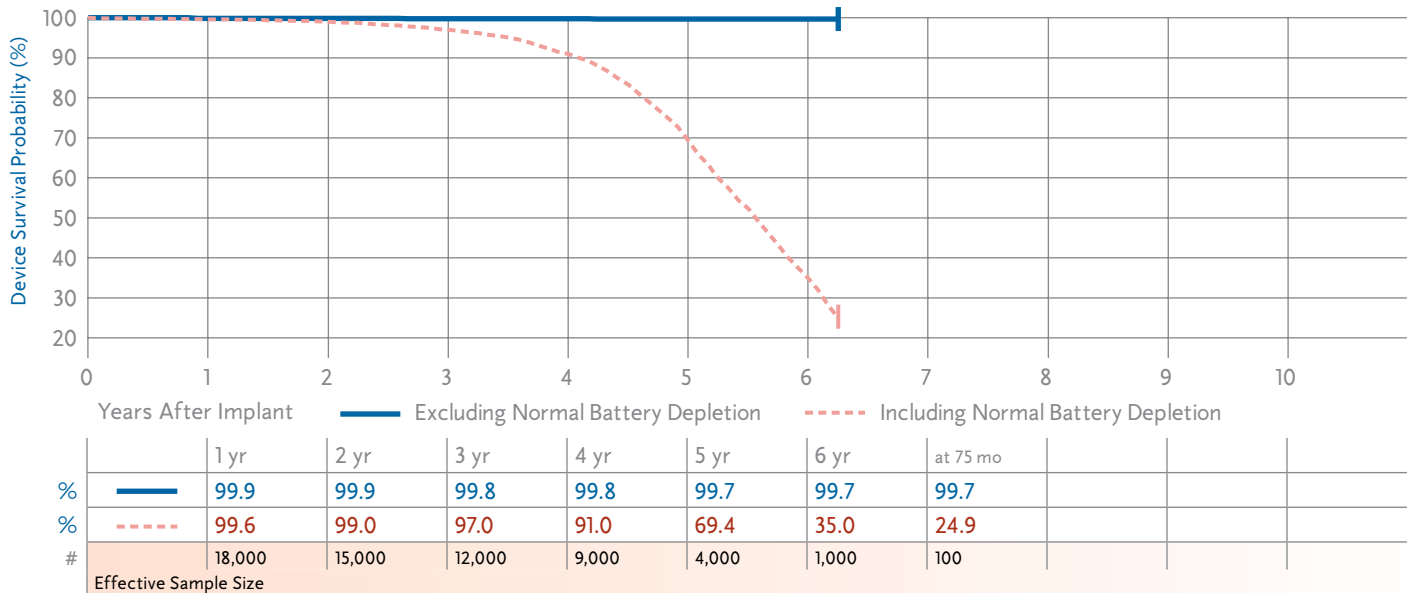

7276 GEM III AT

Product Characteristics


US Market Release	Feb-01	Malfunctions (US)	33	NBD Code	DDED
Registered US Implants	14,000	Therapy Function Not Compromised	26	Serial Number Prefix	PKE
Estimated Active US Implants	2,000	Electrical Component	6	Max Delivered Energy	30 J
Normal Battery Depletions (US)	1,535	Software/Firmware	1	Estimated Longevity	See page 33
Performance Note: see page 157 – Performance note on ICD Battery Discharge Behavior		Possible Early Battery Depletion	19		
		Therapy Function Compromised	7		
		Electrical Component	7		

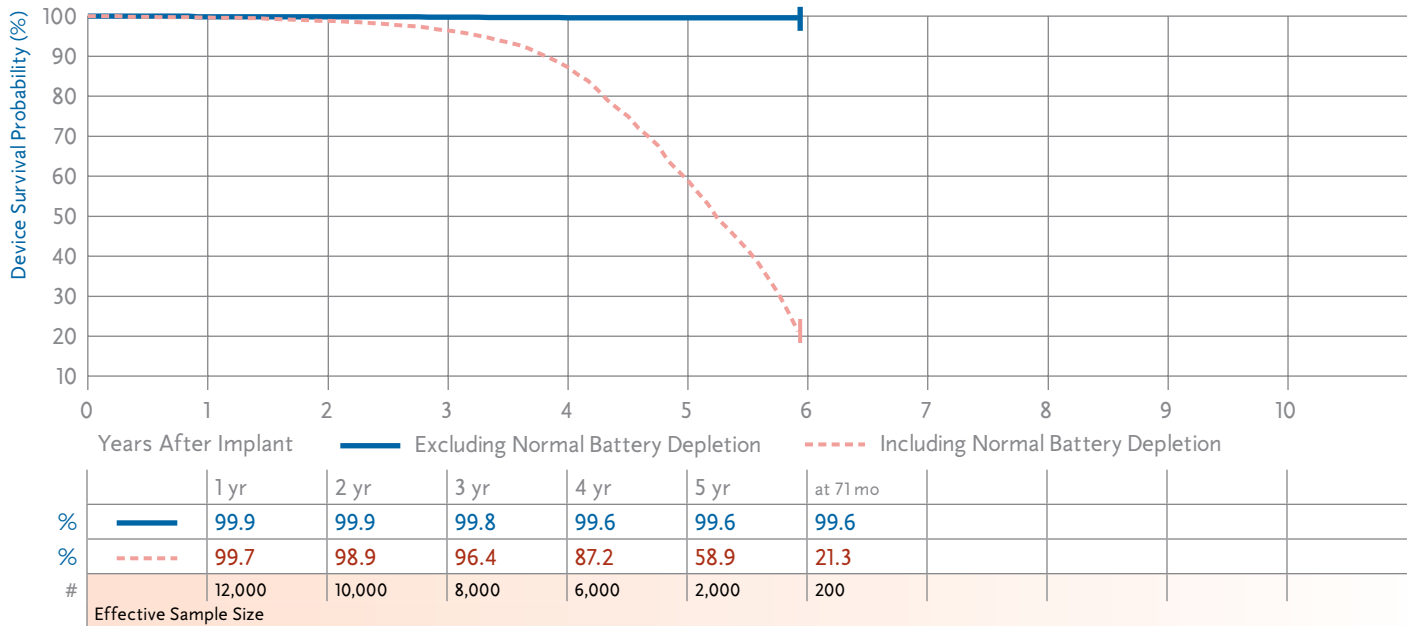

7278 Maximo DR

Product Characteristics


US Market Release	Oct-03	Malfunctions (US)	17	NBD Code	VVED
Registered US Implants	35,000	Therapy Function Not Compromised	10	Serial Number Prefix	PRM
Estimated Active US Implants	27,000	Electrical Component	7	Max Delivered Energy	35 J
Normal Battery Depletions (US)	22	Possible Early Battery Depletion	3	Estimated Longevity	See page 33
Advisories: See page 146 – 2005 Potential Premature Battery Depletion Due to Battery Short		Therapy Function Compromised	7		
		Electrical Component	6		
		Possible Early Battery Depletion	1		

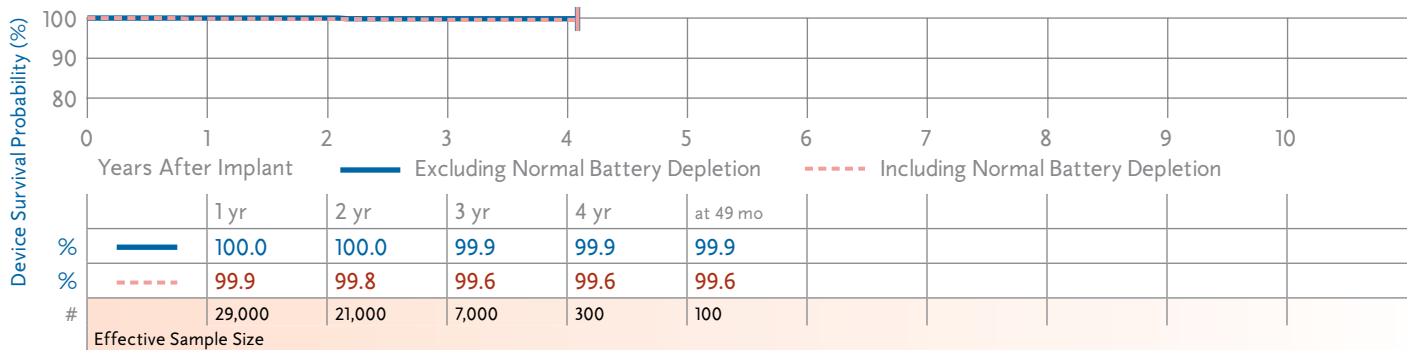

7288 Intrinsic

Product Characteristics


US Market Release	Aug-04	Malfunctions (US)	22	NBD Code	VVED
Registered US Implants	30,000	Therapy Function Not Compromised	16	Serial Number Prefix	PUB
Estimated Active US Implants	25,000	Battery	2	Max Delivered Energy	35 J
Normal Battery Depletions (US)	12	Electrical Component	7	Estimated Longevity	See page 33
Advisories	None	Software/Firmware	1		
		Possible Early Battery Depletion	6		
		Therapy Function Compromised	6		
		Electrical Component	6		

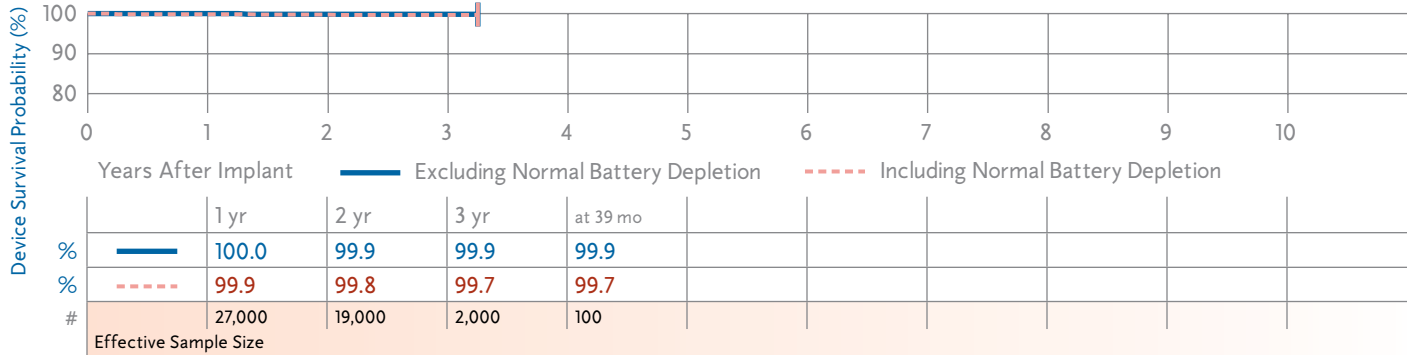

7290 Onyx

Product Characteristics


US Market Release	Mar-04	Malfunctions (US)	3	NBD Code	VVEV
Registered US Implants	1,000	Therapy Function Not Compromised	2	Serial Number Prefix	PRP
Estimated Active US Implants	1,000	Electrical Component	2	Max Delivered Energy	30 J
Normal Battery Depletions (US)	1	Therapy Function Compromised	1	Estimated Longevity	See page 33
Advisories	None	Electrical Component	1		

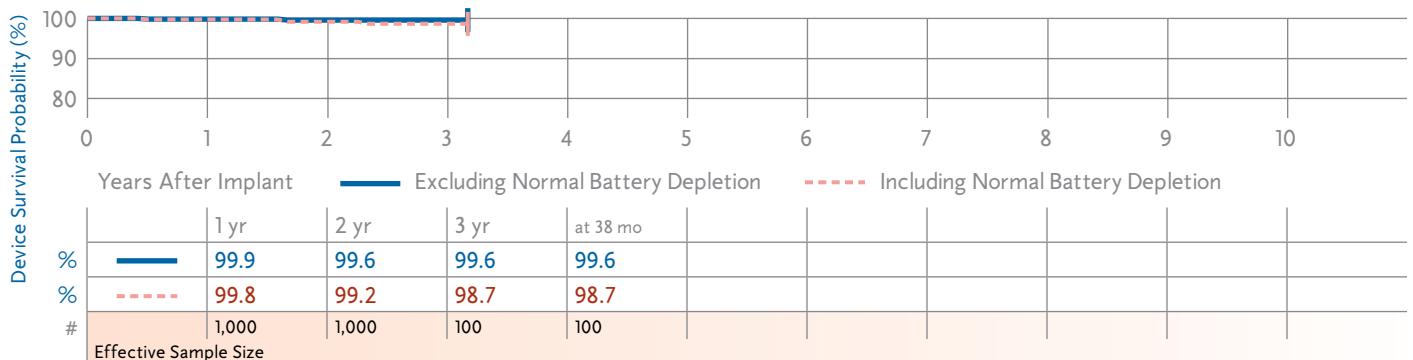

D153ATG, D153DRG EnTrust

Product Characteristics


US Market Release	Jun-05	Malfunctions (US)	3	NBD Code	DDED, VVED
Registered US Implants	400	Therapy Function Not Compromised	2	Serial Number Prefix	PNR
Estimated Active US Implants	300	Possible Early Battery Depletion	2	Max Delivered Energy	30 J
Normal Battery Depletions (US)	0	Therapy Function Compromised	1	Estimated Longevity	See page 34
Advisories	None	Electrical Component	1		

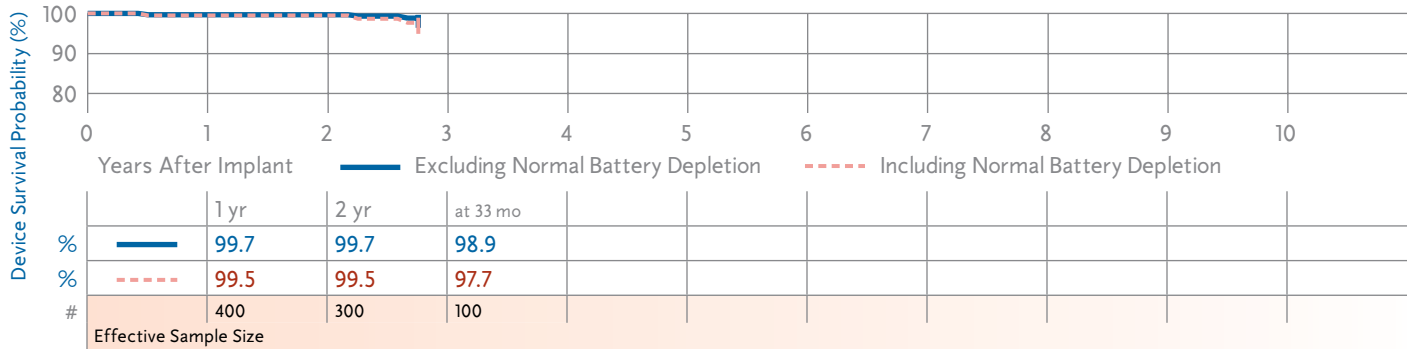

D154ATG, D154DRG EnTrust

Product Characteristics


US Market Release	Jun-05	Malfunctions (US)	9	NBD Code	DDED, VVED
Registered US Implants	26,000	Therapy Function Not Compromised	5	Serial Number Prefix	PNR
Estimated Active US Implants	23,000	Electrical Component	2	Max Delivered Energy	35 J
Normal Battery Depletions (US)	5	Possible Early Battery Depletion	3	Estimated Longevity	See page 34
Advisories	None	Therapy Function Compromised	4		
		Electrical Component	4		

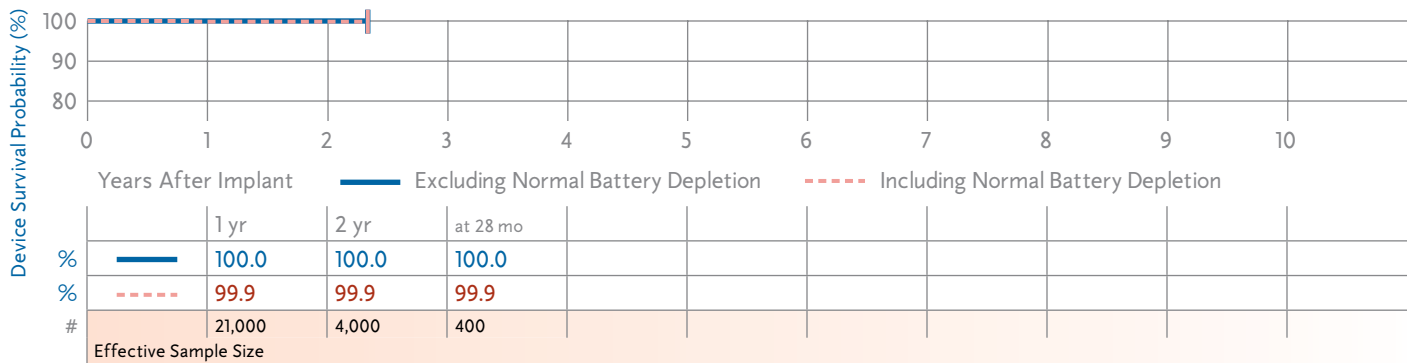

D154AWG, D164AWG Virtuoso

Product Characteristics


US Market Release	May-06	Malfunctions (US)	9	NBD Code	VVED
Registered US Implants	33,000	Therapy Function Not Compromised	2	Serial Number Prefix	PVV, PUL
Estimated Active US Implants	32,000	Electrical Component	2	Max Delivered Energy	35 J
Normal Battery Depletions (US)	2	Therapy Function Compromised	7	Estimated Longevity	See page 34
Advisories	None	Electrical Component	7		

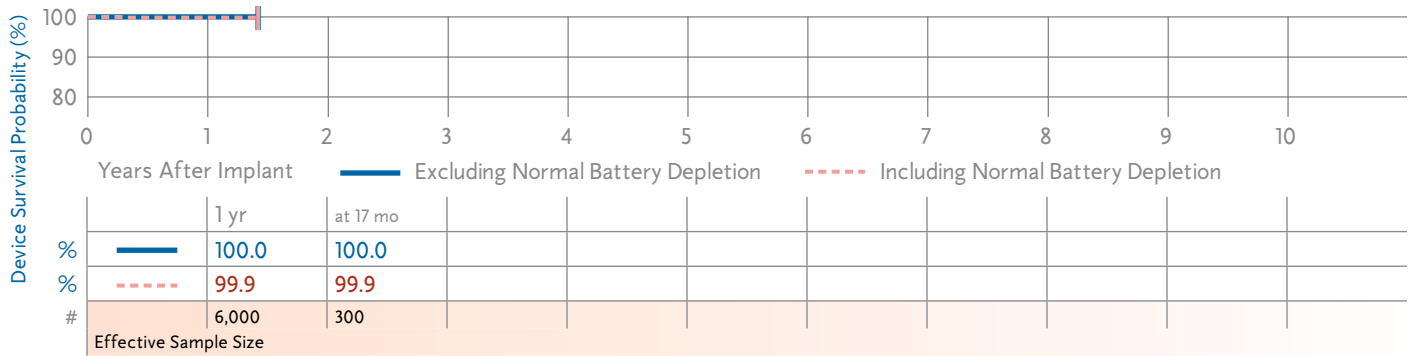

D154VRC EnTrust

Product Characteristics


US Market Release	Jun-05	Malfunctions (US)	9	NBD Code	VVEV
Registered US Implants	14,000	Therapy Function Not Compromised	6	Serial Number Prefix	PNT
Estimated Active US Implants	12,000	Electrical Component	1	Max Delivered Energy	35 J
Normal Battery Depletions (US)	1	Possible Early Battery Depletion	5	Estimated Longevity	See page 34
Advisories	None	Therapy Function Compromised	3		
		Electrical Component	3		

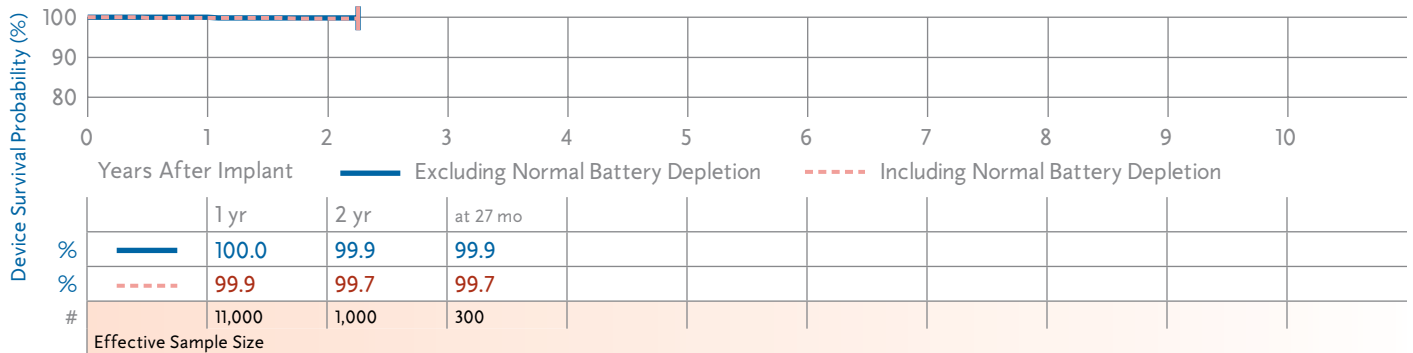

D154VWC, D164VWC Virtuoso

Product Characteristics

US Market Release	May-06	Malfunctions (US)	5	NBD Code	VVEV
Registered US Implants	13,000	Therapy Function Not Compromised	1	Serial Number Prefix	PUN
Estimated Active US Implants	12,000	Electrical Interconnect	1	Max Delivered Energy	35 J
Normal Battery Depletions (US)	1	Therapy Function Compromised	4	Estimated Longevity	See page 34
Advisories	None	Electrical Component	4		

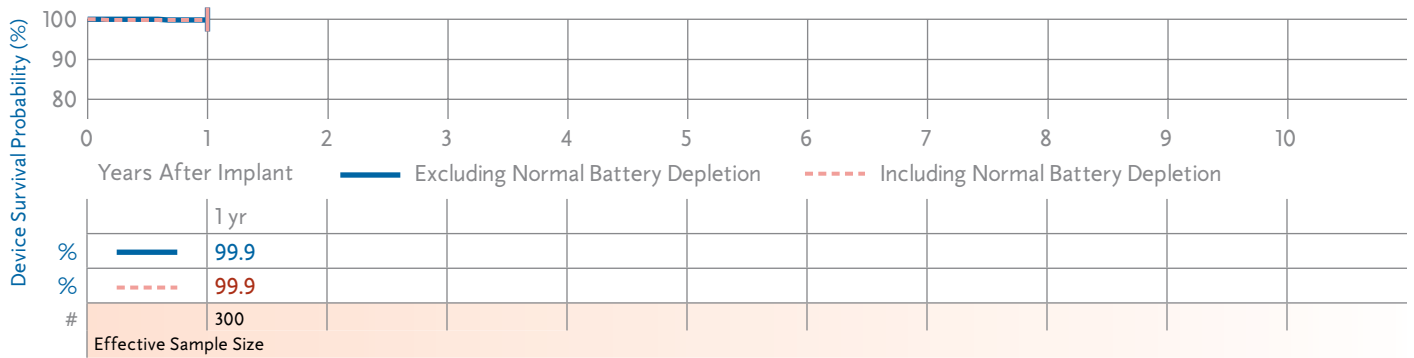

Device Survival Summary (95% Confidence Interval)

The following table shows ICD device survival estimates with 95% confidence intervals. Estimates are shown both with and without normal battery depletions included.

Model Number	Family	US Market Release	Registered US Implants	Estimated Active US Implants	Normal Battery Depletions (US)	Malfunctions (US)			Device Survival Probability (%)									
						Therapy Function Compromised	Therapy Function Not Compromised	Total	Years After Implant									
									1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	
7227	GEM	Oct-98	22,000	6,000	749	—	—	140	99.7 +0.1/-0.1	99.6 +0.1/-0.1	99.5 +0.1/-0.1	99.4 +0.1/-0.1	99.2 +0.1/-0.1	99.2 +0.1/-0.2	99.1 +0.1/-0.2	99.1 +0.1/-0.2	99.1 +0.1/-0.2	99.1 +0.1/-0.2 at 108 mo
	Advisories: see page 148 – 1999 Potential Circuit Overload						—	—	—	99.3 +0.1/-0.1	99.0 +0.1/-0.1	98.7 +0.1/-0.2	98.2 +0.2/-0.2	97.5 +0.2/-0.3	95.8 +0.4/-0.4	85.8 +0.8/-0.8	73.9 +1.2/-1.3	66.9 +1.7/-1.8 at 108 mo
7229	GEM II VR	Jul-99	11,000	1,000	994	—	—	26	99.9 +0.0/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.7 +0.1/-0.1	99.7 +0.1/-0.1	99.7 +0.1/-0.1	99.6 +0.1/-0.2	99.6 +0.1/-0.2	99.6 +0.1/-0.2	99.6 +0.1/-0.2 at 91 mo
	Advisories: see page 148 – 1999 Potential Circuit Overload; also see page 157 – Performance note on ICD Battery Discharge Behavior						—	—	—	99.8 +0.1/-0.1	99.5 +0.1/-0.2	99.3 +0.2/-0.2	98.4 +0.3/-0.3	94.4 +0.5/-0.6	84.2 +1.0/-1.0	56.5 +1.7/-1.7	32.9 +2.8/-2.8 at 91 mo	
7230	Marquis VR	Dec-02	19,000	10,000	8	6	15	= 21	100.0 +0.0/-0.0	99.9 +0.0/-0.1	99.9 +0.0/-0.1	99.9 +0.0/-0.1	99.8 +0.1/-0.2	99.8 +0.1/-0.2	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1
	Advisories: see page 146 – 2005 Potential Premature Battery Depletion Due to Battery Short						(0)	(0)	(0)	99.9 +0.0/-0.1	99.7 +0.1/-0.1	99.6 +0.1/-0.1	99.6 +0.1/-0.1	99.5 +0.2/-0.3	99.5 +0.2/-0.3	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1
7231	GEM III VR	Dec-00	17,000	9,000	223	8	23	= 31	99.9 +0.0/-0.1	99.9 +0.0/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1
	see page 157 – Performance note on ICD Battery Discharge Behavior						—	—	—	99.8 +0.1/-0.1	99.4 +0.1/-0.1	99.1 +0.1/-0.2	98.6 +0.2/-0.2	97.6 +0.3/-0.3	91.6 +0.8/-0.9	90.3 +1.0/-1.1 at 80 mo	90.3 +1.0/-1.1 at 80 mo	90.3 +1.0/-1.1 at 80 mo
7232	Maximo VR	Oct-03	41,000	33,000	7	6	12	= 18	100.0 +0.0/-0.0	100.0 +0.0/-0.0	99.9 +0.0/-0.0	99.9 +0.0/-0.0	99.9 +0.0/-0.0	99.9 +0.0/-0.0	99.9 +0.0/-0.0	99.9 +0.0/-0.0	99.9 +0.0/-0.0	99.9 +0.0/-0.0
	Advisories: see page 146 – 2005 Potential Premature Battery Depletion Due to Battery Short						(0)	(0)	(0)	99.9 +0.0/-0.0	99.9 +0.0/-0.0	99.8 +0.0/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1
7271	GEM DR	Oct-98	15,000	3,000	652	—	—	88	99.9 +0.0/-0.1	99.8 +0.1/-0.1	99.7 +0.1/-0.1	99.5 +0.1/-0.2	99.3 +0.1/-0.2	99.1 +0.2/-0.2	99.0 +0.2/-0.2	99.0 +0.2/-0.2	99.0 +0.2/-0.2	99.0 +0.2/-0.2 at 104 mo
	Advisories: see page 146 – 2005 Potential Premature Battery Depletion Due to Battery Short						—	—	—	99.7 +0.1/-0.1	99.5 +0.1/-0.1	98.8 +0.2/-0.2	97.8 +0.3/-0.3	96.0 +0.4/-0.4	91.2 +0.7/-0.7	82.9 +1.0/-1.1	59.8 +2.1/-2.1	46.6 +3.4/-3.4 at 104 mo
7274	Marquis DR	Mar-02	48,000	21,000	203	63	55	= 118	100.0 +0.0/-0.0	99.9 +0.0/-0.0	99.8 +0.0/-0.1	99.6 +0.1/-0.1	99.5 +0.1/-0.1	99.5 +0.1/-0.1	99.5 +0.1/-0.1	99.5 +0.1/-0.1	99.5 +0.1/-0.1	99.5 +0.1/-0.1 at 68 mo
	Advisories: see page 146 – 2005 Potential Premature Battery Depletion Due to Battery Short						(35)	(2)	(37)	99.8 +0.0/-0.0	99.6 +0.1/-0.1	98.8 +0.1/-0.1	98.0 +0.2/-0.2	96.9 +0.3/-0.3	95.6 +0.5/-0.6	95.6 +0.5/-0.6	95.6 +0.5/-0.6	95.6 +0.5/-0.6

continued

Device Survival Summary continued

Model Number	Family	US Market Release	Registered US Implants	Estimated Active US Implants	Normal Battery Depletions	Malfunctions		Device Survival Probability (%)													
						Therapy Function Compromised	Therapy Function Not Compromised	Years After Implant													
						TI	II + 28 = 39	1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr					
7275	GEM III DR	Nov-00	20,000	3,000	1,980	11	28	= 39	Normal Battery Depletion	99.9 +0.0/-0.0	99.9 +0.0/-0.1	99.8 +0.1/-0.1	99.8 +0.1/-0.1	99.7 +0.1/-0.1	99.7 +0.1/-0.1	99.7 +0.1/-0.1	99.7 +0.1/-0.1	99.7 +0.1/-0.1	99.7 +0.1/-0.1	99.7 +0.1/-0.1	
7276	GEM III AT	Feb-01	14,000	2,000	1,535	7	26	= 33	Excluding Normal Battery Depletion	99.9 +0.1/-0.1	99.9 +0.1/-0.2	99.8 +0.3/-0.3	99.8 +0.3/-0.3	99.7 +0.3/-0.3	99.7 +0.3/-0.3	99.6 +0.3/-0.3	99.6 +0.3/-0.3	99.6 +0.3/-0.3	99.6 +0.3/-0.3	99.6 +0.3/-0.3	
7278	Maximo DR	Oct-03	35,000	27,000	22	7	10	= 17	Including Normal Battery Depletion	99.7 +0.1/-0.1	98.9 +0.2/-0.2	96.4 +0.3/-0.4	87.2 +0.7/-0.8	58.9 +1.4/-1.4	21.3 +2.3/-2.2	99.9 +0.0/-0.0	99.9 +0.0/-0.0	99.9 +0.0/-0.0	99.9 +0.0/-0.0	99.9 +0.0/-0.0	99.9 +0.0/-0.0
7288	Intrinsic	Aug-04	30,000	25,000	12	6	16	= 22	Including Normal Battery Depletion	99.9 +0.0/-0.0	99.8 +0.1/-0.1	99.6 +0.1/-0.1	99.6 +0.1/-0.1	99.6 +0.1/-0.1	99.6 +0.1/-0.1	99.6 +0.1/-0.1	99.6 +0.1/-0.1	99.6 +0.1/-0.1	99.6 +0.1/-0.1	99.6 +0.1/-0.1	
7290	Oryx	Mar-04	1,000	1,000	1	1	2	= 3	Excluding Normal Battery Depletion	99.9 +0.1/-0.7	99.6 +0.3/-0.9	99.6 +0.3/-0.9	99.6 +0.3/-0.9	99.6 +0.3/-0.9	99.6 +0.3/-0.9	99.6 +0.3/-0.9	99.6 +0.3/-0.9	99.6 +0.3/-0.9	99.6 +0.3/-0.9	99.6 +0.3/-0.9	
D154ATG, D153DRG	EnTrust DR	Jun-05	400	300	0	1	2	= 3	Including Normal Battery Depletion	99.7 +0.2/-1.5	99.7 +0.2/-1.5	98.9 +0.8/-2.4	98.9 +0.8/-2.4	98.9 +0.8/-2.4	98.9 +0.8/-2.4	98.9 +0.8/-2.4	98.9 +0.8/-2.4	98.9 +0.8/-2.4	98.9 +0.8/-2.4	98.9 +0.8/-2.4	
D154ATG, D154DRG	EnTrust DR	Jun-05	26,000	23,000	5	4	5	= 9	Including Normal Battery Depletion	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	

continued

Device Survival Summary continued

Model Number	Family	US Market Release	Registered US Implants	Estimated Active US Implants	Normal Battery Depletions	Malfunctions			Device Survival Probability (%)										
						Therapy Function Compromised	Therapy Function Not Compromised	Total	Years After Implant										
					Depletions	7	+	2	=	9	1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	
D154AWG D164AWG	Virtuoso DR	May-06	33,000	32,000	2	7	+	2	=	9	Excluding Normal Battery Depletion	100.0 +0.0/-0.0 at 17 mo	100.0 +0.0/-0.0 at 17 mo						
											Including Normal Battery Depletion	99.9 +0.0/-0.0 at 17 mo	99.9 +0.0/-0.0 at 17 mo						
D154VRC	EnTrust VR	Jun-05	14,000	12,000	1	3	+	6	=	9	Excluding Normal Battery Depletion	100.0 +0.0/-0.1	99.9 +0.1/-0.1 at 27 mo	99.9 +0.1/-0.1 at 27 mo					
											Including Normal Battery Depletion	99.9 +0.0/-0.1	99.7 +0.1/-0.2 at 27 mo	99.7 +0.1/-0.2 at 27 mo					
D154VWC, D164VWC	Virtuoso VR	May-06	13,000	12,000	1	4	+	1	=	5	Excluding Normal Battery Depletion	99.9 +0.0/-0.1							
											Including Normal Battery Depletion	99.9 +0.1/-0.1							

Reference Chart

The longevity estimates provided are mean values calculated for the parameters given. The actual longevity achieved for any device while implanted will depend on the actual programmed parameters and patient factors, and may differ significantly from these estimates.

Model Number	Family	Connector Style	Volume/ Mass*	Delivered Energy	Estimated Longevity					Elective Replacement (ERI)***		End of Life (EOL) Battery Voltage
					Charging Frequency**	100% Pacing‡	50% Pacing‡	15% Pacing‡	100% Sensing	Battery Voltage	Charge Time	
7227	GEM	B, Cx, D, E	49 cc* 90 g	35 J	Monthly	5.3	5.7	6.0	6.1	≤ 2.55 V	—	≤ 2.40 V [§]
					Quarterly	7.7	8.5	9.3	9.6			
					Semiannual	8.8	10.0	11.0	11.5			
7229	GEM II VR	Cx	39 cc 77 g	30 J	Monthly	3.6	3.9	4.1	4.2	≤ 2.55 V	—	≤ 2.40 V
					Quarterly	5.0	5.5	6.0	6.2			
					Semiannual	5.6	6.3	6.9	7.1			
7230	Marquis VR	B, Cx, E	36 cc 75 g	30 J	Monthly	4.9	5.2	5.4	5.5	≤ 2.62 V	> 16-second charge time	3 months after ERI
					Quarterly	7.3	8.0	8.5	8.7			
					Semiannual	8.5	9.3	10.0	10.4			
7231	GEM III VR	Cx	39 cc 77 g	30 J	Monthly	4.3	4.7	5.0	5.2	≤ 2.55 V	—	≤ 2.40 V
					Quarterly	6.0	6.8	7.4	7.8			
					Semiannual	6.6	7.5	8.5	8.9			
7232	Maximo VR	B, Cx, E	39 cc 76 g	35 J	Monthly	4.4	4.7	4.8	4.9	≤ 2.62 V	> 16-second charge time	3 months after ERI
					Quarterly	7.0	7.5	8.0	8.3			
					Semiannual	8.2	9.0	9.7	10.0			
7271	GEM DR	DR	62 cc 115 g	35 J	Monthly	6.0	6.9	7.5	7.8	≤ 4.91 V	—	≤ 4.57 V [§]
					Quarterly	7.4	8.4	9.3	9.8			
					Semiannual	7.9	9.0	10.0	10.6			
7274	Marquis DR	DR+LV	36 cc 75 g	30 J	Monthly	4.0	4.4	4.8	4.9	≤ 2.62 V	> 16-second charge time	3 months after ERI
					Quarterly	5.6	6.4	7.1	7.5			
					Semiannual	6.2	7.2	8.1	8.6			
7275	GEM III DR	DR	39.5 cc 78 g	30 J	Monthly	3.3	3.8	4.3	4.4	≤ 2.55 V	—	≤ 2.40 V
					Quarterly	4.2	5.0	5.8	6.3			
					Semiannual	4.5	5.5	6.5	7.0			
7276	GEM III AT	DR	39 cc 77 g	30 J	Monthly	3.3	3.8	4.3	4.5	≤ 2.55 V	—	≤ 2.40 V
					Quarterly	4.3	5.1	5.9	6.3			
					Semiannual	4.5	5.5	6.5	7.0			
7278	Maximo DR	DR	39 cc 77 g	35 J	Monthly	3.7	4.1	4.3	4.5	≤ 2.62 V	> 16-second charge time	3 months after ERI
					Quarterly	5.3	6.1	6.8	7.1			
					Semiannual	6.0	7.0	8.0	8.5			
7287	Intrinsic 30	DR	36 cc 75 g	30 J	Monthly	4.0	4.3	4.7	4.8	≤ 2.62 V	> 16-second charge time	3 months after ERI
					Quarterly	5.5	6.3	7.0	7.4			
					Semiannual	6.2	7.2	8.2	8.6			
7288	Intrinsic	DR	38 cc 76 g	35 J	Monthly	3.7	4.1	4.3	4.5	≤ 2.62 V	> 16-second charge time	3 months after ERI
					Quarterly	5.4	6.1	6.8	7.1			
					Semiannual	6.1	7.0	8.0	8.5			
7290	Onyx	Cx	39 cc 77 g	30 J	Monthly	3.8	4.1	4.3	4.5	≤ 2.55 V	> 16-second charge time	≤ 2.40 V
					Quarterly	5.0	5.6	6.2	6.4			
					Semiannual	5.4	6.1	6.7	7.0			

* Volume and mass differ by connector style.

** A full charge is a full energy therapeutic shock or capacitor reformation.

*** The minimum time between ERI and EOL is 3 months (100% pacing, two charges per month).

‡ Pacing mode is VVI for single chamber models and DDD for dual chamber and CRT models. Parameter settings: lower rate at 60 ppm, sensing rate at 70 bpm, (A, RV, LV) 3.0 V amplitude, 0.4 ms pulse width, and 510 ohm pace load per applicable channel. CRT models with shared biventricular pacing: InSync Marquis 7277 (LV impedance set to 510 ohms), InSync ICD 7272 (RV amplitude set to 4.0 V).

‡‡ For Model 7223 devices, if charge time exceeds 60 seconds, the devices are at EOL. If 2 consecutive charge cycles exceed 60 seconds, the "charge circuit inactive" indicator is tripped and all therapies except emergency output VVI pacing are disabled.

§ For Model 7271 and 7227 devices, if charge time exceeds 30 seconds, the device is at EOL. Immediate replacement is recommended. If 3 consecutive charge cycles exceed 30 seconds, the "charge circuit inactive" indicator is tripped and all therapies except emergency VVI pacing are disabled.



Reference Chart continued

Model Number	Family	Connector Style	Volume/ Mass*	Delivered Energy	Estimated Longevity					Recommended Replacement (RRT)***		End of Service (EOS)
					Charging Frequency**	100% Pacing†	50% Pacing†	15% Pacing†	100% Sensing	Battery Voltage	Charge Time	
D153ATG, D153DRG	EnTrust	DR	33 cc 63 g	30 J	Monthly	3.5	3.8	4.1	4.2	≤ 2.61 V	—	3 months after RRT or > 16-second charge time
					Quarterly	4.8	5.4	6.0	6.3			
					Semiannual	5.3	6.1	6.9	7.2			
D153VRC	EnTrust	Cx	32 cc 63 g	30 J	Monthly	4.4	4.7	4.9	5.0	≤ 2.61 V	—	3 months after RRT or > 16-second charge time
					Quarterly	6.8	7.4	7.9	8.1			
					Semiannual	7.9	8.7	9.5	9.8			
D154ATG, D154DRG	EnTrust	DR	35 cc 68 g	35 J	Monthly	3.8	4.2	4.4	4.6	≤ 2.61 V	—	3 months after RRT or > 16-second charge time
					Quarterly	5.5	6.1	6.8	7.0			
					Semiannual	6.1	7.0	7.9	8.3			
D154AWG, D164AWG	Virtuoso	DR	37 cc 68 g	35 J	Monthly	4.1	4.5	4.8	5.0	≤ 2.62 V	—	3 months after RRT or > 19-second charge time
					Quarterly	6.3	7.3	8.3	8.8			
					Semiannual	7.3	8.7	10.1	11.0			
D154VRC	EnTrust	Cx	35 cc 68 g	35 J	Monthly	4.8	5.0	5.2	5.3	≤ 2.61 V	—	3 months after RRT or > 16-second charge time
					Quarterly	7.5	8.3	8.8	9.0			
					Semiannual	9.0	10.0	10.7	11.0			
D154VWC, D164VWC	Virtuoso	Cx	37 cc 68 g	35 J	Monthly	4.8	5.1	5.3	5.4	≤ 2.62 V	—	3 months after RRT or > 19-second charge time
					Quarterly	8.1	9.0	9.6	10.0			
					Semiannual	10.0	11.2	12.3	12.9			










* Volume and mass differ by connector style.

** A full charge is a full energy therapeutic shock or capacitor reformation.

*** The minimum time between RRT and EOS is 3 months (100% pacing, two charges per month).

† Pacing mode is VVI for single chamber models and DDD for dual chamber models. Parameter settings: lower rate at 60 ppm, sensing rate at 70 bpm, (A, RV, LV) 3.0 V amplitude, 0.4 ms pulse width, and 510 ohm pace load per applicable channel.

ICD Connector Styles

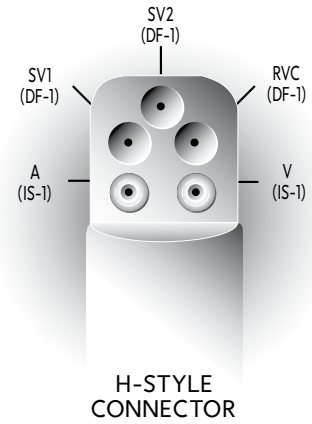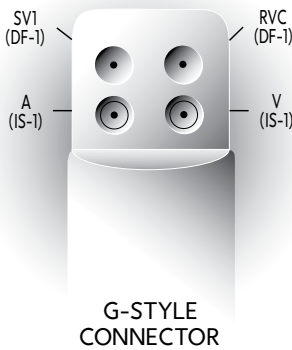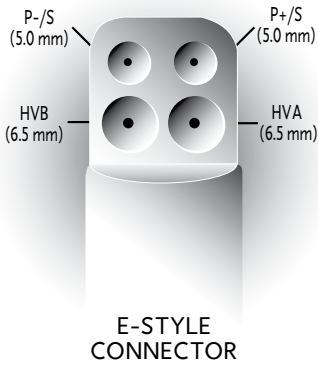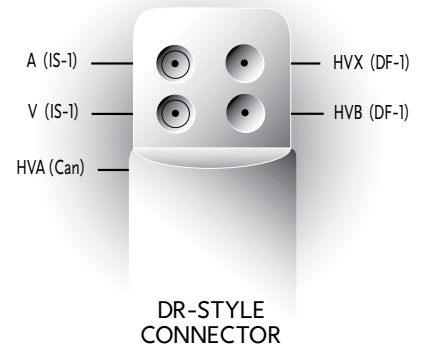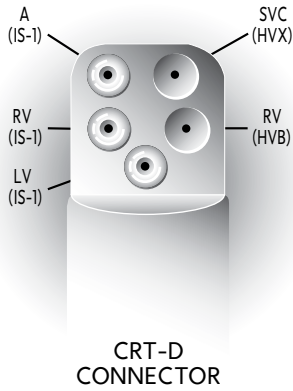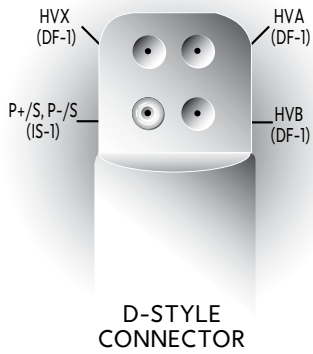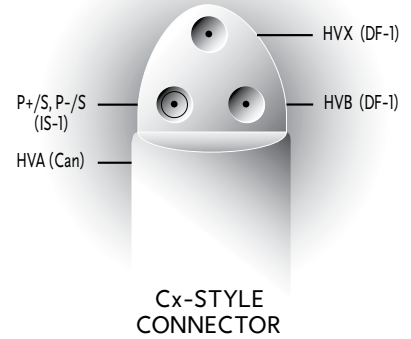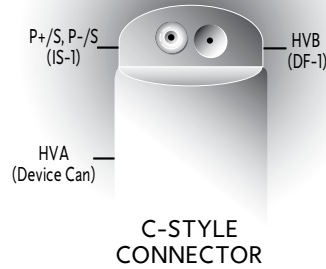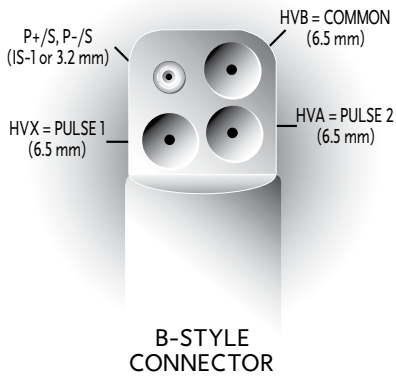


Adapta DR ADDR01, ADDR03, ADDR06, ADD01

Product Characteristics

US Market Release	Jul-06
Registered US Implants	58,000
Estimated Active US Implants	55,000
Normal Battery Depletions (US)	0
Advisories	None

Malfunctions (US)	3
Therapy Function Not Compromised	3
Electrical Component	3
Therapy Function Compromised	0

NBD Code	DDDR, DDD
Serial Number Prefix	PWB, PWD, PWC
Estimated Longevity	See page 71

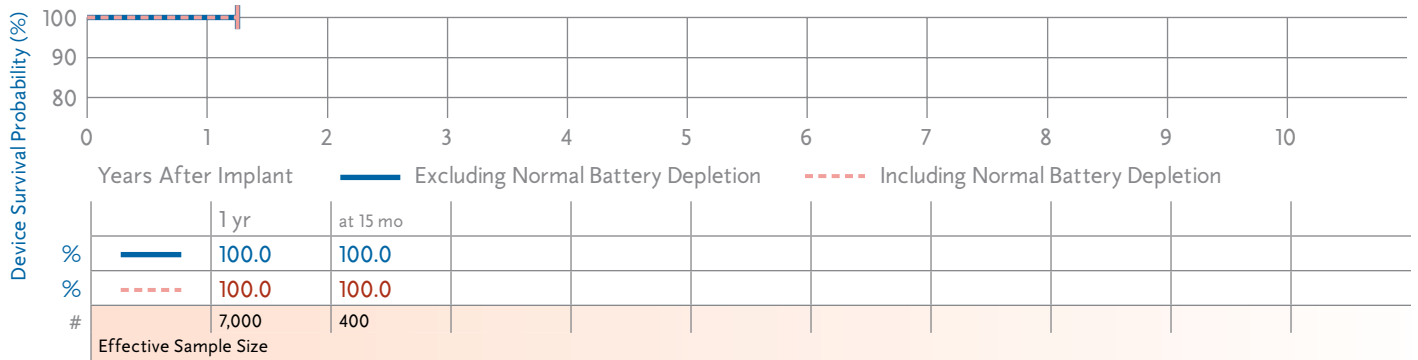


Adapta DR ADDR1

Product Characteristics

US Market Release	Jul-06
Registered US Implants	4,000
Estimated Active US Implants	3,000
Normal Battery Depletions (US)	0
Advisories	None

Malfunctions (US)	0
Therapy Function Not Compromised	0
Therapy Function Compromised	0

NBG Code	SSIR
Serial Number Prefix	PWM, PWP, PWN
Estimated Longevity	See page 71

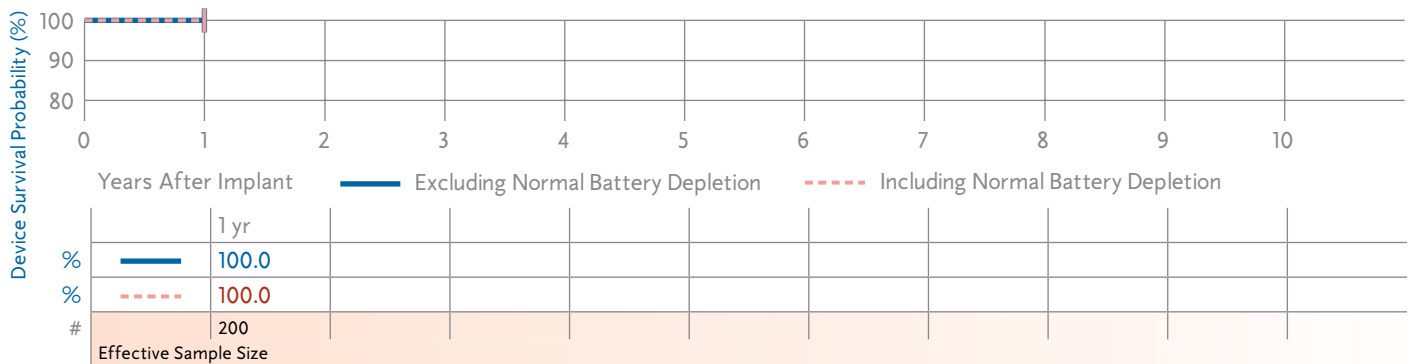


Adapta DR ADDR1

Product Characteristics

US Market Release	Jul-06
Registered US Implants	5,000
Estimated Active US Implants	5,000
Normal Battery Depletions (US)	0
Advisories	None

Malfunctions (US)	0
Therapy Function Not Compromised	0
Therapy Function Compromised	0

NBG Code	SSIR
Serial Number Prefix	PWM, PWP, PWN
Estimated Longevity	See page 71

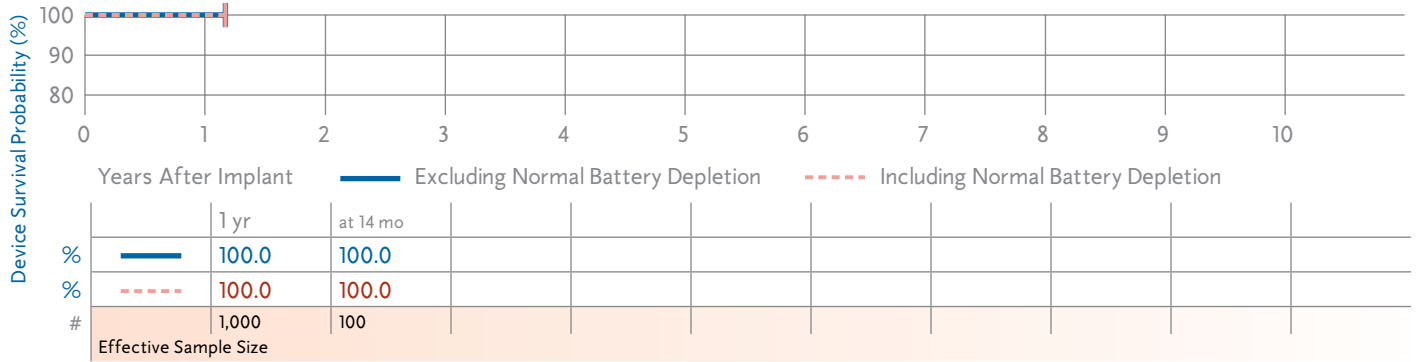


Adapta SR ADSR01, ADSR03, ADSR06

Product Characteristics

US Market Release	Jul-06
Registered US Implants	11,000
Estimated Active US Implants	10,000
Normal Battery Depletions (US)	0
Advisories	None

Malfunctions (US)	0
Therapy Function Not Compromised	0
Therapy Function Compromised	0

NBG Code	SSIR
Serial Number Prefix	PWM, PWP, PWN
Estimated Longevity	See page 71

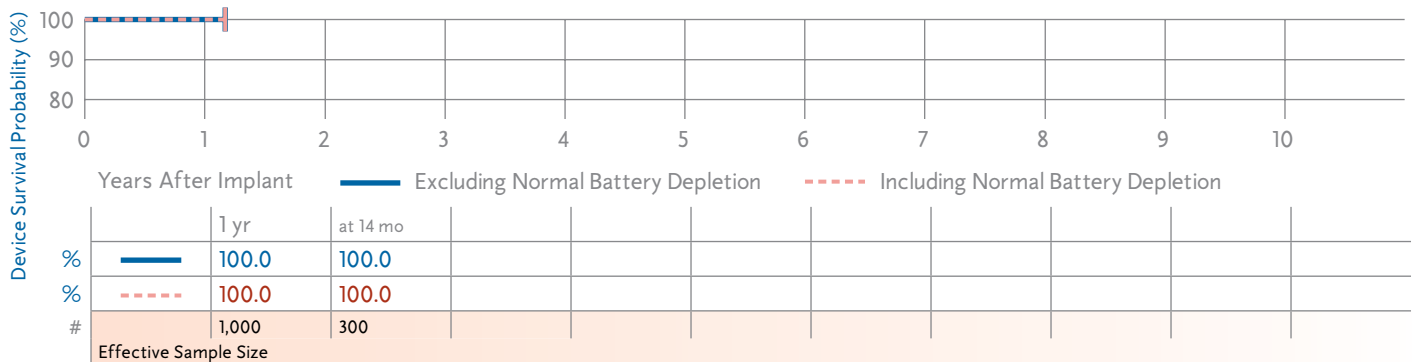


AT500 AT501, 7253

Product Characteristics

US Market Release	Mar-03
Registered US Implants	11,000
Estimated Active US Implants	7,000
Normal Battery Depletions (US)	149
Performance Note: see page 155 – Performance note on AT500 Pacing System Follow-Up Protocol	

Malfunctions (US)	10
Therapy Function Not Compromised	5
Electrical Component	2
Possible Early Battery Depletion	3
Therapy Function Compromised	5
Electrical Component	3
Electrical Interconnect	1
Possible Early Battery Depletion	1

NBG Code	DDDRP
Serial Number Prefix	IJF
Estimated Longevity	See page 71

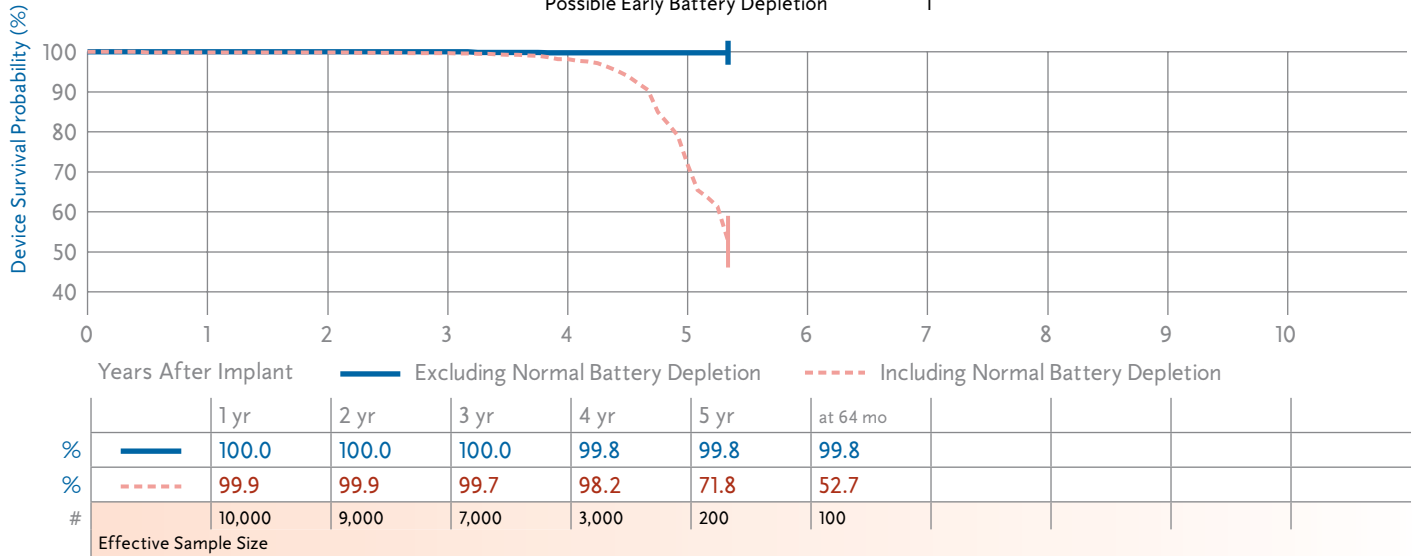


EnPulse DR EIDR01, EIDR03, EIDR06

Product Characteristics

US Market Release	Dec-03
Registered US Implants	7,000
Estimated Active US Implants	5,000
Normal Battery Depletions (US)	4
Advisories	None

Malfunctions (US)	1
Therapy Function Not Compromised	1
Electrical Component	1
Therapy Function Compromised	0

NBG Code	DDDR
Serial Number Prefix	PRA
Estimated Longevity	See page 71

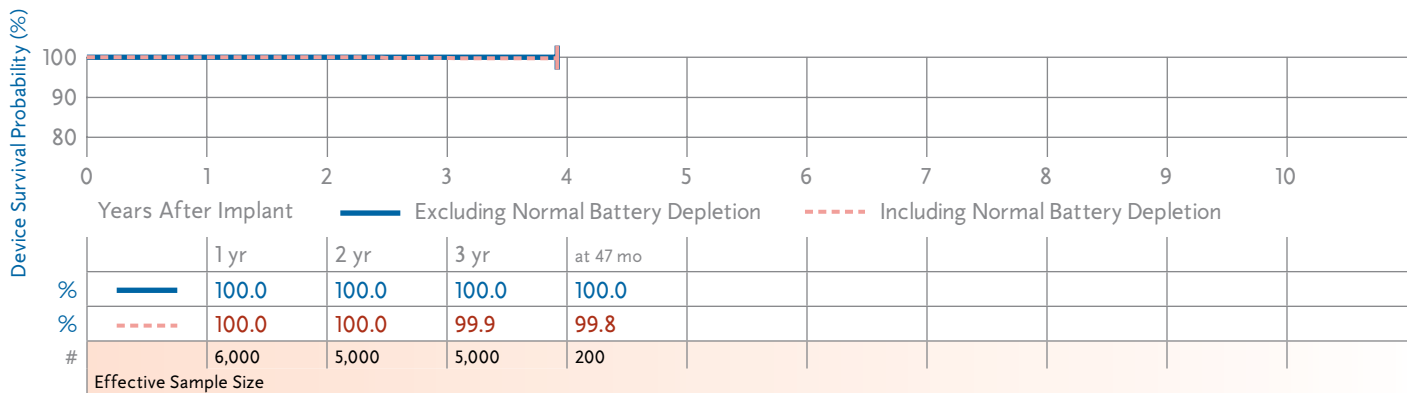


EnPulse DR E1DR21

Product Characteristics

US Market Release	Dec-03
Registered US Implants	2,000
Estimated Active US Implants	1,000
Normal Battery Depletions (US)	3
Advisories	None

Malfunctions (US)	0
Therapy Function Not Compromised	0
Therapy Function Compromised	0

NBG Code	DDDR
Serial Number Prefix	PPT
Estimated Longevity	See page 71

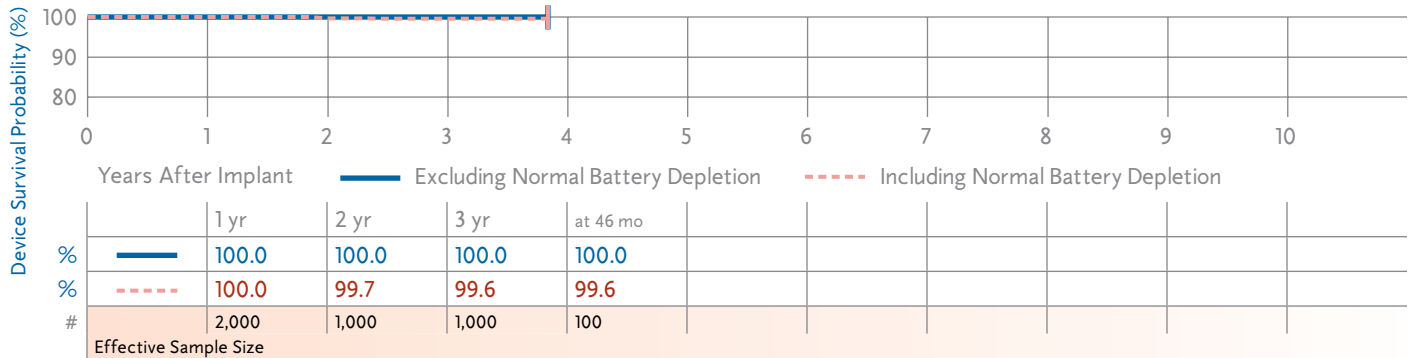


EnPulse 2 DR E2DR01, E2DR03, E2DR06

Product Characteristics

US Market Release	Feb-04
Registered US Implants	101,000
Estimated Active US Implants	78,000
Normal Battery Depletions (US)	6
Advisories	None

Malfunctions (US)	8
Therapy Function Not Compromised	5
Electrical Component	5
Therapy Function Compromised	3
Battery	1
Electrical Component	2

NBG Code	DDDR
Serial Number Prefix	PNB, PNC, PNH
Estimated Longevity	See page 71

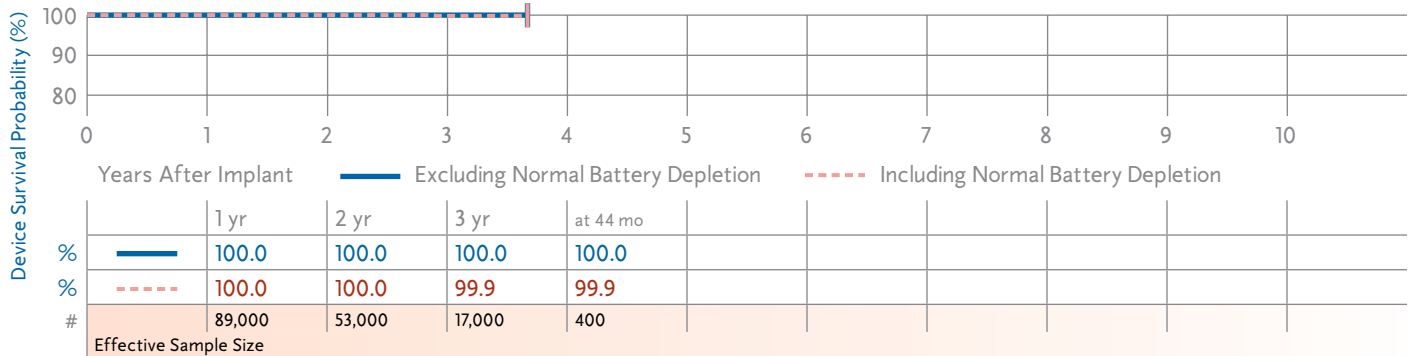


EnPulse 2 DR E2DR21

Product Characteristics

US Market Release	Feb-04
Registered US Implants	12,000
Estimated Active US Implants	9,000
Normal Battery Depletions (US)	11
Advisories	None

Malfunctions (US)	0
Therapy Function Not Compromised	0
Therapy Function Compromised	0

NBG Code	DDDR
Serial Number Prefix	PMU
Estimated Longevity	See page 71

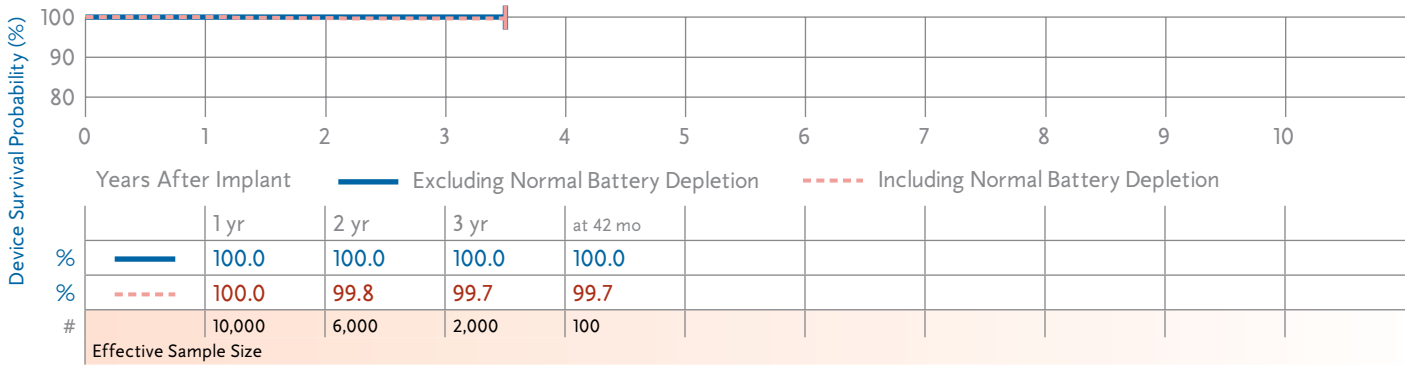


EnPulse 2 DR E2DR31, E2DR33

Product Characteristics

US Market Release	Feb-04
Registered US Implants	1,000
Estimated Active US Implants	500
Normal Battery Depletions (US)	0
Advisories	None

Malfunctions (US)	0
Therapy Function Not Compromised	0
Therapy Function Compromised	0


NBG Code	DDDR
Serial Number Prefix	PNL
Estimated Longevity	See page 71

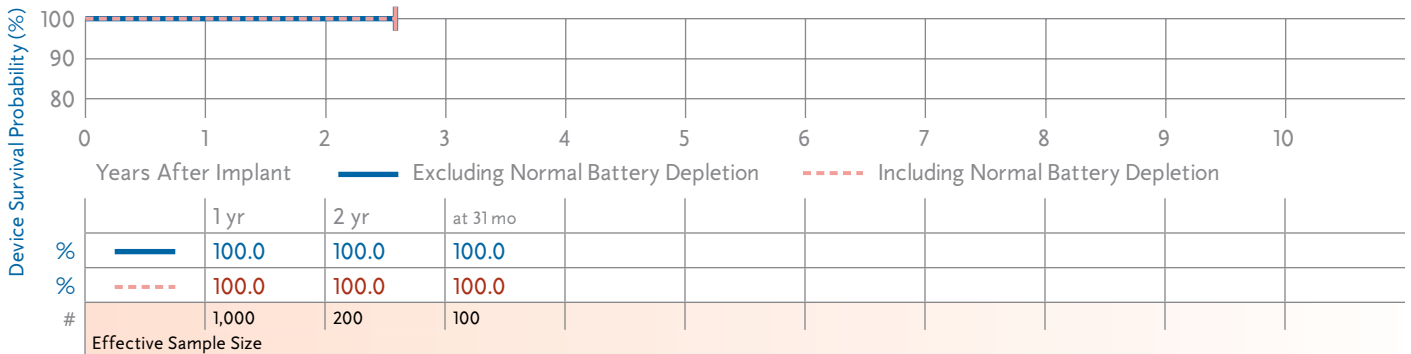

EnPulse 2 SR E2SR01, E2SR03, E2SR06

Product Characteristics


US Market Release	Dec-03	Malfunctions (US)	3	NBG Code	SSIR
Registered US Implants	25,000	Therapy Function Not Compromised	2	Serial Number Prefix	PMW, PMY, PNA
Estimated Active US Implants	18,000	Electrical Component	1	Estimated Longevity	See page 71
Normal Battery Depletions (US)	6	Possible Early Battery Depletion	1		
Advisories	None	Therapy Function Compromised	1		
		Other	1		

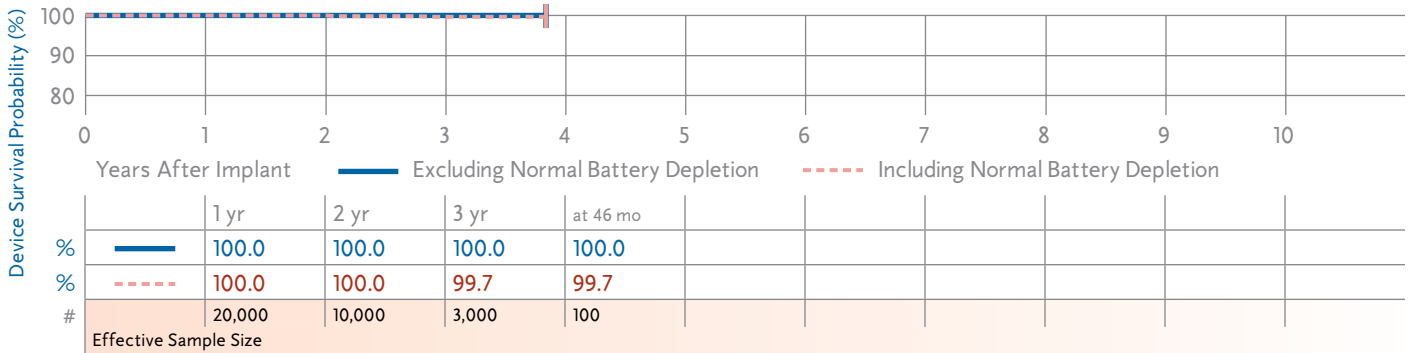

EnPulse 2 VDD E2VDD01

Product Characteristics


US Market Release	Dec-03	Malfunctions (US)	0	NBG Code	VDD
Registered US Implants	1,000	Therapy Function Not Compromised	0	Serial Number Prefix	PMV
Estimated Active US Implants	1,000	Therapy Function Compromised	0	Estimated Longevity	See page 71
Normal Battery Depletions (US)	0				
Advisories	None				

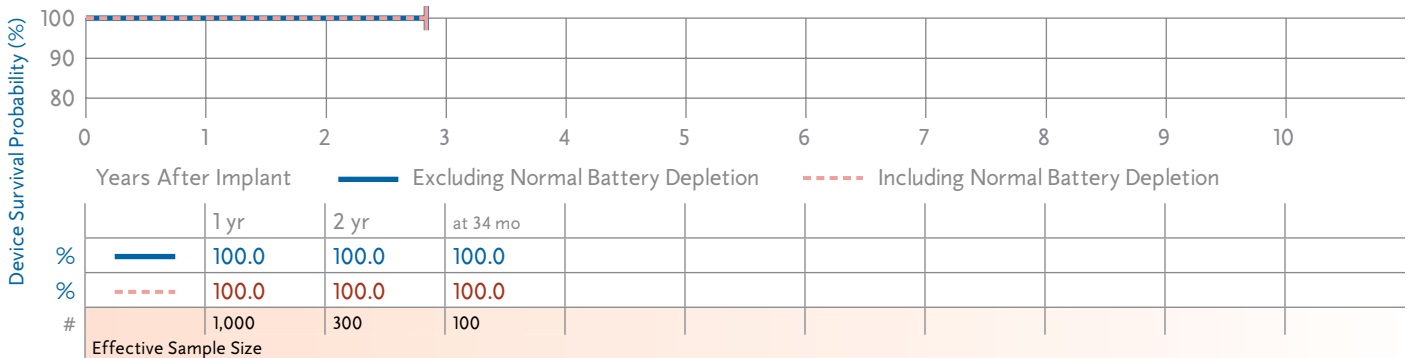

EnRhythm DR P1501DR

Product Characteristics


US Market Release	May-05	Malfunctions (US)	18	NBG Code	DDDRP
Registered US Implants	64,000	Therapy Function Not Compromised	5	Serial Number Prefix	PNP
Estimated Active US Implants	55,000	Electrical Component	5	Estimated Longevity	See page 71
Normal Battery Depletions (US)	0	Therapy Function Compromised	13		
Advisories	None	Electrical Component	13		

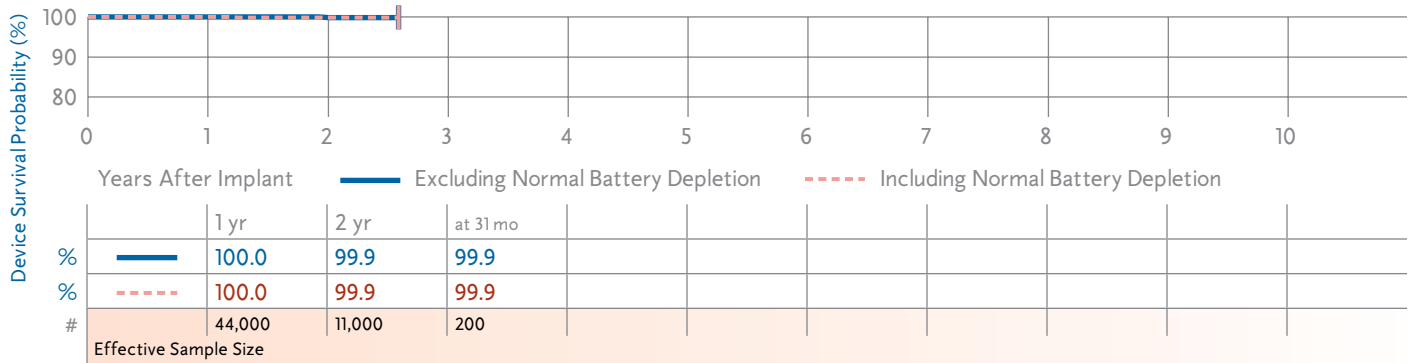

Kappa 400 DR KDR401, KDR403

Product Characteristics


US Market Release	Jan-98	Malfunctions (US)	22	NBG Code	DDD/RO
Registered US Implants	47,000	Therapy Function Not Compromised	13	Serial Number Prefix	PER, PET
Estimated Active US Implants	8,000	Electrical Component	9	Estimated Longevity	See page 71
Normal Battery Depletions (US)	3,269	Electrical Interconnect	1		
Advisories	None	Possible Early Battery Depletion	2		
		Other	1		
		Therapy Function Compromised	9		
		Electrical Component	7		
		Electrical Interconnect	2		

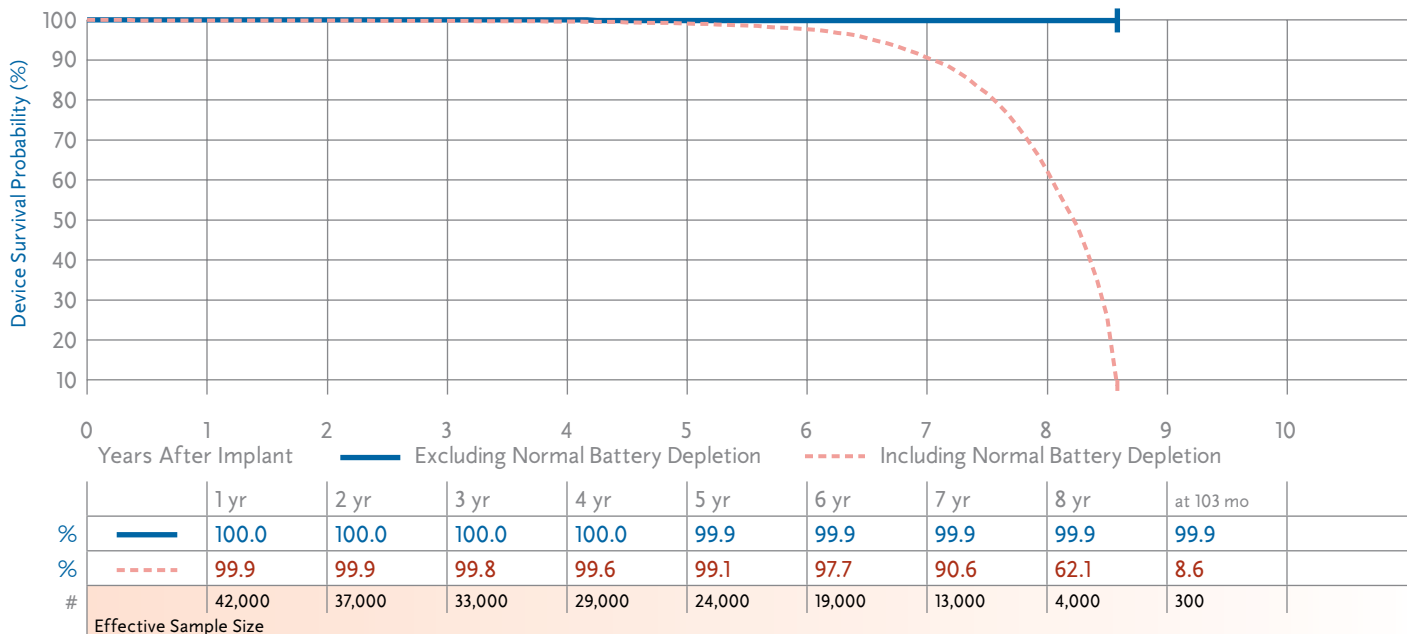

Kappa 400 SR KSR401, KSR403

Product Characteristics


US Market Release	Feb-98	Malfunctions (US)	4	NBG Code	SSI/R
Registered US Implants	15,000	Therapy Function Not Compromised	3	Serial Number Prefix	PEU, PGD
Estimated Active US Implants	4,000	Electrical Component	3	Estimated Longevity	See page 71
Normal Battery Depletions (US)	455	Therapy Function Compromised	1		
Advisories	None	Electrical Interconnect	1		

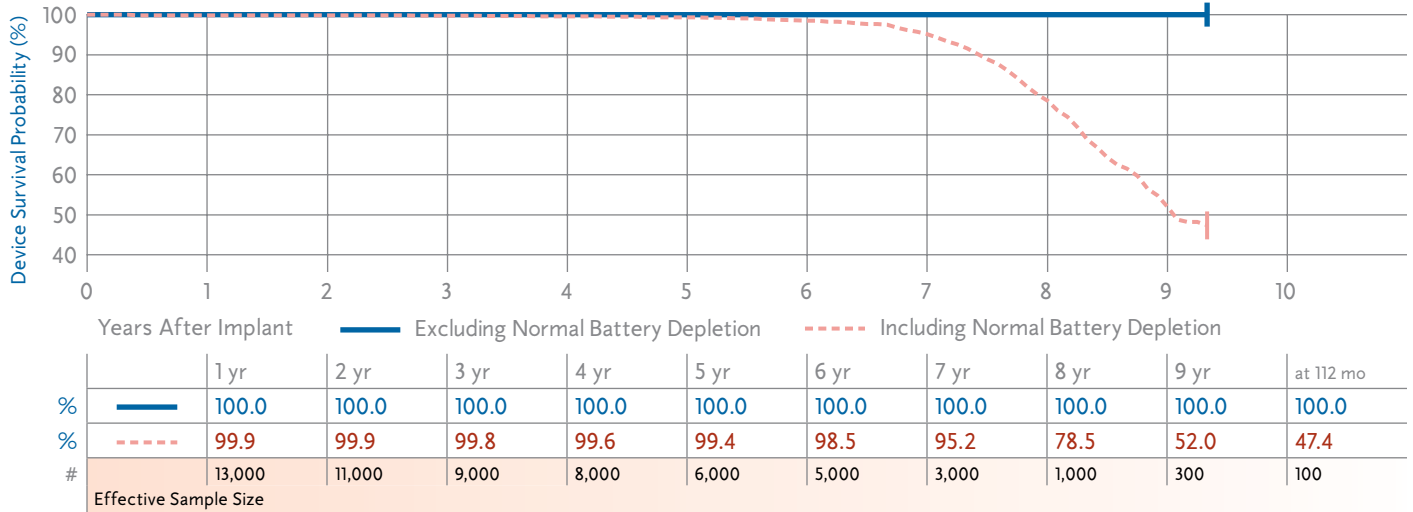

Kappa 600 DR KDR601, KDR603, KDR606

Product Characteristics


US Market Release	Jan-99	Malfunctions (US)	21	NBG Code	DDD/RO
Registered US Implants	24,000	Therapy Function Not Compromised	3	Serial Number Prefix	PHF, PHH, PHG
Estimated Active US Implants	7,000	Electrical Component	3	Estimated Longevity	See page 71
Normal Battery Depletions (US)	746	Therapy Function Compromised	18		
Advisories: See page 147 – 2002 Potential Fractured Power Supply Wires		Electrical Component	2		
		Electrical Interconnect	16		
		<i>(11 malfunctions related to advisory)</i>			

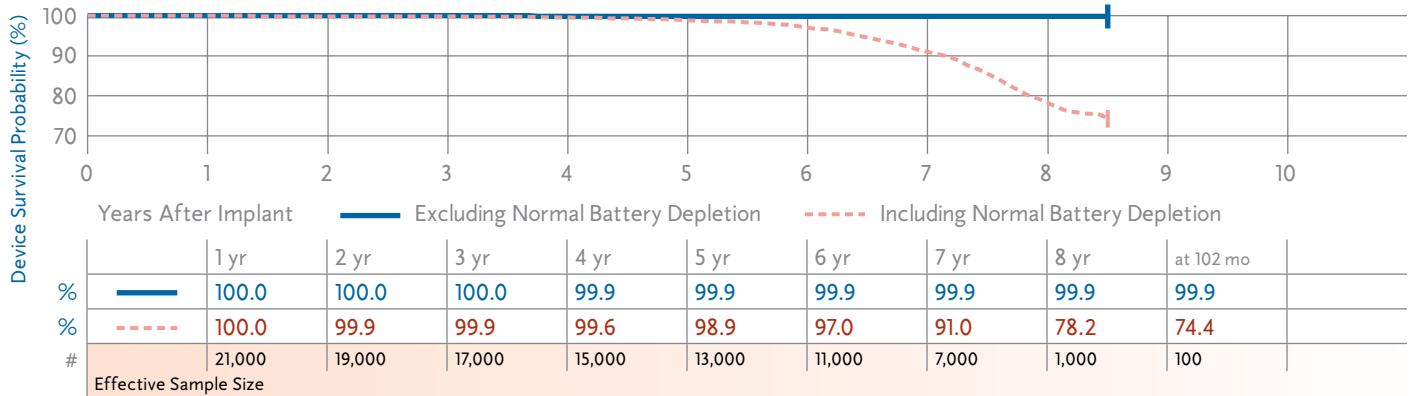

Kappa 600 DR KDR651, KDR653

Product Characteristics


US Market Release	Mar-01	Malfunctions (US)	6	NBG Code	DDD/RO
Registered US Implants	14,000	Therapy Function Not Compromised	2	Serial Number Prefix	PLJ, PLK
Estimated Active US Implants	7,000	Electrical Component	1	Estimated Longevity	See page 71
Normal Battery Depletions (US)	111	Possible Early Battery Depletion	1		
Advisories: See page 147 – 2002 Potential Fractured Power Supply Wires		Therapy Function Compromised	4		
		Electrical Component	1		
		Electrical Interconnect	3		
		<i>(1 malfunction related to advisory)</i>			

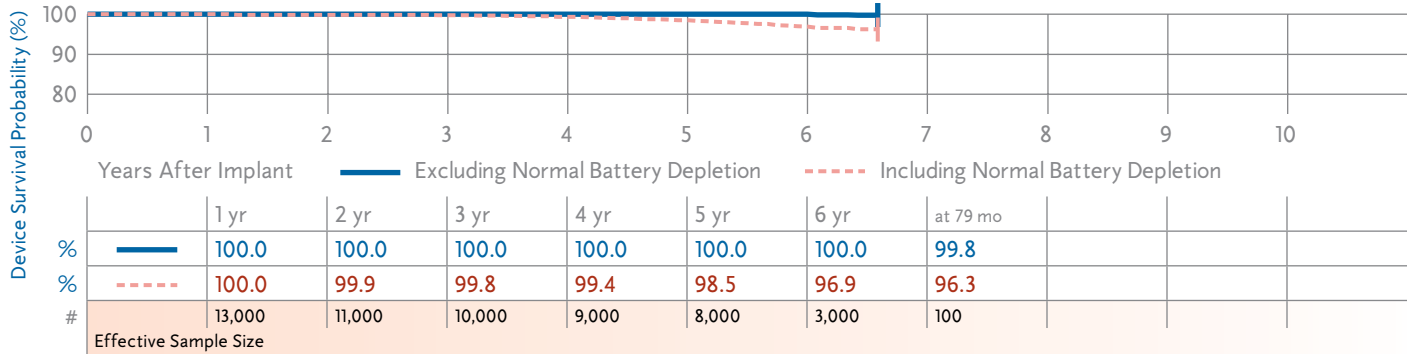

Kappa 700 D KD701, KD703, KD706

Product Characteristics

US Market Release	Jan-99	Malfunctions (US)	0	NBG Code	DDD
Registered US Implants	300	Therapy Function Not Compromised	0	Serial Number Prefix	PHK
Estimated Active US Implants	100	Therapy Function Compromised	0	Estimated Longevity	See page 72
Normal Battery Depletions (US)	5				
Advisories: See page 147 – 2002 Potential Fractured Power Supply Wires					

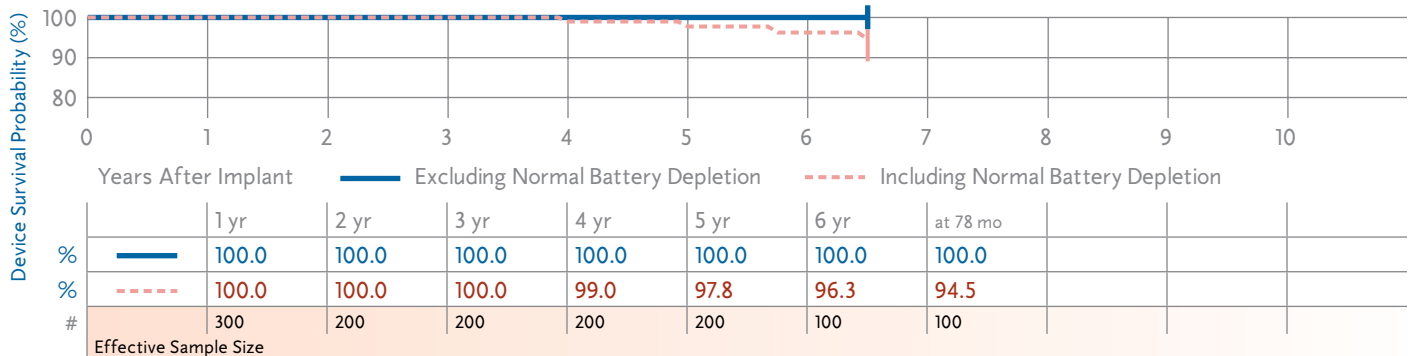

Kappa 700 DR KDR701, KDR703, KDR706

Product Characteristics


US Market Release	Feb-99
Registered US Implants	192,000
Estimated Active US Implants	84,000
Normal Battery Depletions (US)	3,732

Advisories: See page 147 – 2002 Potential Fractured Power Supply Wires

Malfunctions (US)	219
Therapy Function Not Compromised	27
Battery	1
Electrical Component	20
Electrical Interconnect	1
Possible Early Battery Depletion	3
Other	2
Therapy Function Compromised	192
Electrical Component	14
Electrical Interconnect	178

NBG Code	DDD/RO
Serial Number Prefix	PGU, PGY, PGW
Estimated Longevity	See page 72

(124 malfunctions related to advisory)

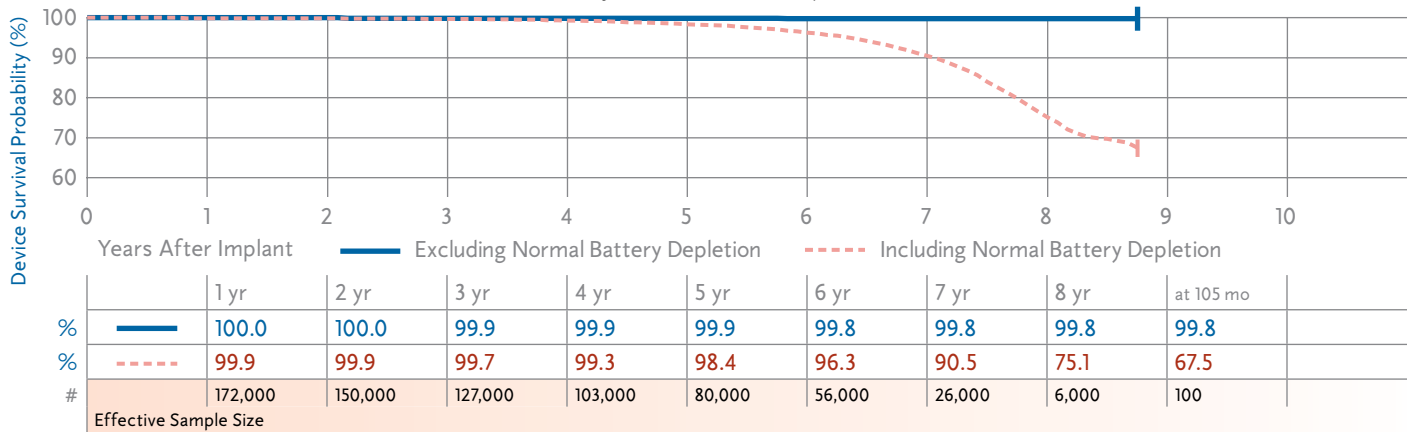

Kappa 700 DR KDR721

Product Characteristics


US Market Release	Feb-99
Registered US Implants	10,000
Estimated Active US Implants	1,000
Normal Battery Depletions (US)	806

Advisories: See page 147 – 2002 Potential Fractured Power Supply Wires

Malfunctions (US)	5
Therapy Function Not Compromised	1
Electrical Component	1
Therapy Function Compromised	4
Electrical Interconnect	4

NBG Code	DDD/RO
Serial Number Prefix	PGR
Estimated Longevity	See page 72


(4 malfunctions related to advisory)

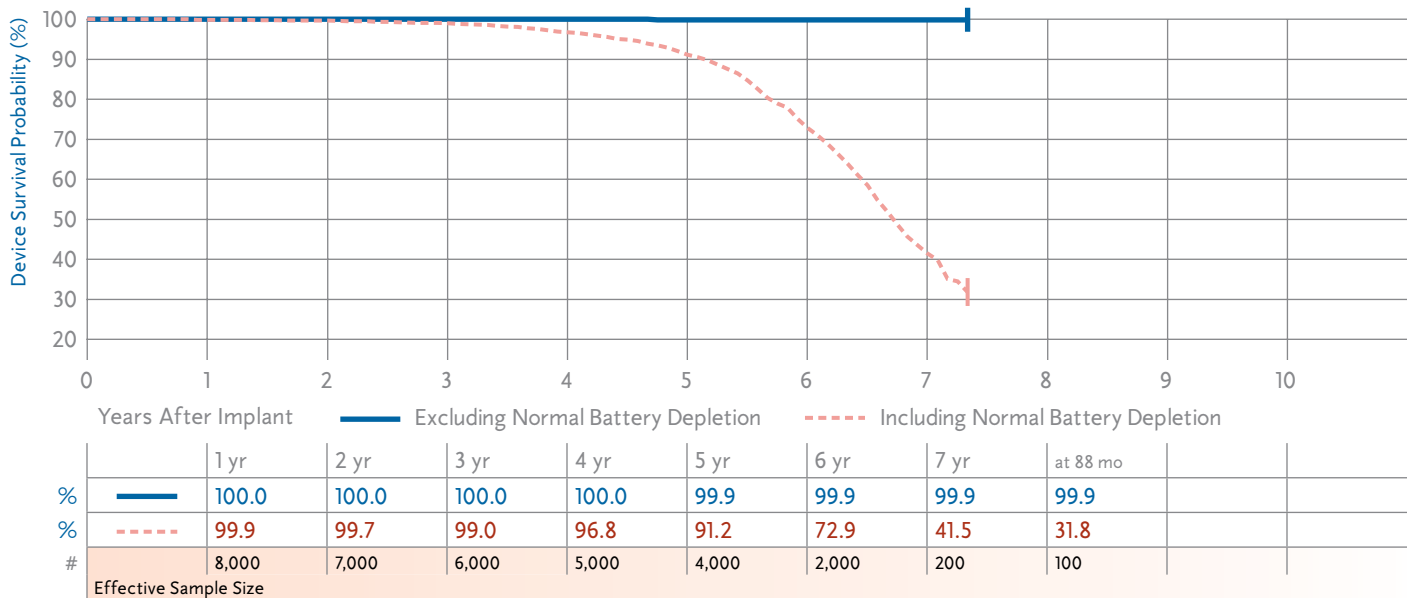

Kappa 700 SR KSR701, KSR703, KSR706

Product Characteristics


US Market Release	Feb-99	Malfunctions (US)	9	NBG Code	SSI/R
Registered US Implants	55,000	Therapy Function Not Compromised	3	Serial Number Prefix	PHT, PHW, PHU
Estimated Active US Implants	19,000	Electrical Component	2	Estimated Longevity	See page 72
Normal Battery Depletions (US)	866	Possible Early Battery Depletion	1		
Advisories	None	Therapy Function Compromised	6		
		Electrical Component	4		
		Electrical Interconnect	2		

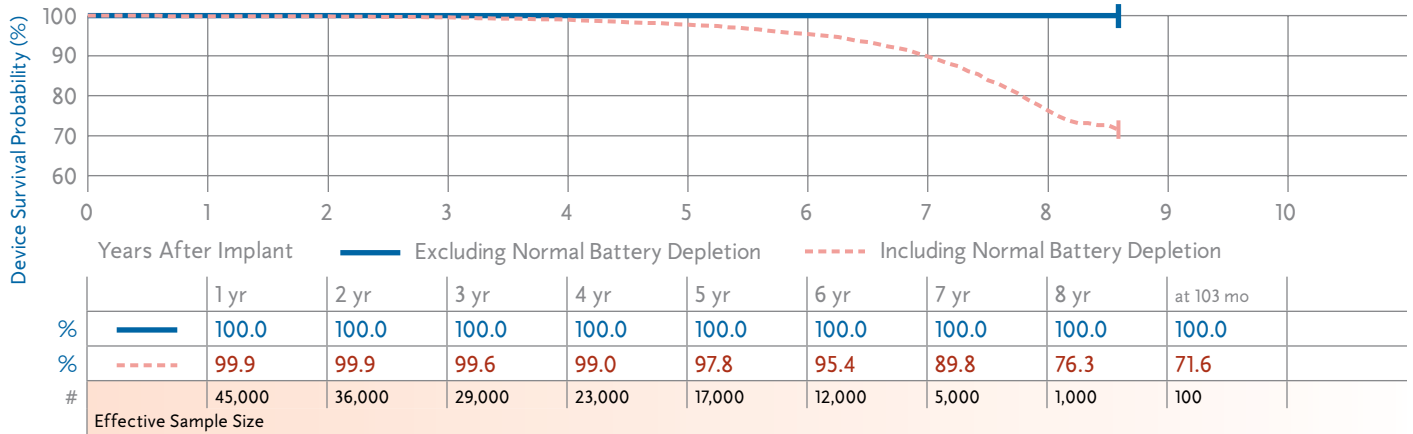

Kappa 700 VDD KVDD701

Product Characteristics


US Market Release	Jan-99	Malfunctions (US)	3	NBG Code	VDD/RO
Registered US Implants	2,000	Therapy Function Not Compromised	0	Serial Number Prefix	PHP
Estimated Active US Implants	400	Therapy Function Compromised	3	Estimated Longevity	See page 72
Normal Battery Depletions (US)	73	Electrical Interconnect	3		
Advisories: See page 147 – 2002 Potential Fractured Power Supply Wires		<i>(3 malfunctions related to advisory)</i>			

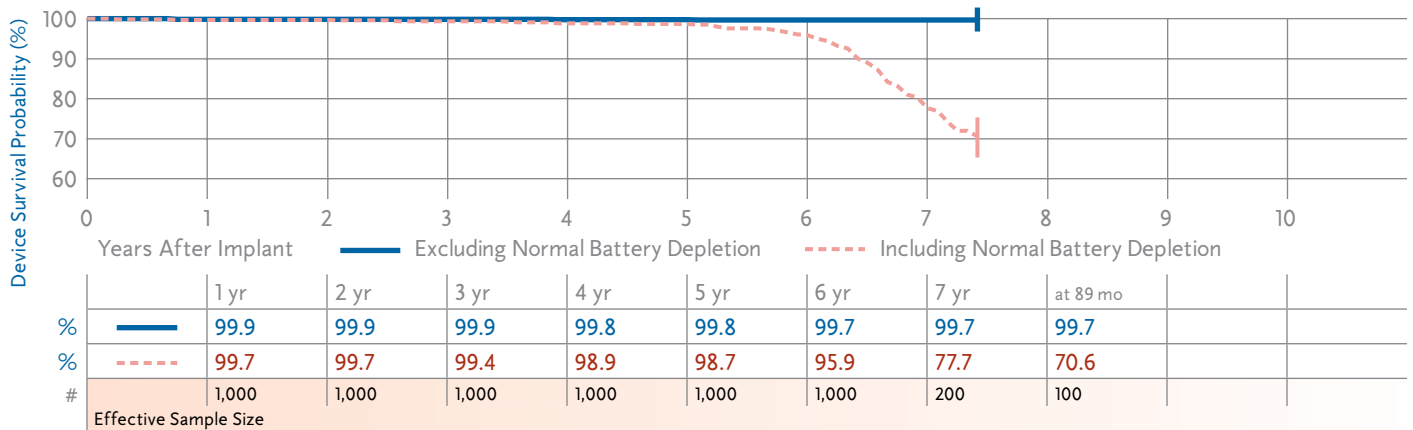

Kappa 800 DR KDR801, KDR803

Product Characteristics


US Market Release	Jan-02	Malfunctions (US)	0	NBG Code	DDD/RO
Registered US Implants	4,000	Therapy Function Not Compromised	0	Serial Number Prefix	PKW, PKY
Estimated Active US Implants	3,000	Therapy Function Compromised	0	Estimated Longevity	See page 72
Normal Battery Depletions (US)	4				
Advisories	None				

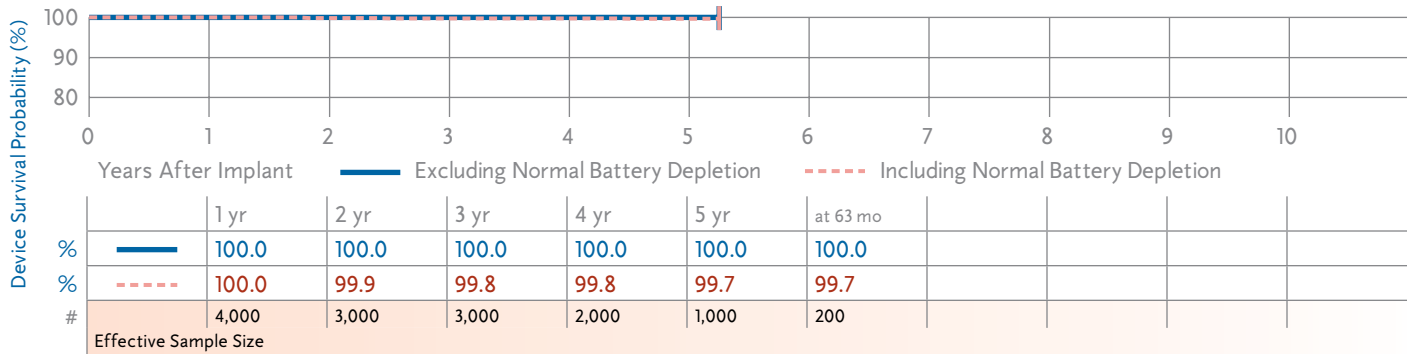

Kappa 900 DR KDR901, KDR903, KDR906

Product Characteristics


US Market Release	Jan-02	Malfunctions (US)	23	NBG Code	DDD/RO
Registered US Implants	125,000	Therapy Function Not Compromised	11	Serial Number Prefix	PKM, PKN, PKP
Estimated Active US Implants	81,000	Electrical Component	11	Estimated Longevity	See page 72
Normal Battery Depletions (US)	191	Therapy Function Compromised	12		
Advisories	None	Electrical Component	8		
		Electrical Interconnect	4		

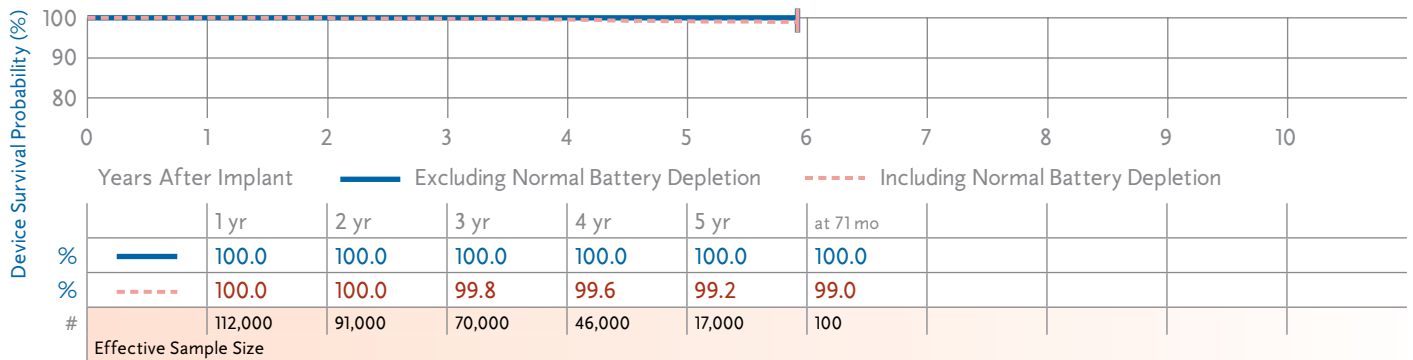

Kappa 920 DR KDR921

Product Characteristics


US Market Release	Jan-02	Malfunctions (US)	1	NBG Code	DDD/RO
Registered US Implants	16,000	Therapy Function Not Compromised	0	Serial Number Prefix	PKR
Estimated Active US Implants	9,000	Therapy Function Compromised	1	Estimated Longevity	See page 72
Normal Battery Depletions (US)	139	Electrical Interconnect	1		
Advisories	None				

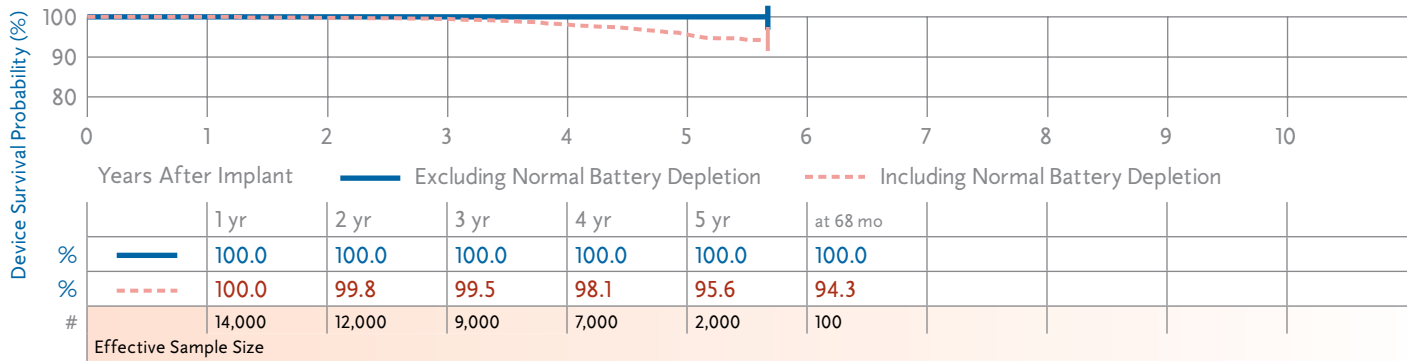

Kappa 900 SR KSR901, KSR903, KSR906

Product Characteristics

US Market Release	Jan-02	Malfunctions (US)	10	NBG Code	VVEV
Registered US Implants	37,000	Therapy Function Not Compromised	8	Serial Number Prefix	PLF, PLG, PLH
Estimated Active US Implants	21,000	Electrical Component	7	Estimated Longevity	See page 72
Normal Battery Depletions (US)	57	Possible Early Battery Depletion	1		
Advisories	None	Therapy Function Compromised	2		
		Electrical Interconnect	2		

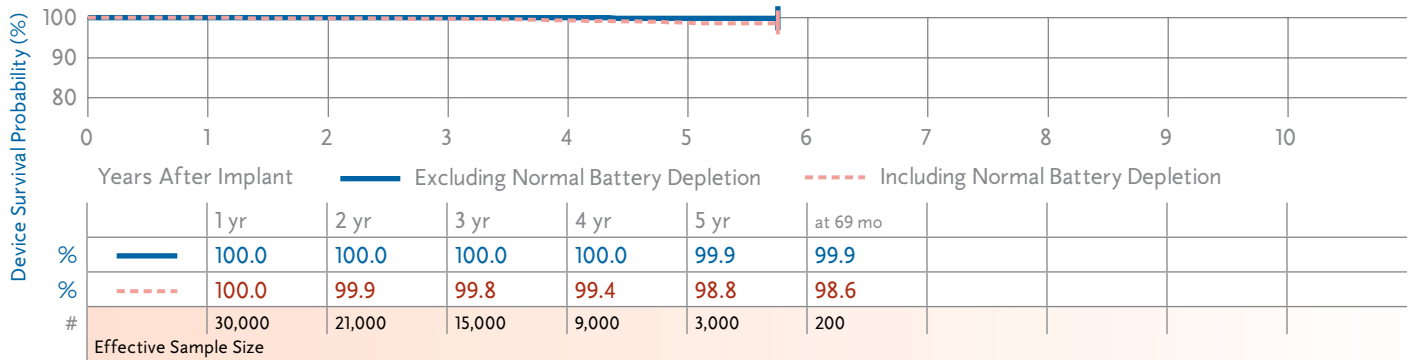


Kappa 900 VDD KVDD901

Product Characteristics

US Market Release	Jan-02
Registered US Implants	1,000
Estimated Active US Implants	400
Normal Battery Depletions (US)	0
Advisories	None

Malfunctions (US)	0
Therapy Function Not Compromised	0
Therapy Function Compromised	0

NBG Code	VDD
Serial Number Prefix	PLE
Estimated Longevity	See page 72

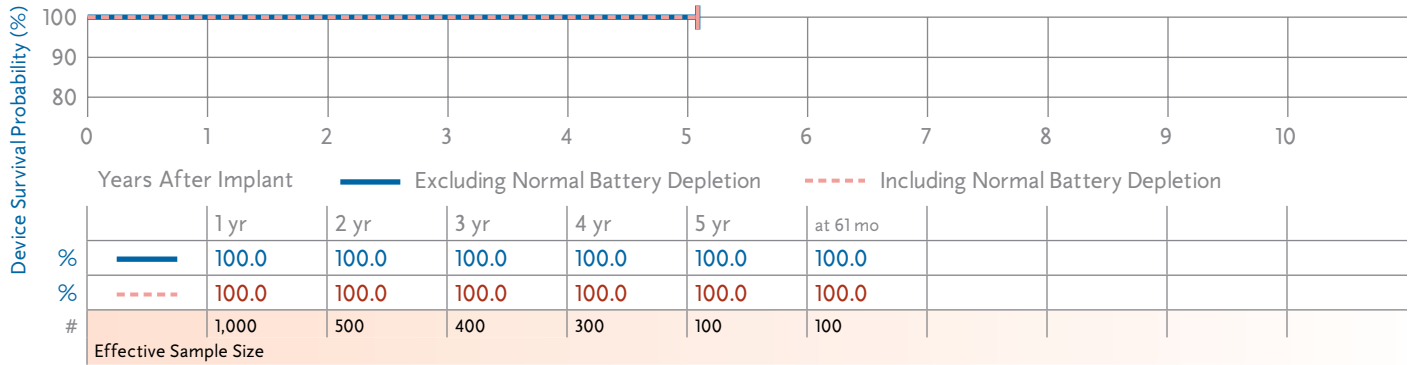


Legend 8416, 8417, 8417M, 8418, 8419

Product Characteristics

US Market Release	Aug-89
Registered US Implants	57,000
Estimated Active US Implants	2,000
Normal Battery Depletions (US)	2,706
Advisories	None

Malfunctions (US)	143
-------------------	-----

NBG Code	SSIRO
Serial Number Prefix	XT, WJ, WN, ZT
Estimated Longevity	See page 72

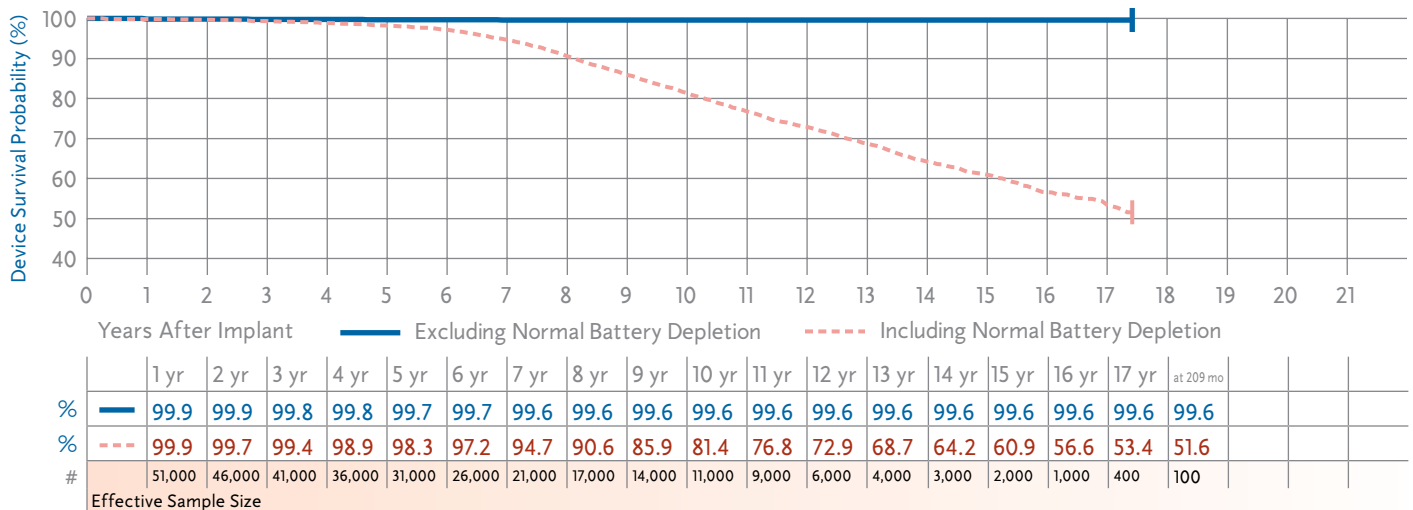


Legend II 8424, 8426, 8427

Product Characteristics

US Market Release	Nov-91
Registered US Implants	59,000
Estimated Active US Implants	5,000
Normal Battery Depletions (US)	1,842
Advisories	None

Malfunctions (US) 36

NBG Code	SSIRO
Serial Number Prefix	2P, 2T, 2U
Estimated Longevity	See page 72

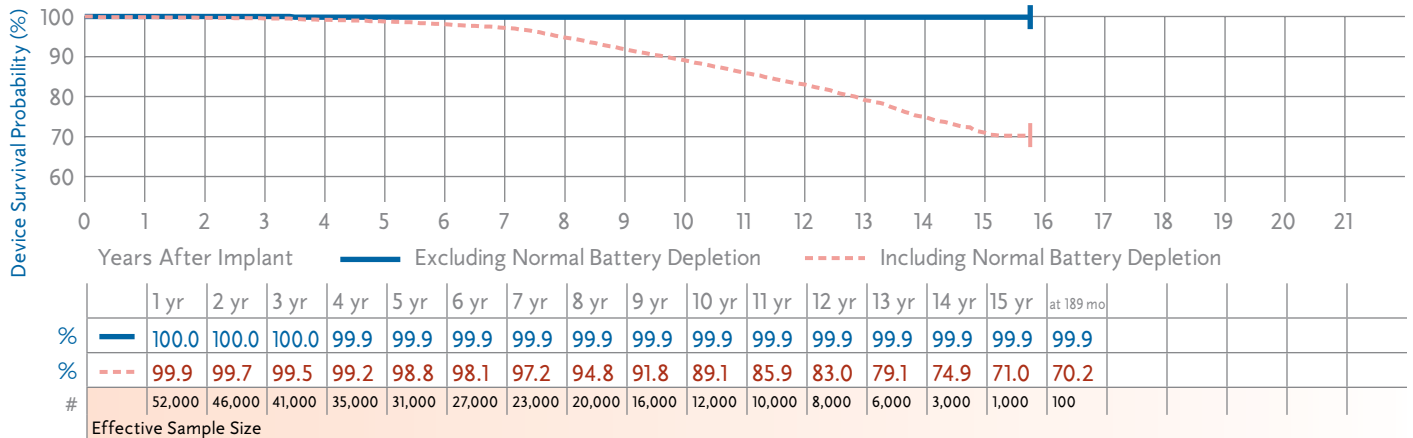

Minix/Minix ST 8330, 8331, 8331M, 8340, 8341, 8341M, 8342


Product Characteristics

US Market Release	Dec-89
Registered US Implants	58,000
Estimated Active US Implants	4,000
Normal Battery Depletions (US)	1,485

Malfunctions (US) 49

NBG Code	SSIRO
Serial Number Prefix	2P, 2T, 2U
Estimated Longevity	See page 72

Advisories: [See page 152](#) – 1991 Potential Delayed Restoration of Permanent Settings

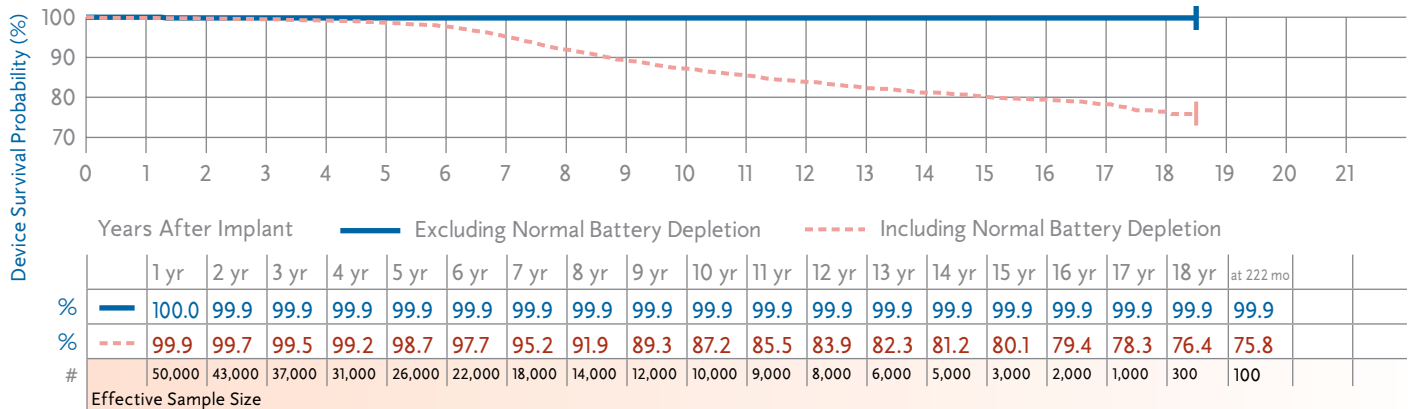


Minuet 7107, 7108

Product Characteristics

US Market Release	Mar-92
Registered US Implants	17,000
Estimated Active US Implants	2,000
Normal Battery Depletions (US)	609
Advisories	None

Malfunctions (US) 4

NBG Code	DDDCO
Serial Number Prefix	1Z1, 2G1
Estimated Longevity	See page 72

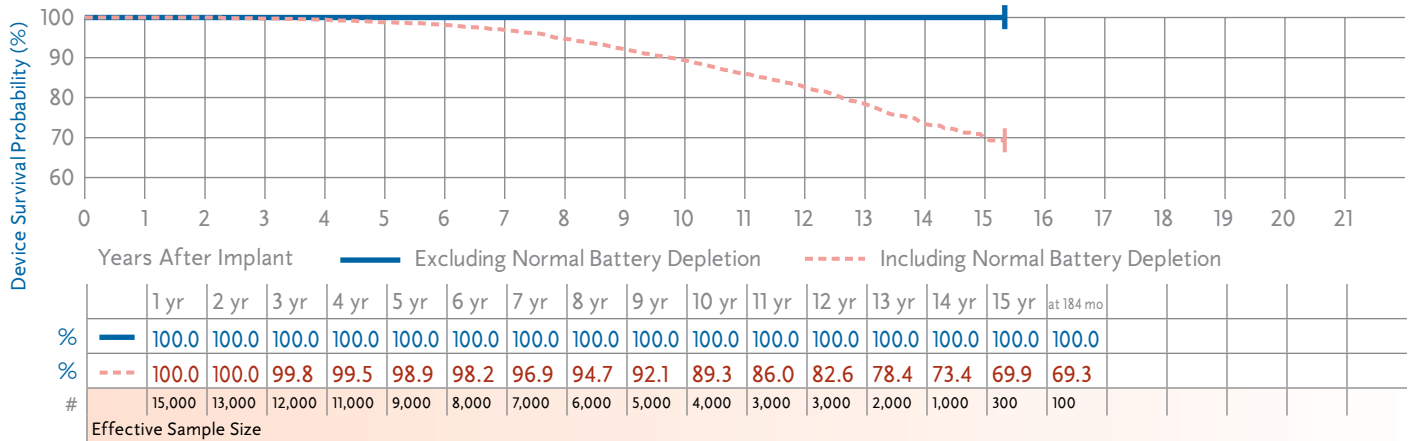


Preva DR 7088, 7089

Product Characteristics

US Market Release	Jul-96
Registered US Implants	26,000
Estimated Active US Implants	5,000
Normal Battery Depletions (US)	941
Advisories	None

Malfunctions (US) 3

NBG Code	DDD/RO
Serial Number Prefix	PGJ, PGK
Estimated Longevity	See page 72

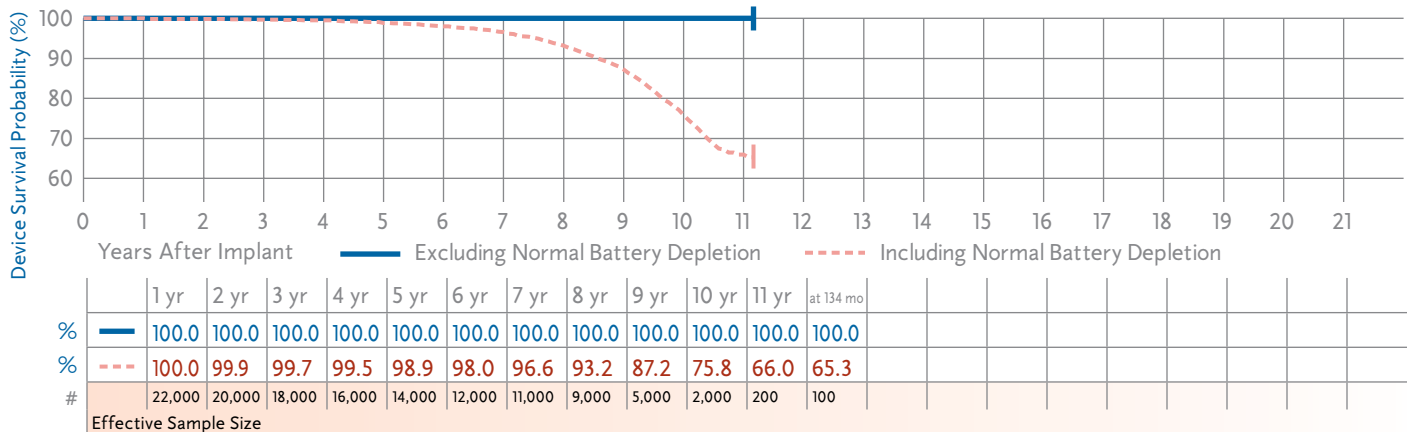


Preva SR 8088, 8089

Product Characteristics

US Market Release	Jul-96
Registered US Implants	18,000
Estimated Active US Implants	3,000
Normal Battery Depletions (US)	399
Advisories	None

Malfunctions (US) 1

NBG Code	SSI/R
Serial Number Prefix	PGL, PGM
Estimated Longevity	See page 72

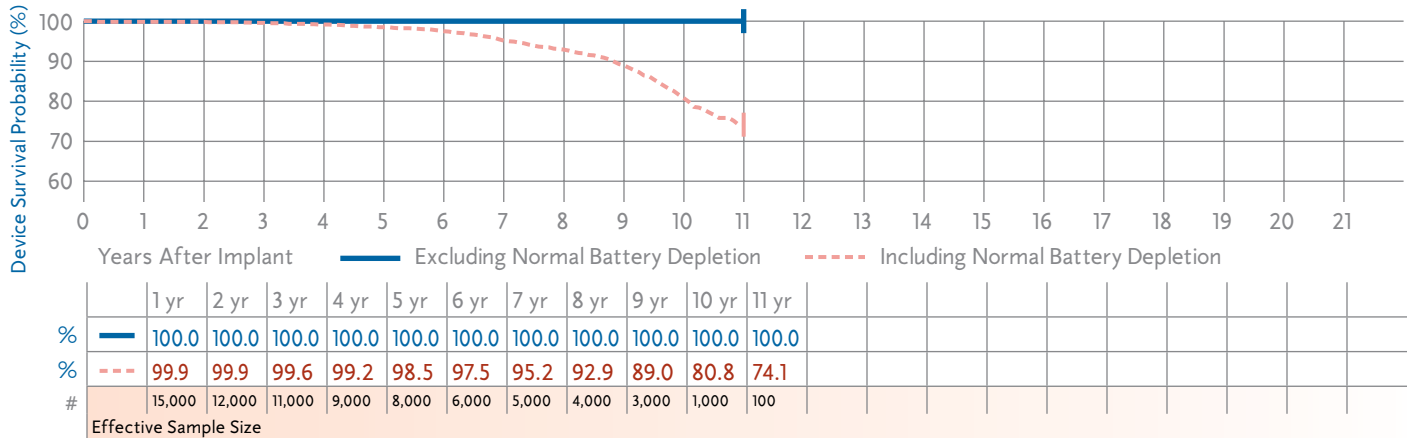


Prevail S 8085, 8086

Product Characteristics

US Market Release	Oct-95
Registered US Implants	4,000
Estimated Active US Implants	1,000
Normal Battery Depletions (US)	22
Advisories	None

Malfunctions (US) 1

NBG Code	SSI
Serial Number Prefix	PGL, PGM
Estimated Longevity	See page 72

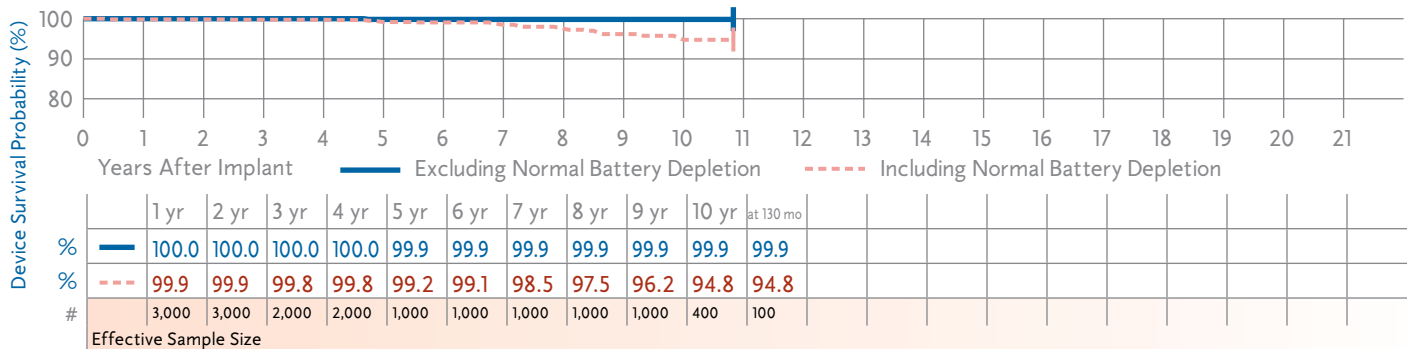


Prodigy D 7864, 7865, 7866

Product Characteristics

US Market Release	Oct-95
Registered US Implants	3,000
Estimated Active US Implants	500
Normal Battery Depletions (US)	93
Advisories	None

Malfunctions (US) 0

NBG Code	DDDCO
Serial Number Prefix	PDL, PDM, PDN
Estimated Longevity	See page 73

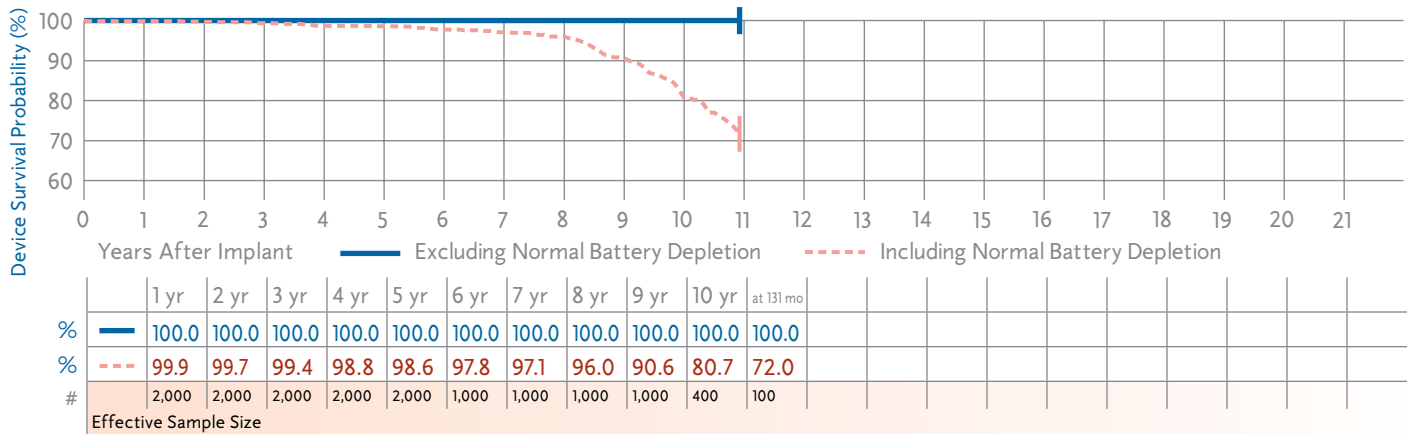


Prodigy DR 7860, 7861, 7862

Product Characteristics

US Market Release	Oct-95
Registered US Implants	38,000
Estimated Active US Implants	8,000
Normal Battery Depletions (US)	1,321
Advisories	None

Malfunctions (US) 11

NBG Code	DDD/RO
Serial Number Prefix	PDH, PDJ, PDK
Estimated Longevity	See page 73

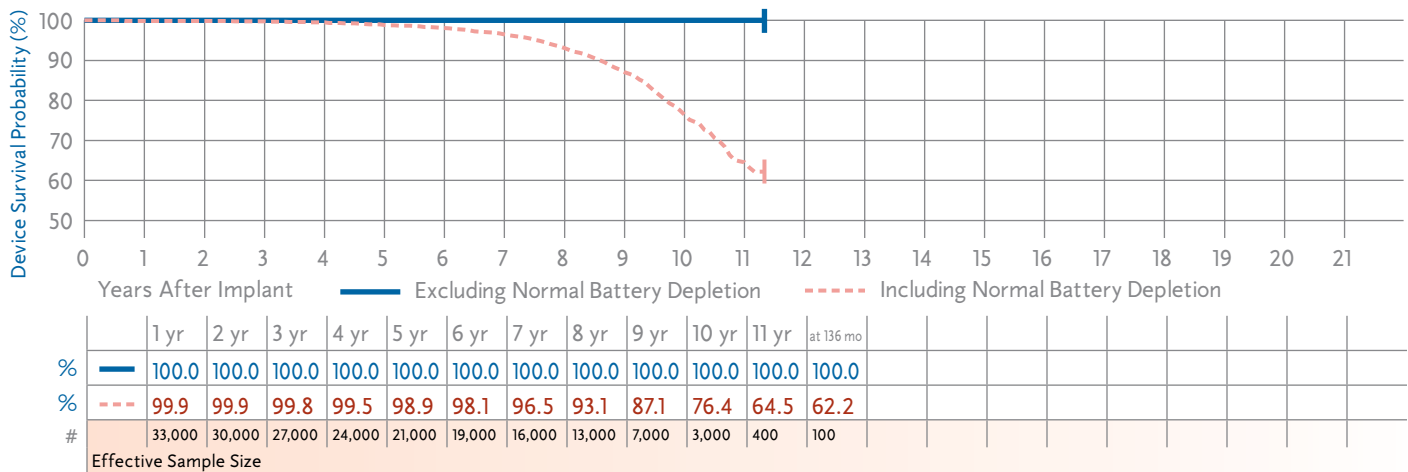


Prodigy S 8164, 8165, 8166

Product Characteristics

US Market Release	Oct-95
Registered US Implants	2,000
Estimated Active US Implants	400
Normal Battery Depletions (US)	26
Advisories	None

Malfunctions (US) 0

NBG Code	SSIC
Serial Number Prefix	PEG, PEH, PEJ
Estimated Longevity	See page 73

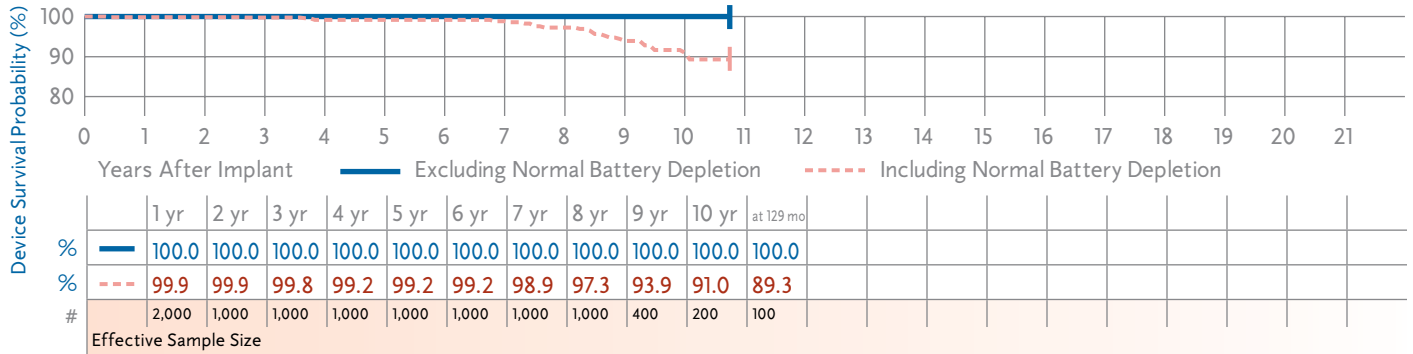


Prodigy SR 8158, 8160, 8161, 8162

Product Characteristics

US Market Release	Oct-95
Registered US Implants	22,000
Estimated Active US Implants	4,000
Normal Battery Depletions (US)	484
Advisories	None

Malfunctions (US) 5

NBG Code	SSI/R
Serial Number Prefix	PEM, PED, PEE, PEF
Estimated Longevity	See page 73

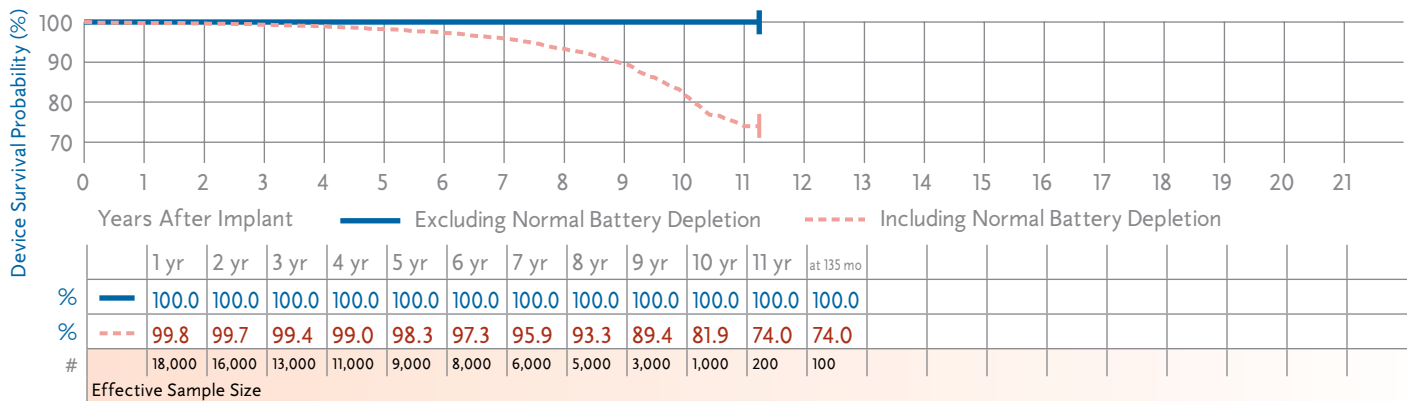


Sensia DR SEDR01, SED01

Product Characteristics

US Market Release	Jul-06
Registered US Implants	20,000
Estimated Active US Implants	18,000
Normal Battery Depletions (US)	0
Advisories	None

Malfunctions (US)	0
Therapy Function Not Compromised	0
Therapy Function Compromised	0

NBG Code	SSI/R
Serial Number Prefix	DDD, DDDR
Estimated Longevity	See page 73

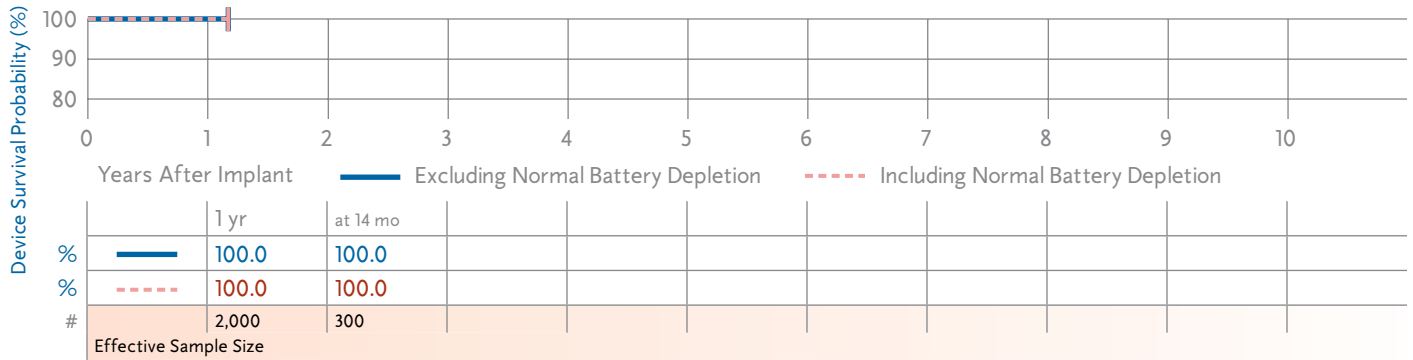


Sensia SR SESR01, SES01

Product Characteristics

US Market Release	Jul-06
Registered US Implants	12,000
Estimated Active US Implants	11,000
Normal Battery Depletions (US)	0
Advisories	None

Malfunctions (US)	0
Therapy Function Not Compromised	0
Therapy Function Compromised	0

NBG Code	SSIR, SSI
Serial Number Prefix	PWR, PWS
Estimated Longevity	See page 73

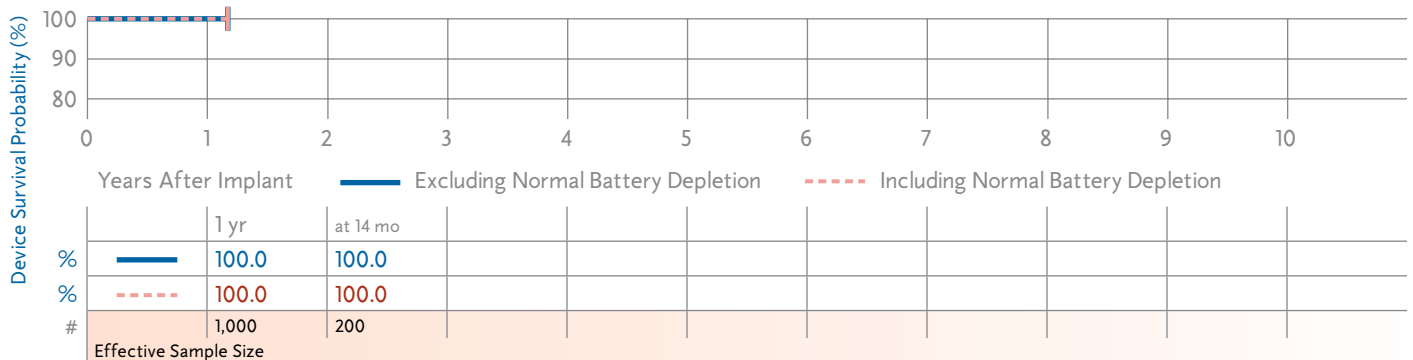


Sigma 100 S SS103, SS106

Product Characteristics

US Market Release	Aug-99	Malfunctions (US)	0	NBG Code	SSI
Registered US Implants	1,000	Therapy Function Not Compromised	0	Serial Number Prefix	PJG, PJH
Estimated Active US Implants	200	Therapy Function Compromised	0	Estimated Longevity	See page 73
Normal Battery Depletions (US)	4				

Advisories: [See page 145](#) – 2005 Potential Separation of Interconnect Wires

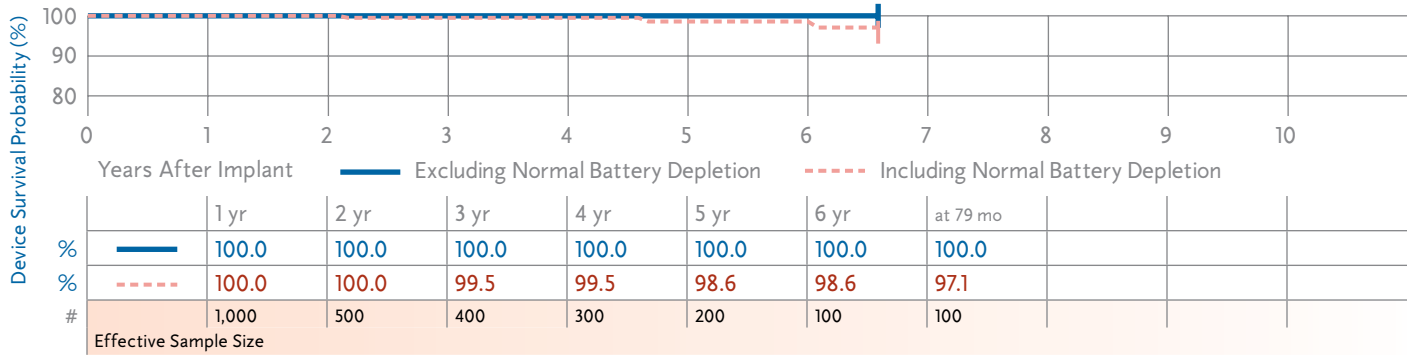


Sigma 200 DR SDR203

Product Characteristics

US Market Release	Aug-99	Malfunctions (US)	4	NBG Code	DDD/RO
Registered US Implants	16,000	Therapy Function Not Compromised	1	Serial Number Prefix	PJD
Estimated Active US Implants	7,000	Electrical Component	1	Estimated Longevity	See page 73
Normal Battery Depletions (US)	39	Therapy Function Compromised	3		
		Electrical Component	1		
		Electrical Interconnect	2		
		<i>(1 malfunction related to advisory)</i>			

Advisories: [See page 145](#) – 2005 Potential Separation of Interconnect Wires

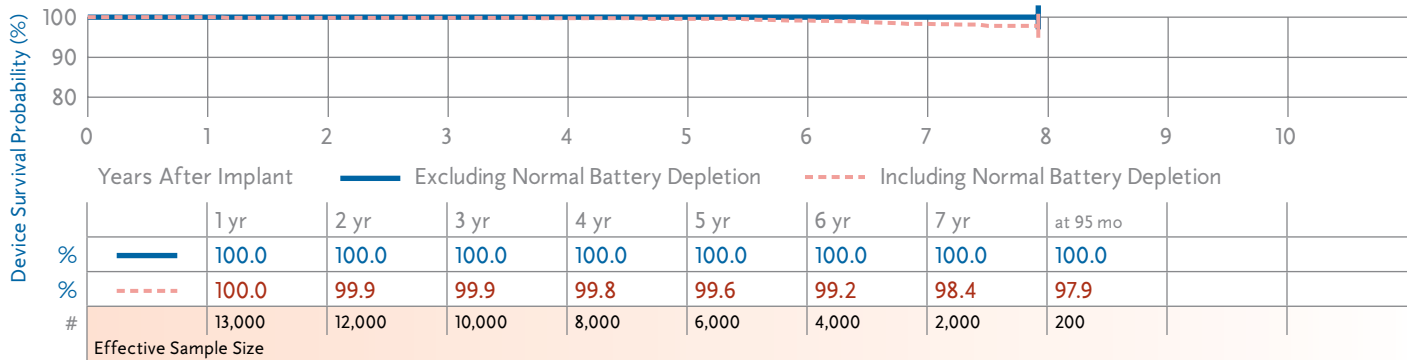


Sigma 200 SR SSR203

Product Characteristics

US Market Release	Sep-99	Malfunctions (US)	3	NBG Code	SSI/R
Registered US Implants	12,000	Therapy Function Not Compromised	0	Serial Number Prefix	PJG
Estimated Active US Implants	4,000	Therapy Function Compromised	3	Estimated Longevity	See page 73
Normal Battery Depletions (US)	21	Electrical Interconnect	3		
		<i>(3 malfunctions related to advisory)</i>			

Advisories: [See page 145](#) – 2005 Potential Separation of Interconnect Wires

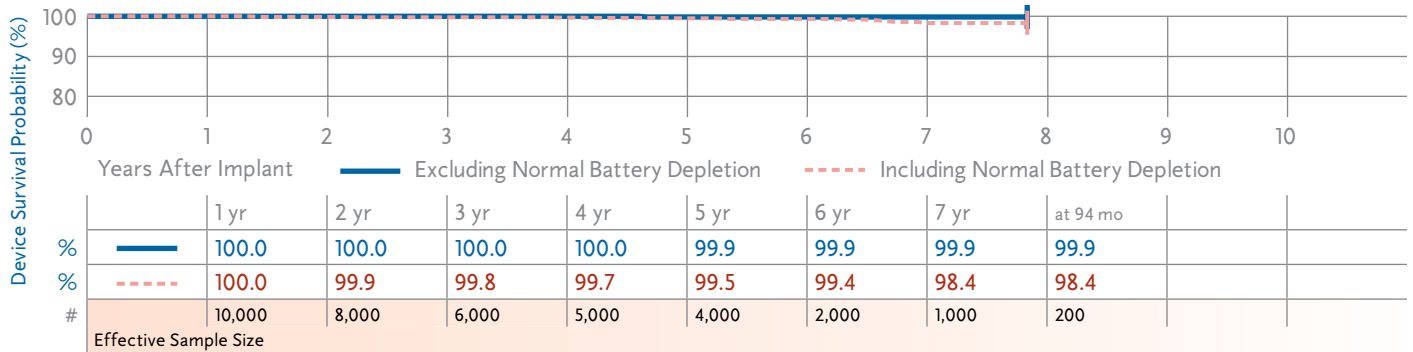


Sigma 300 DR SDR303, SDR306

Product Characteristics

US Market Release	Aug-99	Malfunctions (US)	72	NBG Code	DDD/RO
Registered US Implants	106,000	Therapy Function Not Compromised	10	Serial Number Prefix	PJD, PJE
Estimated Active US Implants	60,000	Electrical Component	4	Estimated Longevity	See page 73
Normal Battery Depletions (US)	129	Electrical Interconnect	5		
		Possible Early Battery Depletion	1		
		Therapy Function Compromised	62		
		Electrical Component	6		
		Electrical Interconnect	56		
		<i>(28 malfunctions related to advisory)</i>			


Advisories: [See page 145](#) – 2005 Potential Separation of Interconnect Wires

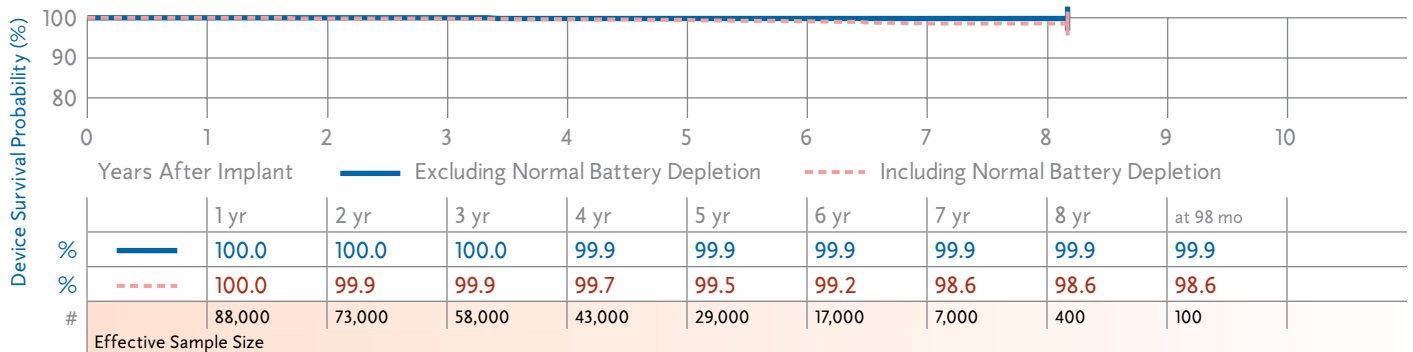

Sigma 300 SR SSR303, SSR306

Product Characteristics


US Market Release	Sep-99	Malfunctions (US)	13	NBG Code	SSI/R
Registered US Implants	53,000	Therapy Function Not Compromised	1	Serial Number Prefix	PJG, PJH
Estimated Active US Implants	24,000	Electrical Component	1	Estimated Longevity	See page 73
Normal Battery Depletions (US)	65	Therapy Function Compromised	12		
Advisories: See page 145 – 2005 Potential Separation of Interconnect Wires		Electrical Component	3		
		Electrical Interconnect	9		
		<i>(5 malfunctions related to advisory)</i>			

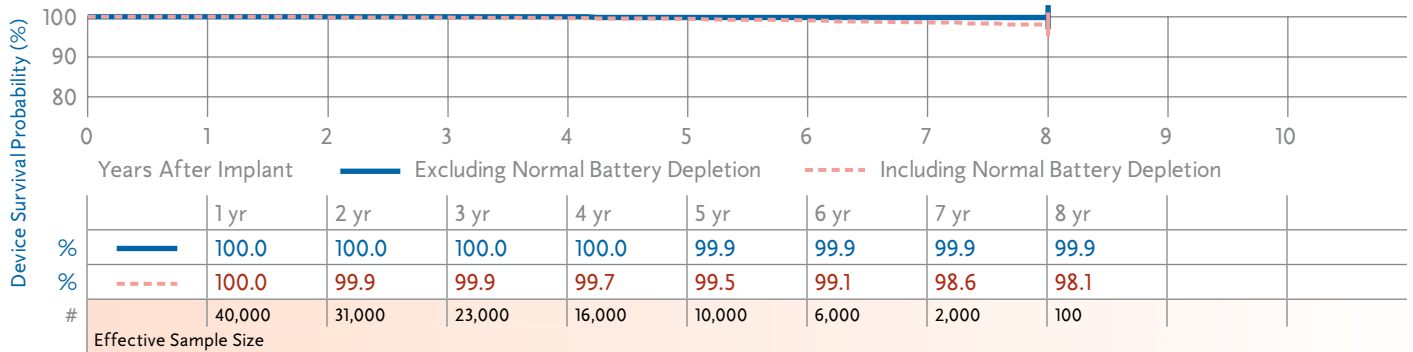

Sigma 300 VDD SVDD303

Product Characteristics

US Market Release	Sep-99	Malfunctions (US)	0	NBG Code	VDDD
Registered US Implants	1,000	Therapy Function Not Compromised	0	Serial Number Prefix	PJD
Estimated Active US Implants	300	Therapy Function Compromised	0	Estimated Longevity	See page 73
Normal Battery Depletions (US)	0				
Advisories: See page 145 – 2005 Potential Separation of Interconnect Wires					

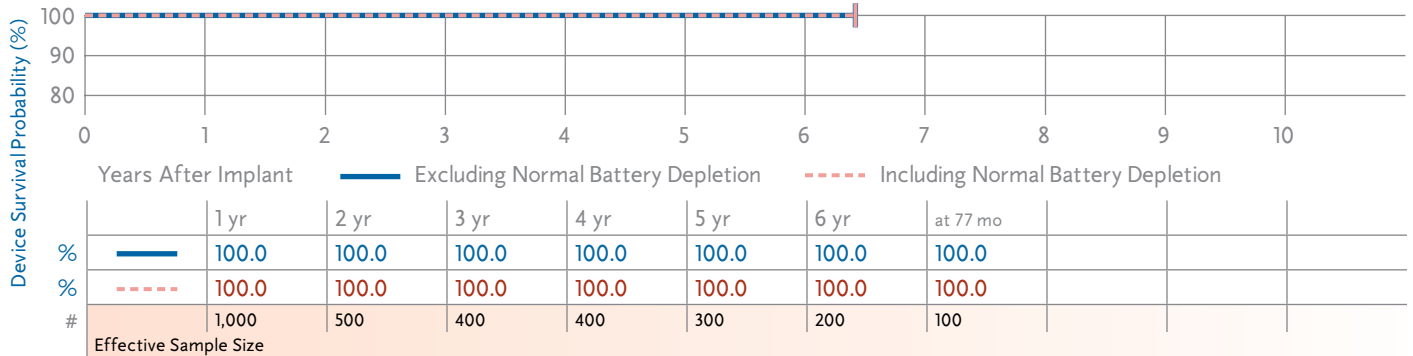

Thera-iD 7964i, 7965i, 7966i


Product Characteristics

US Market Release	Oct-95
Registered US Implants	3,000
Estimated Active US Implants	500
Normal Battery Depletions (US)	133
Advisories	None

Malfunctions (US) 1

NBG Code	DDDCO
Serial Number Prefix	PDE, PDF, PDG

Estimated Longevity [See page 73](#)

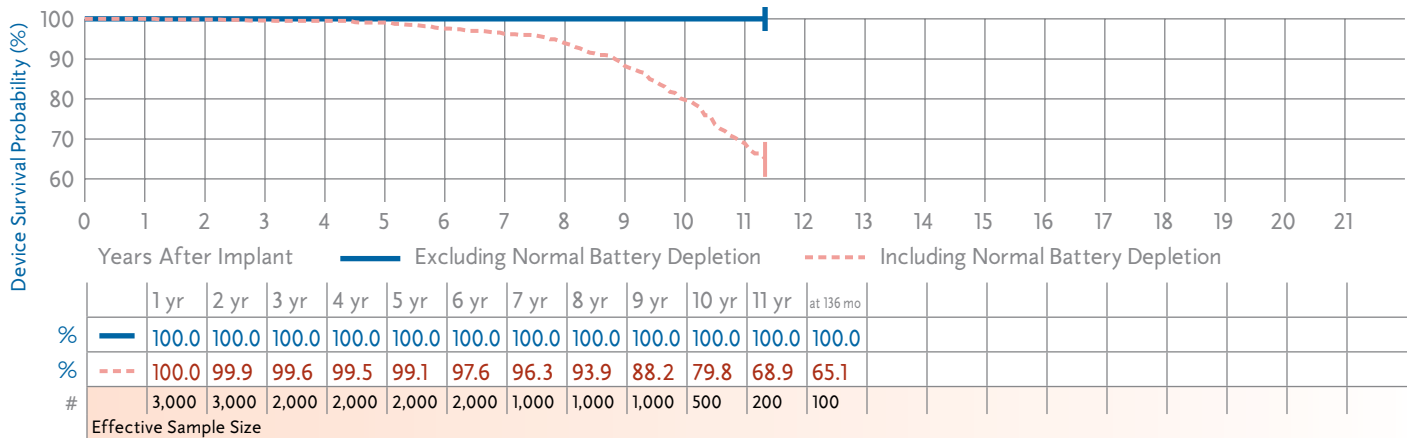

Thera-iDR 7960i, 7961i, 7962i


Product Characteristics

US Market Release	Oct-95
Registered US Implants	122,000
Estimated Active US Implants	17,000
Normal Battery Depletions (US)	5,963
Advisories	None

Malfunctions (US) 50

NBG Code	DDD/RO
Serial Number Prefix	PDB, PDC, PDD

Estimated Longevity [See page 73](#)

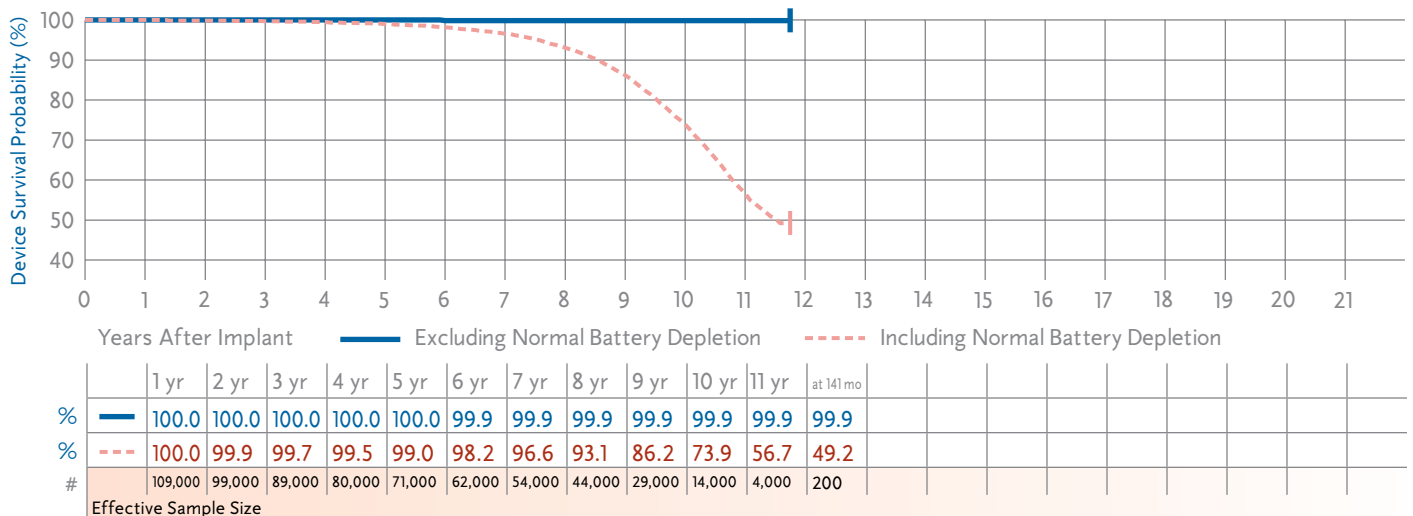


Thera-i DR 7968i

Product Characteristics

US Market Release	Jul-96
Registered US Implants	4,000
Estimated Active US Implants	300
Normal Battery Depletions (US)	233
Advisories	None

Malfunctions (US) 3

NBG Code	DDD/RO
Serial Number Prefix	PGH
Estimated Longevity	See page 73

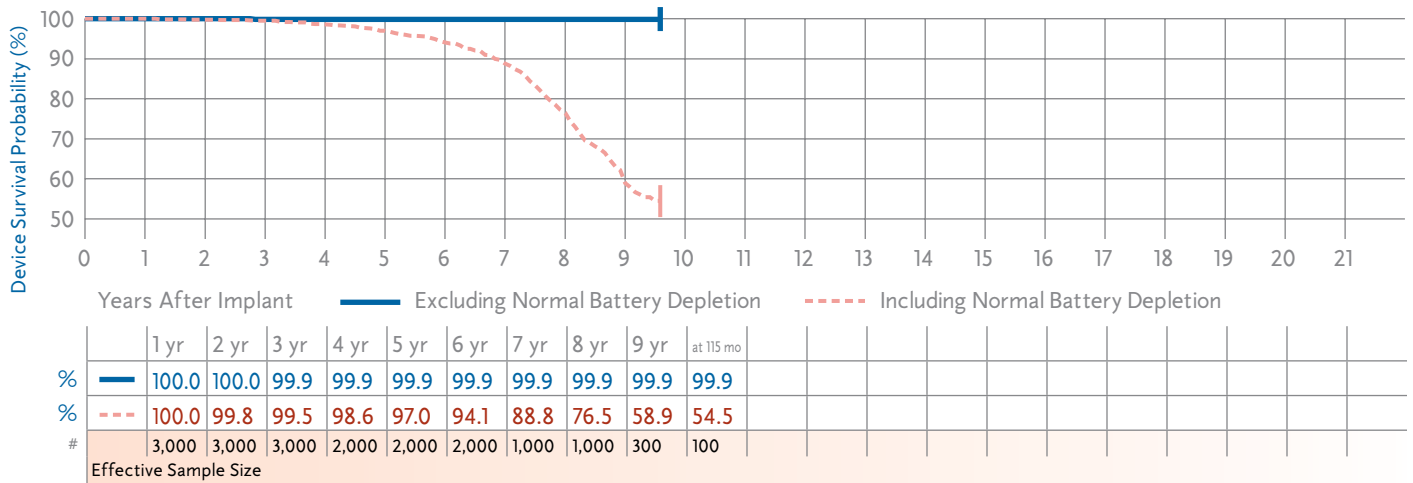


Thera-i S 8964i, 8965i, 8966i

Product Characteristics

US Market Release	Oct-95
Registered US Implants	4,000
Estimated Active US Implants	1,000
Normal Battery Depletions (US)	52
Advisories	None

Malfunctions (US) 1

NBG Code	SSIR
Serial Number Prefix	PDY, PEA, PEB
Estimated Longevity	See page 73

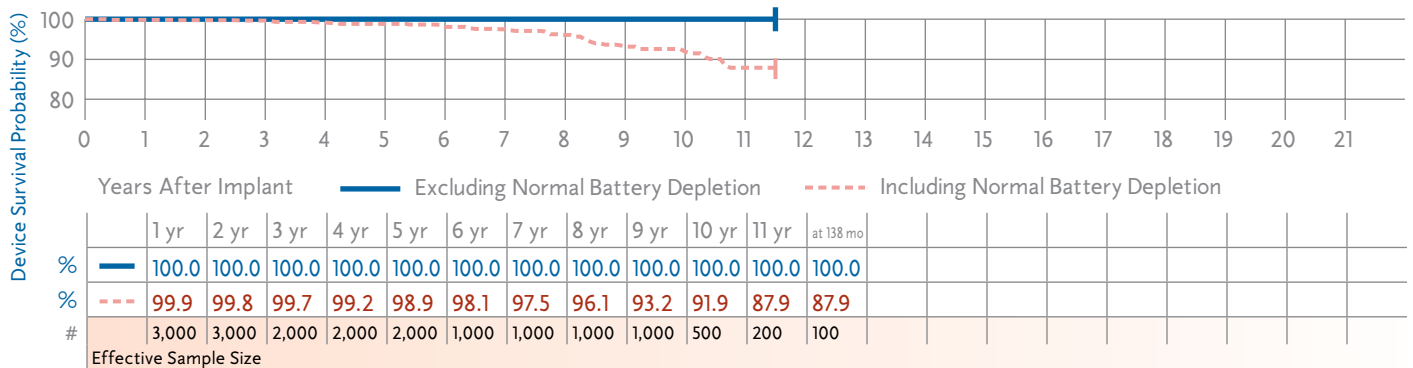


Thera-i SR 8960i, 8961i, 8962i

Product Characteristics

US Market Release	Oct-95
Registered US Implants	50,000
Estimated Active US Implants	7,000
Normal Battery Depletions (US)	1,271
Advisories	None

Malfunctions (US)	7
-------------------	---

NBG Code	SSIR
Serial Number Prefix	PDU, PDV, PDW
Estimated Longevity	See page 73

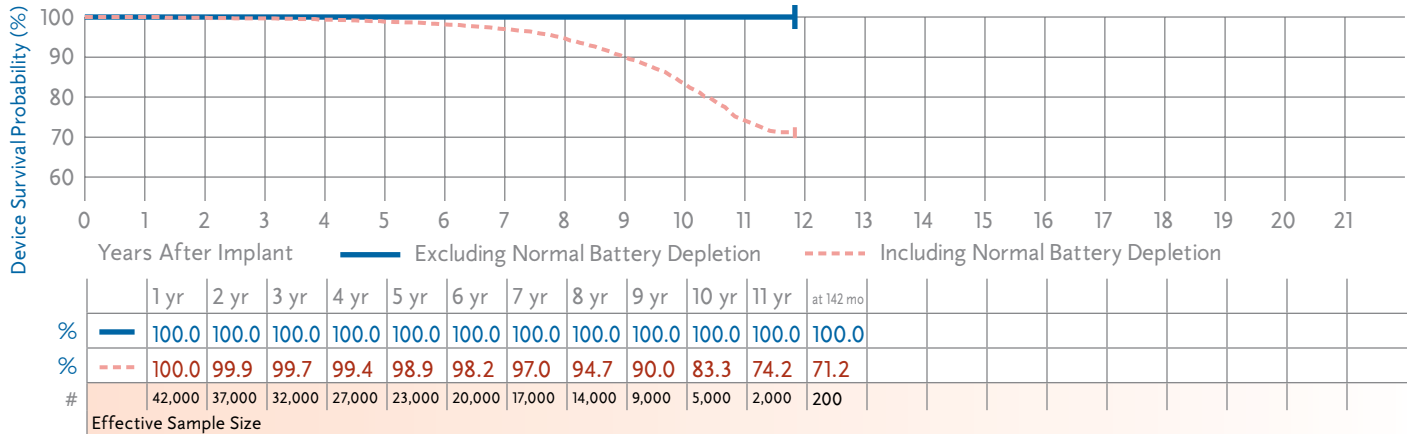


Thera-i VDD 8968i

Product Characteristics

US Market Release	Mar-96
Registered US Implants	5,000
Estimated Active US Implants	1,000
Normal Battery Depletions (US)	81
Advisories	None

Malfunctions (US)	0
-------------------	---


NBG Code	VDD
Serial Number Prefix	PEC
Estimated Longevity	See page 73

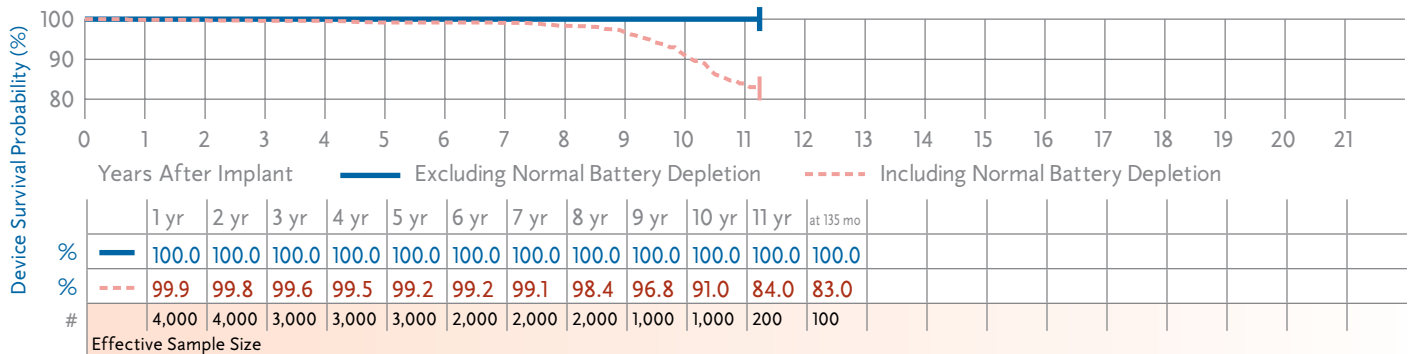

Versa DR VEDR01

Product Characteristics

US Market Release	Jul-06	Malfunctions (US)	0	NBG Code	DDDR
Registered US Implants	20,000	Therapy Function Not Compromised	0	Serial Number Prefix	PWH
Estimated Active US Implants	19,000	Therapy Function Compromised	0	Estimated Longevity	See page 73
Normal Battery Depletions (US)	0				
Advisories	None				

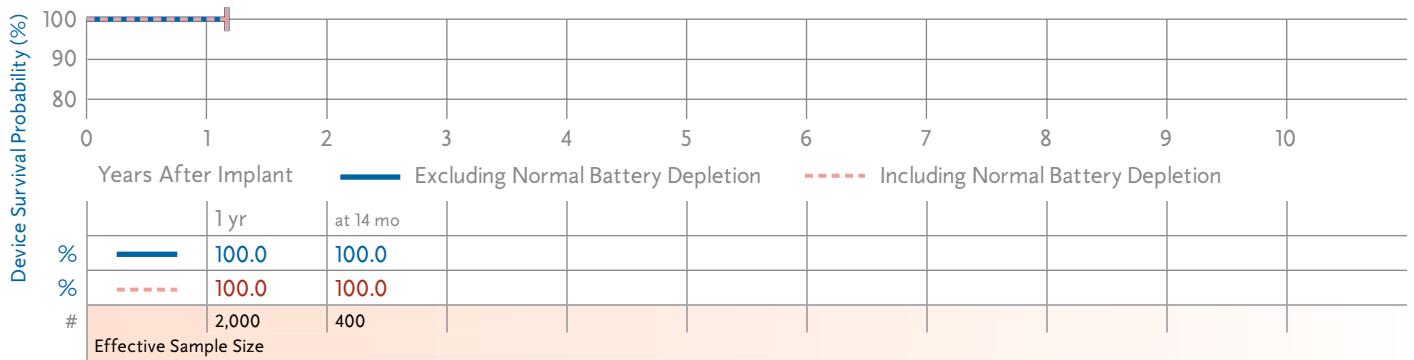

Device Survival Summary (95% Confidence Interval)

The following table shows IPG device survival estimates with 95% confidence intervals. Estimates are shown both with and without normal battery depletions included.

Family		Model Number		US Market Release		Registered US Implants		Estimated Active US Implants		Normal Battery Depletions (US)		Malfunctions (US)		Device Survival Probability (%)										
												Therapy Function Compromised	Therapy Function Not Compromised	Total	Years After Implant									
												1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	12 yr	14 yr	16 yr	
Adapta DR	ADDR01, ADDR03, ADDR06, ADDR01	Jul-06	58,000	55,000	0	0	3	=	3	Excluding Normal Battery Depletion	100.0 +0.0/-0.0 at 15 mo	100.0 +0.0/-0.0 at 15 mo												
						0	0	=	0	Including Normal Battery Depletion	100.0 +0.0/-0.0 at 15 mo	100.0 +0.0/-0.0 at 15 mo												
Adapta DR	ADDR11	Jul-06	4,000	3,000	0	0	0	=	0	Excluding Normal Battery Depletion	100.0 +0.0/-0.0	100.0 +0.0/-0.0												
						0	0	=	0	Including Normal Battery Depletion	100.0 +0.0/-0.0	100.0 +0.0/-0.0												
Adapta DR	ADDRS1	Jul-06	5,000	5,000	0	0	0	=	0	Excluding Normal Battery Depletion	100.0 +0.0/-0.0 at 14 mo	100.0 +0.0/-0.0 at 14 mo												
						0	0	=	0	Including Normal Battery Depletion	100.0 +0.0/-0.0 at 14 mo	100.0 +0.0/-0.0 at 14 mo												
Adapta SR	ADSR01, ADSR03, ADSR06	Jul-06	11,000	10,000	0	0	0	=	0	Excluding Normal Battery Depletion	100.0 +0.0/-0.0 at 14 mo	100.0 +0.0/-0.0 at 14 mo												
						0	0	=	0	Including Normal Battery Depletion	100.0 +0.0/-0.0 at 14 mo	100.0 +0.0/-0.0 at 14 mo												
AT500	AT501, 7253	Mar-03	11,000	7,000	149	5	5	=	10	Excluding Normal Battery Depletion	100.0 +0.0/-0.1	100.0 +0.0/-0.1	100.0 +0.0/-0.1	99.8 +0.1/-0.2 at 64 mo	99.8 +0.1/-0.2 at 64 mo	99.8 +0.1/-0.2 at 64 mo	99.8 +0.1/-0.2 at 64 mo	99.8 +0.1/-0.2 at 64 mo	99.8 +0.1/-0.2 at 64 mo	99.8 +0.1/-0.2 at 64 mo	99.8 +0.1/-0.2 at 64 mo	99.8 +0.1/-0.2 at 64 mo	99.8 +0.1/-0.2 at 64 mo	
						5	5	=	10	Including Normal Battery Depletion	99.9 +0.0/-0.1	99.9 +0.0/-0.1	99.7 +0.1/-0.1	98.2 +0.4/-0.5 at 64 mo	71.8 +4.6/-5.3 at 64 mo	52.7 +6.3/-6.7 at 64 mo	52.7 +6.3/-6.7 at 64 mo	52.7 +6.3/-6.7 at 64 mo	52.7 +6.3/-6.7 at 64 mo	52.7 +6.3/-6.7 at 64 mo	52.7 +6.3/-6.7 at 64 mo	52.7 +6.3/-6.7 at 64 mo	52.7 +6.3/-6.7 at 64 mo	
EnPulse DR	EIDR01, EIDR03, EIDR06	Dec-03	7,000	5,000	4	0	1	=	1	Excluding Normal Battery Depletion	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.1	100.0 +0.0/-0.1 at 47 mo	100.0 +0.0/-0.1 at 47 mo	100.0 +0.0/-0.1 at 47 mo	100.0 +0.0/-0.1 at 47 mo	100.0 +0.0/-0.1 at 47 mo	100.0 +0.0/-0.1 at 47 mo	100.0 +0.0/-0.1 at 47 mo	100.0 +0.0/-0.1 at 47 mo	100.0 +0.0/-0.1 at 47 mo	100.0 +0.0/-0.1 at 47 mo	
						0	1	=	1	Including Normal Battery Depletion	100.0 +0.0/-0.0	100.0 +0.0/-0.0	99.9 +0.1/-0.1	99.8 +0.1/-0.2 at 47 mo	99.8 +0.1/-0.2 at 47 mo	99.8 +0.1/-0.2 at 47 mo	99.8 +0.1/-0.2 at 47 mo	99.8 +0.1/-0.2 at 47 mo	99.8 +0.1/-0.2 at 47 mo	99.8 +0.1/-0.2 at 47 mo	99.8 +0.1/-0.2 at 47 mo	99.8 +0.1/-0.2 at 47 mo	99.8 +0.1/-0.2 at 47 mo	
EnPulse DR	EIDR21	Dec-03	2,000	1,000	3	0	0	=	0	Excluding Normal Battery Depletion	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0 at 46 mo	100.0 +0.0/-0.0 at 46 mo	100.0 +0.0/-0.0 at 46 mo	100.0 +0.0/-0.0 at 46 mo	100.0 +0.0/-0.0 at 46 mo	100.0 +0.0/-0.0 at 46 mo	100.0 +0.0/-0.0 at 46 mo	100.0 +0.0/-0.0 at 46 mo	100.0 +0.0/-0.0 at 46 mo	100.0 +0.0/-0.0 at 46 mo	
						0	0	=	0	Including Normal Battery Depletion	100.0 +0.0/-0.0	100.0 +0.0/-0.0	99.6 +0.2/-0.5 at 46 mo	99.6 +0.2/-0.5 at 46 mo	99.6 +0.2/-0.5 at 46 mo	99.6 +0.2/-0.5 at 46 mo	99.6 +0.2/-0.5 at 46 mo	99.6 +0.2/-0.5 at 46 mo	99.6 +0.2/-0.5 at 46 mo	99.6 +0.2/-0.5 at 46 mo	99.6 +0.2/-0.5 at 46 mo	99.6 +0.2/-0.5 at 46 mo	99.6 +0.2/-0.5 at 46 mo	99.6 +0.2/-0.5 at 46 mo

continued

Device Survival Summary continued

										Device Survival Probability (%)																													
										Years After Implant																													
										1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	12 yr	14 yr	16 yr																		
Family	Model Number	US Market Release	Registered US Implants	Estimated Active US Implants	Normal Battery Depletions (US)	Malfunctions (US)		Therapy Function		Therapy Not Computed		Total																											
						Complished	Not Computed	Complished	Not Computed	Complished	Not Computed	Complished	Not Computed	Excluding Normal Battery Depletion	Including Normal Battery Depletion	Excluding Normal Battery Depletion	Including Normal Battery Depletion	Excluding Normal Battery Depletion	Including Normal Battery Depletion	Excluding Normal Battery Depletion	Including Normal Battery Depletion	Excluding Normal Battery Depletion	Including Normal Battery Depletion	Excluding Normal Battery Depletion	Including Normal Battery Depletion														
EnPulse 2 DR	E2DR01, E2DR03, E2DR06	Feb-04	101,000	78,000	6	3	+	5	=	8	0	+	0	=	0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0
						3	+	5	=	8	0	+	0	=	0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0
EnPulse 2 DR	E2DR21	Feb-04	12,000	9,000	11	0	+	0	=	0	0	+	0	=	0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0
EnPulse 2 DR	E2DR31, E2DR33	Feb-04	1,000	500	0	0	+	0	=	0	0	+	0	=	0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0
EnPulse 2 SR	E2SR01, E2SR03, E2SR06	Dec-03	25,000	18,000	6	1	+	2	=	3	1	+	2	=	3	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0		
EnPulse 2 VDD	E2YDD01	Dec-03	1,000	1,000	0	0	+	0	=	0	0	+	0	=	0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0		
EnRhythm DR	P1501DR	May-05	64,000	55,000	0	13	+	5	=	18	13	+	5	=	18	100.0	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0		
Kappa 400 DR	KDR401, KDR403	Jan-98	47,000	8,000	3,269	9	+	13	=	22	9	+	13	=	22	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0		
Kappa 400 SR	KSR401, KSR403	Feb-98	15,000	4,000	455	1	+	3	=	4	1	+	3	=	4	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	100.0	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0	99.9	+0.0/-0.0		

continued

Device Survival Summary continued

Family		Model Number	US Market Release	Registered US Implants	Estimated Active US Implants	Normal Battery Depletions	Malfunctions		Device Survival Probability (%)															
							Therapy Function Compromised	Therapy Function Not Compromised	Total	Years After Implant														
							0	+	0	=	0	1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	12 yr	14 yr	16 yr	
Kappa 800 DR	KDR801, KDR803	3,000	4,000	3,000	4	0	0	+	0	=	0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
												+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0
Kappa 900 DR	KDR901, KDR903, KDR906	81,000	125,000	81,000	191	12	+	11	=	23	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
											+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0
Kappa 900 SR	KSR901, KSR903, KSR906	21,000	37,000	21,000	57	2	+	8	=	10	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
											+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0
Kappa 900 VDD	KVDD901	400	1,000	400	0	0	+	0	=	0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
											+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0
Kappa 920 DR	KDR921	9,000	16,000	9,000	139	1	+	0	=	1	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
											+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0
Legend	8416, 8417, 8418, 8419	2,000	57,000	2,000	2,706	—	—	—	—	143	99.9	99.9	99.8	99.8	99.8	99.7	99.7	99.6	99.6	99.6	99.6	99.6	99.6	99.6
											+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0
Legend II	8424, 8426, 8427	5,000	59,000	5,000	1,842	—	—	—	—	36	99.9	99.7	99.4	99.4	98.9	98.3	97.2	94.7	90.6	81.4	72.9	64.2	51.6	99.9
											+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0	+0.0/-0.0

continued

Device Survival Summary continued

Family	Model Number	US Market Release	Registered US Implants	Estimated Active US Implants	Normal Battery Depletions	Malfunctions			Device Survival Probability (%)											
						Therapy Function Compromised	Therapy Not Function Compromised	Total	Years After Implant											
									1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	12 yr	14 yr	16 yr
Minix/ Minix ST	8330, 8331, 8331M, 8340, 8341, 8341M, 8342	Dec-89	58,000	4,000	1,485	—	—	49	Excluding Normal Battery Depletion											
						—	—	—	99.9	99.9	99.9	99.9	99.9	99.9	99.9	99.9	99.9	99.9	99.9	99.9
						—	—	—	Including Normal Battery Depletion											
									99.9	99.7	99.5	99.2	98.7	97.7	95.2	91.9	87.2	83.9	81.2	75.8
									+0.0/-0.0	+0.0/-0.0	+0.1/-0.1	+0.1/-0.1	+0.1/-0.1	+0.2/-0.2	+0.3/-0.3	+0.4/-0.4	+0.5/-0.5	+0.6/-0.6	+0.7/-0.7	+1.5/-1.6
									222 mo											
Minuet	7107, 7108	Mar-92	17,000	2,000	609	—	—	4	Excluding Normal Battery Depletion											
						—	—	—	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
						—	—	—	Including Normal Battery Depletion											
									100.0	100.0	99.8	99.5	98.9	98.2	96.9	94.7	89.3	82.6	73.4	69.3
									+0.0/-0.0	+0.0/-0.0	+0.1/-0.1	+0.1/-0.1	+0.2/-0.2	+0.3/-0.3	+0.3/-0.4	+0.5/-0.5	+0.7/-0.8	+1.0/-1.1	+1.5/-1.6	184 mo
Preva DR	7088, 7089	Jul-96	26,000	5,000	941	—	—	3	Excluding Normal Battery Depletion											
						—	—	—	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
						—	—	—	Including Normal Battery Depletion											
									100.0	99.9	99.7	99.5	98.9	98.0	96.6	93.2	75.8	65.3	62.2	62.2
									+0.0/-0.0	+0.0/-0.0	+0.1/-0.1	+0.1/-0.1	+0.2/-0.2	+0.3/-0.3	+0.4/-0.5	+0.6/-0.7	+1.1/-1.2	+2.1/-2.2	+2.1/-2.3	134 mo
Preva SR	8088, 8089	Jul-96	18,000	3,000	399	—	—	1	Excluding Normal Battery Depletion											
						—	—	—	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
						—	—	—	Including Normal Battery Depletion											
									99.9	99.9	99.6	99.2	98.5	97.5	95.2	92.9	80.8	74.1	68.5	68.5
									+0.0/-0.0	+0.0/-0.1	+0.1/-0.1	+0.1/-0.2	+0.2/-0.3	+0.3/-0.4	+0.5/-0.5	+0.6/-0.7	+1.5/-1.6	+2.5/-2.8	+2.5/-2.8	132 mo
Prevail S	8085, 8086	Oct-95	4,000	1,000	22	—	—	1	Excluding Normal Battery Depletion											
						—	—	—	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
						—	—	—	Including Normal Battery Depletion											
									100.0	99.9	99.8	99.8	99.2	99.1	98.5	97.5	94.8	84.8	74.1	74.1
									+0.0/-0.0	+0.1/-0.2	+0.1/-0.2	+0.1/-0.2	+0.3/-0.6	+0.4/-0.6	+0.6/-0.9	+0.8/-1.1	+1.4/-1.9	+1.4/-1.9	+2.2/-2.3	130 mo
Prodigy D	7864, 7865, 7866	Oct-95	3,000	500	93	—	—	0	Excluding Normal Battery Depletion											
						—	—	—	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
						—	—	—	Including Normal Battery Depletion											
									99.9	99.7	99.4	98.8	98.6	97.8	97.1	96.0	80.7	72.0	62.2	62.2
									+0.0/-0.0	+0.2/-0.3	+0.3/-0.4	+0.4/-0.6	+0.4/-0.6	+0.6/-0.8	+0.7/-1.0	+0.9/-1.2	+2.8/-3.2	+4.2/-4.8	+4.2/-4.8	131 mo
Prodigy DR	7860, 7861, 7862	Oct-95	38,000	8,000	1,321	—	—	11	Excluding Normal Battery Depletion											
						—	—	—	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
						—	—	—	Including Normal Battery Depletion											
									99.9	99.9	99.8	99.5	98.9	98.1	96.5	93.1	76.4	62.2	62.2	62.2
									+0.0/-0.0	+0.0/-0.0	+0.0/-0.1	+0.1/-0.1	+0.1/-0.1	+0.2/-0.2	+0.2/-0.3	+0.4/-0.4	+1.0/-1.0	+2.3/-2.4	+2.3/-2.4	136 mo

continued



Device Survival Summary continued

Family	Model Number	US Market Release	Registered US Implants	Estimated Active US Implants	Normal Battery Depletions	Malfunctions		Device Survival Probability (%)																
						Therapy Function Compromised	Therapy Function Not Compromised	Years After Implant																
								1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	12 yr	14 yr	16 yr					
Prodigy S	8164, 8165, 8166	Oct-95	2,000	400	26	0	0	Excluding Normal Battery Depletion	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	+0.0/-0.0 at 129 mo	
								Including Normal Battery Depletion	99.9	99.9	99.8	99.2	99.2	99.2	98.9	97.3	91.0	89.3	+2.7/-3.5 at 129 mo					
Prodigy SR	8158, 8160, 8161, 8162	Oct-95	22,000	4,000	484	5	Excluding Normal Battery Depletion	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	+0.0/-0.0 at 135 mo	
							Including Normal Battery Depletion	99.8	99.7	99.4	99.0	98.3	97.3	95.9	93.3	81.9	74.0	+2.2/-2.4 at 135 mo						
Sensia DR	SEDR01, SED01	Jul-06	20,000	18,000	0	0	Excluding Normal Battery Depletion	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	+0.0/-0.0 at 14 mo	
							Including Normal Battery Depletion	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
Sensia SR	SESR01, SES01	Jul-06	12,000	11,000	0	0	Excluding Normal Battery Depletion	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	+0.0/-0.0 at 14 mo
							Including Normal Battery Depletion	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0
Sigma 100 S	SST05, SST06	Aug-99	1,000	200	4	0	Excluding Normal Battery Depletion	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	+0.0/-0.0 at 79 mo
							Including Normal Battery Depletion	100.0	100.0	99.5	99.5	98.6	98.6	97.1	91.0	89.3	+2.7/-3.5 at 129 mo							
Sigma 200 DR	SDR203	Aug-99	16,000	7,000	39	4	Excluding Normal Battery Depletion	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	+0.0/-0.1 at 95 mo
							Including Normal Battery Depletion	100.0	100.0	99.9	99.8	99.6	99.2	98.4	97.9	91.0	89.3	+2.7/-3.5 at 129 mo						
Sigma 200 SR	SSR203	Sep-99	12,000	4,000	21	3	Excluding Normal Battery Depletion	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	100.0	+0.0/-0.1 at 94 mo
							Including Normal Battery Depletion	100.0	100.0	99.8	99.7	99.5	99.4	98.4	98.4	91.0	89.3	+2.7/-3.5 at 129 mo						

continued

Device Survival Summary continued

Family	Model Number	US Market Release	Registered US Implants	Estimated Active US Implants	Normal Battery Depletions	Malfunctions			Device Survival Probability (%)														
						Therapy Function Compromised	Therapy Not Function Compromised	Total	Years After Implant														
									1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	12 yr	14 yr	16 yr			
Thera-iSR	8960i, 8961i, 8962i	Oct-95	50,000	7,000	1,271	—	—	7	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	
						—	—	—	99.9 +0.0/-0.0	99.7 +0.1/-0.1	99.4 +0.1/-0.1	98.9 +0.1/-0.1	98.2 +0.2/-0.2	97.0 +0.2/-0.2	94.7 +0.3/-0.3	83.3 +0.7/-0.7	71.2 +1.3/-1.4 at 142 mo	71.2 +1.3/-1.4 at 142 mo	71.2 +1.3/-1.4 at 142 mo	71.2 +1.3/-1.4 at 142 mo	71.2 +1.3/-1.4 at 142 mo	71.2 +1.3/-1.4 at 142 mo	71.2 +1.3/-1.4 at 142 mo
Thera-i VDD	8968i	Mar-96	5,000	1,000	81	—	—	0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0
						—	—	—	99.9 +0.1/-0.1	99.6 +0.2/-0.3	99.5 +0.2/-0.3	99.2 +0.2/-0.4	99.2 +0.3/-0.4	99.1 +0.3/-0.4	98.4 +0.4/-0.6	91.0 +1.5/-1.8	83.0 +2.8/-3.3 at 135 mo	83.0 +2.8/-3.3 at 135 mo	83.0 +2.8/-3.3 at 135 mo	83.0 +2.8/-3.3 at 135 mo	83.0 +2.8/-3.3 at 135 mo	83.0 +2.8/-3.3 at 135 mo	83.0 +2.8/-3.3 at 135 mo
Versa DR	VEDR01	Jul-06	20,000	19,000	0	0	+	0 = 0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0
						—	—	—	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0	100.0 +0.0/-0.0

Reference Chart

The longevity estimates provided are mean values calculated for the parameters given. The longevity estimates shown here assume a lower rate of 60 ppm, 100% pacing, and pulse width of 0.4 ms unless noted otherwise. The actual longevity achieved for any device while implanted will depend on the actual programmed parameters and patient factors, and may differ significantly from these estimates. **The elective replacement time is indicated via telemetry indication, and rate and mode change to 65 ppm and VVI respectively (VOO/65 with magnet), unless noted otherwise.**

Family	Model Number	Amplitude Setting	Estimated Longevity		Elective Replacement Indicators
			500 Lead Ω	1000 Lead Ω	
Adapta DR	ADDR01, ADDR03, ADDR06, ADD01	Low 2.5 V (A, RV)	7.4	8.2	**
		Nominal 3.5 V (A, RV)	6.0	7.3	
		High 5.0 V (A, RV)	4.5	6.0	
Adapta DR	ADDRS1	Low 2.5 V (A, RV)	5.5	6.1	**
		Nominal 3.5 V (A, RV)	4.3	5.4	
		High 5.0 V (A, RV)	3.2	4.4	
Adapta DR	ADDRL1	Low 2.5 V (A, RV)	9.1	10.1	**
		Nominal 3.5 V (A, RV)	7.4	9.0	
		High 5.0 V (A, RV)	5.4	7.3	
Adapta SR	ADSR01, ADSR03, ADSR06	Low 2.5 V (RV)	7.3	7.8	**
		Nominal 3.5 V (RV)	6.4	7.4	
		High 5.0 V (RV)	5.0	6.2	
Adapta VDD	ADVDD01	Low 2.5 V (RV)	6.2	6.5	**
		Nominal 3.5 V (RV)	5.5	6.2	
		High 5.0 V (RV)	4.4	5.4	
AT500	AT501, 7253	Low 2.0 V (A, RV)	7.7	8.3	Telemetry indication. Pacing mode and rate (magnet and non-magnet) as programmed.
		Nominal 3.0 V (A, RV)	5.8	7.0	
		High 5.0 V (A, RV)	3.7	5.2	
EnPulse DR	EIDR01, EIDR03, EIDR06	Low 2.5 V (A, RV)	7.5	8.5	**
		Nominal 3.5 V (A, RV)	6.2	7.6	
		High 5.0 V (A, RV)	4.4	5.9	
EnPulse DR	EIDR21	Low 2.5 V (A, RV)	5.4	6.0	**
		Nominal 3.5 V (A, RV)	4.3	5.4	
		High 5.0 V (A, RV)	3.0	4.2	
EnPulse 2 DR	E2DR01, E2DR03, E2DR06	Low 2.5 V (A, RV)	7.5	8.5	**
		Nominal 3.5 V (A, RV)	6.2	7.6	
		High 5.0 V (A, RV)	4.4	5.9	
EnPulse 2 DR	E2DR21	Low 2.5 V (A, RV)	5.4	6.0	**
		Nominal 3.5 V (A, RV)	4.3	5.4	
		High 5.0 V (A, RV)	3.0	4.2	
EnPulse 2 DR	E2DR31, E2DR33	Low 2.5 V (A, RV)	9.0	10.1	**
		Nominal 3.5 V (A, RV)	7.4	9.1	
		High 5.0 V (A, RV)	5.2	7.1	
EnPulse 2 SR	E2SR01, E2SR03, E2SR06	Low 2.5 V (A, RV)	7.2	7.7	**
		Nominal 3.5 V (A, RV)	6.3	7.3	
		High 5.0 V (A, RV)	4.8	6.1	
EnPulse 2 VDD	E2VDD01	Low 2.5 V (RV)	6.1	6.5	**
		Nominal 3.5 V (RV)	5.5	6.2	
		High 5.0 V (RV)	4.3	5.4	
EnRhythm DR	P150IDR	Low 2.5 V (A, RV)	10.6	12.3	**
		Nominal 3.5 V (A, RV)	8.0	10.3	
		High 5.0 V (A, RV)	5.4	7.8	
Kappa 400 DR	KDR401, KDR403	Low 2.5 V (A, RV)	7.8	8.5	**
		Nominal 3.5 V (A, RV)	6.4	7.5	
		High 5.0 V (A, RV)	5.1	6.5	
Kappa 400 SR	KSR401, KSR403	Low 2.5 V (RV)	7.9	8.4	**
		Nominal 3.5 V (RV)	6.9	7.7	
		High 5.0 V (RV)	5.8	7.0	
Kappa 600 DR	KDR601, KDR603, KDR606	Low 2.5 V (A, RV)	7.7	8.6	**
		Nominal 3.5 V (A, RV)	6.3	7.7	
		High 5.0 V (A, RV)	4.4	6.0	
Kappa 600 DR	KDR651, KDR653	Low 2.5 V (A, RV)	7.7	8.6	**
		Nominal 3.5 V (A, RV)	6.3	7.7	
		High 5.0 V (A, RV)	4.4	6.0	

**Telemetry indication. Rate and mode change to 65 ppm and VVI respectively (VOO/65 with magnet).

continued

Reference Chart continued

Family	Model Number	Amplitude Setting	Estimated Longevity		Elective Replacement Indicators
			500 Lead Ω	1000 Lead Ω	
Kappa 700 D	KDR701, KD703, KD706	Low 2.5 V (A, RV)	7.7	8.6	**
		Nominal 3.5 V (A, RV)	6.3	7.7	
		High 5.0 V (A, RV)	4.4	6.0	
Kappa 700 DR	KDR701, KDR703, KDR706	Low 2.5 V (A, RV)	7.7	8.6	**
		Nominal 3.5 V (A, RV)	6.3	7.7	
		High 5.0 V (A, RV)	4.4	6.0	
Kappa 700 DR	KDR721	Low 2.5 V (A, RV)	5.5	6.1	**
		Nominal 3.5 V (A, RV)	4.4	5.5	
		High 5.0 V (A, RV)	3.0	4.2	
Kappa 700 SR	KSR701, KSR703, KSR706	Low 2.5 V (RV)	7.4	7.9	**
		Nominal 3.5 V (RV)	6.5	7.5	
		High 5.0 V (RV)	4.9	6.2	
Kappa 700 VDD	KVDD701	Low 2.5 V (RV)	6.2	6.6	**
		Nominal 3.5 V (RV)	5.6	6.3	
		High 5.0 V (RV)	4.4	5.3	
Kappa 800 DR	KDR801, KDR803	Low 2.5 V (A, RV)	7.7	8.6	**
		Nominal 3.5 V (A, RV)	6.3	7.7	
		High 5.0 V (A, RV)	4.4	6.0	
Kappa 900 DR	KDR901, KDR903, KDR906	Low 2.5 V (A, RV)	7.7	8.6	**
		Nominal 3.5 V (A, RV)	6.3	7.7	
		High 5.0 V (A, RV)	4.4	6.0	
Kappa 920 DR	KDR921	Low 2.5 V (A, RV)	5.5	6.1	**
		Nominal 3.5 V (A, RV)	4.4	5.5	
		High 5.0 V (A, RV)	3.0	4.3	
Kappa 900 SR	KSR901, KSR903, KSR906	Low 2.5 V (RV)	7.3	7.9	**
		Nominal 3.5 V (RV)	6.4	7.4	
		High 5.0 V (RV)	4.9	6.1	
Kappa 900 VDD	KVDD901	Low 2.5 V (RV)	6.2	6.6	**
		Nominal 3.5 V (RV)	5.6	6.3	
		High 5.0 V (RV)	4.4	5.4	
Legend	8416, 8417, 8417M, 8418, 8419	Low 2.5 V (RV)	15.6	17.7	If programmed to non-rate responsive mode (e.g. VVI), rate decrease of 10% from programmed rate. Telemetry indication. If programmed to rate responsive mode (e.g. VVIR), rate change to 65 ppm and mode change to VVI. Telemetry indication.
		Nominal 3.3 V (RV)	11.3	14.5	
		High 5.0 V (RV)	9.0	12.5	
Legend II	8424, 8426, 8427	Low 2.5 V, 0.36 ms (RV)	12.9	14.5	If programmed to non-rate responsive mode (e.g. VVI), rate decrease of 10% from programmed rate. Telemetry indication. If programmed to rate responsive mode (e.g. VVIR), rate change to 65 ppm and mode change to VVI. Telemetry indication.
		Nominal 3.3 V, 0.36 ms (RV)	9.4	11.8	
		High 5.0 V, 0.36 ms (RV)	7.8	10.5	
Minix	8340, 8341, 8341M, 8342	Low 2.5 V (RV)	14.9	17.3	Telemetry indication. Rate decrease of 10% from programmed rate.
		Nominal 3.3 V (RV)	10.2	13.6	
		High 5.0 V (RV)	7.9	11.3	
Minix ST	8330, 8331, 8331M	Low 2.5 V (RV)	14.9	17.3	Telemetry indication. Rate decrease of 10% from programmed rate.
		Nominal 5.0 V (RV)	7.9	11.4	
		High 8.0 V (RV)	4.0	7.0	
Minuet	7107, 7108	Low 2.5 V, 0.36 ms (A, RV)	12.5	15.6	**
		Nominal 4.0 V, 0.36 ms (A, RV)	7.7	10.9	
		High 5.0 V, 0.36 ms (A, RV)	4.7	7.6	
Preva DR	7088, 7089	Low 2.5 V (A, RV)	9.9	11.3	**
		Nominal 3.5 V (A, RV)	7.4	9.4	
		High 5.0 V (A, RV)	5.4	7.5	
Preva SR	8088, 8089	Low 2.5 V (RV)	9.8	10.7	**
		Nominal 3.5 V (RV)	8.0	9.5	
		High 5.0 V (RV)	6.4	8.1	
Prevail S	8085, 8086	Low 2.5 V, 0.42 ms (RV)	16.4	19.4	Telemetry indication. Rate decrease of 10% from programmed rate.
		Nominal 3.3 V, 0.42 ms (RV)	10.8	14.4	
		High 5.0 V, 0.42 ms (RV)	8.6	12.4	

**Telemetry indication. Rate and mode change to 65 ppm and VVI respectively (VOO/65 with magnet).

continued

Reference Chart continued

Family	Model Number	Amplitude Setting	Estimated Longevity		Elective Replacement Indicators
			500 Lead Ω	1000 Lead Ω	
Prodigy D	7864, 7865, 7866	Low 2.5 V (A, RV)	10.0	11.4	**
		Nominal 3.5 V (A, RV)	7.4	9.5	
		High 5.0 V (A, RV)	5.4	7.6	
Prodigy DR	7860, 7861, 7862	Low 2.5 V (A, RV)	9.9	11.3	**
		Nominal 3.5 V (A, RV)	7.4	9.4	
		High 5.0 V (A, RV)	5.4	7.5	
Prodigy S	8164, 8165, 8166	Low 2.5 V (RV)	10.0	10.9	**
		Nominal 3.5 V (RV)	8.1	9.6	
		High 5.0 V (RV)	6.4	8.2	
Prodigy SR	8158, 8160, 8161, 8162	Low 2.5 V (RV)	9.8	10.7	**
		Nominal 3.5 V (RV)	8.0	9.5	
		High 5.0 V (RV)	6.4	8.1	
Sensia DR	SEDR01, SED01	Low 2.5 V (A, RV)	7.5	8.3	**
		Nominal 3.5 V (A, RV)	6.1	7.4	
		High 5.0 V (A, RV)	4.5	6.0	
Sensia DR	SEDRL1	Low 2.5 V (A, RV)	9.1	10.1	**
		Nominal 3.5 V (A, RV)	7.4	9.0	
		High 5.0 V (A, RV)	5.4	7.3	
Sensia SR	SESR01, SES01	Low 2.5 V (RV)	7.3	7.8	**
		Nominal 3.5 V (RV)	6.4	7.4	
		High 5.0 V (RV)	5.0	6.2	
Sigma 100 S	SS103, SS106	Low 2.5 V (RV)	10.1	11.1	**
		Nominal 3.5 V (RV)	8.2	9.8	
		High 5.0 V (RV)	6.4	8.4	
Sigma 200 DR	SDR203	Low 2.5 V (A, RV)	10.1	11.7	**
		Nominal 3.5 V (A, RV)	7.5	9.6	
		High 5.0 V (A, RV)	5.5	7.8	
Sigma 200 SR	SSR203	Low 2.5 V (RV)	10.1	11.1	**
		Nominal 3.5 V (RV)	8.2	9.8	
		High 5.0 V (RV)	6.4	8.4	
Sigma 300 DR	SDR303, SDR306	Low 2.5 V (A, RV)	10.1	11.7	**
		Nominal 3.5 V (A, RV)	7.5	9.6	
		High 5.0 V (A, RV)	5.5	7.8	
Sigma 300 SR	SSR303, SSR306	Low 2.5 V (RV)	10.1	11.1	**
		Nominal 3.5 V (RV)	8.2	9.8	
		High 5.0 V (RV)	6.4	8.4	
Sigma 300 VDD	SVDD303	Low 2.5 V (RV)	8.9	9.7	**
		Nominal 3.5 V (RV)	7.3	8.6	
		High 5.0 V (RV)	5.8	7.4	
Thera-i D	7964i, 7965i, 7966i	Low 2.5 V (A, RV)	10.0	11.4	**
		Nominal 3.5 V (A, RV)	7.4	9.5	
		High 5.0 V (A, RV)	5.4	7.6	
Thera-i DR	7960i, 7961i, 7962i	Low 2.5 V (A, RV)	9.9	11.3	**
		Nominal 3.5 V (A, RV)	7.4	9.4	
		High 5.0 V (A, RV)	5.4	7.5	
Thera-i DR	7968i	Low 2.5 V (A, RV)	7.2	8.3	**
		Nominal 3.5 V (A, RV)	5.4	6.9	
		High 5.0 V (A, RV)	3.9	5.5	
Thera-i S	8964i, 8965i, 8966i	Low 2.5 V (RV)	10.0	10.9	**
		Nominal 3.5 V (RV)	8.1	9.6	
		High 5.0 V (RV)	6.4	8.2	
Thera-i SR	8960i, 8961i, 8962i	Low 2.5 V (RV)	9.8	10.7	**
		Nominal 3.5 V (RV)	8.0	9.5	
		High 5.0 V (RV)	6.4	8.1	
Thera-i VDD	8968i	Low 2.5 V (RV)	11.5	12.4	**
		Nominal 3.5 V (RV)	9.6	11.1	
		High 5.0 V (RV)	7.7	9.7	
Versa DR	VEDR01	Low 2.5 V (A, RV)	7.5	8.3	**
		Nominal 3.5 V (A, RV)	6.1	7.4	
		High 5.0 V (A, RV)	4.5	6.0	

**Telemetry indication. Rate and mode change to 65 ppm and VVI respectively (VOO/65 with magnet).



Method for Estimating Lead Performance

Medtronic CRDM has tracked lead survival for over 20 years with its multicenter, global chronic lead studies.

Leads Performance Analysis

Implanted leads operate in the challenging biochemical environment of the human body and the body's response to foreign objects. Implanted leads are also subject to mechanical stresses associated with heart motion, body motion, and patient anatomy.

In this environment, pacemaker and defibrillation leads cannot be expected to last forever. While IPGs and ICDs have a battery that will deplete after a predictable length of time, a lead's longevity cannot be predicted nor are there simple indicators that a lead is approaching the end of its service life. Therefore, regular monitoring while implanted, and evaluation of lead integrity upon IPG or ICD replacement, is necessary to determine if a lead may be approaching the end of its service life.

Returned Product Analysis Shortfalls

All leads and lead segments returned to Medtronic are analyzed to determine whether or not they meet performance limits established by Medtronic. Although returned product analyses are valuable for gaining insight into lead failure mechanisms, this data cannot be used by itself for determining the survival probability of leads because only a small fraction of leads are explanted and returned for analysis. Additionally, those leads which are returned cannot be assumed to be statistically representative of the performance of the total population for a given lead model. Partial or total lead extraction can result in significant damage to a lead, making a definitive analysis of a suspected failure and its cause impossible. Thus, lead survival probabilities are more appropriately determined through a clinical surveillance study. Although returned product analysis results are presented in this report, Medtronic tracks lead survival through its System Longevity Study.

System Longevity Study (SLS)

The SLS is a prospective, multicenter, global study designed to monitor the performance of market-released cardiac therapy products. Medtronic has been monitoring the performance of its cardiac therapy products for 25 years and has evaluated the performance of more than 75,000 leads, with data reported from 14 countries on 4 continents.

Patients are eligible for enrollment in the study if

- 1 They are within 6 months post-implant of a Medtronic market-released lead connected to a market-released CRT, ICD, or IPG device, and the lead is used for a pacing, sensing, or defibrillation application, or
- 2 They participated in a qualifying study of a market-released Medtronic cardiac therapy product; complete implant and follow-up data are available; and the data is appropriately and legally released for use in the study.

Lead Complications

The SLS complication criteria are defined below. These criteria do not, however, enable a lead integrity or "hardware" failure to be conclusively differentiated from other clinical events such as an undetected lead dislodgement, exit block, or concurrent pulse generator failure manifested as a sensing or capture problem.

A lead-related complication is considered to have occurred if at least one of the following clinical observations is reported and at least one of the following clinical actions is made 30 days or more after the implant.

Clinical Observations

- Failure to capture
- Failure to sense/undersensing
- Oversensing
- Abnormal pacing impedance (based on lead model, but normal range is typically 200-3000 ohms)
- Abnormal defibrillation impedance (based on lead model, but normal range is typically 20-200 ohms)
- Insulation breach, observed visually, that has degraded system performance
- Conductor fracture, observed visually or radiographically
- Extracardiac stimulation
- Cardiac perforation
- Lead dislodgement

continued

The Standard Actuarial Method is used to determine estimates of lead survival.

Clinical Actions

- Lead surgically abandoned/capped
- Lead electrically abandoned/capped
- Lead explanted
- Lead replaced
- Polarity reprogrammed (i.e., bipolar to unipolar; unipolar to bipolar)
- Lead use continued based on medical judgment despite a known clinical performance issue
- Other lead-related surgery performed (e.g., lead mechanical alteration or unsuccessful repositioning)

Note: Successful lead repositioning is not a qualifying action.

Methods

The performance of leads is expressed in terms of lead survival estimates, where “survival” refers to the function of the lead, not the survival of the patient. These survival estimates are intended to illustrate the probability that a lead will survive for a given number of years without a lead-related complication.

The survival estimates are determined from the analysis of the data collected through the SLS. These data are presented graphically and numerically.

The SLS protocol requires regular follow-up reporting on all leads actively followed in the study. Each study center must inform Medtronic whenever a lead complication has occurred or when a patient is no longer participating in the study. Under the study protocol, each lead is assumed to be normally active unless a lead-related complication is confirmed, the lead is abandoned or explanted, or the patient is no longer available for follow-up. The data analyses assume that the patient is still part of the study and there are no lead complications at the time of the report cutoff date unless specifically reported by the center.

Medtronic evaluates center compliance with study protocol through, at a minimum, annual clinical monitoring at each study site. Additionally, study center personnel must be trained in the study procedures prior to participating and they must adhere to the policies and procedures of their local ethics boards.

Implant times are calculated from the implant date to the earlier of the complication date, out-of-service date (for example, patient leaves the study or the lead is no longer being used), or the cutoff date of the report. If a lead experiences more than one complication, the first is used to calculate survival time; although all complications associated with a lead are reported in PPR tables.

Of the several different statistical methods available for survival analysis, the Standard Actuarial Method, with suspensions assumed distributed across the intervals (Cutler-Ederer Method), is used to determine estimates of lead survival. This method is commonly used by medical researchers and clinicians.

On the following pages, each graph includes a survival curve where events include qualifying lead-related complications. This survival estimate is a good representation of the probability a lead will survive a period of time without a lead-related complication. For example, if a survival probability is 95% after 5 years of service, then the lead has a 5% chance of experiencing a lead-related complication in the first 5 years following implant.

Since the survival estimate can become very imprecise with small effective sample sizes, Medtronic truncates the survival curve when the number of leads entering an interval is less than 50 leads. When the number of leads entering an interval reaches 50, the next data point is added to the survival curve.

Although the report provides tabular data in one year intervals, the curves are actually computed and plotted using three-month intervals.

The data in the tables is rounded to the nearest tenth of one percent. Occasionally, a graph may show 100% survival, but have 1 or more complications. This occurs because even with the complications, the data rounds to 100%.

The survival curves are statistical estimates. As performance experience accumulates, the estimation improves. Confidence intervals are provided as a way to indicate the degree of certainty of the estimates. Greenwood’s formula is used to calculate corresponding 95% confidence intervals for the standard errors, and the complementary log-log method is used to produce the confidence bounds.

continued

Medtronic urges all physicians to return explanted product and to notify Medtronic when a product is no longer in use, regardless of reason for explant or removal from use.

Sample Size and How the Population and Population Samples Are Defined

The population sample from which the survival estimates are derived is comprised of the patients successfully enrolled in the SLS as of the report cutoff date. The number of enrolled implants is listed for each model.

This sample based on SLS enrollments is considered to be representative of the worldwide population, including data from 14 countries on 4 continents, and therefore the survival estimates shown in this report should be representative of the performance worldwide of these models.

In general, a model or model family will be included in this report when more than 100 leads have been enrolled and no fewer than 50 leads followed for at least 6 months. Models will remain in the report as long as Medtronic estimates at least 500 leads remain active in the United States, based on estimated US implants.

Returned Product Analysis Results

Every lead or lead portion returned to Medtronic receives an analysis. Although the returned product analysis data is not used to generate the survival estimates, the data provides valuable insight into the causes of lead malfunction.

For reporting returned product analysis results, Medtronic CRDM considers a lead as having malfunctioned whenever the analysis shows that any parameter was outside the performance limits established by Medtronic while implanted and in service. To be considered a malfunction for returned product analysis reporting, the lead must have been returned to Medtronic and analyzed.

Lead malfunctions are divided into three categories: Implant Damage, Electrical, and Other. Typical examples of implant damage are stylet perforation, cut or torn insulation, bent or distorted conductors, over-retracted helixes, and conductor fracture due to overtorquing. An electrical malfunction is defined as a hardware malfunction resulting in a break in the insulation or a break in the conductor that could affect the electrical performance of the lead. A break in the insulation is defined as a breach allowing entry of body fluids, or inappropriate current flow between the conductors, or between the conductor and the body. Examples include cuts, tears, depressions, environmental stress cracking (ESC), and metal ion

oxidation (MIO). A break in the conductor of a lead is defined as the loss of continuity in the metallic components that could interrupt the current flow or voltage. Examples include fractured conductors and defective crimps.

Leads damaged after explant or damaged due to failure to heed warnings or contraindications in the labeling are not considered device malfunctions.

A lead subject to a safety advisory is not considered to have malfunctioned unless it has been returned to Medtronic CRDM and found, through analysis, to actually have performed outside the performance limits established by Medtronic.

For leads designed for either ventricular or atrial use, the numbers listed in the Returned Product Analysis tables include both.

The numbers of malfunctions listed in the Returned Product Analysis tables are the actual numbers confirmed in the returned product analysis from the United States. The numbers of complications listed in the complications tables are the actual numbers observed in the SLS centers around the world.

Estimated Number of Implanted and Active Leads in the United States

In addition to providing the number of leads enrolled in the SLS, this report also provides estimates for the number of leads implanted in the United States and the number remaining active in the United States. The number of US implants is estimated based on the total number of leads sold in the United States. The number of active implants is estimated using the total number of leads sold and projections for normal patient mortality, elective replacement, and lead failure. The number of implanted leads and active leads is adjusted for underreporting of patient mortality, elective replacement, and lead failure.

Some lead models do not have a survival curve presented in this report. These lead models do not have a survival curve because they have insufficient sample size in the System Longevity Study. Returned Product Analysis results for these models are included here for reference and comparison.

Left-Heart Leads

2187 Attain


Product Characteristics

US Market Release	Aug-01	Serial Number Prefix	LEY	<u>US Returned Product Analysis</u>	
Estimated US Implants	17,200	Type and/or Fixation	Transvenous, Left Ventricular Cardiac Vein, Distal Continuous Curve	Implant Damage	7
Estimated US Active	10,200	Polarity	Unipolar	Electrical Malfunction	0
Advisories	None	Steroid	No	Other	16

System Longevity Study Results

Qualifying Complications 1 Total

Number of Leads Enrolled in Study	133	Failure to Capture	1
Cumulative Months of Follow-Up	5,441		
Number of Leads Active in Study	49		

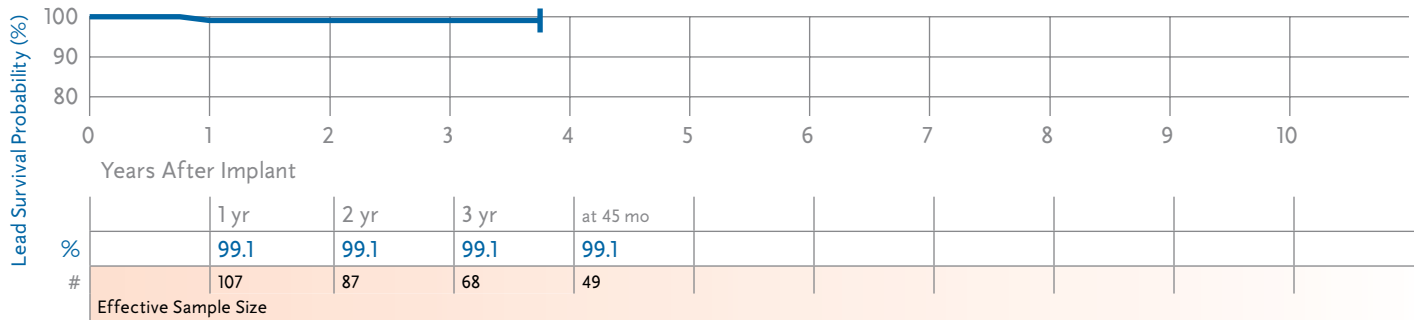

2188 Attain


Product Characteristics

US Market Release	Aug-01	Serial Number Prefix	LEB	<u>US Returned Product Analysis</u>	
Estimated US Implants	2,800	Type and/or Fixation	Transvenous, Coronary Sinus/ Cardiac Vein, Canted	Implant Damage	1
Estimated US Active	1,400	Polarity	Bipolar	Electrical Malfunction	1
Advisories	None	Steroid	No	Other	0

System Longevity Study Results

Qualifying Complications 1 Total

Number of Leads Enrolled in Study	14	Extra Cardiac Stimulation	1
Cumulative Months of Follow-Up	374		
Number of Leads Active in Study	3		

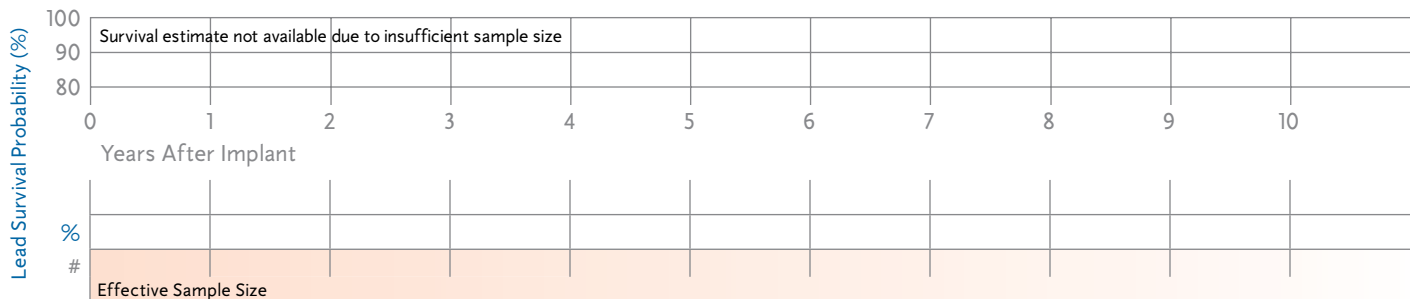

Leads

Left-Heart Leads continued

4193 Attain


Product Characteristics

US Market Release	May-02	Serial Number Prefix	BAA	<u>US Returned Product Analysis</u>	
Estimated US Implants	109,700	Type and/or Fixation	Transvenous, Left Ventricular Cardiac Vein, Distal Double Curve	Implant Damage	60
Estimated US Active	79,500	Polarity	Unipolar	Electrical Malfunction	17
Advisories	None	Steroid	Yes	Other	63

System Longevity Study Results

Qualifying Complications 31 Total

Number of Leads Enrolled in Study	670	Conductor Fracture	1
Cumulative Months of Follow-Up	19,080	Extra Cardiac Stimulation	5
Number of Leads Active in Study	292	Failure to Capture	11
		Lead Dislodgement	11
		Unspecified Clinical Failure	3

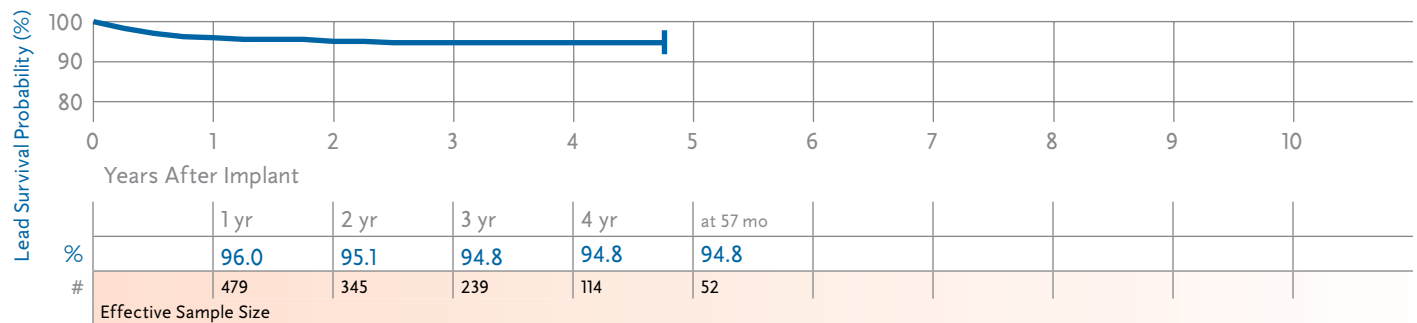

4194 Attain


Product Characteristics

US Market Release	Aug-04	Serial Number Prefix	LFG	<u>US Returned Product Analysis</u>	
Estimated US Implants	67,800	Type and/or Fixation	Transvenous, Left Ventricular Cardiac Vein, Distal Double Curve	Implant Damage	70
Estimated US Active	57,900	Polarity	Bipolar	Electrical Malfunction	2
Advisories	None	Steroid	Yes	Other	6

System Longevity Study Results

Qualifying Complications 5 Total

Number of Leads Enrolled in Study	364	Failure to Capture	1
Cumulative Months of Follow-Up	6,459	Lead Dislodgement	4
Number of Leads Active in Study	274		

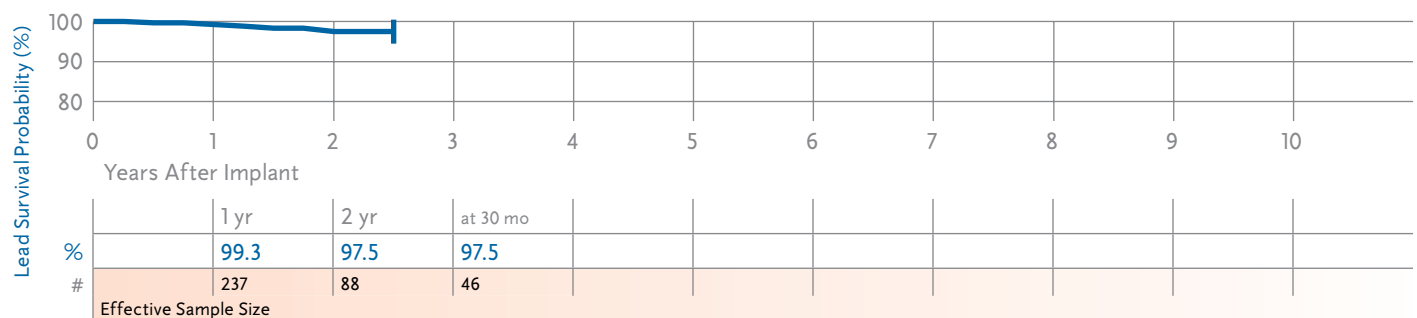

Lead Survival Summary (95% Confidence Interval)

Model Number	Family	US Market Release	Leads Enrolled	Leads Active in Study	Qualifying Complications	Cumulative Months of Follow-Up in Study	Device Survival Probability (%)									
							Years After Implant									
							1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	9 yr	10 yr
2187	Attain	Aug-01	133	49	1	5,441	99.1 +0.8/-5.3	99.1 +0.8/-5.3	99.1 +0.8/-5.3	99.1 +0.8/-5.3 at 45 mo						
2188	Attain	Aug-01	14	3	1	374	Survival estimate not available due to insufficient sample size									
4193	Attain	May-02	670	292	31	19,080	96.0 +1.3/-2.0	95.1 +1.5/-2.2	94.8 +1.6/-2.3	94.8 +1.6/-2.3	94.8 +1.6/-2.3 at 57 mo					
4194	Attain	Aug-04	364	274	5	6,459	99.3 +0.5/-2.1	97.5 +1.5/-3.7	97.5 +1.5/-3.7 at 30 mo							

Source: System Longevity Study
Data as of January 31, 2008

US Returned Product Analysis Summary

Model Number	Family	US Market Release	Estimated US Implants	Estimated US Active	Implant Damage	Electrical Malfunction	Other
2187	Attain	Aug-01	17,200	10,200	7	0	16
2188	Attain	Aug-01	2,800	1,400	1	1	0
4193	Attain	May-02	109,700	79,500	60	17	63
4194	Attain	Aug-04	67,800	57,900	70	2	6

Source: Returned Product Analysis
Data as of January 31, 2008

Reference Chart

Model Number	Family	Type	Insulation	Conductor Material	Tip Electrode	Connector Type
2187	Attain	Transvenous Cardiac Vein Preformed Body	Polyurethane (55D)	MP35N	Platinized Platinum	IS-1 UNI
2188	Attain	Transvenous Cardiac Vein Preformed Body	Polyurethane (55D)	MP35N	Platinized Platinum	IS-1 BI
4193	Attain	Transvenous Cardiac Vein Preformed Body	Polyurethane (55D)	MP35N	Platinized Platinum	IS-1 UNI
4194	Attain	Transvenous Cardiac Vein Preformed Body	Polyurethane (55D)/ Silicone (4719)	MP35N	Platinum Alloy	IS-1 BI

Defibrillation Leads

6721, 6921 Epicardial Patch

Product Characteristics


US Market Release	Feb-93	Serial Number Prefix	TBH, TBG, TBB, TAD, TAC, or TAB	<u>US Returned Product Analysis</u>	
Estimated US Implants	9,100	Type and/or Fixation	Epicardial Defib Patch, Suture	Implant Damage	5
Estimated US Active	2,100	Polarity	Defib Electrode only	Electrical Malfunction	79
Advisories	None	Steroid	No	Other	0

System Longevity Study Results

Number of Leads Enrolled in Study	407
Cumulative Months of Follow-Up	18,151
Number of Leads Active in Study	14

Qualifying Complications 28 Total

Conductor Fracture	20
Failure to Capture	2
Impedance Out of Range	3
Insulation (not further defined)	3

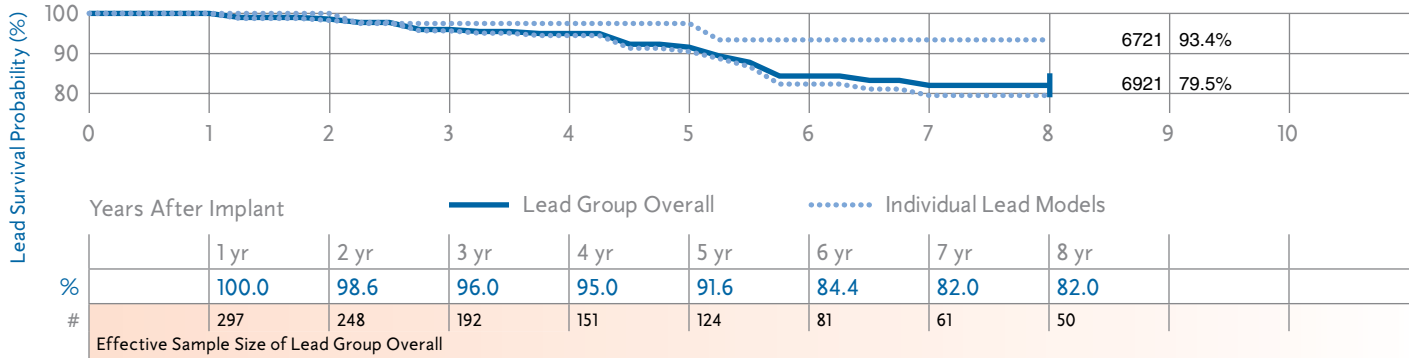

6930 Sprint Fidelis


Product Characteristics

US Market Release	Sep-04	Serial Number Prefix	LFK	<u>US Returned Product Analysis</u>	
Estimated US Implants	400	Type and/or Fixation	Transvenous, Vent, Defib and Pace/ Sense, Tines	Implant Damage	0
Estimated US Active	300	Polarity	True Bipolar/One Coil	Electrical Malfunction	2
Advisories	1	Steroid	Yes	Other	0
see page 144 – 2007 Potential Conductor Wire Fracture					

System Longevity Study Results

Number of Leads Enrolled in Study	4
Cumulative Months of Follow-Up	35
Number of Leads Active in Study	4

Qualifying Complications 0 Total

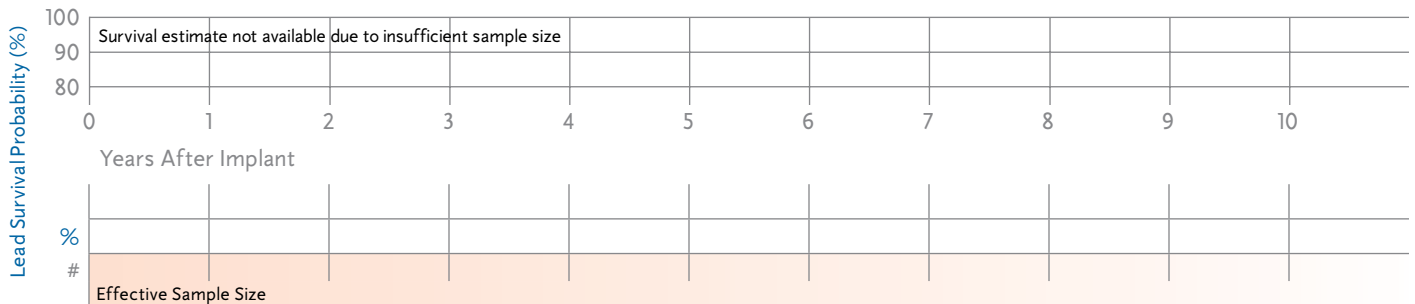

Defibrillation Leads continued

6931 Sprint Fidelis


Product Characteristics

US Market Release	Sep-04	Serial Number Prefix	LFL	US Returned Product Analysis	
Estimated US Implants	8,300	Type and/or Fixation	Transvenous, Vent, Defib and Pace/ Sense, Screw-in	Implant Damage	25
Estimated US Active	7,200	Polarity	True Bipolar/One Coil	Electrical Malfunction	49
Advisories	1	Steroid	Yes	Other	0
see page 144 – 2007 Potential Conductor Wire Fracture					

System Longevity Study Results

Qualifying Complications 8 Total

Number of Leads Enrolled in Study	240	Failure to Capture	3	Lead Dislodgement	1
Cumulative Months of Follow-Up	3,616	Failure to Sense	1	Oversensing	2
Number of Leads Active in Study	201	Impedance Out of Range	1		

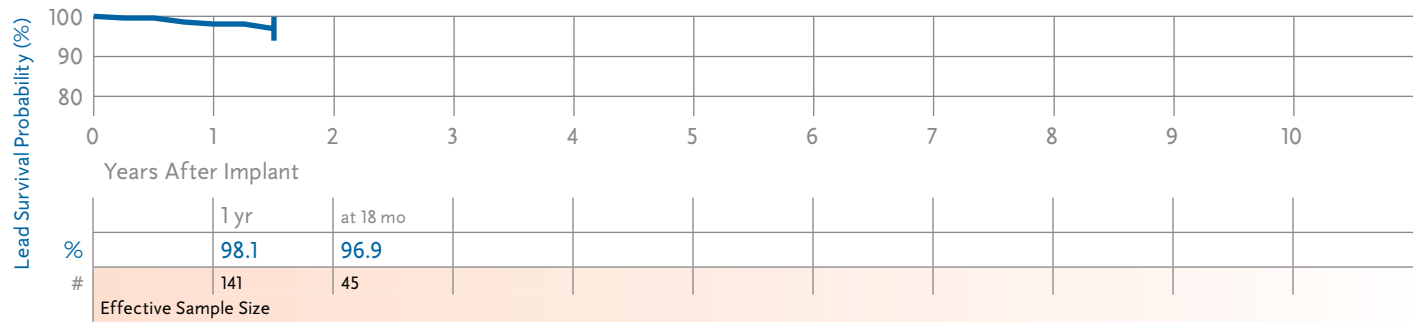

6932 Sprint


Product Characteristics

US Market Release	Aug-96	Serial Number Prefix	TCA	US Returned Product Analysis	
Estimated US Implants	15,300	Type and/or Fixation	Transvenous, Vent, Defib and Pace/ Sense, Tines	Implant Damage	16
Estimated US Active	6,200	Polarity	True Bipolar/One Coil	Electrical Malfunction	37
Advisories	None	Steroid	Yes	Other	7

System Longevity Study Results

Qualifying Complications 8 Total

Number of Leads Enrolled in Study	410	Extra Cardiac Stimulation	1
Cumulative Months of Follow-Up	20,051	Failure to Capture	2
Number of Leads Active in Study	81	Failure to Sense	2
		Oversensing	3

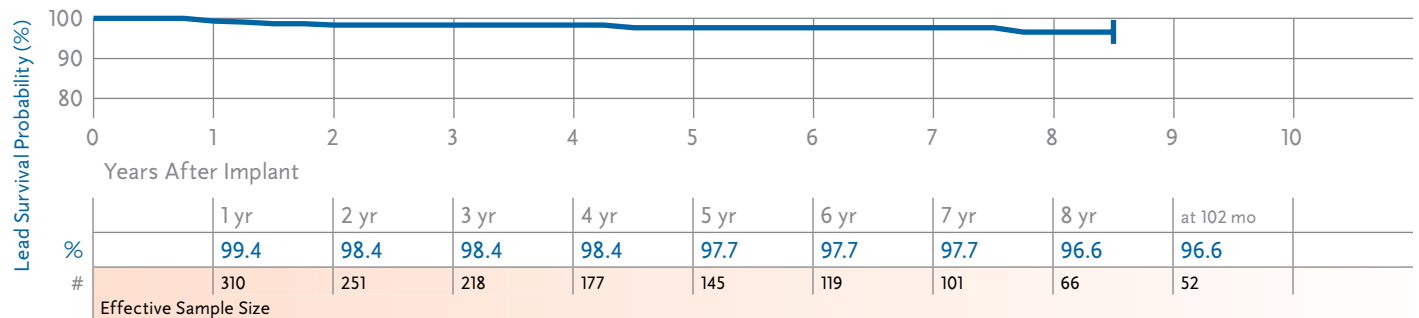

Leads

Defibrillation Leads continued

6933, 6937, 6937A, 6963 SVC/CS


Product Characteristics

US Market Release	Dec-93	Serial Number Prefix	TAT, TBU, or TAF	<u>US Returned Product Analysis</u>	
Estimated US Implants	17,500	Type and/or Fixation	Transvenous CS or SVC Defib	Implant Damage	31
Estimated US Active	5,400	Polarity	One Defib Coil	Electrical Malfunction	195
Advisories	None	Steroid	No	Other	13

System Longevity Study Results

Qualifying Complications 24 Total

Number of Leads Enrolled in Study	966	Conductor Fracture	15	Lead Dislodgement	1
Cumulative Months of Follow-Up	47,305	Failure to Capture	1	Unspecified Clinical Failure	3
Number of Leads Active in Study	47	Impedance Out of Range	2		
		Insulation (not further defined)	2		

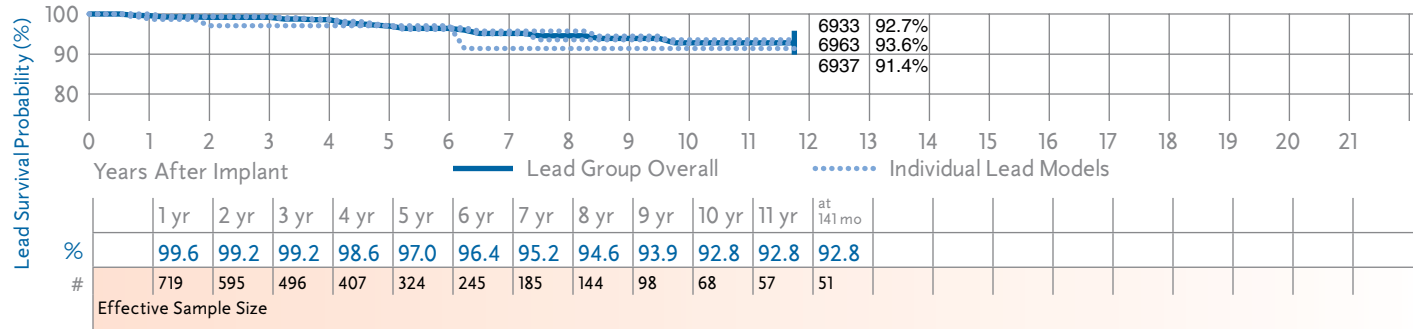

6936, 6966 Transvene


Product Characteristics

US Market Release	Dec-93	Serial Number Prefix	TAV or TAL	<u>US Returned Product Analysis</u>	
Estimated US Implants	24,600	Type and/or Fixation	Transvenous, Vent, Defib and Pace/Sense, Screw-in	Implant Damage	90
Estimated US Active	5,600	Polarity	True Bipolar/One Coil	Electrical Malfunction	458
Advisories	None	Steroid	No	Other	19

System Longevity Study Results

Qualifying Complications 146 Total

Number of Leads Enrolled in Study	1,349	Conductor Fracture	18	Oversensing	91
Cumulative Months of Follow-Up	67,001	Extra Cardiac Stimulation	2	Unspecified Clinical Failure	5
Number of Leads Active in Study	49	Failure to Capture	8		
		Failure to Sense	4		
		Impedance Out of Range	4		
		Insulation (not further defined)	14		

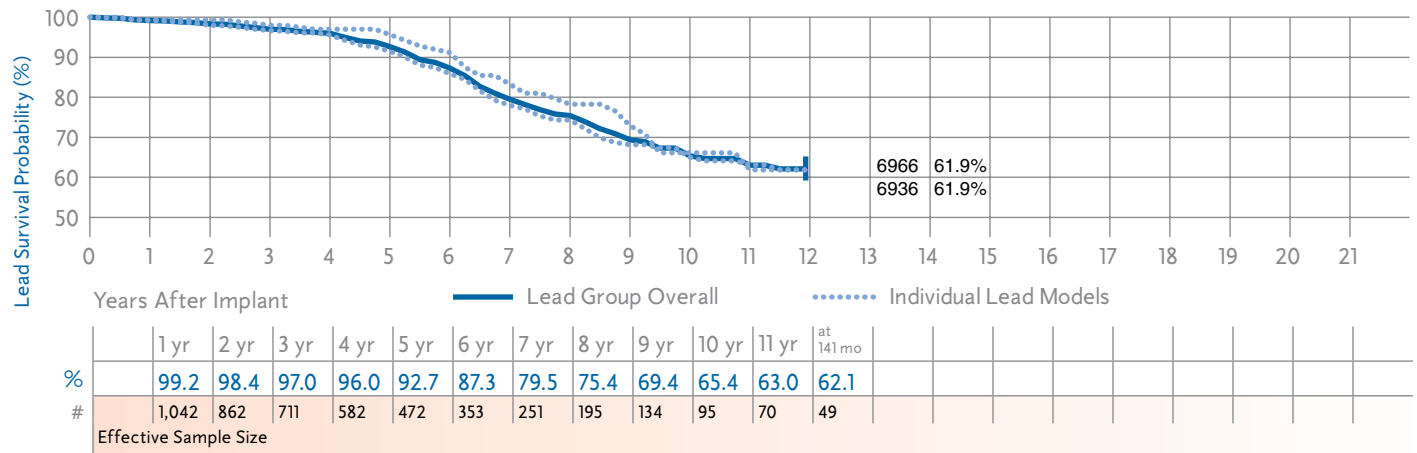

Defibrillation Leads continued

6939, 6999 Sub-Q Patch

Product Characteristics


US Market Release	Dec-93	Serial Number Prefix	TBA or TAP	<u>US Returned Product Analysis</u>	
Estimated US Implants	4,300	Type and/or Fixation	Subcutaneous Defib Patch, Suture	Implant Damage	4
Estimated US Active	900	Polarity	Defib Electrode Only	Electrical Malfunction	33
Advisories	None	Steroid	No	Other	1

System Longevity Study Results

Number of Leads Enrolled in Study	384
Cumulative Months of Follow-Up	17,618
Number of Leads Active in Study	7

Qualifying Complications 20 Total

Conductor Fracture	10
Failure to Capture	2
Insulation (not further defined)	6
Unspecified Clinical Failure	2

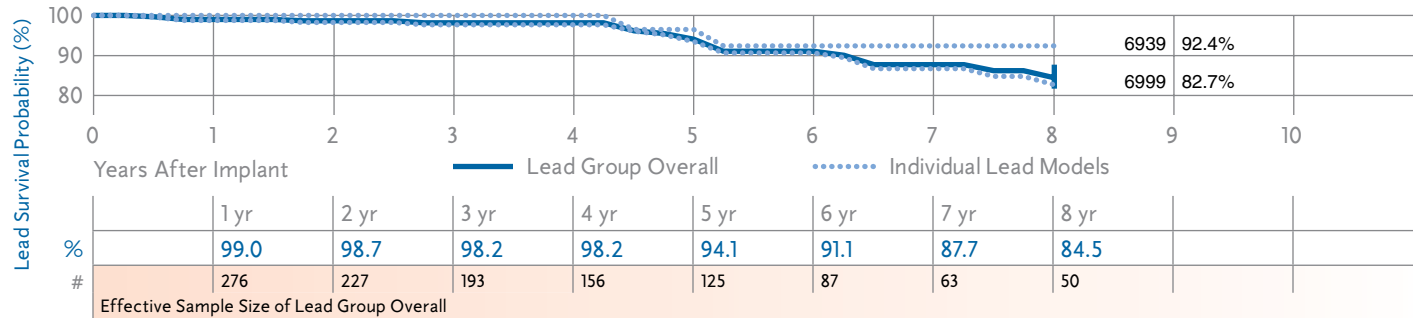

Leads

6942 Sprint

Product Characteristics


US Market Release	Jul-97	Serial Number Prefix	TCB	<u>US Returned Product Analysis</u>	
Estimated US Implants	18,100	Type and/or Fixation	Transvenous, Vent, Defib and Pace/Sense, Tines	Implant Damage	31
Estimated US Active	7,900	Polarity	Integrated Bipolar/Two Coils	Electrical Malfunction	37
Advisories	None	Steroid	Yes	Other	5

System Longevity Study Results

Number of Leads Enrolled in Study	352
Cumulative Months of Follow-Up	14,944
Number of Leads Active in Study	63

Qualifying Complications 7 Total

Conductor Fracture	1
Failure to Sense	1
Lead Dislodgement	1
Oversensing	3
Unspecified Clinical Failure	1

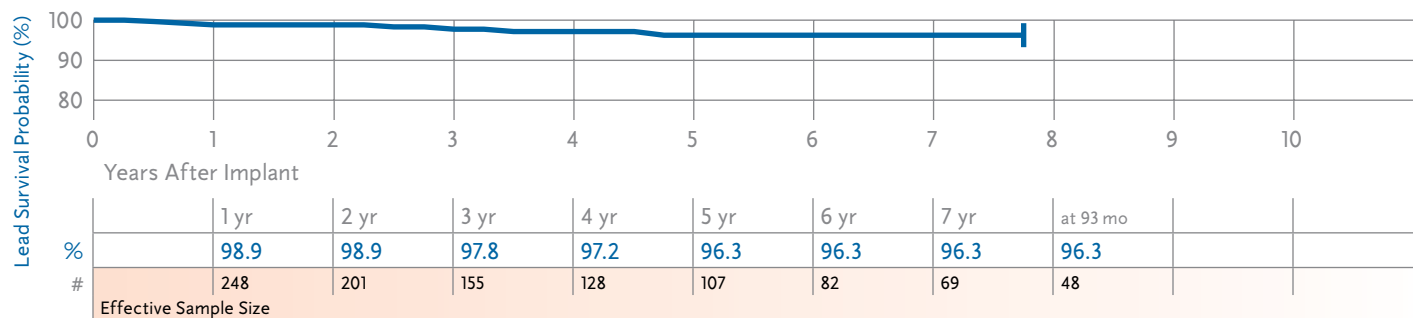

Defibrillation Leads continued

6943 Sprint


Product Characteristics

US Market Release	Oct-97	Serial Number Prefix	TCE	<u>US Returned Product Analysis</u>	
Estimated US Implants	21,300	Type and/or Fixation	Transvenous, Vent, Defib and Pace/Sense, Screw-in	Implant Damage	50
Estimated US Active	9,400	Polarity	True Bipolar/One Coil	Electrical Malfunction	65
Advisories	None	Steroid	Yes	Other	8

System Longevity Study Results

Qualifying Complications 62 Total

Number of Leads Enrolled in Study	1,311	Conductor Fracture	9	Lead Dislodgement	1
Cumulative Months of Follow-Up	62,114	Failure to Capture	7	Oversensing	32
Number of Leads Active in Study	507	Failure to Sense	6	Unspecified Clinical Failure	3
		Impedance Out of Range	3		
		Insulation (not further defined)	1		

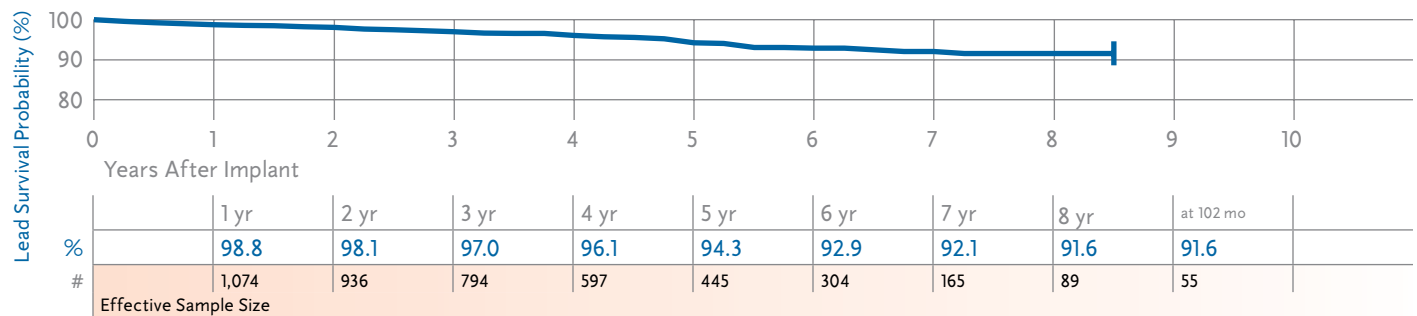

6944 Sprint Quattro


Product Characteristics

US Market Release	Dec-00	Serial Number Prefix	TDC	<u>US Returned Product Analysis</u>	
Estimated US Implants	29,200	Type and/or Fixation	Transvenous, Vent, Defib and Pace/Sense, Tines	Implant Damage	24
Estimated US Active	18,400	Polarity	True Bipolar/Two Coils	Electrical Malfunction	32
Advisories	None	Steroid	Yes	Other	8

System Longevity Study Results

Qualifying Complications 3 Total

Number of Leads Enrolled in Study	171	Oversensing	2
Cumulative Months of Follow-Up	6,688	Unspecified Clinical Failure	1
Number of Leads Active in Study	64		

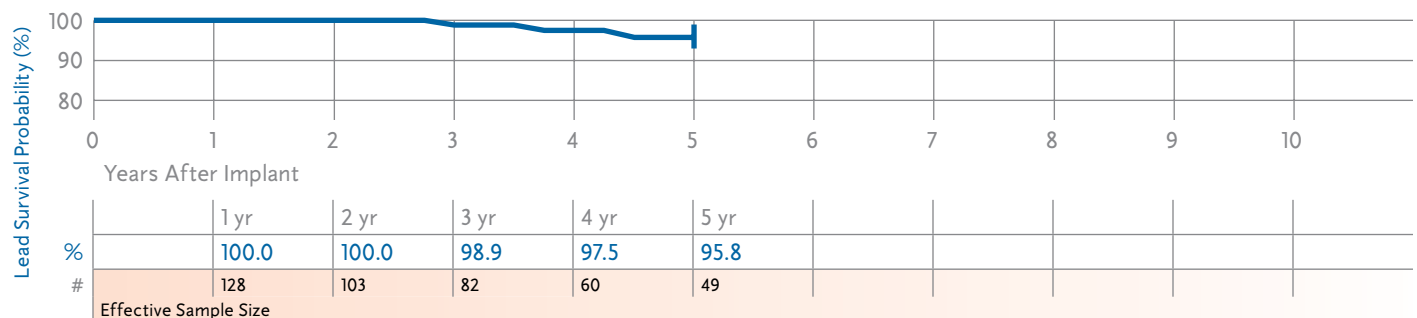

Defibrillation Leads continued

6945 Sprint


Product Characteristics

US Market Release	Sep-97	Serial Number Prefix	TDA	<u>US Returned Product Analysis</u>	
Estimated US Implants	44,000	Type and/or Fixation	Transvenous, Vent, Defib and Pace/Sense, Screw-in	Implant Damage	198
Estimated US Active	20,800	Polarity	Integrated Bipolar/Two Coils	Electrical Malfunction	95
Advisories	None	Steroid	Yes	Other	11

System Longevity Study Results

Qualifying Complications 27 Total

Number of Leads Enrolled in Study	1,158	Conductor Fracture	2	Impedance Out of Range	5
Cumulative Months of Follow-Up	52,625	Extra Cardiac Stimulation	1	Oversensing	13
Number of Leads Active in Study	283	Failure to Capture	1	Unspecified Clinical Failure	1
		Failure to Sense	4		

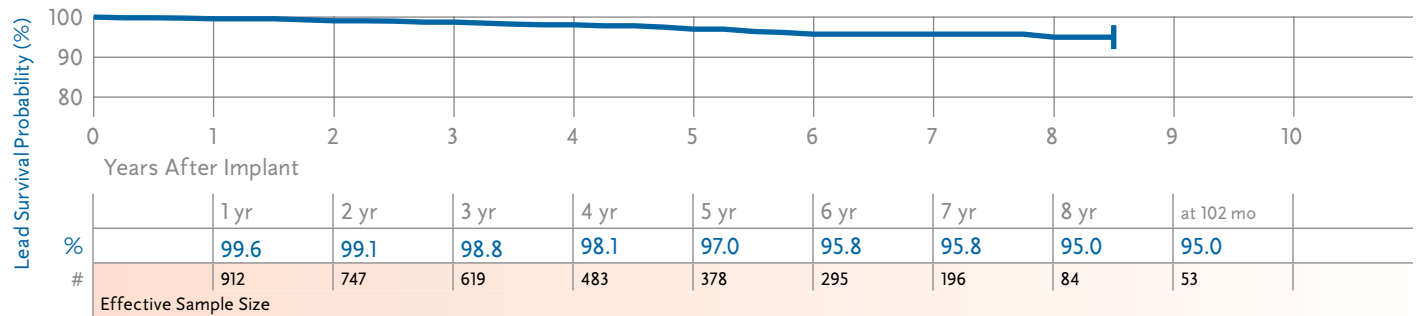

Leads

6947 Sprint Quattro Secure


Product Characteristics

US Market Release	Nov-01	Serial Number Prefix	TDG	<u>US Returned Product Analysis</u>	
Estimated US Implants	142,400	Type and/or Fixation	Transvenous, Vent, Defib and Pace/Sense, Screw-in	Implant Damage	237
Estimated US Active	99,500	Polarity	True Bipolar/Two Coils	Electrical Malfunction	92
Advisories	None	Steroid	Yes	Other	12

System Longevity Study Results

Qualifying Complications 18 Total

Number of Leads Enrolled in Study	1,367	Conductor Fracture	3	Lead Dislodgement	3
Cumulative Months of Follow-Up	48,899	Failure to Sense	1	Oversensing	7
Number of Leads Active in Study	694	Impedance Out of Range	1	Unspecified Clinical Failure	2
		Insulation (not further defined)	1		

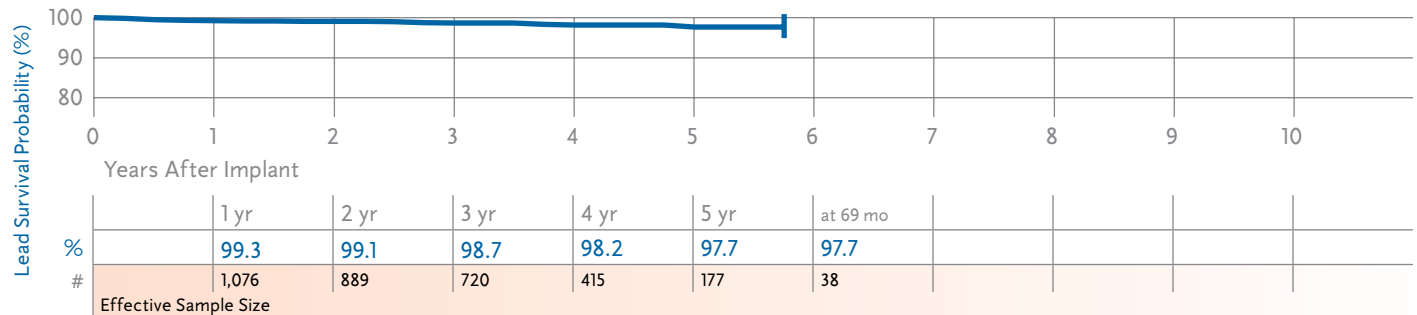

Defibrillation Leads continued

6948 Sprint Fidelis


Product Characteristics

US Market Release	Sep-04	Serial Number Prefix	LFH	<u>US Returned Product Analysis</u>	
Estimated US Implants	10,700	Type and/or Fixation	Transvenous, Vent, Defib and Pace/ Sense, Tines	Implant Damage	9
Estimated US Active	9,200	Polarity	True Bipolar/Two Coils	Electrical Malfunction	10
Advisories	1	Steroid	Yes	Other	4
see page 144 – 2007 Potential Conductor Wire Fracture					

System Longevity Study Results

Qualifying Complications 0 Total

Number of Leads Enrolled in Study	29
Cumulative Months of Follow-Up	486
Number of Leads Active in Study	27

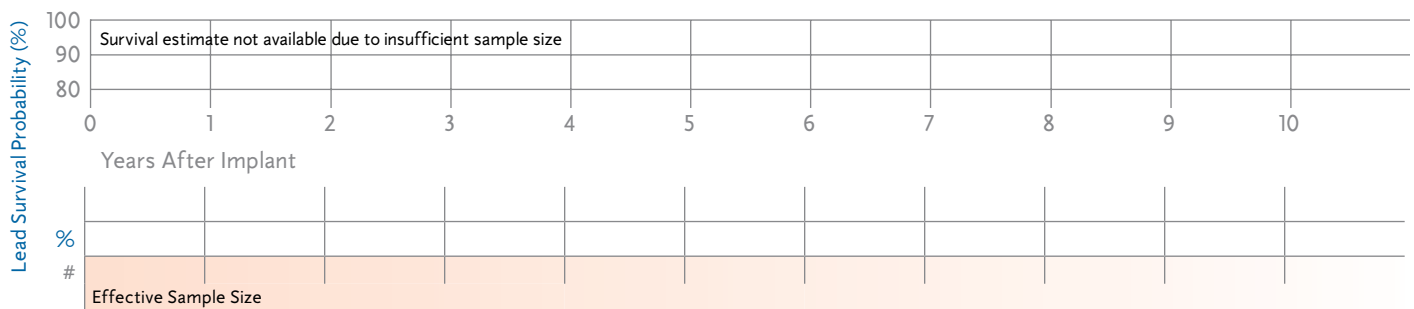

6949 Sprint Fidelis


Product Characteristics

US Market Release	Sep-04	Serial Number Prefix	LFJ	<u>US Returned Product Analysis</u>	
Estimated US Implants	188,200	Type and/or Fixation	Transvenous, Vent, Defib and Pace/ Sense, Screw-in	Implant Damage	448
Estimated US Active	157,900	Polarity	True Bipolar/Two Coils	Electrical Malfunction	702
Advisories	1	Steroid	Yes	Other	41
see page 144 – 2007 Potential Conductor Wire Fracture					

System Longevity Study Results

Qualifying Complications 14 Total

Number of Leads Enrolled in Study	735	Conductor Fracture	1	Lead Dislodgement	1
Cumulative Months of Follow-Up	13,839	Failure to Capture	2	Oversensing	8
Number of Leads Active in Study	607	Failure to Sense	1		
		Insulation (not further defined)	1		

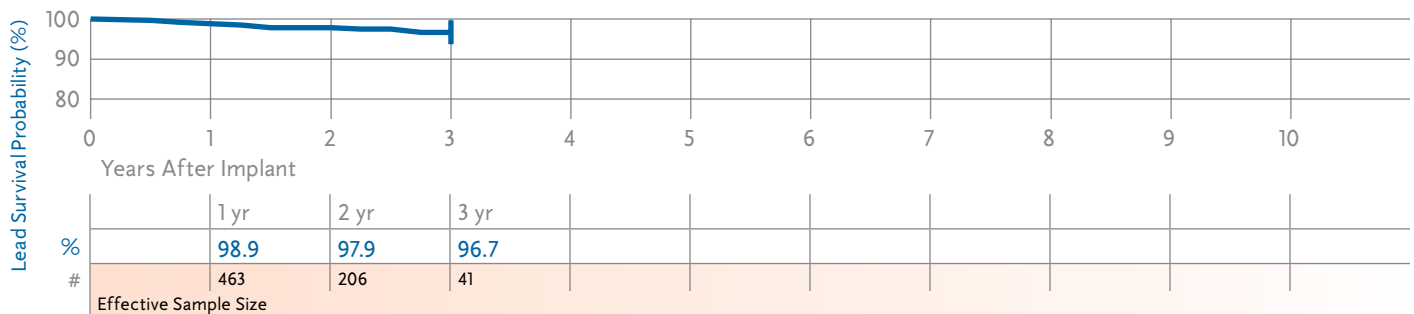

Defibrillation Leads continued

6996 Sub-Q Lead


Product Characteristics

		Product Characteristics		US Returned Product Analysis	
US Market Release	Jun-01	Serial Number Prefix	TCR	Implant Damage	0
Estimated US Implants	2,500	Type and/or Fixation	Subcutaneous Defib Coil, Suture	Electrical Malfunction	2
Estimated US Active	2,000	Polarity	One Defib Coil	Other	0
Advisories	None	Steroid	No		

System Longevity Study Results

Qualifying Complications 0 Total

Number of Leads Enrolled in Study	12
Cumulative Months of Follow-Up	292
Number of Leads Active in Study	12

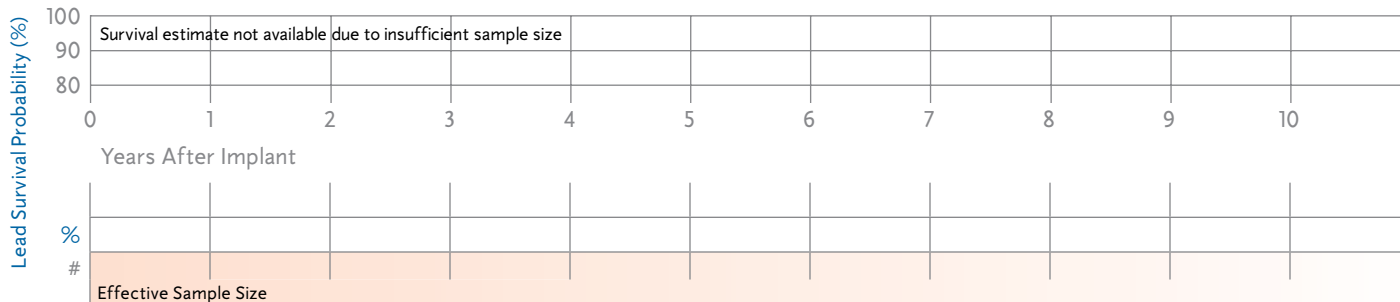

Leads

Defibrillation Leads continued

Lead Survival Summary (95% Confidence Interval)

Model Number	Family	US Market Release	Leads Enrolled	Leads Active in Study	Qualifying Complications	Cumulative Months of Follow-Up in Study	Device Survival Probability (%)											
							Years After Implant											
							1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	12 yr		
6721, 6921	Epicardial Patch	Feb-93	407	14	28	18,151	100.0	98.6 +0.9/-2.3	96.0 +1.9/-3.3	95.0 +2.1/-3.8	91.6 +3.2/-4.9	84.4 +4.9/-7.0	82.0 +5.6/-7.6	82.0 +5.6/-7.6				
6930	Sprint Fidelis	Sep-04	4	4	—	35	Survival estimate not available due to insufficient sample size											
	Advisories: see page 144 - 2007 Potential Conductor Wire Fracture																	
6931	Sprint Fidelis	Sep-04	240	201	8	3,616	98.1 +1.2/-3.2	96.9 +1.2/-4.9 at 18 mo										
	Advisories: see page 144 - 2007 Potential Conductor Wire Fracture																	
6932	Sprint	Aug-96	410	81	8	20,051	99.4 +0.4/-1.8	98.4 +0.9/-2.3	98.4 +0.9/-2.3	98.4 +0.9/-2.3	97.7 +1.3/-2.8	97.7 +1.3/-2.8	97.7 +1.3/-2.8	96.6 +2.0/-4.6	96.6 +2.0/-4.6 at 102 mo			
6933, 6937, 6937A, 6963	SVC/CS	Dec-93	966	47	24	47,305	99.6 +0.3/-0.8	99.2 +0.4/-1.0	99.2 +0.4/-1.0	98.6 +0.7/-1.4	97.0 +1.2/-2.0	96.4 +1.4/-2.2	95.2 +1.8/-2.8	94.6 +2.0/-3.1	92.8 +2.8/-4.6	92.8 +2.8/-4.6 at 141 mo		
6936, 6966	Transvene	Dec-93	1,349	49	146	67,001	99.2 +0.4/-0.7	98.4 +0.6/-1.0	97.0 +0.9/-1.3	96.0 +1.1/-1.6	92.7 +1.7/-2.3	87.3 +2.5/-3.0	79.5 +3.4/-4.0	75.4 +3.9/-4.4	65.4 +5.1/-5.8	62.1 +5.7/-6.4		
6939, 6999	Sub-Q Patch	Dec-93	384	7	20	17,618	99.0 +0.7/-1.9	98.7 +0.8/-2.3	98.2 +1.0/-2.6	98.2 +1.0/-2.6	94.1 +2.7/-4.7	91.1 +3.6/-5.7	87.7 +4.7/-7.1	84.5 +5.8/-8.6				
6942	Sprint	Jul-97	352	63	7	14,944	98.9 +0.8/-2.2	98.9 +0.8/-2.2	97.8 +1.3/-3.1	97.2 +1.5/-3.6	96.3 +2.0/-4.1	96.3 +2.0/-4.1	96.3 +2.0/-4.1	96.3 +2.0/-4.1 at 93 mo				
6943	Sprint	Oct-97	1,311	507	62	62,114	98.8 +0.5/-0.8	98.1 +0.6/-1.0	97.0 +0.8/-1.3	96.1 +1.1/-1.4	94.3 +1.4/-2.0	92.9 +1.7/-2.3	92.1 +2.0/-2.5	91.6 +2.1/-2.9	91.6 +2.1/-2.9 at 102 mo			
6944	Sprint Quattro	Dec-00	171	64	3	6,688	100.0	100.0	98.9 +0.9/-6.8	97.5 +1.9/-7.2	95.8 +2.8/-8.6							
6945	Sprint	Sep-97	1,158	283	27	52,625	99.6 +0.2/-0.7	99.1 +0.5/-0.9	98.8 +0.6/-1.0	98.1 +0.8/-1.2	97.0 +1.1/-1.8	95.8 +1.5/-2.2	95.8 +1.5/-2.2	95.0 +1.9/-3.2 at 102 mo				
6947	Sprint Quattro Secure	Nov-01	1,367	694	18	48,899	99.3 +0.3/-0.7	99.1 +0.4/-0.8	98.7 +0.5/-0.9	98.2 +0.7/-1.2	97.7 +1.0/-1.6	97.7 +1.0/-1.6 at 69 mo						
6948	Sprint Fidelis	Sep-04	29	27	0	486	Survival estimate not available due to insufficient sample size											
	Advisories: see page 144 - 2007 Potential Conductor Wire Fracture																	
6949	Sprint Fidelis	Sep-04	735	607	14	13,839	98.9 +0.6/-1.2	97.9 +1.0/-1.7	96.7 +1.6/-3.1									
	Advisories: see page 144 - 2007 Potential Conductor Wire Fracture																	
6996	Sub-Q Lead	Jun-01	12	12	0	292	Survival estimate not available due to insufficient sample size											

US Returned Product Analysis Summary

Model Number	Family	US Market Release	Estimated US Implants	Estimated US Active	Implant Damage	Electrical Malfunction	Other
6721, 6921	Epicardial Patch	Feb-93	9,100	2,100	5	79	0
6930	Sprint Fidelis	Sep-04	400	300	0	2	0
6931	Sprint Fidelis	Sep-04	8,300	7,200	25	49	0
6932	Sprint	Aug-96	15,300	6,200	16	37	7
6933, 6937, 6937A, 6963	SVC/CS	Dec-93	17,500	5,400	31	195	13
6936, 6966	Transvene	Dec-93	24,600	5,600	90	458	19
6939, 6999	Sub-Q Patch	Dec-93	4,300	900	4	33	1
6942	Sprint	Jul-97	18,100	7,900	31	37	5
6943	Sprint	Oct-97	21,300	9,400	50	65	8
6944	Sprint Quattro	Dec-00	29,200	18,400	24	32	8
6945	Sprint	Sep-97	44,000	20,800	198	95	11
6947	Sprint Quattro Secure	Nov-01	142,400	99,500	237	92	12
6948	Sprint Fidelis	Sep-04	10,700	9,200	9	10	4
6949	Sprint Fidelis	Sep-04	188,200	157,900	448	702	41
6996	Sub-Q Lead	Jun-01	2,500	2,000	0	2	0

Reference Chart

Model Number	Family	Type	Pin Configuration		Lead Body Diameter	Insulation, Lead Body	Fixation, Steroid
			Pace/ Sense	High Voltage			
6721	Epicardial Patch	Epi Patch	—	DF-1	S, M, L	Silicone, Single Lumen	Suture
6921	Epicardial Patch	Epi Patch	—	6.5 mm	S, M, L	Silicone, Single Lumen	Suture
6930	Sprint Fidelis	Endo RV True Bipolar Sensing	IS-1	DF-1	6.6 Fr	Silicone with Polyurethane Overlay, Multilumen	Passive, Steroid
6931	Sprint Fidelis	Endo RV True Bipolar Sensing	IS-1	DF-1	6.6 Fr	Silicone with Polyurethane Overlay, Multilumen	Active, Steroid
6932	Sprint	Endo RV True Bipolar Sensing	IS-1	DF-1	7.8 Fr	Silicone, Multilumen	Passive, Steroid
6933	SVC/CS	Endo SVC/CS Coil	—	DF-1	7 Fr	Silicone, Single Lumen	Passive
6934S	Transvene	Endo RV True Bipolar Sensing	IS-1	DF-1	12 Fr	Silicone, Coaxial	Passive, Steroid
6936	Transvene	Endo RV True Bipolar Sensing	IS-1	DF-1	10 Fr	Polyurethane, Coaxial	Active
6937	SVC/CS	Endo SVC Coil	—	DF-1	5.5 Fr	Silicone, Single Lumen	Passive
6937A	SVC/CS	Endo SVC Coil	—	DF-1	7.5 Fr	Silicone with Polyurethane Overlay, Single Lumen	Passive
6939	Sub-Q Patch	SQ Patch	—	DF-1	One Size	Silicone, Single Lumen	Suture
6942	Sprint	Endo RV/SVC Integrated Bipolar Sensing	IS-1	2 DF-1	7.8 Fr	Silicone, Multilumen	Passive, Steroid
6943	Sprint	Endo RV True Bipolar Sensing	IS-1	DF-1	7.8 Fr	Silicone, Multilumen	Active, Steroid
6944	Sprint Quattro	Endo RV/SVC True Bipolar Sensing	IS-1	2 DF-1	8.2 Fr	Silicone with Polyurethane Overlay, Multilumen	Passive, Steroid
6945	Sprint	Endo RV/SVC Integrated Bipolar Sensing	IS-1	2 DF-1	7.8 Fr	Silicone, Multilumen	Active, Steroid
6947	Sprint Quattro Secure	Endo RV/SVC True Bipolar Sensing	IS-1	2 DF-1	8.2 Fr	Silicone with Polyurethane Overlay, Multilumen	Active, Steroid
6948	Sprint Fidelis	Endo RV/SVC True Bipolar Sensing	IS-1	2 DF-1	6.6 Fr	Silicone with Polyurethane Overlay, Multilumen	Passive, Steroid
6949	Sprint Fidelis	Endo RV/SVC True Bipolar Sensing	IS-1	2 DF-1	6.6 Fr	Silicone with Polyurethane Overlay, Multilumen	Active, Steroid
6963	SVC/CS	Endo SVC/CS Coil	—	6.5 mm	7 Fr	Silicone, Single Lumen	Passive
6966	Transvene	Endo RV True Bipolar Sensing	3.2 mm L.P.	6.5 mm	10 Fr	Polyurethane, Coaxial	Active
6996	Sub-Q Lead	SQ Coil	—	DF-1	7.5 Fr	Silicone, Single Lumen	Passive
6999	Sub-Q Patch	SQ Patch	—	6.5 mm	One Size	Silicone, Single Lumen	Suture

Pacing Leads

3830 SelectSecure

Product Characteristics


US Market Release	Aug-05	Serial Number Prefix	LFF	<u>US Returned Product Analysis</u>	
Estimated US Implants	9,100	Type and/or Fixation	Transvenous, V or A, Screw-in	Implant Damage	14
Estimated US Active	8,000	Polarity	Bipolar	Electrical Malfunction	2
Advisories	None	Steroid	Yes	Other	1

Atrial Placement

System Longevity Study Results

Qualifying Complications 1 Total

Number of Leads Enrolled in Study	152	Failure to Sense	1
Cumulative Months of Follow-Up	4,272		
Number of Leads Active in Study	91		

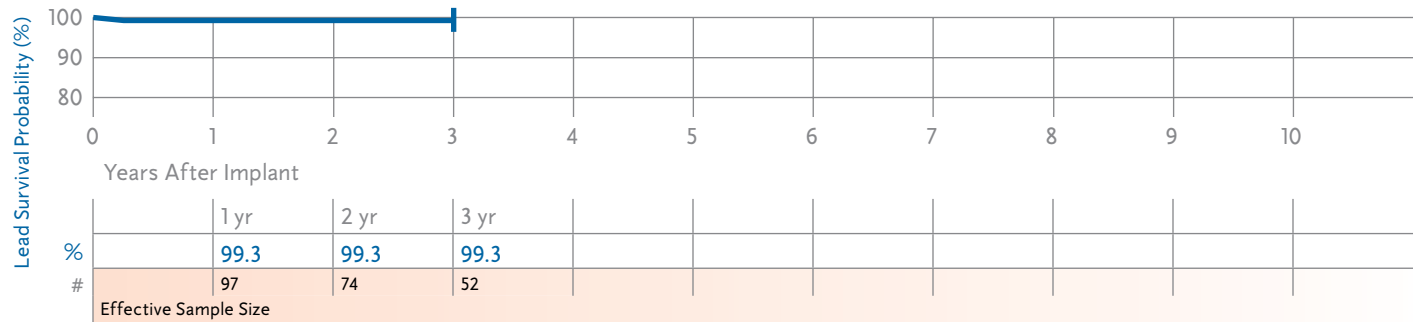


Ventricular Placement

System Longevity Study Results

Qualifying Complications 0 Total

Number of Leads Enrolled in Study	140
Cumulative Months of Follow-Up	4,233
Number of Leads Active in Study	85

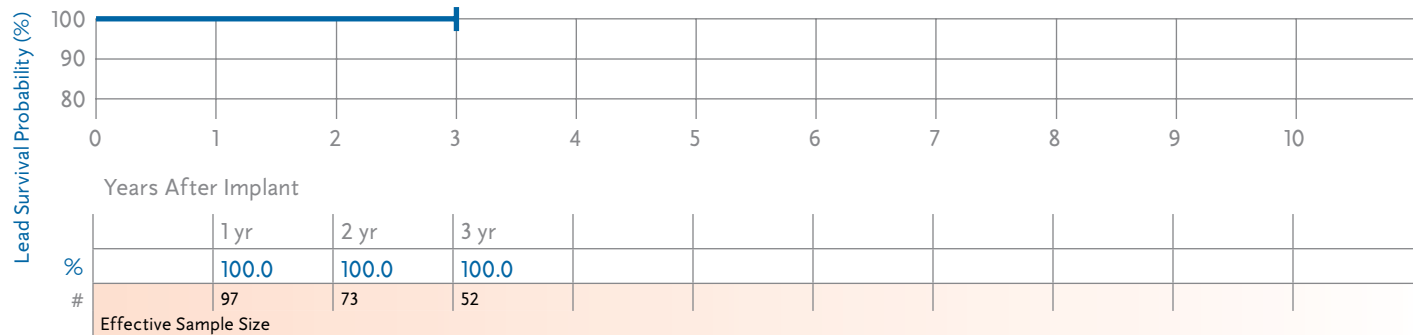

4003, 4003M CapSure

Product Characteristics


US Market Release	Jul-86	Serial Number Prefix	IH or LAX	<u>US Returned Product Analysis</u>	
Estimated US Implants	40,000	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	24
Estimated US Active	6,700	Polarity	Unipolar	Electrical Malfunction	58
Advisories	None	Steroid	Yes	Other	2

Ventricular Placement

System Longevity Study Results

Qualifying Complications

Number of Leads Enrolled in Study	711	Conductor Fracture	1	Failure to Sense	1
Cumulative Months of Follow-Up	45,711	Extra Cardiac Stimulation	2	Oversensing	2
Number of Leads Active in Study	159	Failure to Capture	6		

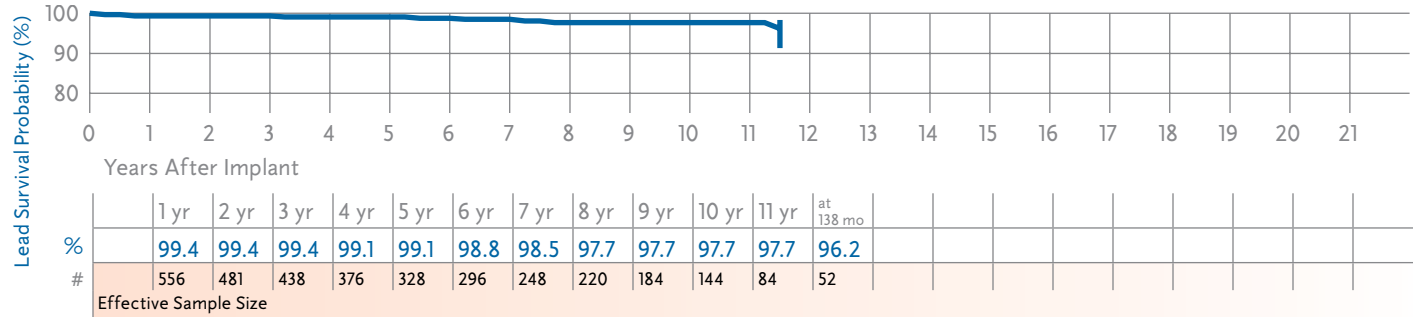

4004, 4004M CapSure

Product Characteristics


US Market Release	Feb-89	Serial Number Prefix	PS or LAV	<u>US Returned Product Analysis</u>	
Estimated US Implants	74,500	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	55
Estimated US Active	2,500	Polarity	Bipolar	Electrical Malfunction	684
Advisories	1	Steroid	Yes	Other	19
see page 150 – 1993 Lead Survival Below Expectations					

Ventricular Placement

System Longevity Study Results

Qualifying Complications 278 Total

Number of Leads Enrolled in Study	1,640	Conductor Fracture	7	Insulation (ESC)	4
Cumulative Months of Follow-Up	71,611	Electrical Abandonment	1	Insulation (MIO)	4
Number of Leads Active in Study	5	Extra Cardiac Stimulation	2	Insulation (not further defined)	8
		Failure to Capture	131	Medical Judgment	1
		Failure to Sense	62	Oversensing	25
		Impedance Out of Range	32	Unspecified Clinical Failure	1

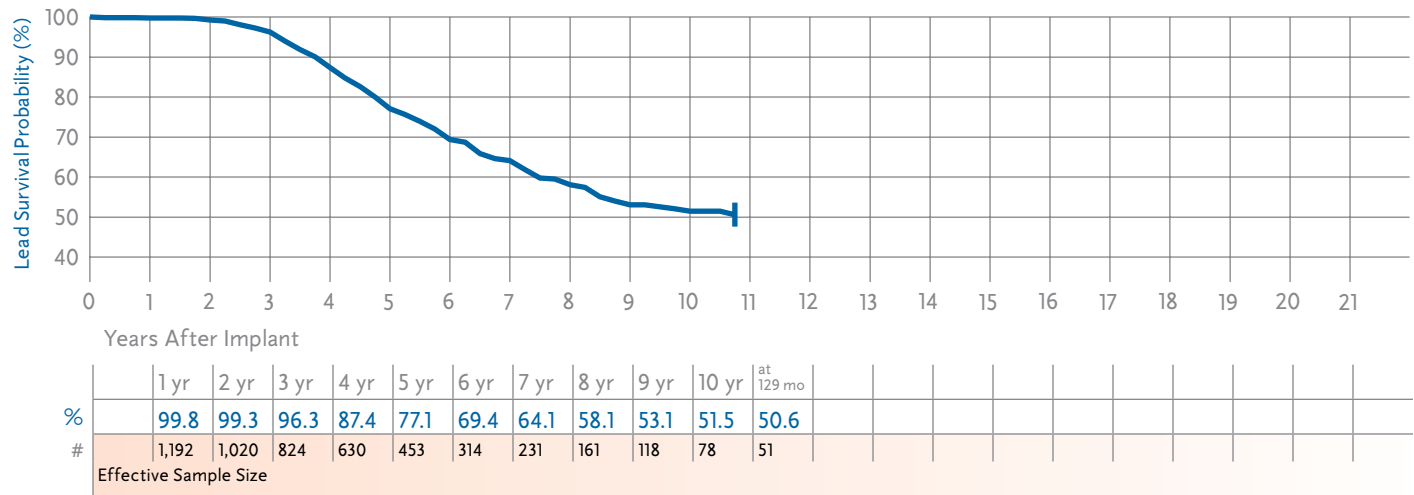

Leads

4011 Target Tip

Product Characteristics


US Market Release	Nov-82	Serial Number Prefix	IB	<u>US Returned Product Analysis</u>	
Estimated US Implants	64,000	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	29
Estimated US Active	6,900	Polarity	Unipolar	Electrical Malfunction	142
Advisories	None	Steroid	No	Other	5

Ventricular Placement

System Longevity Study Results

Qualifying Complications 25 Total

Number of Leads Enrolled in Study	851	Conductor Fracture	1	Insulation (not further defined)	10
Cumulative Months of Follow-Up	54,409	Extra Cardiac Stimulation	4	Oversensing	1
Number of Leads Active in Study	4	Failure to Capture	9		

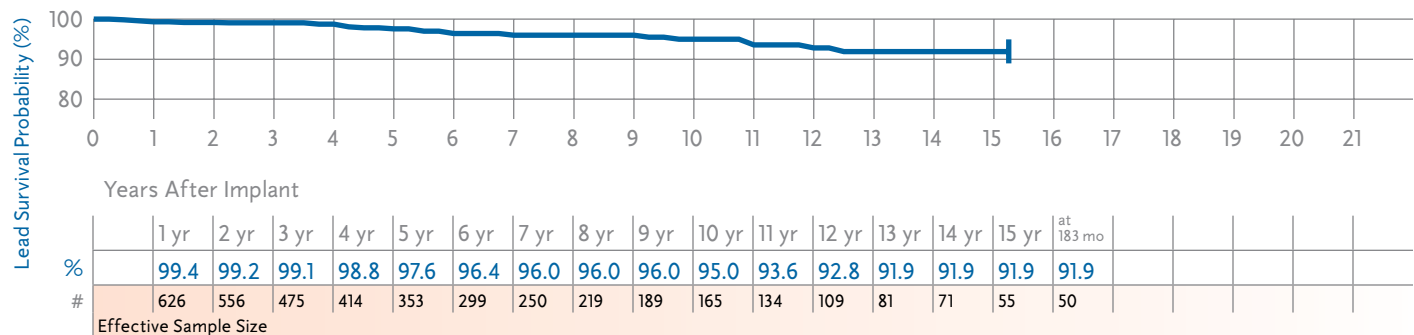

Pacing Leads continued

4012 Target Tip

Product Characteristics


US Market Release	Jul-83	Serial Number Prefix	HQ	<u>US Returned Product Analysis</u>	
Estimated US Implants	96,800	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	50
Estimated US Active	5,300	Polarity	Bipolar	Electrical Malfunction	820
Advisories	1	Steroid	No	Other	34
see page 151 – 1991 Lead Survival Below Expectations					

Ventricular Placement

System Longevity Study Results

Qualifying Complications 316 Total

Number of Leads Enrolled in Study	2,543	Conductor Fracture	6	Insulation (ESC)	9
Cumulative Months of Follow-Up	151,022	Extra Cardiac Stimulation	3	Insulation (MIO)	4
Number of Leads Active in Study	12	Failure to Capture	126	Insulation (not further defined)	16
		Failure to Sense	77	Medical Judgment	1
		Impedance Out of Range	26	Oversensing	48

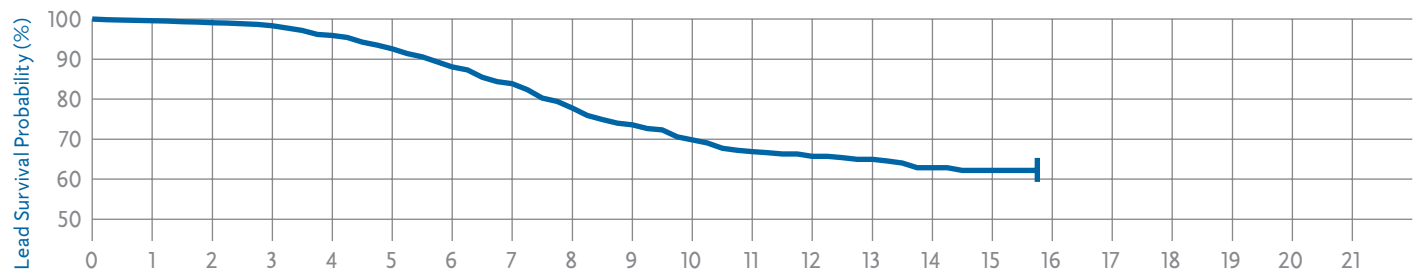

Years After Implant

	1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	9 yr	10 yr	11 yr	12 yr	13 yr	14 yr	15 yr	at 189 mo
%	99.6	99.1	98.4	95.9	92.6	88.1	83.9	77.8	73.6	69.8	66.9	65.7	65.0	62.9	62.2	62.2
#	1,935	1,714	1,528	1,310	1,084	888	698	522	400	307	243	200	144	98	69	51
Effective Sample Size																

4023 CapSure SP

Product Characteristics


US Market Release	Aug-91	Serial Number Prefix	LAK	<u>US Returned Product Analysis</u>	
Estimated US Implants	43,700	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	47
Estimated US Active	14,200	Polarity	Unipolar	Electrical Malfunction	19
Advisories	None	Steroid	Yes	Other	6

Ventricular Placement

System Longevity Study Results

Qualifying Complications 20 Total

Number of Leads Enrolled in Study	1,158	Extra Cardiac Stimulation	1	Insulation (not further defined)	1
Cumulative Months of Follow-Up	62,408	Failure to Capture	15	Lead Dislodgement	2
Number of Leads Active in Study	398	Impedance Out of Range	1		

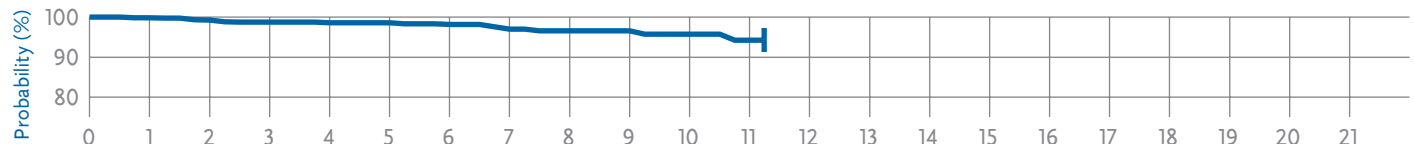

Years After Implant

	1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	9 yr	10 yr	11 yr	at 135 mo
%	99.9	99.3	98.8	98.6	98.6	98.2	97.0	96.6	96.6	95.8	94.3	94.3
#	886	765	682	604	519	391	270	187	123	71	59	51
Effective Sample Size												

4024 CapSure SP

Product Characteristics


US Market Release	Oct-91	Serial Number Prefix	LAJ	<u>US Returned Product Analysis</u>	
Estimated US Implants	229,200	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	264
Estimated US Active	80,700	Polarity	Bipolar	Electrical Malfunction	106
Advisories	None	Steroid	Yes	Other	34

Ventricular Placement

System Longevity Study Results

Qualifying Complications 3 Total

Number of Leads Enrolled in Study	1,215	Failure to Capture	3
Cumulative Months of Follow-Up	51,600		
Number of Leads Active in Study	28		

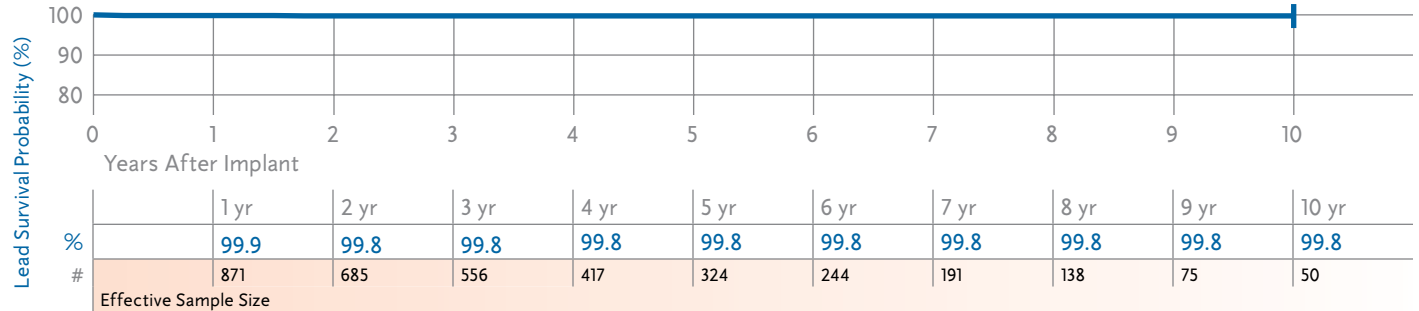

4033 CapSure Z

Product Characteristics


US Market Release	not US released	Serial Number Prefix	LCA	<u>US Returned Product Analysis</u>	
Estimated US Implants	n/a	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	2
Estimated US Active	n/a	Polarity	Unipolar	Electrical Malfunction	0
Advisories	None	Steroid	Yes	Other	0

Ventricular Placement

System Longevity Study Results

Qualifying Complications 11 Total

Number of Leads Enrolled in Study	541	Conductor Fracture	1
Cumulative Months of Follow-Up	28,347	Failure to Capture	8
Number of Leads Active in Study	49	Impedance Out of Range	2

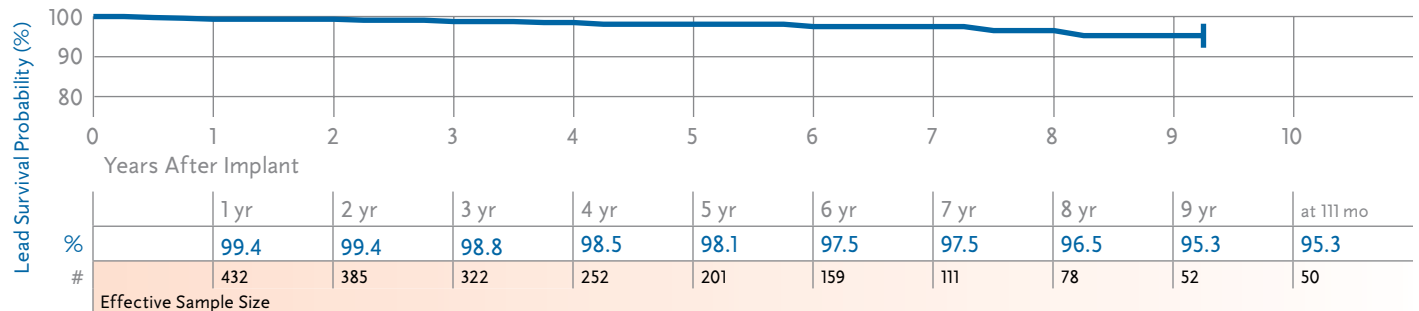

4057, 4057M Screw-In

Product Characteristics


US Market Release	Aug-88	Serial Number Prefix	XQ or LAN	<u>US Returned Product Analysis</u>	
Estimated US Implants	12,100	Type and/or Fixation	Transvenous, V or A, Screw-in	Implant Damage	39
Estimated US Active	2,600	Polarity	Unipolar	Electrical Malfunction	6
Advisories	None	Steroid	No	Other	4

Ventricular Placement

System Longevity Study Results

Qualifying Complications 7 Total

Number of Leads Enrolled in Study	259	Conductor Fracture	2	Failure to Sense	1
Cumulative Months of Follow-Up	15,266	Extra Cardiac Stimulation	2		
Number of Leads Active in Study	13	Failure to Capture	2		

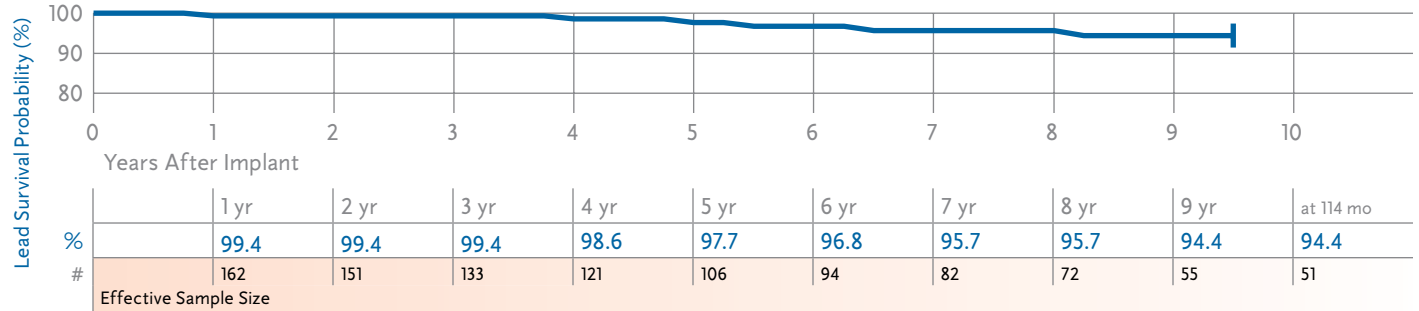

Pacing Leads continued

4058, 4058M Screw-In

Product Characteristics


US Market Release	Jan-89	Serial Number Prefix	ZY or LAW	<u>US Returned Product Analysis</u>	
Estimated US Implants	111,100	Type and/or Fixation	Transvenous, V or A, Screw-in	Implant Damage	388
Estimated US Active	24,600	Polarity	Bipolar	Electrical Malfunction	228
Advisories	None	Steroid	No	Other	23

Atrial Placement

System Longevity Study Results

Qualifying Complications 32 Total

Number of Leads Enrolled in Study	2,364	Extra Cardiac Stimulation	1	Insulation (not further defined)	1
Cumulative Months of Follow-Up	130,879	Failure to Capture	15	Lead Dislodgement	3
Number of Leads Active in Study	58	Failure to Sense	7	Oversensing	1
		Impedance Out of Range	4		

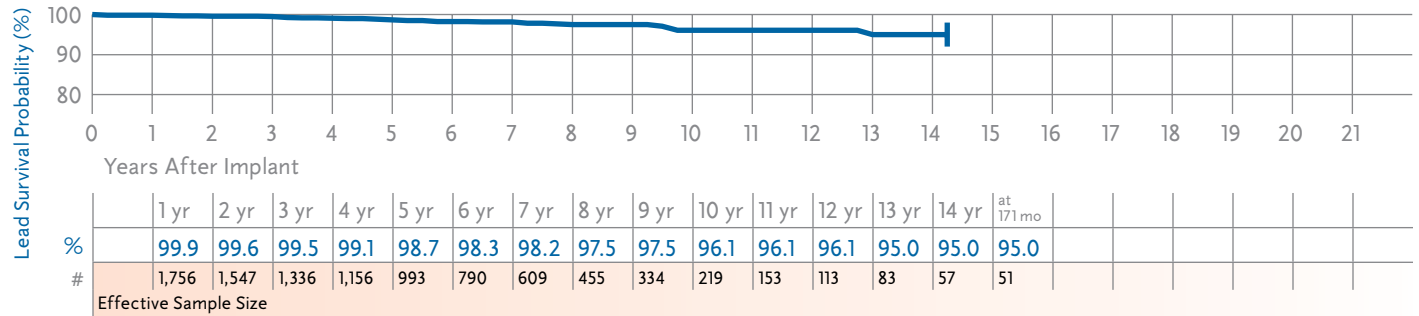


Ventricular Placement

System Longevity Study Results

Qualifying Complications 53 Total

Number of Leads Enrolled in Study	1,690	Conductor Fracture	5	Impedance Out of Range	7
Cumulative Months of Follow-Up	76,863	Extra Cardiac Stimulation	3	Insulation (not further defined)	4
Number of Leads Active in Study	59	Failure to Capture	22	Lead Dislodgement	1
		Failure to Sense	10	Oversensing	1

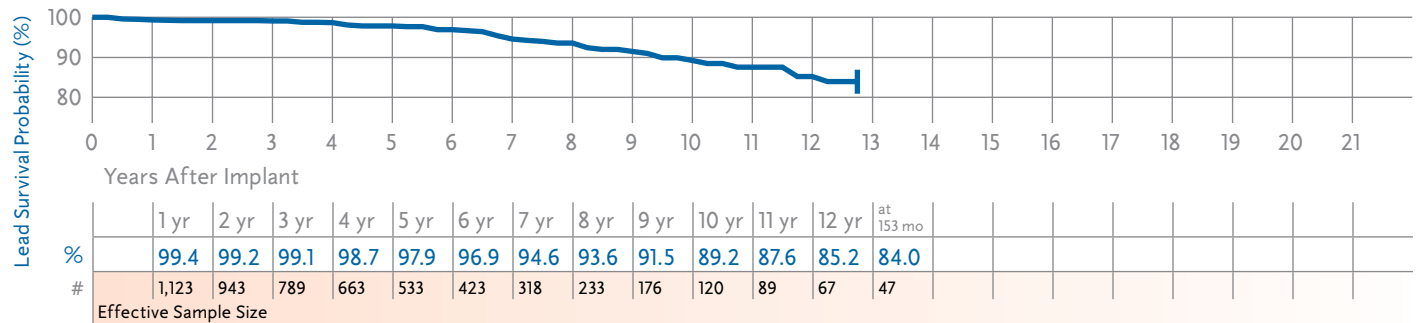

Leads

Pacing Leads continued

4067 CapSureFix

Product Characteristics


US Market Release	Jan-97	Serial Number Prefix	LCV	<u>US Returned Product Analysis</u>	
Estimated US Implants	1,300	Type and/or Fixation	Transvenous, V or A, Screw-in	Implant Damage	3
Estimated US Active	500	Polarity	Unipolar	Electrical Malfunction	1
Advisories	None	Steroid	Yes	Other	1

Atrial Placement

System Longevity Study Results

Qualifying Complications 6 Total

Number of Leads Enrolled in Study	108	Failure to Capture	5
Cumulative Months of Follow-Up	6,054	Oversensing	1
Number of Leads Active in Study	42		

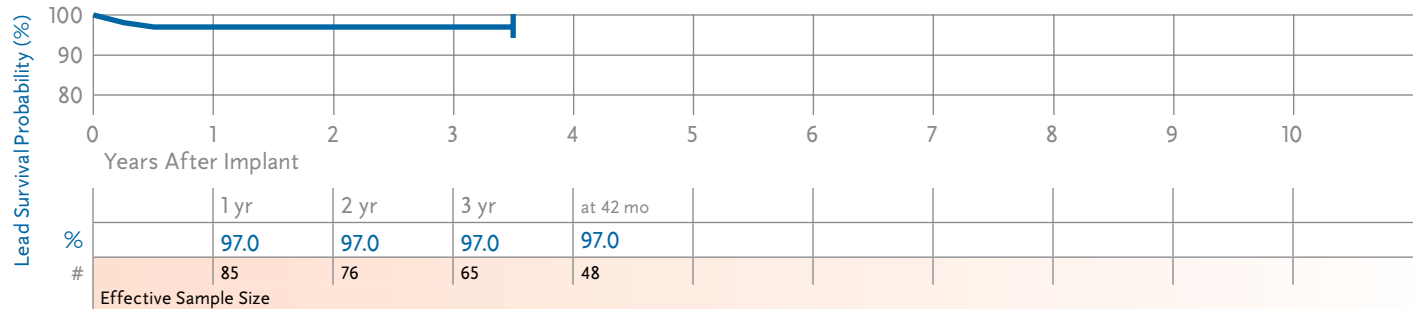

4068 CapSureFix

Product Characteristics

US Market Release	Mar-96	Serial Number Prefix	LCE	<u>US Returned Product Analysis</u>	
Estimated US Implants	131,700	Type and/or Fixation	Transvenous, V or A, Screw-in	Implant Damage	406
Estimated US Active	54,700	Polarity	Bipolar	Electrical Malfunction	83
Advisories	None	Steroid	Yes	Other	11


Atrial Placement

System Longevity Study Results

Number of Leads Enrolled in Study	2,401
Cumulative Months of Follow-Up	117,635
Number of Leads Active in Study	631

Qualifying Complications 55 Total

Conductor Fracture	1	Insulation (ESC)	2
Extra Cardiac Stimulation	1	Lead Dislodgement	8
Failure to Capture	19	Oversensing	8
Failure to Sense	11	Unspecified Clinical Failure	1
Impedance Out of Range	4		

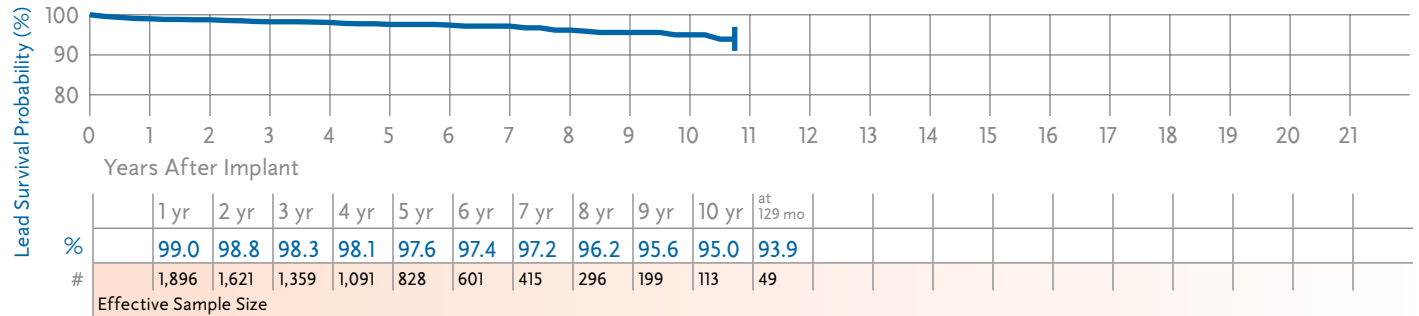


Ventricular Placement

System Longevity Study Results

Number of Leads Enrolled in Study	1,799
Cumulative Months of Follow-Up	84,282
Number of Leads Active in Study	527

Qualifying Complications 33 Total

Conductor Fracture	2	Failure to Sense	3
Extra Cardiac Stimulation	2	Impedance Out of Range	4
Failure to Capture	19	Oversensing	3

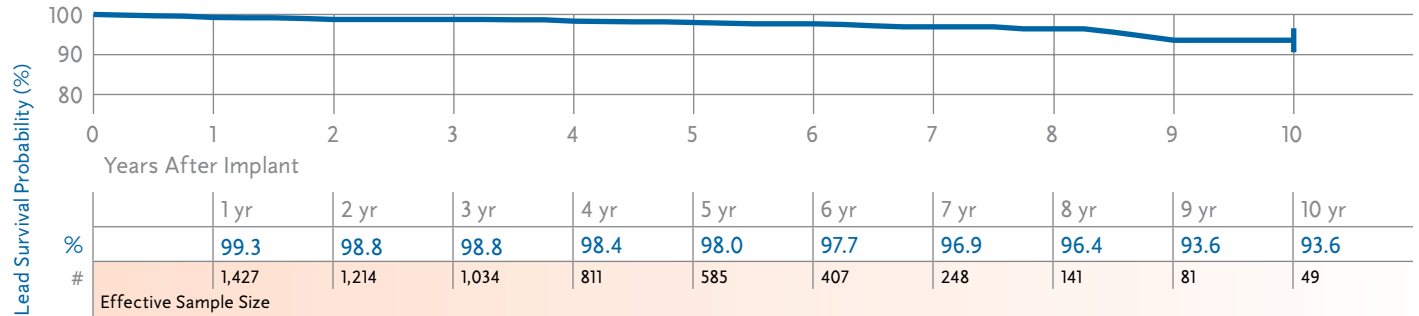

4073 CapSure Sense

Product Characteristics


US Market Release	Jun-02	Serial Number Prefix	BBF	<u>US Returned Product Analysis</u>	
Estimated US Implants	500	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	1
Estimated US Active	400	Polarity	Unipolar	Electrical Malfunction	0
Advisories	None	Steroid	Yes	Other	0

Atrial Placement

System Longevity Study Results

Qualifying Complications 0 Total

Number of Leads Enrolled in Study	1
Cumulative Months of Follow-Up	40
Number of Leads Active in Study	1

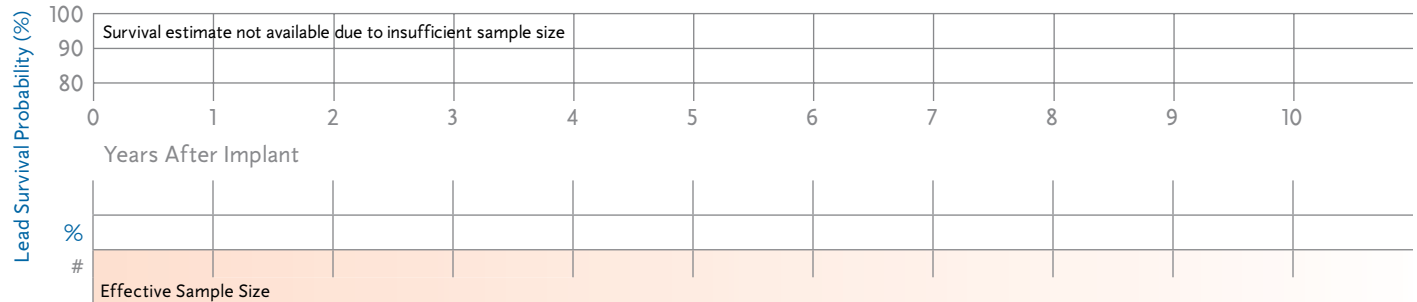


Ventricular Placement

System Longevity Study Results

Qualifying Complications 0 Total

Number of Leads Enrolled in Study	100
Cumulative Months of Follow-Up	3,775
Number of Leads Active in Study	85

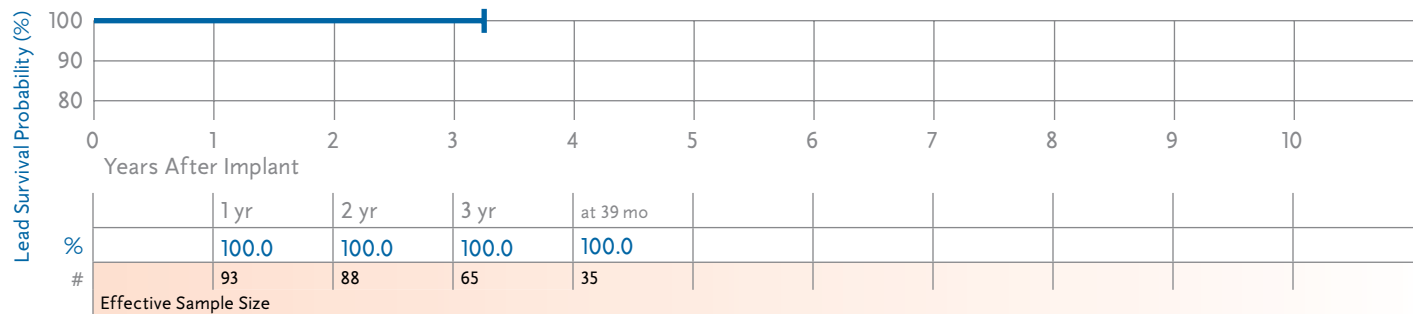

4074 CapSure Sense

Product Characteristics


US Market Release	Jun-02	Serial Number Prefix	BBD	<u>US Returned Product Analysis</u>	
Estimated US Implants	53,400	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	12
Estimated US Active	41,500	Polarity	Bipolar	Electrical Malfunction	3
Advisories	None	Steroid	Yes	Other	1

Ventricular Placement

System Longevity Study Results

Qualifying Complications 6 Total

Number of Leads Enrolled in Study	614	Failure to Capture	1	Lead Dislodgement	2
Cumulative Months of Follow-Up	18,331	Failure to Sense	1		
Number of Leads Active in Study	529	Impedance Out of Range	2		

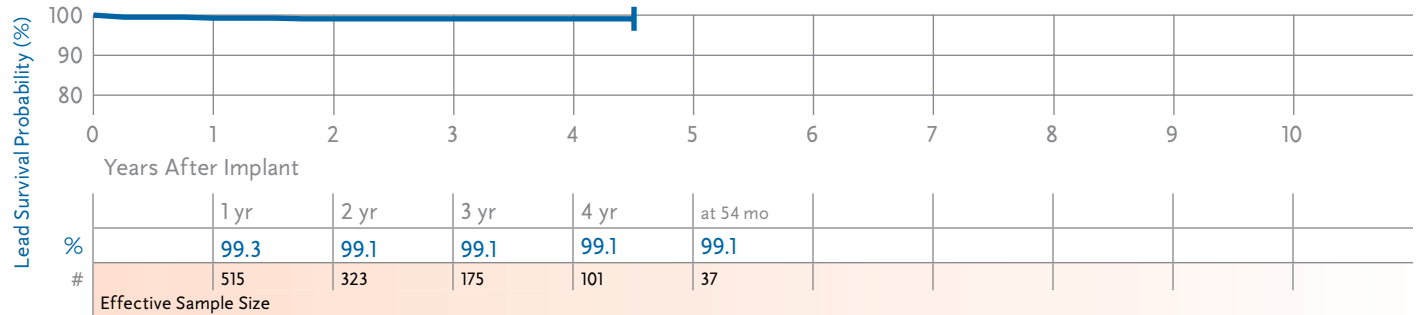

Pacing Leads continued

4076 CapSureFix Novus

Product Characteristics


US Market Release	Feb-04	Serial Number Prefix	BBL	<u>US Returned Product Analysis</u>	
Estimated US Implants	144,400	Type and/or Fixation	Transvenous, V or A, Screw-in	Implant Damage	53
Estimated US Active	122,500	Polarity	Bipolar	Electrical Malfunction	3
Advisories	None	Steroid	Yes	Other	6

Atrial Placement

System Longevity Study Results

Qualifying Complications 2 Total

Number of Leads Enrolled in Study	563	Failure to Capture	1
Cumulative Months of Follow-Up	10,581	Lead Dislodgement	1
Number of Leads Active in Study	495		

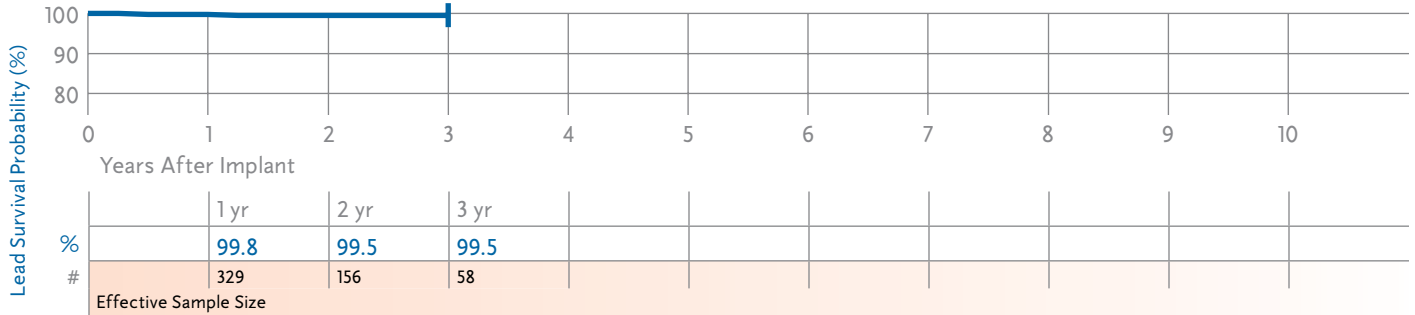


Ventricular Placement

System Longevity Study Results

Qualifying Complications 2 Total

Number of Leads Enrolled in Study	545	Failure to Capture	2
Cumulative Months of Follow-Up	1,633		
Number of Leads Active in Study	480		

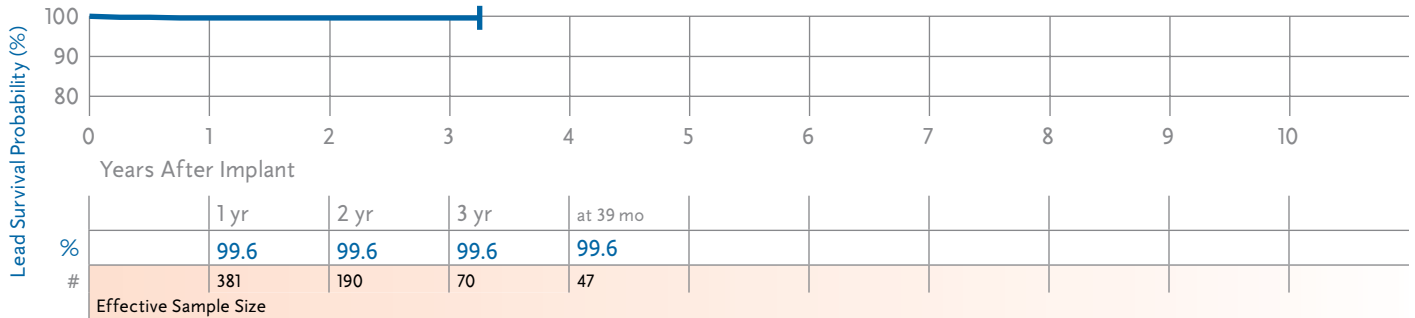

4081 Target Tip

Product Characteristics


US Market Release	Jul-89	Serial Number Prefix	LAC	<u>US Returned Product Analysis</u>	
Estimated US Implants	4,100	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	4
Estimated US Active	900	Polarity	Unipolar	Electrical Malfunction	5
Advisories	None	Steroid	No	Other	0

Ventricular Placement

System Longevity Study Results

Qualifying Complications 3 Total

Number of Leads Enrolled in Study	260	Conductor Fracture	1
Cumulative Months of Follow-Up	9,861	Failure to Sense	2
Number of Leads Active in Study	12		

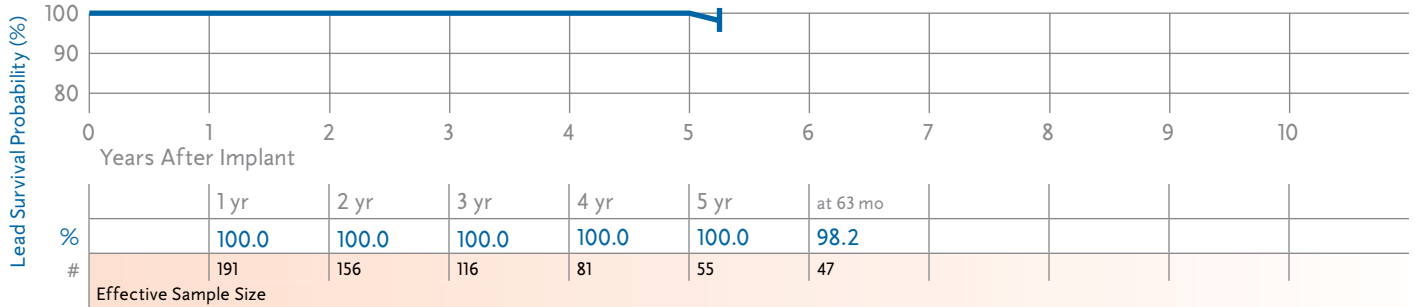

4092 CapSure SP Novus

Product Characteristics


US Market Release	Sep-98	Serial Number Prefix	LEP	<u>US Returned Product Analysis</u>	
Estimated US Implants	144,600	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	35
Estimated US Active	90,400	Polarity	Bipolar	Electrical Malfunction	12
Advisories	None	Steroid	Yes	Other	5

Ventricular Placement

System Longevity Study Results

Qualifying Complications 17 Total

Number of Leads Enrolled in Study	1,144	Conductor Fracture	3	Impedance Out of Range	1
Cumulative Months of Follow-Up	49,981	Extra Cardiac Stimulation	1	Lead Dislodgement	4
Number of Leads Active in Study	597	Failure to Capture	8		

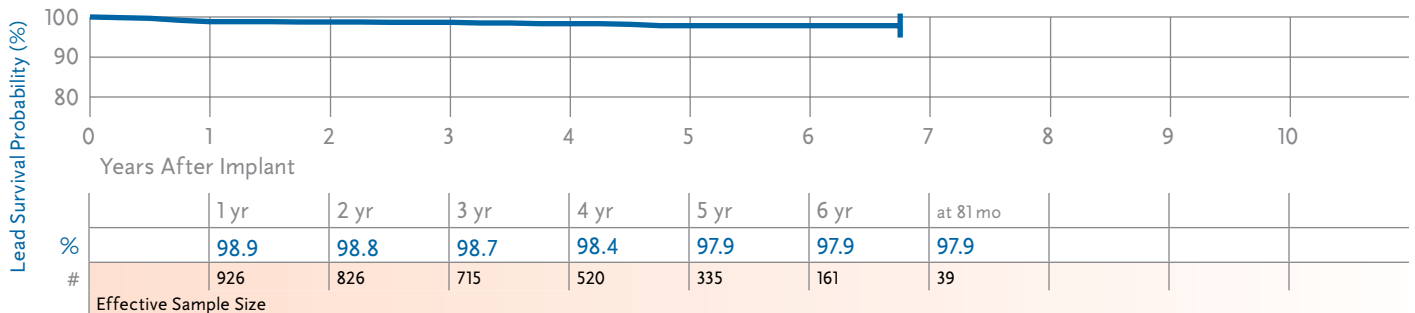

Pacing Leads continued

4503, 4503M CapSure

Product Characteristics


US Market Release	Jul-86	Serial Number Prefix	MQ, LAY	<u>US Returned Product Analysis</u>	
Estimated US Implants	9,000	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	2
Estimated US Active	1,300	Polarity	Unipolar	Electrical Malfunction	11
Advisories	None	Steroid	Yes	Other	0

Atrial Placement

System Longevity Study Results

Qualifying Complications 1 Total

Number of Leads Enrolled in Study	59	Failure to Sense	1
Cumulative Months of Follow-Up	3,206		
Number of Leads Active in Study	6		

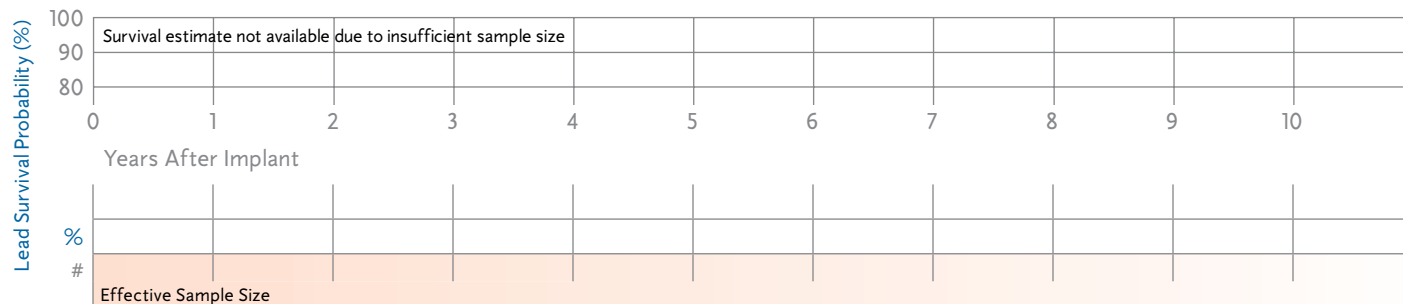

4504, 4504M CapSure

Product Characteristics


US Market Release	Mar-90	Serial Number Prefix	QM or LBA	<u>US Returned Product Analysis</u>	
Estimated US Implants	16,600	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	5
Estimated US Active	1,500	Polarity	Bipolar	Electrical Malfunction	171
Advisories	1	Steroid	Yes	Other	4
see page 149 – 1996 Lead Survival Below Expectations					

Atrial Placement

System Longevity Study Results

Qualifying Complications 48 Total

Number of Leads Enrolled in Study	368	Electrical Abandonment	3	Impedance Out of Range	9
Cumulative Months of Follow-Up	19,867	Extra Cardiac Stimulation	1	Insulation (MIO)	1
Number of Leads Active in Study	1	Failure to Capture	14	Lead Dislodgement	1
		Failure to Sense	16	Oversensing	3

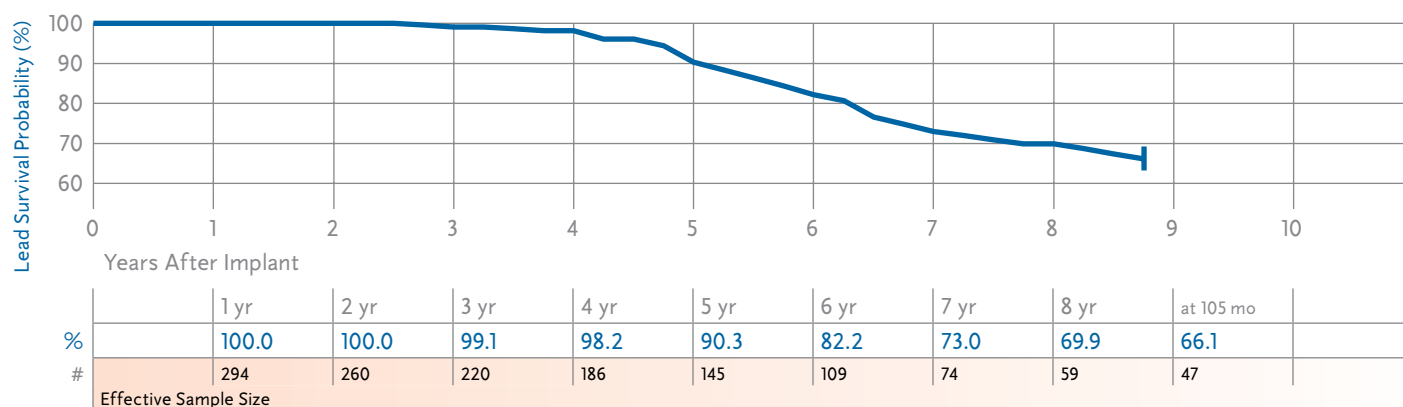

Pacing Leads continued

4512 Target Tip

Product Characteristics


US Market Release	Jul-83	Serial Number Prefix	PF	<u>US Returned Product Analysis</u>	
Estimated US Implants	11,600	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	4
Estimated US Active	1,000	Polarity	Bipolar	Electrical Malfunction	83
Advisories	None	Steroid	No	Other	8

Atrial Placement

System Longevity Study Results

Qualifying Complications 35 Total

Number of Leads Enrolled in Study	600	Electrical Abandonment	1	Insulation (MIO)	4
Cumulative Months of Follow-Up	39,765	Failure to Capture	6	Insulation (not further defined)	2
Number of Leads Active in Study	6	Failure to Sense	14	Lead Dislodgement	1
		Impedance Out of Range	3	Oversensing	2
		Insulation (ESC)	2		

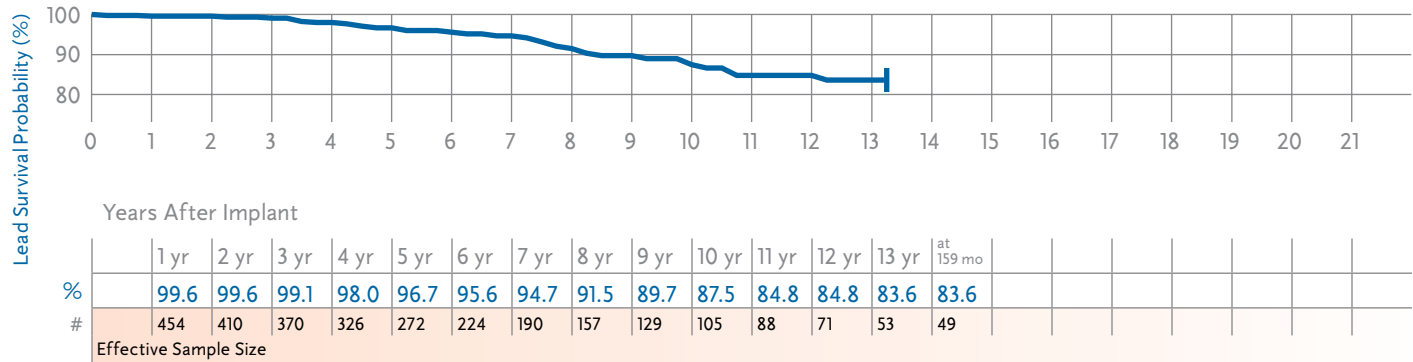

Leads

4523 CapSure SP

Product Characteristics


US Market Release	Aug-91	Serial Number Prefix	ZE	<u>US Returned Product Analysis</u>	
Estimated US Implants	12,000	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	5
Estimated US Active	3,300	Polarity	Unipolar	Electrical Malfunction	2
Advisories	None	Steroid	Yes	Other	1

Atrial Placement

System Longevity Study Results

Qualifying Complications 4 Total

Number of Leads Enrolled in Study	121	Impedance Out of Range	1
Cumulative Months of Follow-Up	7,060	Lead Dislodgement	2
Number of Leads Active in Study	19	Oversensing	1

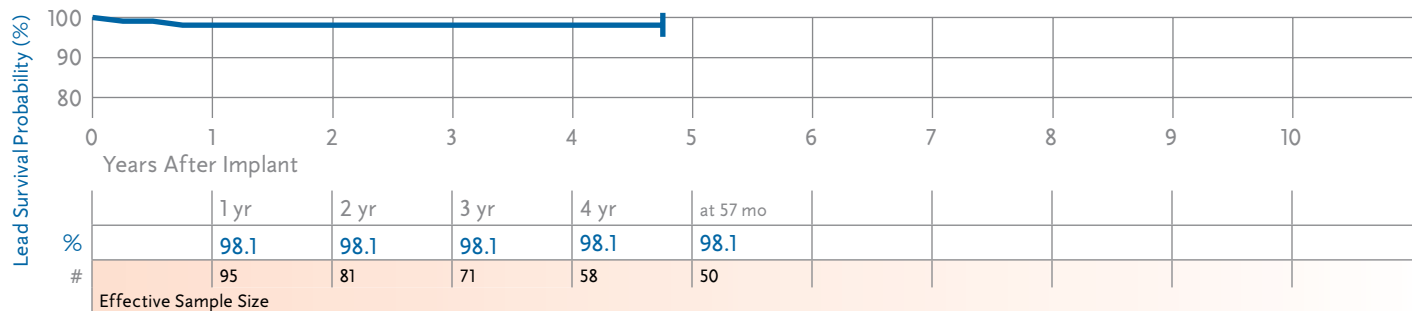

Pacing Leads continued

4524 CapSure SP

Product Characteristics


US Market Release	Oct-91	Serial Number Prefix	LAR	<u>US Returned Product Analysis</u>	
Estimated US Implants	106,900	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	47
Estimated US Active	36,300	Polarity	Bipolar	Electrical Malfunction	23
Advisories	None	Steroid	Yes	Other	8

Atrial Placement

System Longevity Study Results

Qualifying Complications 6 Total

Number of Leads Enrolled in Study	910	Failure to Capture	3
Cumulative Months of Follow-Up	39,326	Failure to Sense	2
Number of Leads Active in Study	59	Lead Dislodgement	1

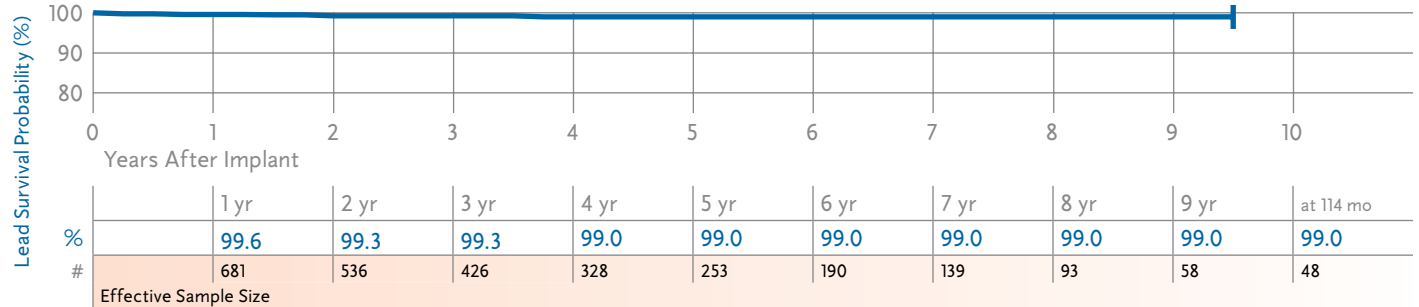

4533 CapSure Z

Product Characteristics


US Market Release	not US released	Serial Number Prefix	LCB	<u>US Returned Product Analysis</u>	
Estimated US Implants	n/a	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	0
Estimated US Active	n/a	Polarity	Unipolar	Electrical Malfunction	0
Advisories	None	Steroid	Yes	Other	0

Atrial Placement

System Longevity Study Results

Qualifying Complications 4 Total

Number of Leads Enrolled in Study	206	Failure to Capture	1	Oversensing	1
Cumulative Months of Follow-Up	11,153	Failure to Sense	1		
Number of Leads Active in Study	19	Lead Dislodgement	1		

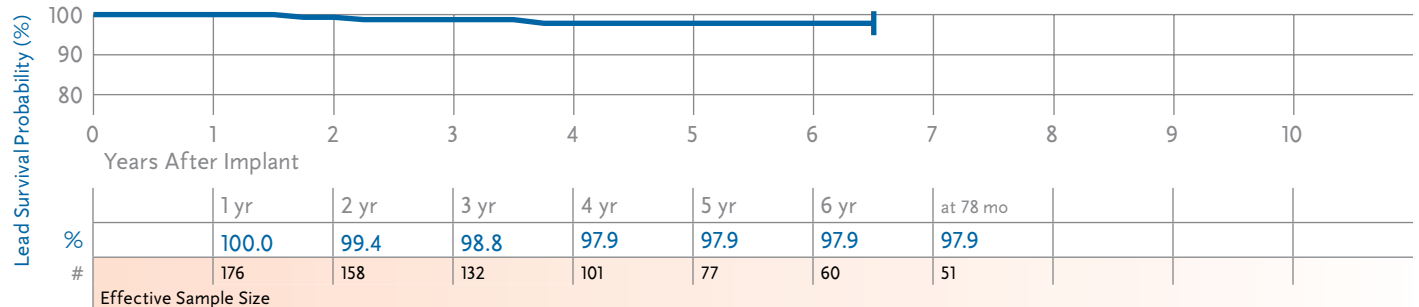

Pacing Leads continued

4557, 4557M Screw-In

Product Characteristics

US Market Release	Aug-88	Serial Number Prefix	VQ or LAM	<u>US Returned Product Analysis</u>	
Estimated US Implants	22,500	Type and/or Fixation	Transvenous, Atrial-J, Screw-in	Implant Damage	53
Estimated US Active	4,900	Polarity	Unipolar	Electrical Malfunction	14
Advisories	None	Steroid	No	Other	4


Atrial Placement

System Longevity Study Results

Number of Leads Enrolled in Study	294
Cumulative Months of Follow-Up	18,357
Number of Leads Active in Study	15

Qualifying Complications

6	Total		
Extra Cardiac Stimulation	1	Oversensing	1
Failure to Capture	3		
Failure to Sense	1		

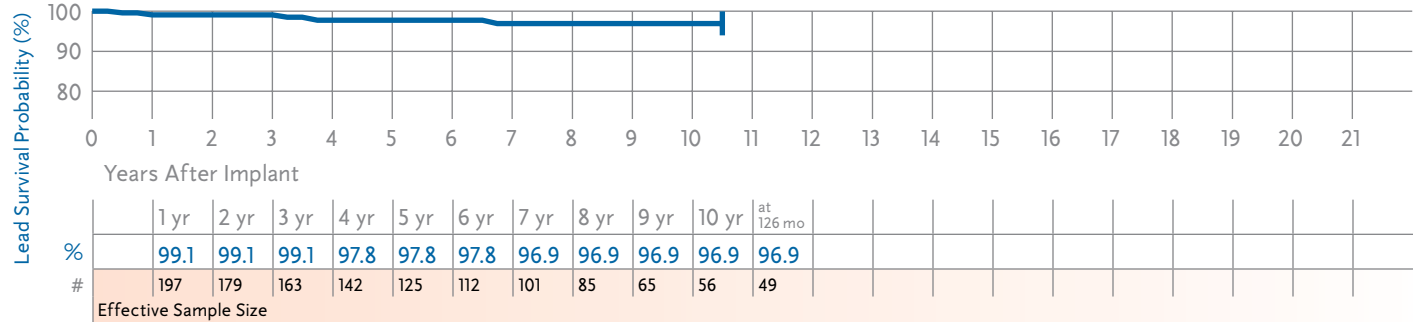

Leads

4558M Screw-In

Product Characteristics

US Market Release	Nov-94	Serial Number Prefix	LDC	<u>US Returned Product Analysis</u>	
Estimated US Implants	21,000	Type and/or Fixation	Transvenous, Atrial-J, Screw-in	Implant Damage	111
Estimated US Active	5,800	Polarity	Bipolar	Electrical Malfunction	11
Advisories	None	Steroid	No	Other	1


Atrial Placement

System Longevity Study Results

Number of Leads Enrolled in Study	539
Cumulative Months of Follow-Up	22,131
Number of Leads Active in Study	28

Qualifying Complications

11	Total		
Electrical Abandonment	1	Impedance Out of Range	2
Failure to Capture	3	Insulation (not further defined)	1
Failure to Sense	2	Oversensing	2

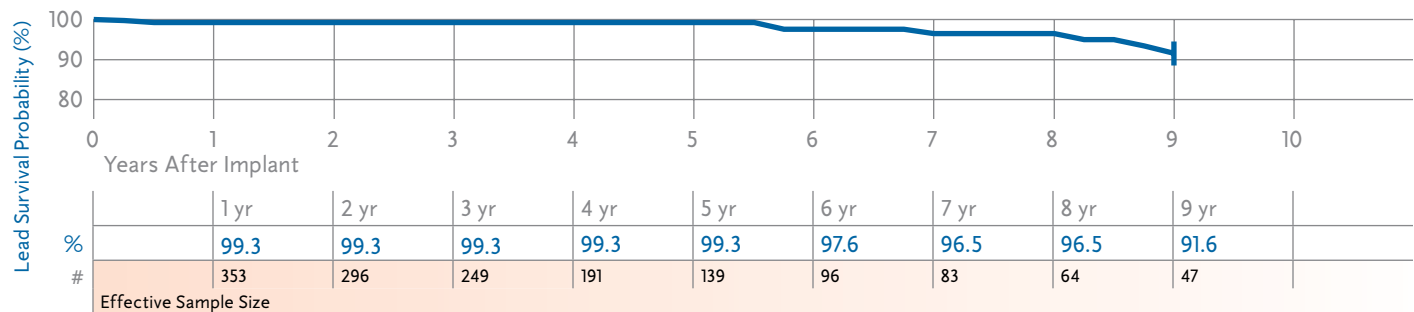

Pacing Leads continued

4568 CapSureFix

Product Characteristics


US Market Release	Jan-97	Serial Number Prefix	LDD	<u>US Returned Product Analysis</u>	
Estimated US Implants	72,800	Type and/or Fixation	Transvenous, Atrial-J, Screw-in	Implant Damage	197
Estimated US Active	35,800	Polarity	Bipolar	Electrical Malfunction	6
Advisories	None	Steroid	Yes	Other	4

Atrial Placement

System Longevity Study Results

Qualifying Complications 30 Total

Number of Leads Enrolled in Study	576	Failure to Capture	19	Medical Judgment	1
Cumulative Months of Follow-Up	21,713	Failure to Sense	2		
Number of Leads Active in Study	223	Lead Dislodgement	8		

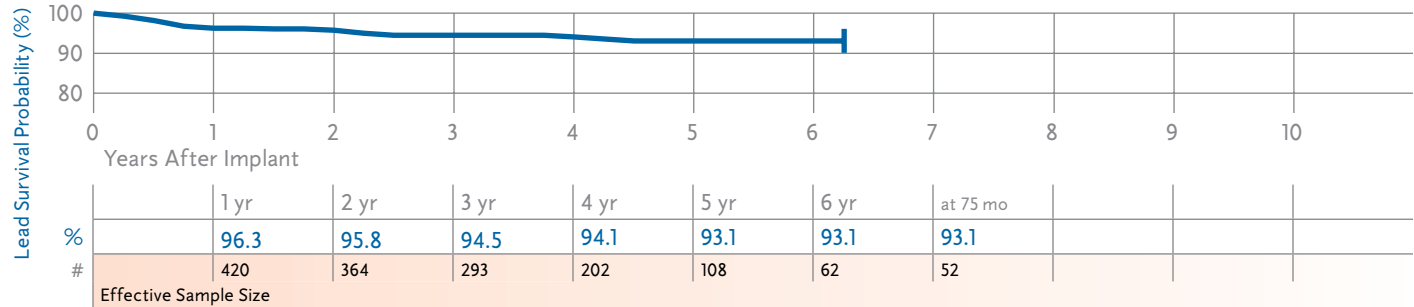

4574 CapSure Sense

Product Characteristics


US Market Release	Jun-02	Serial Number Prefix	BBE	<u>US Returned Product Analysis</u>	
Estimated US Implants	34,500	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	6
Estimated US Active	26,500	Polarity	Bipolar	Electrical Malfunction	2
Advisories	None	Steroid	Yes	Other	0

Atrial Placement

System Longevity Study Results

Qualifying Complications 0 Total

Number of Leads Enrolled in Study	6
Cumulative Months of Follow-Up	145
Number of Leads Active in Study	4

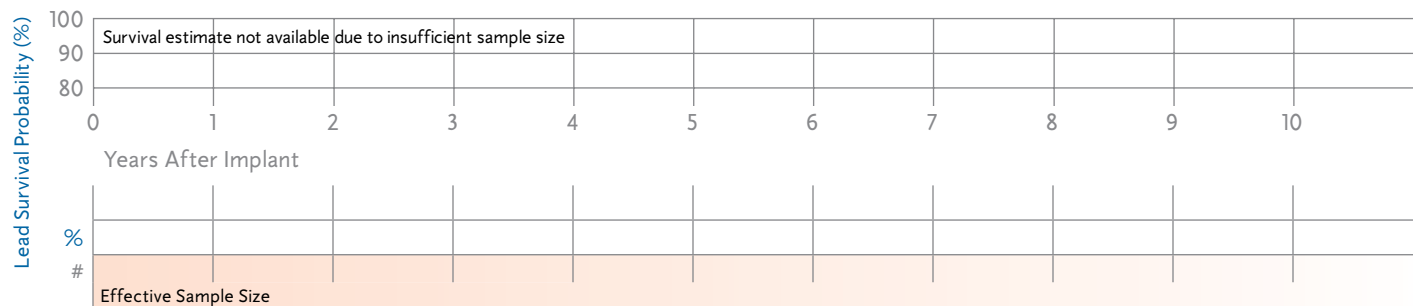

Pacing Leads continued

4592 CapSure SP Novus

Product Characteristics


US Market Release	Oct-98	Serial Number Prefix	LER	<u>US Returned Product Analysis</u>	
Estimated US Implants	73,000	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	12
Estimated US Active	44,400	Polarity	Bipolar	Electrical Malfunction	3
Advisories	None	Steroid	Yes	Other	0

Atrial Placement

System Longevity Study Results

Qualifying Complications 5 Total

Number of Leads Enrolled in Study	244	Failure to Capture	2
Cumulative Months of Follow-Up	10,221	Failure to Sense	1
Number of Leads Active in Study	93	Lead Dislodgement	2

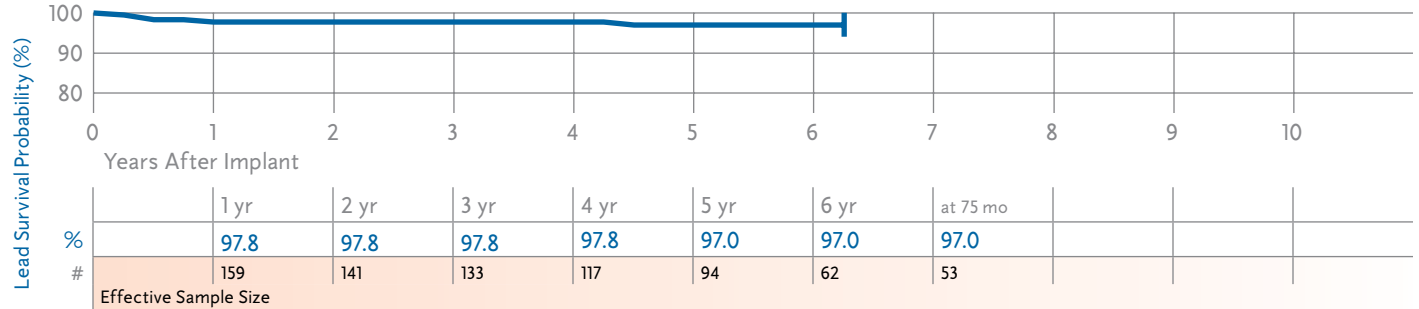

Leads

5023, 5023M CapSure SP

Product Characteristics


US Market Release	Nov-88	Serial Number Prefix	SX or LAS	<u>US Returned Product Analysis</u>	
Estimated US Implants	10,600	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	15
Estimated US Active	2,800	Polarity	Unipolar	Electrical Malfunction	7
Advisories	None	Steroid	Yes	Other	0

Ventricular Placement

System Longevity Study Results

Qualifying Complications 14 Total

Number of Leads Enrolled in Study	1,353	Conductor Fracture	1	Impedance Out of Range	1
Cumulative Months of Follow-Up	65,821	Extra Cardiac Stimulation	3		
Number of Leads Active in Study	550	Failure to Capture	9		

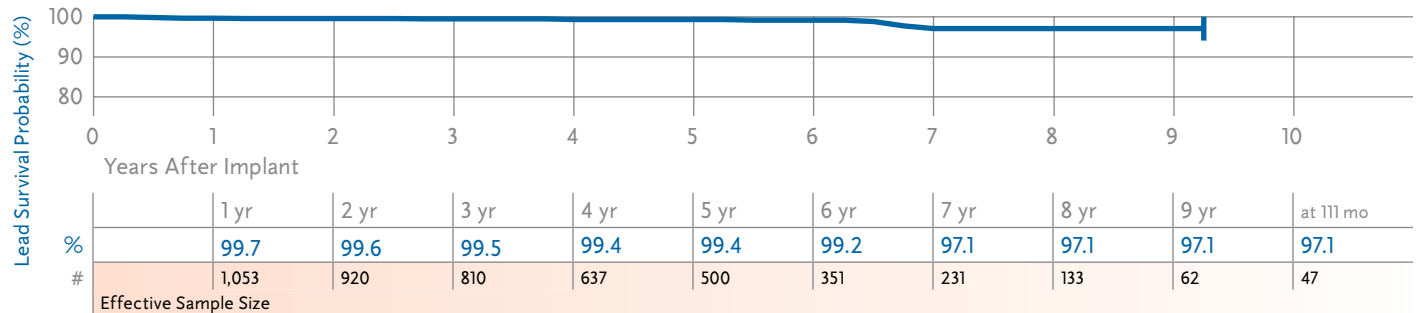

Pacing Leads continued

5024, 5024M CapSure SP

Product Characteristics

US Market Release	Mar-90	Serial Number Prefix	SY or LAT	<u>US Returned Product Analysis</u>	
Estimated US Implants	211,400	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	723
Estimated US Active	69,300	Polarity	Bipolar	Electrical Malfunction	106
Advisories	None	Steroid	Yes	Other	29


Ventricular Placement

System Longevity Study Results

Number of Leads Enrolled in Study	8,142
Cumulative Months of Follow-Up	425,081
Number of Leads Active in Study	711

Qualifying Complications

Conductor Fracture	3	Insulation (ESC)	1
Extra Cardiac Stimulation	2	Insulation (not further defined)	5
Failure to Capture	24	Lead Dislodgement	5
Failure to Sense	2	Oversensing	1
Impedance Out of Range	2		

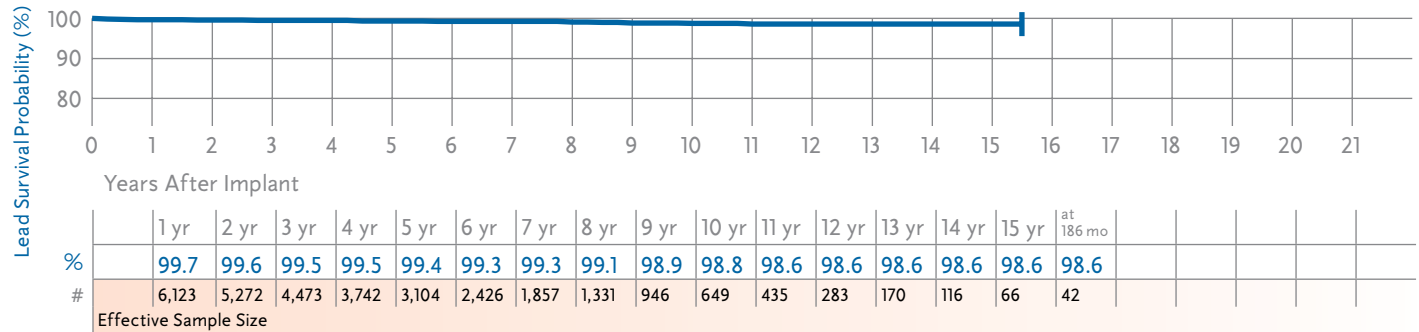

5026 CapSure

Product Characteristics

US Market Release	Feb-88	Serial Number Prefix	RZ	<u>US Returned Product Analysis</u>	
Estimated US Implants	7,800	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	60
Estimated US Active	1,200	Polarity	Bipolar	Electrical Malfunction	7
Advisories	None	Steroid	Yes	Other	1


Ventricular Placement

System Longevity Study Results

Number of Leads Enrolled in Study	168
Cumulative Months of Follow-Up	9,558
Number of Leads Active in Study	6

Qualifying Complications

Electrical Abandonment	1
Failure to Capture	3

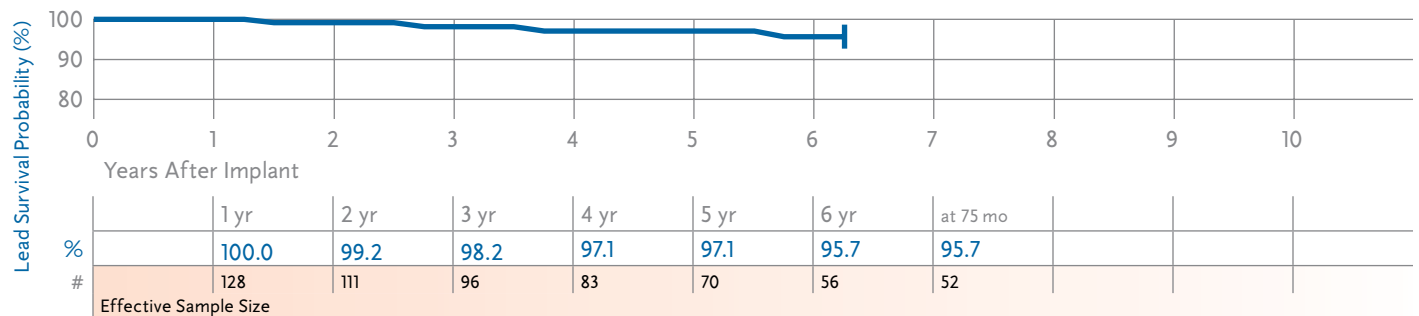

5033 CapSure Z

Product Characteristics


US Market Release	Feb-96	Serial Number Prefix	LDK	<u>US Returned Product Analysis</u>	
Estimated US Implants	2,500	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	6
Estimated US Active	1,000	Polarity	Unipolar	Electrical Malfunction	1
Advisories	None	Steroid	Yes	Other	3

Ventricular Placement

System Longevity Study Results

Qualifying Complications 24 Total

Number of Leads Enrolled in Study	1,901	Cardiac Perforation	1	Impedance Out of Range	4
Cumulative Months of Follow-Up	92,733	Conductor Fracture	5	Insulation (not further defined)	1
Number of Leads Active in Study	313	Failure to Capture	11	Lead Dislodgement	2

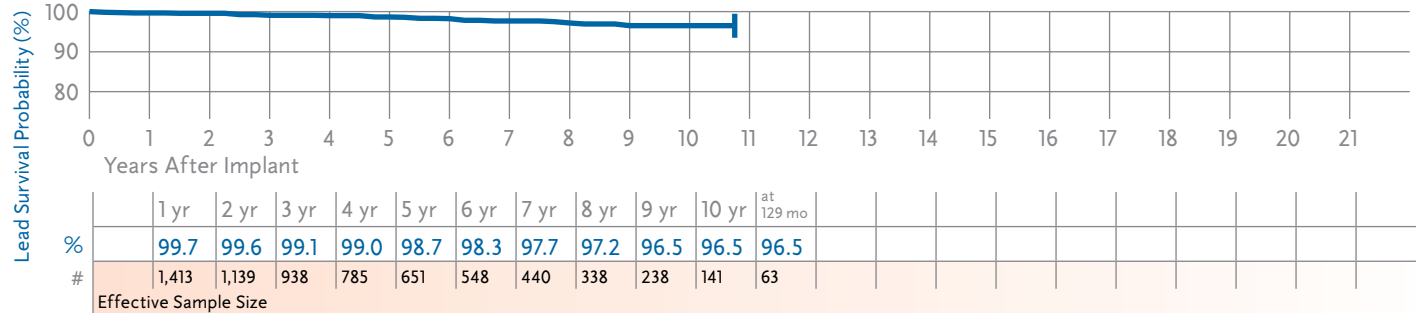

Leads

5034 CapSure Z

Product Characteristics


US Market Release	Feb-96	Serial Number Prefix	LDF	<u>US Returned Product Analysis</u>	
Estimated US Implants	58,700	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	85
Estimated US Active	21,900	Polarity	Bipolar	Electrical Malfunction	29
Advisories	None	Steroid	Yes	Other	11

Ventricular Placement

System Longevity Study Results

Qualifying Complications 13 Total

Number of Leads Enrolled in Study	1,594	Conductor Fracture	1	Impedance Out of Range	1
Cumulative Months of Follow-Up	80,368	Failure to Capture	9	Lead Dislodgement	1
Number of Leads Active in Study	292	Failure to Sense	1		

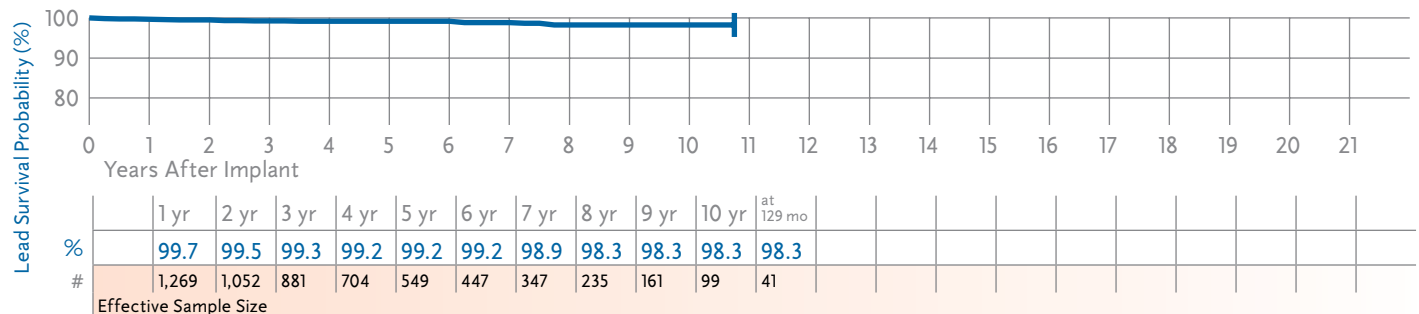

5054 CapSure Z Novus

Product Characteristics


US Market Release	Jun-98	Serial Number Prefix	LEH	<u>US Returned Product Analysis</u>	
Estimated US Implants	84,700	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	40
Estimated US Active	49,700	Polarity	Bipolar	Electrical Malfunction	13
Advisories	None	Steroid	Yes	Other	6

Ventricular Placement

System Longevity Study Results

Qualifying Complications

	n	Total		
Number of Leads Enrolled in Study	1,392		Failure to Capture	7
Cumulative Months of Follow-Up	57,156		Failure to Sense	1
Number of Leads Active in Study	534		Impedance Out of Range	1
			Lead Dislodgement	2

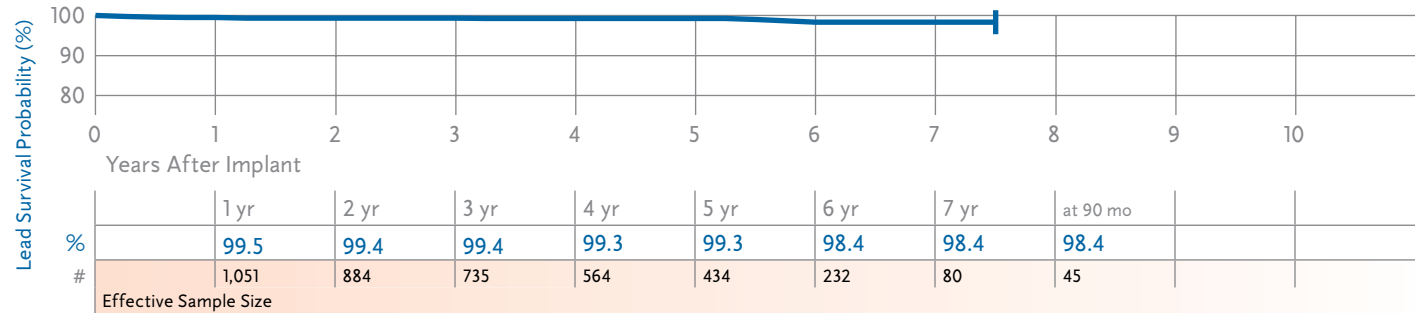

5068 CapSureFix

Product Characteristics


US Market Release		Serial Number Prefix	LDJ	US Returned Product Analysis		
Estimated US Implants	Jan-97	108,000	Type and/or Fixation	Transvenous, V or A, Screw-in	Implant Damage	455
Estimated US Active	49,800	Polarity	Bipolar	Electrical Malfunction	63	
Advisories	None	Steroid	Yes	Other	15	

Atrial Placement

System Longevity Study Results

Qualifying Complications 7 Total

Number of Leads Enrolled in Study	969	Failure to Capture	2	Oversensing	1
Cumulative Months of Follow-Up	32,166	Impedance Out of Range	3		
Number of Leads Active in Study	90	Lead Dislodgement	1		

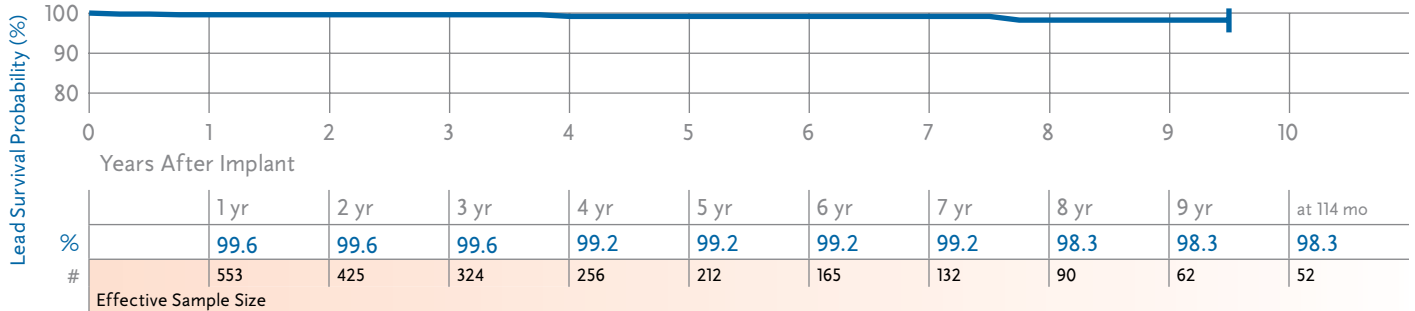


Ventricular Placement

System Longevity Study Results

Qualifying Complications 6 Total

Number of Leads Enrolled in Study	1,360	Conductor Fracture	1	Lead Dislodgement	1
Cumulative Months of Follow-Up	35,786	Failure to Capture	3		
Number of Leads Active in Study	164	Insulation (not further defined)	1		

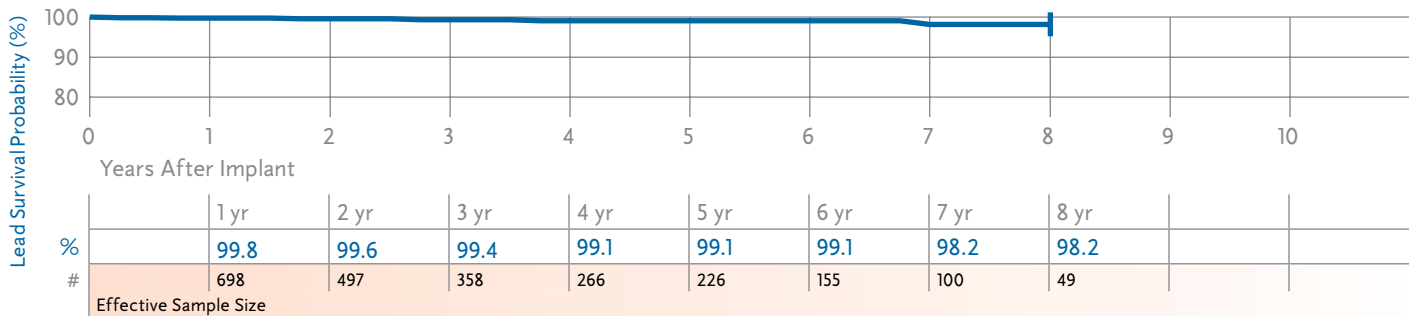

Pacing Leads continued

5072 SureFix

Product Characteristics


		Product Characteristics		US Returned Product Analysis	
US Market Release	Jun-98	Serial Number Prefix	LEM	Implant Damage	26
Estimated US Implants	9,100	Type and/or Fixation	Transvenous, V or A, Screw-in	Electrical Malfunction	4
Estimated US Active	5,000	Polarity	Bipolar	Other	1
Advisories	None	Steroid	Yes		

Atrial Placement

System Longevity Study Results

Qualifying Complications 2 Total

Number of Leads Enrolled in Study	451	Cardiac Perforation	1
Cumulative Months of Follow-Up	20,937	Failure to Capture	1
Number of Leads Active in Study	132		

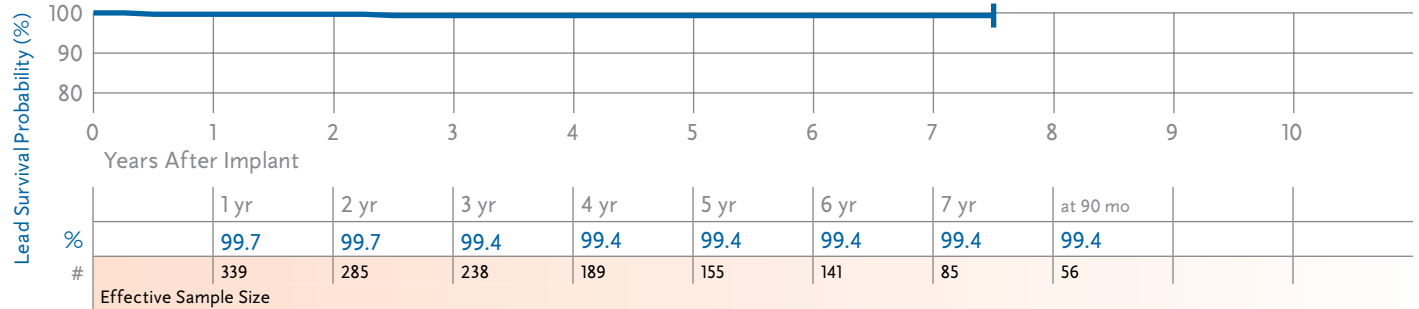

Pacing Leads continued

5076 CapSureFix Novus

Product Characteristics

US Market Release	Aug-00	Serial Number Prefix	PJN	<u>US Returned Product Analysis</u>	
Estimated US Implants	911,600	Type and/or Fixation	Transvenous, V or A, Screw-in	Implant Damage	705
Estimated US Active	665,100	Polarity	Bipolar	Electrical Malfunction	163
Advisories	None	Steroid	Yes	Other	51


Atrial Placement

System Longevity Study Results

Number of Leads Enrolled in Study	2,502
Cumulative Months of Follow-Up	81,429
Number of Leads Active in Study	1,226

Qualifying Complications 15 Total

Cardiac Perforation	1	Impedance Out of Range	1
Conductor Fracture	1	Insulation (not further defined)	1
Extra Cardiac Stimulation	2	Lead Dislodgement	4
Failure to Capture	4	Oversensing	1

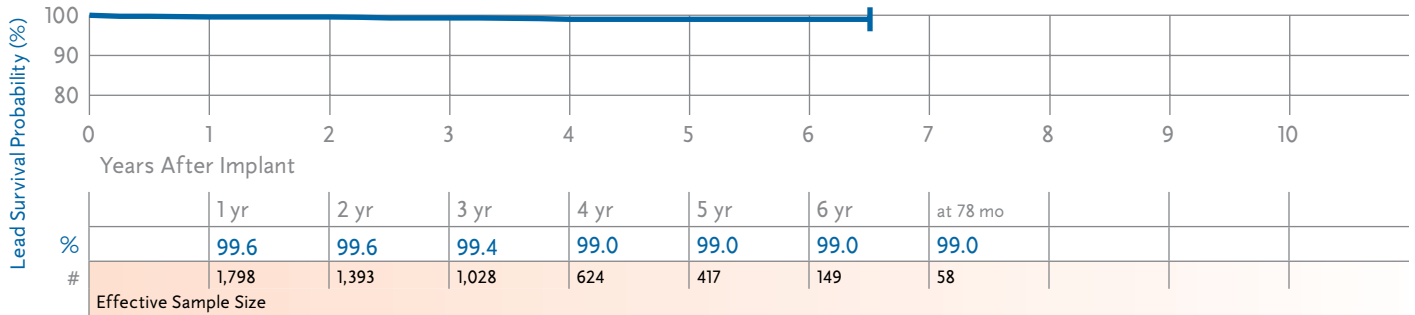


Ventricular Placement

System Longevity Study Results

Number of Leads Enrolled in Study	1,508
Cumulative Months of Follow-Up	48,187
Number of Leads Active in Study	660

Qualifying Complications 9 Total

Cardiac Perforation	1	Failure to Sense	1
Conductor Fracture	1	Impedance Out of Range	1
Failure to Capture	3	Lead Dislodgement	2

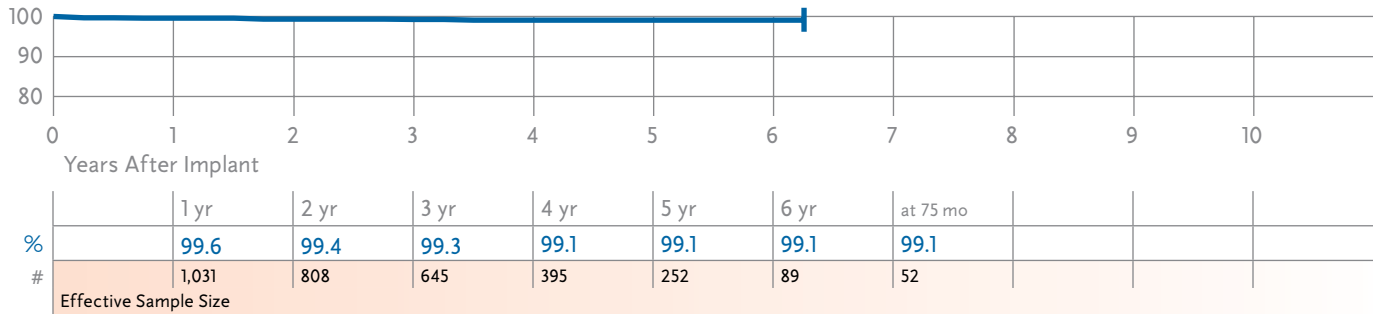

Leads

5092 CapSure SP Novus

Product Characteristics


US Market Release	Jun-98	Serial Number Prefix	LET	<u>US Returned Product Analysis</u>	
Estimated US Implants	109,800	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	47
Estimated US Active	68,900	Polarity	Bipolar	Electrical Malfunction	20
Advisories	None	Steroid	Yes	Other	11

Ventricular Placement

System Longevity Study Results

Qualifying Complications 8 Total

Number of Leads Enrolled in Study	1,171	Extra Cardiac Stimulation	1
Cumulative Months of Follow-Up	38,950	Failure to Capture	2
Number of Leads Active in Study	257	Lead Dislodgement	5

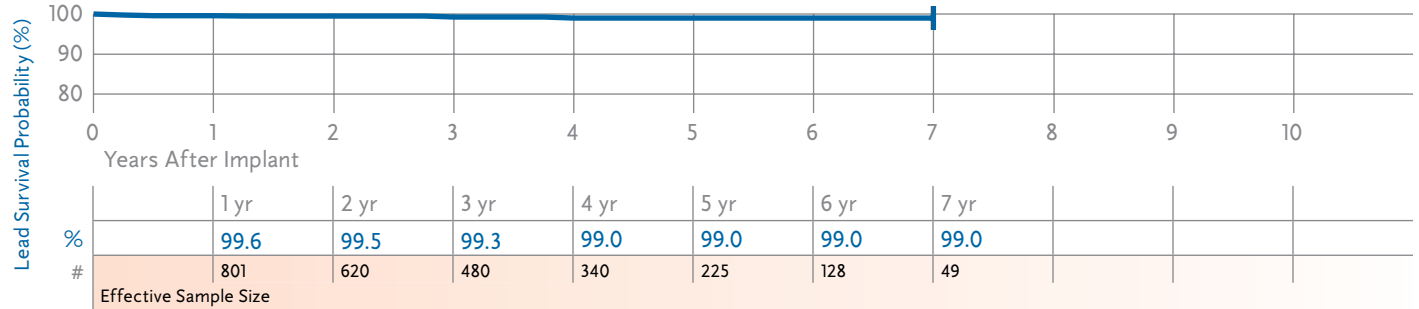

5524, 5524M CapSure SP

Product Characteristics


US Market Release	Mar-90	Serial Number Prefix	XV or LAV	<u>US Returned Product Analysis</u>	
Estimated US Implants	63,800	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	66
Estimated US Active	22,300	Polarity	Bipolar	Electrical Malfunction	21
Advisories	None	Steroid	Yes	Other	7

Atrial Placement

System Longevity Study Results

Qualifying Complications 38 Total

Number of Leads Enrolled in Study	4,440	Conductor Fracture	1	Insulation (not further defined)	2
Cumulative Months of Follow-Up	235,419	Failure to Capture	22	Lead Dislodgement	4
Number of Leads Active in Study	555	Failure to Sense	4	Oversensing	4
		Impedance Out of Range	1		

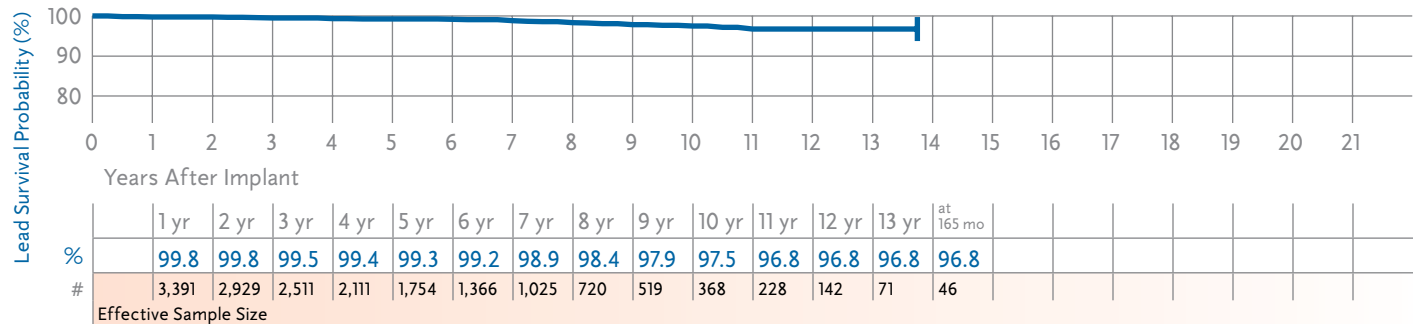

5534 CapSure Z

Product Characteristics

US Market Release	Feb-96	Serial Number Prefix	LDG	<u>US Returned Product Analysis</u>	
Estimated US Implants	27,700	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	29
Estimated US Active	8,700	Polarity	Bipolar	Electrical Malfunction	6
Advisories	None	Steroid	Yes	Other	5


Atrial Placement

System Longevity Study Results

Number of Leads Enrolled in Study	261
Cumulative Months of Follow-Up	12,544
Number of Leads Active in Study	25

Qualifying Complications

Failure to Capture	5
Impedance Out of Range	1

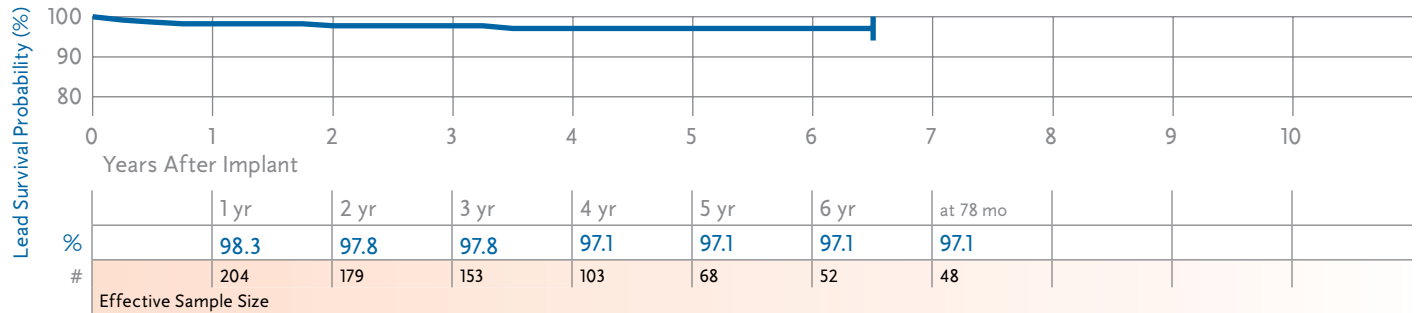

Leads

5554 CapSure Z Novus

Product Characteristics

US Market Release	Jun-98	Serial Number Prefix	LEJ	<u>US Returned Product Analysis</u>	
Estimated US Implants	54,600	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	7
Estimated US Active	32,300	Polarity	Bipolar	Electrical Malfunction	6
Advisories	None	Steroid	Yes	Other	4


Atrial Placement

System Longevity Study Results

Number of Leads Enrolled in Study	351
Cumulative Months of Follow-Up	16,841
Number of Leads Active in Study	64

Qualifying Complications

Failure to Capture	1	Oversensing	1
Impedance Out of Range	1		
Lead Dislodgement	1		

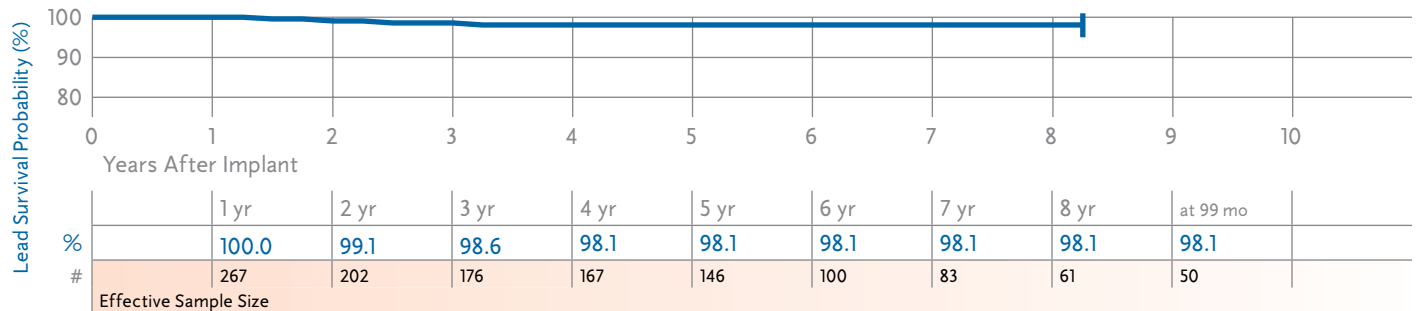

Pacing Leads continued

5568 CapSureFix

Product Characteristics

US Market Release	Jan-97	Serial Number Prefix	LDN	US Returned Product Analysis	
Estimated US Implants	66,500	Type and/or Fixation	Transvenous, Atrial-J, Screw-in	Implant Damage	228
Estimated US Active	44,700	Polarity	Bipolar	Electrical Malfunction	8
Advisories	None	Steroid	Yes	Other	9


Atrial Placement

System Longevity Study Results

Number of Leads Enrolled in Study	893
Cumulative Months of Follow-Up	26,406
Number of Leads Active in Study	187

Qualifying Complications

Failure to Capture	2
Failure to Sense	1
Lead Dislodgement	1
Total	4

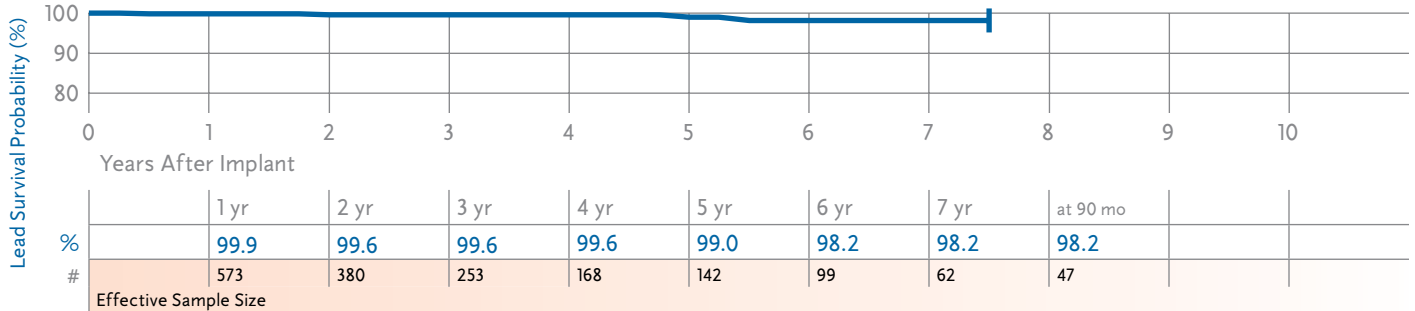

5592 CapSure SP Novus

Product Characteristics

US Market Release	Jun-98	Serial Number Prefix	LEU	US Returned Product Analysis	
Estimated US Implants	26,700	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	6
Estimated US Active	18,200	Polarity	Bipolar	Electrical Malfunction	3
Advisories	None	Steroid	Yes	Other	0


Atrial Placement

System Longevity Study Results

Number of Leads Enrolled in Study	666
Cumulative Months of Follow-Up	23,915
Number of Leads Active in Study	209

Qualifying Complications

Failure to Capture	2
Lead Dislodgement	2
Total	4

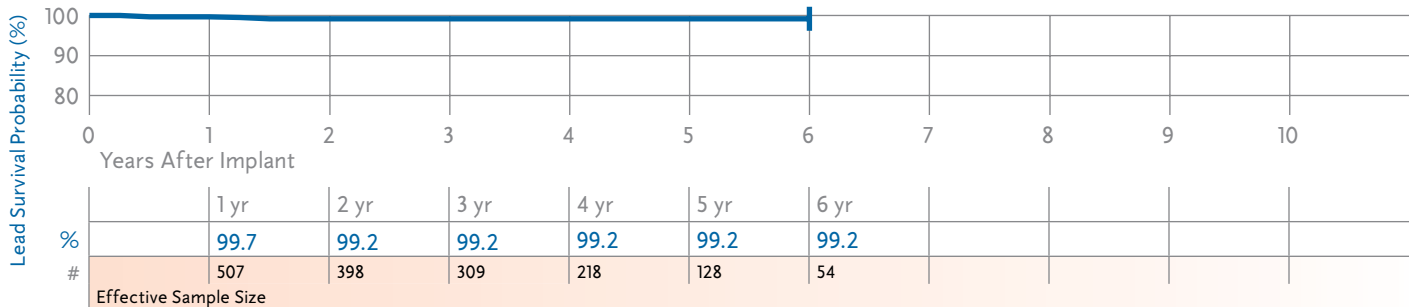

Pacing Leads continued

5594 CapSure SP Novus

Product Characteristics


US Market Release	Jun-01	Serial Number Prefix	LFD	<u>US Returned Product Analysis</u>	
Estimated US Implants	10,000	Type and/or Fixation	Transvenous, Atrial-J, Tines	Implant Damage	0
Estimated US Active	7,400	Polarity	Bipolar	Electrical Malfunction	1
Advisories	None	Steroid	Yes	Other	0

Atrial Placement

System Longevity Study Results

Qualifying Complications 0 Total

Number of Leads Enrolled in Study	17
Cumulative Months of Follow-Up	869
Number of Leads Active in Study	11

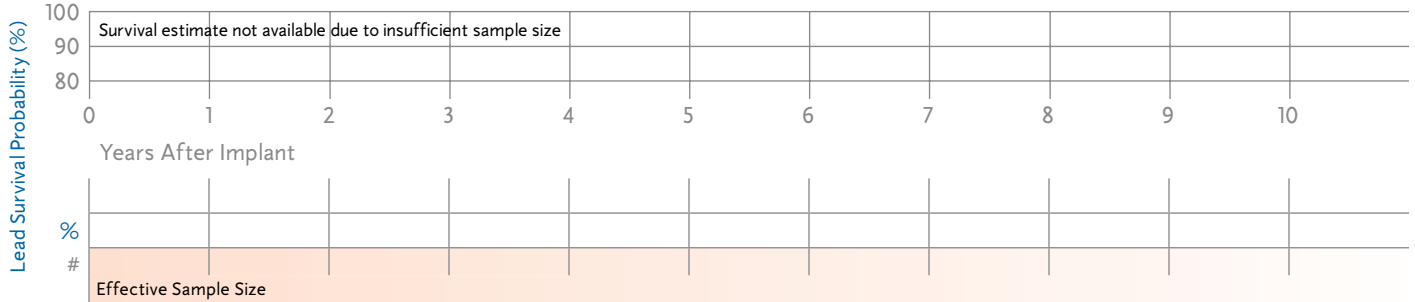

6940 CapSureFix

Product Characteristics


US Market Release	Oct-98	Serial Number Prefix	TCP	<u>US Returned Product Analysis</u>	
Estimated US Implants	26,600	Type and/or Fixation	Transvenous, A or V, Screw-in	Implant Damage	114
Estimated US Active	12,300	Polarity	Bipolar	Electrical Malfunction	19
Advisories	None	Steroid	Yes	Other	3

Atrial Placement

System Longevity Study Results

Qualifying Complications 7 Total

Number of Leads Enrolled in Study	818	Conductor Fracture	1	Oversensing	3
Cumulative Months of Follow-Up	36,774	Failure to Sense	2		
Number of Leads Active in Study	191	Lead Dislodgement	1		

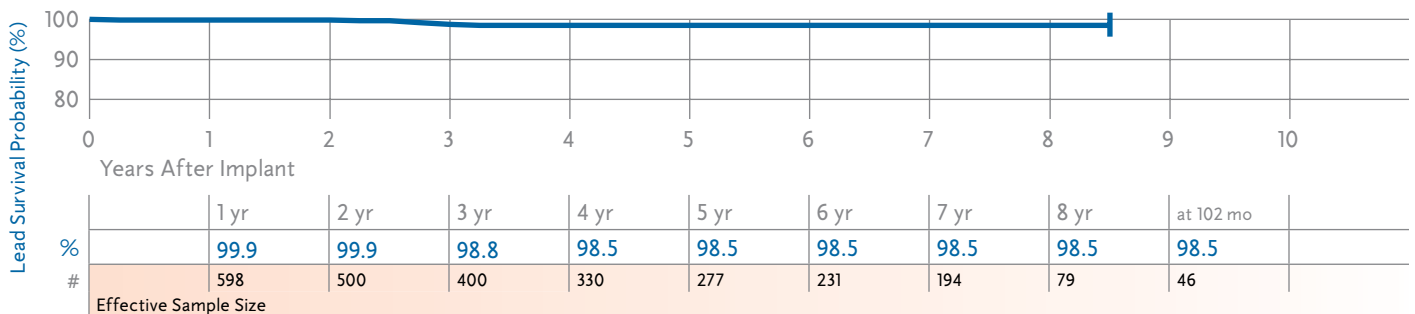

Leads

Pacing Leads continued

6957 Spectraflex

Product Characteristics


US Market Release	Jul-79	Serial Number Prefix	VC	<u>US Returned Product Analysis</u>	
Estimated US Implants	29,100	Type and/or Fixation	Transvenous, V or A, Screw-in	Implant Damage	85
Estimated US Active	2,600	Polarity	Unipolar	Electrical Malfunction	39
Advisories	None	Steroid	No	Other	25

Atrial Placement

System Longevity Study Results

Qualifying Complications 10 Total

Number of Leads Enrolled in Study	673	Extra Cardiac Stimulation	1	Oversensing	1
Cumulative Months of Follow-Up	24,255	Failure to Capture	3		
Number of Leads Active in Study	1	Failure to Sense	5		

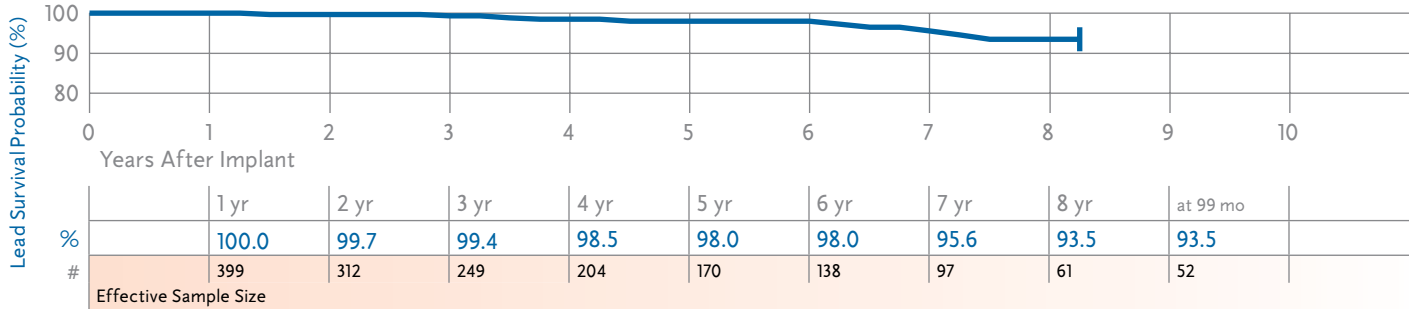


Ventricular Placement

System Longevity Study Results

Qualifying Complications 42 Total

Number of Leads Enrolled in Study	1,853	Conductor Fracture	14	Impedance Out of Range	1
Cumulative Months of Follow-Up	96,172	Extra Cardiac Stimulation	2	Insulation (not further defined)	1
Number of Leads Active in Study	22	Failure to Capture	18	Oversensing	4
		Failure to Sense	2		

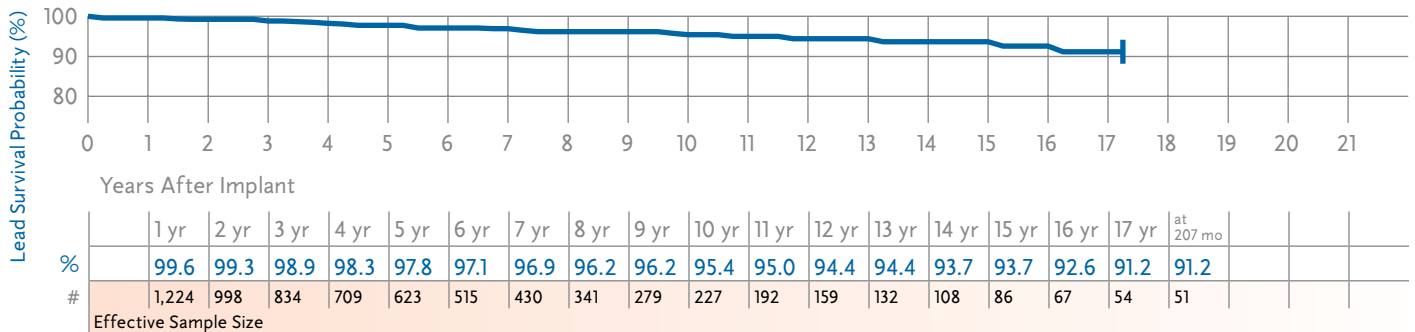

6957J Spectraflex

Product Characteristics

US Market Release	Sep-80	Serial Number Prefix	GG	<u>US Returned Product Analysis</u>	
Estimated US Implants	30,000	Type and/or Fixation	Transvenous, Atrial-J, Screw-in	Implant Damage	74
Estimated US Active	2,100	Polarity	Unipolar	Electrical Malfunction	28
Advisories	None	Steroid	No	Other	30


Atrial Placement

System Longevity Study Results

Number of Leads Enrolled in Study	2,348
Cumulative Months of Follow-Up	160,328
Number of Leads Active in Study	28

Qualifying Complications 88 Total

Conductor Fracture	13	Insulation (ESC)	1
Extra Cardiac Stimulation	3	Insulation (not further defined)	3
Failure to Capture	48	Lead Dislodgement	2
Failure to Sense	14	Oversensing	3
Impedance Out of Range	1		

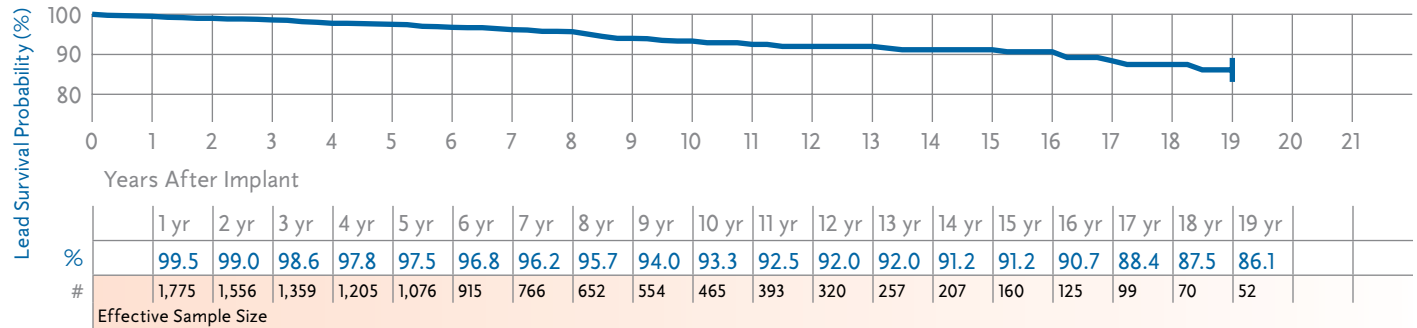

Leads

6961 Tenax

Product Characteristics

US Market Release	Jan-78	Serial Number Prefix	TB	<u>US Returned Product Analysis</u>	
Estimated US Implants	44,700	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	103
Estimated US Active	1,000	Polarity	Unipolar	Electrical Malfunction	27
Advisories	None	Steroid	No	Other	0


Ventricular Placement

System Longevity Study Results

Number of Leads Enrolled in Study	627
Cumulative Months of Follow-Up	42,864
Number of Leads Active in Study	0

Qualifying Complications 22 Total

Extra Cardiac Stimulation	4	Insulation (not further defined)	2
Failure to Capture	8	Lead Dislodgement	1
Failure to Sense	6	Oversensing	1

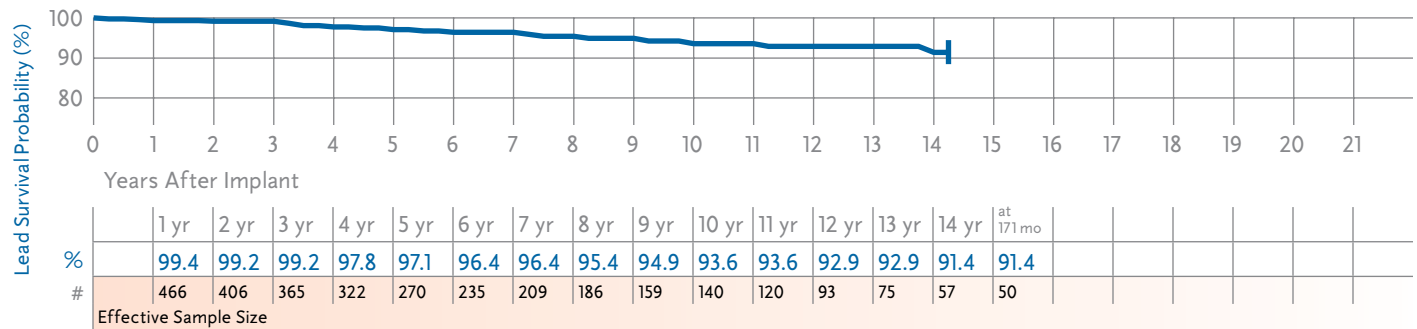

Pacing Leads continued

6962 Tenax

Product Characteristics

US Market Release	Jan-78	Serial Number Prefix	UB	<u>US Returned Product Analysis</u>	
Estimated US Implants	70,600	Type and/or Fixation	Transvenous, Vent., Tines	Implant Damage	170
Estimated US Active	2,000	Polarity	Bipolar	Electrical Malfunction	84
Advisories	None	Steroid	No	Other	0


Ventricular Placement

System Longevity Study Results

Number of Leads Enrolled in Study	1,483
Cumulative Months of Follow-Up	109,926
Number of Leads Active in Study	3

Qualifying Complications 51 Total

Conductor Fracture	5	Impedance Out of Range	2
Extra Cardiac Stimulation	1	Insulation (not further defined)	2
Failure to Capture	27	Lead Dislodgement	1
Failure to Sense	10	Oversensing	3

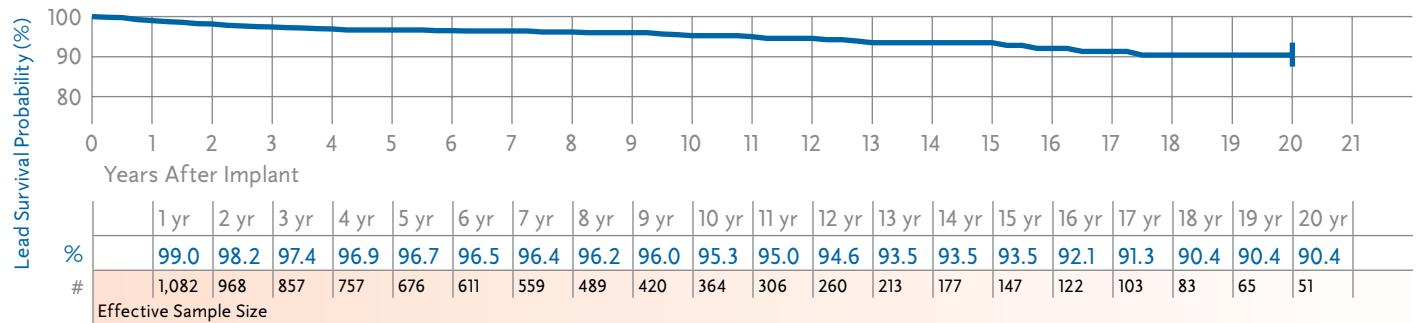

Lead Survival Summary (95% Confidence Interval)

Model Number	Family	Chamber	US Market Release	Leads Enrolled	Leads Active in Study	Qualifying Complications	Cumulative Months of Follow-Up in Study	Device Survival Probability (%)															
								Years After Implant															
								1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	12 yr	14 yr	16 yr	18 yr	20 yr		
3830	SelectSecure	Atrial	Aug-05	152	91	1	4,272	99.3 +0.6/-4.2	99.3 +0.6/-4.2	99.3 +0.6/-4.2	99.1 +0.5/-1.2	98.8 +0.7/-1.5	98.5 +0.8/-1.8	97.7 +1.1/-2.4	97.7 +1.1/-2.4	96.2 +2.2/-4.9 at 138 mo							
3830	SelectSecure	Vent	Aug-05	140	85	0	4,233	100.0	100.0	100.0													
4003, 4003M	CapSure	Vent	Jul-86	711	159	12	45,771	99.4 +0.4/-1.1	99.4 +0.4/-1.1	99.4 +0.4/-1.1	99.1 +0.5/-1.2	98.8 +0.7/-1.5	98.5 +0.8/-1.8	97.7 +1.1/-2.4	97.7 +1.1/-2.4	96.2 +2.2/-4.9 at 138 mo							
4004, 4004M	CapSure	Vent	Feb-89	1,640	5	278	71,611	99.8 +0.1/-0.5	99.3 +0.4/-0.7	96.3 +1.0/-1.4	87.4 +2.1/-2.4	69.4 +3.4/-3.7	64.1 +3.7/-4.1	58.1 +4.2/-4.5	51.5 +4.8/-5.0	50.6 +3.0/-5.2 at 129 mo							
4011	Target Tip	Vent	Nov-82	851	4	25	54,409	99.4 +0.4/-1.0	99.2 +0.5/-1.0	99.1 +0.5/-1.2	98.8 +0.7/-1.2	96.4 +1.4/-2.3	96.0 +1.6/-2.4	96.0 +1.6/-2.4	95.0 +1.9/-3.0	92.8 +2.7/-4.2	91.9 +3.1/-4.7 at 183 mo						
4012	Target Tip	Vent	Jul-83	2,543	12	316	151,022	99.6 +0.2/-0.3	99.1 +0.4/-0.5	98.4 +0.5/-0.7	95.9 +0.8/-1.1	92.6 +1.2/-1.5	88.1 +1.7/-1.9	83.9 +2.0/-2.2	77.8 +2.5/-2.7	65.7 +3.5/-3.7	62.9 +4.0/-4.2 at 189 mo						
4023	CapSure SP	Vent	Aug-91	1,158	398	20	62,408	99.9 +0.1/-0.6	99.3 +0.4/-0.9	98.8 +0.5/-1.1	98.6 +0.6/-1.1	98.2 +0.8/-1.4	97.0 +1.2/-2.1	96.6 +1.3/-2.3	95.8 +1.8/-3.1	94.3 +2.7/-5.1 at 135 mo							
4024	CapSure SP	Vent	Oct-91	1,215	28	3	51,600	99.9 +0.1/-0.5	99.8 +0.1/-0.7	99.8 +0.1/-0.7	99.8 +0.1/-0.7	99.8 +0.1/-0.7	99.8 +0.1/-0.7	99.8 +0.1/-0.7	99.8 +0.1/-0.7								
4033	CapSure Z	Vent	not US released	541	49	11	28,347	99.4 +0.4/-1.4	99.4 +0.4/-1.4	98.8 +0.7/-1.7	98.5 +0.8/-1.9	97.5 +1.3/-2.7	97.5 +1.3/-2.7	96.5 +1.9/-3.8	95.3 +2.5/-5.2 at 111 mo								
4057, 4057M	Screw-In	Vent	Aug-88	259	13	7	15,266	99.4 +0.5/-3.5	99.4 +0.5/-3.5	99.4 +0.5/-3.5	98.6 +1.1/-4.1	97.7 +1.6/-4.7	96.8 +2.0/-5.3	95.7 +2.5/-5.9	94.4 +3.1/-6.8 at 114 mo								
4058, 4058M	Screw-In	Atrial	Jan-89	2,364	58	32	130,879	99.9 +0.1/-0.4	99.6 +0.2/-0.4	99.5 +0.2/-0.5	99.1 +0.4/-0.6	98.7 +0.5/-0.7	98.3 +0.6/-0.9	98.2 +0.6/-1.0	97.5 +0.8/-1.3	96.1 +1.4/-2.1	95.0 +2.1/-3.5 at 171 mo						
4058, 4058M	Screw-In	Vent	Jan-89	1,690	59	53	76,863	99.4 +0.3/-0.7	99.2 +0.4/-0.7	99.1 +0.4/-0.8	98.7 +0.5/-1.0	97.9 +0.8/-1.2	96.9 +1.1/-1.6	94.6 +1.7/-2.3	89.2 +3.1/-4.2	85.2 +4.5/-6.0 at 153 mo							
4067	CapSureFix	Atrial	Jan-97	108	42	6	6,054	97.0 +2.0/-5.9	97.0 +2.0/-5.9	97.0 +2.0/-5.9	97.0 +2.0/-5.9	97.0 +2.0/-5.9	97.0 +2.0/-5.9	97.0 +2.0/-5.9	97.0 +2.0/-5.9								
4068	CapSureFix	Atrial	Mar-96	2,401	631	55	117,635	99.0 +0.4/-0.5	98.8 +0.4/-0.6	98.3 +0.5/-0.7	98.1 +0.5/-0.8	97.6 +0.6/-1.0	97.4 +0.7/-1.0	97.2 +0.8/-1.0	96.2 +1.2/-1.5	93.9 +2.3/-3.7 at 129 mo							
4068	CapSureFix	Vent	Mar-96	1,799	527	33	84,282	99.3 +0.3/-0.6	98.8 +0.4/-0.7	98.8 +0.4/-0.7	98.4 +0.6/-0.8	98.0 +0.7/-1.0	97.7 +0.8/-1.2	96.9 +1.0/-1.7	96.4 +1.3/-2.1	93.6 +2.7/-4.6							

continued



Lead Survival Summary continued

Model Number	Family	Chamber	US Market Release	Leads Enrolled	Leads Active in Study	Qualifying Complications	Cumulative Months of Follow-Up in Study	Device Survival Probability (%)																	
								Years After Implant																	
								1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	12 yr	14 yr	16 yr	18 yr	20 yr				
4073	CapSure Sense	Atrial Jun-02	1	1	0	40		Survival estimate not available due to insufficient sample size																	
4073	CapSure Sense	Vent Jun-02	100	85	0	3,775	100.0	100.0 at 39 mo																	
4074	CapSure Sense	Vent Jun-02	614	529	6	18,331	99.3 +0.4/-1.1	99.1 +0.5/-1.3	99.1 +0.5/-1.3	99.1 +0.5/-1.3 at 54 mo															
4076	CapSureFix Novus	Atrial Feb-04	563	495	2	10,581	99.8 +0.2/-1.1	99.5 +0.4/-1.5	99.5 +0.4/-1.5																
4076	CapSureFix Novus	Vent Feb-04	545	480	2	11,633	99.6 +0.3/-1.2	99.6 +0.3/-1.2	99.6 +0.3/-1.2 at 39 mo																
4081	Target Tip	Vent Jul-89	260	12	3	9,861	100.0	100.0	100.0	100.0	98.2 +1.5/-10.5 at 63 mo														
4092	CapSure SP Novus	Vent Sep-98	1,144	597	17	49,981	98.9 +0.5/-0.9	98.8 +0.5/-0.9	98.7 +0.5/-1.0	98.4 +0.6/-1.1	97.9 +0.8/-1.3	97.9 +0.8/-1.3 at 81 mo													
4503, 4503M	CapSure	Atrial Jul-86	59	6	1	3,206	Survival estimate not available due to insufficient sample size																		
4504, 4504M	CapSure	Atrial Mar-90	368	1	48	19,867	100.0	100.0	99.1 +0.7/-2.5	98.2 +1.1/-3.0	90.3 +3.5/-5.3	82.2 +5.1/-6.8	73.0 +6.5/-8.2	69.9 +7.0/-8.7	66.1 +7.7/-9.2 at 103 mo										
4512	Target Tip	Atrial Jul-83	600	6	35	39,765	99.6 +0.3/-1.2	99.6 +0.3/-1.2	99.1 +0.6/-1.5	98.0 +1.0/-2.0	96.7 +1.4/-2.4	95.6 +1.8/-2.8	94.7 +2.0/-3.2	91.5 +2.9/-4.3	87.5 +3.9/-5.5	84.8 +4.6/-6.3 at 139 mo									
4523	CapSure SP	Atrial Aug-91	121	19	4	7,060	98.1 +1.4/-5.3	98.1 +1.4/-5.3	98.1 +1.4/-5.3	98.1 +1.4/-5.3 at 57 mo															
4524	CapSure SP	Atrial Oct-91	910	59	6	39,326	99.6 +0.3/-0.7	99.3 +0.4/-1.0	99.3 +0.4/-1.0	99.0 +0.6/-1.2	99.0 +0.6/-1.2	99.0 +0.6/-1.2	99.0 +0.6/-1.2	99.0 +0.6/-1.2	99.0 +0.6/-1.2 at 114 mo										
4533	CapSure Z	Atrial not US released	206	19	4	11,153	100.0	99.4 +0.5/-3.5	98.8 +0.9/-3.6	97.9 +1.4/-4.2	97.9 +1.4/-4.2	97.9 +1.4/-4.2 at 78 mo													
4557, 4557M	Screw-In	Atrial Aug-88	294	15	6	18,357	99.1 +0.7/-2.8	99.1 +0.7/-2.8	99.1 +0.7/-2.8	97.8 +1.4/-3.6	97.8 +1.4/-3.6	97.8 +1.4/-3.6	96.9 +1.8/-4.4	96.9 +1.8/-4.4	96.9 +1.8/-4.4	96.9 +1.8/-4.4 at 126 mo									
4558M	Screw-In	Atrial Nov-94	539	28	11	22,131	99.3 +0.5/-1.4	99.3 +0.5/-1.4	99.3 +0.5/-1.4	99.3 +0.5/-1.4	99.3 +0.5/-1.4	97.6 +1.6/-4.2	96.5 +2.1/-5.2	96.5 +2.1/-5.2	91.6 +4.5/-9.0 at 108 mo										

continued

Pacing Leads continued

Lead Survival Summary continued

Model Number	Family	Chamber	US Market Release	Leads Enrolled	Leads Active in Study	Qualifying Complications	Cumulative Months of Follow-Up in Study	Device Survival Probability (%)															
								Years After Implant															
								1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	12 yr	14 yr	16 yr	18 yr	20 yr		
4568	CapSureFix	Atrial	Jan-97	576	223	30	21,713	96.3 +1.4/-2.1	95.8 +1.5/-2.2	94.5 +1.8/-2.6	94.1 +1.9/-2.8	93.1 +2.2/-3.2	93.1 +2.2/-3.2	93.1 +2.2/-3.2	93.1 +2.2/-3.2 at 75 mo								
4574	CapSure Sense	Atrial	Jun-02	6	4	0	145	Survival estimate not available due to insufficient sample size															
4592	CapSure SP Novus	Atrial	Oct-98	244	93	5	10,221	97.8 +1.4/-3.5	97.8 +1.4/-3.5	97.8 +1.4/-3.5	97.8 +1.4/-3.5	97.0 +1.8/-4.3	97.0 +1.8/-4.3	97.0 +1.8/-4.3 at 75 mo									
5023, 5023M	CapSure SP	Vent	Nov-88	1,353	550	14	65,821	99.7 +0.2/-0.5	99.6 +0.3/-0.6	99.5 +0.3/-0.6	99.4 +0.3/-0.8	99.4 +0.3/-0.8	99.2 +0.4/-1.0	99.2 +0.4/-1.0	97.1 +1.3/-2.5	97.1 +1.3/-2.5 at 111 mo							
5024, 5024M	CapSure SP	Vent	Mar-90	8,142	711	45	425,081	99.7 +0.1/-0.2	99.6 +0.1/-0.2	99.5 +0.2/-0.2	99.5 +0.1/-0.2	99.4 +0.2/-0.2	99.3 +0.2/-0.2	99.3 +0.2/-0.2	99.3 +0.2/-0.2	99.3 +0.3/-0.4	98.8 +0.4/-0.6	98.6 +0.5/-0.8	98.6 +0.5/-0.8 at 186 mo				
5026	CapSure	Vent	Feb-88	168	6	4	9,558	100.0	99.2 +0.7/-4.8	98.2 +1.4/-5.2	97.1 +2.0/-5.9	97.1 +2.0/-5.9	97.1 +2.0/-5.9	95.7 +2.7/-7.2 at 75 mo									
5033	CapSure Z	Vent	Feb-96	1,901	313	24	92,733	99.7 +0.2/-0.4	99.6 +0.2/-0.4	99.1 +0.4/-0.7	99.0 +0.3/-0.7	98.7 +0.6/-0.9	98.3 +0.7/-1.2	98.3 +0.7/-1.2	97.7 +0.9/-1.4	97.2 +1.0/-1.6	96.5 +1.3/-1.9	96.5 +1.3/-1.9 at 129 mo					
5034	CapSure Z	Vent	Feb-96	1,594	292	13	80,368	99.7 +0.2/-0.5	99.5 +0.3/-0.6	99.3 +0.3/-0.7	99.2 +0.4/-0.8	99.2 +0.4/-0.8	99.2 +0.4/-0.8	99.2 +0.4/-0.8	98.9 +0.5/-0.9	98.3 +0.8/-1.5	98.3 +0.8/-1.5	98.3 +0.8/-1.5					
5054	CapSure Z Novus	Vent	Jun-98	1,392	534	11	57,156	99.5 +0.3/-0.6	99.4 +0.3/-0.6	99.4 +0.3/-0.6	99.3 +0.3/-0.8	99.3 +0.3/-0.8	99.3 +0.3/-0.8	98.4 +0.8/-1.6	98.4 +0.8/-1.6 at 90 mo								
5068	CapSureFix	Atrial	Jan-97	969	90	7	32,166	99.6 +0.3/-0.9	99.6 +0.3/-0.9	99.6 +0.3/-0.9	99.2 +0.5/-1.5	99.2 +0.5/-1.5	99.2 +0.5/-1.5	99.2 +0.5/-1.5	99.2 +0.5/-1.5	98.3 +1.2/-3.6 at 114 mo							
5068	CapSureFix	Vent	Jan-97	1,360	164	6	35,786	99.8 +0.1/-0.6	99.6 +0.3/-0.8	99.4 +0.4/-1.1	99.1 +0.5/-1.5	99.1 +0.5/-1.5	99.1 +0.5/-1.5	99.1 +0.5/-1.5	98.2 +1.2/-3.5	98.2 +1.2/-3.5							
5072	SureFix	Atrial	Jun-98	451	132	2	20,937	99.7 +0.3/-1.5	99.7 +0.3/-1.5	99.4 +0.4/-1.9	99.4 +0.4/-1.9	99.4 +0.4/-1.9	99.4 +0.4/-1.9	99.4 +0.4/-1.9	99.4 +0.4/-1.9	99.4 +0.4/-1.9 at 90 mo							
5076	CapSureFix Novus	Atrial	Aug-00	2,502	1,226	15	81,429	99.6 +0.2/-0.3	99.6 +0.2/-0.4	99.4 +0.3/-0.5	99.0 +0.5/-0.7	99.0 +0.5/-0.7	99.0 +0.5/-0.7	99.0 +0.5/-0.7	99.0 +0.5/-0.7 at 78 mo								
5076	CapSureFix Novus	Vent	Aug-00	1,508	660	9	48,187	99.6 +0.2/-0.5	99.4 +0.3/-0.6	99.3 +0.3/-0.8	99.1 +0.4/-0.9	99.1 +0.4/-0.9	99.1 +0.4/-0.9	99.1 +0.4/-0.9	99.1 +0.4/-0.9 at 75 mo								
5092	CapSure SP Novus	Vent	Jun-98	1,171	257	8	38,950	99.6 +0.2/-0.7	99.5 +0.3/-0.8	99.3 +0.4/-1.0	99.0 +0.6/-1.2	99.0 +0.6/-1.2	99.0 +0.6/-1.2	99.0 +0.6/-1.2	99.0 +0.6/-1.2								
5524, 5524M	CapSure SP	Atrial	Mar-90	4,440	555	38	235,419	99.8 +0.1/-0.2	99.8 +0.1/-0.3	99.5 +0.2/-0.3	99.4 +0.2/-0.4	99.3 +0.2/-0.4	99.3 +0.2/-0.4	99.2 +0.3/-0.4	98.9 +0.4/-0.5	98.4 +0.5/-0.8	97.5 +0.8/-1.3	96.8 +1.1/-1.7 at 165 mo	96.8 +1.1/-1.7 at 165 mo				

continued

Leads

US Returned Product Analysis Summary

Model Number	Family	US Market Release	Estimated US Implants	Estimated US Active	Implant Damage	Electrical Malfunction	Other
3830	SelectSecure	Aug-05	9,100	8,000	14	2	1
4003, 4003M	CapSure	Jul-86	40,000	6,700	24	58	2
4004, 4004M	CapSure	Feb-89	74,500	2,500	55	684	19
4011	Target Tip	Nov-82	64,000	6,900	29	142	5
4012	Target Tip	Jul-83	96,800	5,300	50	820	34
4023	CapSure SP	Aug-91	43,700	14,200	47	19	6
4024	CapSure SP	Oct-91	229,200	80,700	264	106	34
4033	CapSure Z	not US released	N/A	N/A	2	0	0
4057, 4057M	Screw-in	Aug-88	12,100	2,600	39	6	4
4058, 4058M	Screw-in	Jan-89	111,100	24,600	388	228	23
4067	CapSureFix	Jan-97	1,300	500	3	1	1
4068	CapSureFix	Mar-96	131,700	54,700	406	83	11
4073	CapSure Sense	Jun-02	500	400	1	0	0
4074	CapSure Sense	Jun-02	53,400	41,500	12	3	1
4076	CapSureFix Novus	Feb-04	144,400	122,500	53	3	6
4081	Target Tip	Jul-89	4,100	900	4	5	0
4092	CapSure SP Novus	Sep-98	144,600	90,400	35	12	5
4503, 4503M	CapSure	Jul-86	9,000	1,300	2	11	0
4504, 4504M	CapSure	Mar-90	16,600	1,500	5	171	4
4512	Target Tip	Jul-83	11,600	1,000	4	83	8
4523	CapSure SP	Aug-91	12,000	3,300	5	2	1
4524	CapSure SP	Oct-91	106,900	36,300	47	23	8
4533	CapSure Z	not US released	N/A	N/A	0	0	0
4557, 4557M	Screw-in	Aug-88	22,500	4,900	53	14	4
4558M	Screw-in	Nov-94	21,000	5,800	111	11	1
4568	CapSureFix	Jan-97	72,800	35,800	197	6	4
4574	CapSure Sense	Jun-02	34,500	26,500	6	2	0
4592	CapSure SP Novus	Oct-98	73,000	44,400	12	3	0
5023, 5023M	CapSure SP	Nov-88	10,600	2,800	15	7	0
5024, 5024M	CapSure SP	Mar-90	211,400	69,300	723	106	29
5026	CapSure	Feb-88	7,800	1,200	60	7	1
5033	CapSure Z	Feb-96	2,500	1,000	6	1	3
5034	CapSure Z	Feb-96	58,700	21,900	85	29	11
5054	CapSure Z Novus	Jun-98	84,700	49,700	40	13	6
5068	CapSureFix	Jan-97	108,000	49,800	455	63	15
5072	SureFix	Jun-98	9,100	5,000	26	4	1
5076	CapSureFix Novus	Aug-00	911,600	665,100	705	163	51
5092	CapSure SP Novus	Jun-98	109,800	68,900	47	20	11
5524, 5524M	CapSure SP	Mar-90	63,800	22,300	66	21	7
5534	CapSure Z	Feb-96	27,700	8,700	29	6	5
5554	CapSure Z Novus	Jun-98	54,600	32,300	7	6	4
5568	CapSureFix	Jan-97	66,500	44,700	228	8	9
5592	CapSure SP Novus	Jun-98	26,700	18,200	6	3	0

continued

US Returned Product Analysis Summary continued

Model Number	Family	US Market Release	Estimated US Implants	Estimated US Active	Implant Damage	Electrical Malfunction	Other
5594	CapSure SP Novus	Jun-01	10,000	7,400	0	1	0
6940	CapSureFix	Oct-98	26,600	12,300	114	19	3
6957	Spectraflex	Jul-79	29,100	2,600	85	39	25
6957J	Spectraflex	Sep-80	30,000	2,100	74	28	30
6961	Tenax	Jan-78	44,700	1,000	103	27	0
6962	Tenax	Jan-78	70,600	2,000	170	84	0

Reference Chart

Model Number	Family	Type	Insulation	Conductor Material	Tip Electrode	Connector Type
3830	SelectSecure	Transvenous V or A Screw-In	Polyurethane/Silicone (55D,4719)	MP35N 5 Filars/Cable	1.8 mm Helix/Steroid	IS-1 BI
4003, 4003M	CapSure	Transvenous Ventricular Tines	Polyurethane (80A)	MP35N 4 Filars	Porous/Steroid	5 mm (4003) IS-1 UNI (4003M)
4004, 4004M	CapSure	Transvenous Ventricular Tines	Polyurethane (80A)	MP35N 6/4 Filars	Porous/Steroid	3.2 mm Low Profile (4004) IS-1 BI (4004M)
4011	Target Tip	Transvenous Ventricular Tines	Polyurethane (80A)	MP35N 4 Filars	Target Tip Concentric Grooves	5 mm
4012	Target Tip	Transvenous Ventricular Tines	Polyurethane (80A)	MP35N 6/4 Filars	Target Tip Concentric Grooves	3.2 mm Low Profile
4023	CapSure SP	Transvenous Ventricular Tines	Polyurethane (55D)	MP35N 4 Filars	Porous Platinized/Steroid	IS-1 UNI
4024	CapSure SP	Transvenous Ventricular Tines	Polyurethane (55D)	MP35N 4/5 Filars	Porous Platinized/Steroid	IS-1 BI
4033	CapSure Z	Transvenous Ventricular Tines	Polyurethane (55D)	MP35N 2 Filars	CapSure Z Platinized/Steroid	IS-1 UNI
4057, 4057M	Screw-In	Transvenous V or A Screw-In	Polyurethane (80A)	MP35N 1 Filar	2.0 mm Helix	5 mm (4057) IS-1 UNI (4057M)
4058, 4058M	Screw-In	Transvenous V or A Screw-In	Polyurethane (80A/55D)	MP35N 4/1 Filars	2.0 mm Helix	3.2 mm Low Profile (4058) IS-1 BI (4058M)
4067	CapSureFix	Transvenous V or A Screw-In	Polyurethane (80A)	MP35N 3 Filars	1.8 mm Helix/Steroid	IS-1 UNI
4068	CapSureFix	Transvenous V or A Screw-In	Polyurethane (80A/55D)	MP35N 4/3 Filars	1.8 mm Helix/Steroid	IS-1 BI
4073	CapSure Sense	Transvenous Ventricular Tines	Polyurethane (55D)	MP35N 5 Filars	TiN Coated Platinum Iridium/Steroid	IS-1 UNI
4074	CapSure Sense	Transvenous Ventricular Tines	Polyurethane/Silicone (55D, 4719)	MP35N 5/5 Filars	TiN Coated Platinum Iridium/Steroid	IS-1 BI
4076	CapSureFix Novus	Transvenous V or A Screw-In	Polyurethane/Silicone (55D, 4719)	MP35N 4/6 Filars	TiN Coated Platinum Alloy/Steroid	IS-1 BI
4081	Target Tip	Transvenous Ventricular Tines	Polyurethane (80A)	MP35N 4 Filars	Target Tip Concentric Grooves	IS-1 UNI w/Removable 5 mm Sleeve
4092	CapSure SP Novus	Transvenous Ventricular Tines	Polyurethane/Silicone (55D/4719)	MP35N 6/4 Filars	Porous Platinized/Steroid	IS-1 BI
4503, 4503M	CapSure	Transvenous Atrial-J Tines	Polyurethane (80A)	MP35N 4 Filars	Porous/Steroid	5 mm (4503) IS-1 UNI (4503M)
4504, 4504M	CapSure	Transvenous Atrial-J Tines	Polyurethane (80A)	MP35N 3/4 Filars	Porous/Steroid	3.2 mm Low Profile (4504) IS-1 BI (4504M)
4512	Target Tip	Transvenous Atrial-J Tines	Polyurethane (80A)	MP35N 2/4 Filars	Target Tip Concentric Grooves	3.2 mm Low Profile
4523	CapSure SP	Transvenous Atrial-J Tines	Polyurethane (55D)	MP35N 2 Filars	Porous Platinized/Steroid	IS-1 UNI
4524	CapSure SP	Transvenous Atrial-J Tines	Polyurethane (55D)	MP35N 4/5 Filars	Porous Platinized/Steroid	IS-1 BI
4533	CapSure Z	Transvenous Atrial-J Tines	Polyurethane (55D)	MP35N 2 Filars	CapSure Z Platinized/Steroid	IS-1 UNI
4557, 4557M	Screw-In	Transvenous Atrial-J Screw-In	Polyurethane (80A)	MP35N 1 Filar	1.5 mm Helix	5 mm (4557) IS-1 UNI (4557M)
4558M	Screw-In	Transvenous Atrial-J Screw-In	Polyurethane (80A/55D)	MP35N 6/3 Filars	1.8 mm Helix/Steroid	IS-1 BI
4568	CapSureFix	Transvenous Atrial-J Screw-In	Polyurethane (80A/55D)	MP35N 6/3 Filars	1.8 mm Helix/Steroid	IS-1 BI
4574	CapSure Sense	Transvenous Atrial-J Tines	Polyurethane/Silicone (55D,4719)	MP35N 5/5 Filars	TiN Coated Platinum Iridium	IS-1 BI
4592	CapSure SP Novus	Transvenous Atrial-J Tines	Polyurethane/Silicone (55D/4719)	MP35N 6/3 Filars	Porous Platinized/Steroid	IS-1 BI
5023, 5023M	CapSure SP	Transvenous Ventricular Tines	Silicone	MP35N 4 Filars	Porous Platinized/Steroid	5 mm (5023) IS-1 UNI (5023M)

continued

Reference Chart continued

Model Number	Family	Type	Insulation	Conductor Material	Tip Electrode	Connector Type
5024, 5024M	CapSure SP	Transvenous Ventricular Tines	Silicone	MP35N 4/5 Filars	Porous Platinized/ Steroid	3.2 mm Low Profile (5024) IS-1 BI (5024M)
5026	CapSure	Transvenous Ventricular Tines	Silicone	MP35N 6/4 Filars	Porous Platinized/ Steroid	3.2 mm Low Profile
5033	CapSure Z	Transvenous Ventricular Tines	Silicone	MP35N 4 Filars	CapSure Z Platinized/Steroid	IS-1 UNI
5034	CapSure Z	Transvenous Ventricular Tines	Silicone	MP35N 4/5 Filars	CapSure Z Platinized/Steroid	IS-1 BI
5054	CapSure Z Novus	Transvenous Ventricular Tines	Silicone (4719)	MP35N 5/5 Filars	CapSure Z Porous/Platinized/ Steroid	IS-1 BI
5068	CapSureFix	Transvenous V or A Screw-In	Silicone	MP35N 4/3 Filars	1.8 mm Helix/Steroid	IS-1 BI
5072	SureFix	Transvenous V or A Screw-In	Silicone	MP35N 4/5 Filars	1.8 mm Helix/Steroid	IS-1 BI
5076	CapSureFix Novus	Transvenous V or A Screw-In	Silicone (4719)	MP35N 4/6 Filars	Porous Platinized/ Steroid	IS-1 BI
5092	CapSure SP Novus	Transvenous Ventricular Tines	Silicone (4719)	MP35N 5/5 Filars	Porous Platinized/ Steroid	IS-1 BI
5524, 5524M	CapSure SP	Transvenous Atrial-J Tines	Silicone	MP35N 6/5 Filars	Porous Platinized/ Steroid	3.2 mm Low Profile (5524) IS-1 BI (5524M)
5534	CapSure Z	Transvenous Atrial-J Tines	Silicone	MP35N 4/5 Filars	CapSure Z Platinized/Steroid	IS-1 BI
5554	CapSure Z Novus	Transvenous Atrial-J Tines	Silicone (4719)	MP35N 6/5 Filars	CapSure Z Porous Platinized/ Steroid	IS-1 BI
5568	CapSureFix	Transvenous Atrial-J Screw-In	Silicone	MP35N 6/3 Filars	1.8 mm Helix/Steroid	IS-1 BI
5592	CapSure SP Novus	Transvenous Atrial-J Tines	Silicone (4719)	MP35N 6/5 Filars	Porous Platinized/ Steroid	IS-1 BI
5594	CapSure SP Novus	Transvenous Atrial-J Tines	Silicone (4719)	MP35N 6/5 Filars	Platinized Platinum/ Steroid	IS-1 BI
6940	CapSureFix	Transvenous A or V Screw-In	Silicone	MP35N 3/6 Filars	Platinum Alloy	IS-1 BI
6957	Spectraflex	Transvenous V or A Screw-In	Polyurethane (80A)	MP35N 1 Filar	2.0 mm Helix	5 mm
6957J	Spectraflex	Transvenous Atrial-J Screw-In	Polyurethane (80A)	MP35N 1 Filar	1.5 mm Helix	5 mm
6961	Tenax	Transvenous Ventricular Tines	Silicone	MP35N 3 Filars	Ring Tip	5 mm
6962	Tenax	Transvenous Ventricular Tines	Silicone	MP35N 4 Filars	Ring Tip	5 mm Bifurcated

Epi/Myocardial Pacing Leads

4951, 4951M Spectraflex


Product Characteristics

US Market Release	Oct-81	Serial Number Prefix	TF or LBJ	US Returned Product Analysis	
Estimated US Implants	25,300	Type and/or Fixation	Myocardial Stab-in, V or A, Peds	Implant Damage	15
Estimated US Active	3,600	Polarity	Unipolar	Electrical Malfunction	96
Advisories	None	Steroid	No	Other	28

System Longevity Study Results

Qualifying Complications

Number of Leads Enrolled in Study	179	Failure to Capture	4	Insulation (ESC)	1
Cumulative Months of Follow-Up	6,308	Failure to Sense	3	Insulation (not further defined)	1
Number of Leads Active in Study	4	Impedance Out of Range	1		

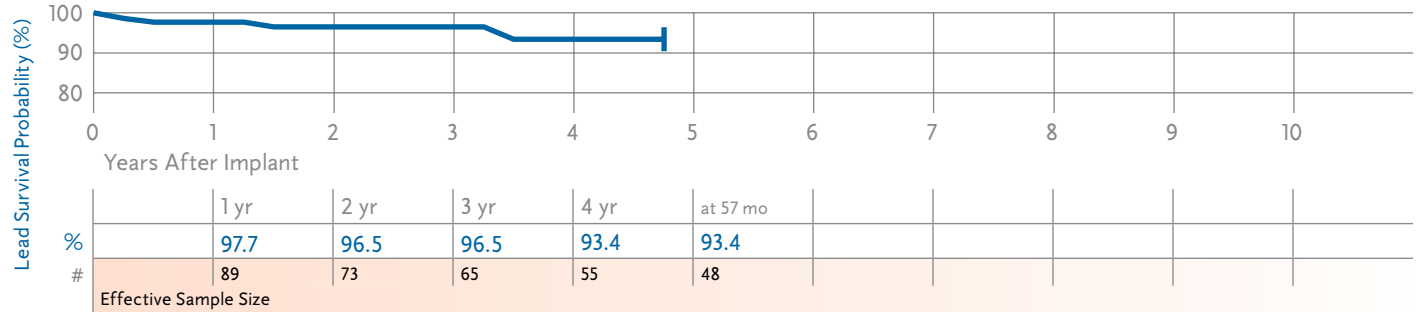

Leads

4965 CapSure Epi


Product Characteristics

US Market Release	Sep-96	Serial Number Prefix	LBT	US Returned Product Analysis	
Estimated US Implants	19,300	Type and/or Fixation	Epicardial Suture-On V or A	Implant Damage	8
Estimated US Active	10,600	Polarity	Unipolar	Electrical Malfunction	81
Advisories	None	Steroid	Yes	Other	2

System Longevity Study Results

Qualifying Complications

Number of Leads Enrolled in Study	172	Conductor Fracture	3	Oversensing	2
Cumulative Months of Follow-Up	4,148	Failure to Capture	2		
Number of Leads Active in Study	10	Failure to Sense	1		

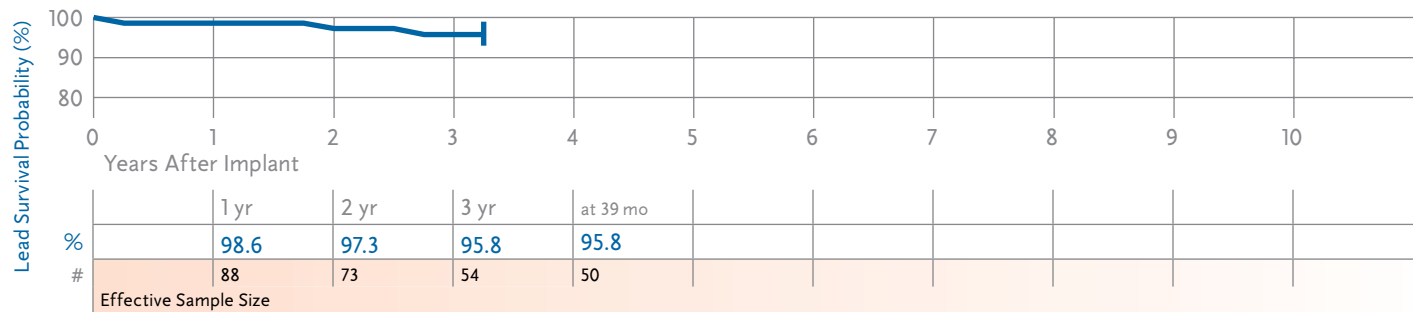

Epi/Myocardial Pacing Leads continued

4968 CapSure Epi


Product Characteristics

US Market Release	Sep-99	Serial Number Prefix	LEN	US Returned Product Analysis	
Estimated US Implants	15,300	Type and/or Fixation	Epicardial Suture-On V or A	Implant Damage	2
Estimated US Active	10,800	Polarity	Bipolar	Electrical Malfunction	3
Advisories	None	Steroid	Yes	Other	0

System Longevity Study Results

Qualifying Complications 31 Total

Number of Leads Enrolled in Study	459	Conductor Fracture	6	Impedance Out of Range	3
Cumulative Months of Follow-Up	17,943	Failure to Capture	11	Insulation (not further defined)	2
Number of Leads Active in Study	290	Failure to Sense	5	Oversensing	4

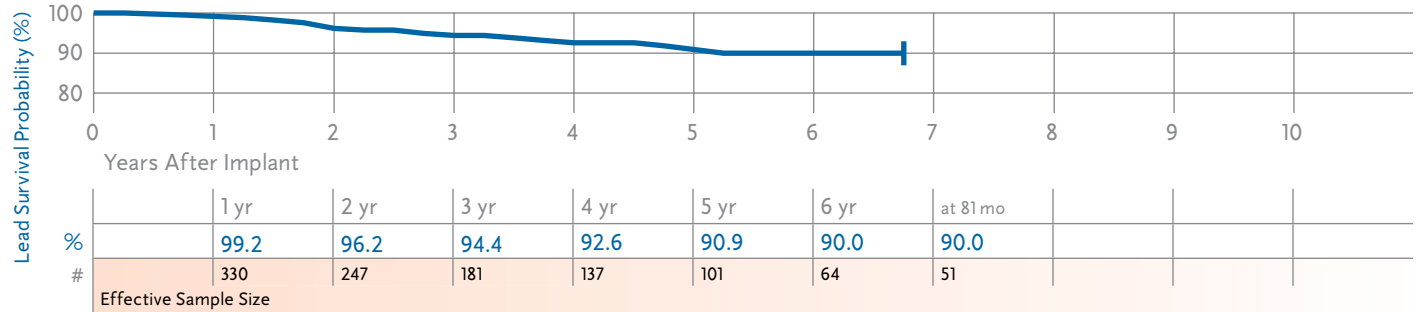

5071


Product Characteristics

US Market Release	Dec-92	Serial Number Prefix	LAQ	US Returned Product Analysis	
Estimated US Implants	36,200	Type and/or Fixation	Myocardial Screw-in Vent.	Implant Damage	24
Estimated US Active	21,700	Polarity	Unipolar	Electrical Malfunction	4
Advisories	None	Steroid	No	Other	1

System Longevity Study Results

Qualifying Complications 10 Total

Number of Leads Enrolled in Study	214	Failure to Capture	8
Cumulative Months of Follow-Up	6,482	Oversensing	2
Number of Leads Active in Study	31		

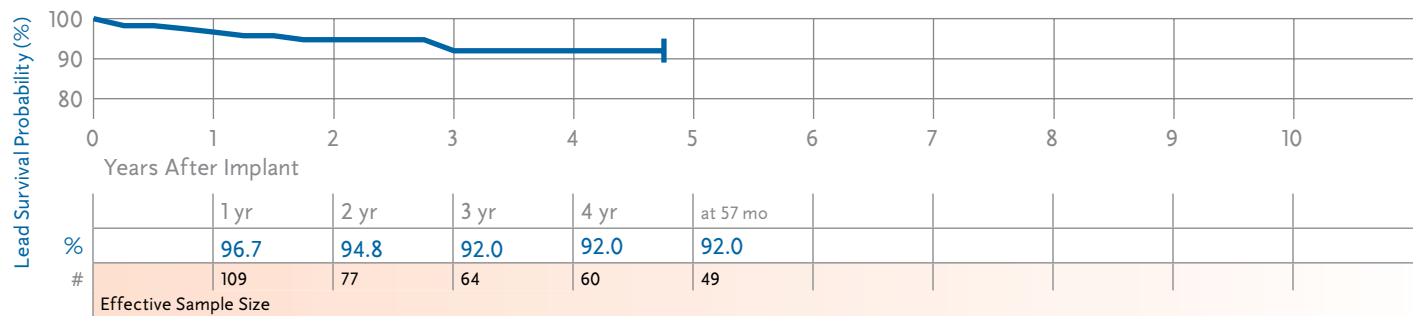

Epi/Myocardial Pacing Leads continued

6917, 6917A Tenax


Product Characteristics

US Market Release	Jun-73	Serial Number Prefix	WV or WC	<u>US Returned Product Analysis</u>	
Estimated US Implants	180,100	Type and/or Fixation	Myocardial Screw-in Vent.	Implant Damage	115
Estimated US Active	5,000	Polarity	Unipolar	Electrical Malfunction	42
Advisories	None	Steroid	No	Other	1

System Longevity Study Results

Qualifying Complications 69 Total

Number of Leads Enrolled in Study	985	Conductor Fracture	6	Impedance Out of Range	2
Cumulative Months of Follow-Up	47,470	Extra Cardiac Stimulation	1	Insulation (MIO)	1
Number of Leads Active in Study	6	Failure to Capture	30	Oversensing	18
		Failure to Sense	11		

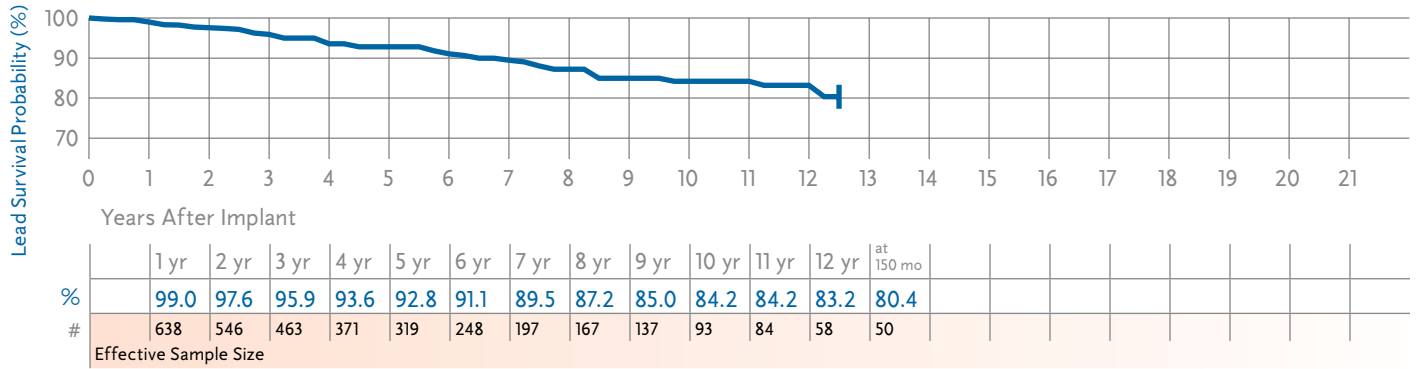

Leads

Epi/Myocardial Pacing Leads continued

Lead Survival Summary (95% Confidence Interval)

Model Number	Family	US Market Release	Leads Enrolled	Leads Active in Study	Qualifying Complications	Cumulative Months of Follow-Up in Study	Device Survival Probability (%)																
							Years After Implant																
							1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	10 yr	12 yr	14 yr	16 yr					
4951, 4951M	Spectraflex	Oct-81	179	4	10	6,308	97.7 +1.6/-4.8	96.5 +2.2/-5.8	96.5 +2.2/-5.8	93.4 +3.7/-8.1	93.4 +3.7/-8.1 at 57 mo												
4965	CapSure Epi	Sep-96	172	10	8	4,184	98.6 +1.1/-4.0	97.3 +1.9/-5.9	95.8 +2.7/-7.4 at 39 mo	95.8 +2.7/-7.4 at 39 mo													
4968	CapSure Epi	Sep-99	459	290	31	17,943	99.2 +0.6/-1.6	96.2 +1.6/-2.9	94.4 +2.2/-3.5	92.6 +2.7/-4.2	90.9 +3.3/-4.9	90.0 +3.6/-5.3 at 81 mo											
5071	(no brand name)	Dec-92	214	31	10	6,482	96.7 +1.9/-4.5	94.8 +2.7/-5.6	92.0 +3.9/-7.5	92.0 +3.9/-7.5	92.0 +3.9/-7.5 at 57 mo												
6917, 6917A	Tenax	Jun-73	985	6	69	47,470	99.0 +0.5/-1.0	97.6 +0.9/-1.5	95.9 +1.3/-2.0	93.6 +1.8/-2.5	92.8 +2.0/-2.6	91.1 +2.3/-3.1	89.5 +2.7/-3.4	87.2 +3.1/-4.1	84.2 +3.9/-4.8	83.2 +4.2/-5.3	80.4 +5.2/-6.8 at 150 mo						

US Returned Product Analysis Summary

Model Number	Family	US Market Release	Estimated US Implants	Estimated US Active	Implant Damage	Electrical Malfunction	Other
4951, 4951M	Spectraflex	Oct-81	25,300	3,600	15	96	28
4965	CapSure Epi	Sep-96	19,300	10,600	8	81	2
4968	CapSure Epi	Sep-99	15,300	10,800	2	3	0
5071	(no brand name)	Dec-92	36,200	21,700	24	4	1
6917, 6917A	Tenax	Jun-73	180,100	5,000	115	42	1

Source: Returned Product Analysis
Data as of January 31, 2008

Reference Chart

Model Number	Family	Type	Insulation	Conductor Material	Tip Electrode	Connector Type
4951, 4951M	Spectraflex	Myocardial Stab-In V or A/Peds	Polyurethane (80A)	MP35N 4 Filars	Barb	5 mm (4951) IS-1 UNI (4951M)
4965	CapSure Epi	Epicardial Suture-On V or A	Silicone	MP35N 5 Filars	Porous Platinized/ Steroid	IS-1 UNI
4968	CapSure Epi	Epicardial Suture V or A	Silicone	MP35N 5 Filars	Porous Platinized/ Steroid	IS-1 B1
5069	(no brand name)	Myocardial Screw-In	Silicone	MP35N Multifilars	3-Turn Helix	IS-1 UNI
5071	(no brand name)	Myocardial Screw-In Ventricular	Silicone	MP35N Multifilars	2-Turn Helix	IS-1 UNI
6917	Tenax	Myocardial Screw-In Ventricular	Silicone	Pt Ir Tinsel Wire	3-Turn Helix	5 mm
6917A	Tenax	Myocardial Screw-In Ventricular	Silicone	Pt Ir Tinsel Wire	2-Turn Helix	5 mm

VDD Single Pass Pacing Leads

5032 CapSure VDD


Product Characteristics

US Market Release	Mar-96	Serial Number Prefix	LCL, LCN, LCM	US Returned Product Analysis	
Estimated US Implants	5,400	Type and/or Fixation	Transvenous, Atr-Vent.,Tines	Implant Damage	24
Estimated US Active	2,000	Polarity	Quadripolar	Electrical Malfunction	12
Advisories	None	Steroid	Yes	Other	0

System Longevity Study Results

Qualifying Complications

Number of Leads Enrolled in Study	38	Failure to Sense	1
Cumulative Months of Follow-Up	1,915		
Number of Leads Active in Study	0		

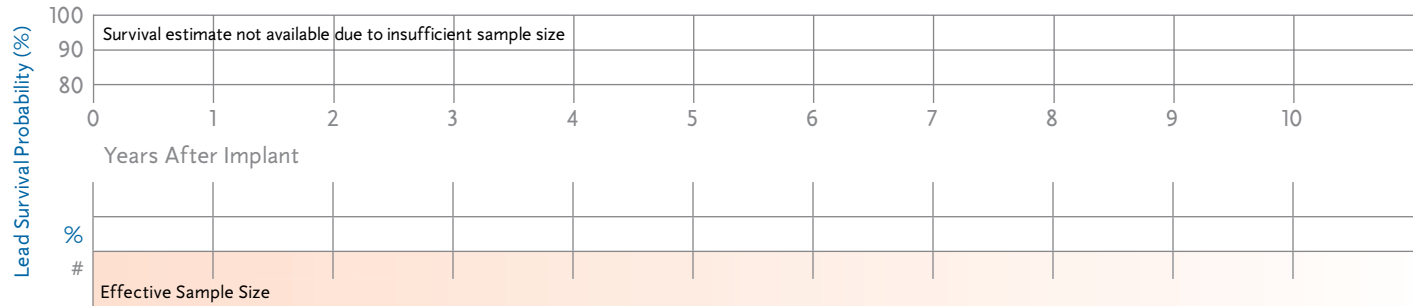

5038 CapSure VDD-2


Product Characteristics

US Market Release	Sep-98	Serial Number Prefix	LEE, LEG, or LEF	US Returned Product Analysis	
Estimated US Implants	7,700	Type and/or Fixation	Transvenous, Atr-Vent.,Tines	Implant Damage	6
Estimated US Active	4,300	Polarity	Quadripolar	Electrical Malfunction	3
Advisories	None	Steroid	Yes	Other	1

System Longevity Study Results

Qualifying Complications

Number of Leads Enrolled in Study	547	Conductor Fracture	3
Cumulative Months of Follow-Up	20,132	Failure to Capture	1
Number of Leads Active in Study	97	Failure to Sense	2

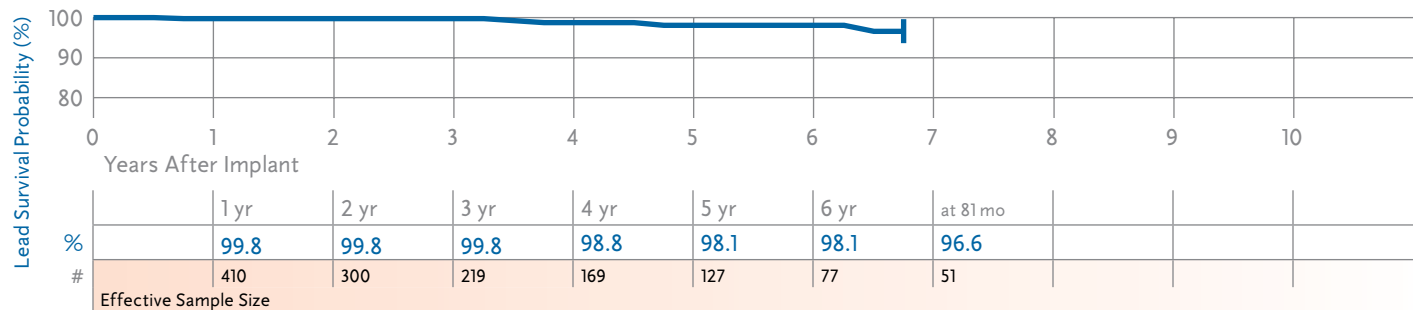

VDD Single Pass Pacing Leads continued

Lead Survival Summary (95% Confidence Interval)

Model Number	Family	US Market Release	Leads Enrolled	Leads Active in Study	Qualifying Complications	Cumulative Months of Follow-Up in Study	Device Survival Probability (%)										
							Years After Implant										
							1 yr	2 yr	3 yr	4 yr	5 yr	6 yr	7 yr	8 yr	9 yr	10 yr	
5032	CapSure VDD	Mar-96	38	0	1	1,915	Survival estimate not available due to insufficient sample size										
5038	CapSure VDD-2	Sep-98	547	97	6	20,132	99.8 +0.2/-1.4	99.8 +0.2/-1.4	99.8 +0.2/-1.4	98.8 +0.8/-2.8	98.1 +1.2/-3.4	98.1 +1.2/-3.4	96.6 +2.2/-5.9 at 81 mo				

Source: System Longevity Study
Data as of January 31, 2008

US Returned Product Analysis Summary

Model Number	Family	US Market Release	Estimated US Implants	Estimated US Active	Implant Damage	Electrical Malfunction	Other
5032	CapSure VDD	Mar-96	5,400	2,100	24	12	0
5038	CapSure VDD-2	Sep-98	7,600	4,400	6	3	1

Source: Returned Product Analysis
Data as of January 31, 2008

Reference Chart

Model Number	Family	Type	Insulation	Conductor Material	Tip Electrode	Connector Type
5032	CapSure VDD	Transvenous V and A Tines	Silicone	MP35N 5/6/1 Filars	Porous Platinized/ Steroid	Atr. IS-1 BI, Vent. IS-1 BI
5038	CapSure VDD-2	Transvenous Ventricular Tines	Silicone	MP35N	Porous Platinized/ Steroid	Atr. IS-1 BI, Vent. IS-1 BI

ICD and CRT-D Charge Time Performance

Medtronic continues its commitment to providing updated information on charge time performance.

Introduction

Information on charge time performance of Medtronic is presented in this section of the CRDM Product Performance Report. Medtronic implemented the collection of charge time data on July 1, 1999. The data are collected via our ongoing active clinical study of long-term system performance called the System Longevity Study. The study protocol requests device data be routinely taken and sent to Medtronic at no more than six-month intervals.

In our analysis performed for this report, only charge times resulting from full energy charges are considered. To ensure consistent reporting across devices, the charge time reported at implant represents the last charge time available from date of implant. When more than one charge time is available in a six-month interval, a conservative approach has been adopted whereby only the maximum charge in each 6-month interval is reported. As charge time is directly proportional to the time elapsed since the last capacitor reformation, charges occurring within 15 days of a previous charge are excluded. This precludes the reporting of overly optimistic results.



Data from over 20,000 devices contribute to the charge time data in this report. By tracking and reporting this charge time data, Medtronic is able to ascertain the actual performance of its charging circuitry. The insight gained through this information is applied to Medtronic's ongoing efforts to provide charge times that are short and consistent over the life of the product.

Data Presentation


Charge time data for ICD and CRT-D models are presented using boxplots at 6-month intervals. The shaded box on the plots represents the middle half of the data – the Interquartile Range (IQR). The white line in the middle of each box is the median charge time. The top of the box representing the IQR is the 75th percentile (i.e., 75% of all charge times fall below this line), whereas the bottom of the box represents the 25th percentile. The brackets around the box represent the variance in charge times (analogous to a confidence interval), and are calculated as a function of the median and IQR. Individual values falling outside the brackets are labeled as outliers.

Results


As shown in the graph below, the performance of Medtronic ICD and CRT-D devices has improved. This graph shows the overall maximums, minimums, and medians for Medtronic ICD and CRT-D products, beginning with the 7221 Micro Jewel. A progression toward shorter mean charge times and less variation has occurred between 1996 and 2002. Models released after 2002 have limited experience, but appear to be continuing this performance.

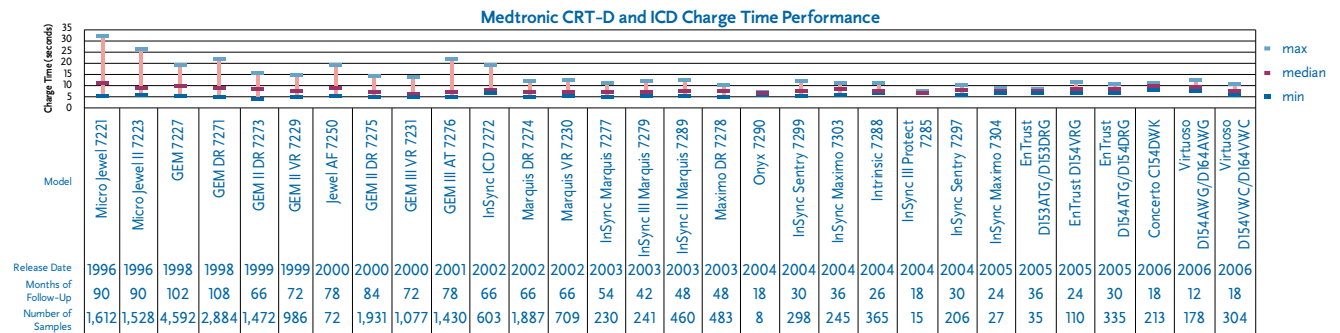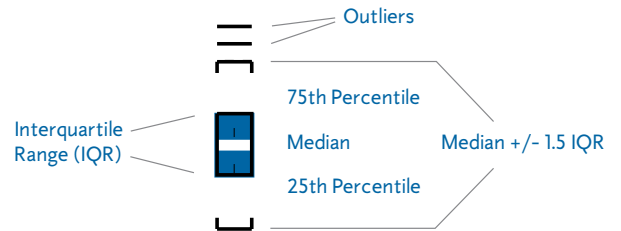


7227 GEM Charge Time

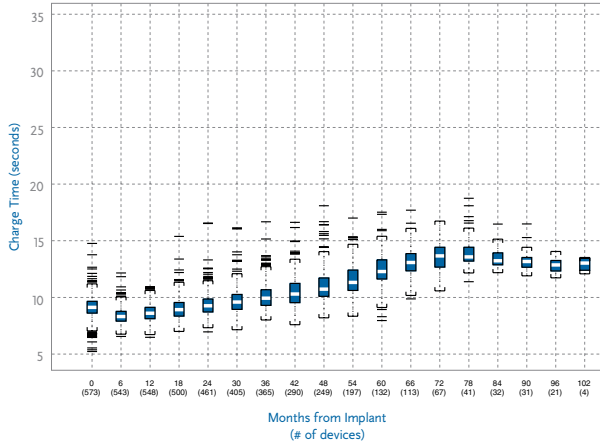


7229 GEM II VR Charge Time

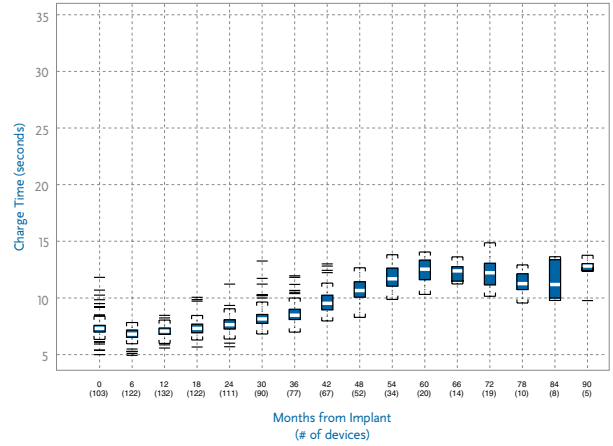


7230 Marquis VR Charge Time

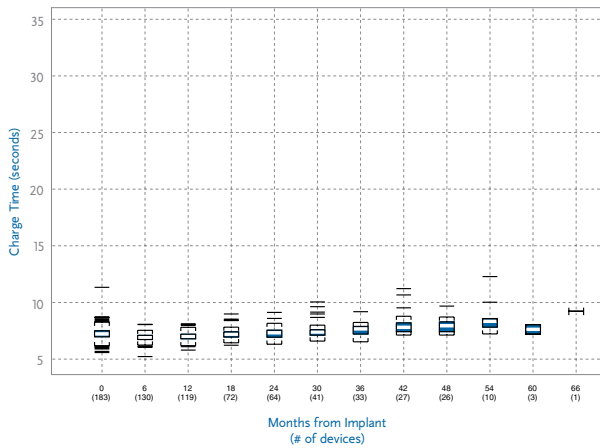


7231 GEM III VR Charge Time

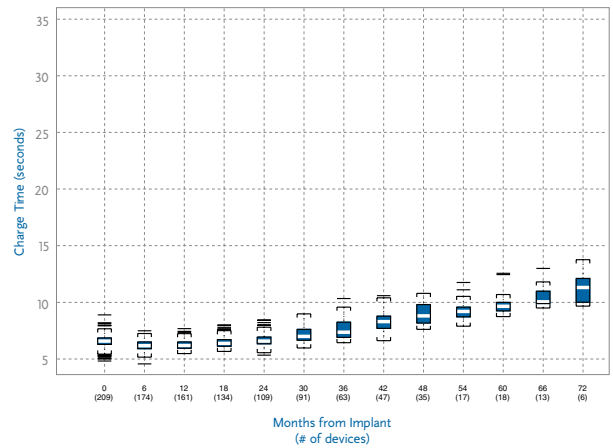

7271 GEM DR Charge Time

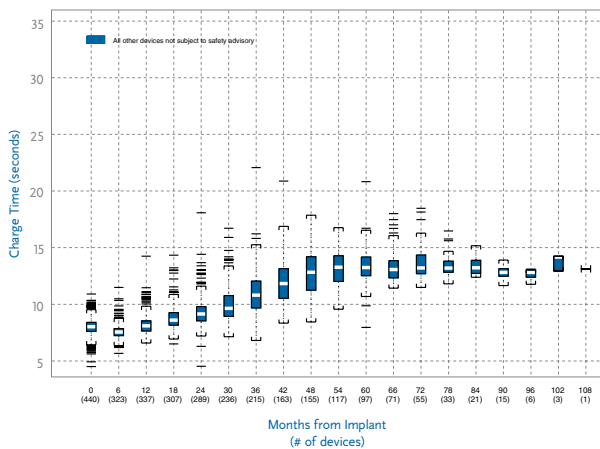


7272 InSync ICD Charge Time

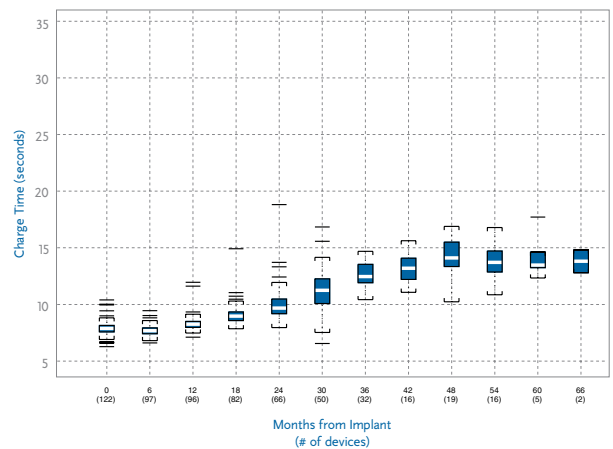


ICD Charge Times

ICD and CRT-D Charge Time Performance continued


7274 Marquis DR Charge Time

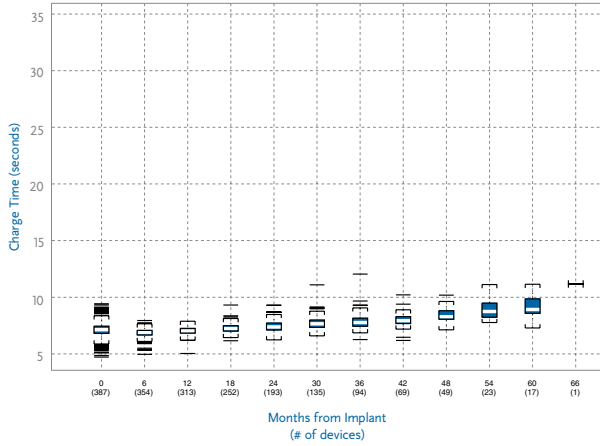


7275 GEM III DR Charge Time

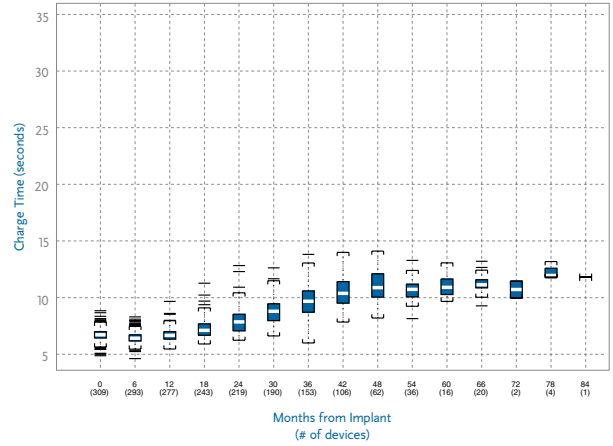


7276 GEM III AT Charge Time

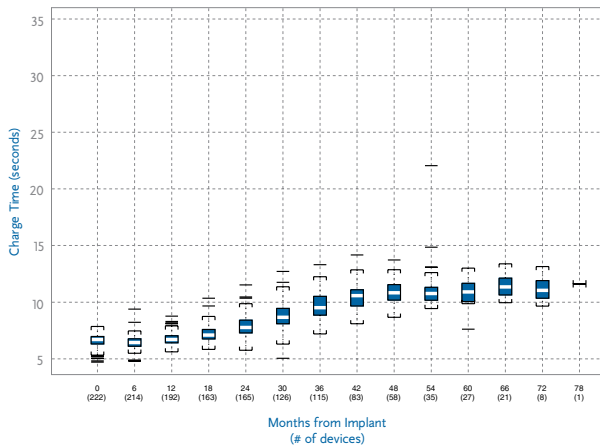


7277 InSync Marquis Charge Time

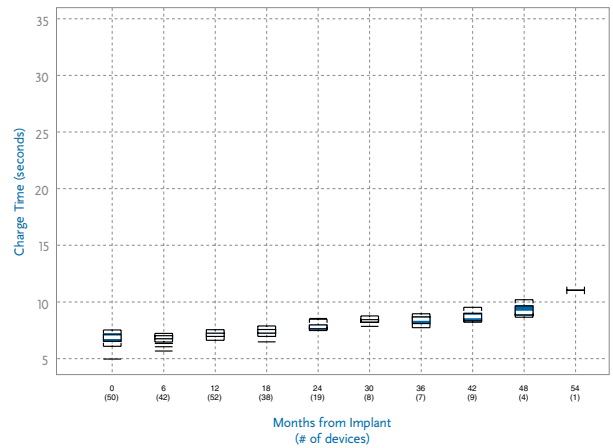

7278 Maximo DR Charge Time

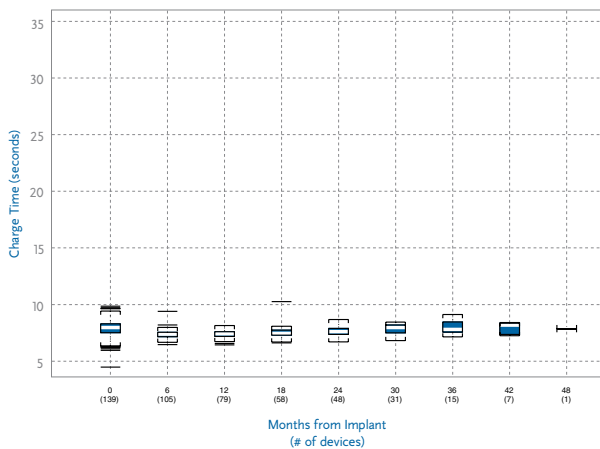


7279 InSync III Marquis Charge Time

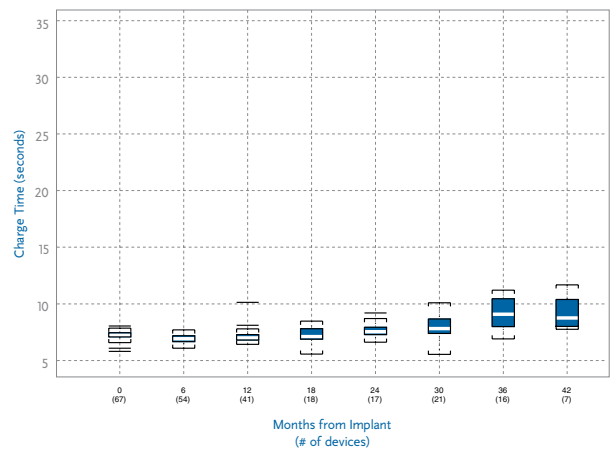


ICD and CRT-D Charge Time Performance continued


7285 InSync III Protect Charge Time

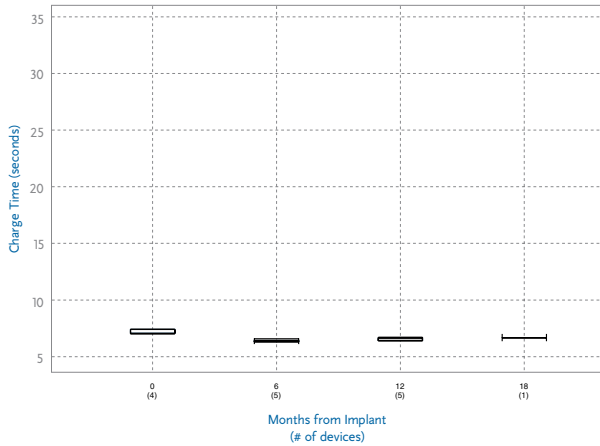


7288 Intrinsic Charge Time

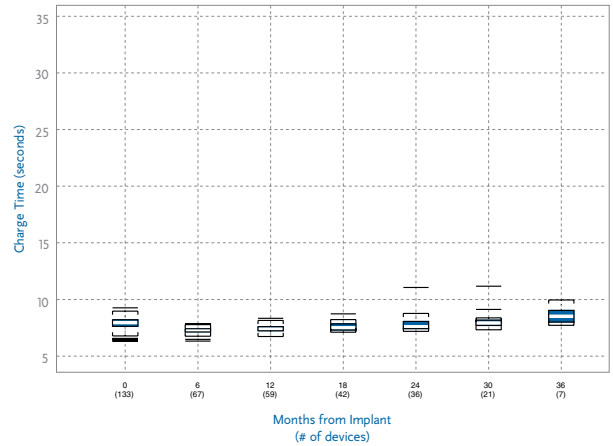


7289 InSync II Marquis Charge Time

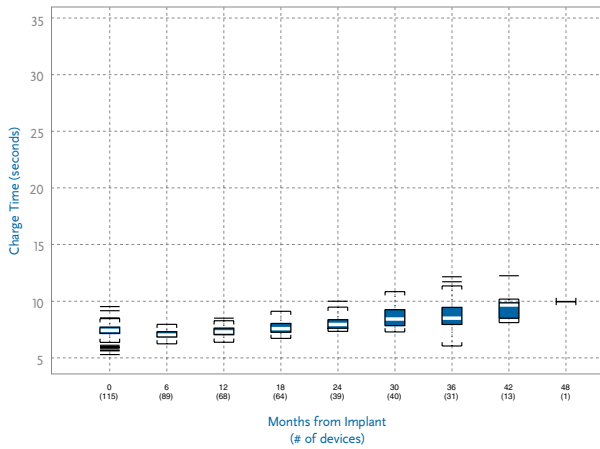


7290 Onyx Charge Time

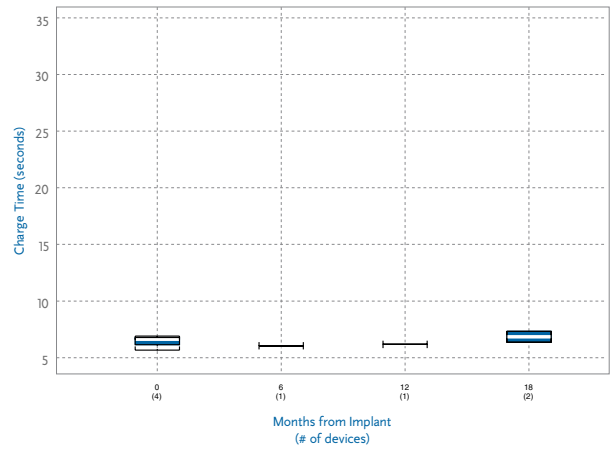

7297 InSync Sentry Charge Time

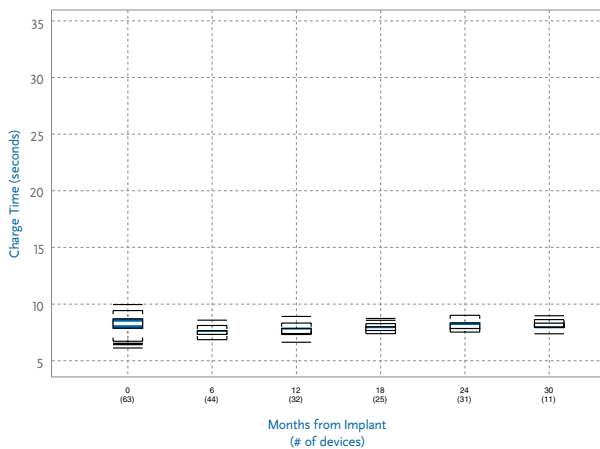


7299 InSync Sentry Charge Time

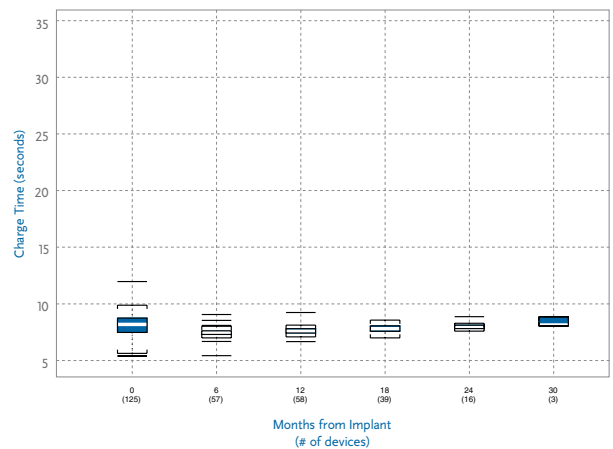


ICD Charge Times

ICD and CRT-D Charge Time Performance continued


7303 InSync Maximo Charge Time

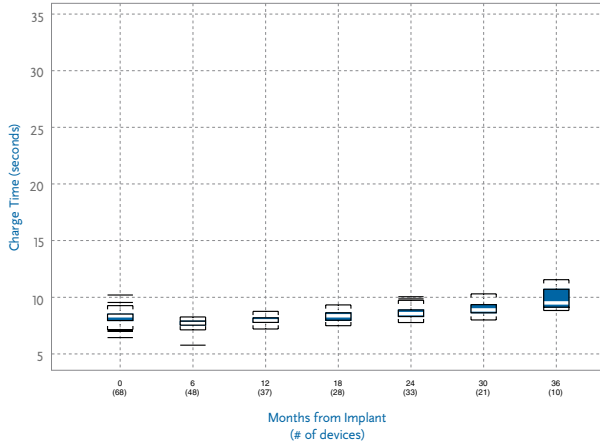


7304 InSync Maximo Charge Time

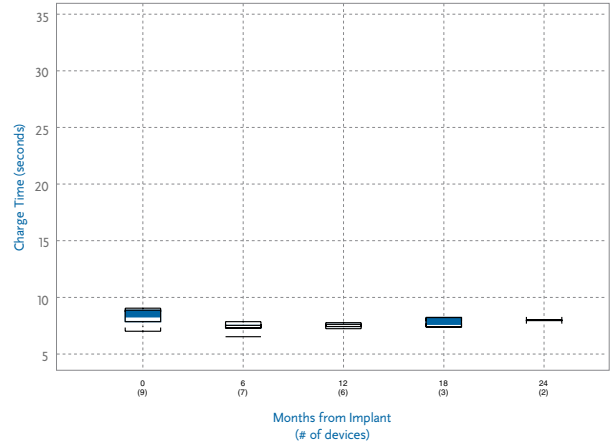


C154DWK Concerto Charge Time

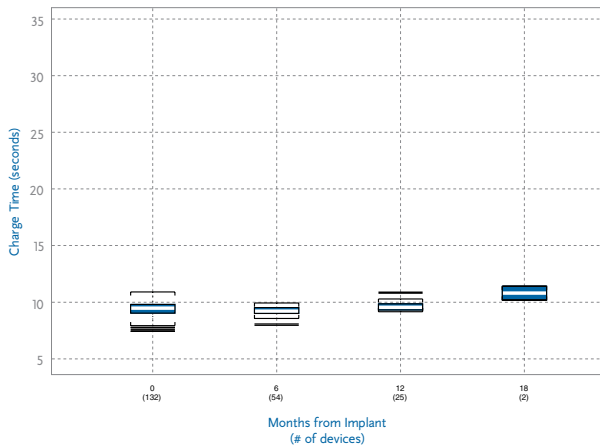


D153ATG, D153DRG EnTrust Charge Time

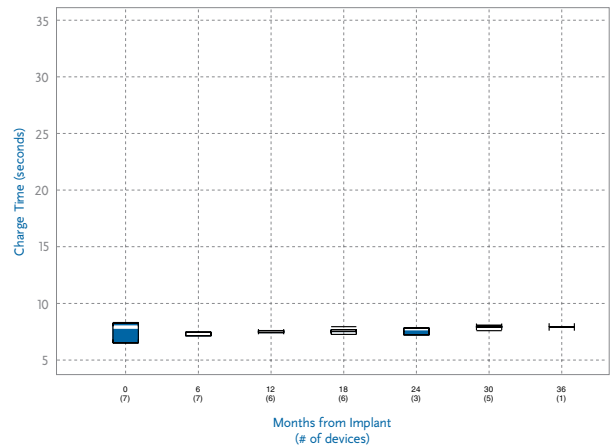

D154ATG, D154DRG EnTrust Charge Time

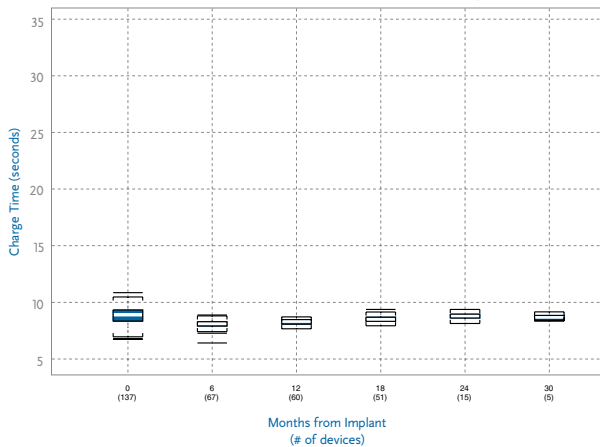


D154VRC EnTrust Charge Time

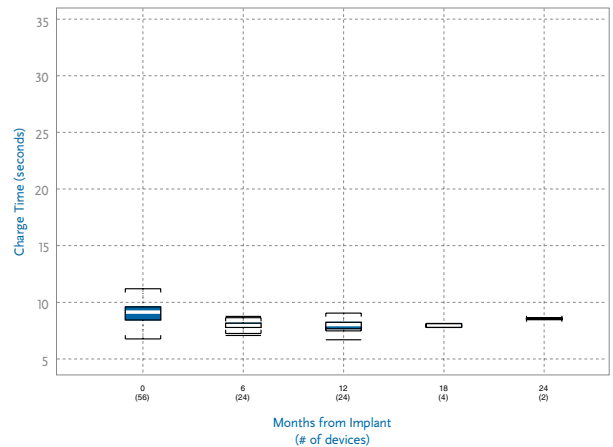


ICD and CRT-D Charge Time Performance continued

D154AWG Virtuoso Charge Time

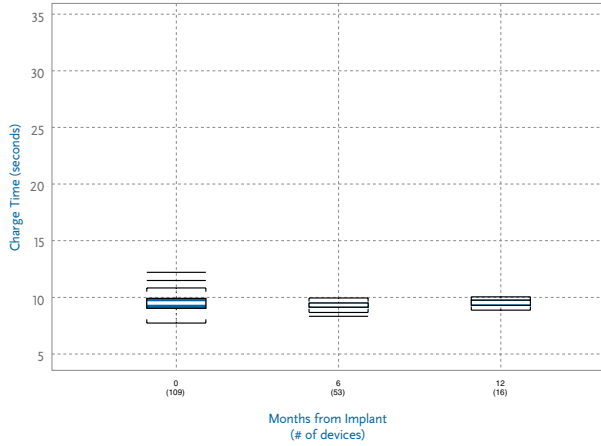

D154VWC Virtuoso Charge Time

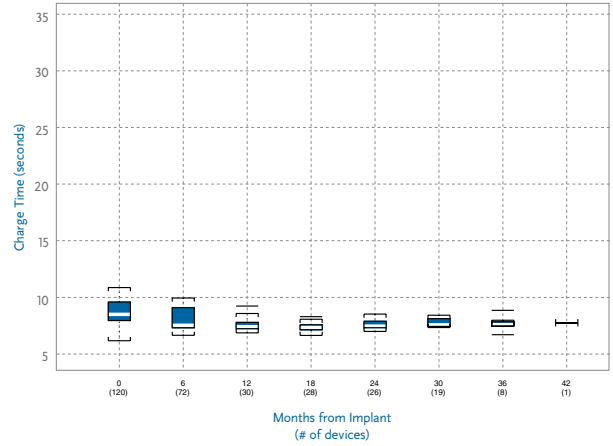

ICD Charge Times

6930, 6931, 6948, 6949 Sprint Fidelis Defibrillation Leads

Original Date of Advisory: October 2007

Potential Conductor Wire Fracture

Product

All Models 6930, 6931, 6948, and 6949 Implantable Defibrillation Leads.

Advisory

There are two primary locations where chronic conductor fractures have occurred on Sprint Fidelis leads: 1) the distal portion of the lead, affecting the anode (ring electrode) and 2) near the anchoring sleeve tie-down, predominantly affecting the cathode (helix tip electrode), and occasionally the high voltage conductor. These two locations account for 90% of the chronic fractures identified in Returned Product Analysis (RPA). The remaining 10% of chronic fractures occurred in the DF-1 connector leg and the proximal portion of the RV coil. High voltage conductor fractures could result in the inability to deliver defibrillation therapy. Anode or cathode conductor fractures (at either location) may present clinically as increased impedance, oversensing, increased interval counts, multiple inappropriate shocks, and/or loss of pacing output.

Patient Management Recommendations

Medtronic recommends you consider the following as part of routine follow-up for each patient.

- To reduce the risk of inappropriate detection and therapy due to oversensing, program VF detection for initial Number of Intervals to Detect (NID) to nominal settings (18/24) or longer at physician discretion and Redetect NID to nominal settings (12/16).
- Turn ON Patient Alert for RV Pacing, RV Defibrillation, and SVC Defibrillation impedance. For Concerto and Virtuoso devices enrolled on the Medtronic CareLink Network, turn ON the Medtronic CareAlert Notifications for these same parameters.
- To optimize effectiveness of the lead impedance alert:
 - Review V Pacing Lead Performance Trend to determine typical chronic impedance value for the patient (typical values for Fidelis leads should be 350-1,000 ohms).
 - Program lead impedance alert threshold for RV Pacing to 1,000 ohms, if the typical chronic impedance for the patient is \leq 700 ohms, or

- Program lead impedance alert threshold for RV Pacing to 1,500 ohms, if the typical chronic impedance for the patient is $>$ 700 ohms.
- Program lead impedance alert threshold for RV Defibrillation and SVC Defibrillation to 100 ohms.

Status Update

Sprint Fidelis lead performance continues to be in line with the information provided in the October 2007 initial advisory communication. After consideration of updated performance information, as well as ongoing reviews by our Independent Physician Quality Panel, **patient management recommendations remain unchanged.**

- The risk of prophylactic intervention appears to be greater than the risk of serious injury resulting from lead fracture even for pacemaker dependent patients, except in select individual patient circumstances as determined by the physician.
- When a lead fracture is suspected or confirmed, we strongly recommend prompt patient attention. Patients should contact their physician without delay if they experience unexpected shocks.
- Implementation of our patient management recommendations is expected to provide two days advance notice prior to inappropriate therapy to 49% of the patients with lead fractures. The remainder will receive less than two days advance notice or no notice. This percentage may vary by implanted device.

Out of the initial implant population of 204,000 in the United States, approximately 167,000 remain implanted. According to System Longevity Study results, lead survival is estimated to be 96.7% at 36 months.

As part of our commitment to keep you informed about Sprint Fidelis lead performance, starting in August 2008, Medtronic will publish the quarterly System Longevity Study's all-cause survival curve for the 6949 lead model at www.medtronic.com/fidelis. Updates will also continue to be provided in this Product Performance Report. Additional information about the Sprint Fidelis lead is available at www.medtronic.com/fidelis.

Sigma Implantable Pulse Generators

Original Date of Advisory: November 2005

Potential Separation of Interconnect Wires

Product

A specific subset of Sigma series pacemakers may fail due to separation of interconnect wires from the hybrid circuit. Specific model and serial numbers of affected devices are available online at <http://SigmaSNList.medtronic.com>.

Advisory

This subset of Sigma series pacemakers that may fail due to separation of interconnect wires from the hybrid circuit may present clinically as loss of rate response, premature battery depletion, intermittent or total loss of telemetry, or no output.

Separation of redundant interconnect wires has been observed on hybrid terminal blocks. Device failure occurs only where both interconnect wires separate from a hybrid terminal block. In October 2005, testing and analysis identified the root cause of these failures and the affected population. Hybrid circuits used in this subset of devices were cleaned during manufacturing with a particular cleaning solvent that could potentially reduce the strength of the interconnect wire bond over time.

Our modeling predicts a failure rate from 0.17% to 0.30% over the remaining lifetime of these pacemakers. No provocative testing can predict which devices may fail.

Patient Management Recommendations

To assist physicians in their patient care and after discussion with physician consultants, Medtronic offers the following recommendations:

- Medtronic does not recommend replacement of these devices prior to normal elective replacement (ERI), based on the low probability of occurrence of a serious event in this population.
- Continue routine follow-up in accordance with standard practice.
- Advise patients to seek attention immediately if they experience return of symptoms (e.g., syncope or light-headedness).
- Determine whether device replacement is warranted on a case-by-case basis based upon consultation with patients, review of the individual

patient's medical history, and consideration of the relative risks of an invasive procedure.

Status Update

The Sigma Family device performance related to the interconnect wires separation mechanism continues to be within Medtronic's engineering projections. As of January 31, 2008, 139 devices out of approximately 40,000 devices worldwide have been confirmed as having experienced interconnect wire separation. Thirty-eight (38) of these devices were returned from the United States. **There have been no confirmed serious injuries or deaths due to this issue.**

Ninety-three (93) of the 139 devices (0.22%) were returned with information indicating a problem with the patient's pacing system prior to explant. The remaining 46 devices (0.11%) were returned with no information indicating a potential malfunction while implanted or with insufficient information to determine the state of the device at explant. Lacking definite information indicating proper operation until explant, these devices are conservatively categorized as having experienced interconnect wire separation while implanted.

Implant duration for the 139 devices confirmed as having experienced interconnect wire separation has ranged between 17 and 68 months, with an average of 50 months.

Out of the initial advisory population of 40,000 worldwide, approximately 19,200 remain implanted. Approximately 4,500 of these are in the United States.

The Patient Management Recommendations set forth in the advisory remain unchanged.

7274 Marquis DR
7230 Marquis VR

7278 Maximo DR
7232 Maximo VR

7277 InSync Marquis
7289 InSync II Marquis

7279 InSync III Marquis
7285 InSync III Protect

Original Date of Advisory: February 2005

Potential Premature Battery Depletion Due to Battery Short

Product

The specific subset of Marquis family ICD and CRT-D devices having batteries manufactured prior to December 2003 is affected. Devices manufactured with batteries produced after December 2003 are not affected. Specific model and serial numbers of affected devices are available online at <http://MarquisSNList.medtronic.com>.

Advisory

Medtronic Marquis family of ICD and CRT-D devices having batteries manufactured prior to December 2003 may experience rapid battery depletion due to a specific internal battery short mechanism. Battery design changes were implemented in December 2003 that eliminate the possibility of this internal shorting mechanism.

Highly accelerated bench testing indicated the rate of this shorting mechanism may increase as the battery is depleted. As of February 2005, the rate of shorting was approximately 1 in 10,000 (0.01%); bench test data indicated the rate may increase to between 0.2% and 1.5% over the second half of device life.

No provocative testing can predict which of these devices will experience this issue. Once a short occurs, battery depletion can take place within a few hours to a few days. After depletion the device ceases to function. It is also possible that as the battery depletes quickly, patients may experience temporary warmth in the area surrounding the ICD.

Patient Management Recommendations

We recommend you consider the following patient management options:

- Conduct quarterly (i.e., every three months) follow-up procedures.
- Inform patients that should they experience warmth in the area surrounding the ICD to seek follow-up care promptly.
- Program Low Battery Voltage ERI Patient Alert to "On-High." This will result in an audible, alternating tone in the limited circumstances where a battery depletes slowly over a number of days. Data indicates most shorts will occur rapidly and will not be detected by this feature.

- Provide a hand-held magnet to patients to check device status and program the Low Battery Voltage ERI Patient Alert to "On-High." Device operation may be monitored periodically (e.g., daily) by patients placing the magnet over the device for 1-2 seconds. If the device is functional, a steady tone will sound for approximately 20 seconds. If no tone is heard, follow-up care should be sought promptly.

Status Update

The Marquis Family device performance related to the battery shorting mechanism continues to be within Medtronic's engineering projections. As of January 31, 2008, 93 Marquis Family devices have been confirmed as having this internal battery shorting mechanism. Fifty-two (52) of these devices were returned from the United States. **There have been no confirmed serious injuries or deaths due to this issue.**

Of the 93 returns, 33 have been identified by patients reporting warmth in the ICD pocket, 37 by a regularly scheduled follow-up or during a nondevice related hospital visit, 12 by hand-held magnet test or CareLink attempt, 7 by return of bradycardia symptoms, and 4 by the Patient Alert sounding.

Implant duration for the 93 devices ranged between 11 to 53 months, with an average of 34 months.

Consistent with Medtronic projections, the observed rate of shorting is higher in the second half of device life than in the first half of device life. Of the devices that have exhibited shorting in the last half of device life, 46% occurred in the last quarter of device life and 30% in the last 10% of device life.

Out of the initial advisory population of 87,000 worldwide, approximately 29,900 remain implanted. Approximately 26,300 of these are in the United States.

The Patient Management Recommendations set forth in the advisory remain unchanged.

Warranty

All Marquis devices are subject to a Limited Warranty. Devices returned to Medtronic and determined to be malfunctioning will be replaced or credited in accordance with the warranty terms. In addition, for devices subject to the Marquis advisory, should a physician decide to replace a device for a patient who is pacemaker dependent or who receives frequent VT/VF therapy, Medtronic will, upon receipt of a written statement from the physician setting forth the basis for early replacement of the device, provide a replacement device at no cost.

Kappa 600, 700 Dual Chamber (D, DR, and VDD) IPGs

Original Date of Advisory: March 15, 2002

Potential Fractured Power Supply Wires

Product

A specific subset of Kappa 700/600 Dual Chamber (D, DR, and VDD) Implantable Pulse Generators have been identified by serial numbers. Hospitals and Physicians were notified. Specific model and serial numbers of affected devices are available by calling US Technical Services at 1 (800) 505-4636.

Advisory

As of March 15, 2002, Medtronic observed 53 related failures (0.02%) in over 255,000 Kappa 700/600 Dual Chamber (D, DR, and VDD) Series devices sold worldwide. Medtronic voluntarily communicated this information to physicians because these failures had been observed in patients having submuscular implants.

These devices have presented with an electrical reset, intermittent output, or no output. Our investigation identified the root cause as fractured wires supplying power to the pacemaker. This has been directly correlated to submuscular placement of these devices. Submuscular implant locations (e.g., subpectoral, abdominal, etc.) can result in additional stress and repetitive flexing on the implanted device causing excessive fatigue on these wires. Of the estimated 4,000 devices implanted submuscular, approximately 200 (5%) may experience this failure. These stresses on the implanted device are unique to submuscular implant sites and do not exist with subcutaneous implants.

Patient Management Recommendations

While there is no provocative testing or time dependency that will predict which submuscular placed device will fail, certain electrical resets may be an indicator that a wire fracture has occurred. Normal electrical resets can occur as a result of electrosurgical procedures such as cautery and ablation or from defibrillation therapy. If none of the normal causes of electrical reset can be confirmed, or if a device serial number presents as "000000" following an electrical reset, this may be an indicator of a wire fracture.

For patients who have submuscular implants of devices within the designated serial number range and who are pacemaker dependent with no underlying rhythm, replacement of the device should be considered. Medtronic will provide the replacement device free-of-charge under the terms of its warranty program if a device is replaced in these patients.

For patients having subcutaneous implants, no change to your current patient care and follow-up is advised.

Status

Device performance related to this advisory continues to be within Medtronic's engineering projections. Patient management recommendations remain unchanged. As of January 31, 2008, 286 out of approximately 180,000 (0.16% incidence) Kappa family devices worldwide have been confirmed as having fractured power supply wires. One hundred forty-four (144) of these devices were returned from the United States. Out of the initial implant population of 121,000 in the United States, approximately 41,000 remain implanted.

7227Cx GEM 7229Cx GEM II VR

Original Date of Advisory: October 15, 1999

Potential Circuit Overload

Product

Model 7227Cx and Model 7229Cx Implantable Cardioverter Defibrillators supplied before October 15, 1999, with serial numbers ending in an "H." For example, PIPxxxxxxH or PJJxxxxxxH, where x is a variable numeric, may be affected. Specific model and serial numbers of affected devices are available by calling US Technical Services at 1 (800) 723-4636.

IMPORTANT REMINDER:

Medtronic strongly advises physicians who have patients under their care affected by this issue to reprogram the Patient Alert feature "ON" without delay.

Advisory

Manufacturing error in a small percentage of devices may cause circuit overload when $AX \geq B$ High Voltage energy is delivered via an integrated bipolar lead. GEM Model 7227Cx and GEM II VR Model 7229Cx devices with dedicated bipolar sensing leads are not affected by this issue. Devices affected may not be able to subsequently charge to full energy and experience "charge circuit timeout."

Patient Management Recommendations

- Assessment of all patients with the potentially affected devices implanted **AND** an integrated bipolar ICD lead such as the 6942 and 6945 should take place without delay.
- Reprogram polarity pathway to $B \geq AX$ for all cardioversion and defibrillation therapies.
- Confirm correct device function:
 - Perform a full energy charging sequence.
 - If "charge circuit timeout" is observed, contact your Medtronic representative.
 - If device charges normally, it has not been damaged and will function appropriately with polarity programmed $B \geq AX$.

Recent studies have demonstrated that DFTs are similar or lower in a $B \geq AX$ polarity pathway when compared to $AX \geq B$.

Devices implanted with functional dedicated bipolar leads such as the 6932, 6934S, 6936, 6943, and 6966 are not affected.

Status

Device performance related to this advisory continues to be within Medtronic's engineering projections. Patient management recommendations remain unchanged. Out of the initial implant population of 10,000 in the United States, approximately 2,000 remain implanted. The devices affected by this advisory are nearing the end of their expected battery longevity.

4504, 4504M CapSure Atrial Lead

4582 Target Tip Atrial Lead

Original Date of Advisory: October 4, 1996

Lead Survival Below Expectations

Product

All Models 4504, 4504M, and 4582 Implantable Pacing Leads

Advisory

Lead survival probability is below expectations and is primarily associated with insulation degradation due to Metal Ion Oxidation (MIO).

Patient Management Recommendations

- Follow patients in accordance with Medicare Guidelines.
- Avoid the use of the AAI or AOO mode.
- During patient evaluation, give careful attention to lead performance such as:
 - Review patient ECG for indications of transient sensing and/or capture abnormalities.
 - Monitor in clinic for impedance less than 250 ohms or a decrease of more than 30% from implant values (or an established baseline using telemetry) which would suggest lead failure.
- Consider the use of unipolar if the pulse generator has this capability.
- At the time of pacemaker system revision (e.g., normal pulse generator or ventricular lead revision), carefully evaluate lead integrity and patient status before choosing to reuse.

Status

Patient management recommendations remain unchanged. Laboratory analysis trends and engineering conclusions remain unchanged.

Out of the initial implant population of 16,600 in the United States, approximately 1,500 remain implanted. According to System Longevity Study results, lead survival is estimated to be 66.1% at 8 years, 9 months.

4004, 4004M CapSure Ventricular Lead 4082 Target Tip Ventricular Lead

Original Date of Advisory: October 8, 1993

Lead Survival Below Expectations

Product

All Models 4004/4004M and 4082 Implantable Pacing Leads

Advisory

Lead survival probability is below expectations due primarily to polyurethane insulation failure (MIO) and conductor fracture (associated with “subclavian crush”).

Patient Management Recommendations

- Increase, as appropriate, the frequency of patient evaluation through in-clinic visits supplemented with transtelephonic and/or ambulatory monitoring; for example, consistent with Guideline I under Medicare Pacemaker Monitoring Guidelines (50-1 Cardiac Pacemaker Evaluation Services).
- During patient evaluations, give careful attention to lead performance such as:
 - Reviewing patient ECGs carefully for indications of transient sensing and/or capture abnormalities.
 - Monitoring in-clinic for impedances less than 300 ohms or a decrease of more than 30% from implant values (or an established baseline using telemetry) which would suggest lead failure.
 - Eliciting and thoroughly investigating any patient complaints suggestive of lead failure.
- Consider whether prophylactic replacement would be appropriate, especially in patients at high risk, such as pacemaker dependent patients.
- Carefully evaluate lead integrity when performing routine pulse generator replacements. Replace lead if
 - insulation breaches are observed.
 - lead impedance is less than 300 ohms or has decreased by more than 30% from implant values.
 - impedance or voltage threshold measurements vary significantly when multiple readings are taken.
 - if the risk of continued use outweighs the risk associated with implanting a new lead.
- As always, individual circumstances and medical judgment dictate patient care and frequency of follow-up.
- Consider lead replacement during normal pulse generator change-out. Carefully evaluate lead integrity and patient status before choosing to reuse.

Status

Patient management recommendations remain unchanged. Laboratory analysis trends and engineering conclusions remain unchanged.

Out of the initial implant population of 77,000 in the United States, approximately 2,900 remain implanted. According to System Longevity Study results, lead survival is 50.6% at 10 years, 9 months.

4012 Target Tip Ventricular Lead

Original Date of Advisory: September 26, 1991

Lead Survival Below Expectations

Product

All Model 4012 Implantable Pacing Leads

Advisory

Lead survival probability beyond 5 years is below expectations due primarily to polyurethane insulation failure (due to ESC and/or MIO) and conductor fracture (associated with “subclavian crush”).

Patient Management Recommendations

Consider increasing frequency of monitoring (e.g., from quarterly to bimonthly or monthly). Consider the following activities as part of normal follow-up procedures:

- Monitor for significant changes in impedance which could be an indication of impending failure (pulse generator must have impedance telemetry capabilities).
- Review patient ECGs carefully for indications of transient sensing and/or capture abnormalities. This can be done using transtelephonic or in-clinic monitoring and/or using ambulatory monitoring.
- Elicit any patient complaints suggestive of lead failure and investigate thoroughly lead integrity/performance characteristics following reports of patient complaints or symptoms using the above techniques.

- Consider whether prophylactic replacement would be appropriate in patients at high risk, such as pacemaker dependent patients.
- Evaluate carefully the integrity of the lead during routine pulse generator replacement before choosing to reuse. Specifically, Medtronic recommends placement of a new lead if:
 - insulation breaches are observed.
 - lead impedance is less than 300 ohms or has decreased by more than 30% from implant values.
 - electrical properties such as impedance and threshold vary significantly when multiple readings are taken.

As always, medical judgment must be used to establish the appropriate schedule and course of care for every individual, particularly pacemaker dependent or other patients at higher risk.

Status

Patient management recommendations remain unchanged. Laboratory analysis trends and engineering conclusions remain unchanged.

Out of the initial implant population of 96,800 in the United States, approximately 5,300 remain implanted. The System Longevity Study results show 62.2% lead survival at 15 years, 9 months.

Minix, Minix ST, Micro Minix IPGs

Original Date of Advisory: May 6, 1991

Potential Delayed Restoration of Permanent Settings

Product

All Models of the Minix, Minix ST, and Micro Minix families of Implantable Pulse Generators

Advisory

Possibility of delayed restoration of permanent pacing mode and parameters, after the magnet or programming head is removed under certain conditions.

Patient Management Recommendations

To eliminate any potential risk associated with temporary programming, depress the INTERROGATE KEY and verify successful interrogation before moving the programming head away from the pulse generator. The delay condition can also be terminated by repositioning the programming head and depressing the EMERGENCY VVI key.

Status

Device performance related to this advisory continues to be within Medtronic's engineering projections. Patient management recommendations remain unchanged. Out of the initial implant population of 65,000 in the United States, approximately 4,000 remain implanted. The devices affected by this advisory are nearing the end of their expected longevity.

Performance Notes

Ensuring the Accuracy of Battery Longevity Estimates

Purpose of this Information

This article is intended to help the clinician understand how Medtronic estimates CRT-D, ICD, and IPG device longevity and Medtronic's performance against these estimates.

Device Longevity and Battery Depletion

The device service life ends when the usable battery capacity is depleted. The time to battery depletion depends on three factors:

- the amount of electrical energy expended in providing therapy to the patient
- the amount of energy consumed by the electronic circuitry to perform the functions of the device (e.g., operating the microprocessor, telemetry, memory, and charging component)
- the energy capacity of the battery

Medtronic has developed a statistical model for device longevity that accounts for each of these factors, and has validated the model with real time clinical performance. During the development of its products, Medtronic engineers characterize device longevity using this model. Testing begins during development and continues after market release to ensure the accuracy of device longevity estimates.


Using Survival Curves to Assess Longevity

The survival curves in the Product Performance Report represent the composite experience of thousands of devices over a wide range of programming options and patient use conditions. While the curves are useful for understanding the overall performance of a population of devices, they cannot be used to accurately predict the longevity of a specific device in a specific patient. To get a longevity prediction for a specific device, the longevity model must be used. The model is available by contacting Medtronic's Technical Services Department.

Because the survival curves are an aggregate result, the Reference pages in the Product Performance Report include several longevity estimates for a range of use conditions. These longevity estimates, originally published in the device Technical Manual, are mean values calculated for the parameters given. This range of longevity estimates can be compared to the survival curve including normal battery depletion to assess the overall clinical performance of a device model against the original longevity estimates.

If most of a device model's population is being used at nominal parameters and conditions, the time at which the survival curve including normal battery depletion equals 50% should approximate the midpoint in the range of longevity estimates.

If devices tend to be used at conditions that consume more or less energy than nominal, then the time at which the survival curve equals 50% should tend toward the lower or higher end of the range of longevity estimates, respectively.

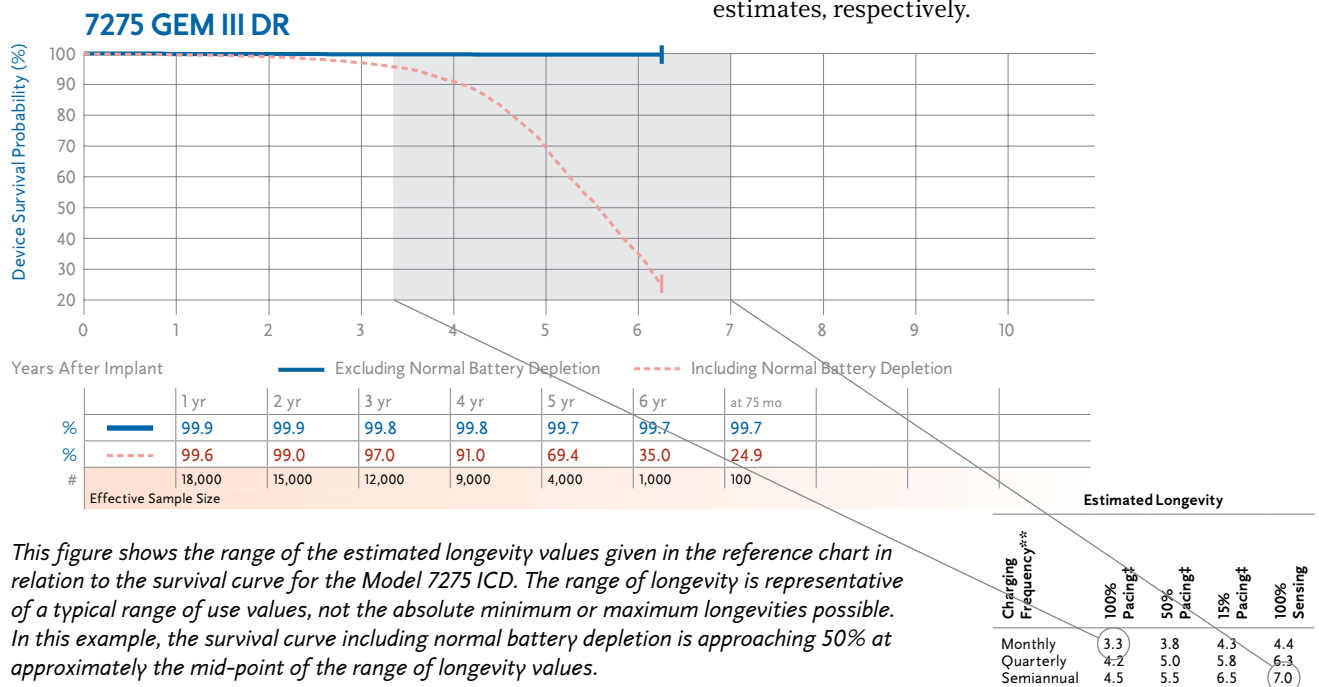

This figure shows the range of the estimated longevity values given in the reference chart in relation to the survival curve for the Model 7275 ICD. The range of longevity is representative of a typical range of use values, not the absolute minimum or maximum longevity possible. In this example, the survival curve including normal battery depletion is approaching 50% at approximately the mid-point of the range of longevity values.

Interactions between Cardiac Pacing and Ventricular Arrhythmia Initiation.

Purpose of this Information

This article is intended to provide information for consideration when programming pacemaker operation in ICDs and pacemakers.

Background

Right ventricular pacing has been associated with increased risk of appropriate therapy for ventricular tachycardia (VT) and ventricular fibrillation (VF) in ICD patients.¹ Abrupt changes in ventricular cycle lengths (short-long-short, S-L-S) may precede initiation of VT/VF in some instances. S-L-S sequences may be permitted in all forms of cardiac pacing. The pause lengths depend upon pacing mode and lower rate programming.²⁻⁴ Because pauses may be associated with VT/VF initiation, pause suppression algorithms have been developed in ICDs. Although pause suppression may have utility in specific patients with repolarization abnormalities and pause dependent VT, it has not been shown to reduce arrhythmia incidence in the general ICD population.⁵ Conversely, S-L-S sequences may occur with ventricular pacing in a variety of ways, including atrial tracking of premature atrial contractions (PACs) or by terminating pauses with ventricular paced beats.⁶ In some patients, the ectopic depolarization pattern of a ventricular paced beat may be pro-arrhythmic, independent of pause timing. These observations have further enforced the desire to reduce unnecessary ventricular pacing.

Clinical Trial Observations

Medtronic-sponsored clinical trials were retrospectively analyzed to further understand pause-mediated (i.e., S-L-S) scenarios prior to VT/VF. S-L-S onset scenarios were observed in a minority of patients in all pacing modes. Pacemaker interactions prior to VT/VF are dependent on patient conditions, as well as the technical aspects of pacing operation (i.e., pacing mode, lower rate and AV interval). Because a very low frequency of ventricular pacing is observed during Managed Ventricular Pacing (MVP)⁷⁻⁹ or VVI 40 pacing modes,¹⁰ the long interval tended to terminate with a ventricular sense. In DDD mode, the long interval tended to be terminated by a ventricular pace. Long intervals of > 1000 ms prior to VT/VF were rare in MVP mode. In these analyses, only an association between cardiac pacing and VT/VF initiation can be observed, causality cannot be established. The ongoing MVP (Managed Ventricular Pacing vs. VVI 40 Pacing) Trial, a 2-year, 1000-patient prospective, randomized trial in ICD patients may offer more insight into the frequency of VT/VF across pacing modes.¹¹

Pacemaker Patients

In pacemaker patients, ventricular pacing has been associated with higher incidence of AT/AF and heart failure hospitalization.^{12,13} MVP provides atrial rate support while dramatically reducing ventricular pacing in patients with sinus node dysfunction and transient AV block.⁹ However, as stated in Medtronic reference manuals, depending upon the patient's intrinsic rhythm and conduction, MVP may allow ventricular cycle variation and occasional pauses of up to twice the lower rate.

DDD pacing with long AV intervals may reduce ventricular pacing and may decrease the potential length of pauses compared to MVP. However, DDD with long AV interval programming does not appear to be as effective as AAI-based pacing modes at reducing ventricular pacing,^{13,14} may lead to endless loop tachycardia,^{14,15} and does not completely eliminate pauses. Also, in DDD mode, a higher programmed lower rate or activation of rate response can lead to an increase in AV conduction times and a higher percentage of ventricular pacing. The potential benefits of reducing ventricular pacing must be weighed against the potential for longer ventricular pauses. Therefore, careful consideration should be given to pacemaker mode and lower rate programming, particularly in the setting of frequent AV block and repolarization abnormalities due to congenital Long QT, electrolyte imbalances, and some medications which prolong QT.

Conclusion

Pacemaker operation may interact with VT/VF initiation in a variety of ways. The patient's heart failure status, arrhythmia substrate, medications, and the relative importance of maintaining ventricular synchrony vs. ensuring ventricular rate support must be weighed when choosing optimal hardware (ICD vs. pacemaker) and pacemaker programming (pacing mode, lower rate, etc.).

References

- Steinberg JS, Fischer A, Wang P, et al. The clinical implications of cumulative right ventricular pacing in the Multicenter Automatic Defibrillator Trial II. *J Cardiovasc Electrophysiol*. April 2005;16(4):359-365.
- Pinski SL, Eguia LE, Trohman RG. What is the minimal pacing rate that prevents Torsades de Pointes? Insights from patients with permanent pacemakers. *PACE*. November 2002; 25(11):1612-1615.
- Goldman DS, Levine PA. Pacemaker-mediated polymorphic ventricular tachycardia. *PACE*. October 1998; 21(10):1993-1995.
- Gray CJ, Basta M, Sapp JL, Parkash R, Gardner MJ. Inappropriate application of managed ventricular pacing in a patient with Brugada syndrome leading to polymorphic ventricular tachycardia, ventricular fibrillation and implantable cardioverter defibrillator shocks. *Heart Rhythm*. 2006, Abstract P1-89.
- Friedman PA, Jalal S, Kaufman S, et al. Effects of a rate smoothing algorithm for prevention of ventricular arrhythmias: results of the Ventricular Arrhythmia Suppression Trial (VAST). *Heart Rhythm*. May 2006;3(5):573-580.
- Himmrich E, Przbille O, Zellerhoff C, et al. Proarrhythmic effect of pacemaker stimulation in patients with implanted cardioverter-defibrillators. *Circulation*. July 15, 2003;108(2):192-197.
- Sweeney MO, Ellenbogen KA, Casavant D, et al. Multicenter, prospective, randomized trial of a new atrial-based Managed Ventricular Pacing Mode (MVP) in dual chamber ICDs. *J Cardiovasc Electrophysiol*. 2005;16:1-7.
- Sweeney MO, Shea JB, Fox V, et al. Randomized pilot study of a new atrial-based minimal ventricular pacing mode in dual-chamber implantable cardioverter-defibrillators. *Heart Rhythm*. July 2004;1(2):160-167.
- Gillis AM, Purerfellner H, Israel CW, et al. Reducing unnecessary right ventricular pacing with the managed ventricular pacing mode in patients with sinus node disease and AV block. *PACE*. July 2006; 29(7):697-705.
- The DAVID Trial Investigators. Dual-chamber pacing or ventricular backup pacing in patients with an implantable defibrillator: the Dual Chamber and VVI Implantable Defibrillator (DAVID) Trial. *JAMA*. December 25, 2002;288(24):3115-3123.
- Sweeney MO, Ellenbogen KA, Whellan D, et al. The Managed Ventricular Pacing vs. VVI 40 Pacing (MVP) Trial: Clinical Background, Rationale, Design and Implementation. *J Cardiovasc Electrophysiol*. 2006 (In Press).
- Sweeney MO, Hellkamp AS, Ellenbogen KA, et al. Adverse effect of ventricular pacing on heart failure and atrial fibrillation among patients with normal baseline QRS duration in a clinical trial of pacemaker therapy for sinus node dysfunction. *Circulation*. June 17, 2003;107(23):2932-2937.
- Nielsen JC, Kristensen L, Andersen HR, et al. A randomized comparison of atrial and dual-chamber pacing in 177 consecutive patients with sick sinus syndrome: echocardiographic and clinical outcome. *J Am Coll Cardiol*. August 20, 2003;42(4):614-623.
- Nielsen JC, Pedersen AK, Mortensen PT, Andersen HR. Programming a fixed long atrioventricular delay is not effective in preventing ventricular pacing in patients with sick sinus syndrome. *Europace*. April 1999; 1(2):113-120.
- Dennis MJ, Sparks PB. Pacemaker mediated tachycardia as a complication of the autointinsic conduction search function. *PACE*. June 2004;27(6 Pt 1):824-826.

AT500 Pacing System Follow-Up Protocol

Purpose of this Information

This article is intended to provide clinical guidance regarding follow-up practice and patient management when the AT500 battery voltage approaches the Elective Replacement Indicator (ERI) level of 2.6 volts.

Background

Many AT500 pacing systems are now reaching their ERI voltage level (2.6 volts). This is expected since the battery used has an approximate longevity of 5-6 years under normal conditions (100% DDD pacing, 3 volts, 0.4 ms).

Technical Services has received reports of battery voltage levels below End-of-Life (EOL of 2.2 volts) where EGM pre-storage is programmed ON, or higher outputs and/or pacing rates are necessary. It is important for physicians and allied professionals to understand battery depletion characteristics between ERI and EOL so that they, in turn, can understand how this affects management of follow-up visits for the AT500 as this device nears the end of its expected longevity.

AT500 Battery and Longevity Information

In contrast to other IPGs, the AT500 does not change its mode, stimulation rate, or any other parameter when the battery voltage drops below the ERI level of 2.6 volts (with or without magnet applied). The Threshold Margin Test (TMT) is also not available.

Therefore, it is not possible to perform trans-telephonic assessment of AT500 battery status. This must be done during an in-clinic follow-up session. A warning will be displayed on the Quick Look screen at the beginning of a programmer (follow-up) session when the ERI battery level

occurs. The measured battery voltage will also appear on the programmer display and on printouts.

Battery depletion curves at **common parameter settings** are shown in Figure 1, with special focus on device longevity when programming EGM pre-storage ON or OFF.

Medtronic's review of ongoing AT500 battery life test data matches our original longevity modeling and so meets our expectations. However, when using longer durations between follow-up periods (> 3 months), clinicians should consider the following in setting their remaining longevity expectations.

- Enabling the "EGM Pre-storage On" capability will increase current and reduce device longevity by approximately 9 days for each month pre-storage is ON.
- Longevity decreases with an increase in pacing rate, an increase in pacing amplitude or pulse width, a decrease in pacing impedance, a higher ratio of paced to sensed events, or extended use of the Atrial Preference Pacing, EGM pre-storage, or Holter Telemetry features.

Recommendations

Follow-up frequency should always be accelerated as devices reach ERI voltage levels to ensure device explant/replacement occurs prior to End-of-Life voltage levels. With the wide variety of follow-up schedules being used, Medtronic recommends a 3-month follow-up frequency for the AT500 pacing systems. This is particularly important for patients in whom EGM pre-storage is programmed ON, or higher outputs and/or pacing rates are necessary.

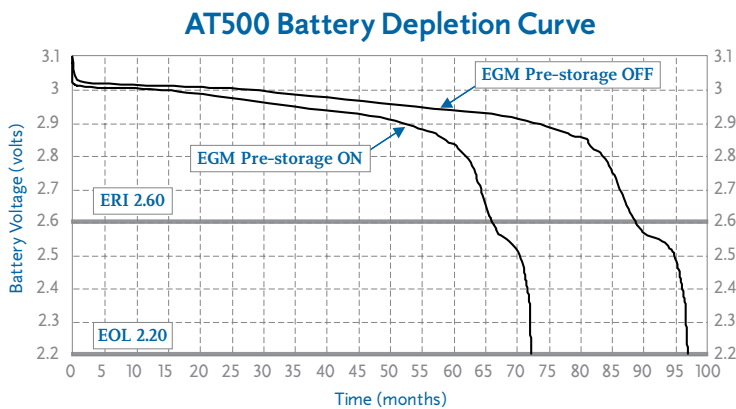


Figure 1
AT500 battery depletion curve for common parameter settings of DDDR, LR 70 ppm, UR 120 ppm, 100% pacing, Atrial – 2 V, 0.4 ms, 600 ohms, Ventricle – 2 V, 0.6 ms, 900 ohms, and EGM Pre-storage ON versus OFF.

Insertion of the Lead into the Device

The implantable system consists of a pulse generator and at least 1 lead. The system operation depends on proper electrical and mechanical operation. With the advent of internationally recognized connector standards the challenge of ensuring proper mechanical fit between the lead and device connectors has been simplified, although the international connector standard does not address all aspects of the procedure for connecting a lead to the device.

If the lead connector is not fully installed, oversensing may result as described in the connector problems section of the technical article, "Clinical Management of High Voltage Lead System Oversensing."

Performing the following steps can be used for each lead connection during the implant procedure.


- 1 Insert the torque wrench into the appropriate setscrew. For easier lead insertion, insert the lead closest to the device first.

- 2 Look down the connector port to verify that the port is not obstructed. If the port is obstructed, retract the setscrew to clear the bore. Take care not to disengage the setscrew from the connector block.
- 3 Push the lead into the connector port until the lead pin is clearly visible beyond the setscrew block.
- 4 Hold the lead in position while tightening the setscrew until the torque wrench clicks.
- 5 Tug gently on the lead to confirm a secure fit.


Current publications may provide additional information on implant procedures used by others, e.g., radiographic evaluation of the terminal pin beyond the terminal post.¹

¹Pickett RA III, Saavedra P, Ali MF, Darbar D, Rottman JN. Implantable cardioverter-defibrillator malfunction due to mechanical failure of the header connection. *J Cardiovasc Electrophysiol*. September 2004;15(9):1095-1099.


Connector module before lead insertion

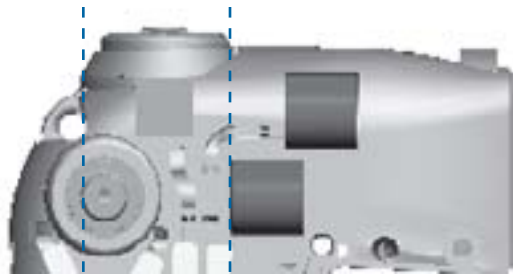

Cross-section of connector module after lead fully installed

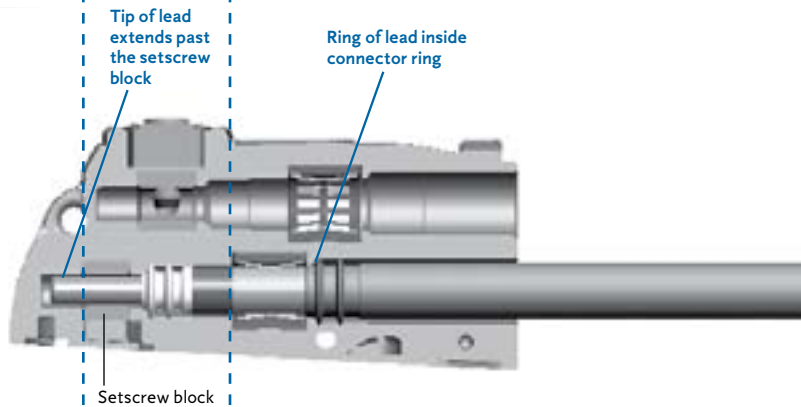

X-ray image of connector module after lead fully installed

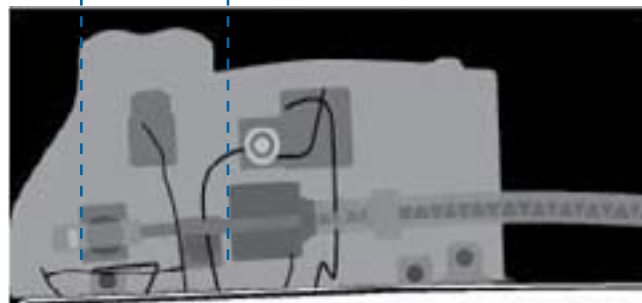

GEM II DR/VR and GEM III DR/VR/AT ICD Battery Discharge Behavior

Medtronic manufactures and utilizes a unique Lithium/Silver Vanadium Oxide battery in the GEM II/III family of ICDs. This battery has a distinctive voltage discharge with two regions of constant voltage at 3.2 volts and 2.6 volts.

The battery discharge curve (see curve below) is characterized by a significant decrease in the battery voltage approaching Middle-of-Life (MOL), followed by a plateau (MOL to ERI) where the battery voltage remains around 2.6 volts. The transition to the plateau could be easily misinterpreted as the battery rapidly approaches ERI, which occurs at 2.55 volts, when the battery may in fact have several years remaining until ERI.

It is important to understand that this battery voltage decrease in the GEM II/III family of ICDs is a normal


characteristic of the battery function in these devices and should not create a need for additional follow-up or monitoring.

As a general rule of thumb, the longevity from implant to MOL = MOL to ERI.

The design of the battery in subsequently released models has been modified to present a more linear battery discharge curve.

If you are concerned about early ERI in your patient's device, you can utilize the battery trend measurements stored in the save-to-disk file, which can be accessed and interpreted through the Medtronic Technical Services at 1 (800) 723-4636.

GEM II/III Battery Discharge Curve

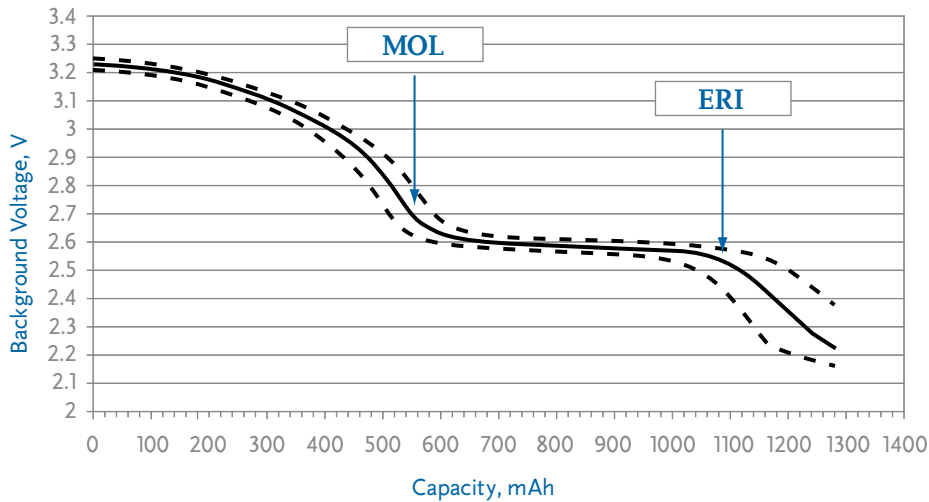

General Follow-Up and Replacement of ICD Leads

Implanted leads operate in the challenging biochemical environment of the human body and the body's response to foreign objects. Implanted leads are also subject to mechanical stresses associated with heart motion, body motion, and patient anatomy.

In this environment, pacemaker and defibrillation leads cannot be expected to last forever. Unlike implantable cardioverter defibrillators (ICDs), a lead's longevity cannot be predicted nor are there simple indicators that a lead is approaching the end of its service life. The determination that a lead may be approaching end of service life requires follow-up of the chronically implanted lead and thorough evaluation of lead integrity at ICD replacement.

Follow-Up of Chronically Implanted Leads

The frequency of follow-up for ICD patients will depend on a number of factors including the patient's medical condition, ICD system implant time, hospital/clinic follow-up practice, and Medicare guidelines. In all cases, it is important to assess the functionality of the ICD system and the integrity. For newly implanted leads, it is beneficial to establish a baseline of chronic performance parameters once the lead has stabilized, generally within 6 to 12 months after implant. These performance parameters should include pacing and sensing thresholds and impedance. During routine patient follow-up, these procedures can be used to evaluate lead integrity.

- Measure pacing and sensing threshold and compare to the chronic baseline. Significant increases or decreases may be indicative of lead failure, dislodgement, perforation, exit block, etc.
- Measure pacing impedance where possible and compare to the chronic baseline. Decreases of 30% or more or pacing impedances below 200-250 ohms may be indicative of insulation failure. Sudden and significant increases in pacing impedance may be indicative of conductor fracture.
- High voltage lead circuit impedance should be between 10-75 ohms at system implant. Chronic measurements below 10 and above 200 ohms may be indicative of high voltage lead circuit failure.
- Carefully review ECGs or the non-sustained detection log on Medtronic ICDs for indications of pacing and/or sensing abnormalities such as oversensing, undersensing, and loss of capture.
- Elicit and investigate any patient complaints/symptoms which may be suggestive of potential lead failure.

Where routine follow-up indicates, additional tools should be used to further evaluate performance. Tools include radiographic data, ICD electrograms, ICD Patient Alert and performance information from the System Longevity Study (SLS).

The final decision on the functional integrity and continued use of an implanted lead must be a matter of medical judgment based on these factors as well as specific patient conditions.

General Criteria for Lead Replacement

The evaluation of a chronically implanted lead is an important part of the decision to continue to use the lead with a new ICD. However, these results alone do not necessarily predict the future integrity of that lead. With the expected longevity of today's ICDs varying between approximately 5 and 10 years, a physician replacing a device should consider a number of factors, including those listed below.

Factors which should be considered in a decision to replace or continue to use include:

- Pacing and sensing thresholds should be evaluated for the potential to maintain acceptable levels.
- Pacing impedance should be measured. Bear in mind that pacing impedance below 250 ohms results in excessive battery current drain, which may seriously compromise ICD longevity, regardless of lead integrity.
- The physical appearance of the lead should be examined for insulation cracks, breaches, or other indications of lead wear or degradation.
- Medtronic System Longevity Study data should be referenced. Actuarial survival of the lead and the observed lead failure mechanisms are specific factors to consider. Use of a new lead should be considered if failure mechanisms suggest an increased time dependency as suggested in the shape of performance curve for the specific lead model.
- Current publications may provide additional information on the clinical management of leads.¹⁻³ Ultimately, the decision to replace an implanted lead involves medical judgment.

¹ Hauser RG, Cannom D, Hayes DL, et al. Long-term structural failure of coaxial polyurethane implantable cardioverter defibrillator leads. *PACE*. June 2002;25(6):879-882.

² Ellenbogen KA, Wood MA, Shepard RK, et al. Detection and management of an implantable cardioverter defibrillator lead failure: incidence and clinical implications. *J Am Coll Cardiol*. January 1, 2003;41(1):73-80.

³ Hauser RG, Kallinen LM, Almquist AK, Gornick CC, Katsiyannis WT. Early Failure of a Small Diameter High Voltage Implantable Cardioverter Defibrillator Lead, *Heart Rhythm* (2007), doi:10.1016/j.hrthm.2007.03.041

Clinical Management of High Voltage Lead System Oversensing

Appropriate sensing by an ICD system refers to the sensing of cardiac events that may or may not require therapy delivery. ICD systems must sense relatively large QRS complexes while avoiding sensing of smaller T-waves, yet continue to sense often small variable amplitude ventricular fibrillation. Thus, ICD systems attempt to dynamically adjust sensing of electrical events, and discriminate between them based on detection algorithms and programmed settings.

Inappropriate sensing can occur when an ICD system classifies events of non-cardiac origin as QRS/VF events, or senses and counts T- and far field P-waves as ventricular depolarizations. This is often referred to as "oversensing," and may result in delivery of inappropriate high voltage therapies. This is due, in part, to the desire to err on the side of delivering lifesaving high voltage therapy rather than

withholding it. Thus, an ICD system which is experiencing oversensing issues will continue to deliver therapeutic shocks as required, but may also subject the patient to unnecessary shocks.

Oversensing can be difficult to manage, in that the precipitating cause of the oversensing can be problematic to isolate. Oversensing can be caused by many factors, including myopotentials/far field sensing, electromagnetic interference, T-wave sensing, connector issues, incomplete or complete conductor fractures, and insulation breaches. While the individual physician must exercise medical judgment in determination of appropriate clinical management of ICD systems, the chart below may assist in the process of causal factor differentiation and possible intervention.

Phenomenon	Causal Factors	Characteristics	Management/Comments
Myopotentials/ Far Field Sensing	Diaphragmatic muscle potentials in breathing, wide tip-ring (coil on integrated bipolar leads) spacing.	Nonphysiological sensed event on EGM, which may confuse detection potentially resulting in false positive shocks.	Check R-waves for deterioration. Reprogram sensitivity. Try repositioning lead. Consider change-out to true bipolar lead, or if true bipolar lead in use, one with closer tip-ring spacing than current lead.
EMI (Electro-Magnetic Interference)	Arc welders, electrical generators, store walk-through security scanners, poorly insulated electrical equipment.	Multiple and consecutive short intervals (< 140 ms) independent of underlying sinus beats. Associated with proximity to the EMI source.	Avoid EMI areas. True bipolar leads less susceptible.
T-wave Sensing	Drugs, ischemic tissue, exercise, long QT syndrome, electrolyte imbalance.	Sense markers seen on EGM related to T-wave. False positive detection.	Check for R-wave deterioration and characteristics. If R-wave > 3.0 mV, reprogram sensitivity. If R-wave < 3.0 mV, reposition/replace lead. Address causal factor (e.g., drugs [if appropriate/medically viable]).
Connector Problems	Loose setscrew, cross-threaded setscrew, incomplete lead insertion into header.	This is an acute phenomenon seen within 6 months of implant (usually sooner).	Requires invasive check of connections. May be reproducible with pocket manipulation.
Incomplete Conductor Fracture	One or more filars of a multifilar conductor fracturing while leaving enough filars intact to provide a conduction circuit.	Characterized by chaotic oversensing related to motion of the fracture site.	Check EGMs and x-rays. Manipulate lead at suspected fracture site if possible as a provocative test. If confirmed, replace lead.
Lead Insulation Breach	Cuts, tears, metal ion oxidization, abrasion, cold flow, environmental stress cracking.	Characterized by cyclical and/or erratic, intermittent, spontaneous oversensing; often post-pace or post-shock can cause false positives.	Replace lead. If acute, usually secondary to implant damage/replacement damage. If late, material characteristic.
Oversensing during interrogation with programming head (not wireless telemetry) with complete lead fracture	Interrogation with a programming head in combination with complete lead fracture that creates an open circuit can induce noise on the sensing circuitry inside the ICD can.	Nonphysiologic sensed event on EGM. If detection is enabled during interrogation, oversensing may result in inappropriate therapy.	Quickly remove the programming head. CANCEL the interrupted interrogation and manually load the software for the specific device model. Reposition the programmer head over the device and immediately select SUSPEND. Device will resume detection when programming head is removed, or when RESUME is selected. Replace lead.

Technical Services is available at all times to advise clinicians in the troubleshooting and management of Medtronic products. For assistance in the United States, please call 1 (800) 723-4636. In other countries, please contact your local Medtronic representative.

Tests and Observations for Clinical Assessment of Chronic Pacing Leads

Test/Observation	Possible Insulation Failure	Possible Conductor Failure	Possible Other System Failure	Effect on Test/Observation
Pacing Impedance (Telemetered or Measured Invasively)	Sudden and Significant Decrease	Sudden and Significant Increase	Dislodgement. Perforation. Electrolyte Imbalance. Improper IPG/Lead Connection. . .	Decrease Increase or Decrease Increase or Decrease Increase or Decrease
Pacing Thresholds (Telemetered/Programmed or Measured Invasively)	Sudden and Significant Increase Especially in Bipolar System	Sudden and Significant Increase	Dislodgement. Exit Block. Infarct at Electrode Site. Perforation. Improper IPG/Lead Connection. . .	Increase Increase Increase Increase Increase
Electrograms (Telemetered or Measured Invasively)	Sudden and Significant Decrease in Amplitudes and/or Slew Rates for P- and/or R-Waves	Sudden and Significant Decrease or Disappearance of Amplitudes and/or Slew Rates for P- and/or R-Waves	Dislodgement. Perforation Infarct at Electrode Site. Electrolyte Imbalance. Improper IPG/Lead Connection. . .	Decrease Decrease Decrease Decrease Decrease
Waveform Analysis (Oscillographs of Pacer Artifact from ECG Electrodes)	Sudden Increase in Ratios of Leading-Edge Voltages to Trailing-Edge Voltages (i.e., over 25% increase)	Intermittent or No Pacer Artifacts (Even in Asynchronous Mode)	Improper IPG/Lead Connection	Intermittent or No Pacer Artifacts (Even in Asynchronous Mode)
Radiographs (Post-Implant, Recent, Current)	Not Discernible	Visual Observation of Conductor/Connector/ Electrode Fracture (Sometimes Discernible)	Dislodgement or Perforation. Improper IPG/Lead Connection.	Sometimes Discernible
Visual Inspection (Invasive)	Insulation Breach and/or Degradation, or Ligature Cut-Through	Not Easily Discernible	Connector Defect or Connector Pulled Apart. Improper IPG/Lead Connection.	Sometimes Discernible
Pectoral Muscle Stimulation	Sudden Onset Especially in Bipolar System		Connector Defect in Bipolar or Unipolar. Hypersensitivity to Unipolar Pulse Generator Can. Anti-Stim Coating or Protection Deficient.	
Phrenic Nerve/ Diaphragmatic Stimulation	Sudden Onset in Bipolar or Unipolar Systems		Perforation or Displacement of Atrial Lead (Phrenic Nerve)	
Pacemaker ECG Stimulus Artifact Size and Morphology Change (May Not Be Possible with Digital ECG)	Sudden Onset and Significant Change, Especially in Bipolar System (Increase in Size)	Sudden Changes, Usually a Decrease in Size	Perforation or Dislodgement. Connector Defect. Improper IPG/Lead Connection.	Sometimes Discernible
Oversensing (Intermittent or Continuous)	Sudden Onset, Especially in Bipolar Systems		Physical Contact between the Electrode(s) on the Lead and that of Another Lead. Inappropriate IPG Parameter Setting. Improper IPG/Lead Connection.	Sometimes Discernible
Undersensing (Intermittent or Continuous)	Sudden Onset in Either Unipolar or Bipolar Systems	Sudden Onset in Either Unipolar or Bipolar Systems	Dislodgement or Perforation. Infarct at Electrode Site. Electrolyte Imbalance. Inappropriate IPG Parameter Setting. Improper IPG/Lead Connection.	Sometimes Discernible
Loss of Capture	See "Pacing Thresholds" Above	See "Pacing Thresholds" Above	See "Pacing Thresholds" Above	

By Model Number

2187 77, 79
 2188 77, 79
 3830 91, 123, 127, 129
 4003 92, 123, 127, 129
 4003M 92, 123, 127, 129
 4004 93, 123, 127, 129, 150
 4004M 93, 123, 127, 129, 150
 4011 93, 123, 127, 129
 4012 94, 123, 127, 129, 151
 4023 94, 123, 127, 129
 4024 95, 123, 127, 129
 4033 95, 123, 127, 129
 4057 96, 123, 127, 129
 4057M 96, 123, 127, 129
 4058 97, 123, 127, 129
 4058M 97, 123, 127, 129
 4067 98, 123, 127, 129
 4068 99, 123, 127, 129
 4073 100, 124, 127, 129
 4074 101, 124, 127, 129
 4076 102, 124, 127, 129
 4081 103, 124, 127, 129
 4082 150
 4092 103, 124, 127, 129
 4193 78, 79
 4194 78, 79
 4503 104, 124, 127, 129
 4503M 104, 124, 127, 129
 4504 104, 124, 127, 129, 149
 4504M 104, 124, 127, 129, 149
 4512 105, 124, 127, 129
 4523 105, 124, 127, 129
 4524 106, 124, 127, 129
 4533 106, 124, 127, 129
 4557 107, 124, 127, 129
 4557M 107, 124, 127, 129
 4558M 107, 124, 127, 129
 4568 108, 125, 127, 129
 4574 108, 125, 127, 129
 4582 149
 4592 109, 125, 127, 129
 4951 131, 134, 135
 4951M 131, 134, 135
 4965 131, 134, 135
 4968 132, 134, 135
 5023 109, 125, 127, 129
 5023M 109, 125, 127, 129
 5024 110, 125, 127, 130
 5024M 110, 125, 127, 130
 5026 110, 125, 127, 130
 5032 136, 137
 5033 111, 125, 127, 130
 5034 111, 125, 127, 130
 5038 136, 137
 5054 112, 125, 127, 130
 5068 113, 125, 127, 130
 5069 135
 5071 132, 134, 135
 5072 114, 125, 127, 130
 5076 115, 125, 127, 130
 5092 116, 125, 127, 130
 5524 116, 125, 127, 130
 5524M 116, 125, 127, 130
 5534 117, 126, 127, 130
 5554 117, 126, 127, 130
 5568 118, 126, 127, 130
 5592 118, 126, 127, 130
 5594 119, 126, 128, 130
 6721 80, 88, 89, 90
 6917 133, 134, 135
 6917A 133, 134, 135
 6921 80, 88, 89, 90
 6930 80, 88, 89, 90, 144
 6931 81, 88, 89, 90, 144
 6932 81, 88, 89, 90, 148
 6933 82, 88, 89, 90
 6934S 90, 148
 6936 82, 88, 89, 90, 148
 6937 82, 88, 89, 90
 6937A 82, 88, 89, 90
 6939 83, 88, 89, 90
 6940 119, 126, 128, 130
 6942 83, 88, 89, 90, 148
 6943 84, 88, 89, 90, 148
 6944 84, 88, 89, 90
 6945 85, 88, 89, 90, 148
 6947 85, 88, 89, 90
 6948 86, 88, 89, 90
 6949 86, 88, 89, 90
 6957 120, 126, 128, 130
 6957J 121, 126, 128, 130
 6961 121, 126, 128, 130
 6962 122, 126, 128, 130
 6963 82, 88, 89, 90
 6966 82, 88, 89, 90
 6996 87, 88, 89, 90, 148
 6999 83, 88, 89, 90
 7088 51, 67, 72
 7089 51, 67, 72
 7107 51, 67, 72
 7108 51, 67, 72
 7223 33
 7227 21, 30, 33, 139, 148
 7229 21, 30, 33, 139, 148
 7230 22, 30, 33, 139, 146
 7231 22, 30, 33, 139
 7232 23, 30, 33, 146
 7253 38, 63, 71
 7271 23, 30, 33, 139
 7272 13, 18, 20, 33, 139
 7274 24, 30, 33, 140, 146
 7275 24, 31, 33, 140, 153
 7276 25, 31, 33, 140
 7277 13, 18, 20, 33, 140, 146
 7278 25, 31, 33, 140, 146
 7279 140, 146
 7285 141, 146
 7287 33
 7288 26, 31, 33, 141
 7289 14, 18, 20, 141, 146
 7290 26, 31, 33, 141
 7295 20
 7297 14, 18, 20, 141
 7299 15, 18, 20, 141
 7303 15, 18, 20, 142
 7304 16, 18, 20, 142
 7860 53, 67, 73
 7861 53, 67, 73
 7862 53, 67, 73
 7864 53, 67, 73
 7865 53, 67, 73
 7866 53, 67, 73
 7960i 59, 69, 73
 7961i 59, 69, 73
 7962i 59, 69, 73
 7964i 59, 69, 73
 7965i 59, 69, 73
 7966i 59, 69, 73
 7968i 60, 69, 73
 8040 16, 19, 20
 8042 17, 19, 20
 8085 52, 67, 72
 8086 52, 67, 72
 8088 52, 67, 72
 8089 52, 67, 72
 8158 54, 68, 73
 8160 54, 68, 73
 8161 54, 68, 73
 8162 54, 68, 73
 8164 54, 68, 73
 8165 54, 68, 73
 8166 54, 68, 73
 8330 50, 67, 72
 8331 50, 67, 72
 8340 50, 67, 72
 8341 50, 67, 72
 8341M 50, 67, 72
 8342 50, 67, 72
 8416 49, 66, 72
 8417 49, 66, 72
 8417M 49, 66, 72
 8418 49, 66, 72
 8419 49, 66, 72
 8424 50, 66, 72
 8426 50, 66, 72
 8427 50, 66, 72
 8960i 61, 70, 73
 8961i 61, 70, 73
 8962i 61, 70, 73
 8964i 60, 69, 73
 8965i 60, 69, 73
 8966i 60, 69, 73
 8968i 61, 70, 73
 ADD01 36, 63, 71
 ADDR01 36, 63, 71
 ADDR03 36, 63, 71
 ADDR06 36, 63, 71
 ADDR1 36, 63, 71
 ADDR5 37, 63, 71
 ADSR01 37, 63, 71
 ADSR03 37, 63, 71
 ADSR06 37, 63, 71
 ADVDD01 71
 AT501 38, 63, 71
 C154DWK 17, 19, 20, 142
 C164AWK 17, 19, 20
 C174AWK 17, 19, 20
 D153ATG 27, 31, 34, 142
 D153DRG 27, 31, 34, 142
 D153VRC 34
 D154ATG 27, 31, 34, 142
 D154AWG 28, 32, 34, 143
 D154DRG 27, 31, 34, 142
 D154VRC 28, 32, 34, 142
 D154VWC 29, 32, 34, 143
 D164AWG 28, 32, 34
 D164VWC 29, 32, 34
 E1DR01 38, 63, 71
 E1DR03 38, 63, 71
 E1DR06 38, 63, 71
 E1DR21 39, 63, 71
 E2DR01 39, 64, 71
 E2DR03 39, 64, 71
 E2DR06 39, 64, 71
 E2DR21 40, 64, 71
 E2DR31 40, 64, 71
 E2DR33 40, 64, 71
 E2SR01 41, 64, 71
 E2SR03 41, 64, 71
 E2SR06 41, 64, 71
 E2VDD01 41, 64, 71
 KD701 44, 65, 72, 147
 KD703 44, 65, 72, 147
 KD706 44, 65, 72, 147
 KDR401 42, 64, 71
 KDR403 42, 64, 71
 KDR601 43, 65, 71, 147
 KDR603 43, 65, 71, 147
 KDR606 43, 65, 71, 147
 KDR651 44, 65, 71, 147
 KDR653 44, 65, 71, 147
 KDR701 45, 65, 72, 147
 KDR703 45, 65, 72, 147
 KDR706 45, 65, 72, 147
 KDR721 45, 65, 72, 147
 KDR801 47, 66, 72
 KDR803 47, 66, 72
 KDR901 47, 66, 72
 KDR903 47, 66, 72
 KDR906 47, 66, 72
 KDR921 48, 66, 72
 KSR401 45, 65, 72, 147
 KSR403 43, 64, 71
 KSR701 46, 65, 72
 KSR703 46, 65, 72
 KSR706 46, 65, 72
 KSR901 48, 66, 72
 KSR903 48, 66, 72
 KSR906 48, 66, 72
 KVDD701 46, 65, 72, 147
 KVDD901 49, 66, 72
 P1501DR 42, 64, 71
 SDR203 56, 68, 73
 SDR303 57, 69, 73
 SDR306 57, 69, 73
 SED01 55, 68, 73
 SEDR01 55, 68, 73
 SEDRL1 73
 SES01 55, 68, 73
 SESR01 55, 68, 73
 SS103 56, 68, 73
 SS106 56, 68, 73
 SSR203 57, 68, 73
 SSR303 58, 69, 73
 SSR306 58, 69, 73
 SVDD303 58, 69, 73
 VEDR01 62, 70, 73

By Family

A

Adapta DR
 ADD01 36, 63, 71
 ADDR01 36, 63, 71
 ADDR03 36, 63, 71
 ADDR06 36, 63, 71
 ADDR1 36, 63, 71
 ADDRS1 37, 63, 71
 Adapta SR
 ADSR01 37, 63, 71
 ADSR03 37, 63, 71
 ADSR06 37, 63, 71
 Adapta VDD
 ADVDD01 71
 AT500
 7253 38, 63, 71, 155
 AT501 38, 63, 71, 155
 Attain
 2187 77, 79
 2188 77, 79
 4193 78, 79
 4194 78, 79

C

CapSure
 4003 92, 123, 127, 129
 4003M 92, 123, 127, 129
 4004 93, 123, 127, 129, 150
 4004M 93, 123, 127, 129, 150
 4503 104, 124, 127, 129
 4503M 104, 124, 127, 129
 4504 104, 124, 127, 129, 149
 4504M 104, 124, 127, 129, 149
 5026 110, 125, 127, 130
 CapSureFix
 4067 98, 123, 127, 129
 4068 99, 123, 127, 129
 4568 108, 125, 127, 129
 5068 113, 125, 127, 130
 5568 118, 126, 127, 130
 6940 119, 126, 128, 130
 CapSureFix Novus
 4076 102, 124, 127, 129
 5076 115, 125, 127, 130
 CapSure Epi
 4965 131, 134, 135
 4968 132, 134, 135
 CapSure Sense
 4073 100, 124, 127, 129
 4074 101, 124, 127, 129
 4574 108, 125, 127, 129
 CapSure SP
 4023 94, 123, 127, 129
 4024 95, 123, 127, 129
 4523 105, 124, 127, 129
 4524 106, 124, 127, 129
 5023 109, 125, 127, 129
 5023M 109, 125, 127, 129
 5024 110, 125, 127, 130
 5024M 110, 125, 127, 130
 5524 116, 125, 127, 130
 5524M 116, 125, 127, 130

CapSure SP Novus
 4092 103, 124, 127, 129
 4592 109, 125, 127, 129
 5092 116, 125, 127, 130
 5592 118, 126, 127, 130
 5594 119, 126, 128, 130
 CapSure VDD
 5032 136, 137
 CapSure VDD-2
 5038 136, 137
 CapSure Z
 4033 95, 123, 127, 129
 4533 106, 124, 127, 129
 5033 111, 125, 127, 130
 5034 111, 125, 127, 130
 5534 117, 126, 127, 130
 CapSure Z Novus
 5054 112, 125, 127, 130
 5554 117, 126, 127, 130
 Concerto
 C154DWK 17, 19, 20, 142
 C164AWK 17, 19, 20
 C174AWK 17, 19, 20

E

EnPulse DR
 E1DR01 38, 63, 71
 E1DR03 38, 63, 71
 E1DR06 38, 63, 71
 E1DR21 39, 63, 71
 EnPulse 2 DR
 E2DR01 39, 64, 71
 E2DR03 39, 64, 71
 E2DR06 39, 64, 71
 E2DR21 40, 64, 71
 E2DR31 40, 64, 71
 E2DR33 40, 64, 71
 EnPulse 2 SR
 E2SR01 41, 64, 71
 E2SR03 41, 64, 71
 E2SR06 41, 64, 71
 EnPulse 2 VDD
 E2VDD01 41, 64, 71
 EnRhythm DR
 P1501DR 42, 64, 71
 EnTrust
 D153ATG 27, 31, 34, 142
 D153DRG 27, 31, 34, 142
 D153VRC 34
 D154ATG 27, 31, 34, 142
 D154DRG 27, 31, 34, 142
 D154VRC 28, 32, 34, 142
 Epicardial Patch
 6721 80, 88, 89, 90
 6921 80, 88, 89, 90

G

GEM
 7227 21, 30, 33, 139, 148
 GEM DR
 7271 23, 30, 33, 139
 GEM II VR
 7229 21, 30, 33, 139, 148, 157
 GEM III AT
 7276 25, 31, 33, 140, 157
 GEM III DR
 7275 24, 31, 33, 140, 153, 157
 GEM III VR
 7231 22, 30, 33, 139, 157

I

InSync
 8040 16, 19, 20
 InSync ICD
 7272 13, 18, 20, 33, 139
 InSync Marquis
 7277 13, 18, 20, 33, 140, 146
 InSync Maximo
 7303 15, 18, 20
 7304 16, 18, 20
 InSync Sentry
 7297 14, 18, 20
 7299 15, 18, 20
 InSync II Marquis
 7289 14, 18, 20, 141, 146
 InSync II Protect
 7295 20
 InSync III Protect
 7285 141, 146
 InSync III
 8042 17, 19, 20
 InSync III Marquis
 7279 140, 146
 Intrinsic
 7288 26, 31, 33, 141
 Intrinsic 30
 7287 33

K

Kappa 400 DR
 KDR401 42, 64, 71
 KDR403 42, 64, 71
 Kappa 400 SR
 KSR401 43, 64, 71
 KSR403 43, 64, 71
 Kappa 600 DR
 KDR601 43, 65, 71, 147
 KDR603 43, 65, 71, 147
 KDR606 43, 65, 71, 147
 KDR651 44, 65, 71, 147
 KDR653 44, 65, 71, 147

Kappa 700 D
 KDR701 44, 65, 72, 147
 KD703 44, 65, 72, 147
 KD706 44, 65, 72, 147
 Kappa 700 DR
 KDR701 45, 65, 72, 147
 KDR703 45, 65, 72, 147
 KDR706 45, 65, 72, 147
 KDR721 45, 65, 72, 147
 Kappa 700 SR
 KSR701 46, 65, 72
 KSR703 46, 65, 72
 KSR706 46, 65, 72
 Kappa 700 VDD
 KVDD701 46, 65, 72, 147
 Kappa 800 DR
 KDR801 47, 66, 72
 KDR803 47, 66, 72
 Kappa 900 DR
 KDR901 47, 72
 KDR903 47, 72
 KDR906 47, 72
 Kappa 900 SR
 KSR901 48, 66, 72
 KSR903 48, 66, 72
 KSR906 48, 66, 72
 Kappa 900 VDD
 KVDD901 49, 66, 72
 Kappa 920 DR
 KDR921 48, 66, 72

L

Legend
 8416 49, 66, 72
 8417 49, 66, 72
 8417M 49, 66, 72
 8418 49, 66, 72
 8419 49, 66, 72
 Legend II
 8424 50, 66, 72
 8426 50, 66, 72
 8427 50, 66, 72

M

Marquis DR
 7274 24, 30, 33, 140, 146
 Marquis VR
 7230 22, 30, 33, 139, 146
 Maximo DR
 7278 25, 31, 33, 140, 146
 Maximo VR
 7232 23, 30, 33, 146
 Minix/Minix ST
 8330 50, 67, 72, 152
 8331 50, 67, 72, 152
 8331M 50, 67, 72, 152
 8340 50, 67, 72, 152
 8341 50, 67, 72, 152
 8341M 50, 67, 72, 152
 8342 50, 67, 72, 152
 Minuet
 7107 51, 67, 72
 7108 51, 67, 72

By Family continued

O

Onyx
7290 26, 31, 33, 141

P

Preva DR
7088 51, 67, 72
7089 51, 67, 72
Preva SR
8088 52, 67, 72
8089 52, 67, 72
Prevail S
8085 52, 67, 72
8086 52, 67, 72
Prodigy D
7864 53, 67, 73
7865 53, 67, 73
7866 53, 67, 73
Prodigy DR
7860 53, 67, 73
7861 53, 67, 73
7862 53, 67, 73
Prodigy S
8164 54, 68, 73
8165 54, 68, 73
8166 54, 68, 73
Prodigy SR
8158 54, 68, 73
8160 54, 68, 73
8161 54, 68, 73
8162 54, 68, 73

S

Screw-In
4057 96, 123, 127, 129
4057M 96, 123, 127, 129
4058 97, 123, 127, 129
4058M 97, 123, 127, 129
4557 107, 124, 127, 129
4557M 107, 124, 127, 129
4558M 107, 124, 127, 129
SelectSecure
3830 91, 123, 127, 129
Sensia DR
SED01 55, 68, 73
SEDR01 55, 68, 73
SEDRL1 73
Sensia SR
SES01 55, 68, 73
SESR01 55, 68, 73
Sigma 100 S
SS103 56, 68, 73
SS106 56, 68, 73
Sigma 200 DR
SDR203 56, 68, 73
Sigma 200 SR
SSR203 57, 68, 73

Sigma 300 DR
SDR303 57, 69, 73
SDR306 57, 69, 73
Sigma 300 SR
SSR303 58, 69, 73
SSR306 58, 69, 73
Sigma 300 VDD
SVDD303 58, 69, 73
Spectraflex
4951 131, 134, 135
4951M 131, 134, 135
6957 120, 126, 128, 130
6957J 121, 126, 128, 130
Sprint
6932 81, 88, 89, 90, 148
6942 83, 88, 89, 90, 148
6943 84, 88, 89, 90, 148
6945 85, 88, 89, 90, 148
Sprint Fidelis
6930 80, 88, 89, 90, 144
6931 81, 88, 89, 90, 144
6948 86, 88, 89, 90, 144
6949 86, 88, 89, 90, 144
Sprint Quattro
6944 84, 88, 89, 90
Sprint Quattro Secure
6947 85, 88, 89, 90
Sub-Q Lead
6996 87, 88, 89, 90
Sub-Q Patch
6939 83, 88, 89, 90
6999 83, 88, 89, 90
SureFix
5072 114, 125, 127, 130
SVC/CS
6933 82, 88, 89, 90
6937 82, 88, 89, 90
6937A 82, 88, 89, 90
6963 82, 88, 89, 90

T

Target Tip
4011 93, 123, 127, 129
4012 94, 123, 127, 129, 151
4081 103, 124, 127, 129
4082 150
4512 105, 124, 127, 129
4582 149
Tenax
6917 133, 134, 135
6917A 133, 134, 135
6961 121, 126, 128, 130
6962 122, 126, 128, 130
Thera-i D
7964i 59, 69, 73
7965i 59, 69, 73
7966i 59, 69, 73
Thera-i DR
7960i 59, 69, 73
7961i 59, 69, 73
7962i 59, 69, 73
7968i 60, 69, 73

Thera-i S
8964i 60, 69, 73
8965i 60, 69, 73
8966i 60, 69, 73
Thera-i SR
8960i 61, 70, 73
8961i 61, 70, 73
8962i 61, 70, 73
Thera-i VDD
8968i 61, 70, 73
Transvene
6934S 90, 148
6936 82, 88, 89, 90, 148
6966 82, 88, 89, 90, 148

V

Versa DR
VEDR01 62, 70, 73
Virtuoso
D154AWG 28, 32, 34, 143
D164AWG 28, 32, 34
D154VWC 29, 32, 34, 143
D164VWC 29, 32, 34

If you are looking for a model number or family that is not included in this report, you may call US Technical Services (see page 2).

Mailer Kits Available for Returning Product

Medtronic urges all physicians to return explanted product and to notify Medtronic when a product is no longer in use, regardless of reason for explant or removal from use. The procedures for returning product vary by geographic location.

Mailer kits (pictured right) with prepaid US postage are available for use within the United States to send CRT, ICD, IPG, and leads to Medtronic's CRDM Returned Product Analysis Lab. These mailers are sized to accommodate the devices and leads from a single patient or clinical event and are designed to meet postal regulations for mailing biohazard materials.

If the product being returned is located outside the United States, please contact your local Medtronic representative for instructions.

Medtronic also requests the return of devices from non-clinical sources such as funeral homes, and will assume responsibility for storage and disposal of the product once received. For return of larger quantities of explanted products than the mailer can accommodate, Medtronic has handling and shipping guidelines available upon request.

Both mailers and guidelines can be requested by contacting the Returned Product Lab.

CRDM Returned Product Analysis Laboratory
Medtronic, Inc.
7000 Central Avenue NE MS RCE172
Minneapolis, MN 55432-3576 USA
Phone: 1 (800) 328-2518, ext. 44800
email: crdm.returnedproduct@medtronic.com



World Headquarters

Medtronic, Inc.
710 Medtronic Parkway
Minneapolis, MN 55432-5604
USA
Tel: (763) 514-4000
Fax: (763) 514-4879
www.medtronic.com

Medtronic USA, Inc.
Toll-free: 1 (800) 328-2518
(24-hour technical support for
physicians and medical professionals)

Europe

Medtronic International Trading Sàrl
Route du Molliau 31
CH-1131 Tolochenaz
Switzerland
Tel: (41 21) 802 7000
Fax: (41 21) 802 7900
www.medtronic.com

Canada

Medtronic of Canada Ltd.
6733 Kitimat Road
Mississauga, Ontario L5N 1W3
Canada
Tel: (905) 826-6020
Fax: (905) 826-6620
Toll-free: 1 (800) 268-5346

Asia Pacific

Medtronic International, Ltd.
16/F Manulife Plaza
The Lee Gardens, 33 Hysan Avenue
Causeway Bay
Hong Kong
Tel: (852) 2891 4456
Fax: (852) 2891 6830
enquiryap@medtronic.com
www.medtronic.com

Latin America

Medtronic USA, Inc.
Doral Corporate Center II
3750 NW 87th Avenue Suite 700
Miami, FL 33178
USA
Tel: (305) 500-9328
Fax: (786) 709-4244
www.medtronic.com

UC200804878 EN
© Medtronic, Inc. 2008
All Rights Reserved
Printed in USA
May 2008